
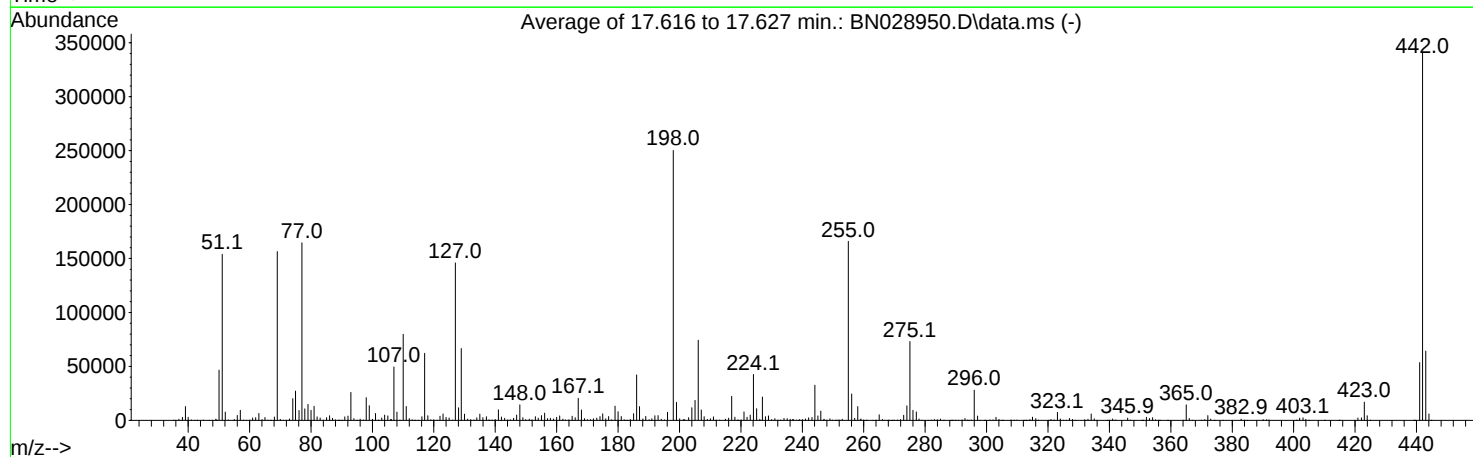


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120123\
 Data File : BN028950.D
 Acq On : 01 Dec 2023 16:59
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN113023.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Dec 04 00:28:48 2023

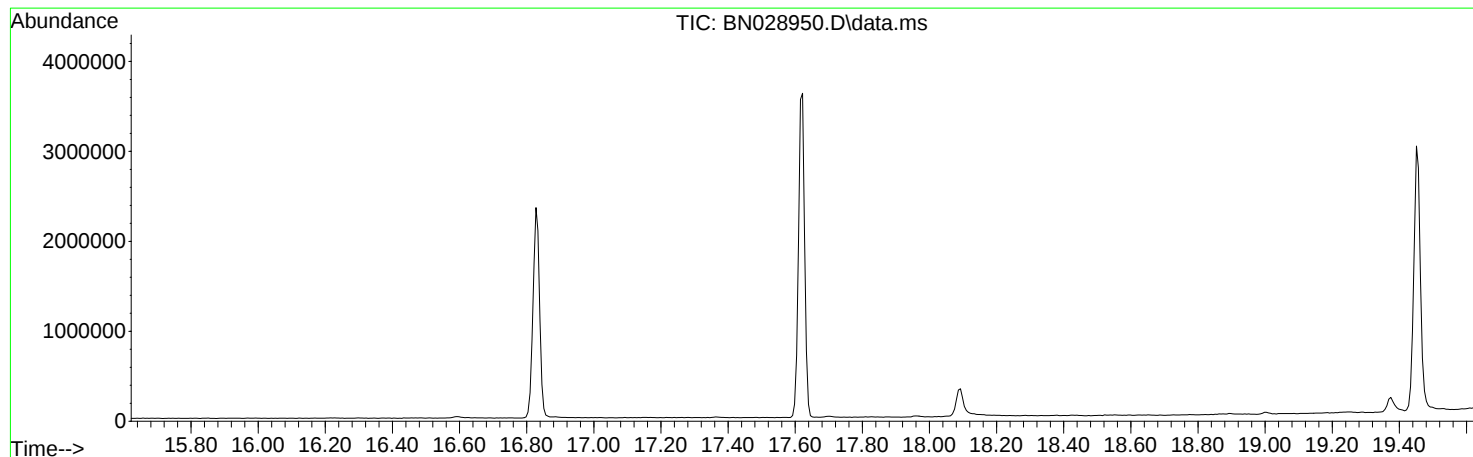




AutoFind: Scans 2470, 2471, 2472; Background Corrected with Scan 2463

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	61.5	153987	PASS
68	69	0.00	2	2.0	3087	PASS
69	198	0.00	100	62.5	156407	PASS
70	69	0.00	2	0.5	839	PASS
127	198	10	80	58.3	145984	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	250197	PASS
199	198	5	9	6.7	16769	PASS
275	198	10	60	29.3	73187	PASS
365	198	1	100	5.7	14371	PASS
441	198	0.01	100	21.4	53488	PASS
442	442	50	100	100.0	340928	PASS
443	442	15	24	18.8	64213	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120123\
Data File : BN028950.D
Acq On : 01 Dec 2023 16:59
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 01 23:57:29 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 01 23:28:24 2023
Response via : Initial Calibration

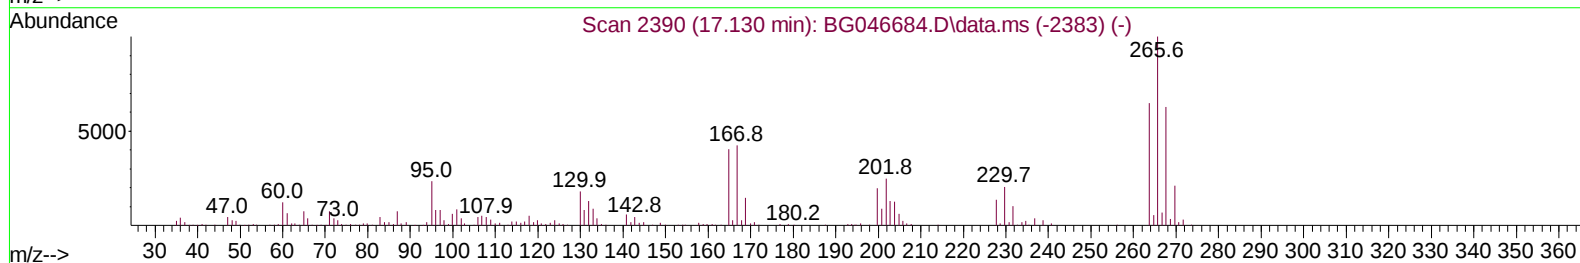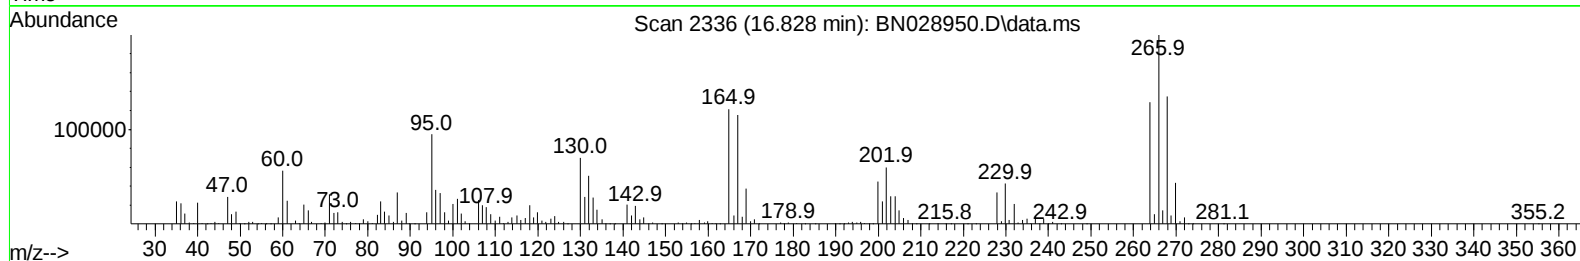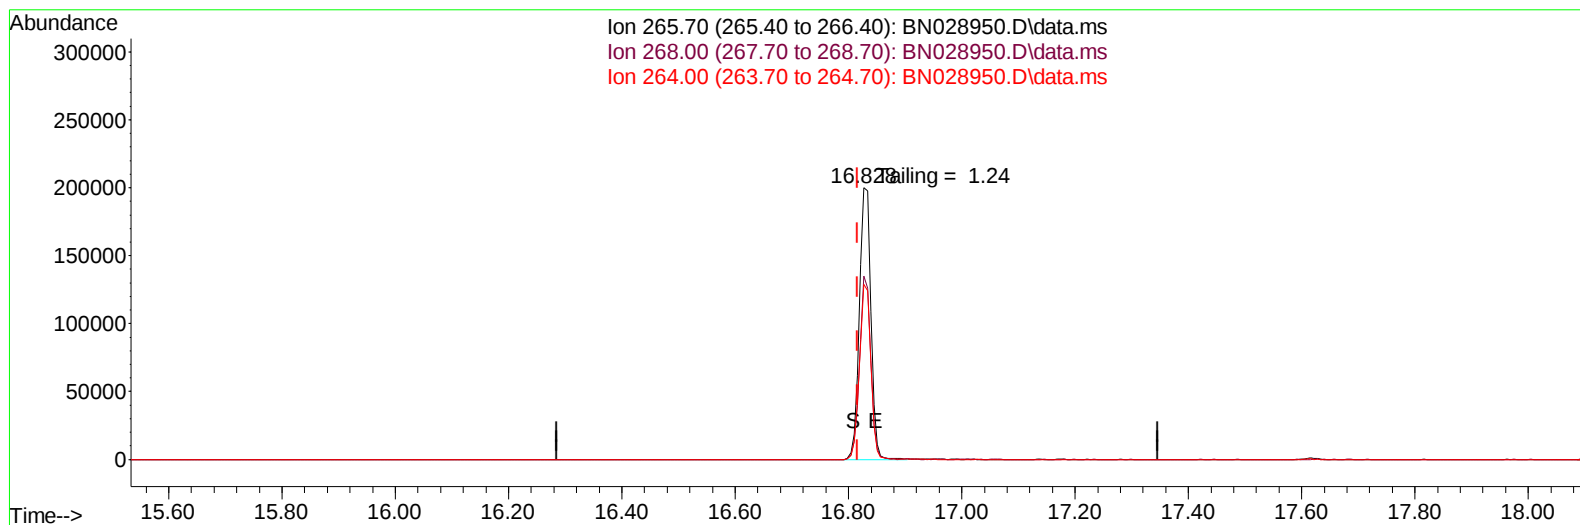

TIC: BN028950.D\data.ms

(70) Pentachlorophenol (C)

16.828min (+ 0.012) 16726.07 ng




response 280113

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	67.53
264.00	61.60	64.39
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120123\
Data File : BN028950.D
Acq On : 01 Dec 2023 16:59
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 01 23:57:29 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 01 23:28:24 2023
Response via : Initial Calibration

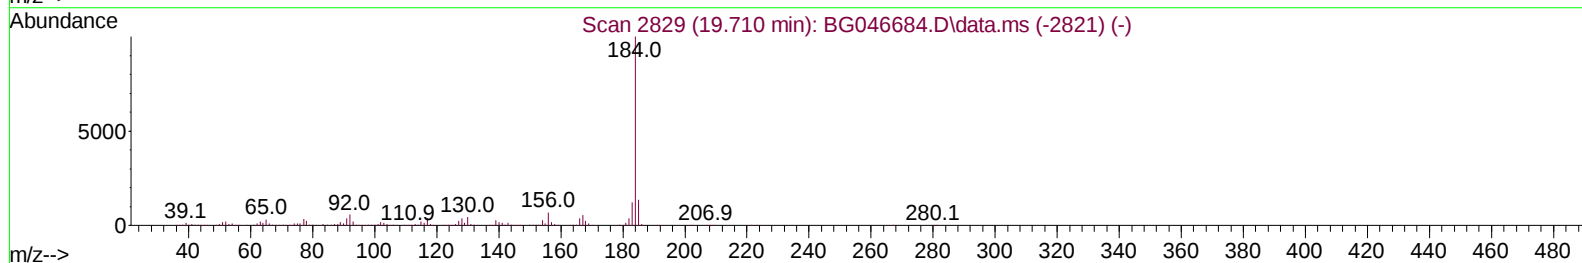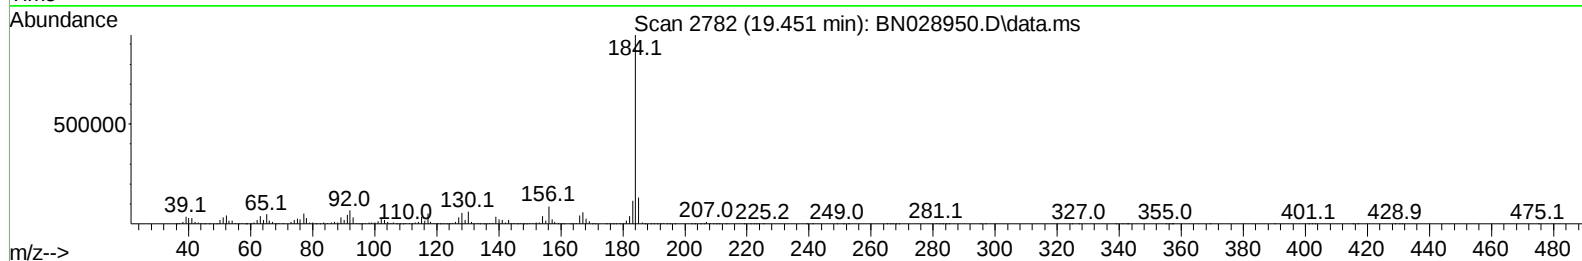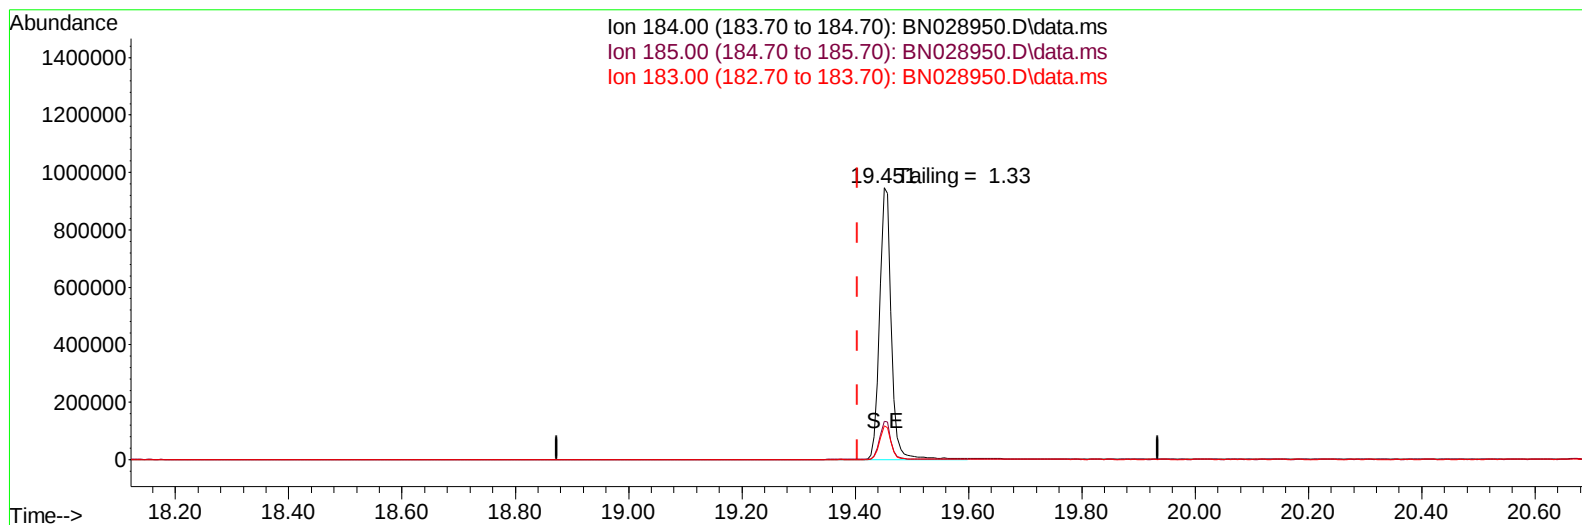

TIC: BN028950.D\data.ms

(77) Benzidine

19.451min (+ 0.047) 49438.77 ng

response 1350236

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.08
183.00	13.20	12.40
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/1/2023	BNA_N	<u>BN028950.D</u>
Compound Name	Response	Retention Time
DDT	660710	20.674
DDD	103162	20.233
DDE	422	19.716
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
103584	764294	13.55

Instrument :
BNA_N
ClientSampleId :
DFTPP