
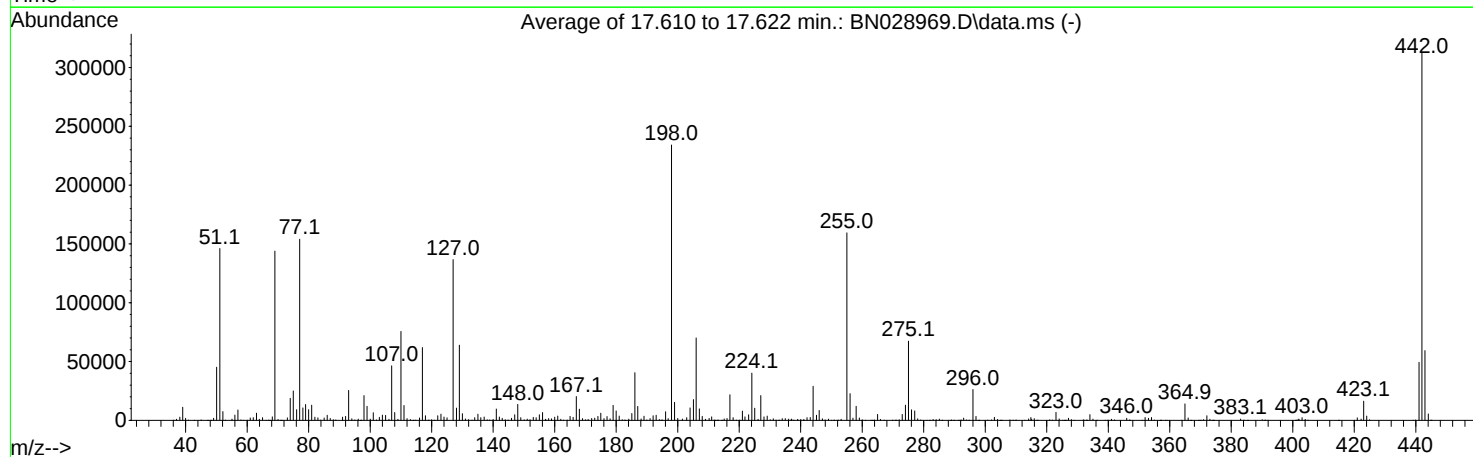


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120123\
Data File : BN028969.D
Acq On : 02 Dec 2023 05:03
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN113023.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Dec 04 00:28:48 2023

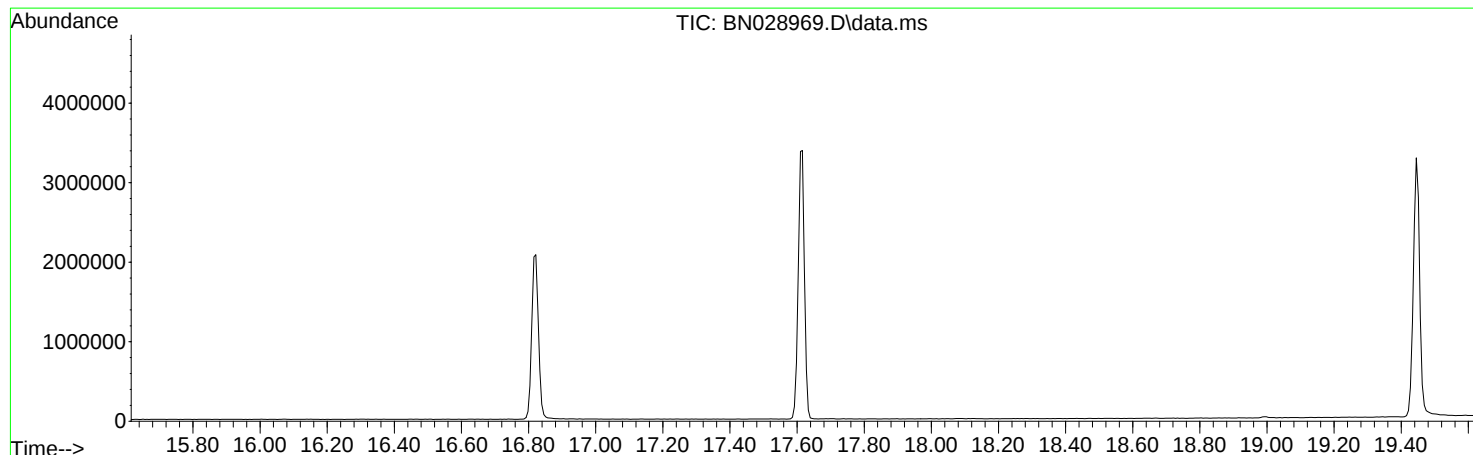




AutoFind: Scans 2469, 2470, 2471; Background Corrected with Scan 2462

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	62.4	146051	PASS
68	69	0.00	2	2.1	3006	PASS
69	198	0.00	100	61.5	143931	PASS
70	69	0.00	2	0.6	798	PASS
127	198	10	80	58.4	136712	PASS
197	198	0.00	2	0.7	1523	PASS
198	198	100	100	100.0	234112	PASS
199	198	5	9	6.6	15417	PASS
275	198	10	60	28.8	67384	PASS
365	198	1	100	6.0	14005	PASS
441	198	0.01	100	21.1	49368	PASS
442	442	50	100	100.0	312768	PASS
443	442	15	24	19.0	59288	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120123\
 Data File : BN028969.D
 Acq On : 02 Dec 2023 05:03
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Dec 02 06:21:28 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 01 23:28:24 2023
 Response via : Initial Calibration

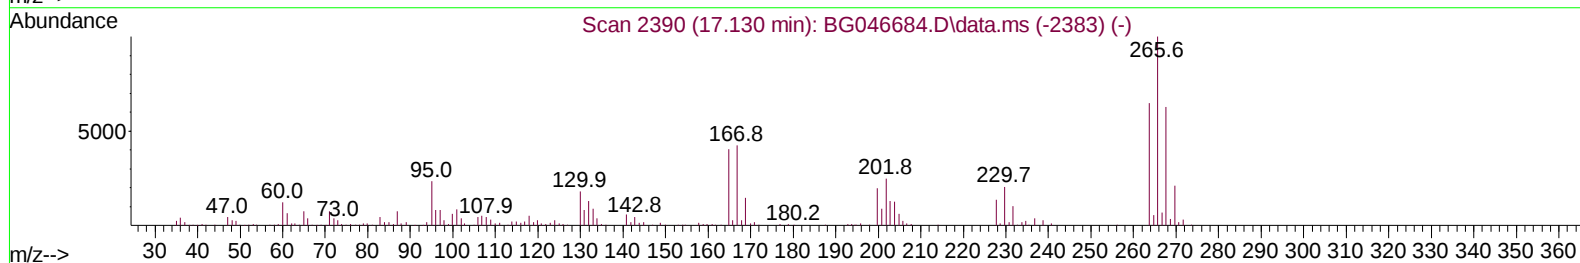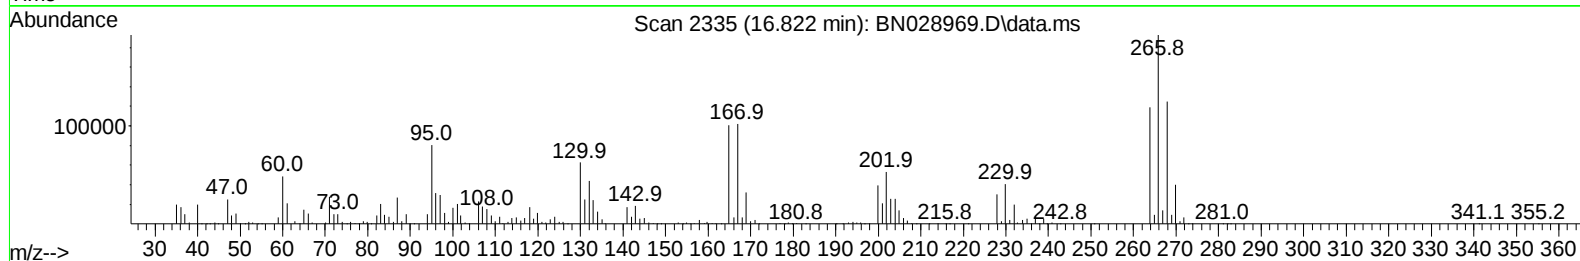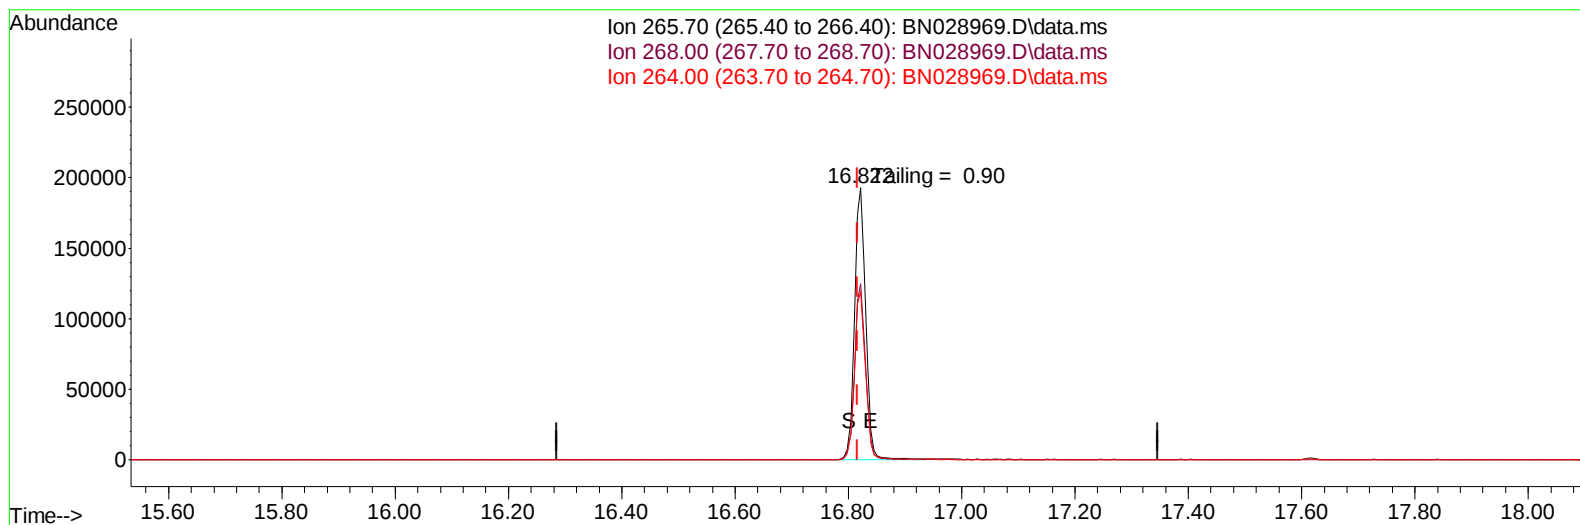

TIC: BN028969.D\data.ms

(70) Pentachlorophenol (C)

16.822min (+ 0.006) 16582.59 ng

response 263135

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.66
264.00	61.60	61.85
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/1/2023	BNA_N	<u>BN028969.D</u>
Compound Name	Response	Retention Time
DDT	745743	20.663
DDD	82499	20.222
DDE	454	19.71
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
82953	828696	10.01

Instrument :
BNA_N
ClientSampleId :
DFTPP