
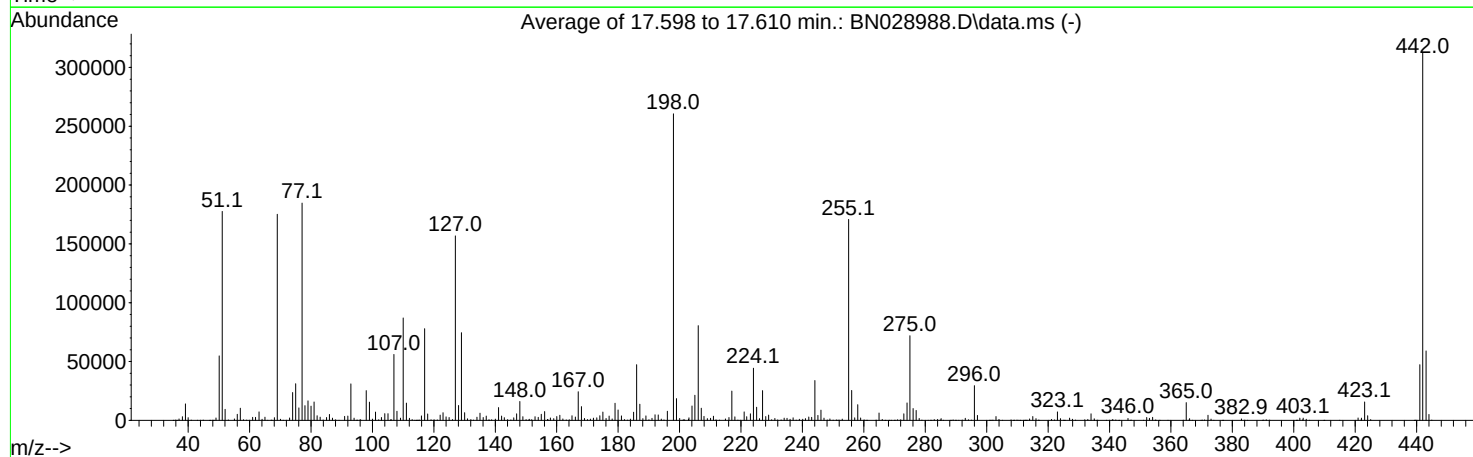


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120123\
Data File : BN028988.D
Acq On : 02 Dec 2023 18:12
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN113023.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Dec 04 00:28:48 2023

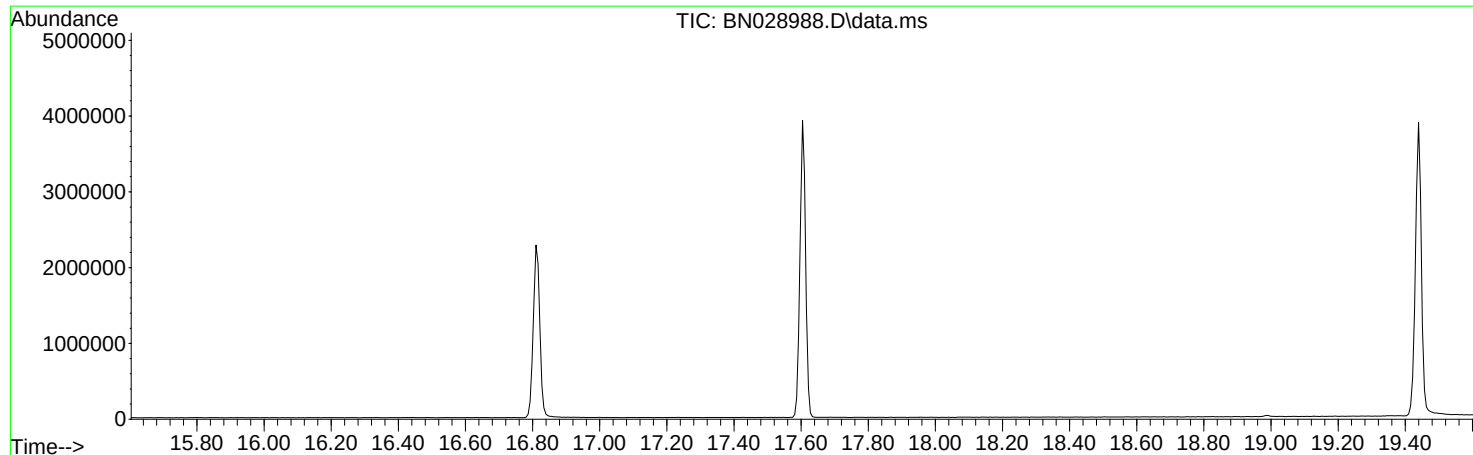




AutoFind: Scans 2467, 2468, 2469; Background Corrected with Scan 2460

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	68.1	177600	PASS
68	69	0.00	2	1.3	2259	PASS
69	198	0.00	100	67.2	175168	PASS
70	69	0.00	2	0.6	965	PASS
127	198	10	80	60.2	156821	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	260608	PASS
199	198	5	9	7.1	18521	PASS
275	198	10	60	27.6	71925	PASS
365	198	1	100	5.8	15071	PASS
441	198	0.01	100	18.2	47403	PASS
442	442	50	100	100.0	312661	PASS
443	442	15	24	18.9	58989	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120123\
 Data File : BN028988.D
 Acq On : 02 Dec 2023 18:12
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Dec 04 03:00:32 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 01 23:28:24 2023
 Response via : Initial Calibration

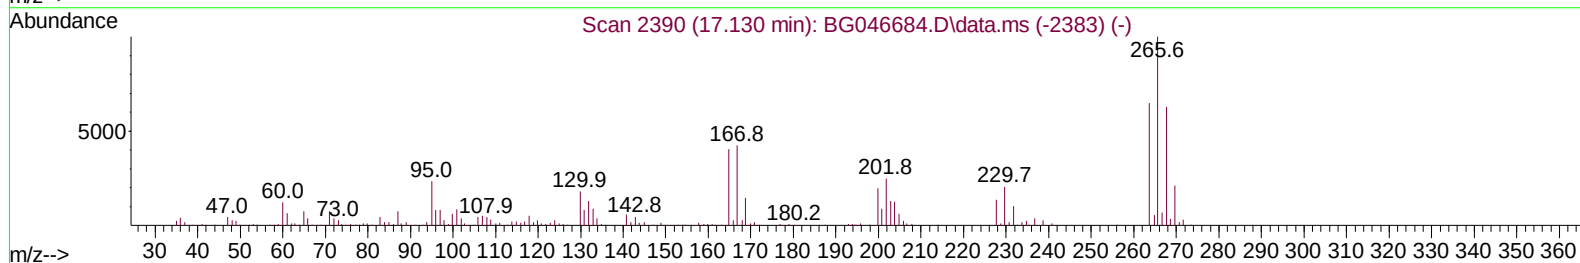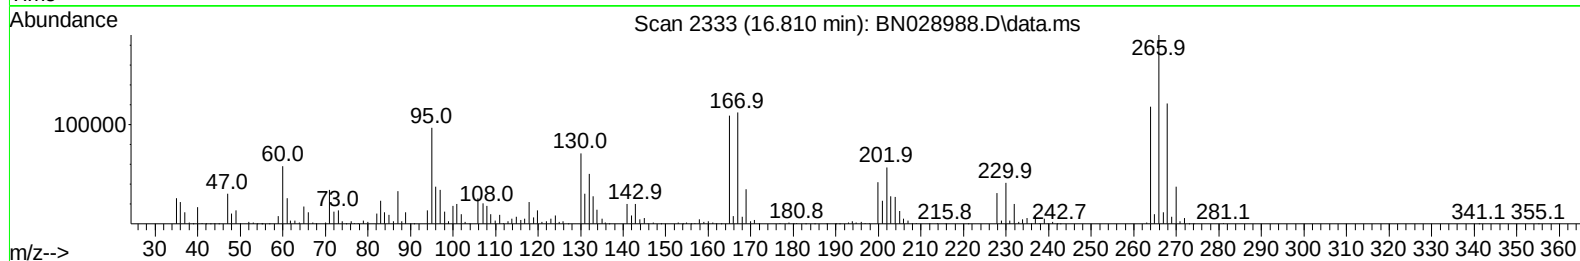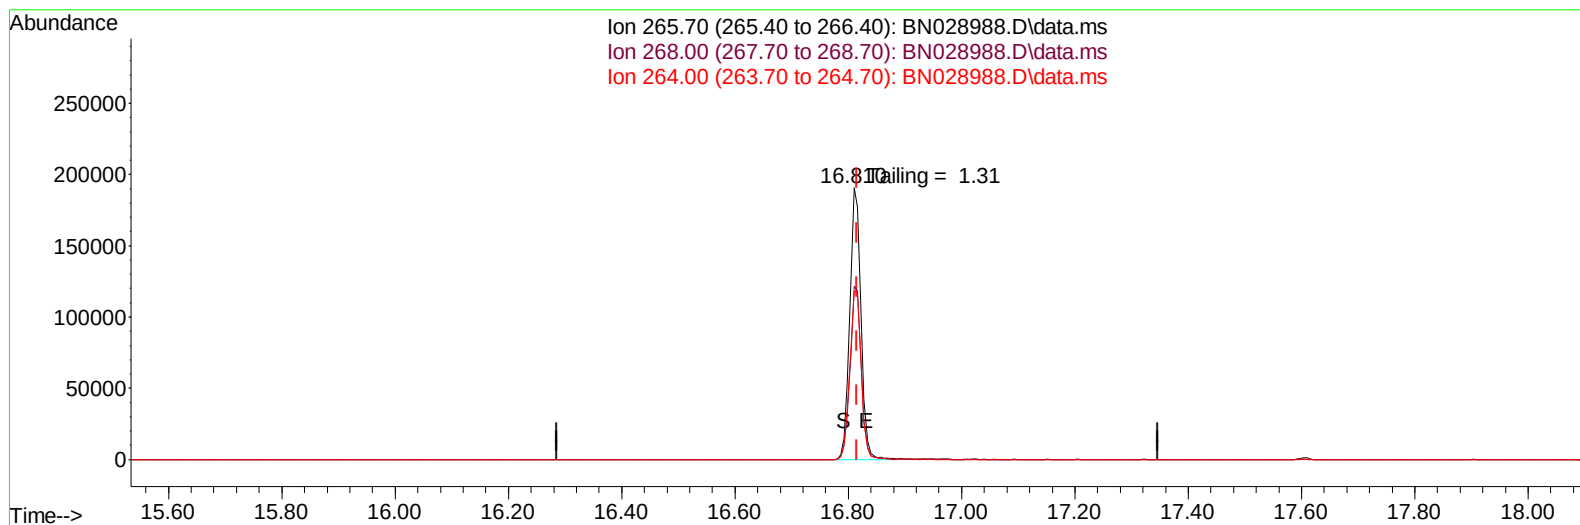

TIC: BN028988.D\data.ms

(70) Pentachlorophenol (C)

16.810min (-0.006) 16409.79 ng




response 263870

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.86
264.00	61.60	61.91
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120123\
Data File : BN028988.D
Acq On : 02 Dec 2023 18:12
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 04 03:00:32 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 01 23:28:24 2023
Response via : Initial Calibration

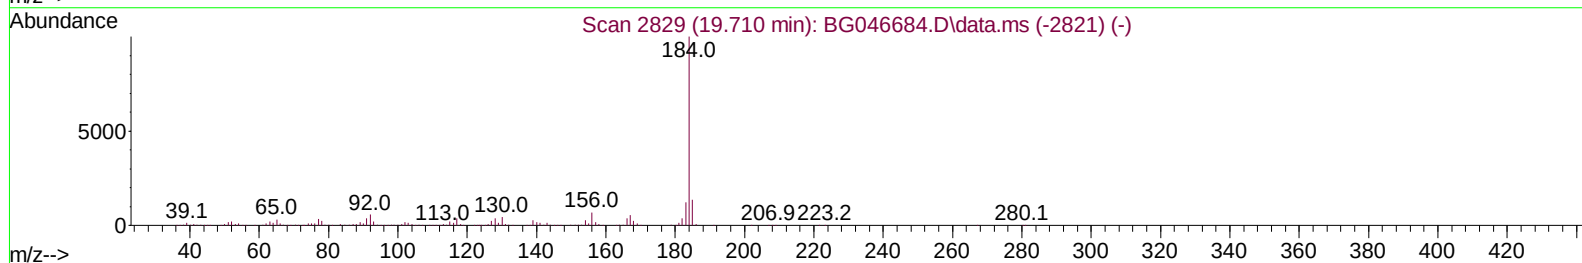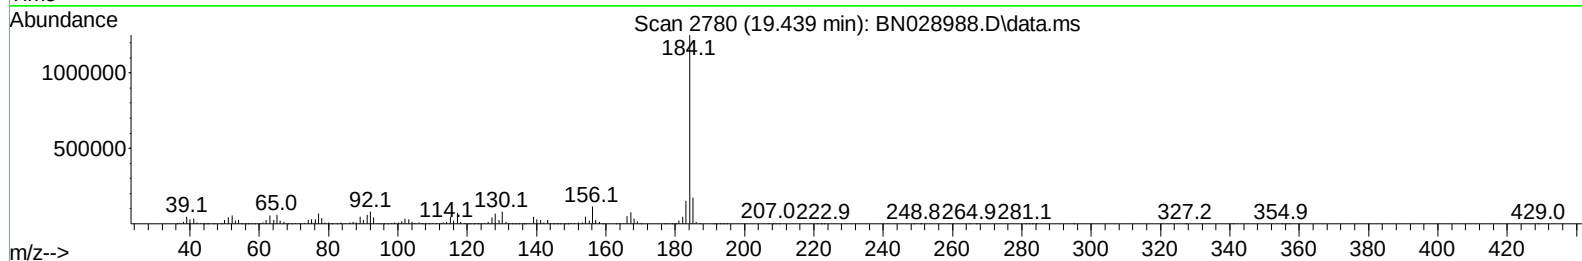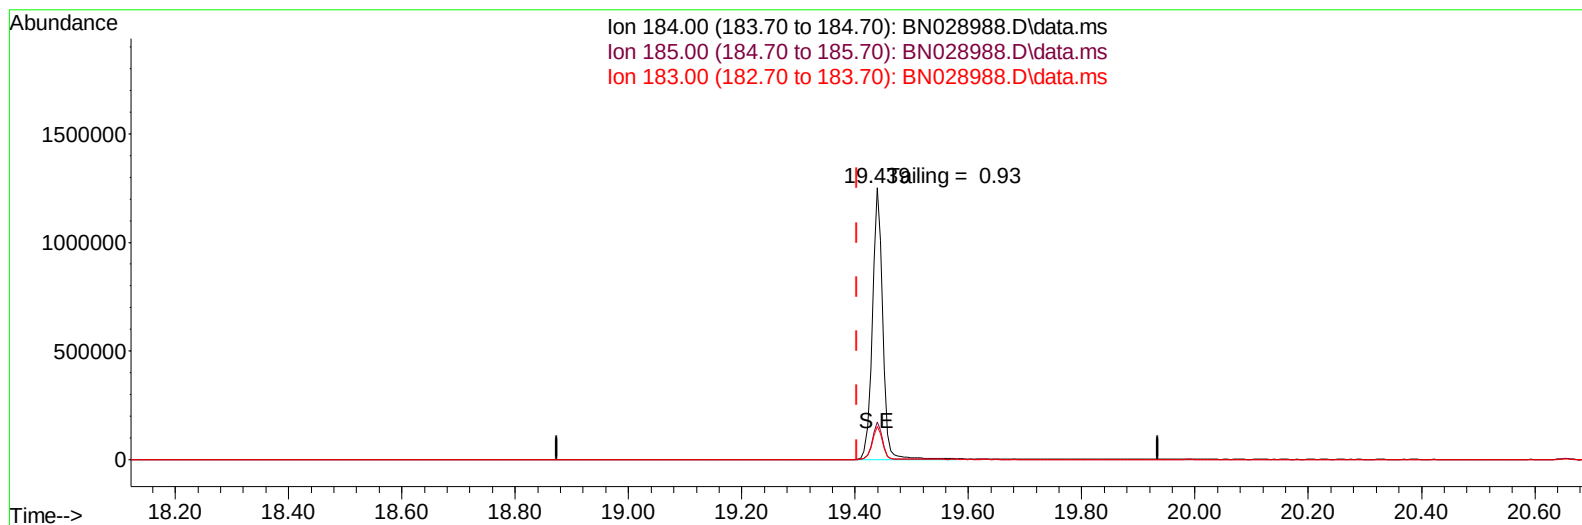

TIC: BN028988.D\data.ms

(77) Benzidine

19.439min (+ 0.035) 887549.21 ng

response 1586824

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.91
183.00	13.20	12.16
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/1/2023	BNA_N	<u>BN028988.D</u>
Compound Name	Response	Retention Time
DDT	816529	20.657
DDD	58459	20.216
DDE	413	19.704
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
58872	875401	6.73

Instrument :
BNA_N
ClientSampleId :
DFTPP