

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120125\
 Data File : BN038231.D
 Acq On : 01 Dec 2025 18:28
 Operator : RC/JU
 Sample : PB170712BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Dec 02 01:08:26 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN112725.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 28 21:04:10 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.768	152	8256	0.400	ng	0.00
7) Naphthalene-d8	10.573	136	22952	0.400	ng	0.00
13) Acenaphthene-d10	14.430	164	10779	0.400	ng	0.00
19) Phenanthrene-d10	17.186	188	14873	0.400	ng	# 0.00
29) Chrysene-d12	21.375	240	10479	0.400	ng	0.00
35) Perylene-d12	23.680	264	10853	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.341	112	6987	0.362	ng	0.00
5) Phenol-d6	6.930	99	7715	0.320	ng	0.00
8) Nitrobenzene-d5	8.918	82	6631	0.361	ng	0.00
11) 2-Methylnaphthalene-d10	12.166	152	10344	0.317	ng	0.00
14) 2,4,6-Tribromophenol	15.944	330	556	0.164	ng	0.01
15) 2-Fluorobiphenyl	13.051	172	16277	0.391	ng	0.00
27) Fluoranthene-d10	19.220	212	11729	0.364	ng	0.00
31) Terphenyl-d14	19.819	244	8472	0.350	ng	0.00
Target Compounds						Qvalue
20) 4,6-Dinitro-2-methylph...	15.572	198	1	0.173	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120125\
Data File : BN038231.D
Acq On : 01 Dec 2025 18:28
Operator : RC/JU
Sample : PB170712BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :


Quant Time: Dec 02 01:08:26 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN112725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 28 21:04:10 2025
Response via : Initial Calibration

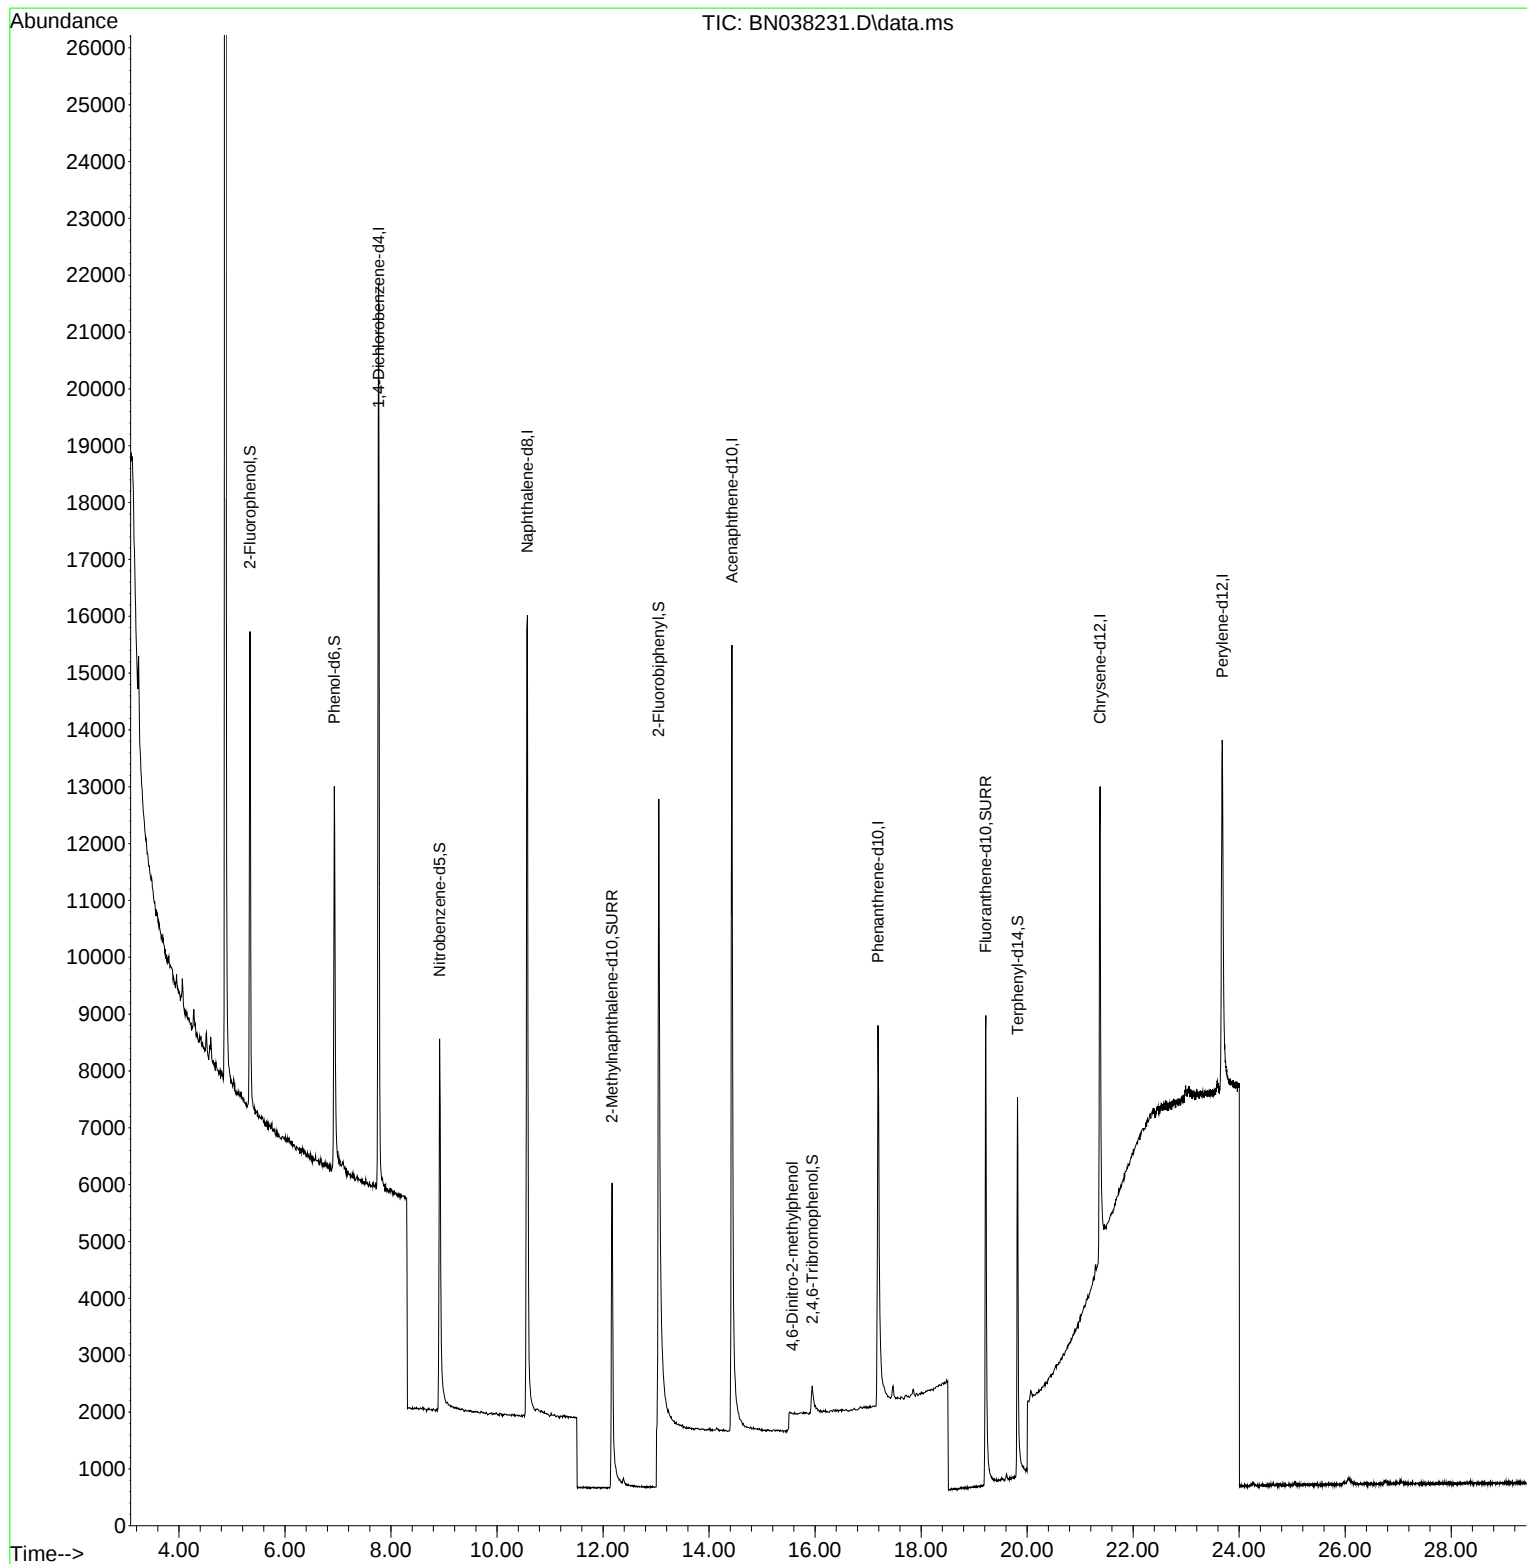



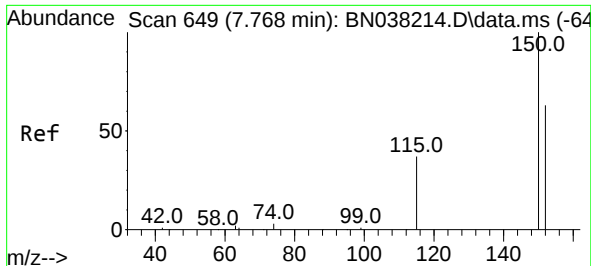


#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.768 min Scan# 649
 Delta R.T. -0.000 min
 Lab File: BN038231.D
 Acq: 01 Dec 2025 18:28


Instrument :
 BNA_N
 ClientSampleId :

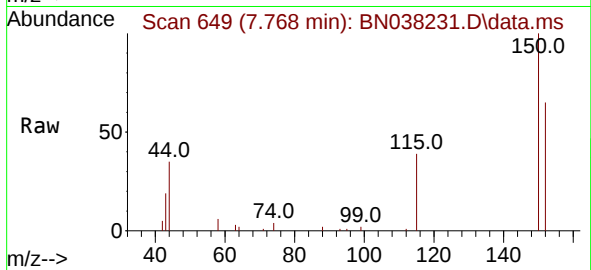



Tgt Ion:152 Resp: 8256
 Ion Ratio Lower Upper
 152 100
 150 154.8 125.3 187.9
 115 59.8 49.0 73.4

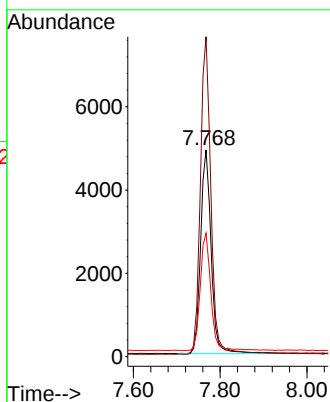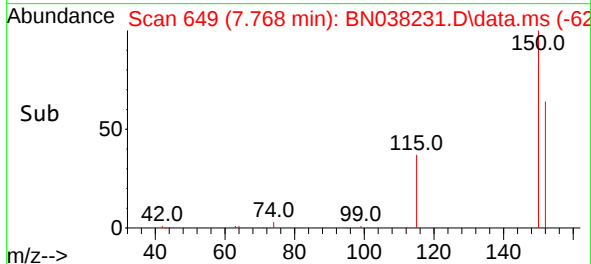


#4
 2-Fluorophenol
 Concen: 0.362 ng
 RT: 5.341 min Scan# 313
 Delta R.T. -0.000 min
 Lab File: BN038231.D
 Acq: 01 Dec 2025 18:28

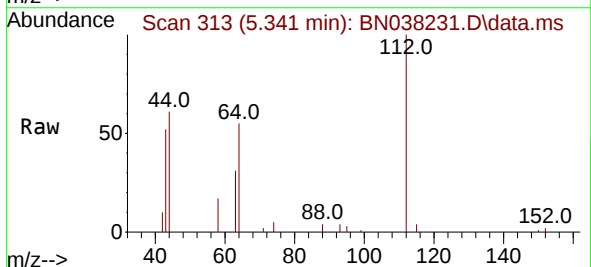

Tgt Ion:112 Resp: 6987
 Ion Ratio Lower Upper
 112 100
 64 56.1 45.0 67.4
 63 30.5 23.2 34.8



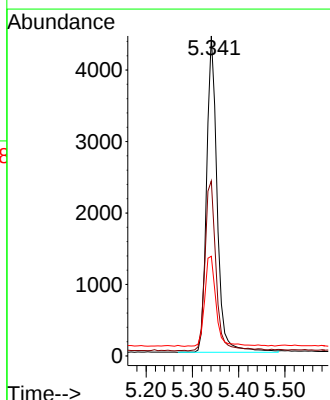



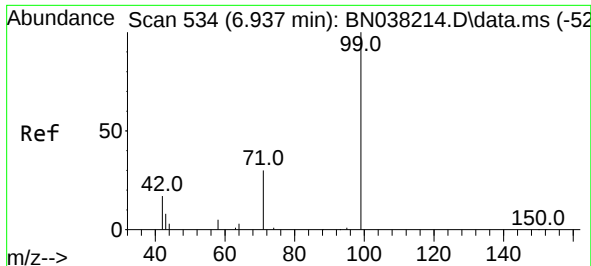

#5
Phenol-d6
Concen: 0.320 ng
RT: 6.930 min Scan# 511
Delta R.T. -0.007 min
Lab File: BN038231.D
Acq: 01 Dec 2025 18:28




Instrument :
BNA_N
ClientSampleId :


Tgt Ion: 99 Resp: 7715
Ion Ratio Lower Upper
99 100
42 20.1 17.0 25.6
71 32.9 25.4 38.2

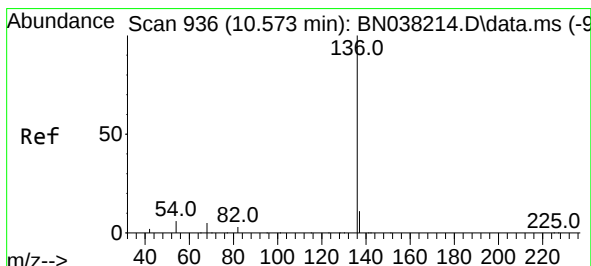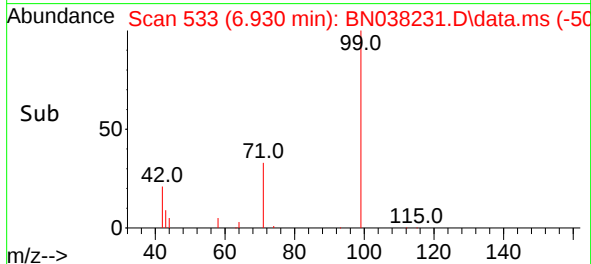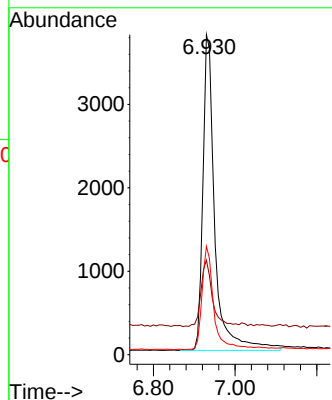

#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.573 min Scan# 936
Delta R.T. -0.000 min
Lab File: BN038231.D
Acq: 01 Dec 2025 18:28


Tgt Ion: 136 Resp: 22952
Ion Ratio Lower Upper
136 100
137 11.5 8.9 13.3
54 7.0 5.4 8.0
68 5.4 4.1 6.1

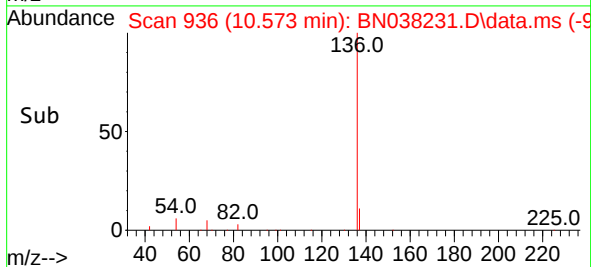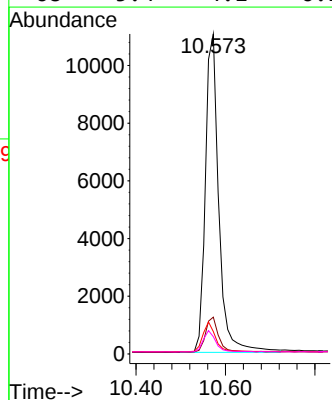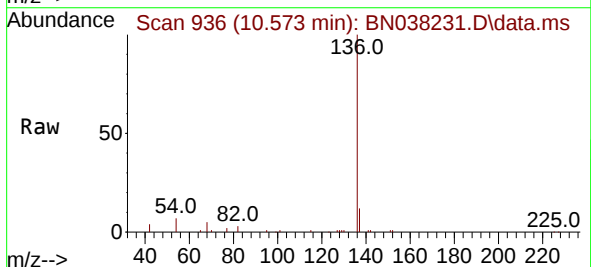



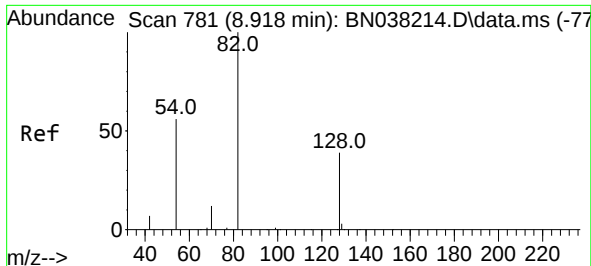


#8
Nitrobenzene-d5
Concen: 0.361 ng
RT: 8.918 min Scan# 781
Delta R.T. -0.000 min
Lab File: BN038231.D
Acq: 01 Dec 2025 18:28

Instrument :
BNA_N
ClientSampleId :







Tgt Ion: 82 Resp: 6631
Ion Ratio Lower Upper
82 100
128 41.0 32.6 48.8
54 56.7 45.4 68.0

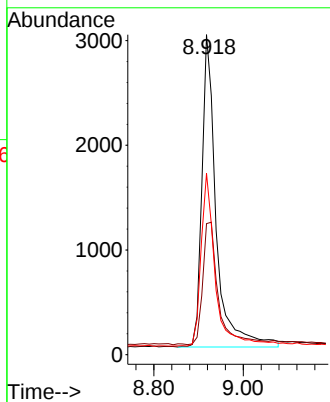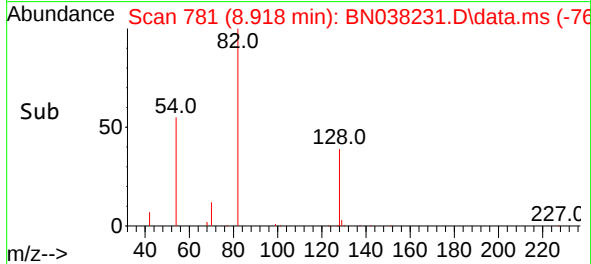

#11
2-Methylnaphthalene-d10
Concen: 0.317 ng
RT: 12.166 min Scan# 1153
Delta R.T. -0.000 min
Lab File: BN038231.D
Acq: 01 Dec 2025 18:28

Tgt Ion: 152 Resp: 10344
Ion Ratio Lower Upper
152 100
151 20.5 16.7 25.1

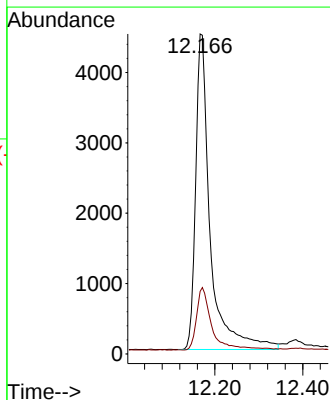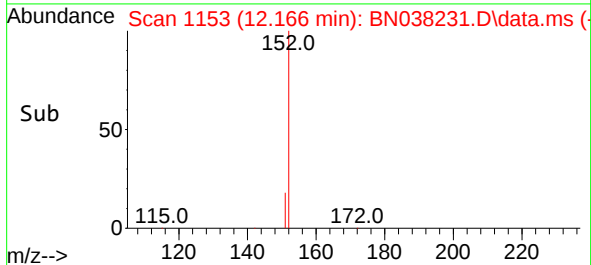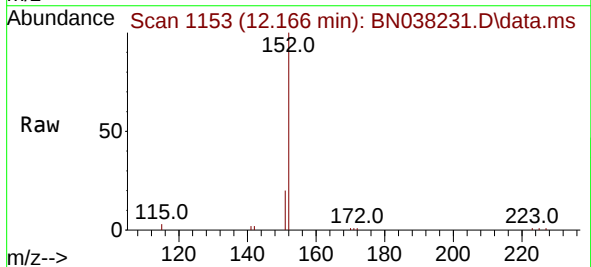



#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.430 min Scan# 14

Delta R.T. -0.000 min


Lab File: BN038231.D

Acq: 01 Dec 2025 18:28

Instrument :

BNA_N

ClientSampleId :

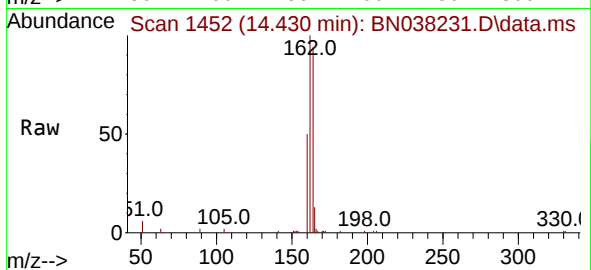




Tgt Ion:164 Resp: 10779

Ion Ratio Lower Upper

164 100

162 106.8 83.8 125.8

160 53.5 41.6 62.4

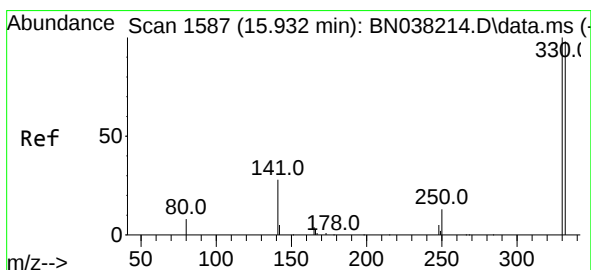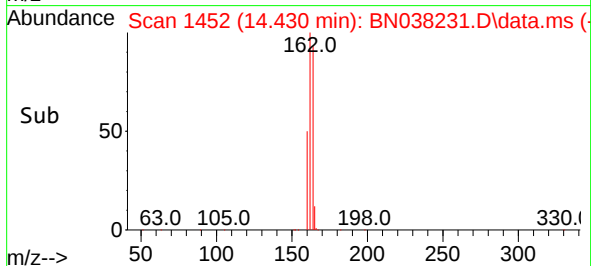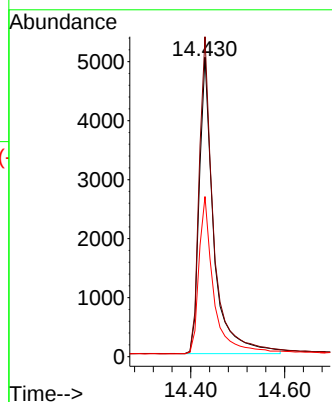

#14

2,4,6-Tribromophenol

Concen: 0.164 ng

RT: 15.944 min Scan# 1588

Delta R.T. 0.012 min

Lab File: BN038231.D

Acq: 01 Dec 2025 18:28




Tgt Ion:330 Resp: 556


Ion Ratio Lower Upper

330 100

332 95.7 77.8 116.6


141 43.3 33.0 49.4

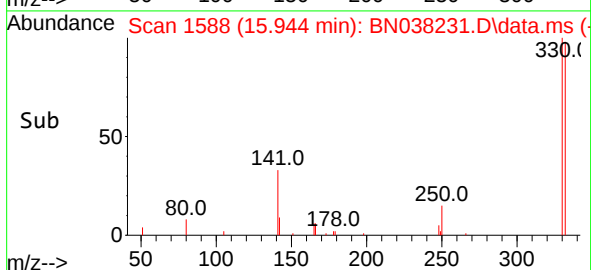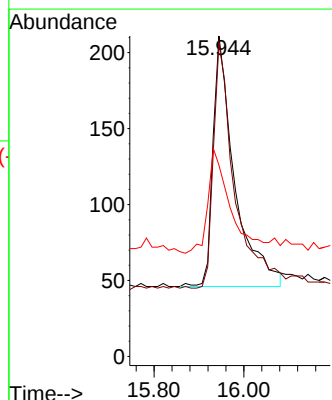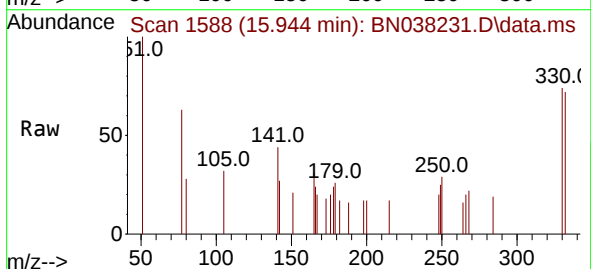



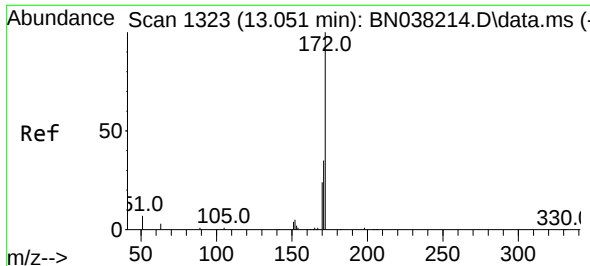


#15
2-Fluorobiphenyl
Concen: 0.391 ng
RT: 13.051 min Scan# 11
Delta R.T. 0.000 min
Lab File: BN038231.D
Acq: 01 Dec 2025 18:28

Instrument :
BNA_N
ClientSampleId :



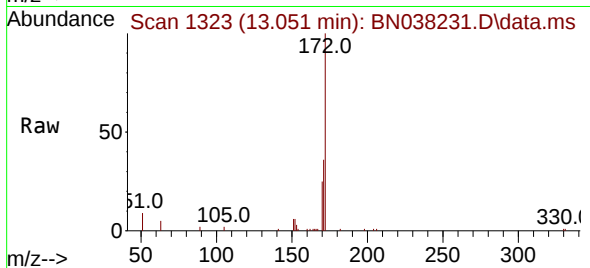



Tgt Ion:172 Resp: 16277
Ion Ratio Lower Upper
172 100
171 36.2 28.1 42.1
170 25.0 19.1 28.7

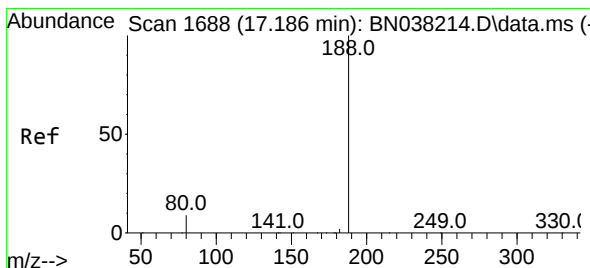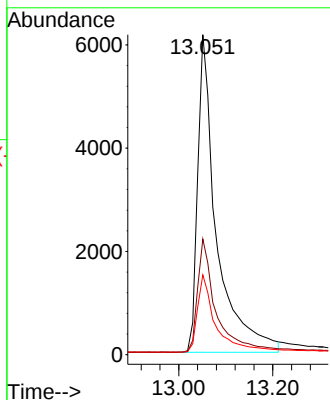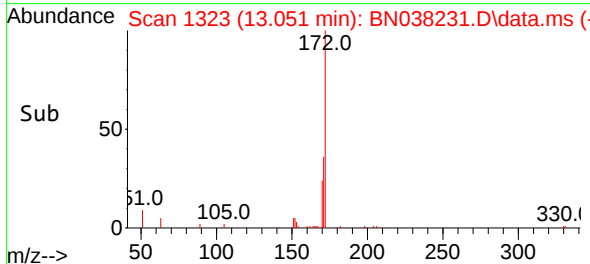

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.186 min Scan# 1688
Delta R.T. -0.000 min
Lab File: BN038231.D
Acq: 01 Dec 2025 18:28

Tgt Ion:188 Resp: 14873
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 14.2 7.7 11.5#


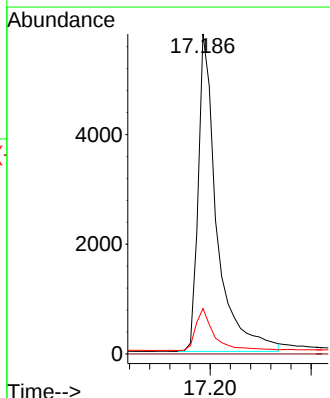
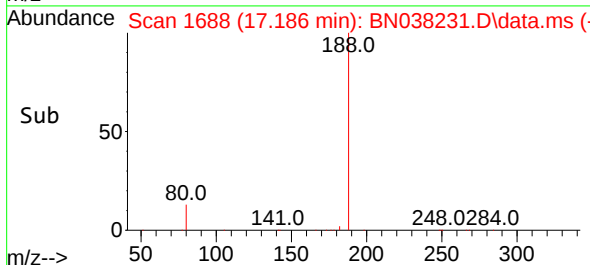
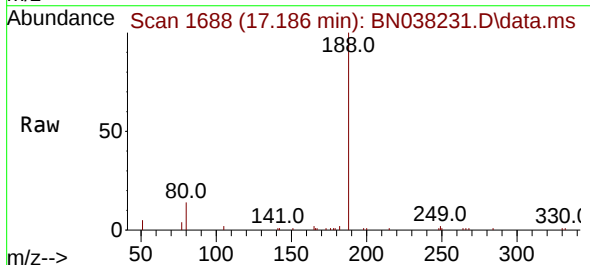




#20
4,6-Dinitro-2-methylphenol
Concen: 0.173 ng
RT: 15.572 min Scan# 1
Delta R.T. 0.000 min
Lab File: BN038231.D
Acq: 01 Dec 2025 18:28




Instrument :
BNA_N
ClientSampleId :


Tgt Ion:198 Resp: 1
Ion Ratio Lower Upper
198 100
51 606.3 205.1 307.7#
105 189.6 61.6 92.4#

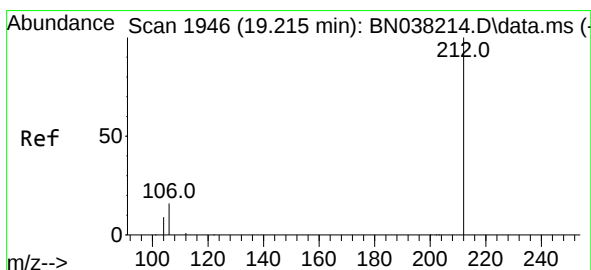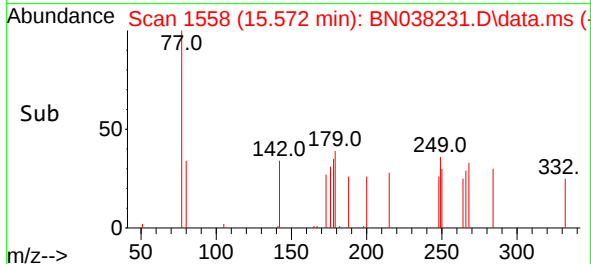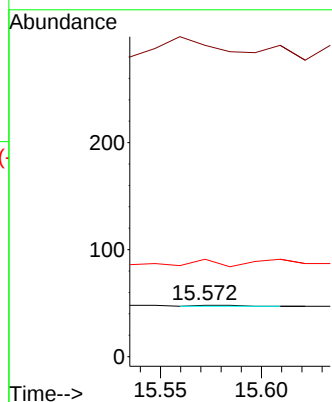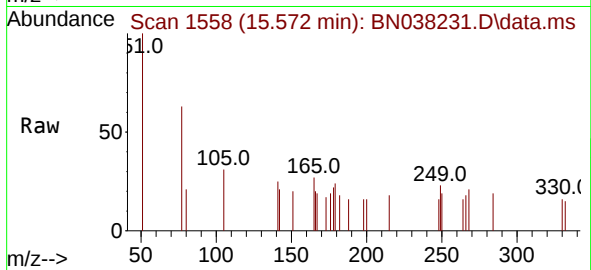

#27
Fluoranthene-d10
Concen: 0.364 ng
RT: 19.220 min Scan# 1947
Delta R.T. 0.005 min
Lab File: BN038231.D
Acq: 01 Dec 2025 18:28


Tgt Ion:212 Resp: 11729
Ion Ratio Lower Upper
212 100
106 16.9 12.7 19.1
104 10.0 7.3 10.9

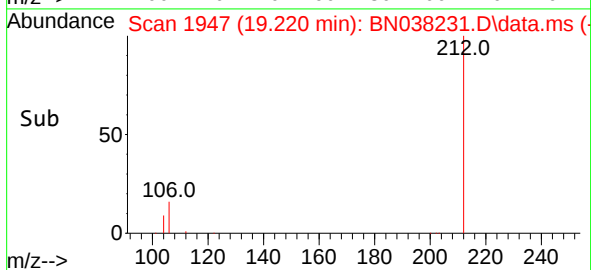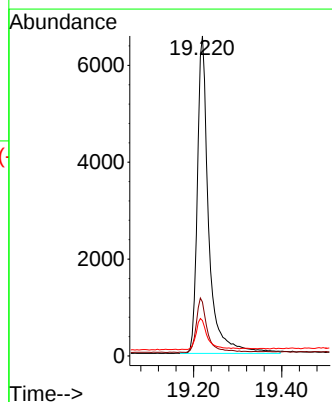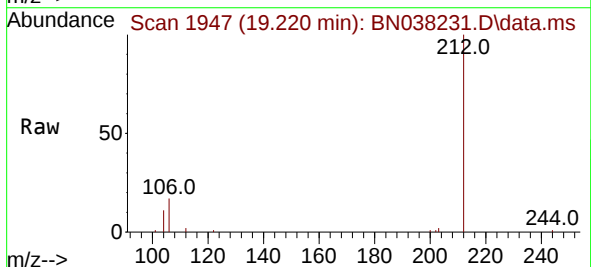






#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.375 min Scan# 21
Delta R.T. 0.009 min
Lab File: BN038231.D
Acq: 01 Dec 2025 18:28

Instrument :
BNA_N
ClientSampleId :







Tgt Ion:240 Resp: 10479
Ion Ratio Lower Upper
240 100
120 18.6 18.1 27.1
236 30.0 24.2 36.4

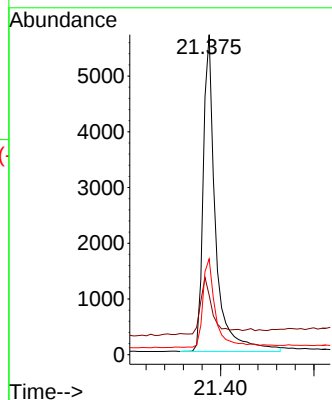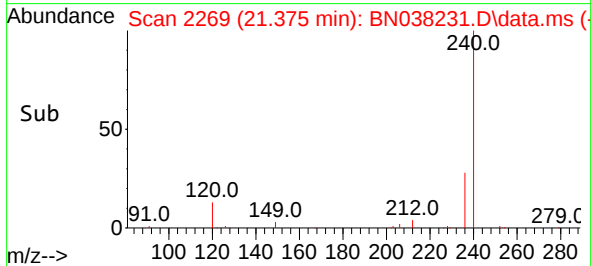

#31
Terphenyl-d14
Concen: 0.350 ng
RT: 19.819 min Scan# 2076
Delta R.T. -0.000 min
Lab File: BN038231.D
Acq: 01 Dec 2025 18:28


Tgt Ion:244 Resp: 8472
Ion Ratio Lower Upper
244 100
212 10.6 7.7 11.5
122 19.4 13.6 20.4

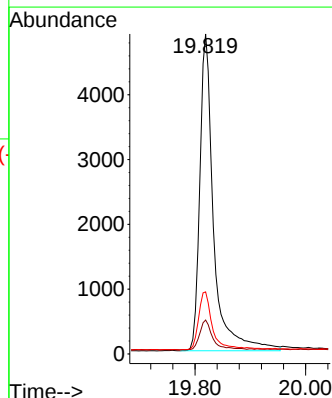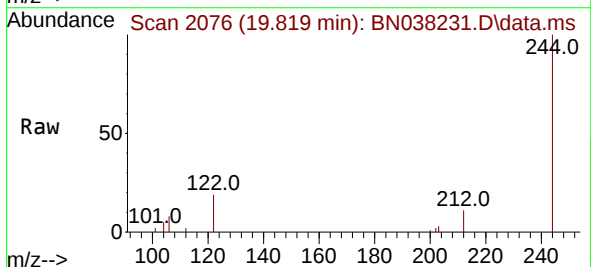

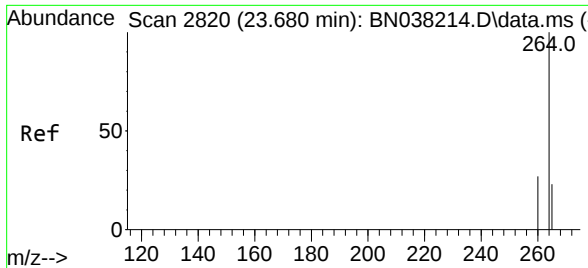

#35
 Perylene-d12
 Concen: 0.400 ng
 RT: 23.680 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: BN038231.D
 Acq: 01 Dec 2025 18:28

Instrument :
 BNA_N
 ClientSampleId :

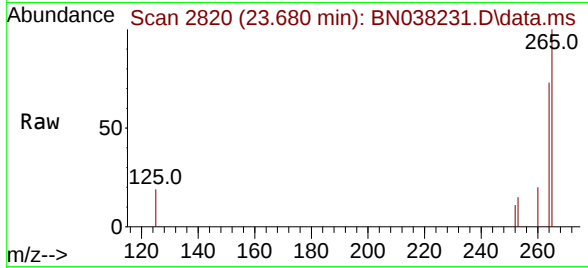

Tgt Ion:264 Resp: 10853

Ion	Ratio	Lower	Upper
264	100		
260	27.9	21.7	32.5
265	137.9	98.0	147.0

