

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120125\
 Data File : BN038247.D
 Acq On : 02 Dec 2025 04:08
 Operator : RC/JU
 Sample : Q3692-03
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Dec 02 04:35:14 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN112725.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 28 21:04:10 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.768	152	8471	0.400	ng	0.00
7) Naphthalene-d8	10.562	136	24467	0.400	ng	#-0.01
13) Acenaphthene-d10	14.430	164	11133	0.400	ng	0.00
19) Phenanthrene-d10	17.173	188	17137	0.400	ng	#-0.01
29) Chrysene-d12	21.366	240	13919	0.400	ng	0.00
35) Perylene-d12	23.671	264	14663	0.400	ng	# 0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.341	112	3110	0.157	ng	0.00
5) Phenol-d6	6.930	99	2084	0.084	ng	0.00
8) Nitrobenzene-d5	8.918	82	6829	0.349	ng	0.00
11) 2-Methylnaphthalene-d10	12.162	152	10619	0.306	ng	0.00
14) 2,4,6-Tribromophenol	15.920	330	1388	0.396	ng	-0.01
15) 2-Fluorobiphenyl	13.040	172	16634	0.387	ng	-0.01
27) Fluoranthene-d10	19.215	212	16582	0.446	ng	0.00
31) Terphenyl-d14	19.815	244	12878	0.401	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.247	88	489	0.055	ng	# 34
3) n-Nitrosodimethylamine	3.499	42	741	0.067	ng	# 1
20) 4,6-Dinitro-2-methylph...	15.572	198	4	0.174	ng	# 1
34) Bis(2-ethylhexyl)phtha...	21.286	149	3405	0.132	ng	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120125\
Data File : BN038247.D
Acq On : 02 Dec 2025 04:08
Operator : RC/JU
Sample : Q3692-03
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :


Quant Time: Dec 02 04:35:14 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN112725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 28 21:04:10 2025
Response via : Initial Calibration

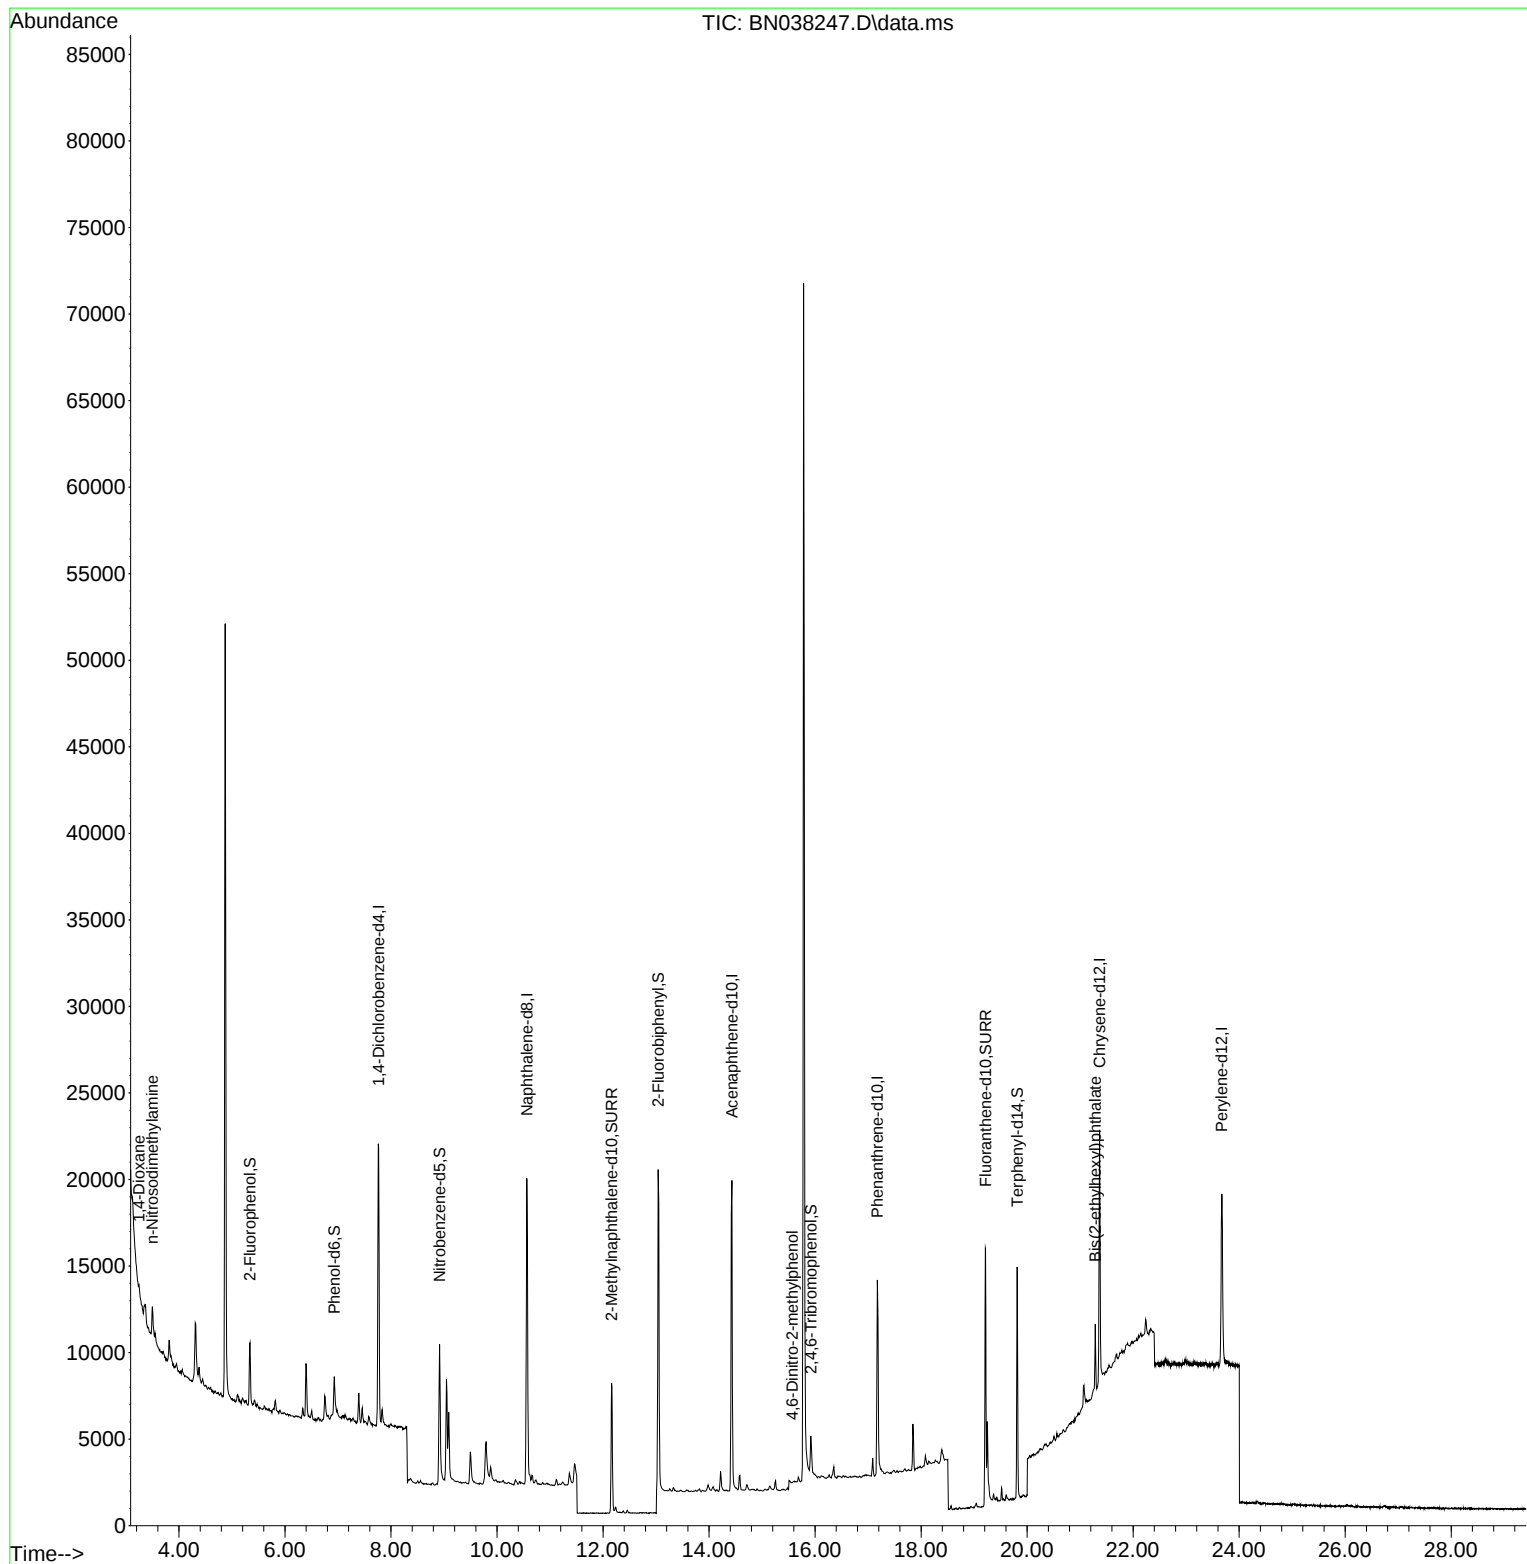



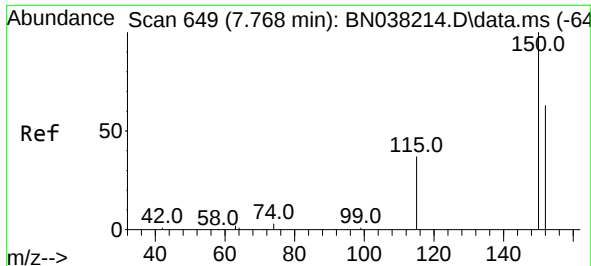


#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.768 min Scan# 64
 Delta R.T. -0.000 min
 Lab File: BN038247.D
 Acq: 02 Dec 2025 04:08


Instrument :
 BNA_N
 ClientSampleId :

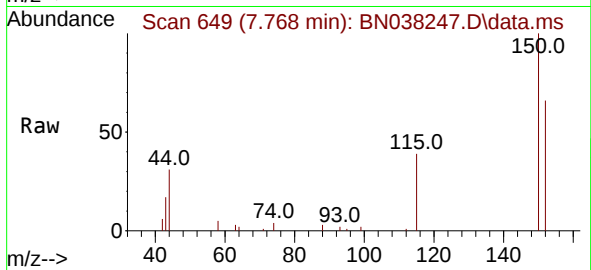



Tgt Ion:152 Resp: 8471
 Ion Ratio Lower Upper
 152 100
 150 151.4 125.3 187.9
 115 58.6 49.0 73.4

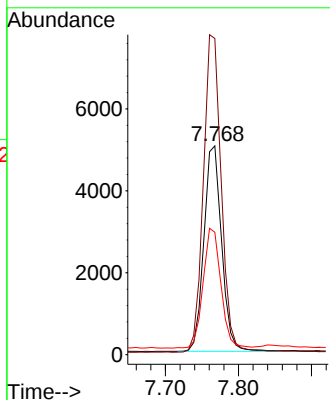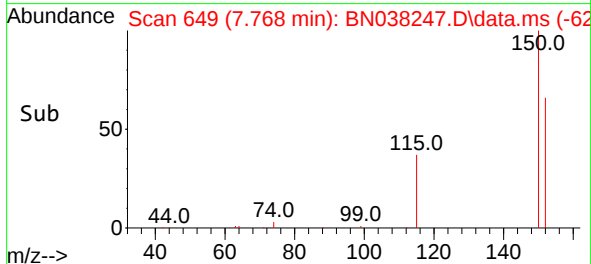


#2
 1,4-Dioxane
 Concen: 0.055 ng
 RT: 3.247 min Scan# 23
 Delta R.T. -0.007 min
 Lab File: BN038247.D
 Acq: 02 Dec 2025 04:08

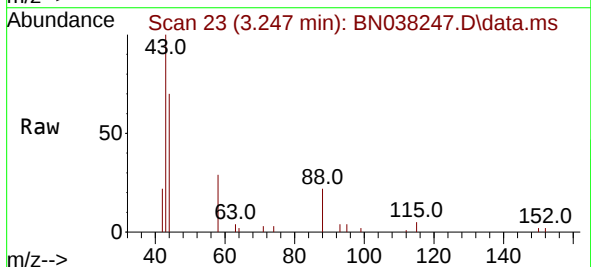

Tgt Ion: 88 Resp: 489
 Ion Ratio Lower Upper
 88 100
 43 0.0 24.8 37.2#
 58 16.2 61.1 91.7#



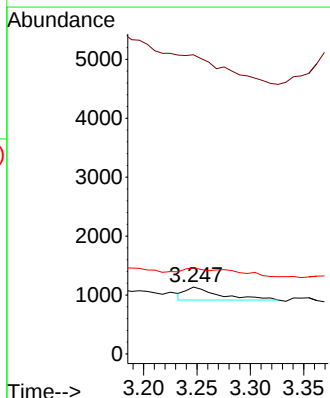



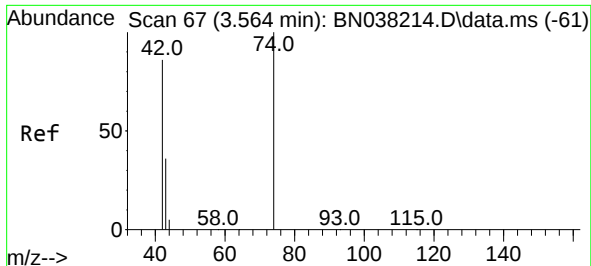

#3
 n-Nitrosodimethylamine
 Concen: 0.067 ng
 RT: 3.499 min Scan# 51
 Delta R.T. -0.065 min
 Lab File: BN038247.D
 Acq: 02 Dec 2025 04:08




Instrument :
 BNA_N
 ClientSampleId :


Tgt Ion: 42 Resp: 741
 Ion Ratio Lower Upper
 42 100
 74 0.0 96.2 144.2#
 44 113.1 8.0 12.0#

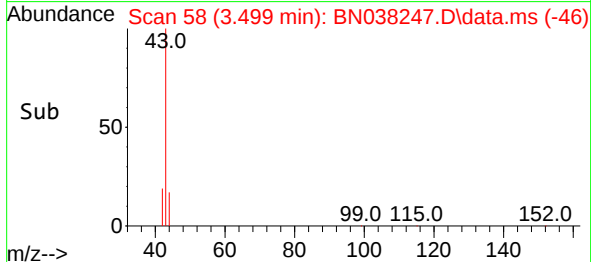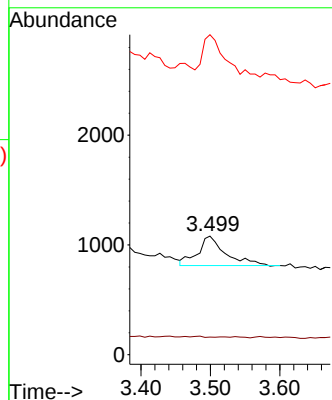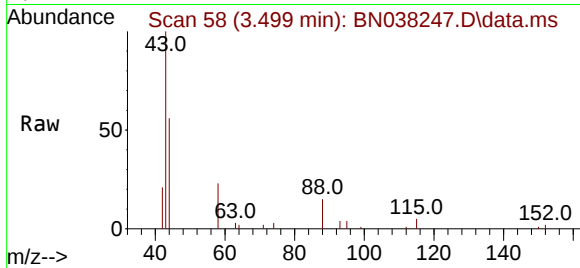

#4
 2-Fluorophenol
 Concen: 0.157 ng
 RT: 5.341 min Scan# 313
 Delta R.T. 0.000 min
 Lab File: BN038247.D
 Acq: 02 Dec 2025 04:08


Tgt Ion: 112 Resp: 3110
 Ion Ratio Lower Upper
 112 100
 64 56.3 45.0 67.4
 63 29.3 23.2 34.8

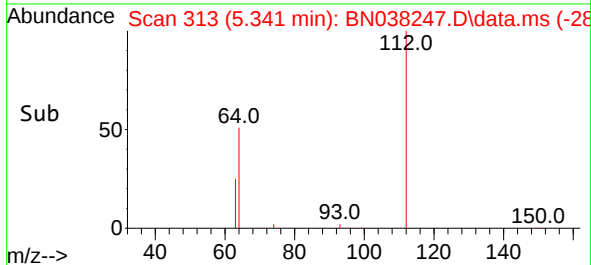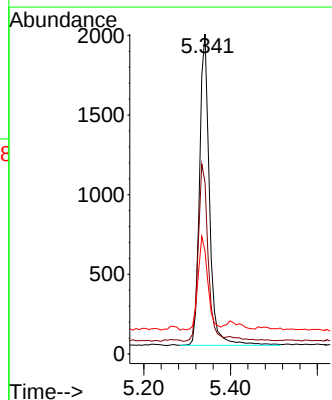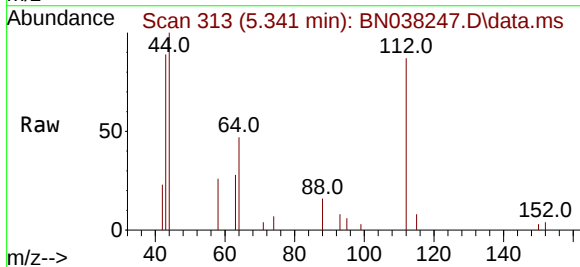






#5
Phenol-d6
Concen: 0.084 ng
RT: 6.930 min Scan# 511
Delta R.T. -0.007 min
Lab File: BN038247.D
Acq: 02 Dec 2025 04:08

Instrument :
BNA_N
ClientSampleId :



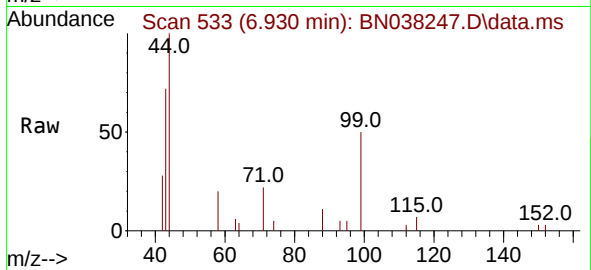



Tgt Ion: 99 Resp: 2084
Ion Ratio Lower Upper
99 100
42 29.8 17.0 25.6#
71 38.5 25.4 38.2#

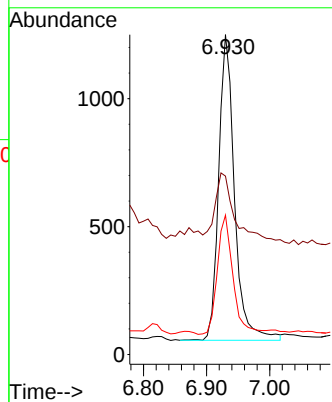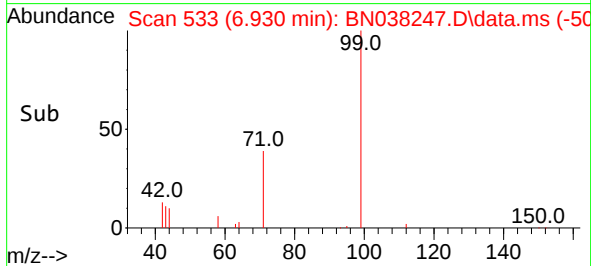

#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.562 min Scan# 935
Delta R.T. -0.011 min
Lab File: BN038247.D
Acq: 02 Dec 2025 04:08


Tgt Ion: 136 Resp: 24467
Ion Ratio Lower Upper
136 100
137 11.5 8.9 13.3
54 9.5 5.4 8.0#
68 7.0 4.1 6.1#

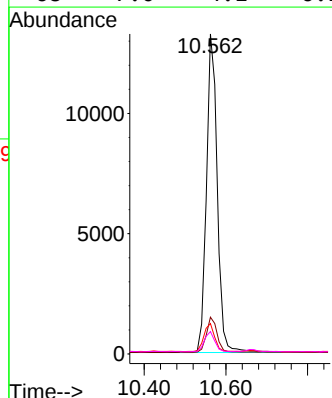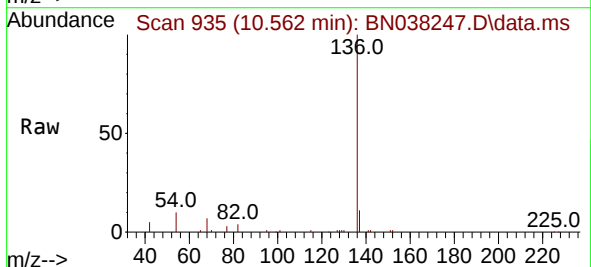



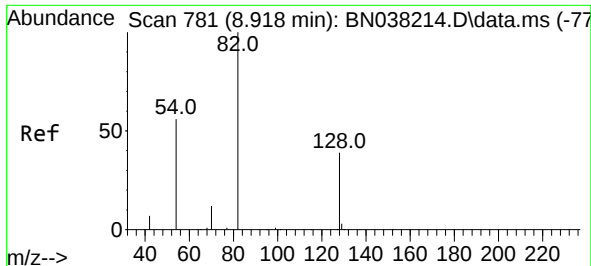


#8
 Nitrobenzene-d5
 Concen: 0.349 ng
 RT: 8.918 min Scan# 781
 Delta R.T. 0.000 min
 Lab File: BN038247.D
 Acq: 02 Dec 2025 04:08

Instrument :
 BNA_N
 ClientSampleId :







Tgt Ion: 82 Resp: 6829
 Ion Ratio Lower Upper
 82 100
 128 44.4 32.6 48.8
 54 54.2 45.4 68.0

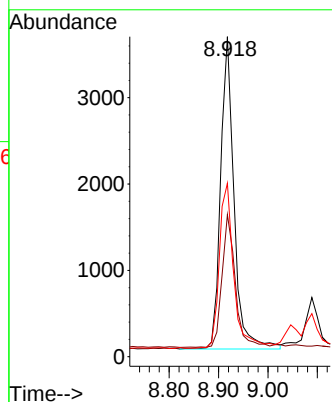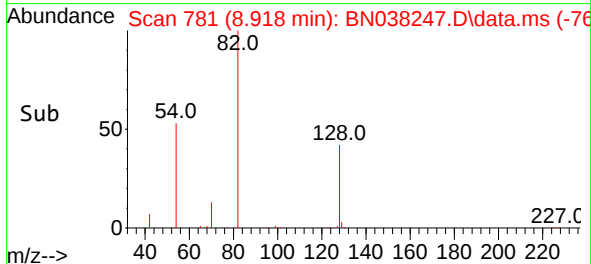

#11
 2-Methylnaphthalene-d10
 Concen: 0.306 ng
 RT: 12.162 min Scan# 1152
 Delta R.T. -0.005 min
 Lab File: BN038247.D
 Acq: 02 Dec 2025 04:08

Tgt Ion: 152 Resp: 10619
 Ion Ratio Lower Upper
 152 100
 151 20.9 16.7 25.1

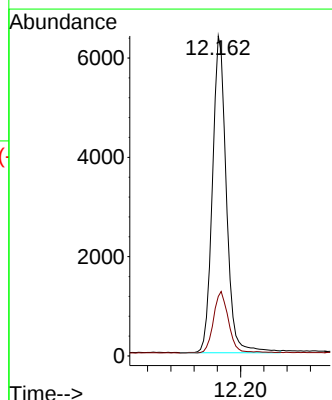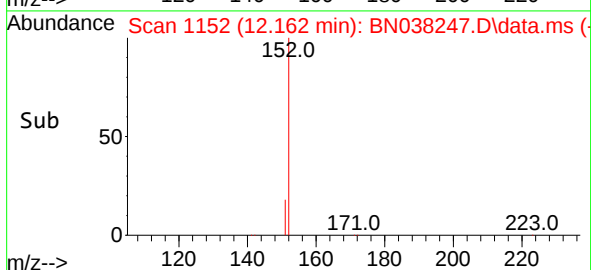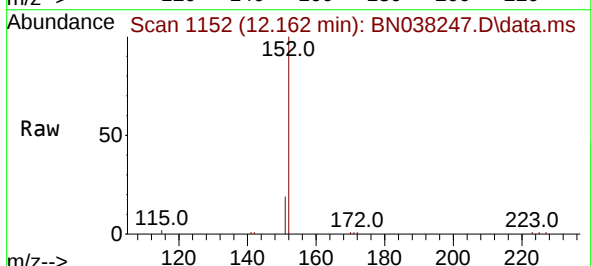



#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.430 min Scan# 14

Delta R.T. 0.000 min


Lab File: BN038247.D

Acq: 02 Dec 2025 04:08

Instrument :

BNA_N

ClientSampleId :

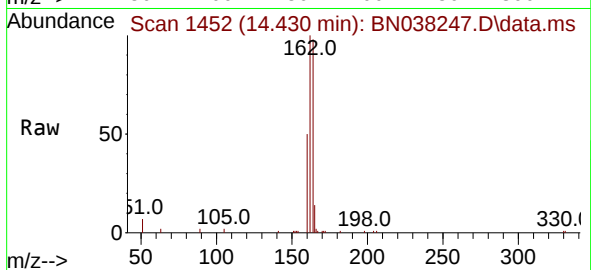




Tgt Ion:164 Resp: 11133

Ion Ratio Lower Upper

164 100

162 101.8 83.8 125.8

160 50.4 41.6 62.4

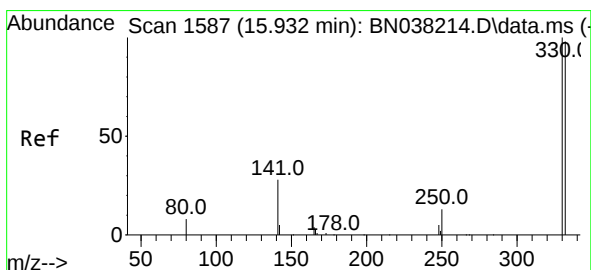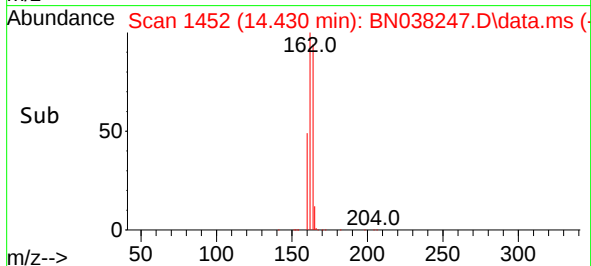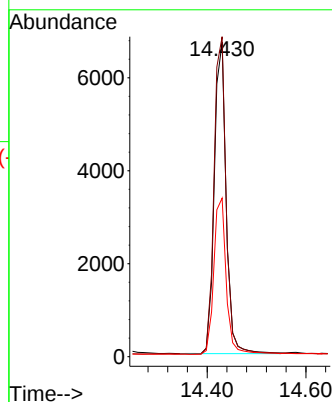

#14

2,4,6-Tribromophenol

Concen: 0.396 ng

RT: 15.920 min Scan# 1586

Delta R.T. -0.012 min

Lab File: BN038247.D

Acq: 02 Dec 2025 04:08




Tgt Ion:330 Resp: 1388


Ion Ratio Lower Upper

330 100

332 94.3 77.8 116.6

141 41.5 33.0 49.4


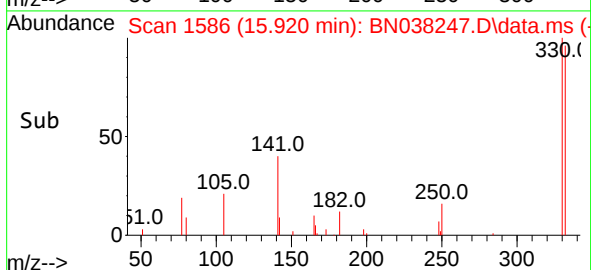
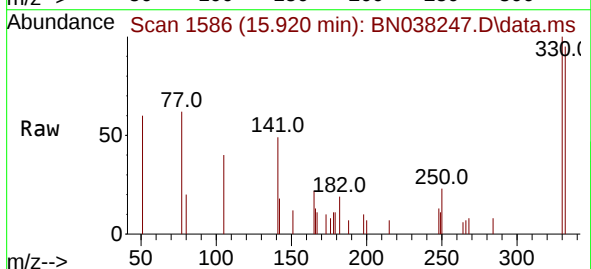
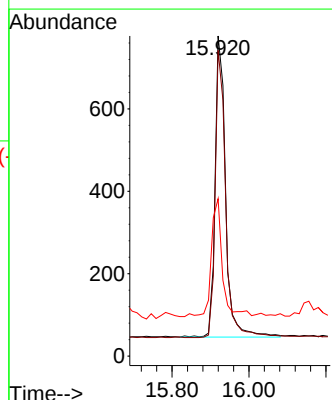


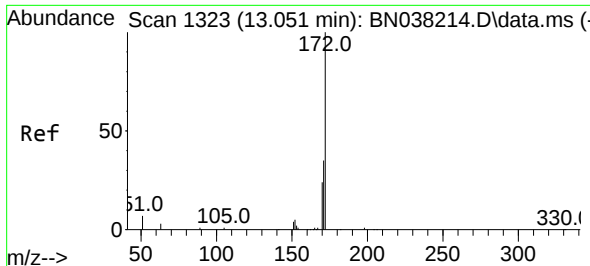

#15
2-Fluorobiphenyl
Concen: 0.387 ng
RT: 13.040 min Scan# 11
Delta R.T. -0.011 min
Lab File: BN038247.D
Acq: 02 Dec 2025 04:08




Instrument :
BNA_N
ClientSampleId :


Tgt Ion:172 Resp: 16634
Ion Ratio Lower Upper
172 100
171 36.2 28.1 42.1
170 24.5 19.1 28.7

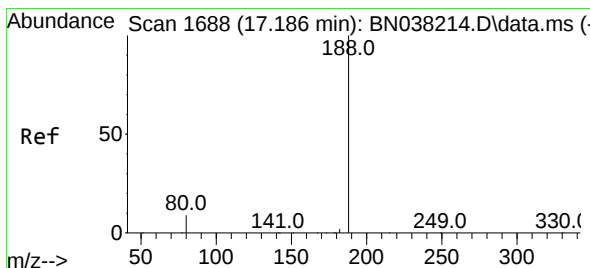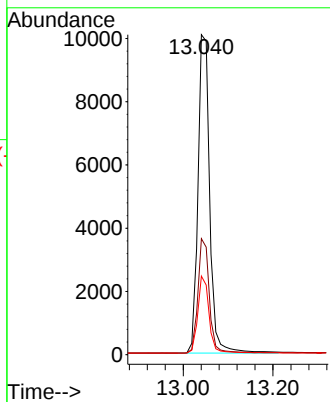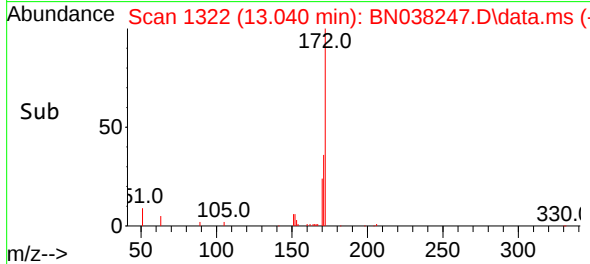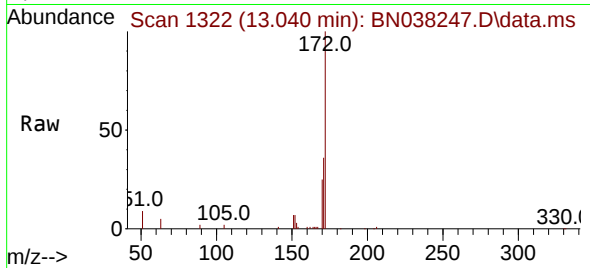

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.173 min Scan# 1687
Delta R.T. -0.012 min
Lab File: BN038247.D
Acq: 02 Dec 2025 04:08

Tgt Ion:188 Resp: 17137
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 15.0 7.7 11.5#


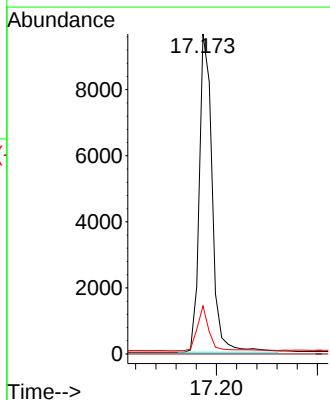
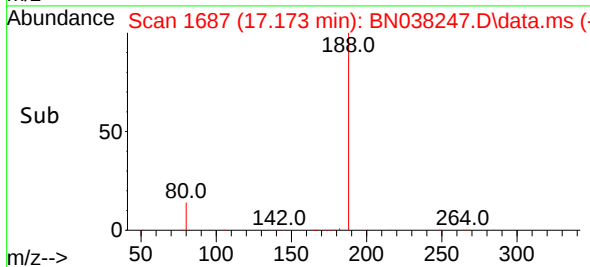
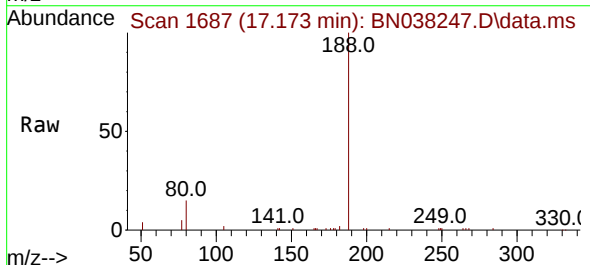




#20
4,6-Dinitro-2-methylphenol
Concen: 0.174 ng
RT: 15.572 min Scan# 11
Delta R.T. 0.000 min
Lab File: BN038247.D
Acq: 02 Dec 2025 04:08




Instrument :
BNA_N
ClientSampleId :


Tgt Ion:198 Resp: 4
Ion Ratio Lower Upper
198 100
51 829.4 205.1 307.7#
105 284.3 61.6 92.4#

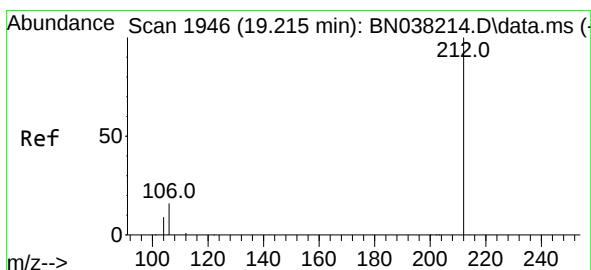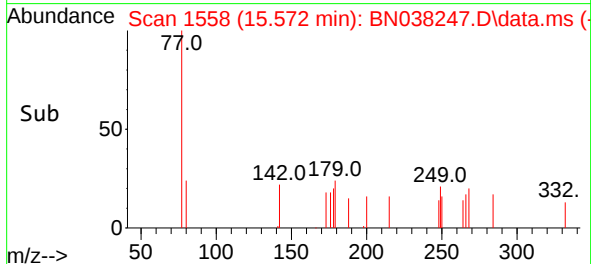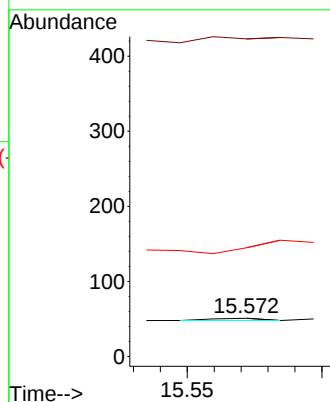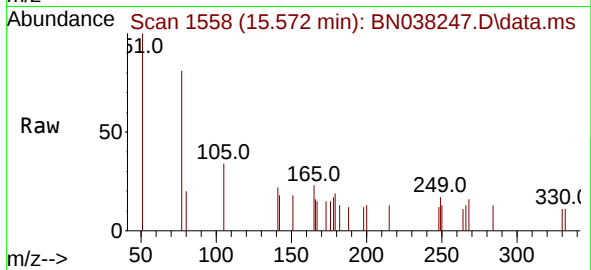

#27
Fluoranthene-d10
Concen: 0.446 ng
RT: 19.215 min Scan# 1946
Delta R.T. 0.000 min
Lab File: BN038247.D
Acq: 02 Dec 2025 04:08


Tgt Ion:212 Resp: 16582
Ion Ratio Lower Upper
212 100
106 16.4 12.7 19.1
104 9.4 7.3 10.9

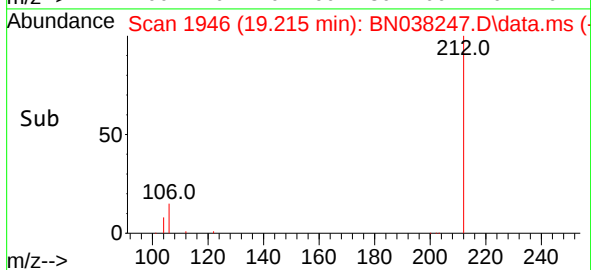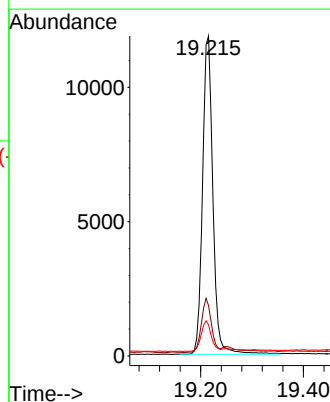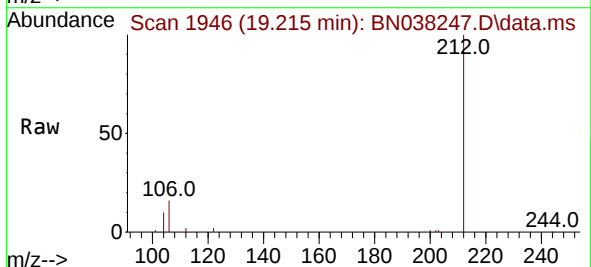



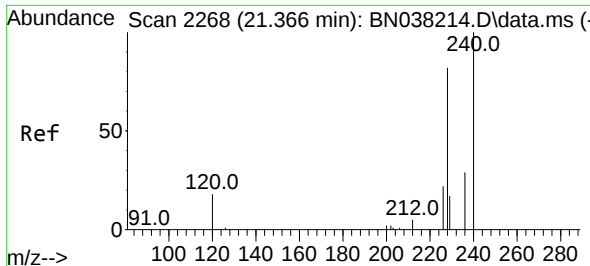


#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.366 min Scan# 21
Delta R.T. 0.000 min
Lab File: BN038247.D
Acq: 02 Dec 2025 04:08


Instrument :
BNA_N
ClientSampleId :

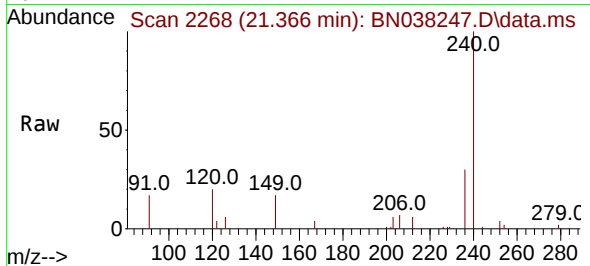



Tgt Ion	Ratio	Lower	Upper
240	100		
120	19.7	18.1	27.1
236	29.6	24.2	36.4

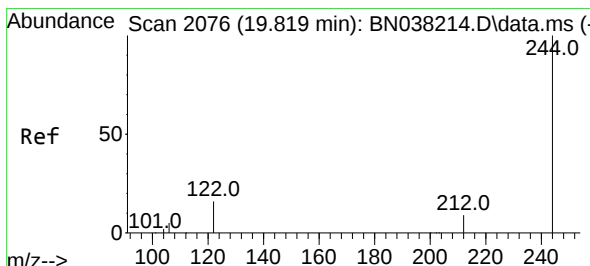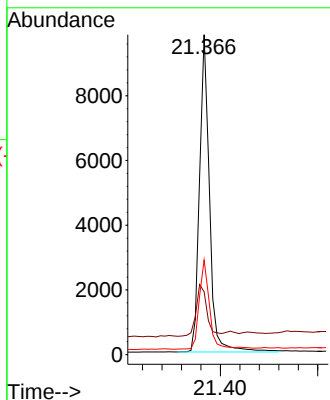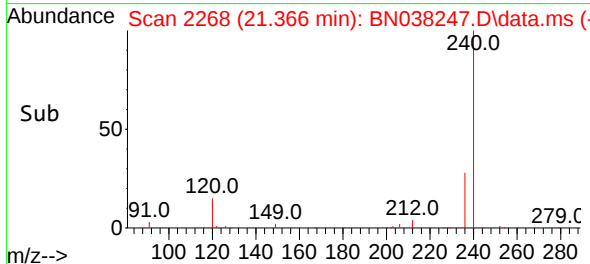


#31
Terphenyl-d14
Concen: 0.401 ng
RT: 19.815 min Scan# 2075
Delta R.T. -0.005 min
Lab File: BN038247.D
Acq: 02 Dec 2025 04:08

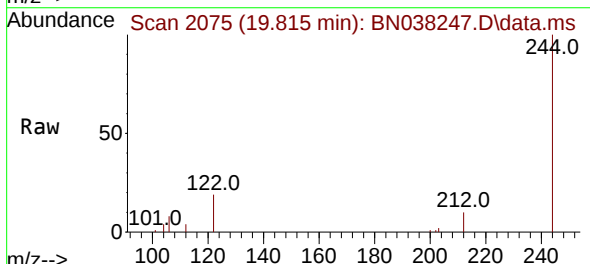

Tgt Ion	Ratio	Lower	Upper
244	100		
212	9.6	7.7	11.5
122	18.6	13.6	20.4



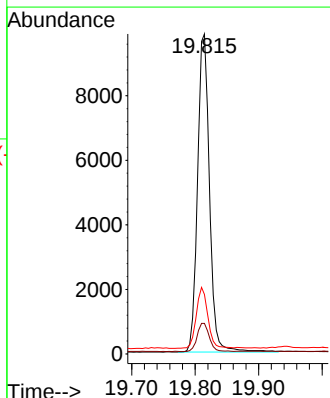
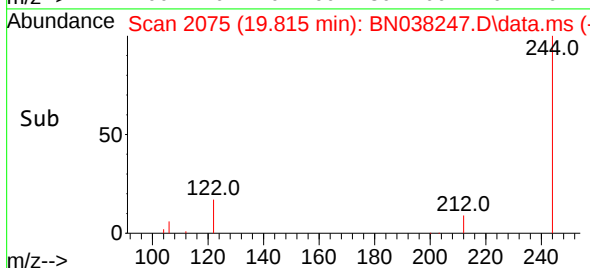


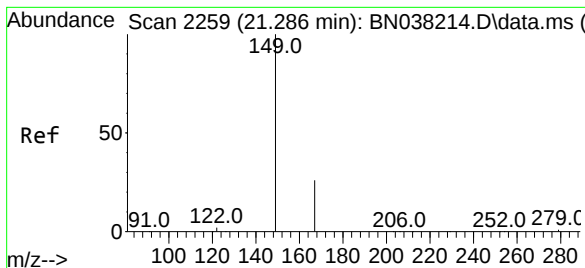

#34
 Bis(2-ethylhexyl)phthalate
 Concen: 0.132 ng
 RT: 21.286 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: BN038247.D
 Acq: 02 Dec 2025 04:08

Instrument :
 BNA_N
 ClientSampleId :

Tgt Ion:149 Resp: 3405
 Ion Ratio Lower Upper
 149 100
 167 24.6 20.7 31.1
 279 3.6 2.5 3.7

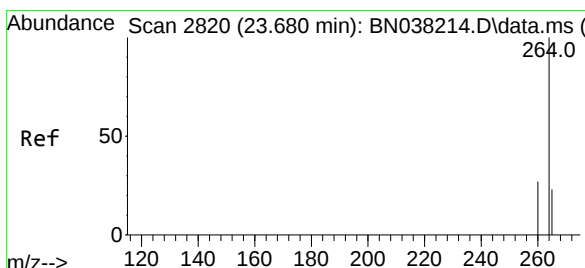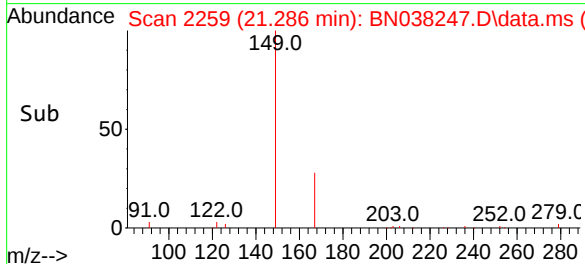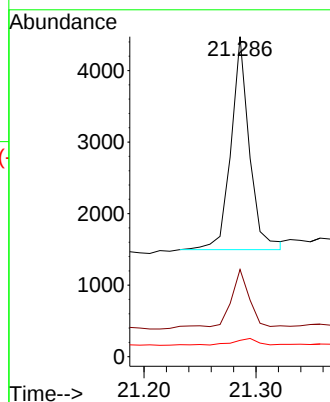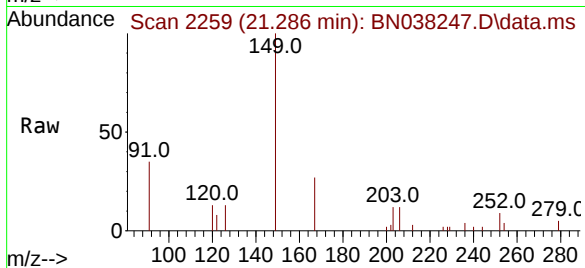

#35
 Perylene-d12
 Concen: 0.400 ng
 RT: 23.671 min Scan# 2817
 Delta R.T. -0.009 min
 Lab File: BN038247.D
 Acq: 02 Dec 2025 04:08

Tgt Ion:264 Resp: 14663
 Ion Ratio Lower Upper
 264 100
 260 27.5 21.7 32.5
 265 97.3 98.0 147.0#

