
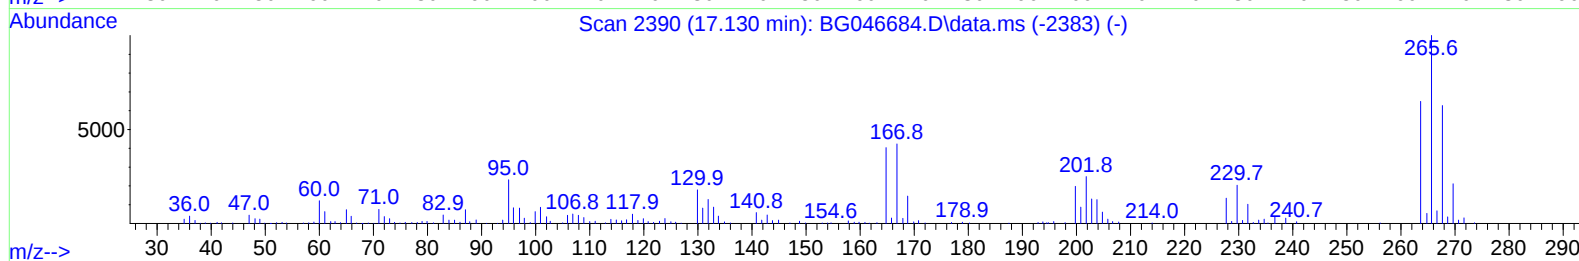
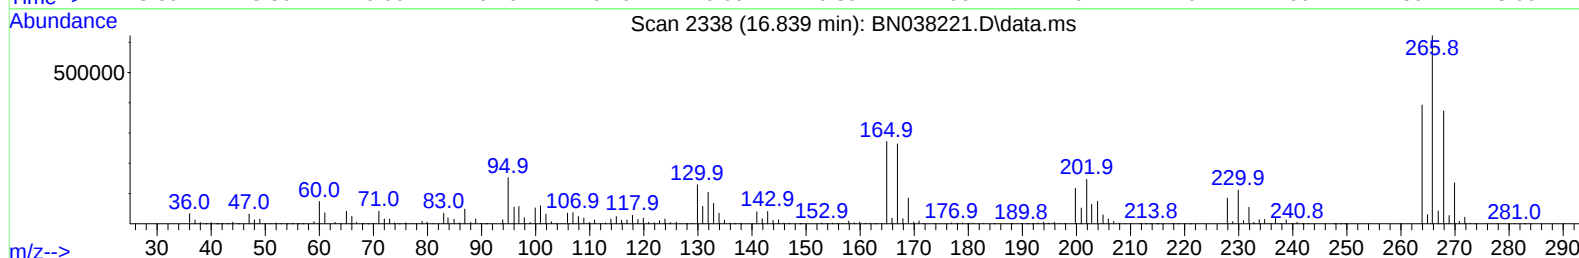


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120125\
Data File : BN038221.D
Acq On : 01 Dec 2025 09:44
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 01 10:15:18 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 01 10:15:10 2025
Response via : Initial Calibration

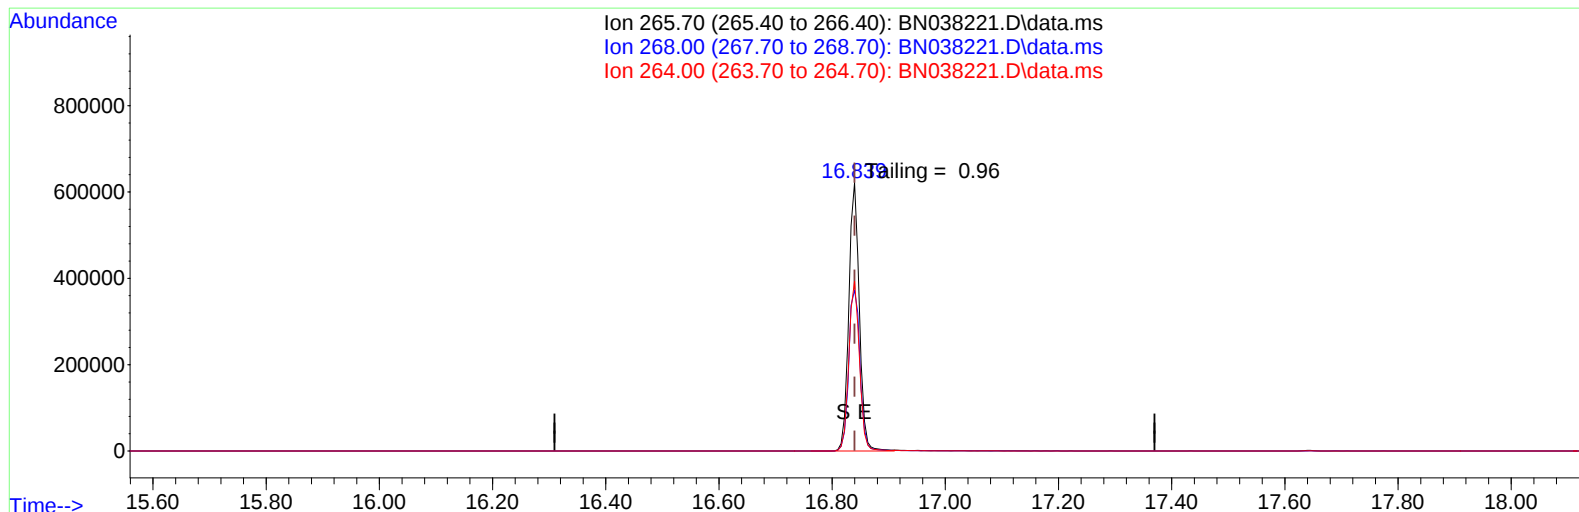

TIC: BN038221.D\data.ms

(70) Pentachlorophenol (C)




16.839min (0.000) 277.71 ng

response 805839

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	59.99
264.00	61.60	63.18
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120125\
Data File : BN038221.D
Acq On : 01 Dec 2025 09:44
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 01 10:15:18 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 01 10:15:10 2025
Response via : Initial Calibration

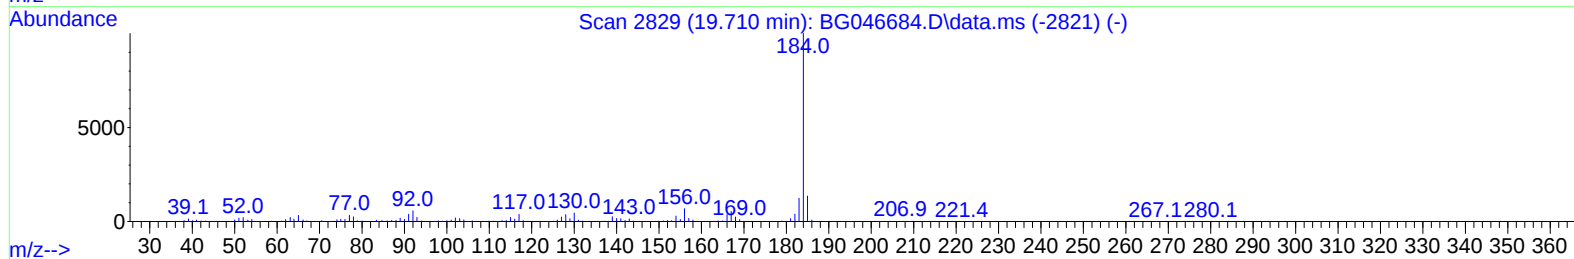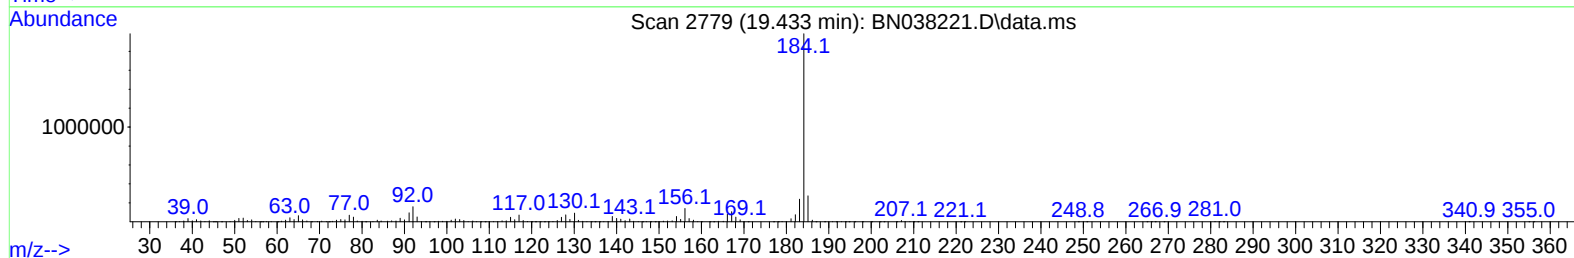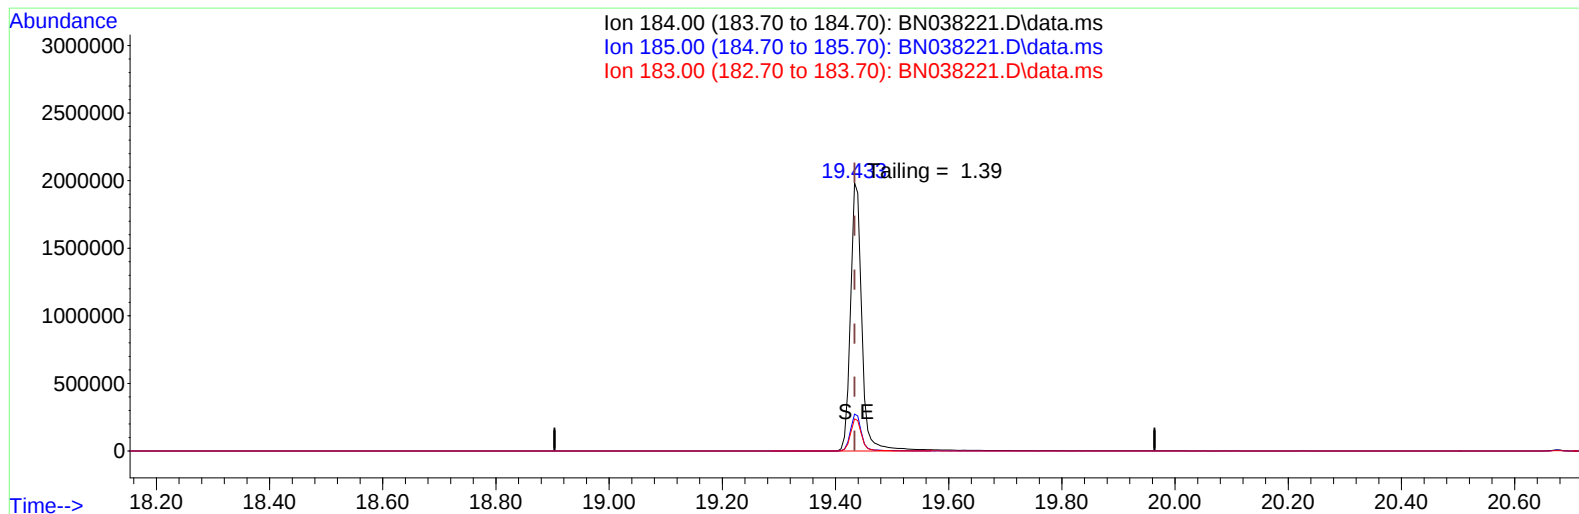

TIC: BN038221.D\data.ms

(77) Benzidine

19.433min (0.000) 0.00 ng

response 2788820

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.78
183.00	13.20	12.01
0.00	0.00	0.00