

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120125\
 Data File : BN038238.D
 Acq On : 01 Dec 2025 22:42
 Operator : RC/JU
 Sample : PB170712BSD
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 PB170712BSD

Quant Time: Dec 04 12:03:40 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN112725.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 28 21:04:10 2025
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.768	152	9081	0.400	ng	0.00
7) Naphthalene-d8	10.562	136	25072	0.400	ng	#-0.01
13) Acenaphthene-d10	14.430	164	10824	0.400	ng	0.00
19) Phenanthrene-d10	17.173	188	16101	0.400	ng	#-0.01
29) Chrysene-d12	21.366	240	14003	0.400	ng	0.00
35) Perylene-d12	23.671	264	15858	0.400	ng	# 0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.341	112	8650	0.408	ng	0.00
5) Phenol-d6	6.930	99	9418	0.355	ng	0.00
8) Nitrobenzene-d5	8.918	82	8050	0.402	ng	0.00
11) 2-Methylnaphthalene-d10	12.162	152	12286	0.345	ng	0.00
14) 2,4,6-Tribromophenol	15.932	330	1178	0.346	ng	0.00
15) 2-Fluorobiphenyl	13.051	172	17945	0.429	ng	0.00
27) Fluoranthene-d10	19.215	212	13574	0.389	ng	0.00
31) Terphenyl-d14	19.815	244	10255	0.317	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.254	88	2880	0.301	ng	# 65
3) n-Nitrosodimethylamine	3.557	42	4504	0.382	ng	# 97
6) bis(2-Chloroethyl)ether	7.183	93	9517	0.375	ng	96
9) Naphthalene	10.616	128	24829	0.357	ng	100
10) Hexachlorobutadiene	10.915	225	4570	0.386	ng	# 99
12) 2-Methylnaphthalene	12.238	142	13648	0.298	ng	98
16) Acenaphthylene	14.142	152	18881	0.390	ng	100
17) Acenaphthene	14.484	154	11726	0.348	ng	98
18) Fluorene	15.478	166	14142	0.324	ng	99
20) 4,6-Dinitro-2-methylph...	15.560	198	159	0.266	ng	# 58
21) 4-Bromophenyl-phenylether	16.379	248	3955	0.355	ng	99
22) Hexachlorobenzene	16.491	284	4649	0.339	ng	98
23) Atrazine	16.640	200	2811	0.395	ng	# 93
24) Pentachlorophenol	16.838	266	2524	0.671	ng	99
25) Phenanthrene	17.223	178	17571	0.348	ng	98
26) Anthracene	17.310	178	16311	0.378	ng	99
28) Fluoranthene	19.243	202	18836	0.387	ng	100
30) Pyrene	19.606	202	19886	0.284	ng	99
32) Benzo(a)anthracene	21.349	228	19111	0.403	ng	99
33) Chrysene	21.402	228	20271	0.362	ng	99
34) Bis(2-ethylhexyl)phtha...	21.286	149	11826	0.455	ng	# 98
36) Indeno(1,2,3-cd)pyrene	26.022	276	28125	0.383	ng	99
37) Benzo(b)fluoranthene	22.975	252	21654	0.333	ng	98
38) Benzo(k)fluoranthene	23.019	252	22543	0.333	ng	99
39) Benzo(a)pyrene	23.572	252	21487	0.394	ng	94
40) Dibenzo(a,h)anthracene	26.039	278	21580	0.388	ng	98
41) Benzo(g,h,i)perylene	26.735	276	23394	0.352	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120125\
Data File : BN038238.D
Acq On : 01 Dec 2025 22:42
Operator : RC/JU
Sample : PB170712BSD
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PB170712BSD


Quant Time: Dec 04 12:03:40 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN112725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 28 21:04:10 2025
Response via : Initial Calibration

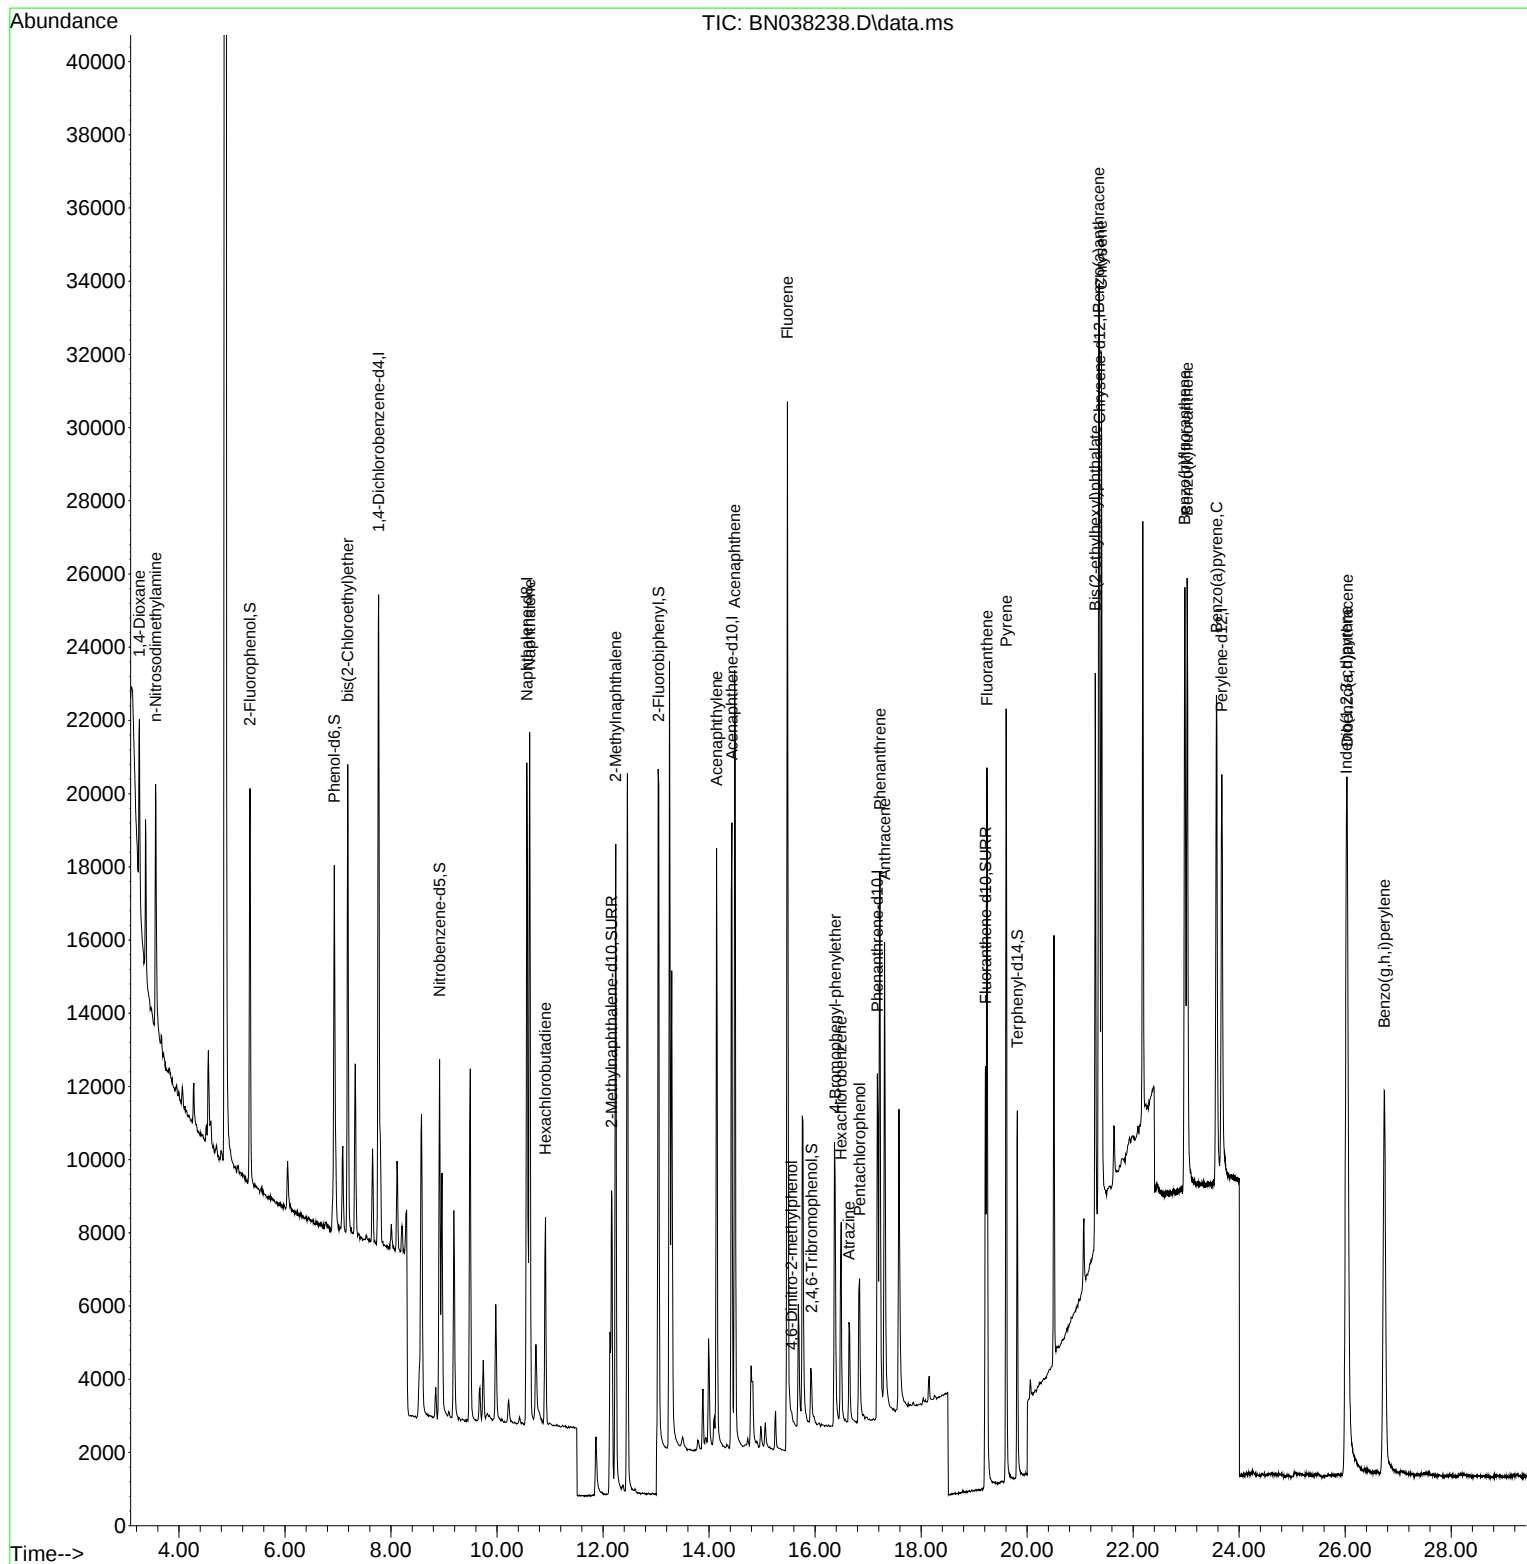



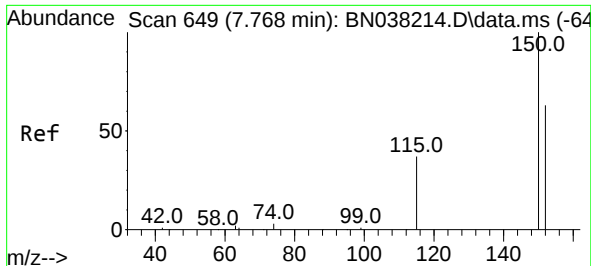


#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.768 min Scan# 64
 Delta R.T. -0.000 min
 Lab File: BN038238.D
 Acq: 01 Dec 2025 22:42


Instrument :
 BNA_N
 ClientSampleId :
 PB170712BSD

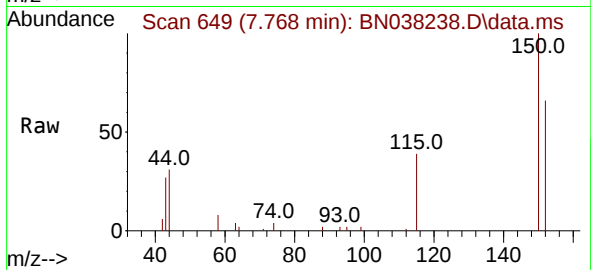



Tgt Ion:152 Resp: 9081
 Ion Ratio Lower Upper
 152 100
 150 152.2 125.3 187.9
 115 59.6 49.0 73.4

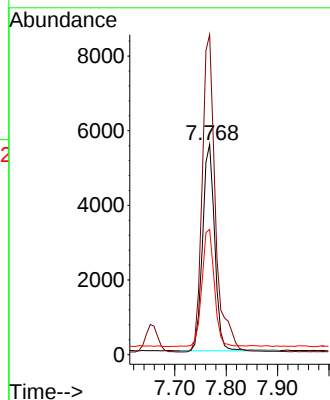


#2
 1,4-Dioxane
 Concen: 0.301 ng
 RT: 3.254 min Scan# 24
 Delta R.T. 0.000 min
 Lab File: BN038238.D
 Acq: 01 Dec 2025 22:42

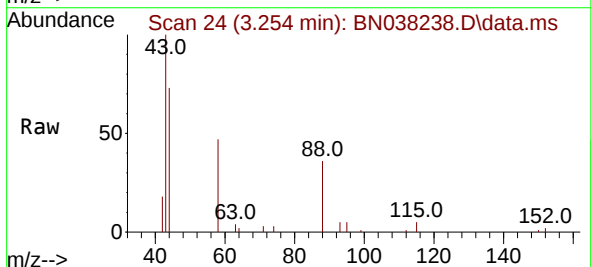

Tgt Ion: 88 Resp: 2880
 Ion Ratio Lower Upper
 88 100
 43 81.3 24.8 37.2#
 58 87.1 61.1 91.7



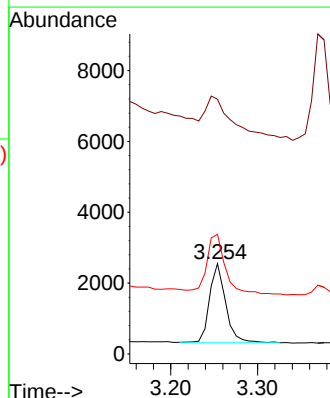



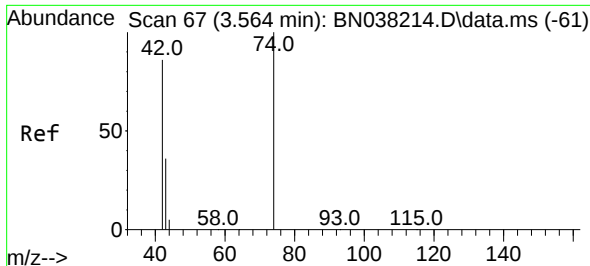

#3
n-Nitrosodimethylamine
Concen: 0.382 ng
RT: 3.557 min Scan# 61
Delta R.T. -0.007 min
Lab File: BN038238.D
Acq: 01 Dec 2025 22:42




Instrument :
BNA_N
ClientSampleId :
PB170712BSD


Tgt Ion: 42 Resp: 4504
Ion Ratio Lower Upper
42 100
74 120.0 96.2 144.2
44 23.7 8.0 12.0#

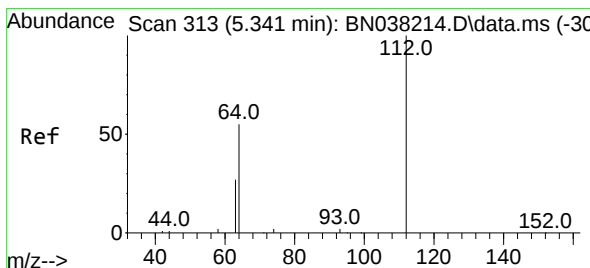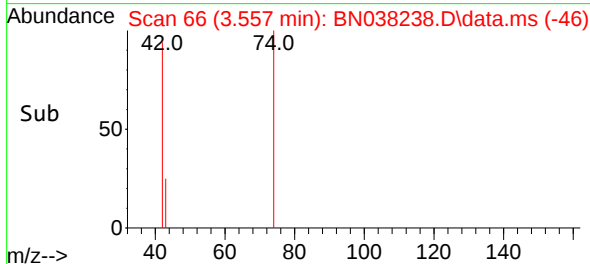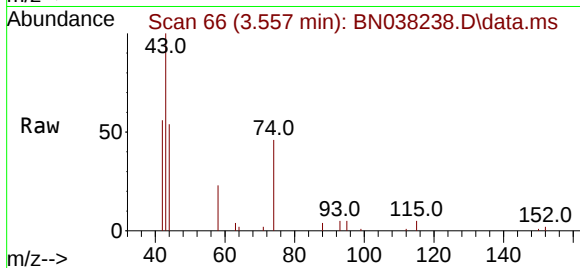

#4
2-Fluorophenol
Concen: 0.408 ng
RT: 5.341 min Scan# 313
Delta R.T. 0.000 min
Lab File: BN038238.D
Acq: 01 Dec 2025 22:42

Tgt Ion: 112 Resp: 8650
Ion Ratio Lower Upper
112 100
64 56.2 45.0 67.4
63 30.5 23.2 34.8


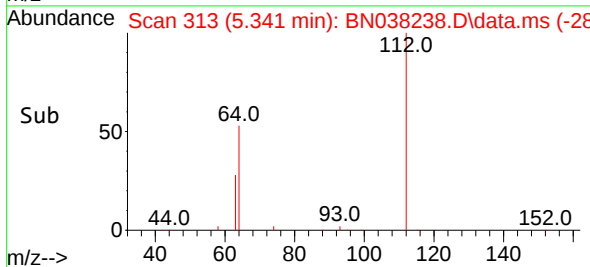

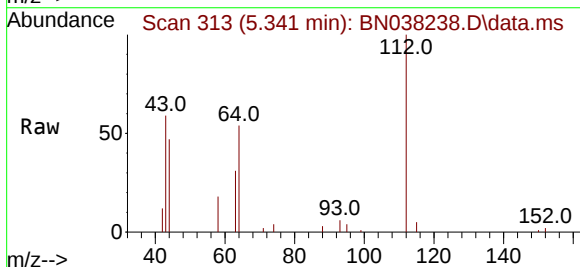




#5
Phenol-d6
Concen: 0.355 ng
RT: 6.930 min Scan# 51
Delta R.T. -0.007 min
Lab File: BN038238.D
Acq: 01 Dec 2025 22:42




Instrument :
BNA_N
ClientSampleId :
PB170712BSD


Tgt Ion: 99 Resp: 9418
Ion Ratio Lower Upper
99 100
42 21.9 17.0 25.6
71 32.7 25.4 38.2



#6
bis(2-Chloroethyl)ether
Concen: 0.375 ng
RT: 7.183 min Scan# 568
Delta R.T. -0.007 min
Lab File: BN038238.D
Acq: 01 Dec 2025 22:42

Tgt Ion: 93 Resp: 9517
Ion Ratio Lower Upper
93 100
63 76.5 58.1 87.1
95 32.3 25.1 37.7


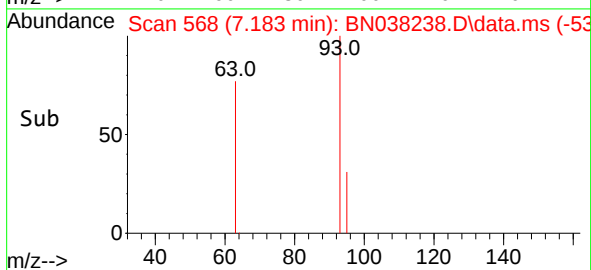






#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.562 min Scan# 91
Delta R.T. -0.011 min
Lab File: BN038238.D
Acq: 01 Dec 2025 22:42




Instrument :
BNA_N
ClientSampleId :
PB170712BSD


Tgt Ion:	136	Resp:	25072
Ion Ratio	Lower	Upper	
136	100		
137	11.3	8.9	13.3
54	9.9	5.4	8.0#
68	7.0	4.1	6.1#

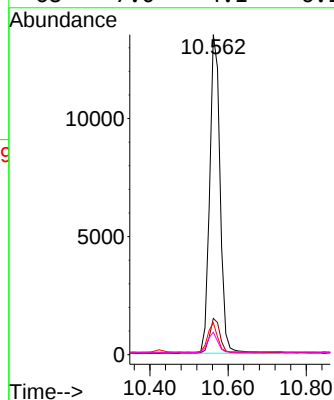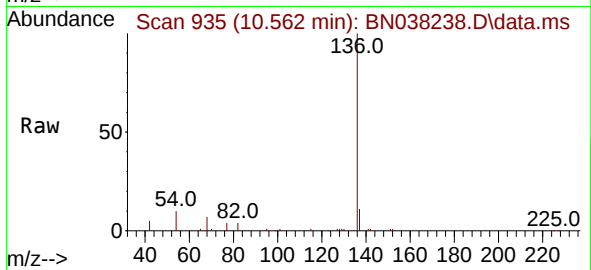

#8
Nitrobenzene-d5
Concen: 0.402 ng
RT: 8.918 min Scan# 781
Delta R.T. 0.000 min
Lab File: BN038238.D
Acq: 01 Dec 2025 22:42

Tgt Ion:	82	Resp:	8050
Ion Ratio	Lower	Upper	
82	100		
128	45.6	32.6	48.8
54	53.6	45.4	68.0

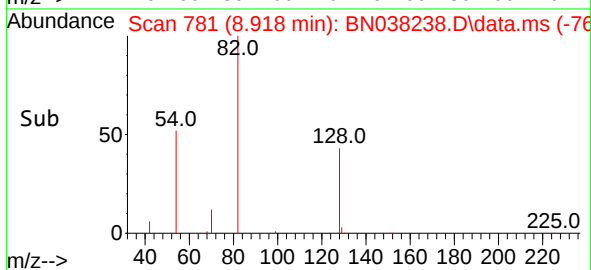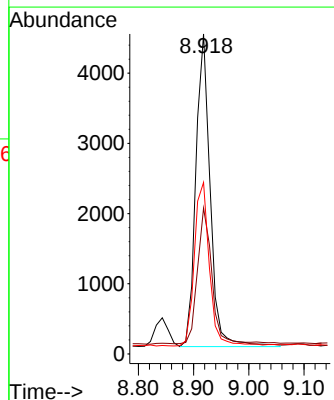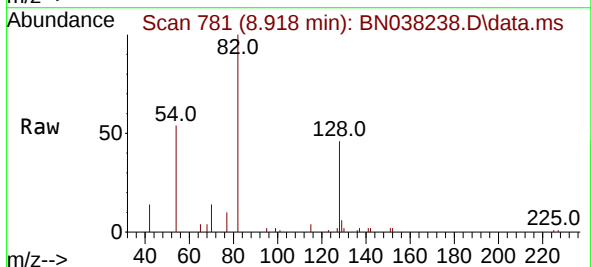

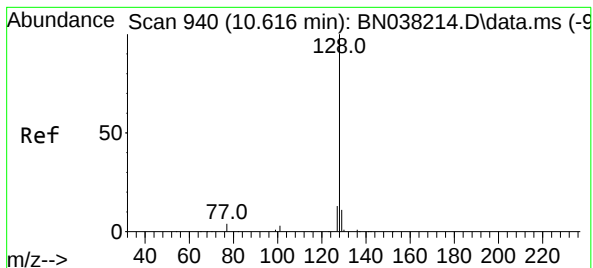

#9

Naphthalene

Concen: 0.357 ng

RT: 10.616 min Scan# 940

Delta R.T. 0.000 min

Lab File: BN038238.D

Acq: 01 Dec 2025 22:42

Instrument :

BNA_N

ClientSampleId :

PB170712BSD





Tgt Ion:128 Resp: 24829

Ion Ratio Lower Upper

128 100

129 11.7 9.1 13.7

127 13.3 10.6 16.0

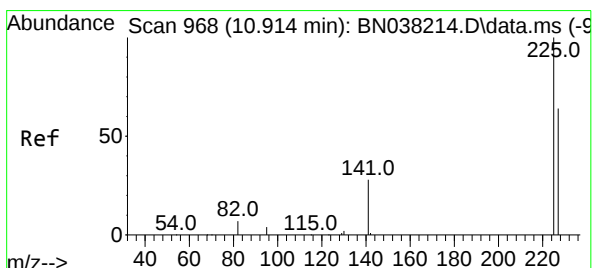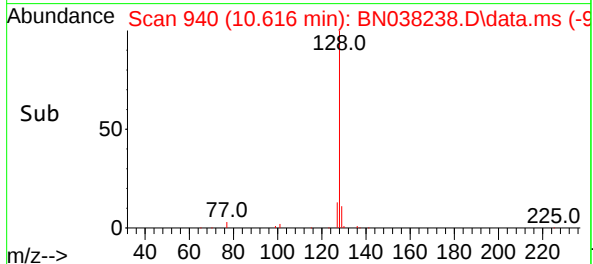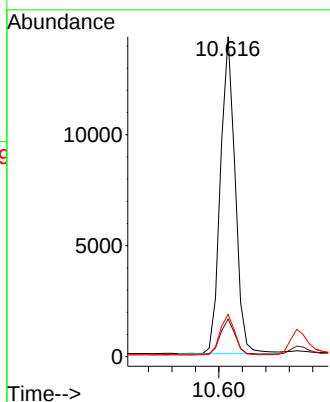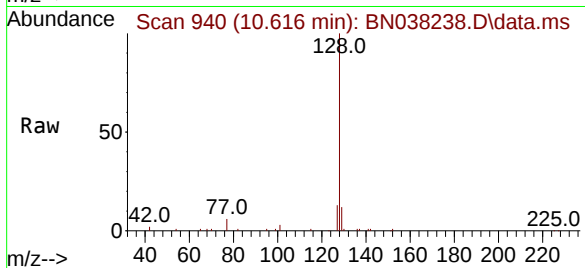

#10

Hexachlorobutadiene

Concen: 0.386 ng

RT: 10.915 min Scan# 968

Delta R.T. 0.000 min

Lab File: BN038238.D

Acq: 01 Dec 2025 22:42




Tgt Ion:225 Resp: 4570


Ion Ratio Lower Upper

225 100

223 0.0 0.0 0.0

227 64.0 50.5 75.7


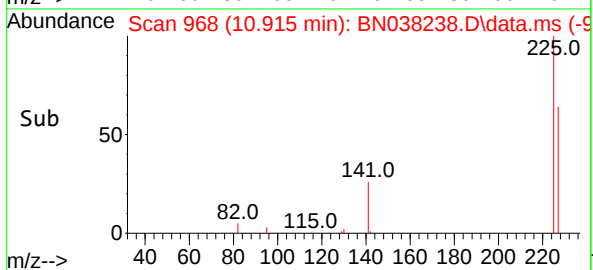
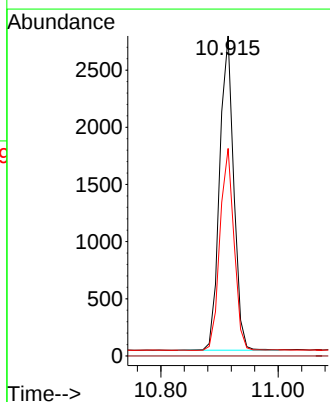
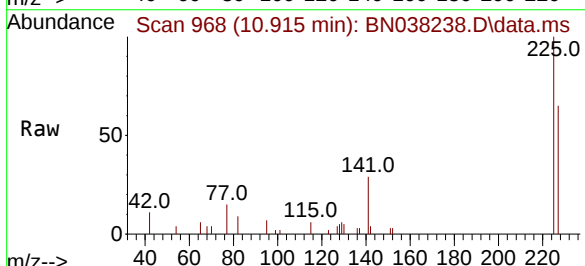




#11
2-Methylnaphthalene-d10
Concen: 0.345 ng
RT: 12.162 min Scan# 1152
Delta R.T. -0.005 min
Lab File: BN038238.D
Acq: 01 Dec 2025 22:42




Instrument :
BNA_N
ClientSampleId :
PB170712BSD


Tgt Ion:152 Resp: 12286
Ion Ratio Lower Upper
152 100
151 20.1 16.7 25.1



#12
2-Methylnaphthalene
Concen: 0.298 ng
RT: 12.238 min Scan# 1167
Delta R.T. -0.005 min
Lab File: BN038238.D
Acq: 01 Dec 2025 22:42

Tgt Ion:142 Resp: 13648
Ion Ratio Lower Upper
142 100
141 89.7 70.9 106.3
115 36.6 27.7 41.5


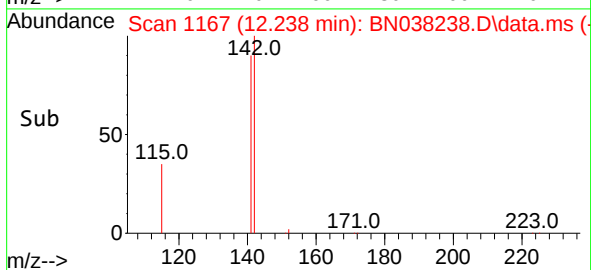

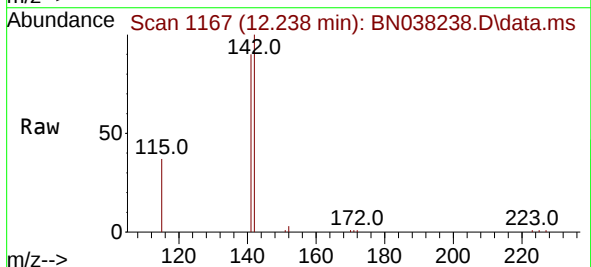




#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.430 min Scan# 1452
Delta R.T. 0.000 min
Lab File: BN038238.D
Acq: 01 Dec 2025 22:42




Instrument :
BNA_N
ClientSampleId :
PB170712BSD


Tgt Ion:164 Resp: 10824
Ion Ratio Lower Upper
164 100
162 101.8 83.8 125.8
160 48.5 41.6 62.4

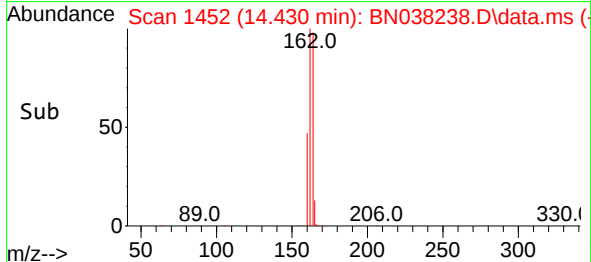

#14
2,4,6-Tribromophenol
Concen: 0.346 ng
RT: 15.932 min Scan# 1587
Delta R.T. 0.000 min
Lab File: BN038238.D
Acq: 01 Dec 2025 22:42

Tgt Ion:330 Resp: 1178
Ion Ratio Lower Upper
330 100
332 97.9 77.8 116.6
141 42.4 33.0 49.4


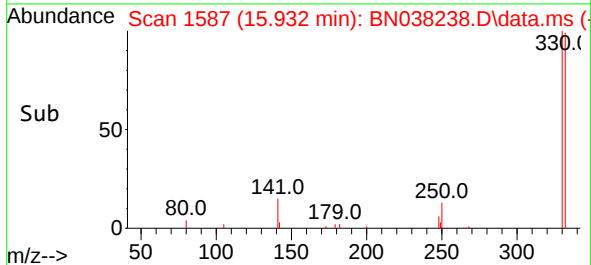

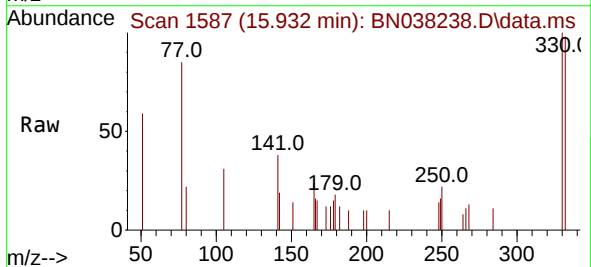


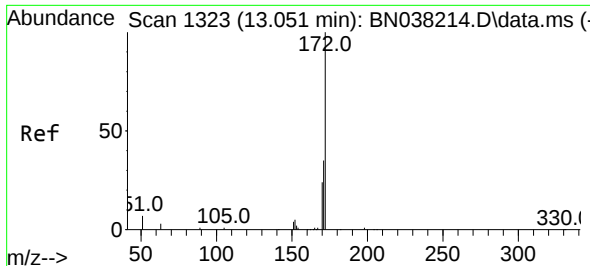

#15
2-Fluorobiphenyl
Concen: 0.429 ng
RT: 13.051 min Scan# 1323
Delta R.T. 0.000 min
Lab File: BN038238.D
Acq: 01 Dec 2025 22:42




Instrument :
BNA_N
ClientSampleId :
PB170712BSD


Tgt Ion:172 Resp: 17945
Ion Ratio Lower Upper
172 100
171 34.4 28.1 42.1
170 22.5 19.1 28.7

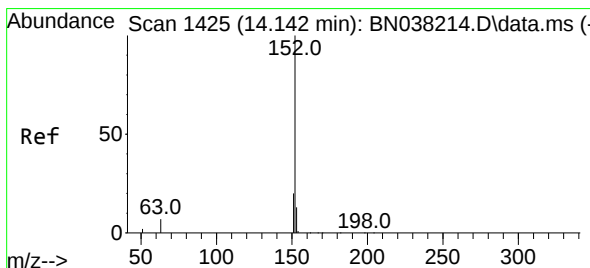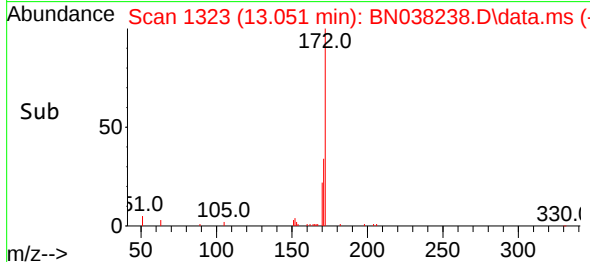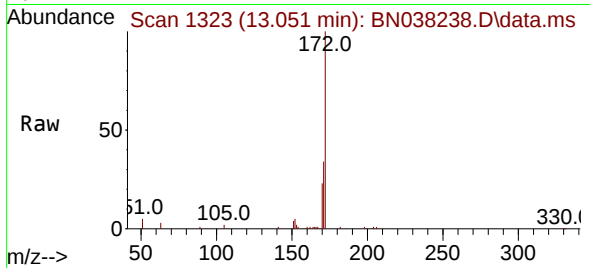

#16
Acenaphthylene
Concen: 0.390 ng
RT: 14.142 min Scan# 1425
Delta R.T. 0.000 min
Lab File: BN038238.D
Acq: 01 Dec 2025 22:42

Tgt Ion:152 Resp: 18881
Ion Ratio Lower Upper
152 100
151 19.7 15.6 23.4
153 13.2 10.6 15.8


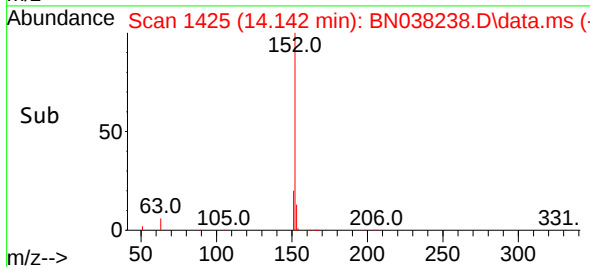

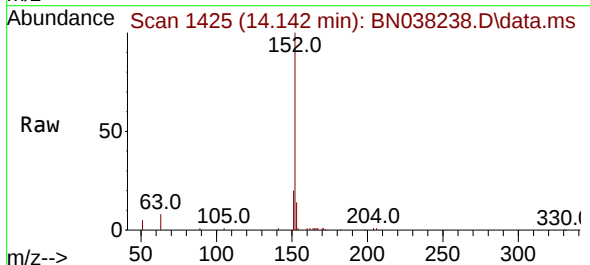


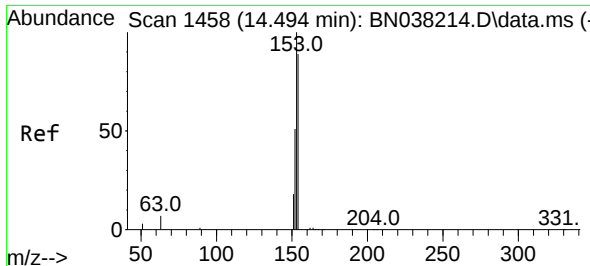

#17
Acenaphthene
Concen: 0.348 ng
RT: 14.484 min Scan# 1457
Delta R.T. -0.011 min
Lab File: BN038238.D
Acq: 01 Dec 2025 22:42




Instrument :
BNA_N
ClientSampleId :
PB170712BSD


Tgt Ion:154 Resp: 11726
Ion Ratio Lower Upper
154 100
153 114.7 91.1 136.7
152 57.7 48.2 72.2

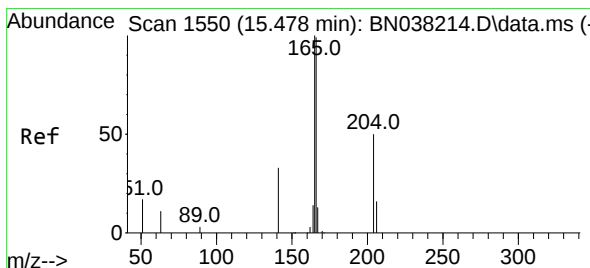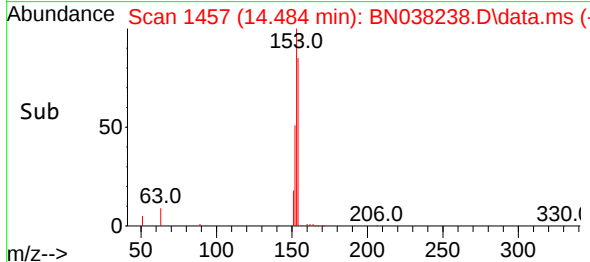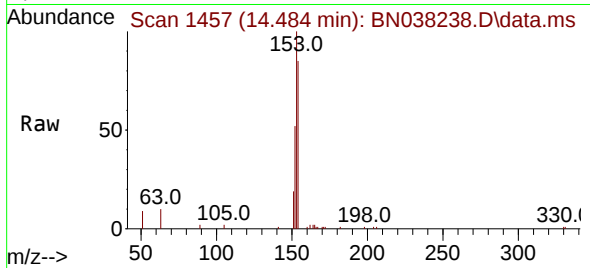

#18
Fluorene
Concen: 0.324 ng
RT: 15.478 min Scan# 1550
Delta R.T. 0.000 min
Lab File: BN038238.D
Acq: 01 Dec 2025 22:42

Tgt Ion:166 Resp: 14142
Ion Ratio Lower Upper
166 100
165 99.1 78.7 118.1
167 13.9 10.9 16.3


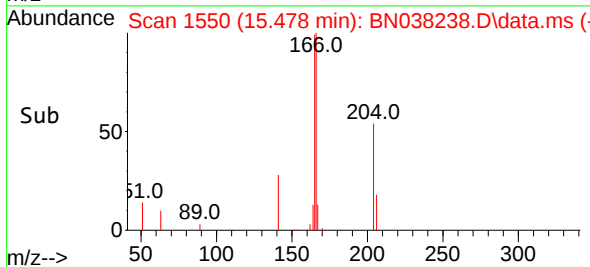

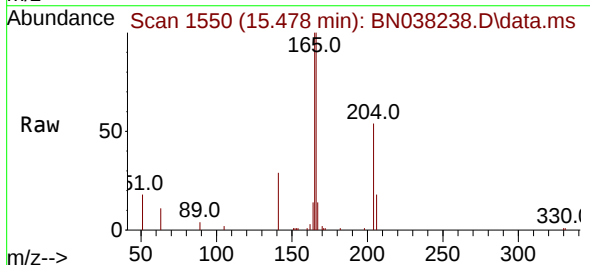


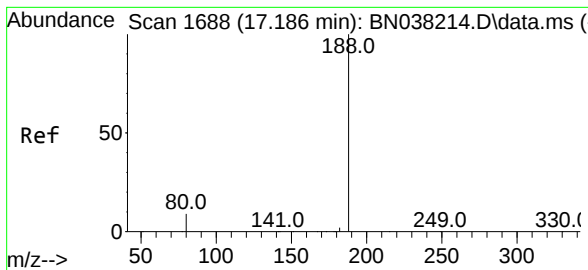

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.173 min Scan# 1687
Delta R.T. -0.012 min
Lab File: BN038238.D
Acq: 01 Dec 2025 22:42




Instrument :
BNA_N
ClientSampleId :
PB170712BSD


Tgt Ion:188 Resp: 16101
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 14.7 7.7 11.5#

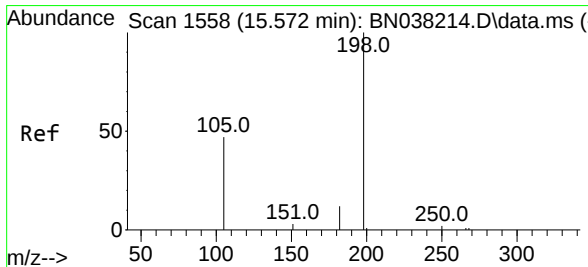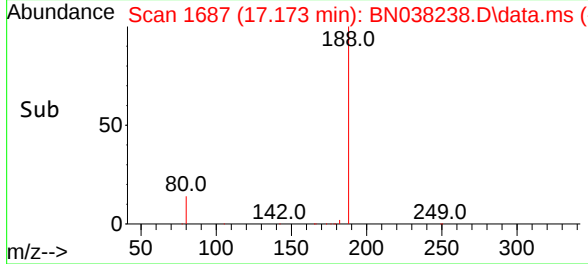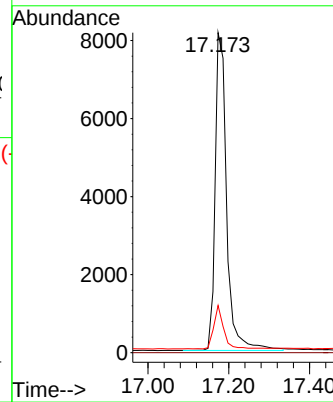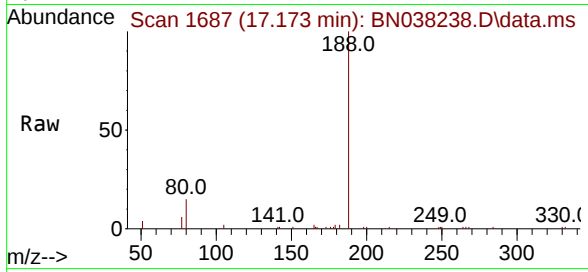

#20
4,6-Dinitro-2-methylphenol
Concen: 0.266 ng
RT: 15.560 min Scan# 1557
Delta R.T. -0.012 min
Lab File: BN038238.D
Acq: 01 Dec 2025 22:42

Tgt Ion:198 Resp: 159
Ion Ratio Lower Upper
198 100
51 308.3 205.1 307.7#
105 151.2 61.6 92.4#


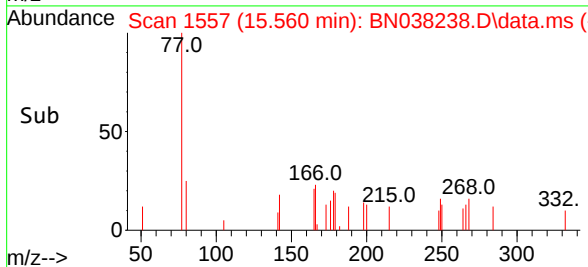
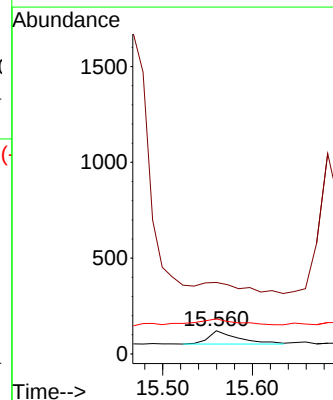
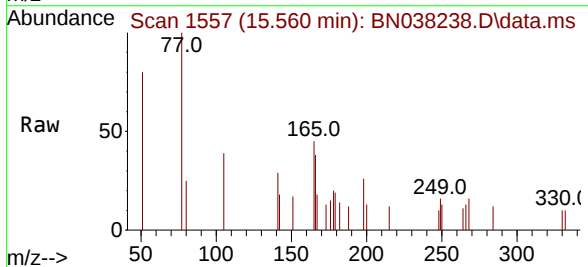


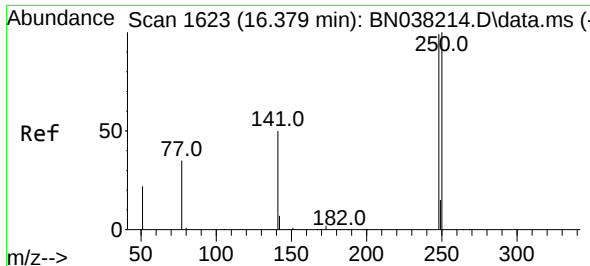

#21
4-Bromophenyl-phenylether
Concen: 0.355 ng
RT: 16.379 min Scan# 1623
Delta R.T. 0.000 min
Lab File: BN038238.D
Acq: 01 Dec 2025 22:42




Instrument :
BNA_N
ClientSampleId :
PB170712BSD


Tgt Ion:248 Resp: 3955
Ion Ratio Lower Upper
248 100
250 102.1 80.8 121.2
141 50.3 41.0 61.6

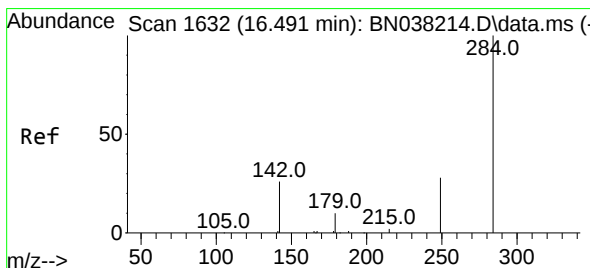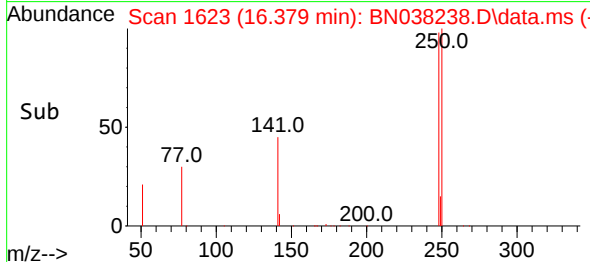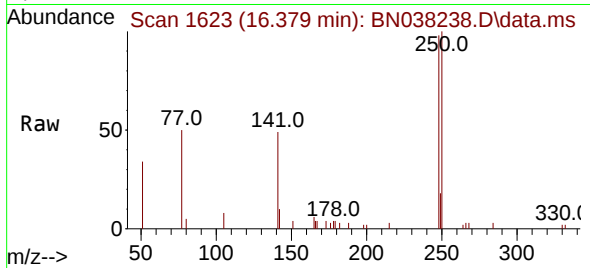

#22
Hexachlorobenzene
Concen: 0.339 ng
RT: 16.491 min Scan# 1632
Delta R.T. 0.000 min
Lab File: BN038238.D
Acq: 01 Dec 2025 22:42

Tgt Ion:284 Resp: 4649
Ion Ratio Lower Upper
284 100
142 37.3 30.5 45.7
249 30.7 23.8 35.8


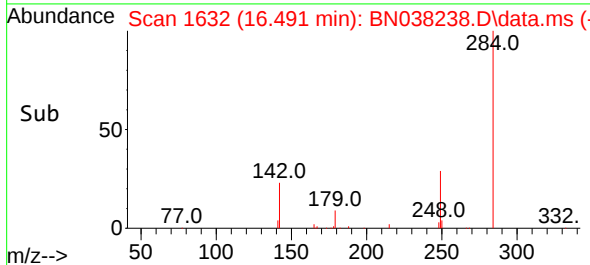

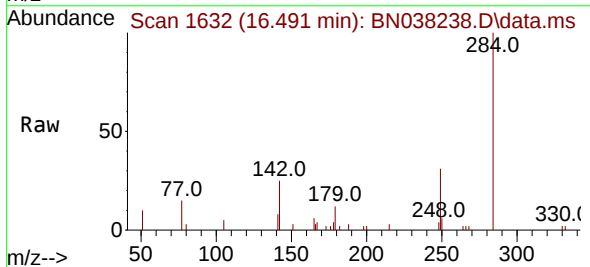




#23
 Atrazine
 Concen: 0.395 ng
 RT: 16.640 min Scan# 1644
 Delta R.T. -0.012 min
 Lab File: BN038238.D
 Acq: 01 Dec 2025 22:42




Instrument :
 BNA_N
 ClientSampleId :
 PB170712BSD


Tgt Ion:200 Resp: 2811
 Ion Ratio Lower Upper
 200 100
 173 34.9 21.0 31.6#
 215 46.7 37.8 56.8

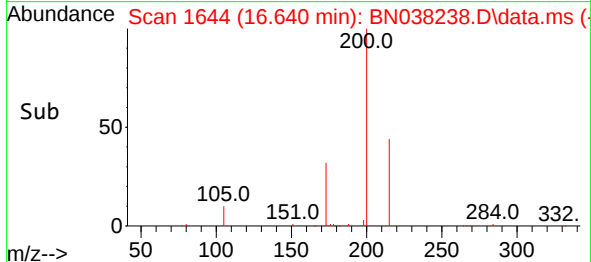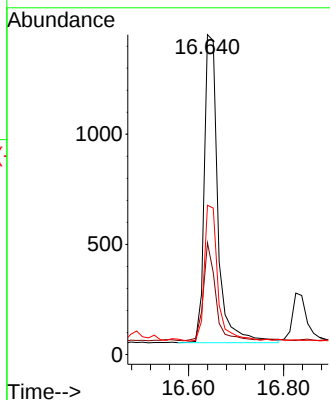

#24
 Pentachlorophenol
 Concen: 0.671 ng
 RT: 16.838 min Scan# 1660
 Delta R.T. 0.000 min
 Lab File: BN038238.D
 Acq: 01 Dec 2025 22:42

Tgt Ion:266 Resp: 2524
 Ion Ratio Lower Upper
 266 100
 264 61.3 48.9 73.3
 268 64.6 50.2 75.2


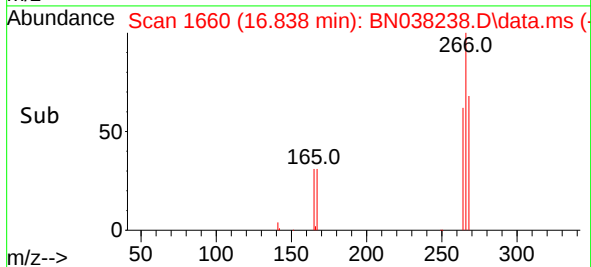
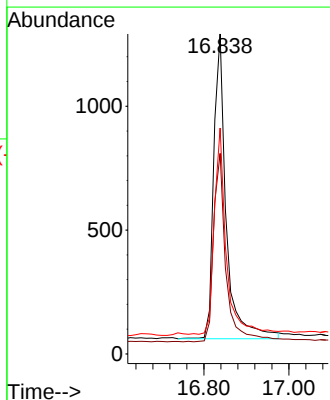
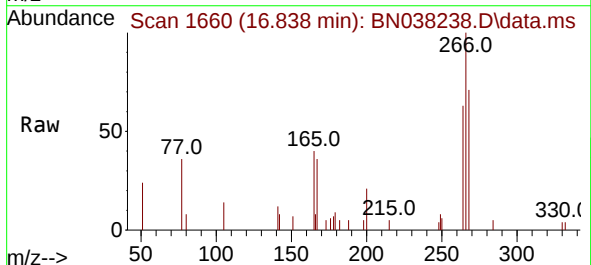




#25
Phenanthrene
Concen: 0.348 ng
RT: 17.223 min Scan# 1691
Delta R.T. 0.000 min
Lab File: BN038238.D
Acq: 01 Dec 2025 22:42




Instrument :
BNA_N
ClientSampleId :
PB170712BSD


Tgt Ion:178 Resp: 17571
Ion Ratio Lower Upper
178 100
176 19.6 15.3 22.9
179 16.0 12.0 18.0

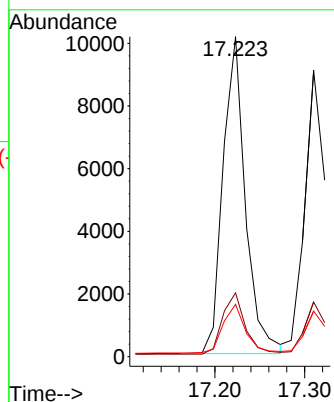

#26
Anthracene
Concen: 0.378 ng
RT: 17.310 min Scan# 1698
Delta R.T. 0.000 min
Lab File: BN038238.D
Acq: 01 Dec 2025 22:42

Tgt Ion:178 Resp: 16311
Ion Ratio Lower Upper
178 100
176 18.7 14.7 22.1
179 15.0 12.3 18.5


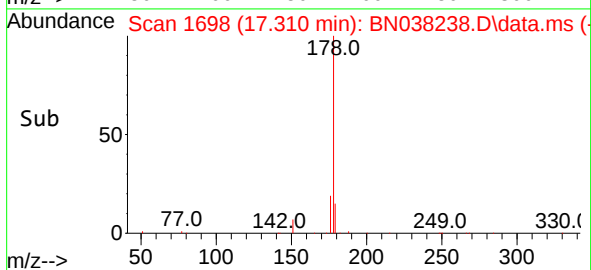
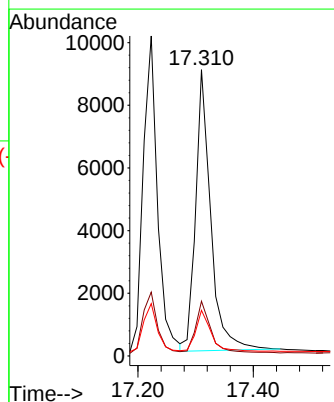





#27
Fluoranthene-d10
Concen: 0.389 ng
RT: 19.215 min Scan# 1946
Delta R.T. 0.000 min
Lab File: BN038238.D
Acq: 01 Dec 2025 22:42




Instrument :
BNA_N
ClientSampleId :
PB170712BSD


Tgt Ion:212 Resp: 13574
Ion Ratio Lower Upper
212 100
106 15.6 12.7 19.1
104 9.1 7.3 10.9

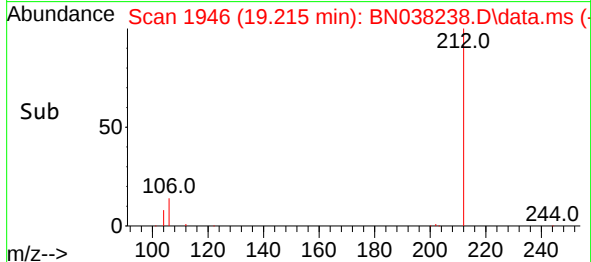

#28
Fluoranthene
Concen: 0.387 ng
RT: 19.243 min Scan# 1952
Delta R.T. -0.005 min
Lab File: BN038238.D
Acq: 01 Dec 2025 22:42

Tgt Ion:202 Resp: 18836
Ion Ratio Lower Upper
202 100
101 12.1 9.8 14.6
203 17.0 13.6 20.4


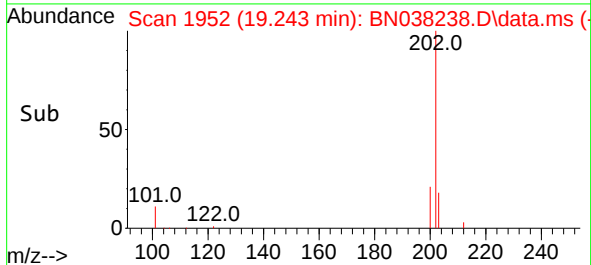

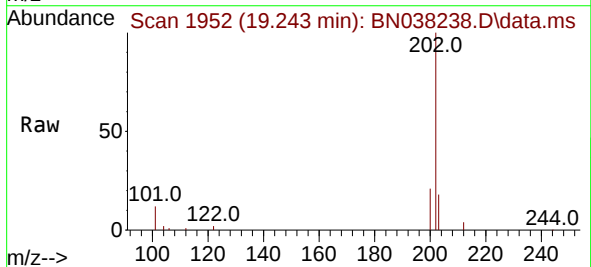




#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.366 min Scan# 21
Delta R.T. 0.000 min
Lab File: BN038238.D
Acq: 01 Dec 2025 22:42




Instrument :
BNA_N
ClientSampleId :
PB170712BSD


Tgt Ion:	240	Resp:	14003
Ion Ratio	Lower	Upper	
240	100		
120	19.6	18.1	27.1
236	30.4	24.2	36.4

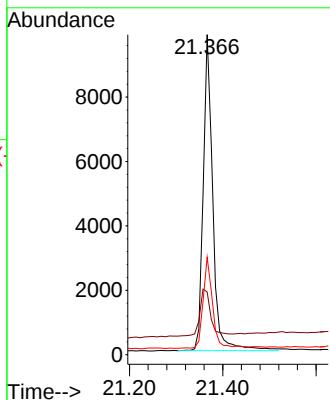

#30
Pyrene
Concen: 0.284 ng
RT: 19.606 min Scan# 2030
Delta R.T. -0.005 min
Lab File: BN038238.D
Acq: 01 Dec 2025 22:42

Tgt Ion:	202	Resp:	19886
Ion Ratio	Lower	Upper	
202	100		
200	21.3	16.8	25.2
203	17.7	14.4	21.6


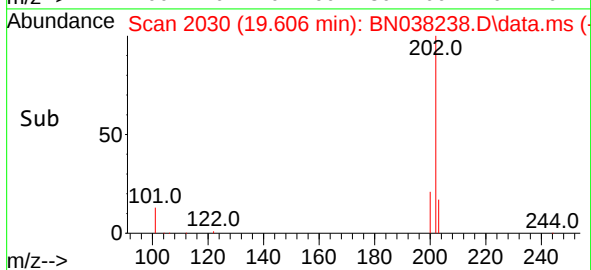
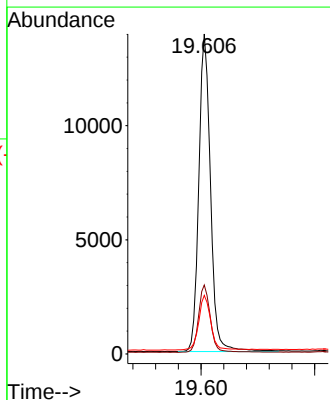





#31
 Terphenyl-d14
 Concen: 0.317 ng
 RT: 19.815 min Scan# 2076
 Delta R.T. -0.005 min
 Lab File: BN038238.D
 Acq: 01 Dec 2025 22:42




Instrument :
 BNA_N
 ClientSampleId :
 PB170712BSD


Tgt Ion:244 Resp: 10255
 Ion Ratio Lower Upper
 244 100
 212 10.2 7.7 11.5
 122 19.4 13.6 20.4

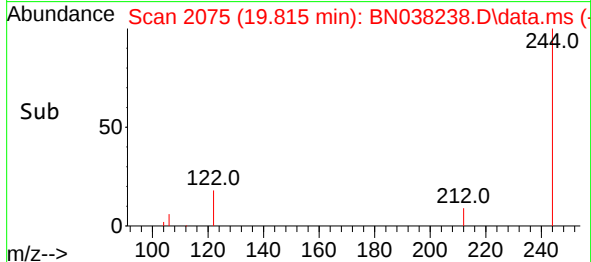

#32
 Benzo(a)anthracene
 Concen: 0.403 ng
 RT: 21.349 min Scan# 2266
 Delta R.T. -0.009 min
 Lab File: BN038238.D
 Acq: 01 Dec 2025 22:42

Tgt Ion:228 Resp: 19111
 Ion Ratio Lower Upper
 228 100
 226 28.8 22.6 33.8
 229 20.4 15.8 23.8

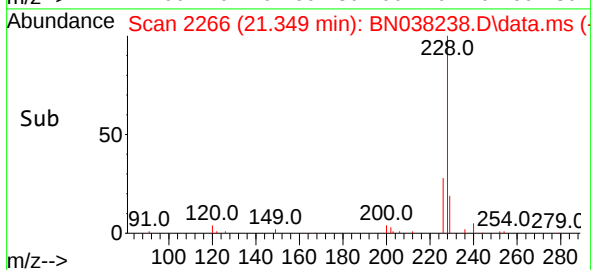




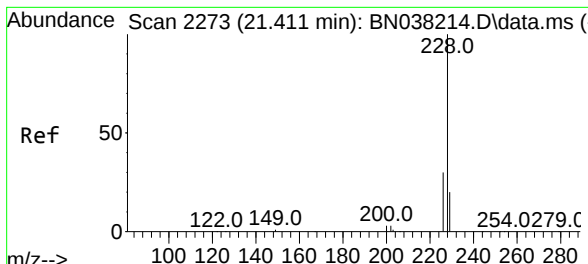


#33
 Chrysene
 Concen: 0.362 ng
 RT: 21.402 min Scan# 21
 Delta R.T. -0.009 min
 Lab File: BN038238.D
 Acq: 01 Dec 2025 22:42

Instrument :
 BNA_N
 ClientSampleId :
 PB170712BSD

Tgt Ion:228 Resp: 20271




Ion	Ratio	Lower	Upper
228	100		
226	31.1	23.8	35.8
229	20.1	16.1	24.1

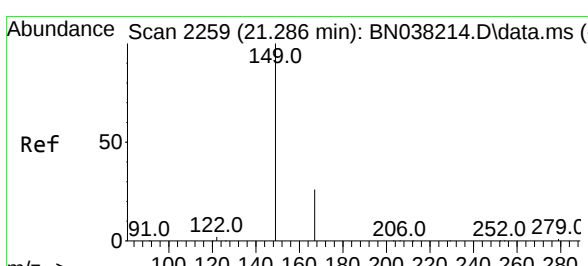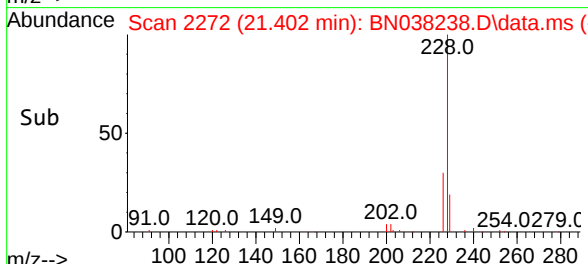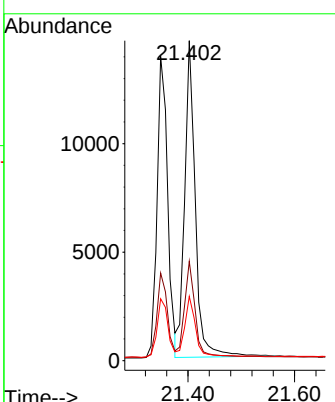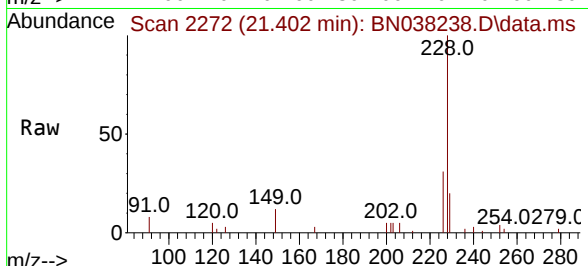


#34
 Bis(2-ethylhexyl)phthalate
 Concen: 0.455 ng
 RT: 21.286 min Scan# 2259
 Delta R.T. 0.000 min
 Lab File: BN038238.D
 Acq: 01 Dec 2025 22:42

Tgt Ion:149 Resp: 11826


Ion	Ratio	Lower	Upper
149	100		
167	27.1	20.7	31.1
279	3.7	2.5	3.7

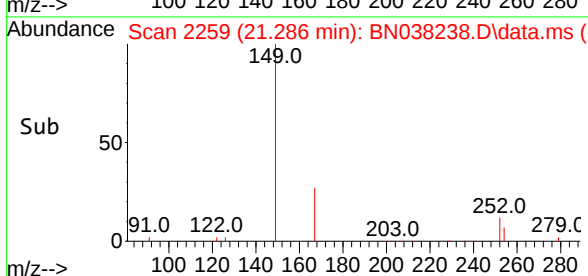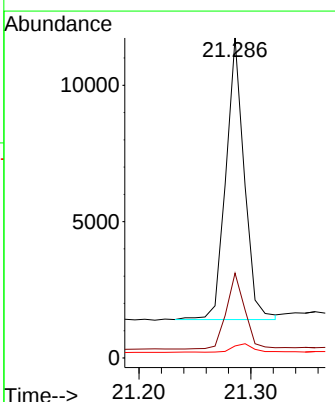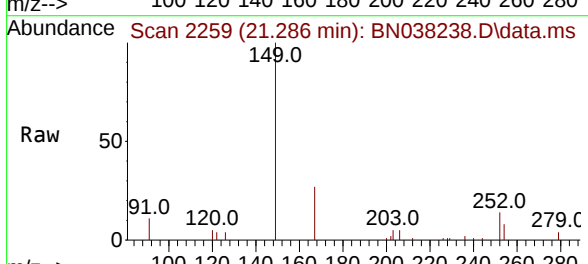






#35
Perylene-d12
Concen: 0.400 ng
RT: 23.671 min Scan# 21
Delta R.T. -0.009 min
Lab File: BN038238.D
Acq: 01 Dec 2025 22:42

Instrument :
BNA_N
ClientSampleId :
PB170712BSD







Tgt Ion:264 Resp: 15858
Ion Ratio Lower Upper
264 100
260 28.0 21.7 32.5
265 96.3 98.0 147.0#

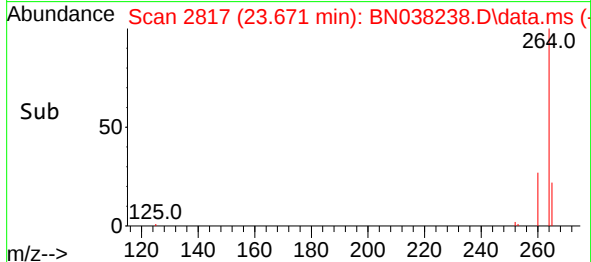

#36
Indeno(1,2,3-cd)pyrene
Concen: 0.383 ng
RT: 26.022 min Scan# 3621
Delta R.T. -0.015 min
Lab File: BN038238.D
Acq: 01 Dec 2025 22:42

Tgt Ion:276 Resp: 28125
Ion Ratio Lower Upper
276 100
138 27.3 21.4 32.2
277 24.6 19.1 28.7


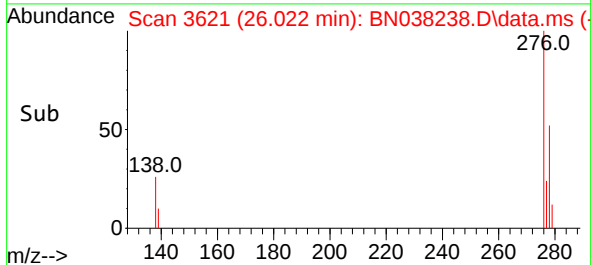
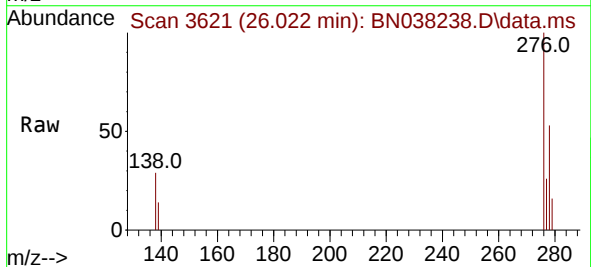





#37
Benzo(b)fluoranthene
Concen: 0.333 ng
RT: 22.975 min Scan# 2579
Delta R.T. -0.006 min
Lab File: BN038238.D
Acq: 01 Dec 2025 22:42




Instrument :
BNA_N
ClientSampleId :
PB170712BSD


Tgt Ion:252 Resp: 21654
Ion Ratio Lower Upper
252 100
253 28.9 22.2 33.4
125 22.2 18.0 27.0

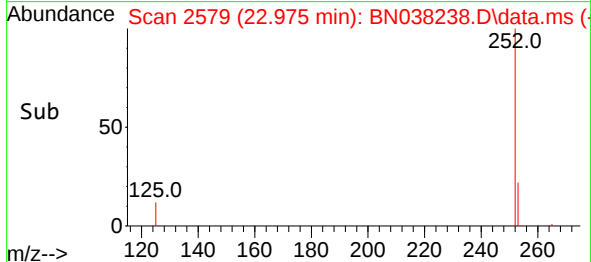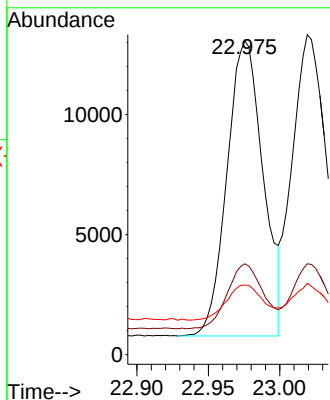

#38
Benzo(k)fluoranthene
Concen: 0.333 ng
RT: 23.019 min Scan# 2594
Delta R.T. -0.006 min
Lab File: BN038238.D
Acq: 01 Dec 2025 22:42


Tgt Ion:252 Resp: 22543
Ion Ratio Lower Upper
252 100
253 28.4 22.4 33.6
125 22.3 17.5 26.3

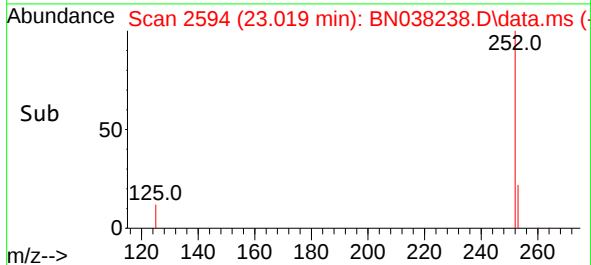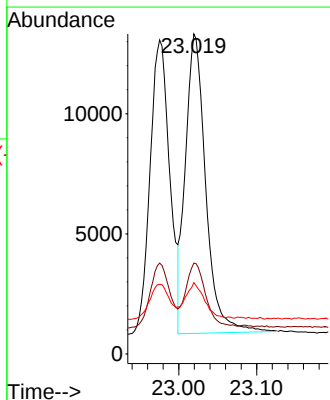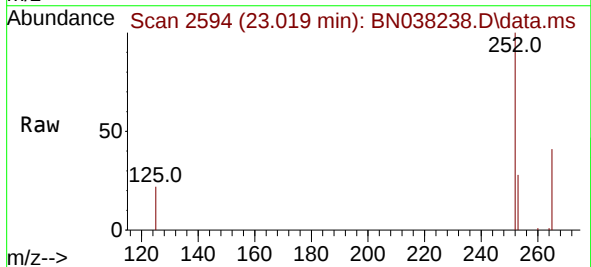






#39
Benzo(a)pyrene
Concen: 0.394 ng
RT: 23.572 min Scan# 21
Delta R.T. -0.006 min
Lab File: BN038238.D
Acq: 01 Dec 2025 22:42


Instrument :
BNA_N
ClientSampleId :
PB170712BSD





Tgt Ion:252 Resp: 21487
Ion Ratio Lower Upper
252 100
253 30.3 25.3 37.9
125 26.2 25.2 37.8

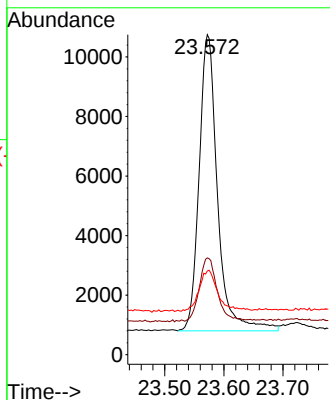


#40
Dibenzo(a,h)anthracene
Concen: 0.388 ng
RT: 26.039 min Scan# 3627
Delta R.T. -0.017 min
Lab File: BN038238.D
Acq: 01 Dec 2025 22:42

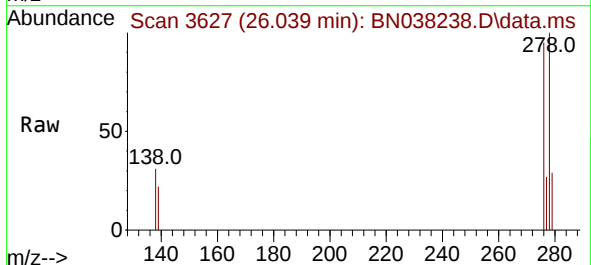


Tgt Ion:278 Resp: 21580
Ion Ratio Lower Upper
278 100
139 22.4 17.6 26.4
279 28.6 24.2 36.4

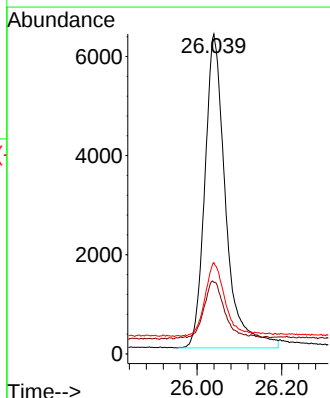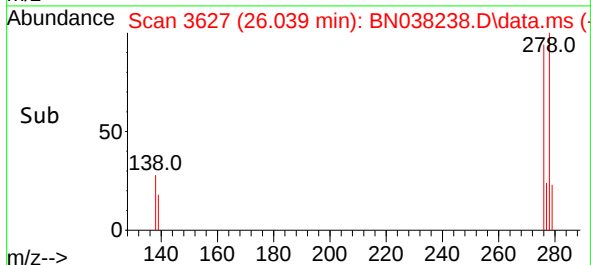

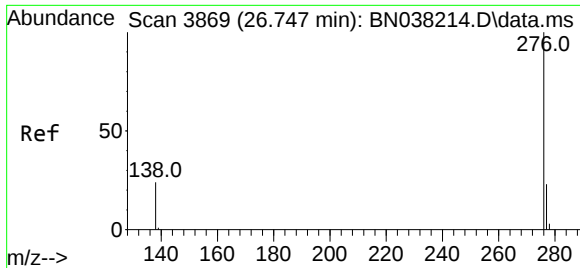

#41
 Benzo(g,h,i)perylene
 Concen: 0.352 ng
 RT: 26.735 min Scan# 31
 Delta R.T. -0.012 min
 Lab File: BN038238.D
 Acq: 01 Dec 2025 22:42

Instrument :
 BNA_N
 ClientSampleId :
 PB170712BSD

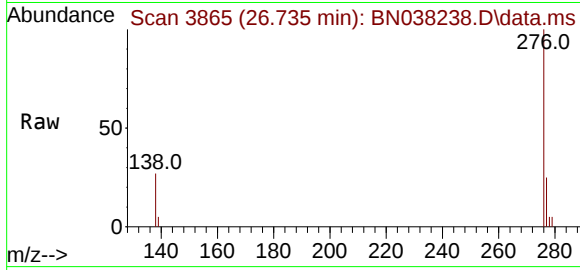

Tgt Ion:	276	Resp:	23394
Ion	Ratio	Lower	Upper
276	100		
277	25.2	20.2	30.2
138	26.8	20.8	31.2

