



Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120225\
Data File : BN038251.D
Acq On : 02 Dec 2025 12:48
Operator : RC/JU
Sample : PB170718BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK718

Manual IntegrationsAPPROVED

Quant Time: Dec 03 00:21:58 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN112625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 01 16:36:13 2025
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/03/2025
Supervised By :Sohil Jodhani 12/03/2025

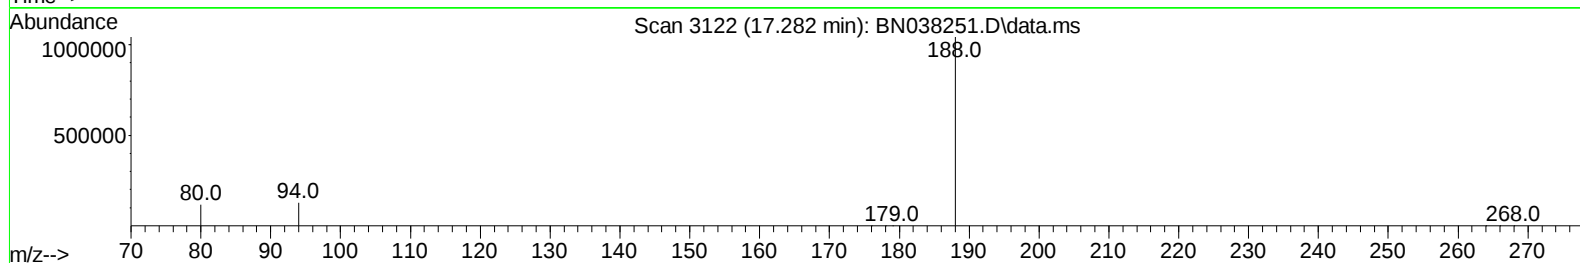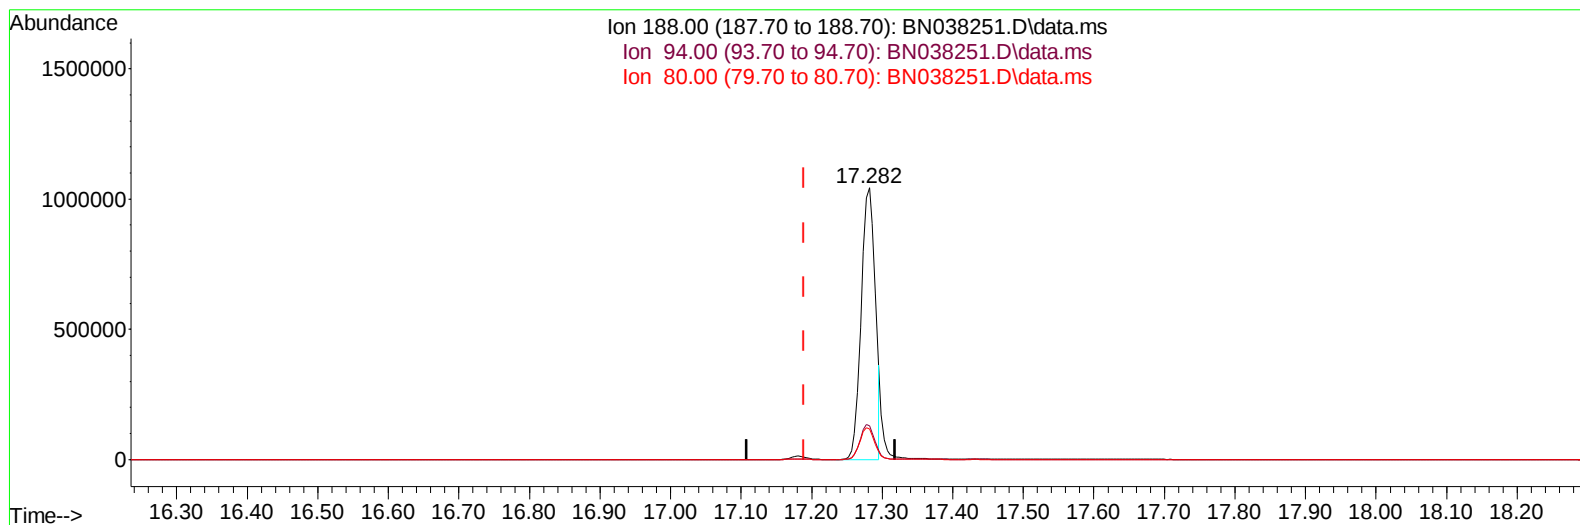

TIC: BN038251.D\data.ms

(13) Phenanthrene-d10 (I)

17.282min (+ 0.093) 0.40 ng/u1

response 1433180

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	11.20	12.31
80.00	12.20	11.21
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120225\
Data File : BN038251.D
Acq On : 02 Dec 2025 12:48
Operator : RC/JU
Sample : PB170718BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK718

Manual IntegrationsAPPROVED

Quant Time: Dec 03 00:21:58 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN112625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 01 16:36:13 2025
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/03/2025
Supervised By :Sohil Jodhani 12/03/2025

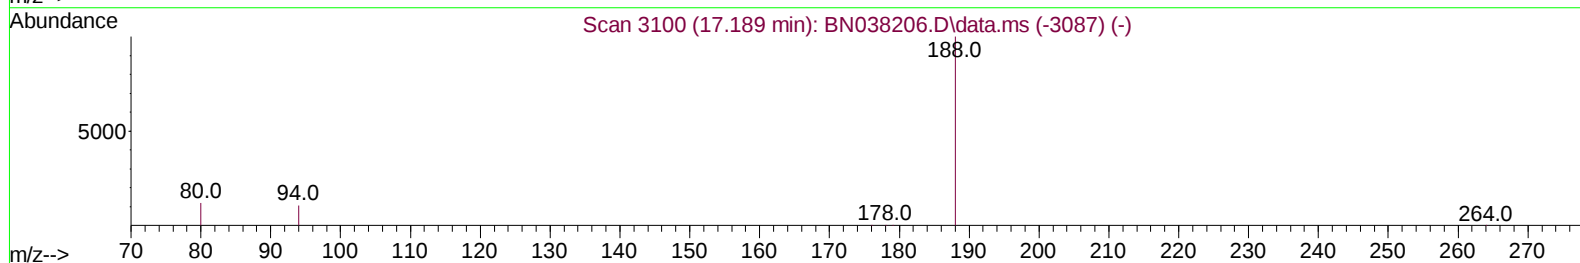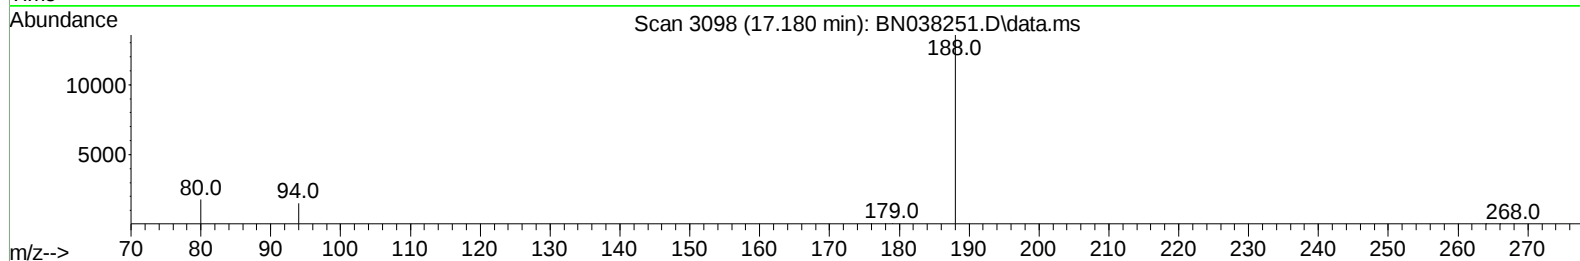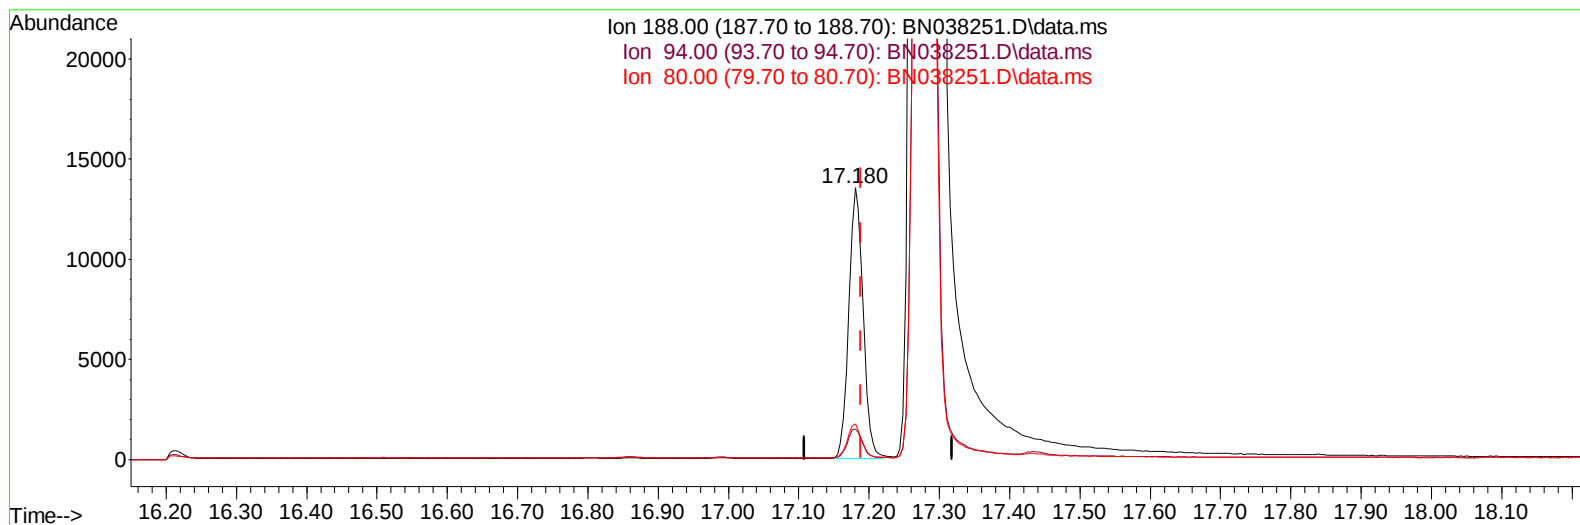

TIC: BN038251.D\data.ms

(13) Phenanthrene-d10 (I)

17.180min (-0.008) 0.40 ng/ul m

response 18893

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	11.20	11.31
80.00	12.20	13.08
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120225\
Data File : BN038251.D
Acq On : 02 Dec 2025 12:48
Operator : RC/JU
Sample : PB170718BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK718

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 12/03/2025
Supervised By :Sohil Jodhani 12/03/2025

Quant Time: Dec 03 00:21:58 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN112625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 01 16:36:13 2025
Response via : Initial Calibration

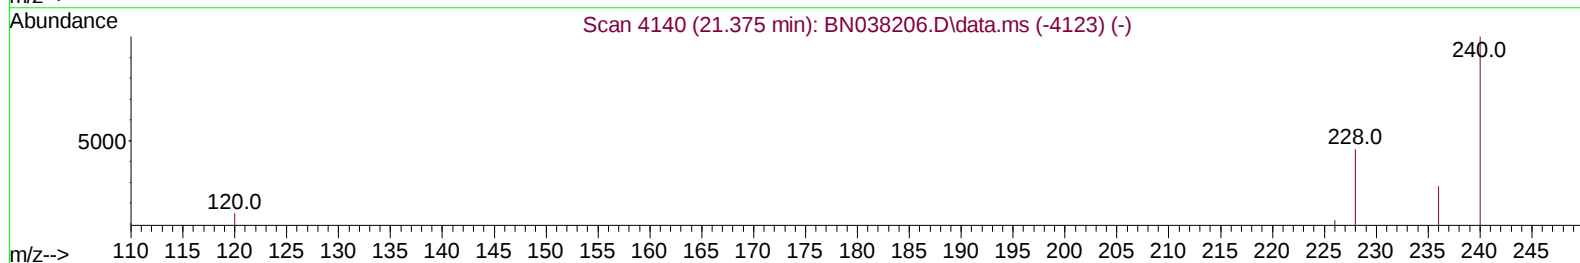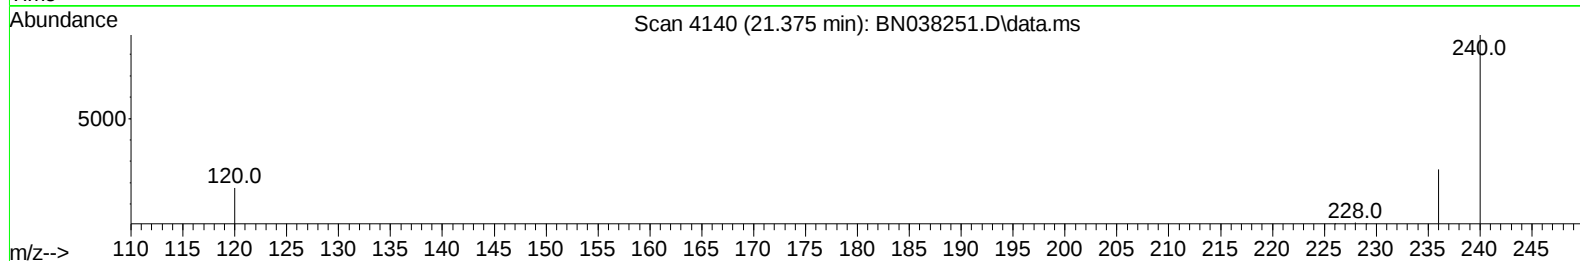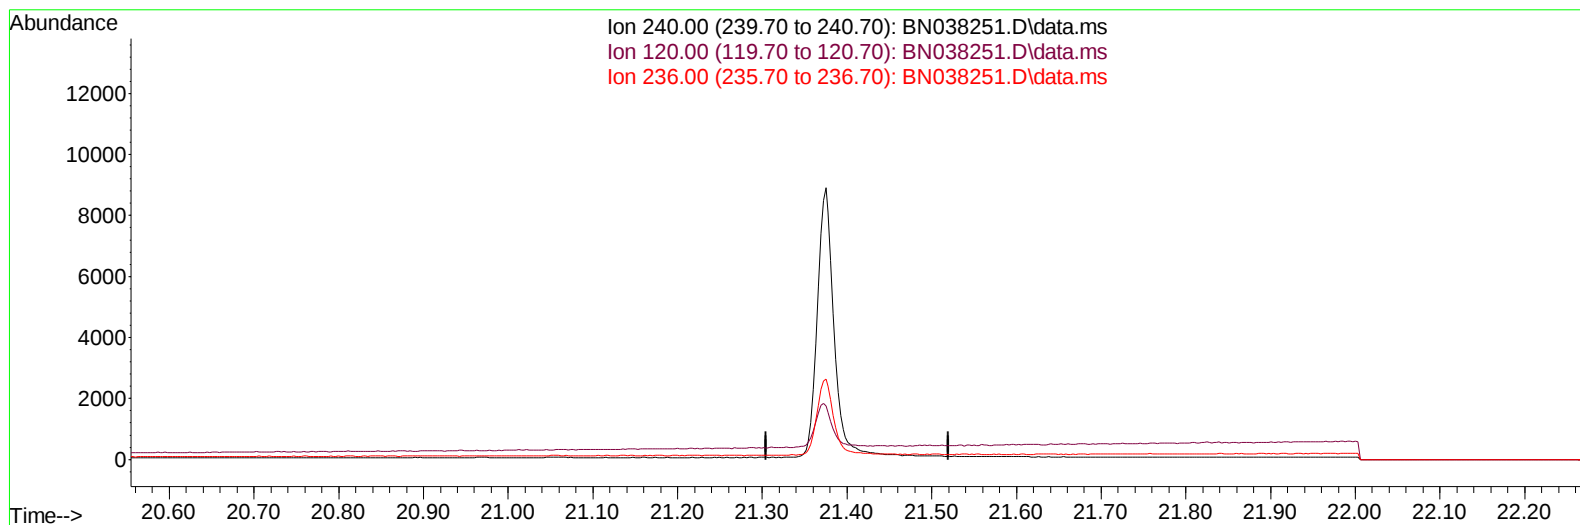

TIC: BN038251.D\data.ms

(17) Chrysene-d12

21.375min (-21.375) 0.00 ng/u1

response 0

Ion	Exp%	Act%
240.00	100.00	0.00
120.00	19.90	0.00#
236.00	29.60	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120225\
Data File : BN038251.D
Acq On : 02 Dec 2025 12:48
Operator : RC/JU
Sample : PB170718BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK718

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 12/03/2025
Supervised By :Sohil Jodhani 12/03/2025

Quant Time: Dec 03 00:21:58 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN112625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 01 16:36:13 2025
Response via : Initial Calibration

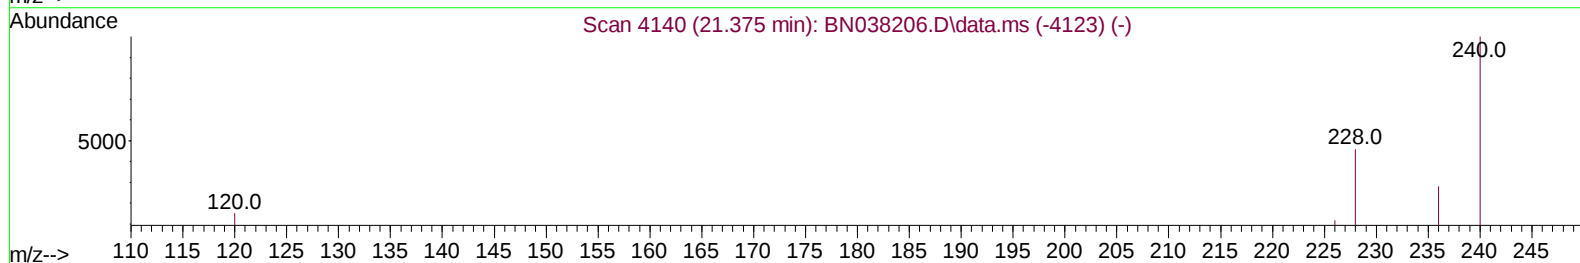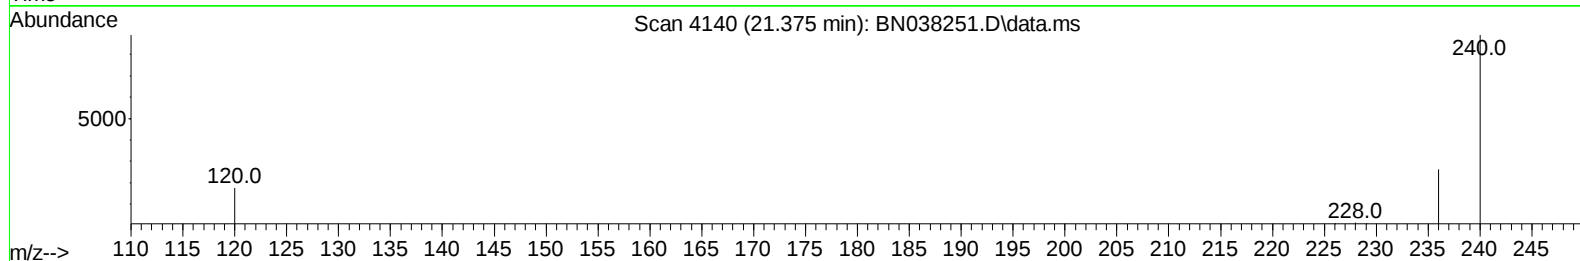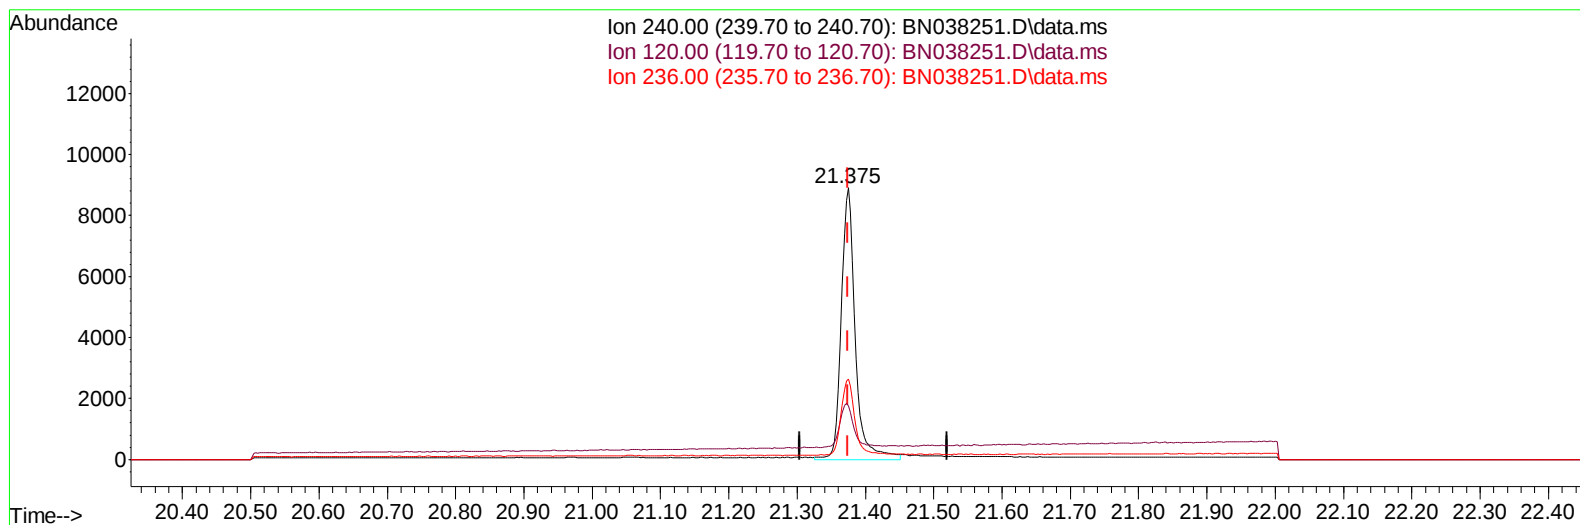

TIC: BN038251.D\data.ms

(17) Chrysene-d12

21.375min (+ 0.000) 0.40 ng/ul m

response 12697

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	19.90	19.61
236.00	29.60	29.55
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120225\
 Data File : BN038251.D
 Acq On : 02 Dec 2025 12:48
 Operator : RC/JU
 Sample : PB170718BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK718

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 12/03/2025
 Supervised By :Sohil Jodhani 12/03/2025

Quant Time: Dec 03 00:21:58 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN112625.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 01 16:36:13 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.762	152	8277	0.400	ng/ul	0.00
4) Naphthalene-d8	10.562	136	25091	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.429	164	12425	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.180	188	18893m	0.400	ng/ul	0.00
17) Chrysene-d12	21.375	240	12697m	0.400	ng/ul	0.00
23) Perylene-d12	23.681	264	18424	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.210	96	54996	6.332	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.168	152	11344	0.317	ng/ul	0.00
18) Fluoranthene-d10	19.212	212	14112	0.286	ng/ul	0.00

Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120225\
Data File : BN038251.D
Acq On : 02 Dec 2025 12:48
Operator : RC/JU
Sample : PB170718BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK718

Manual IntegrationsAPPROVED

Quant Time: Dec 03 00:21:58 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN112625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 01 16:36:13 2025
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/03/2025
Supervised By :Sohil Jodhani 12/03/2025

