



Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120225\
Data File : BN038268.D
Acq On : 02 Dec 2025 23:42
Operator : RC/JU
Sample : PB170722BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK722

Manual IntegrationsAPPROVED

Quant Time: Dec 03 01:40:14 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN112625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 01 16:36:13 2025
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/03/2025
Supervised By :Sohil Jodhani 12/03/2025

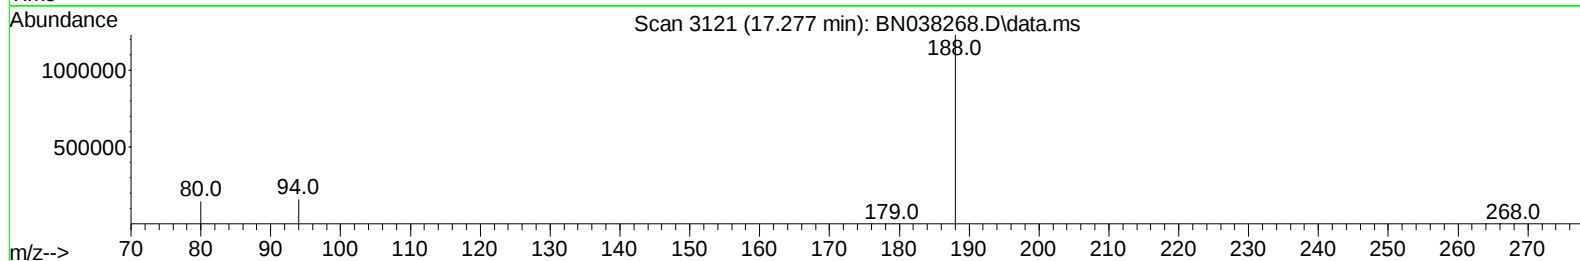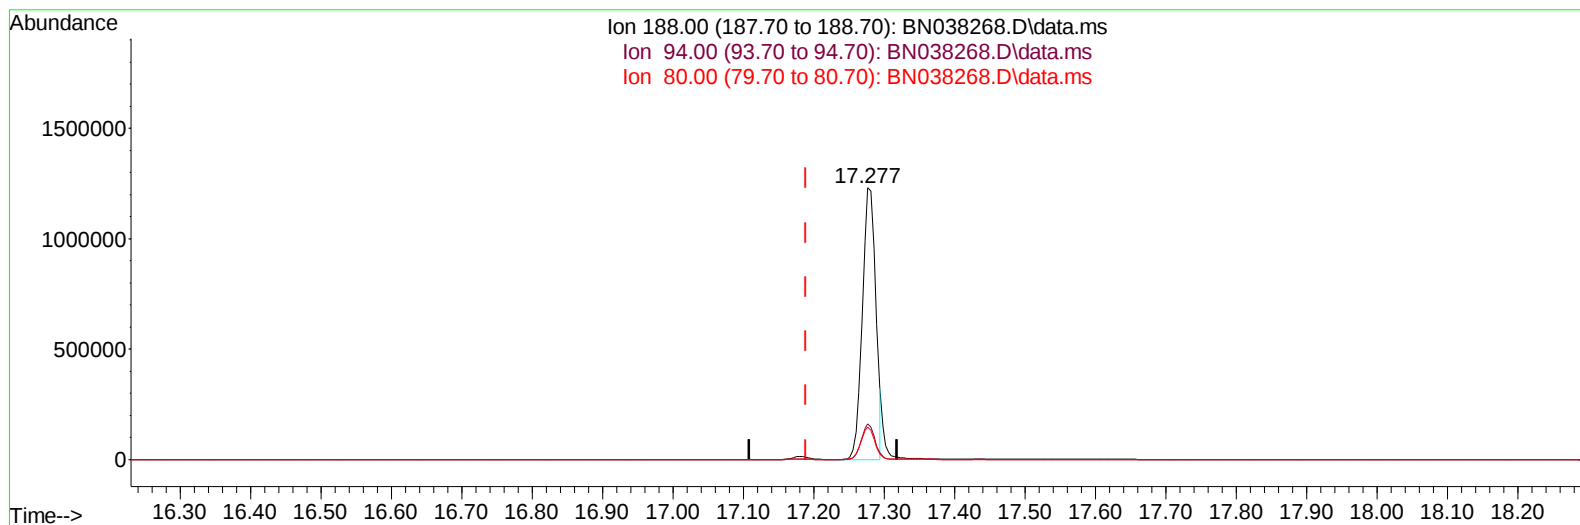

TIC: BN038268.D\data.ms

(13) Phenanthrene-d10 (I)

17.277min (+ 0.088) 0.40 ng/u1

response 1626739

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	11.20	13.06
80.00	12.20	11.97
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120225\
Data File : BN038268.D
Acq On : 02 Dec 2025 23:42
Operator : RC/JU
Sample : PB170722BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK722

Manual IntegrationsAPPROVED

Quant Time: Dec 03 01:40:14 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN112625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 01 16:36:13 2025
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/03/2025
Supervised By :Sohil Jodhani 12/03/2025

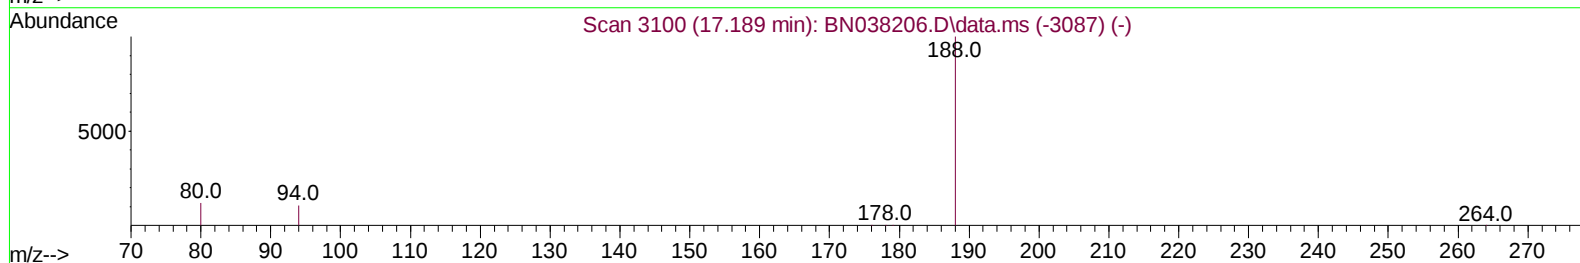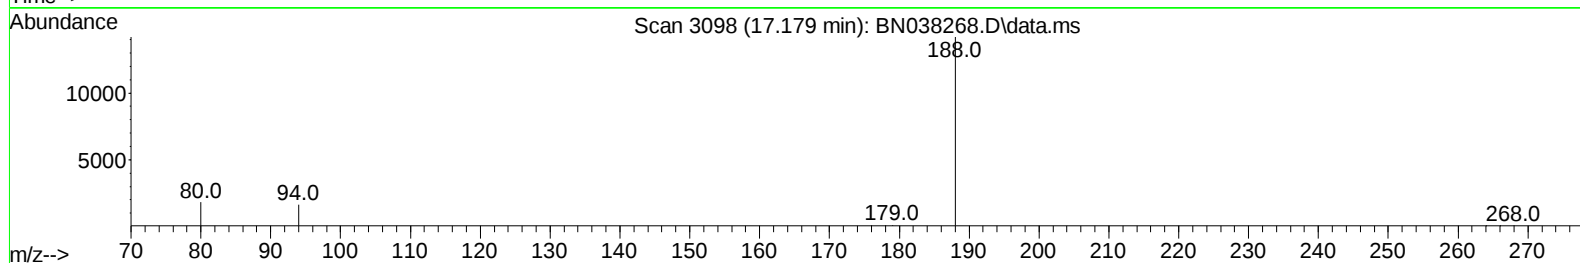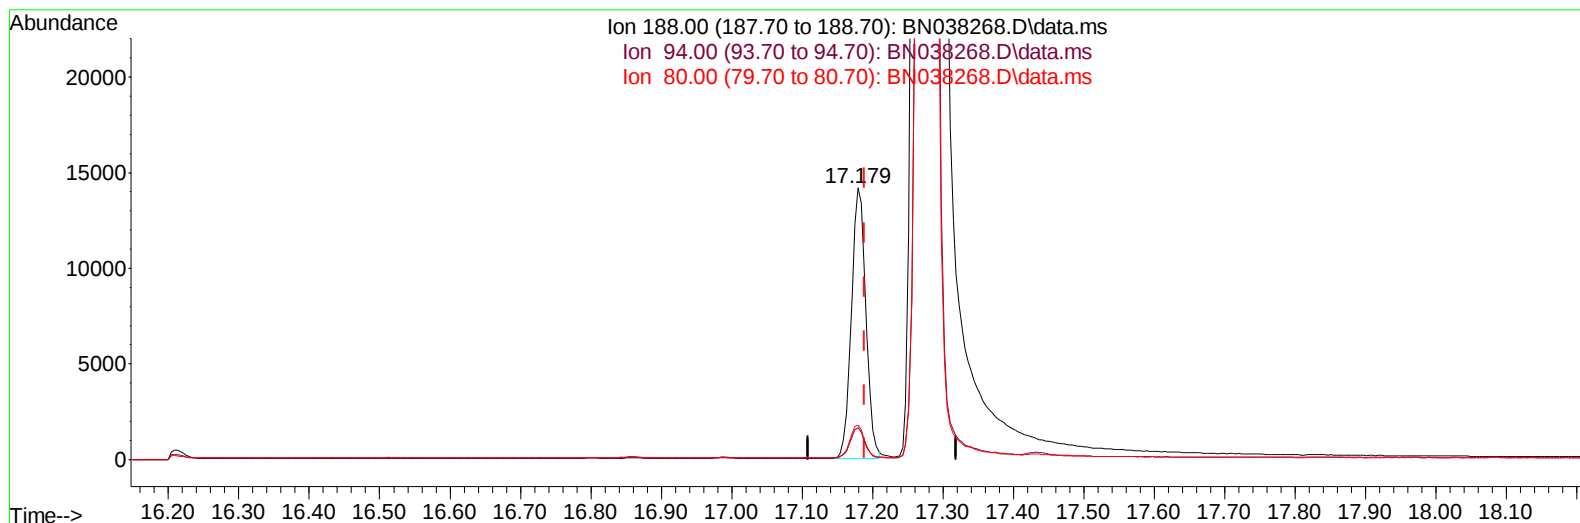

TIC: BN038268.D\data.ms

(13) Phenanthrene-d10 (I)

17.179min (-0.009) 0.40 ng/u1 m

response 20142

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	11.20	11.60
80.00	12.20	12.71
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120225\
Data File : BN038268.D
Acq On : 02 Dec 2025 23:42
Operator : RC/JU
Sample : PB170722BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK722

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 12/03/2025
Supervised By :Sohil Jodhani 12/03/2025

Quant Time: Dec 03 01:40:14 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN112625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 01 16:36:13 2025
Response via : Initial Calibration

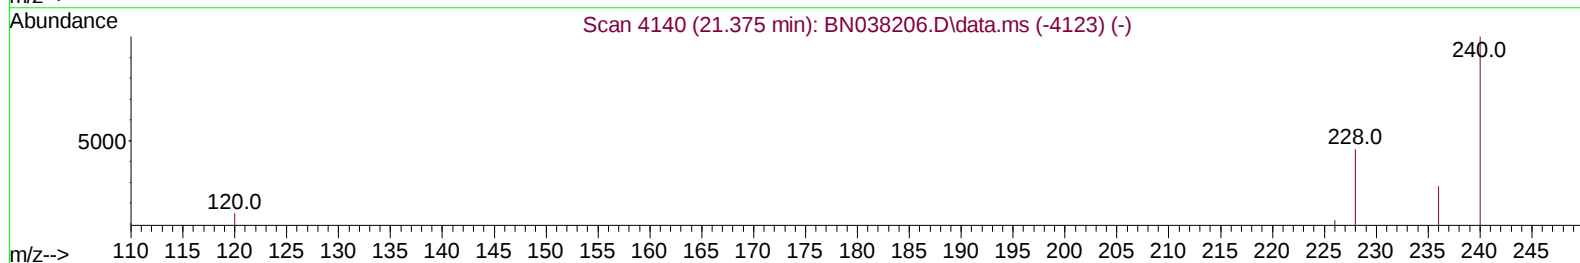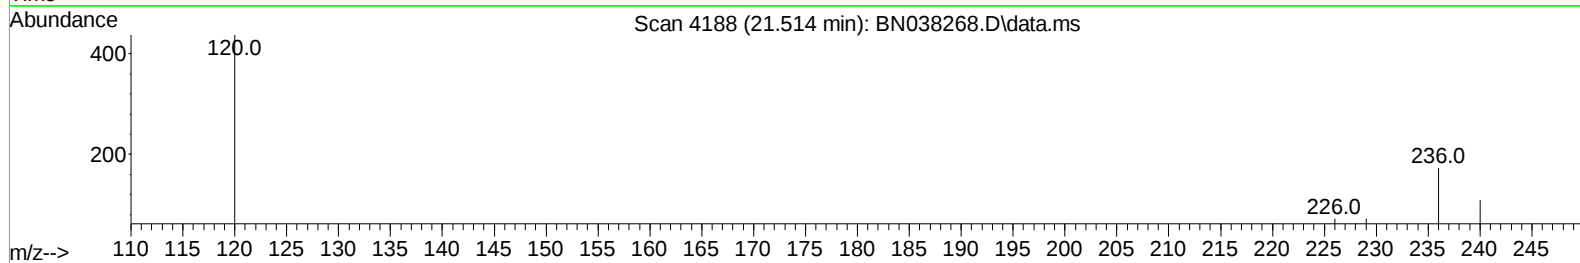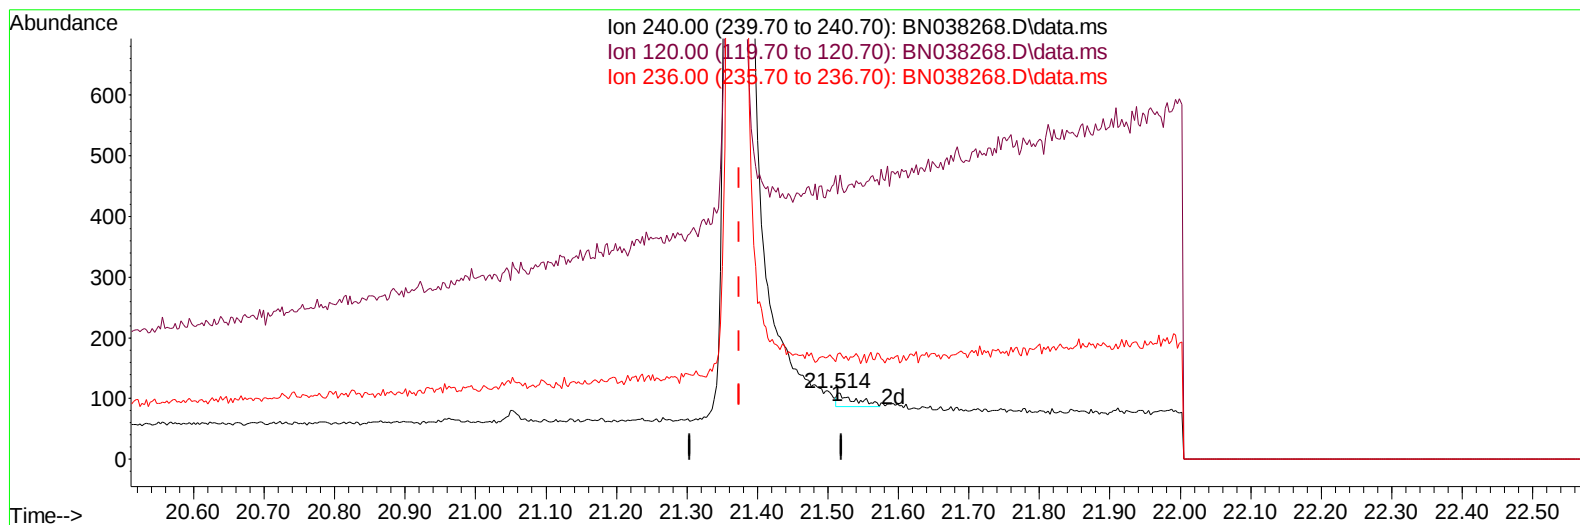

TIC: BN038268.D\data.ms

(17) Chrysene-d12

21.514min (+ 0.139) 0.40 ng/u1

response 38

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	19.90	400.92#
236.00	29.60	158.72#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120225\
Data File : BN038268.D
Acq On : 02 Dec 2025 23:42
Operator : RC/JU
Sample : PB170722BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK722

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 12/03/2025
Supervised By :Sohil Jodhani 12/03/2025

Quant Time: Dec 03 01:40:14 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN112625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 01 16:36:13 2025
Response via : Initial Calibration

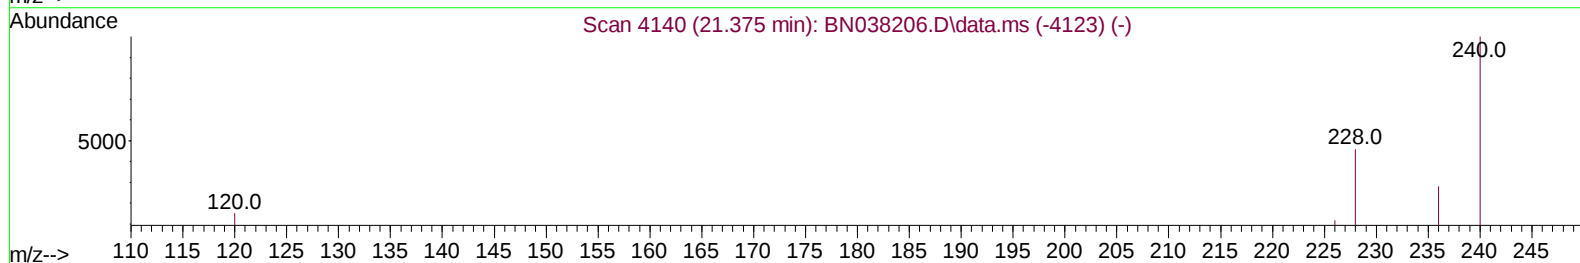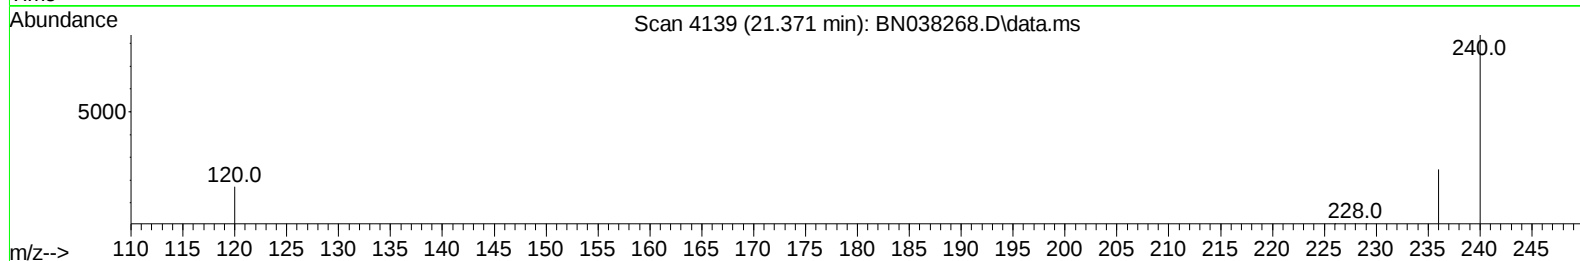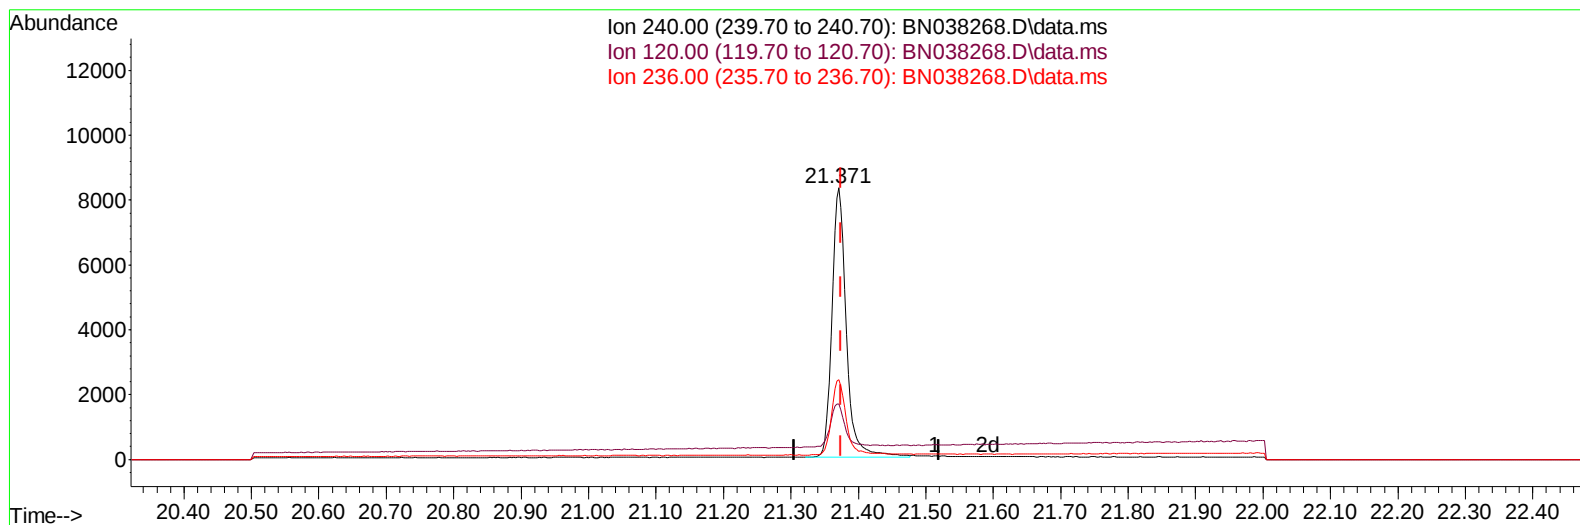

TIC: BN038268.D\data.ms

(17) Chrysene-d12

21.371min (-0.004) 0.40 ng/ul m

response 12497

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	19.90	20.46
236.00	29.60	29.40
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120225\
Data File : BN038268.D
Acq On : 02 Dec 2025 23:42
Operator : RC/JU
Sample : PB170722BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK722

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 12/03/2025
Supervised By :Sohil Jodhani 12/03/2025

Quant Time: Dec 03 01:40:14 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN112625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 01 16:36:13 2025
Response via : Initial Calibration

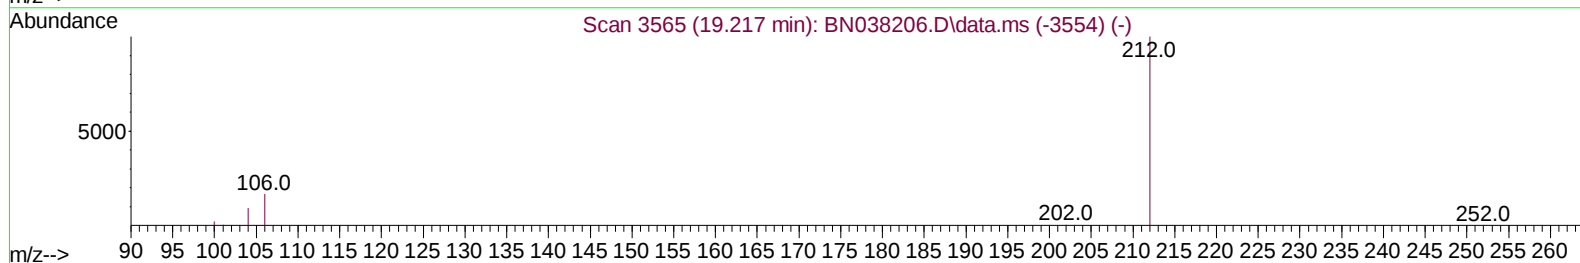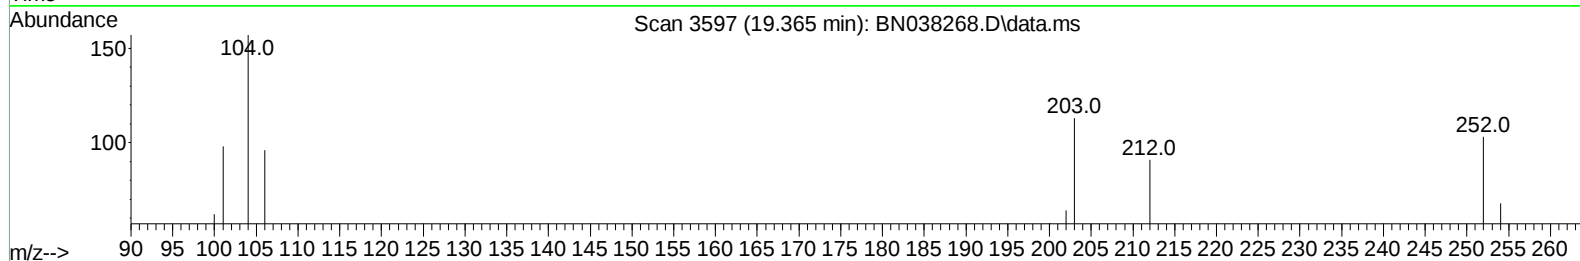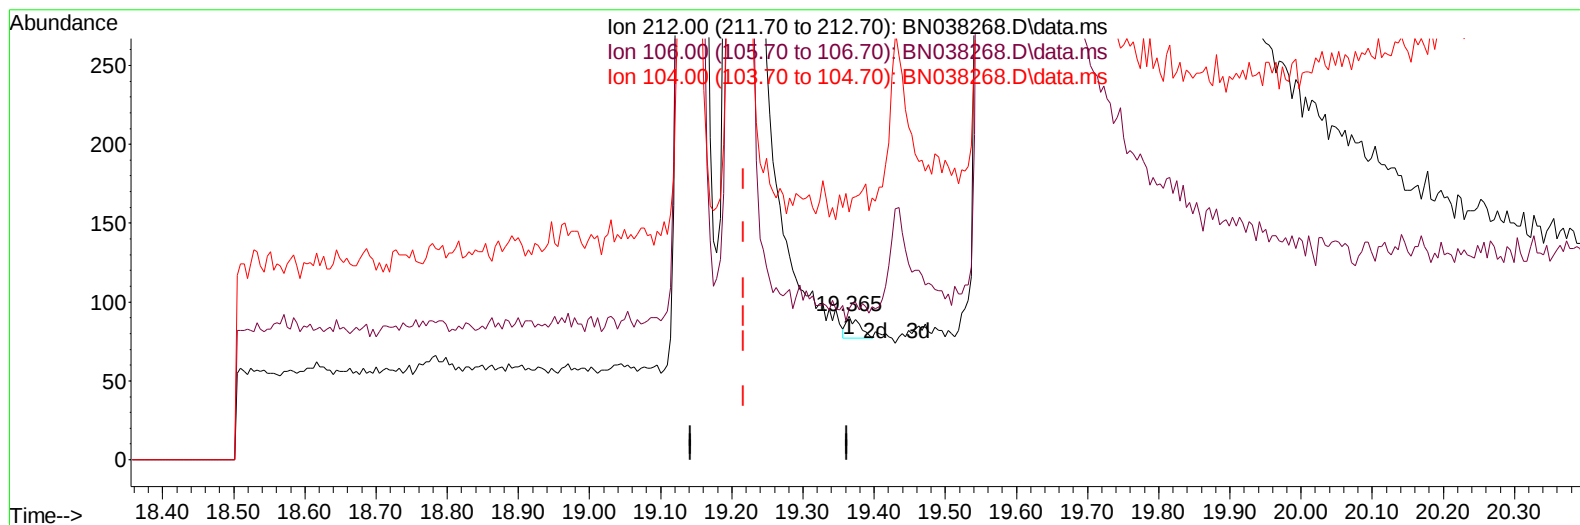

TIC: BN038268.D\data.ms

(18) Fluoranthene-d10 (SURR)

19.365min (+ 0.148) 0.00 ng/u1

response 18

Ion	Exp%	Act%
212.00	100.00	100.00
106.00	16.00	0.00#
104.00	9.20	72.22#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120225\
Data File : BN038268.D
Acq On : 02 Dec 2025 23:42
Operator : RC/JU
Sample : PB170722BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK722

Manual IntegrationsAPPROVED

Quant Time: Dec 03 01:40:14 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN112625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 01 16:36:13 2025
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/03/2025
Supervised By :Sohil Jodhani 12/03/2025

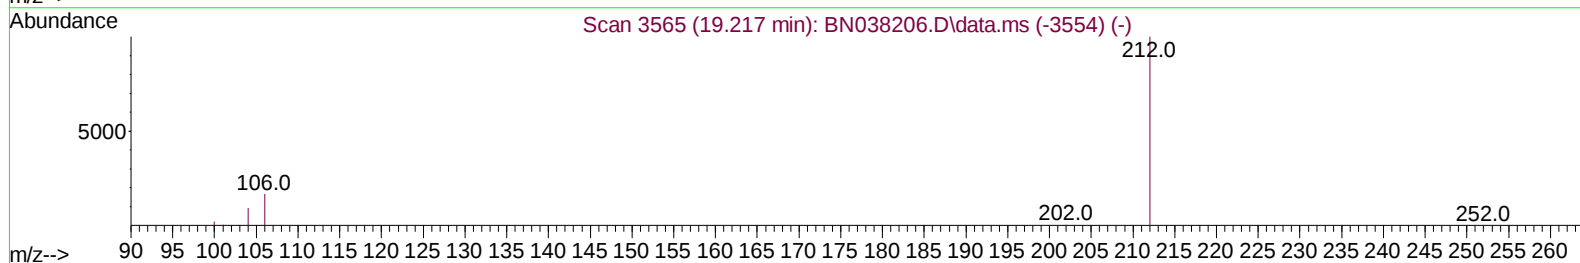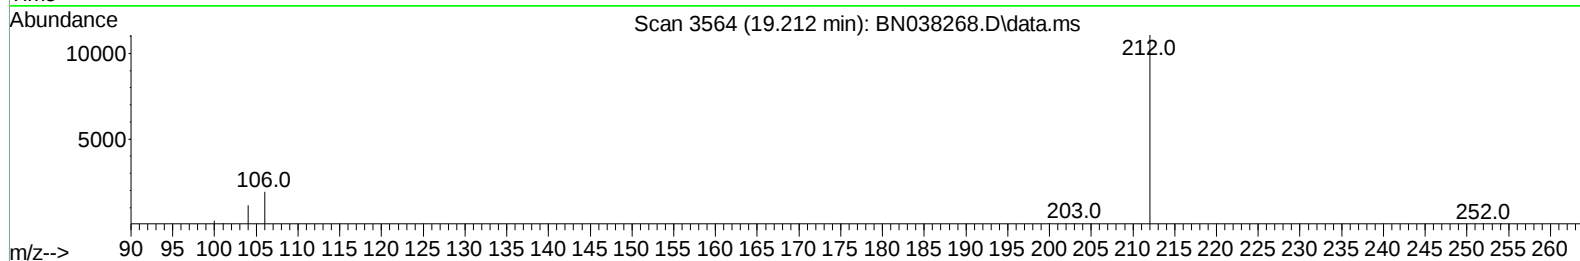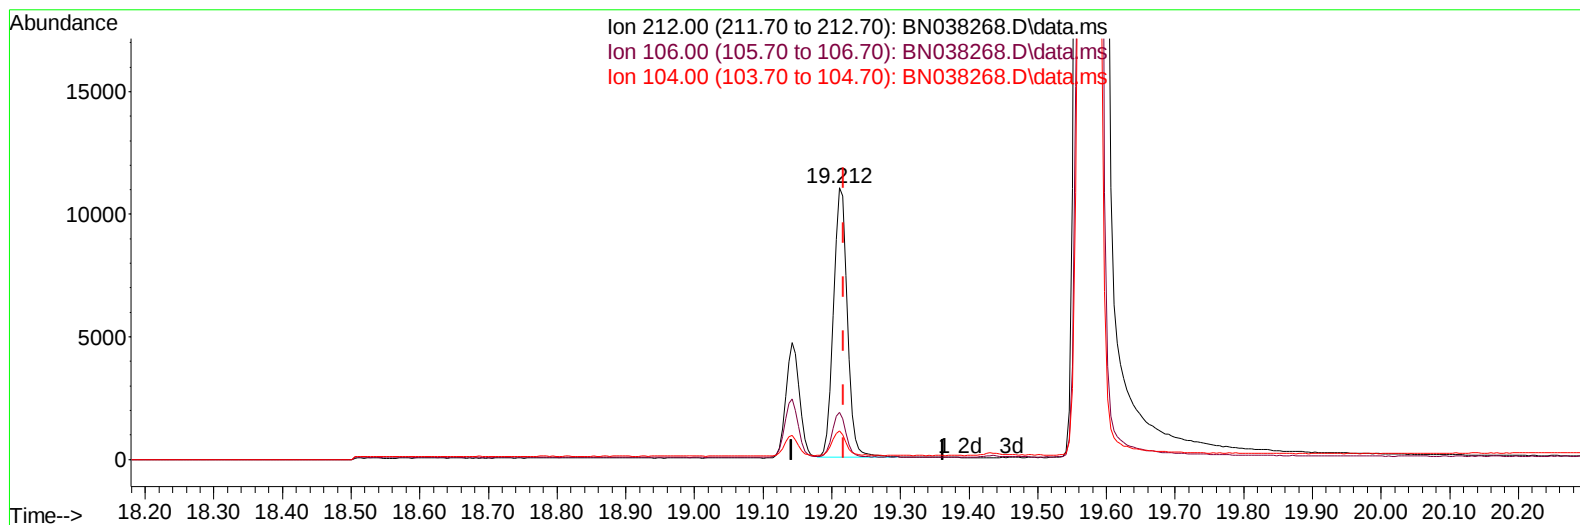

TIC: BN038268.D\data.ms

(18) Fluoranthene-d10 (SURR)

19.212min (-0.005) 0.32 ng/u1 m

response 15342

Ion	Exp%	Act%
212.00	100.00	100.00
106.00	16.00	0.00#
104.00	9.20	0.08#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120225\
Data File : BN038268.D
Acq On : 02 Dec 2025 23:42
Operator : RC/JU
Sample : PB170722BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK722

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 12/03/2025
Supervised By :Sohil Jodhani 12/03/2025

Quant Time: Dec 03 01:40:14 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN112625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 01 16:36:13 2025
Response via : Initial Calibration

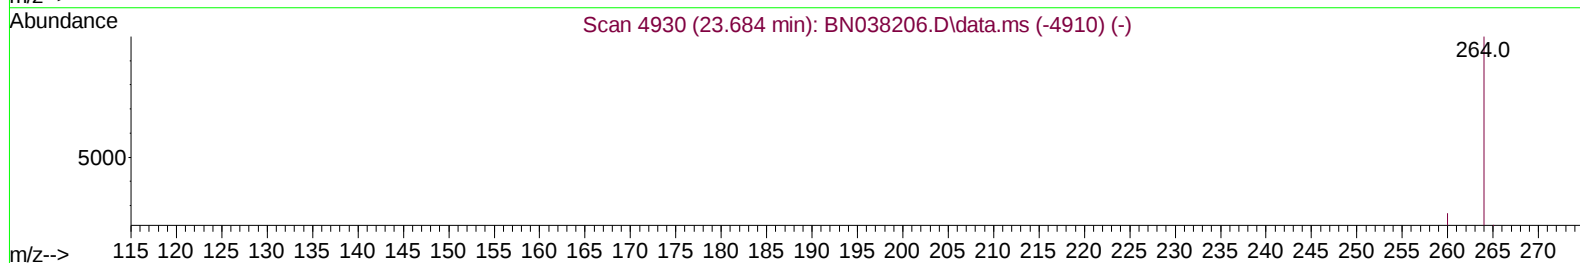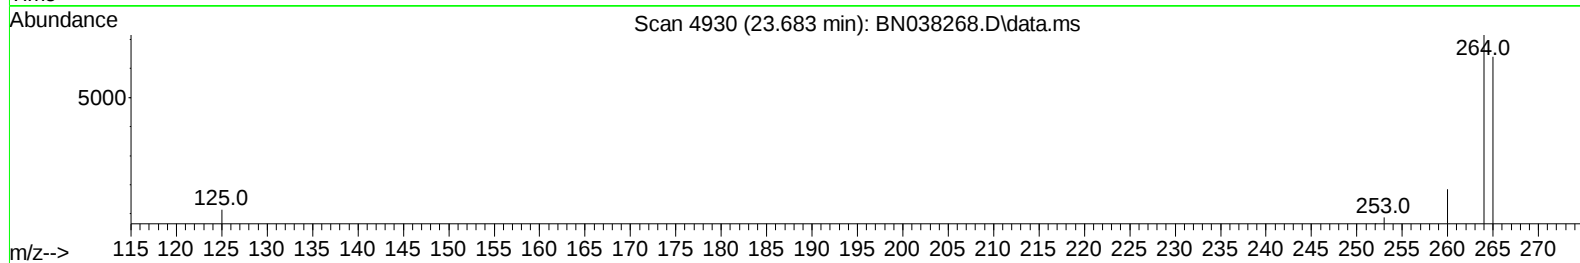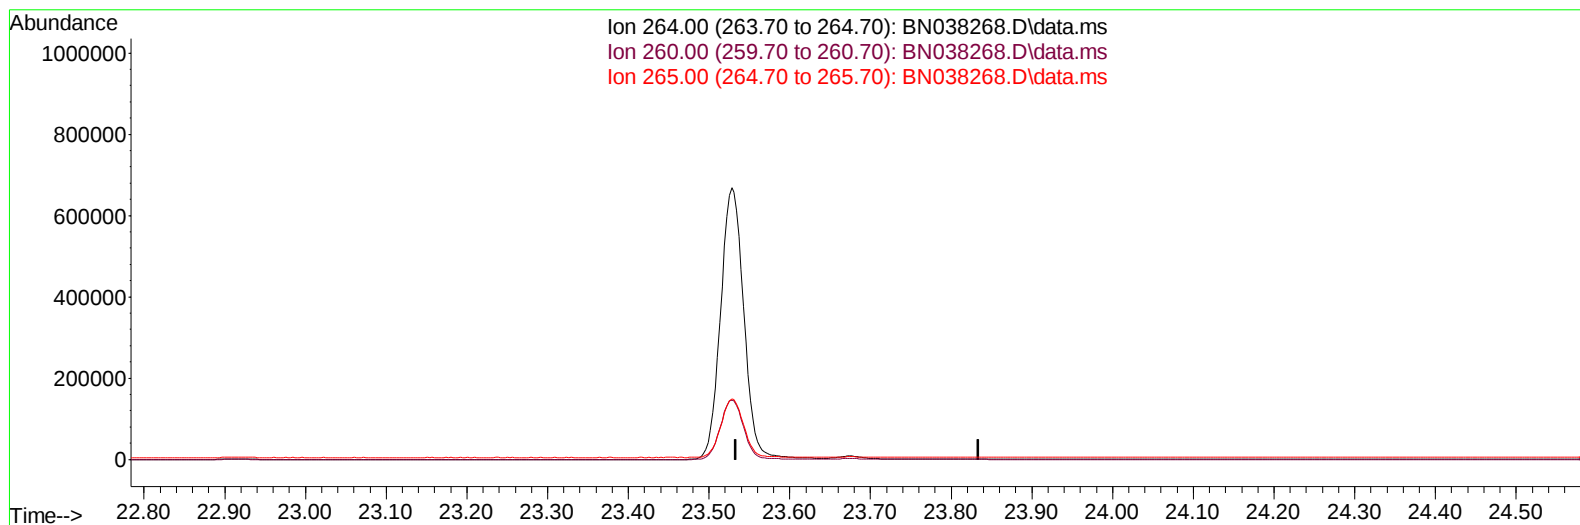

TIC: BN038268.D\data.ms

(23) Perylene-d12 (I)

23.684min (-23.684) 0.00 ng/u1

response 0

Ion	Exp%	Act%
264.00	100.00	0.00
260.00	27.40	0.00#
265.00	124.40	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120225\
Data File : BN038268.D
Acq On : 02 Dec 2025 23:42
Operator : RC/JU
Sample : PB170722BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK722

Manual IntegrationsAPPROVED

Quant Time: Dec 03 01:40:14 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN112625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 01 16:36:13 2025
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/03/2025
Supervised By :Sohil Jodhani 12/03/2025

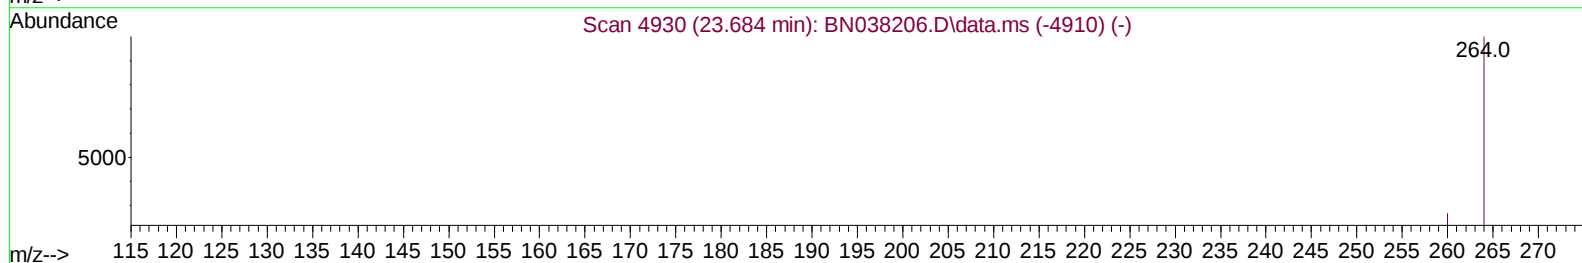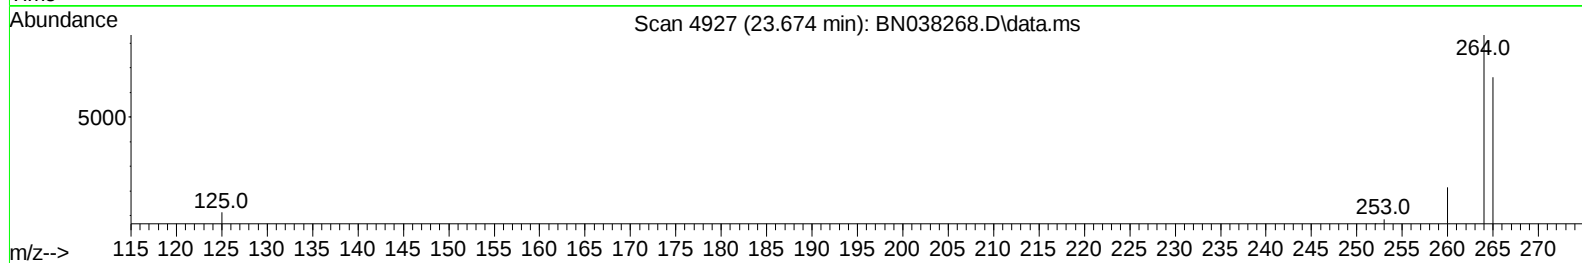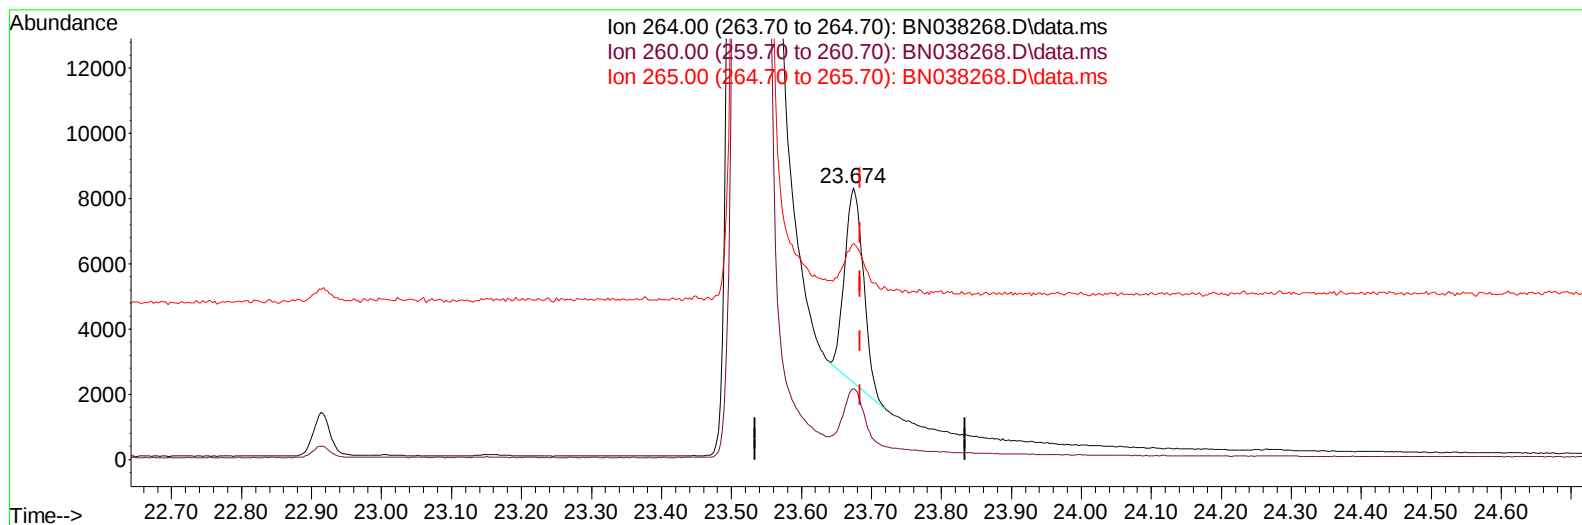

TIC: BN038268.D\data.ms

(23) Perylene-d12 (I)

23.674min (-0.010) 0.40 ng/ul m

response 11142

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.40	25.98
265.00	124.40	79.52#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120225\
 Data File : BN038268.D
 Acq On : 02 Dec 2025 23:42
 Operator : RC/JU
 Sample : PB170722BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK722

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 12/03/2025
 Supervised By :Sohil Jodhani 12/03/2025

Quant Time: Dec 03 01:40:14 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN112625.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 01 16:36:13 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.762	152	8301	0.400	ng/ul	0.00
4) Naphthalene-d8	10.562	136	26322	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.428	164	13967	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.179	188	20142m	0.400	ng/ul	0.00
17) Chrysene-d12	21.371	240	12497m	0.400	ng/ul	0.00
23) Perylene-d12	23.674	264	11142m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.210	96	59171	6.794	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.162	152	13225	0.352	ng/ul	-0.01
18) Fluoranthene-d10	19.212	212	15342m	0.316	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120225\
Data File : BN038268.D
Acq On : 02 Dec 2025 23:42
Operator : RC/JU
Sample : PB170722BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK722

Manual IntegrationsAPPROVED

Quant Time: Dec 03 01:40:14 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN112625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 01 16:36:13 2025
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/03/2025
Supervised By :Sohil Jodhani 12/03/2025

