

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120225\
 Data File : BN038257.D
 Acq On : 02 Dec 2025 16:26
 Operator : RC/JU
 Sample : Q3688-06
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 M-321

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 12/03/2025
 Supervised By :Sohil Jodhani 12/03/2025

Quant Time: Dec 03 00:43:24 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN112625.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 01 16:36:13 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.762	152	8089	0.400	ng/ul	0.00
4) Naphthalene-d8	10.568	136	24913	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.428	164	14131	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.180	188	23380m	0.400	ng/ul	0.00
17) Chrysene-d12	21.368	240	11606m	0.400	ng/ul	0.00
23) Perylene-d12	23.674	264	9964m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.214	96	42920	5.057	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.163	152	9207	0.259	ng/ul	-0.01
18) Fluoranthene-d10	19.212	212	21186m	0.470	ng/ul	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.248	88	308	0.034	ng/ul#	47

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120225\
Data File : BN038257.D
Acq On : 02 Dec 2025 16:26
Operator : RC/JU
Sample : Q3688-06
Misc :
ALS Vial : 9 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
M-32I

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 12/03/2025
Supervised By :Sohil Jodhani 12/03/2025


Quant Time: Dec 03 00:43:24 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN112625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 01 16:36:13 2025
Response via : Initial Calibration

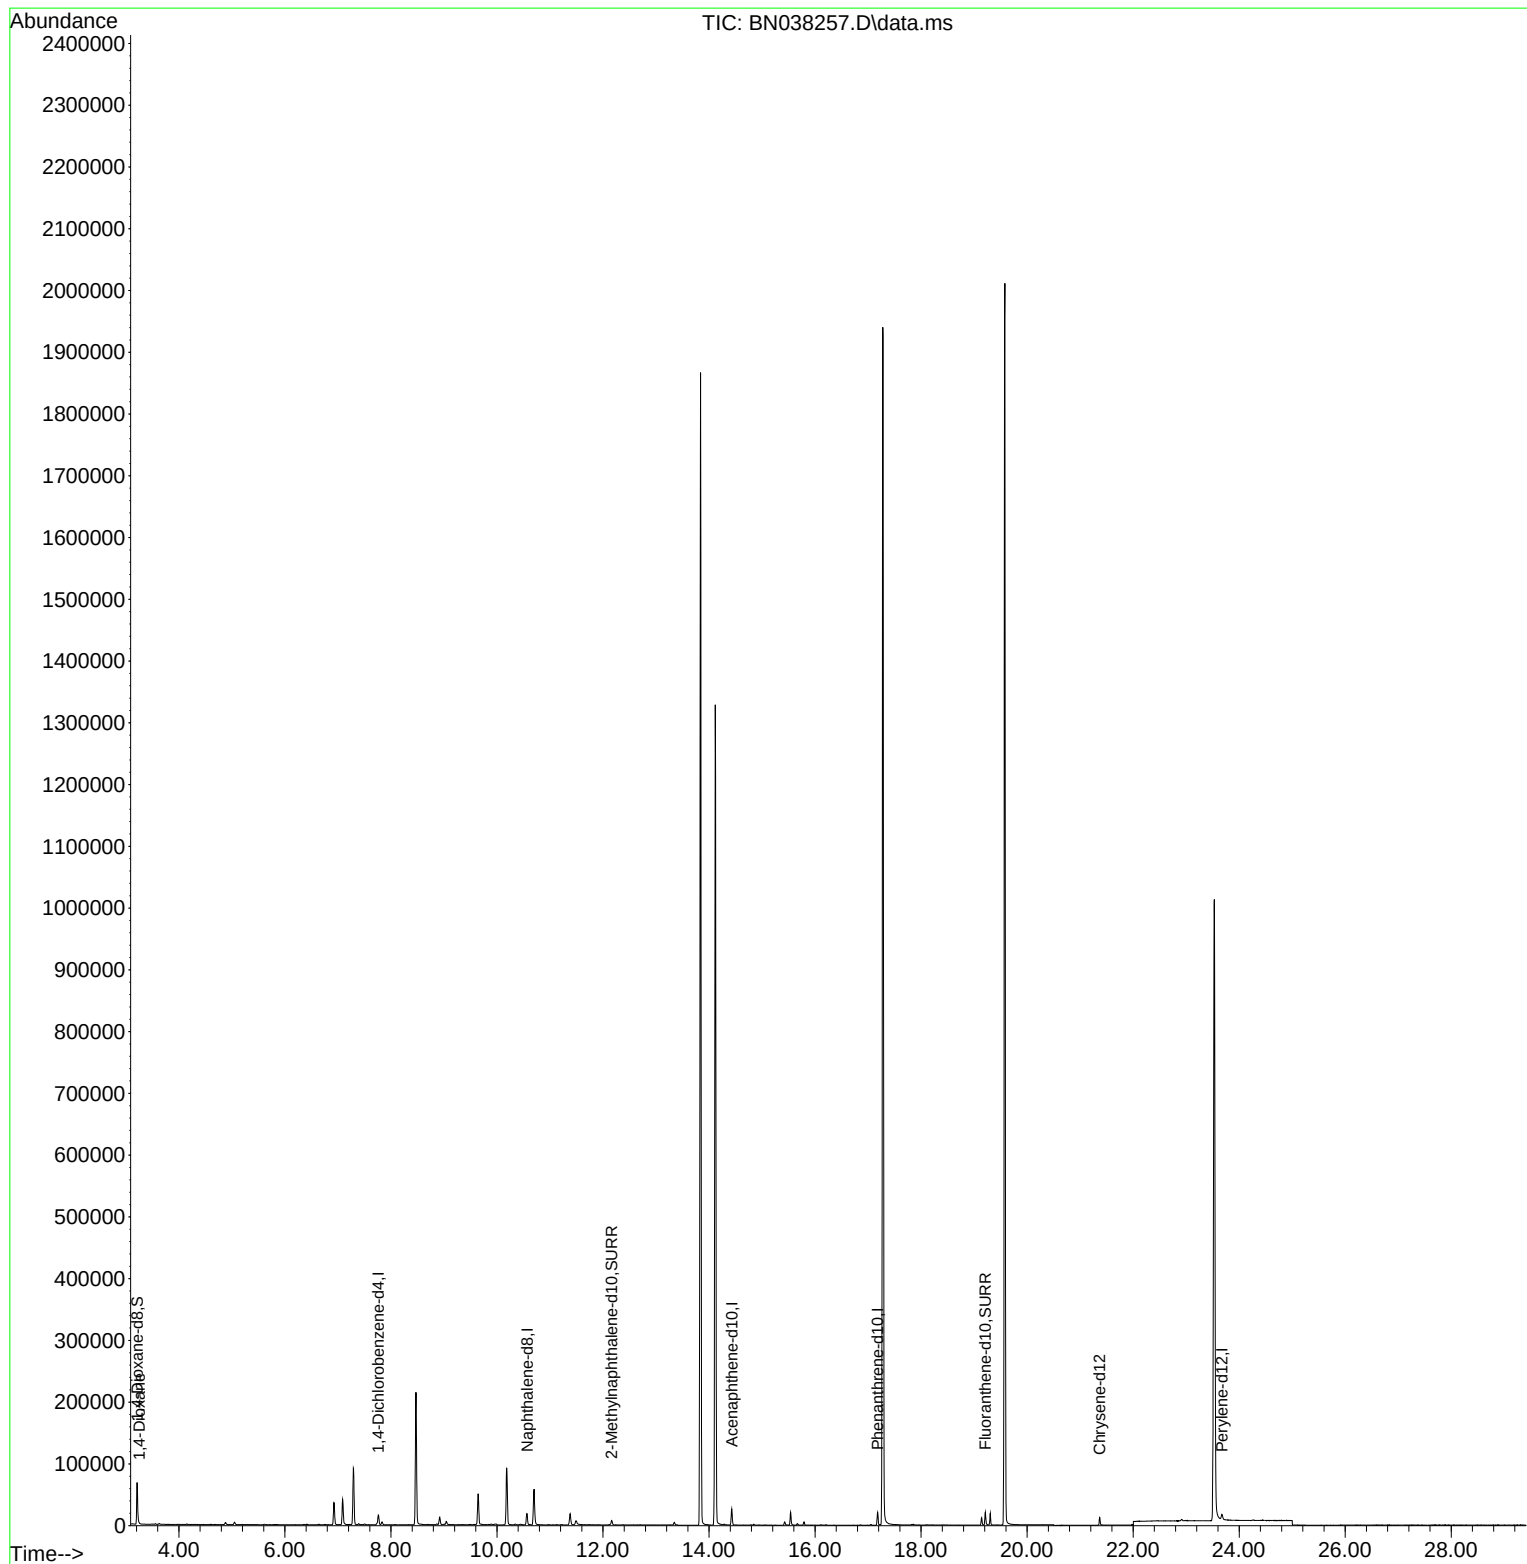

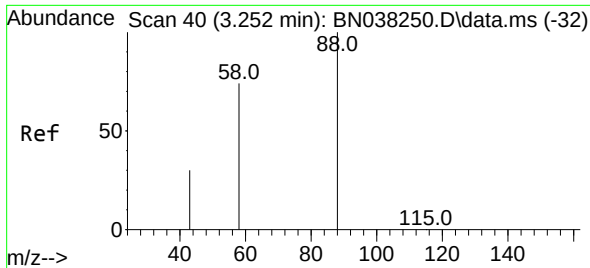

#2
 1,4-Dioxane
 Concen: 0.034 ng/ul
 RT: 3.248 min Scan# 39
 Delta R.T. -0.004 min
 Lab File: BN038257.D
 Acq: 02 Dec 2025 16:26

Instrument :
 BNA_N
 ClientSampleId :
 M-32I

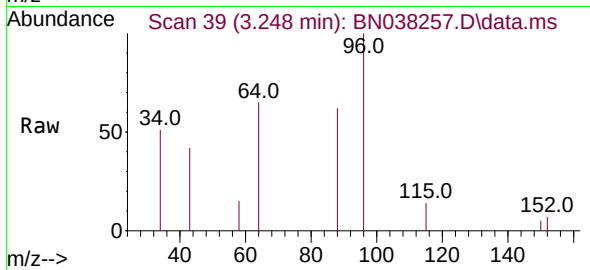

Tgt Ion: 88 Resp: 308

Ion	Ratio	Lower	Upper
88	100		
43	67.8	27.5	41.3
58	24.4	50.5	75.7

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 12/03/2025
 Supervised By :Sohil Jodhani 12/03/2025

