

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120225\
 Data File : BN038260.D
 Acq On : 02 Dec 2025 18:15
 Operator : RC/JU
 Sample : Q3688-11
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 RBGW-20251120

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 12/03/2025
 Supervised By :Sohil Jodhani 12/03/2025

Quant Time: Dec 03 01:04:52 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN112625.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 01 16:36:13 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc Units	Dev(Min)

Internal Standards					
1) 1,4-Dichlorobenzene-d4	7.762	152	8734	0.400 ng/ul	0.00
4) Naphthalene-d8	10.566	136	28184	0.400 ng/ul	0.00
9) Acenaphthene-d10	14.426	164	15261	0.400 ng/ul	0.00
13) Phenanthrene-d10	17.183	188	22280m	0.400 ng/ul	0.00
17) Chrysene-d12	21.372	240	12995m	0.400 ng/ul	0.00
23) Perylene-d12	23.675	264	11448m	0.400 ng/ul	0.00
System Monitoring Compounds					
3) 1,4-Dioxane-d8	3.214	96	46768	5.103 ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.167	152	11222	0.279 ng/ul	0.00
18) Fluoranthene-d10	19.215	212	19161m	0.379 ng/ul	0.00
Target Compounds					Qvalue
2) 1,4-Dioxane	3.252	88	538	0.054 ng/ul#	55

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120225\
Data File : BN038260.D
Acq On : 02 Dec 2025 18:15
Operator : RC/JU
Sample : Q3688-11
Misc :
ALS Vial : 12 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
RBGW-20251120

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 12/03/2025
Supervised By :Sohil Jodhani 12/03/2025


Quant Time: Dec 03 01:04:52 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN112625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 01 16:36:13 2025
Response via : Initial Calibration

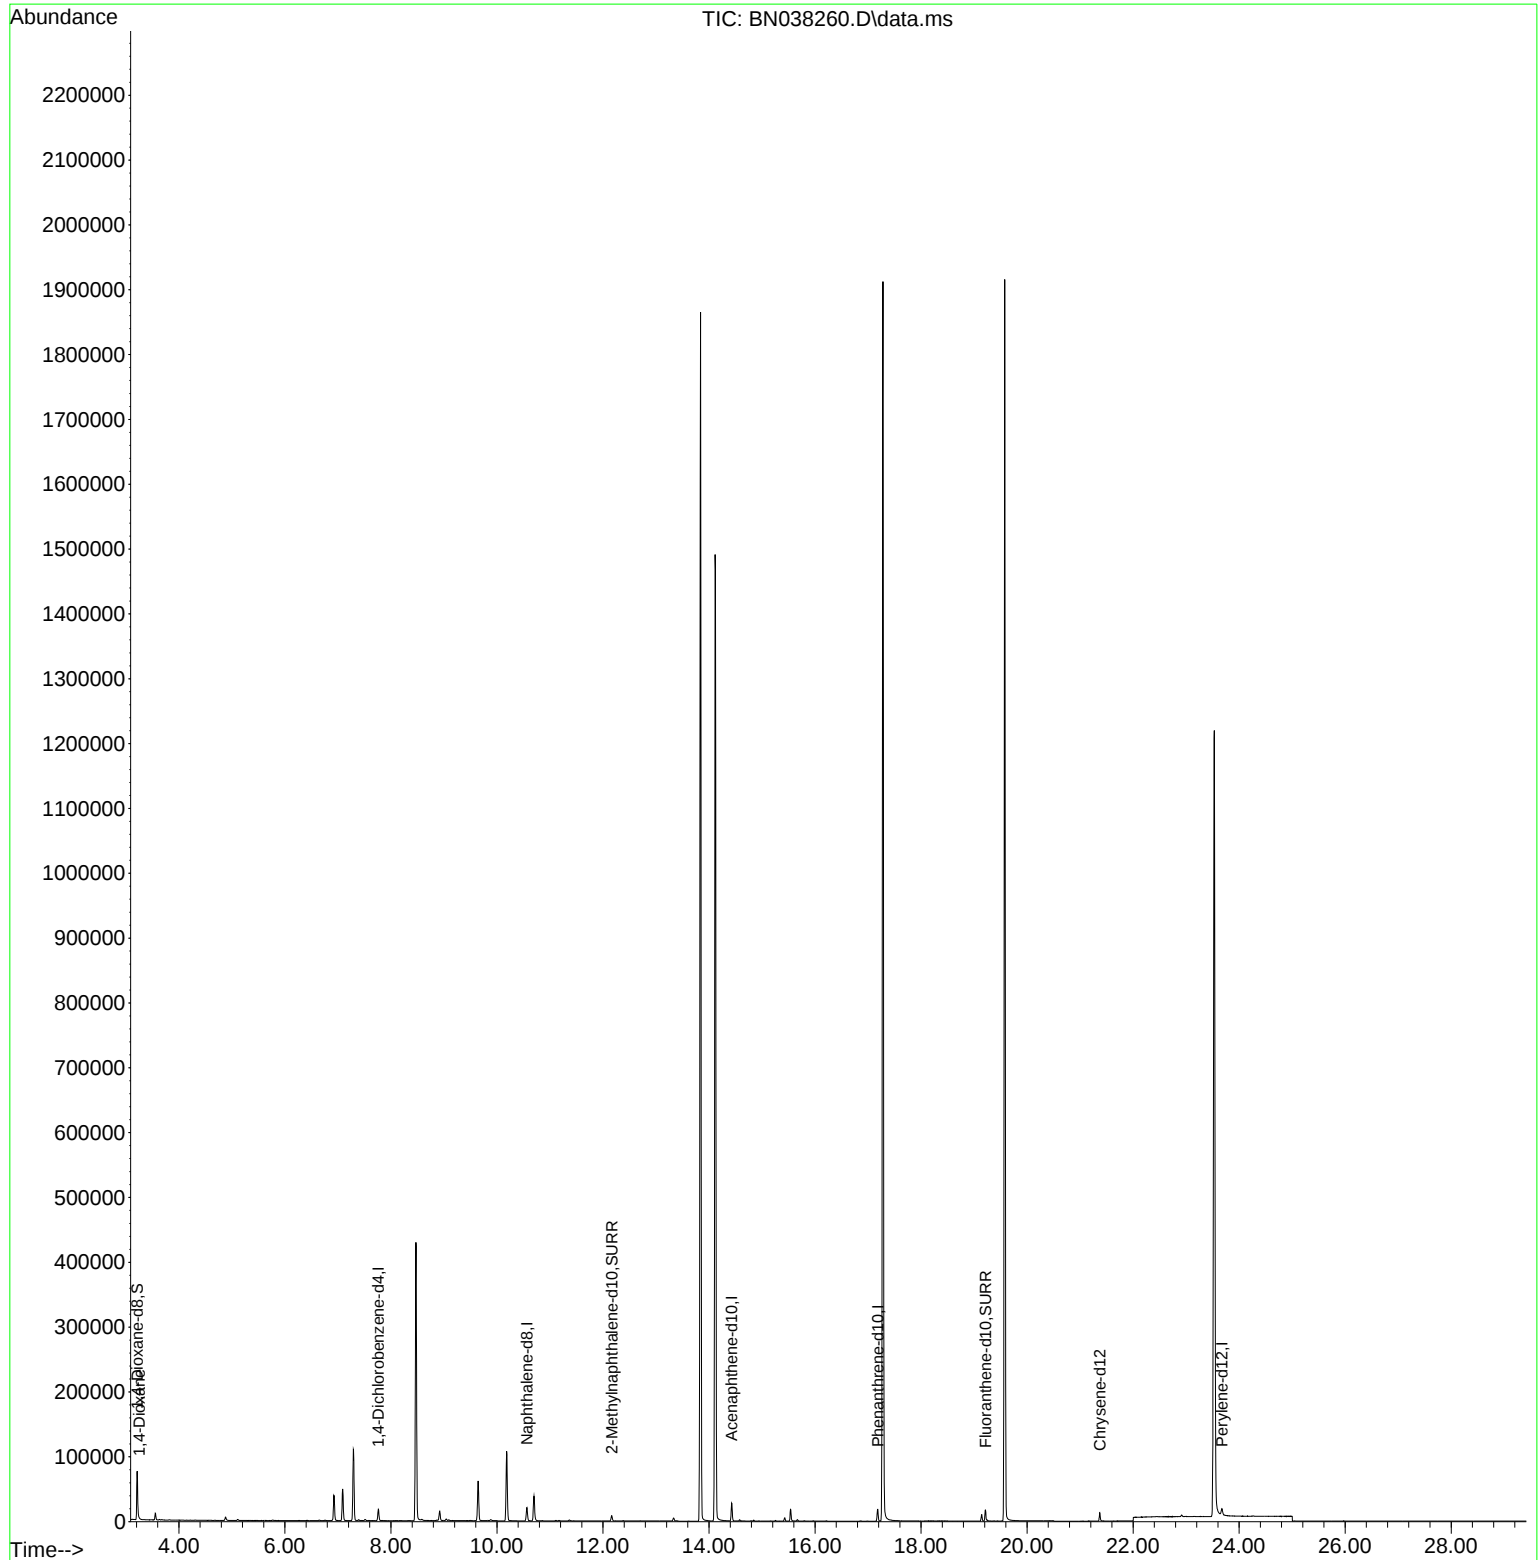

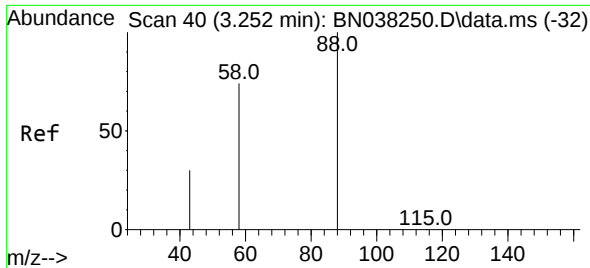

#2
 1,4-Dioxane
 Concen: 0.054 ng/ul
 RT: 3.252 min Scan# 40
 Delta R.T. 0.000 min
 Lab File: BN038260.D
 Acq: 02 Dec 2025 18:15

Instrument :
 BNA_N
 ClientSampleId :
 RBGW-20251120

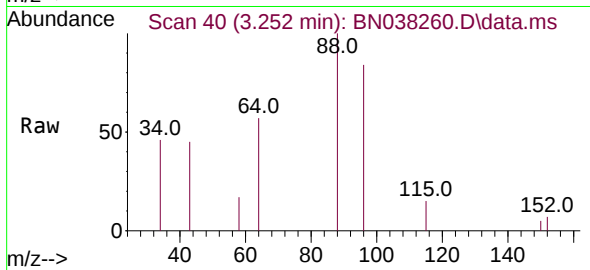

Tgt Ion: 88 Resp: 538
 Ion Ratio Lower Upper
 88 100
 43 45.1 27.5 41.3
 58 16.7 50.5 75.7

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 12/03/2025
 Supervised By :Sohil Jodhani 12/03/2025

