

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN120318\
Quantitation Report (Not Reviewed)

Data File : BN003679.D
Acq On : 03 Dec 2018 13:26
Operator : JU/SJ
Sample : J6096-10MSD
Misc :
ALS Vial : 5 Sample Multiplier: 1


Quant Time: Dec 04 01:20:01 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 04 01:17:12 2018
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
-----	-----	-----	-----	-----	-----	-----
1) 1,4-Dichlorobenzene-d4	7.84	152	4084	0.40	ng/ul	0.00
2) Naphthalene-d8	10.64	136	16271	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.47	164	8489	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.22	188	20737	0.40	ng/ul	0.00
16) Chrysene-d12	21.40	240	18036	0.40	ng/ul	0.00
20) Perylene-d12	23.71	264	16922	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.22	152	9375	0.37	ng/ul	0.00
14) Fluoranthene-d10	19.24	212	22020	0.36	ng/ul	0.00
Target Compounds						Qvalue
8) Acenaphthene	14.54	153	13509	0.403	ng/ul	100
11) Pentachlorophenol	16.86	266	2127	0.569	ng/ul	98
17) Pyrene	19.64	202	28560	0.442	ng/ul	99
-----	-----	-----	-----	-----	-----	-----

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BN003679.D
Acq On : 03 Dec 2018 13:26
Operator : JU/SJ
Sample : J6096-10MSD
Misc :
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Dec 04 01:20:01 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 04 01:17:12 2018
Response via : Initial Calibration

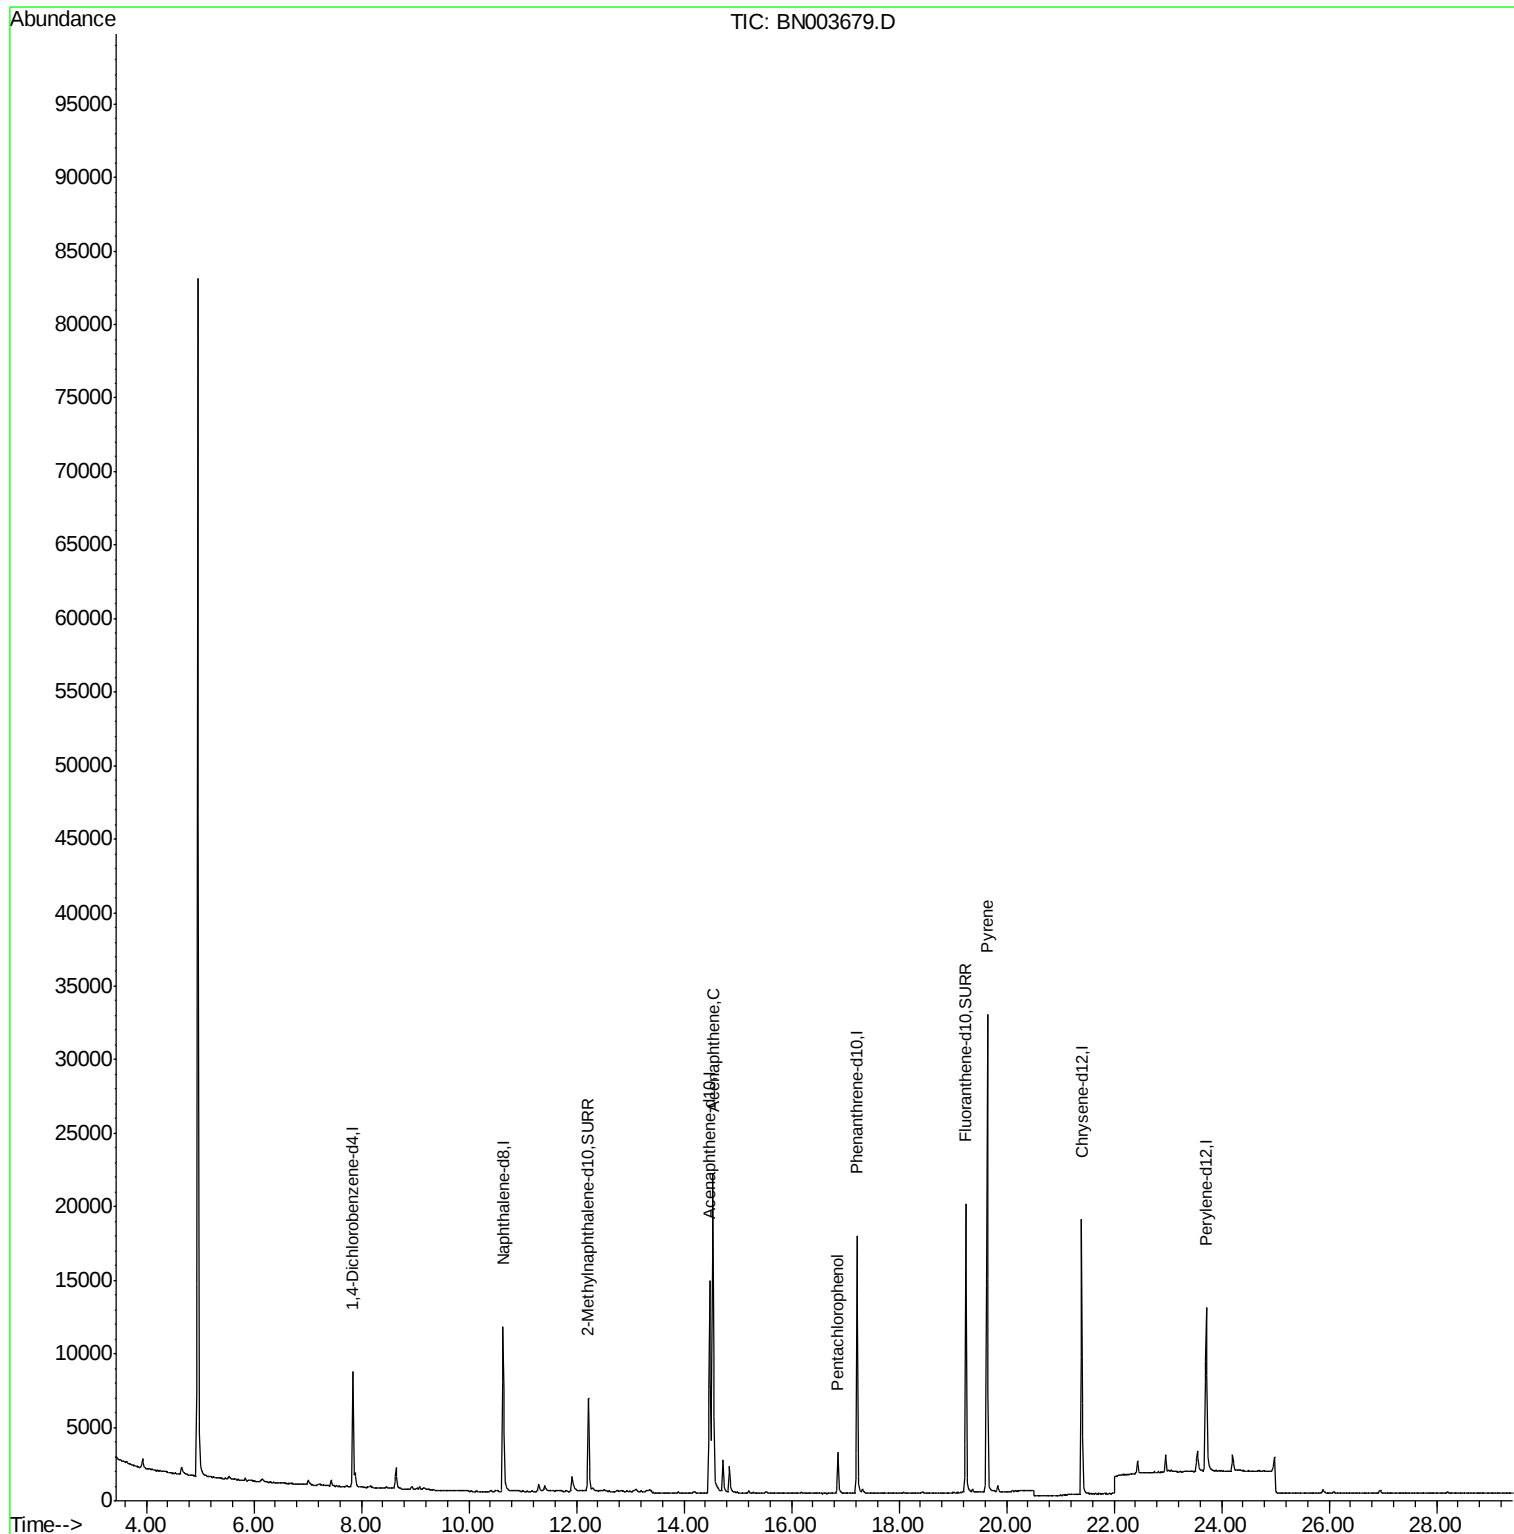

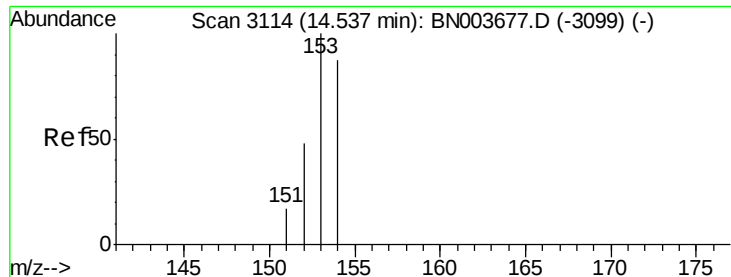

#8

Acenaphthene

Concen: 0.403 ng/ul

RT: 14.54 min Scan# 3114

Delta R.T. -0.00 min

Lab File: BN003679.D

Acq: 03 Dec 2018 13:26


Tgt Ion:153 Resp: 13509

Ion Ratio Lower Upper




153 100

152 48.5 39.3 58.9

154 87.9 70.3 105.5

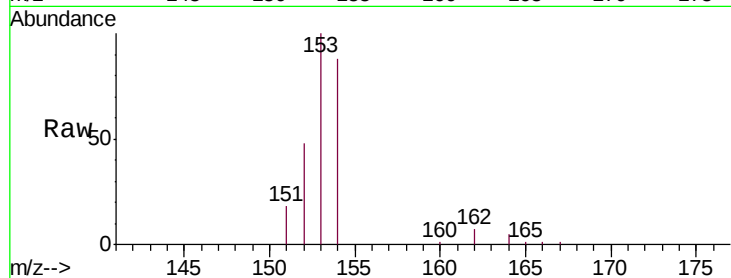

Abundance Ion 153.00 (152.70 to 153.70): E
Ion 152.00 (151.70 to 152.70): E
Ion 154.00 (153.70 to 154.70): E

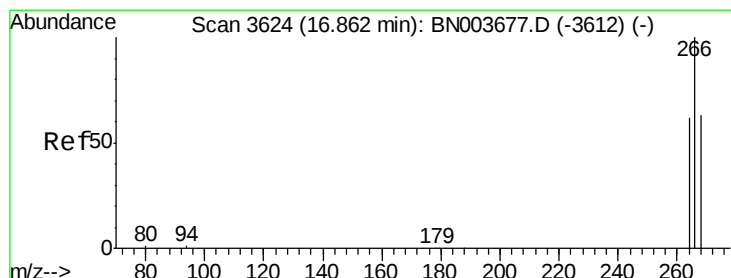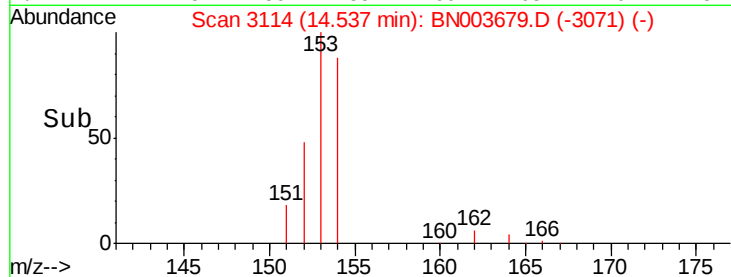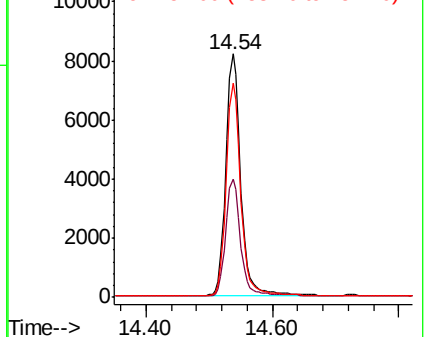

#11

Pentachlorophenol

Concen: 0.569 ng/ul

RT: 16.86 min Scan# 3624

Delta R.T. -0.00 min

Lab File: BN003679.D

Acq: 03 Dec 2018 13:26


Tgt Ion:266 Resp: 2127

Ion Ratio Lower Upper



266 100


264 63.0 49.4 74.2

268 62.2 51.7 77.5

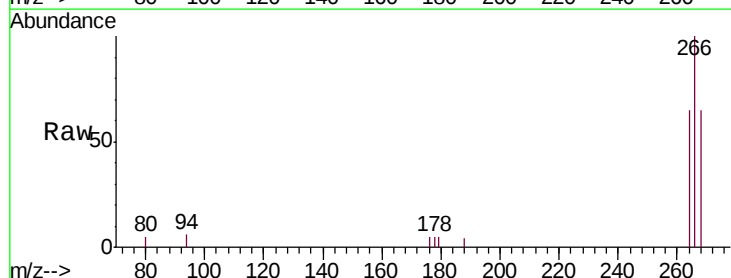

Abundance Ion 266.00 (265.70 to 266.70): E
Ion 264.00 (263.70 to 264.70): E
Ion 268.00 (267.70 to 268.70): E

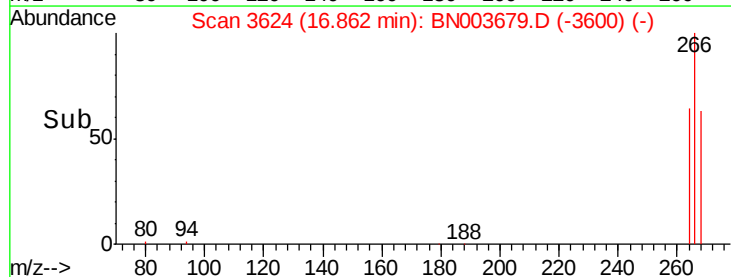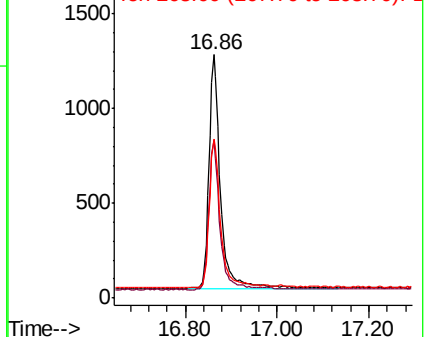

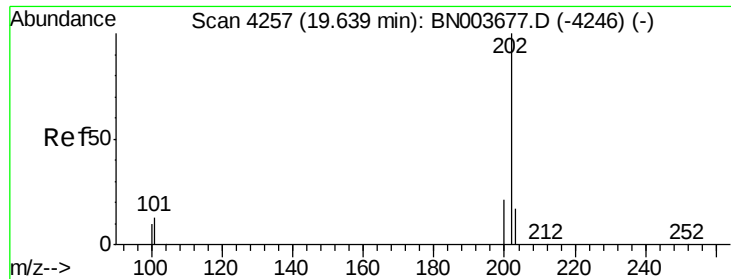

#17
 Pyrene
 Concen: 0.442 ng/ul
 RT: 19.64 min Scan# 4257
 Delta R.T. -0.00 min
 Lab File: BN003679.D
 Acq: 03 Dec 2018 13:26

Tgt Ion:	202	Resp:	28560
Ion	Ratio	Lower	Upper
202	100		
101	12.9	10.3	15.5
100	10.2	8.5	12.7

