

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN120318\
Quantitation Report (Not Reviewed)

Data File : BN003685.D
Acq On : 03 Dec 2018 19:24
Operator : JU/SJ
Sample : J6096-27
Misc :
ALS Vial : 6 Sample Multiplier: 1

Quant Time: Dec 04 01:26:56 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 04 01:23:55 2018
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	5197	0.40	ng/ul	0.00
2) Naphthalene-d8	10.63	136	21277	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.47	164	13612	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.32	188	2074744	0.40	ng/ul	0.10
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.40
20) Perylene-d12	23.71	264	28410	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.22	152	10829	0.33	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
9) Fluorene	15.47	166	3811	0.061	ng/ul#	12
23) Benzo(a)pyrene	23.56	252	8364	0.082	ng/ul#	72


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN120318\
Quantitation Report (Not Reviewed)

Data File : BN003685.D
Acq On : 03 Dec 2018 19:24
Operator : JU/SJ
Sample : J6096-27
Misc :
ALS Vial : 6 Sample Multiplier: 1





Quant Time: Dec 04 01:26:56 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 04 01:23:55 2018
Response via : Initial Calibration

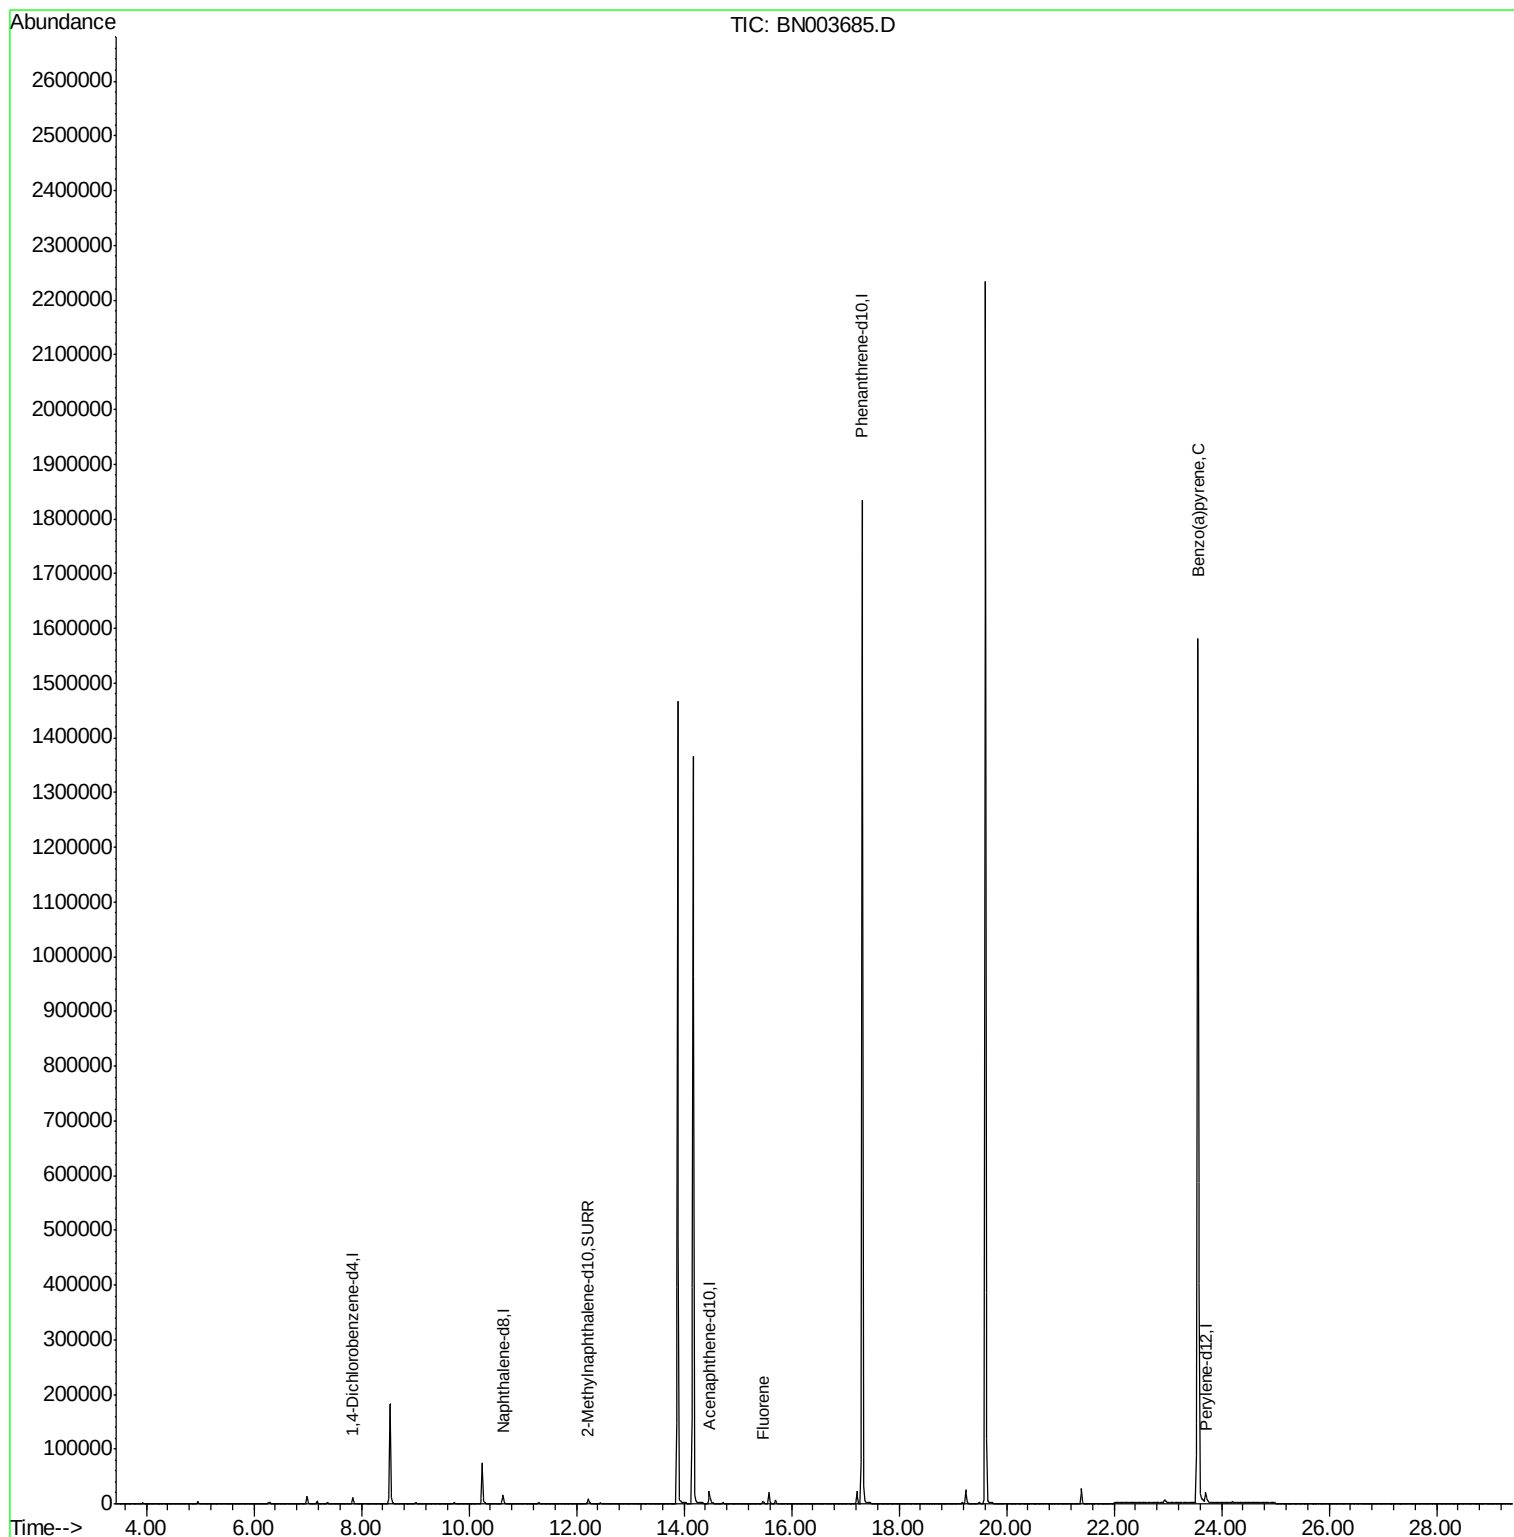

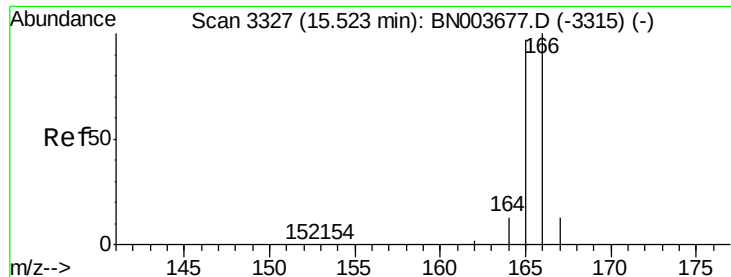

#9
Fluorene
 Concen: 0.061 ng/ul
 RT: 15.47 min Scan# 3315
 Delta R.T. -0.06 min
 Lab File: BN003685.D
 Acq: 03 Dec 2018 19:24

Tgt Ion:	166	Resp:	3811
Ion	Ratio	Lower	Upper
166	100		
165	5.2	78.3	117.5#
167	32.8	11.3	16.9#

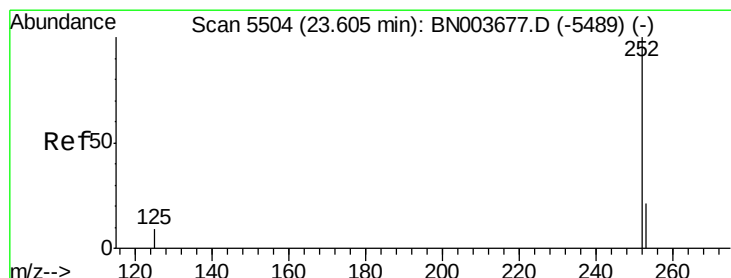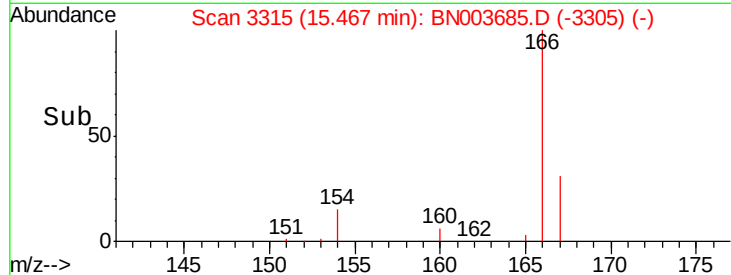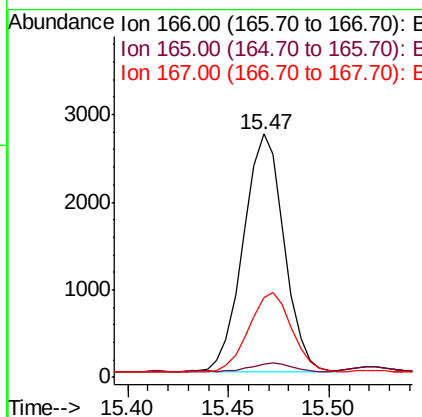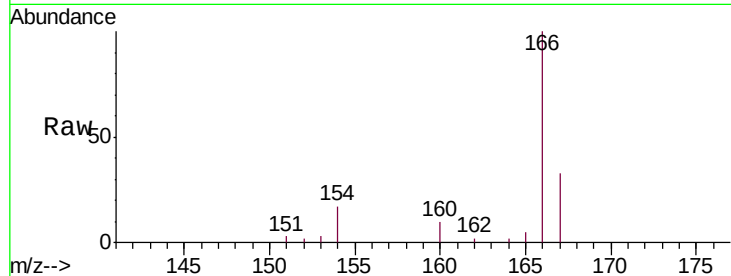

#23
Benzo(a)pyrene
 Concen: 0.082 ng/ul
 RT: 23.56 min Scan# 5489
 Delta R.T. -0.05 min
 Lab File: BN003685.D
 Acq: 03 Dec 2018 19:24

Tgt Ion:	252	Resp:	8364
Ion	Ratio	Lower	Upper
252	100		
253	34.9	19.0	28.4#
125	27.4	10.2	15.4#

