

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN120318\
Quantitation Report (QT Reviewed)

Data File : BN003682.D

Acq On : 03 Dec 2018 17:38

Operator : JU/SJ

Sample : PB115256BL

Misc :

ALS Vial : 3 Sample Multiplier: 1


Quant Time: Dec 04 01:30:08 2018

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Dec 04 01:23:55 2018




Response via : Initial Calibration

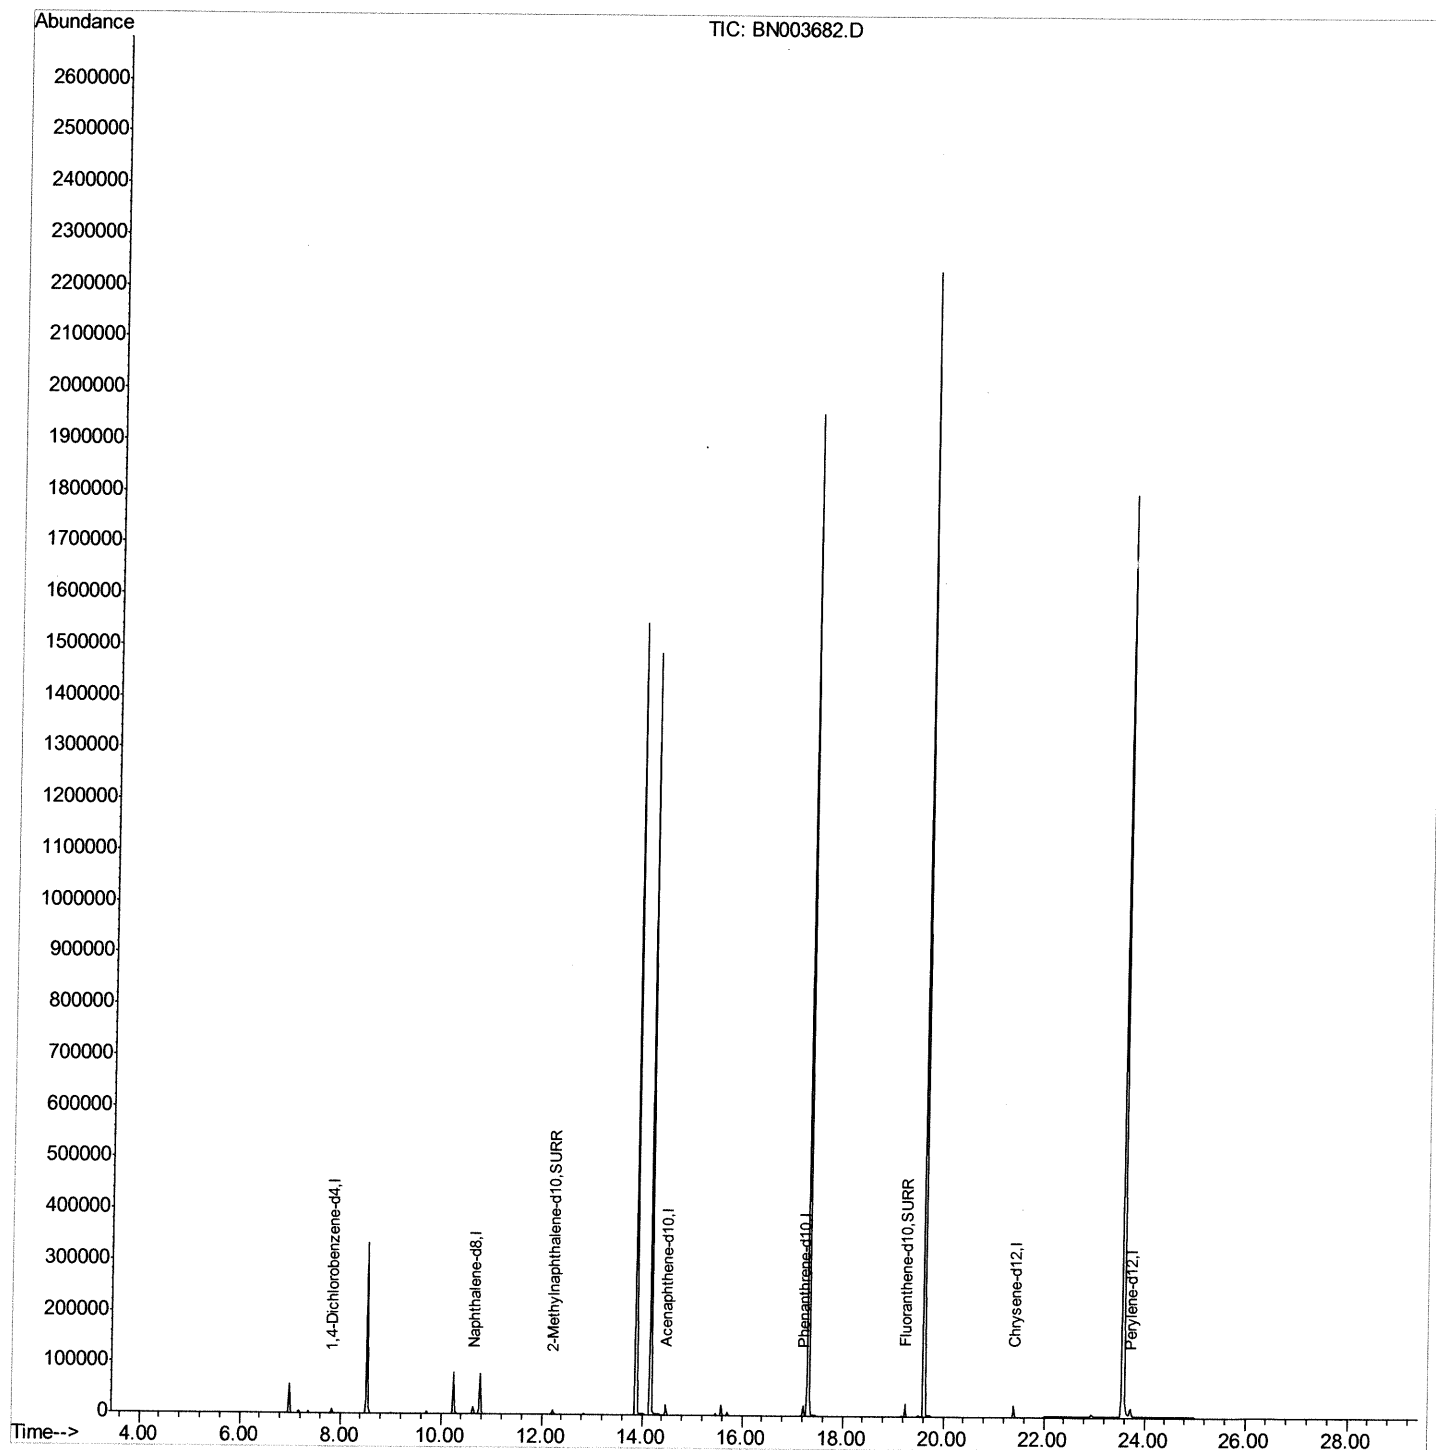

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN120318\
Quantitation Report (Qedit)

Data File : BN003682.D
Acq On : 03 Dec 2018 17:38
Operator : JU/SJ
Sample : PB115256BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Dec 04 01:26:41 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 04 01:23:55 2018
Response via : Initial Calibration

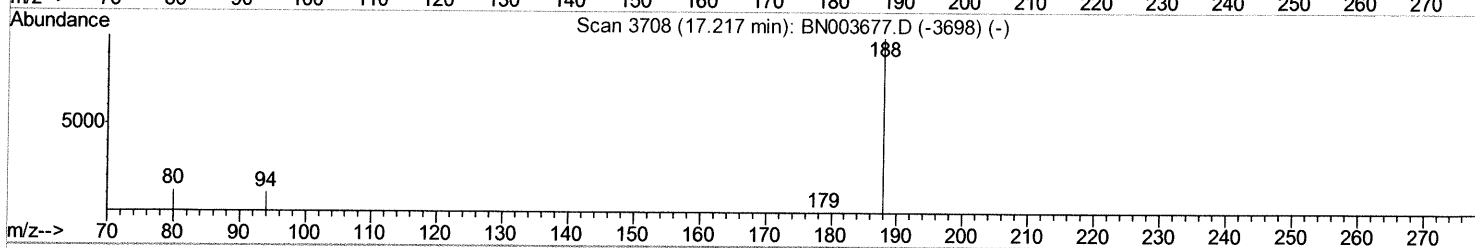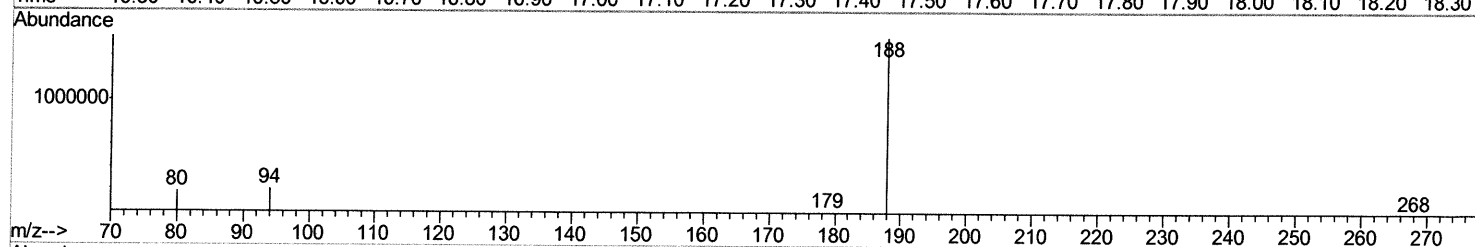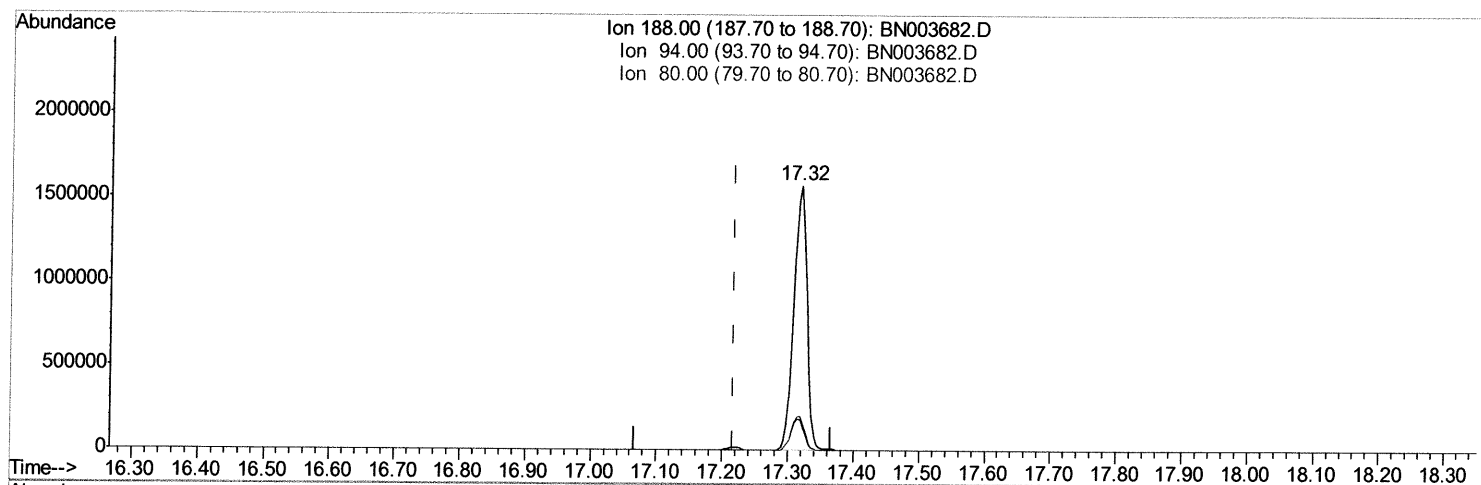

TIC: BN003682.D

(10) Phenanthrene-d10 (I)

17.318min (+0.101) 0.40ng/ul




response 2148520

Ion	Exp%	Act%
188.00	100	100
94.00	10.40	12.93#
80.00	11.60	11.49
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN120318\
Quantitation Report (Qedit)

Data File : BN003682.D
Acq On : 03 Dec 2018 17:38
Operator : JU/SJ
Sample : PB115256BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Dec 04 01:26:41 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 04 01:23:55 2018
Response via : Initial Calibration

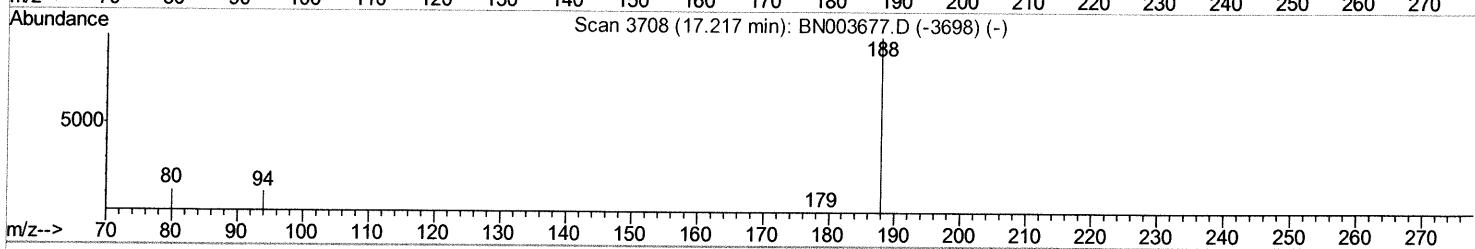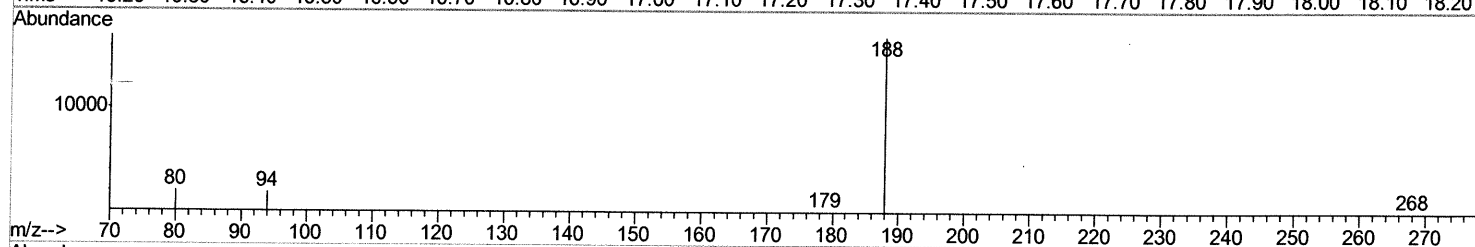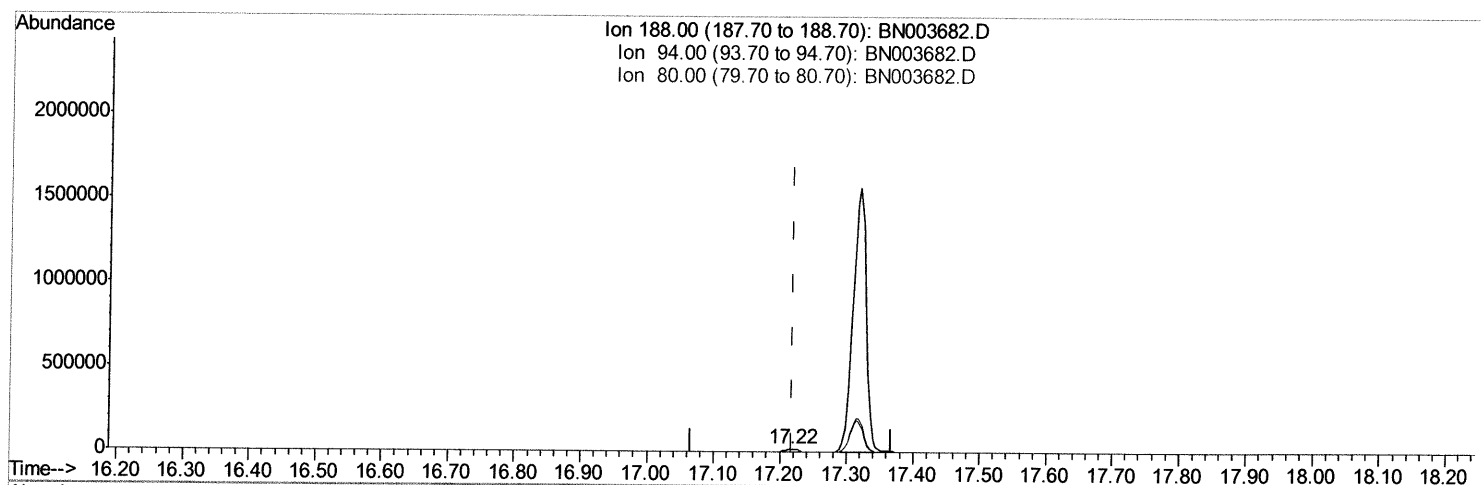

TIC: BN003682.D

(10) Phenanthrene-d10 (I)

17.217min (-0.000) 0.40ng/ul m>

50 12/11/18




response 23315

Ion	Exp%	Act%
188.00	100	100
94.00	10.40	10.88
80.00	11.60	11.79
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN120318\
Quantitation Report (Qedit)

Data File : BN003682.D
Acq On : 03 Dec 2018 17:38
Operator : JU/SJ
Sample : PB115256BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Dec 04 01:28:45 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 04 01:23:55 2018
Response via : Initial Calibration

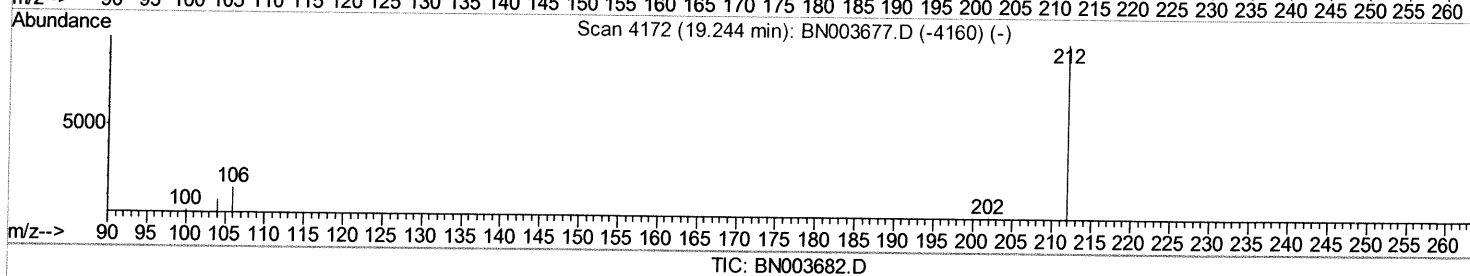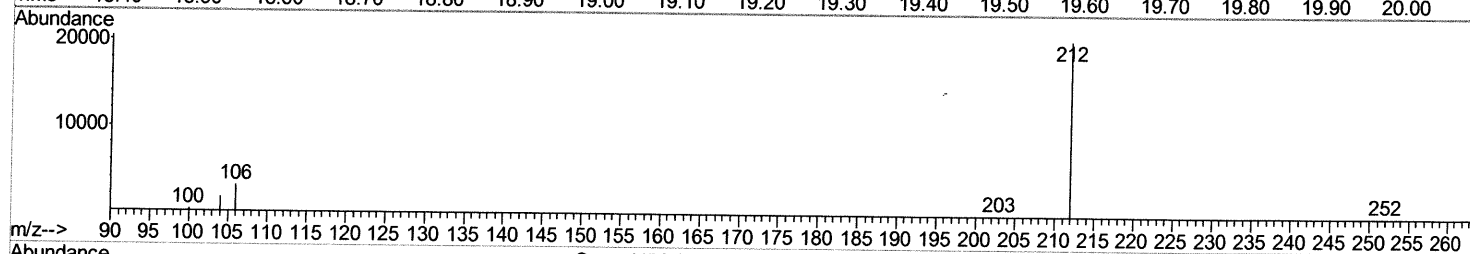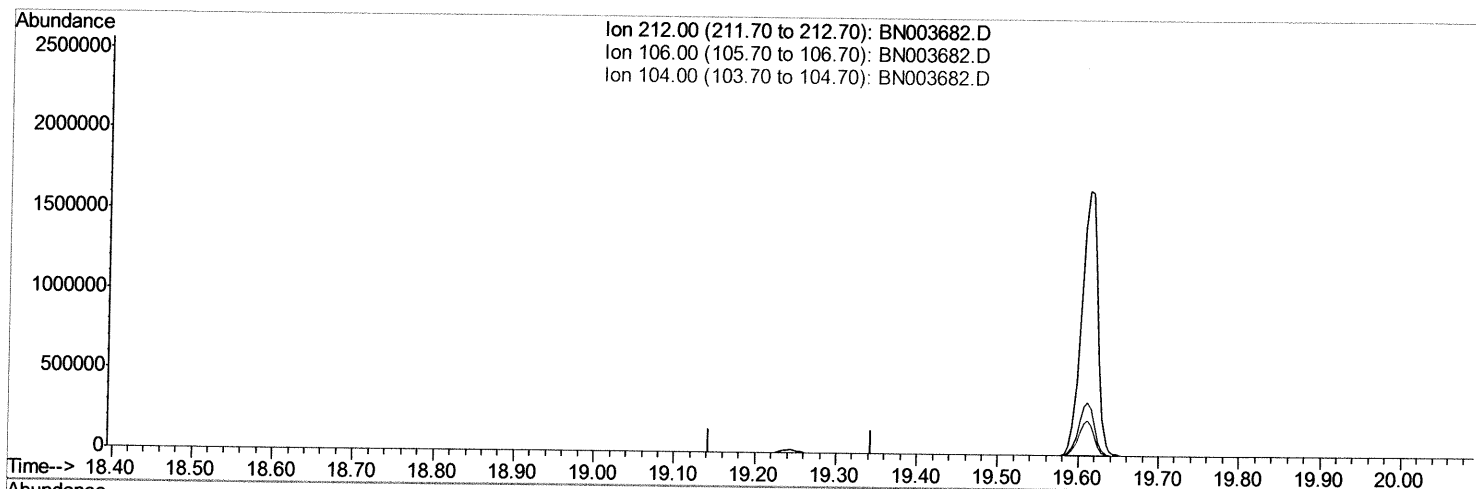

(14) Fluoranthene-d10 (SURR)

19.244min (-19.244) 0.00ng/ul




response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	14.20	0.00#
104.00	8.00	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN120318\
Quantitation Report (Qedit)

Data File : BN003682.D
Acq On : 03 Dec 2018 17:38
Operator : JU/SJ
Sample : PB115256BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Dec 04 01:28:45 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 04 01:23:55 2018
Response via : Initial Calibration

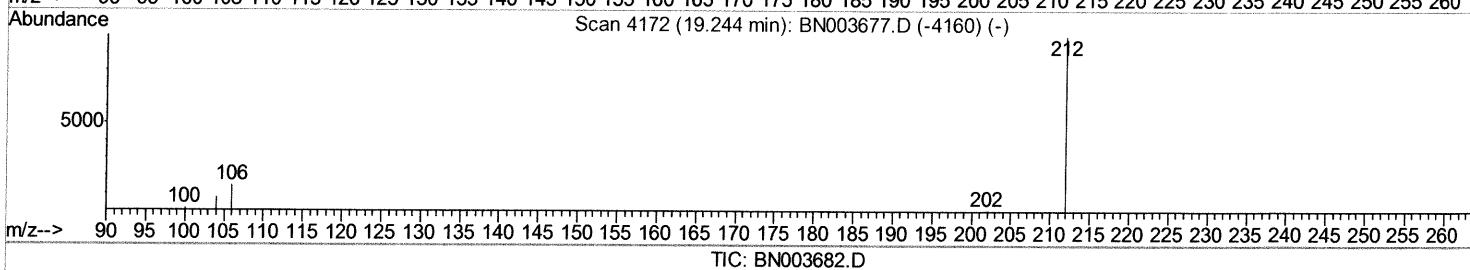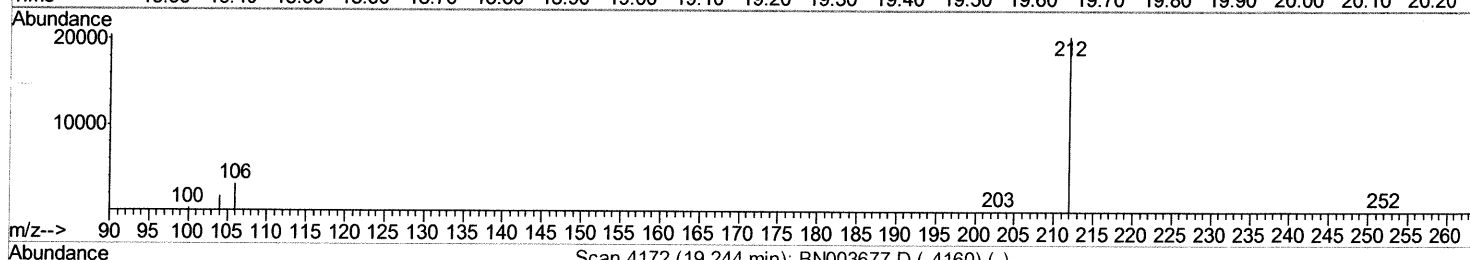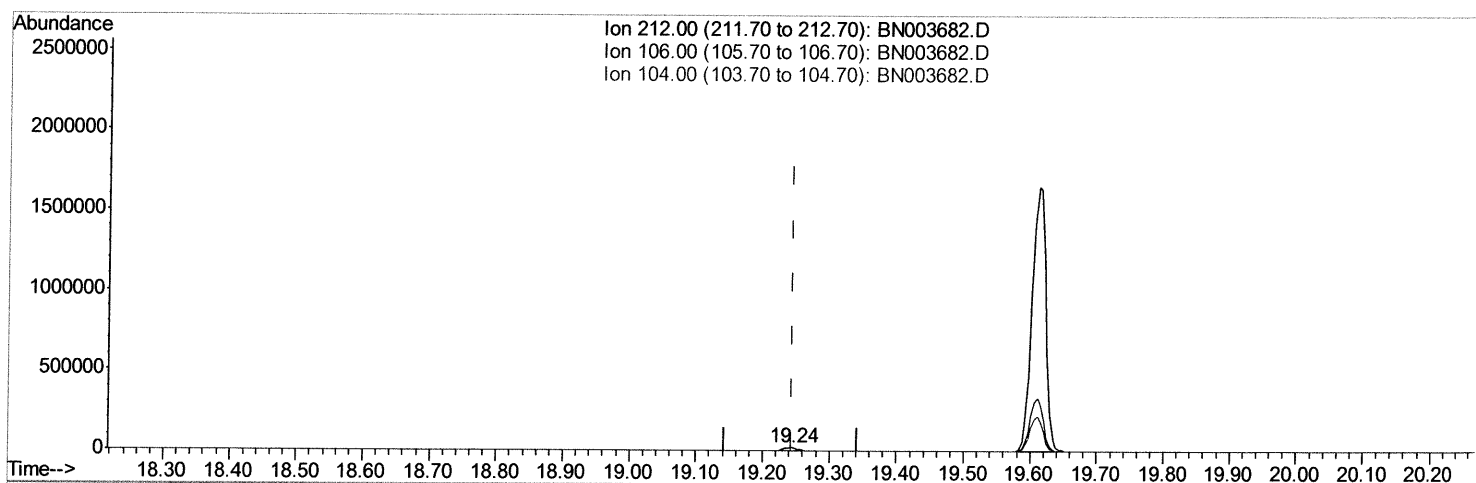

(14) Fluoranthene-d10 (SURR)

19.243min (-0.000) 0.40ng/ul m) SJ 12/11/18




response 27180

Ion	Exp%	Act%
212.00	100	100
106.00	14.20	0.00#
104.00	8.00	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN120318\
Quantitation Report (Qedit)

Data File : BN003682.D
Acq On : 03 Dec 2018 17:38
Operator : JU/SJ
Sample : PB115256BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Dec 04 01:28:45 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 04 01:23:55 2018
Response via : Initial Calibration

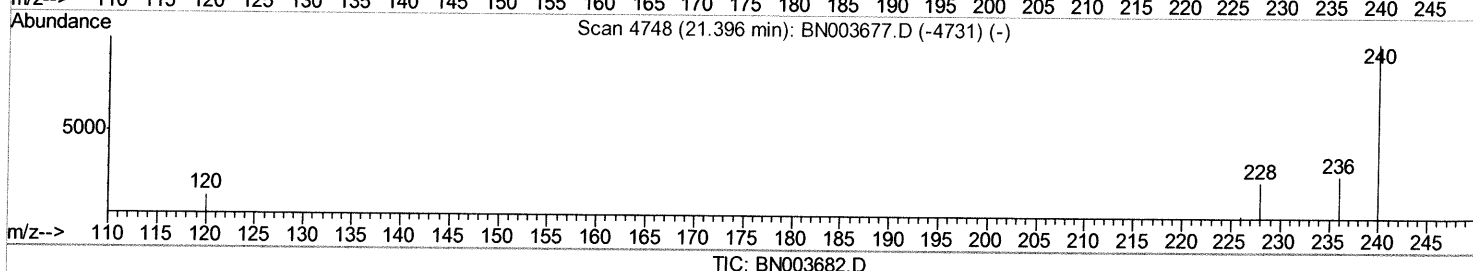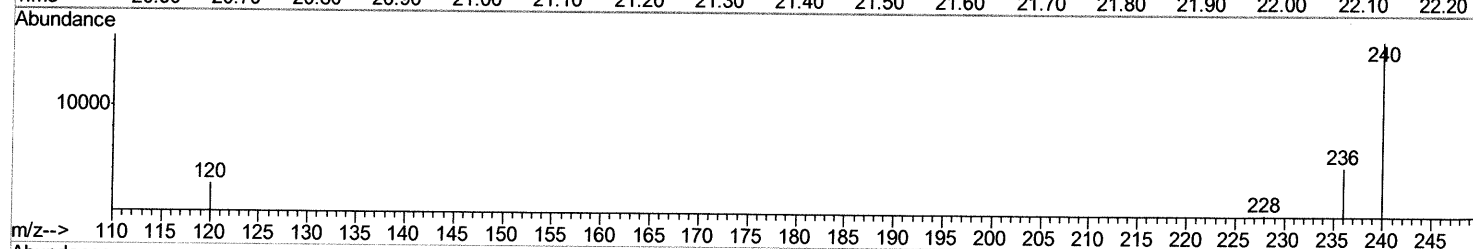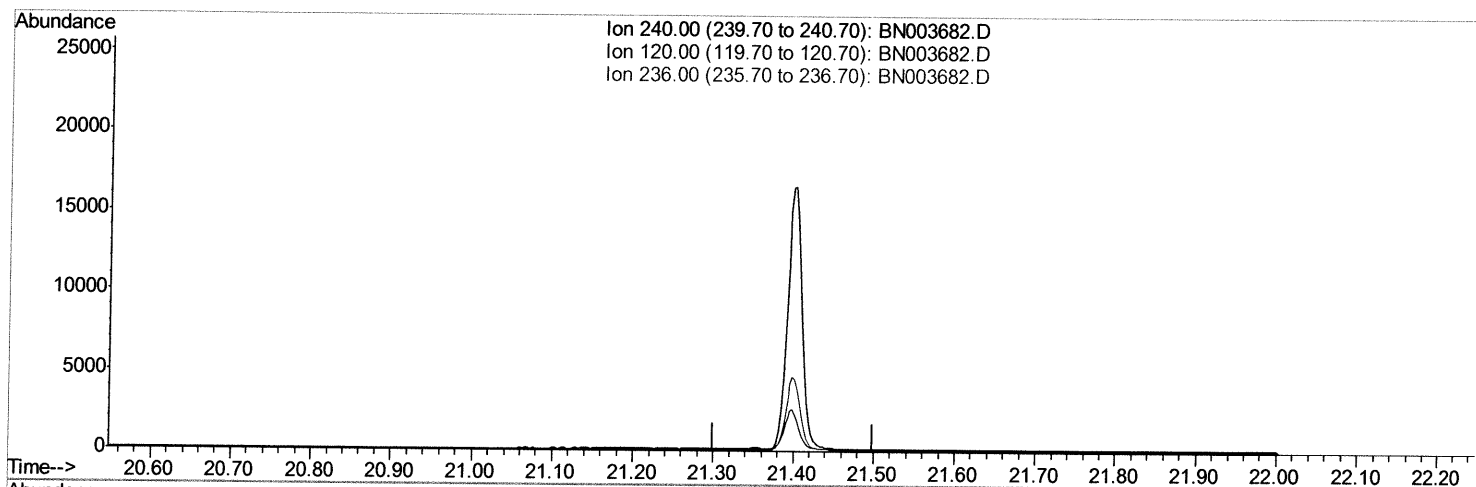

TIC: BN003682.D

(16) Chrysene-d12 (I)

21.400min (-21.400) 0.00ng/ul




response 0

Ion	Exp%	Act%
240.00	100	0.00
120.00	14.00	0.00#
236.00	27.60	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN120318\
Quantitation Report (Qedit)

Data File : BN003682.D
Acq On : 03 Dec 2018 17:38
Operator : JU/SJ
Sample : PB115256BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Dec 04 01:28:45 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 04 01:23:55 2018
Response via : Initial Calibration

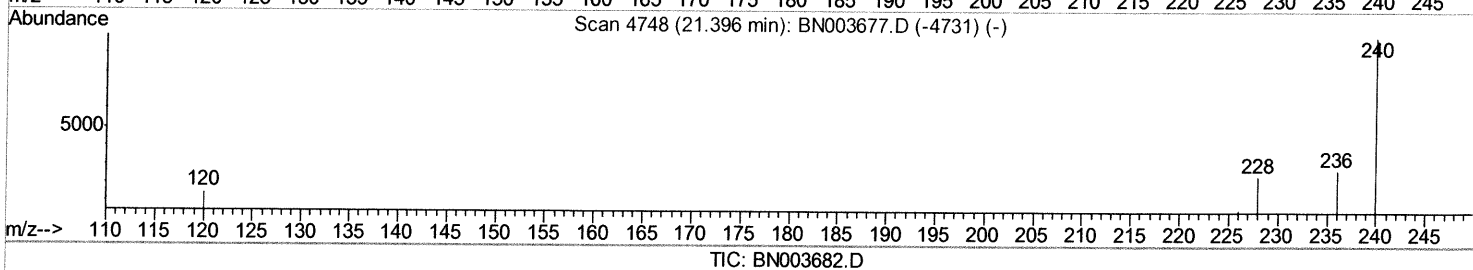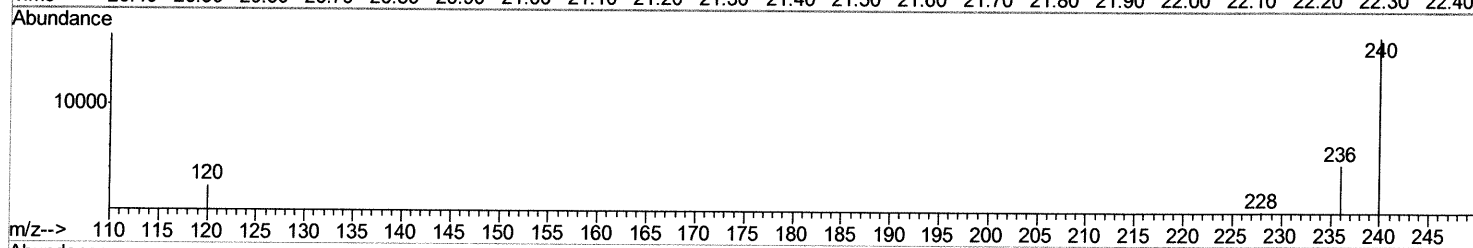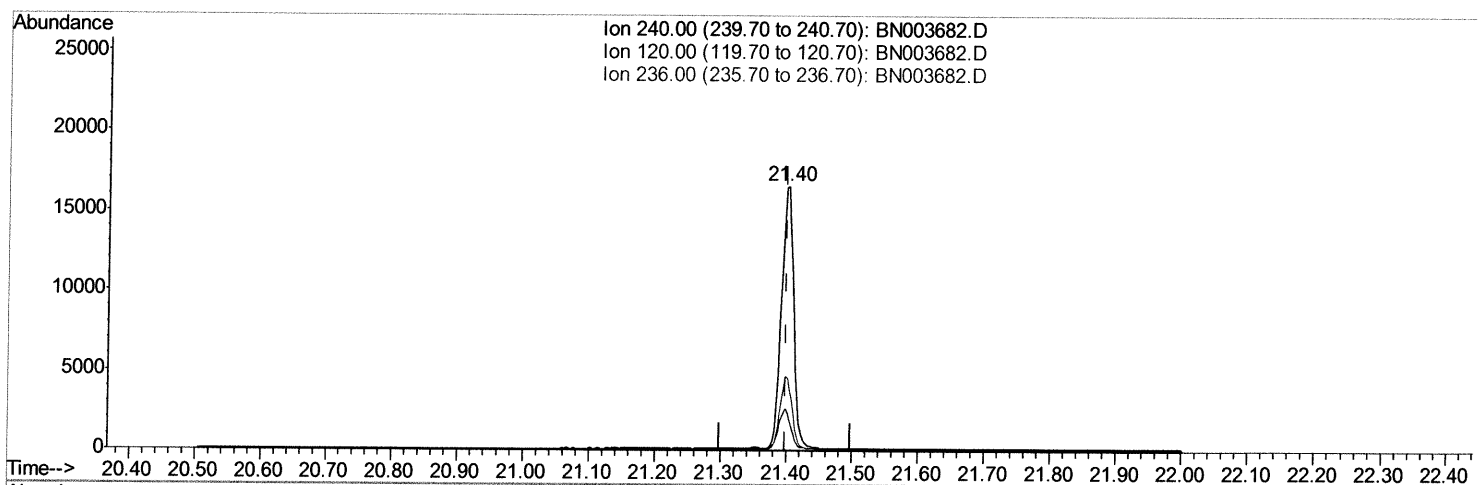

(16) Chrysene-d12 (I)

21.401min (+0.002) 0.40ng/ul m > 50 12/11/18




response 21546

Ion	Exp%	Act%
240.00	100	100
120.00	14.00	14.23
236.00	27.60	27.49
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN120318\
Quantitation Report (Qedit)

Data File : BN003682.D
Acq On : 03 Dec 2018 17:38
Operator : JU/SJ
Sample : PB115256BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Dec 04 01:29:21 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 04 01:23:55 2018
Response via : Initial Calibration

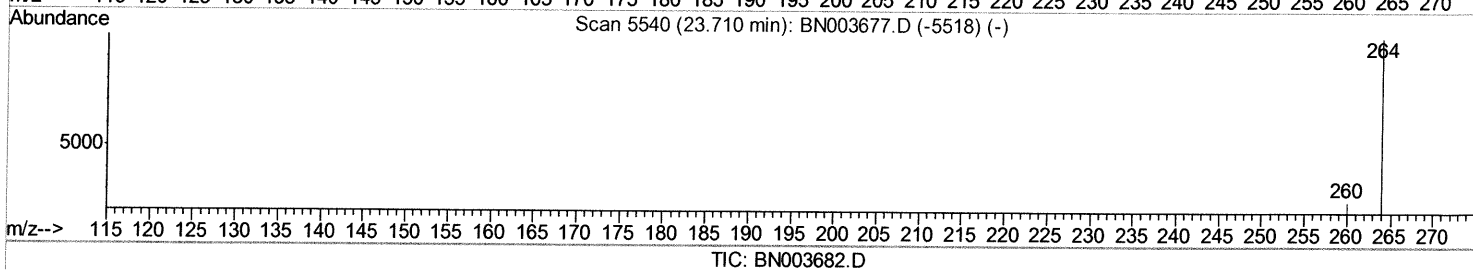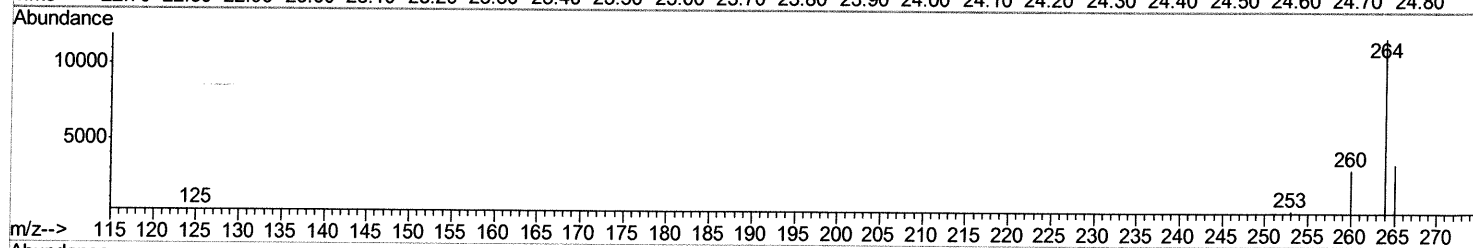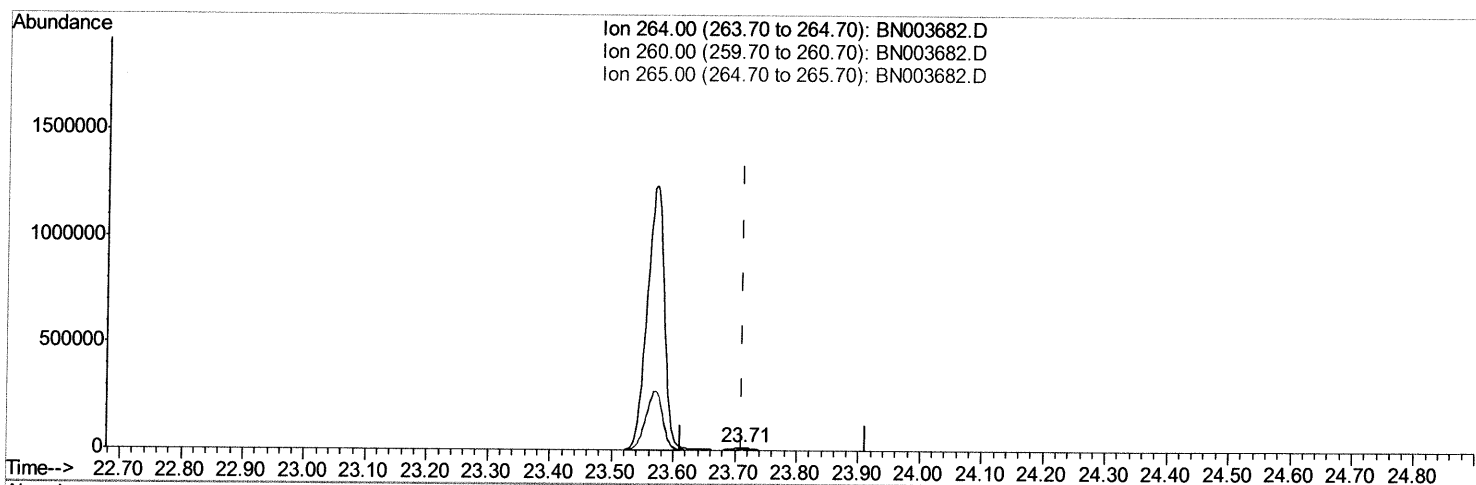

(20) Perylene-d12 (I)

23.713min (+0.002) 0.40ng/ul




response 28336

Ion	Exp%	Act%
264.00	100	100
260.00	26.20	26.02
265.00	33.50	29.74
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN120318\
Quantitation Report (Qedit)

Data File : BN003682.D
Acq On : 03 Dec 2018 17:38
Operator : JU/SJ
Sample : PB115256BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Dec 04 01:29:21 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 04 01:23:55 2018
Response via : Initial Calibration

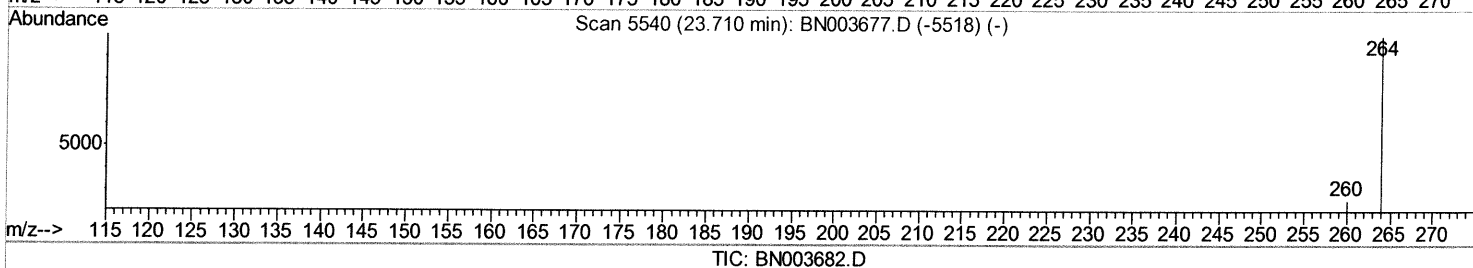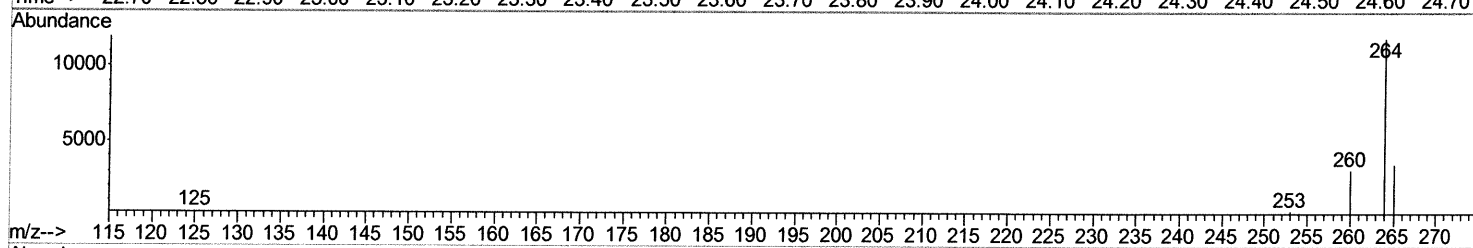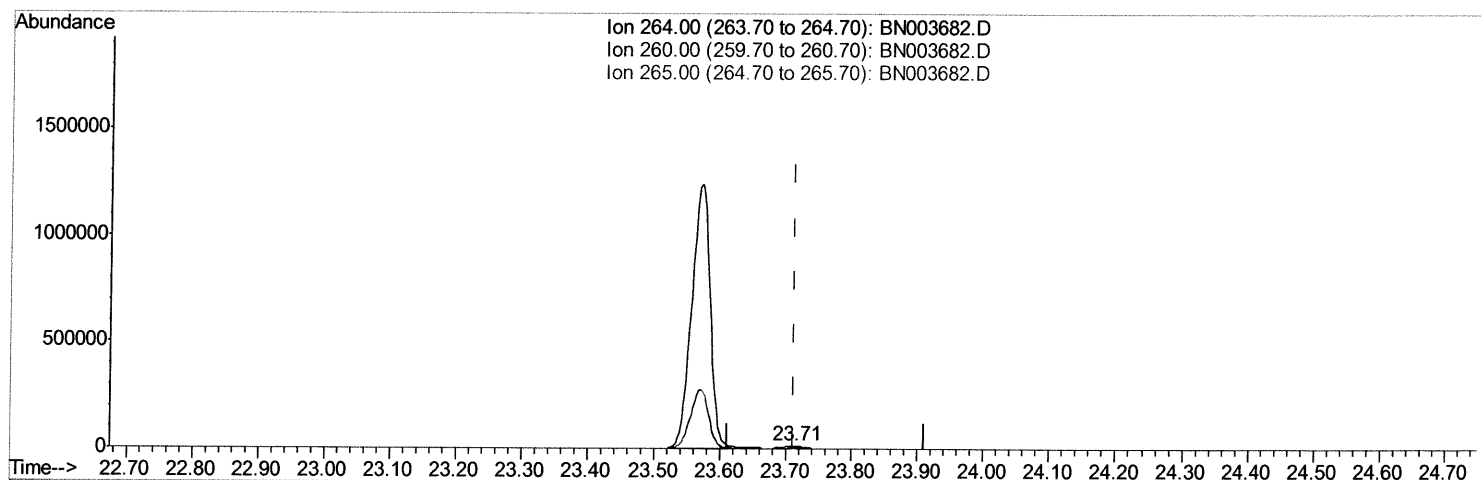

(20) Perylene-d12 (I)

23.713min (+0.002) 0.40ng/ul m) 50 12/11/18

response 19085

Ion	Exp%	Act%
264.00	100	100
260.00	26.20	26.02
265.00	33.50	29.74
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN120318\
Quantitation Report (QT Reviewed)

Data File : BN003682.D
Acq On : 03 Dec 2018 17:38
Operator : JU/SJ
Sample : PB115256BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Dec 04 01:30:08 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 04 01:23:55 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	4672	0.40	ng/ul	0.00
2) Naphthalene-d8	10.63	136	19012	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.47	164	11049	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.22	188	23315m	0.40	ng/ul	0.00
16) Chrysene-d12	21.40	240	21546m	0.40	ng/ul	0.00
20) Perylene-d12	23.71	264	19085m	0.40	ng/ul	0.00

SJ 12/11/18

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	12.22	152	11606	0.40	ng/ul	0.00
14) Fluoranthene-d10	19.24	212	27180m	0.40	ng/ul	0.00

SJ 12/11/18

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed