

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120318\
 Data File : BN003683.D
 Acq On : 03 Dec 2018 18:13
 Operator : JU/SJ
 Sample : J6077-20
 Misc :
 ALS Vial : 4 Sample Multiplier: 1


Quant Time: Dec 04 01:35:00 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 04 01:23:55 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	4921	0.40	ng/ul	0.00
2) Naphthalene-d8	10.63	136	20463	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.47	164	11874	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.22	188	25465m	0.40	ng/ul	0.00
16) Chrysene-d12	21.40	240	23578m	0.40	ng/ul	0.00
20) Perylene-d12	23.71	264	19493m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.22	152	9886	0.31	ng/ul	0.00
14) Fluoranthene-d10	19.24	212	24642m	0.33	ng/ul	0.00
Target Compounds				Ovalue		
3) Naphthalene	10.68	128	3154	0.055	ng/ul#	93
5) 2-Methylnaphthalene	12.29	142	1976	0.049	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120318\
Data File : BN003683.D
Acq On : 03 Dec 2018 18:13
Operator : JU/SJ
Sample : J6077-20
Misc :
ALS Vial : 4 Sample Multiplier: 1

Quant Time: Dec 04 01:35:00 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 04 01:23:55 2018
Response via : Initial Calibration

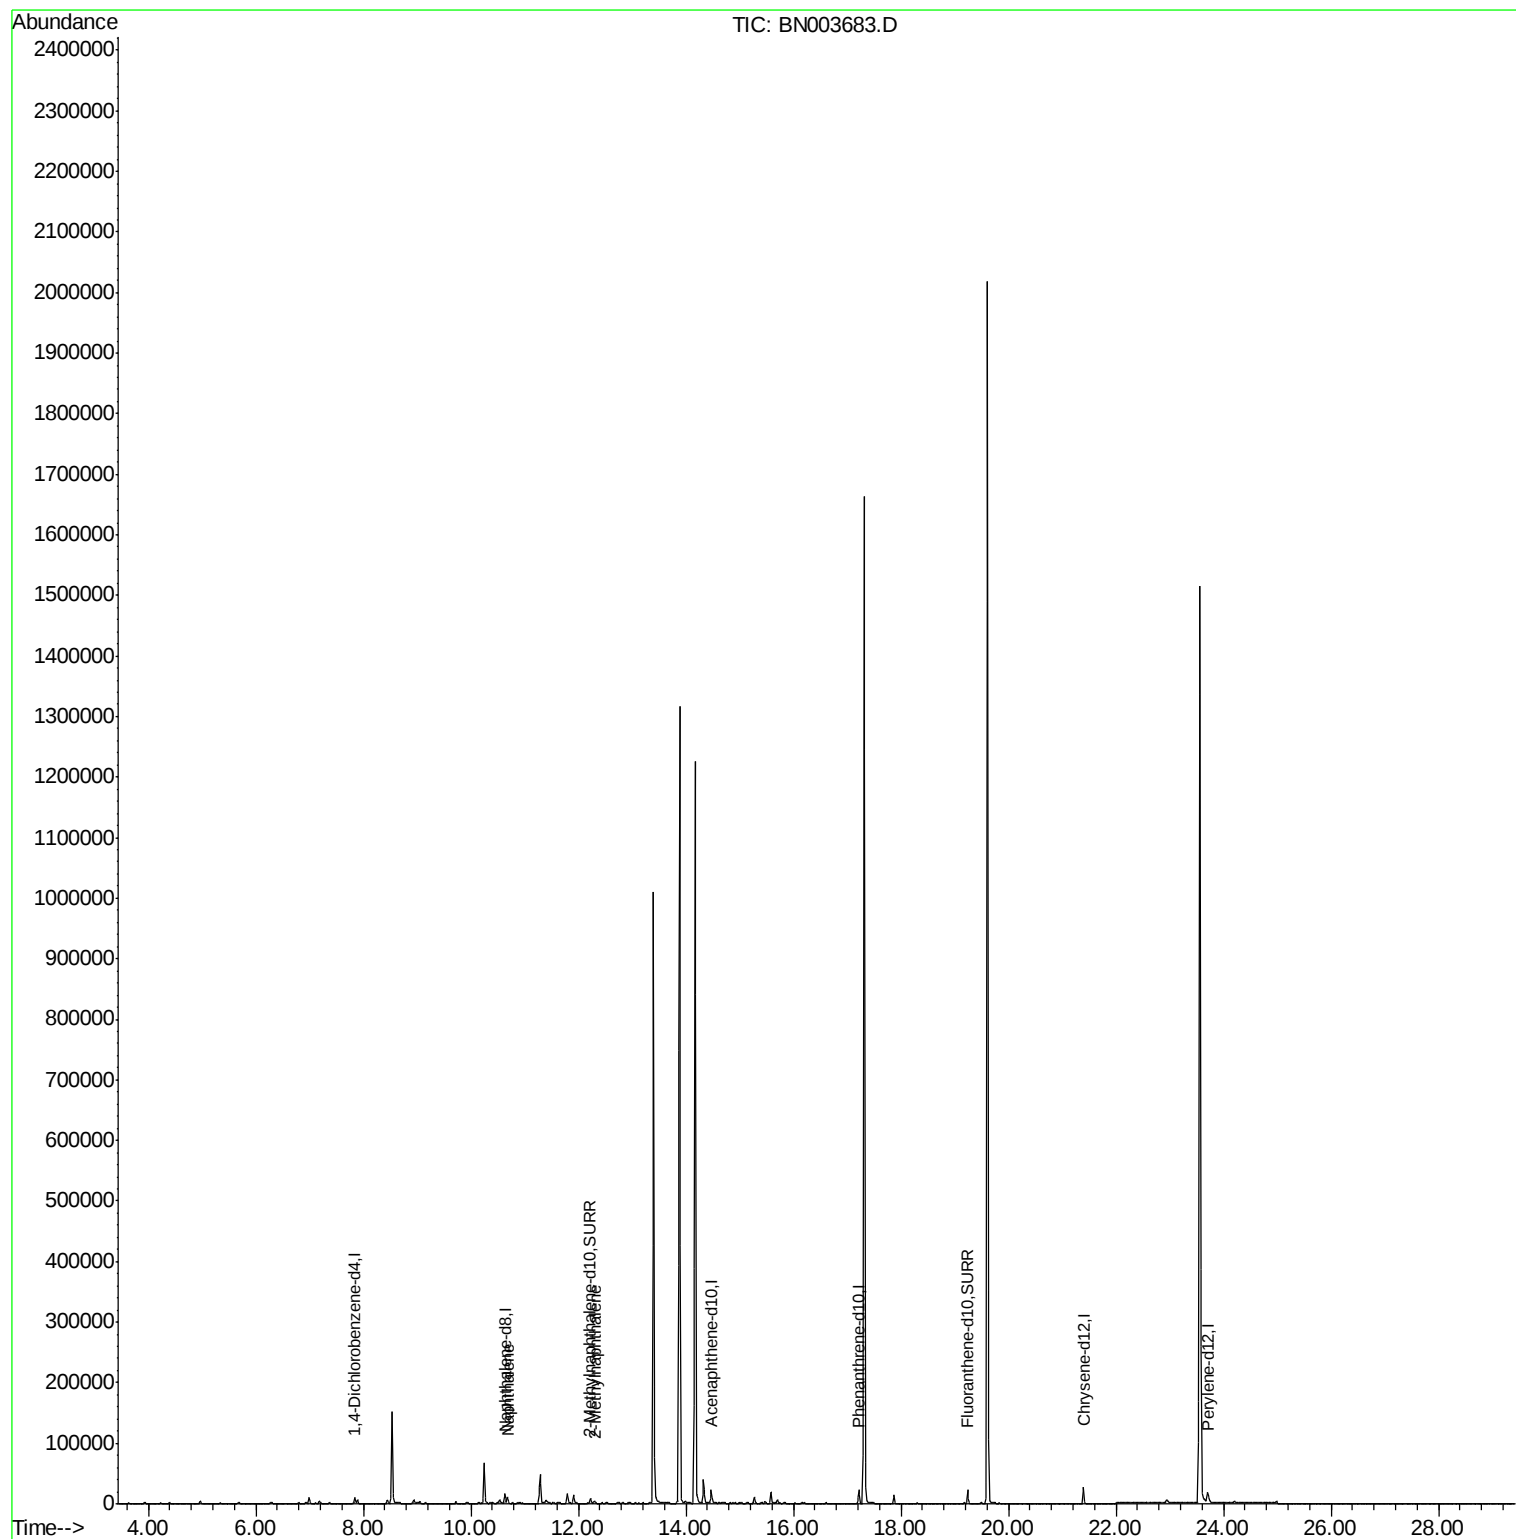

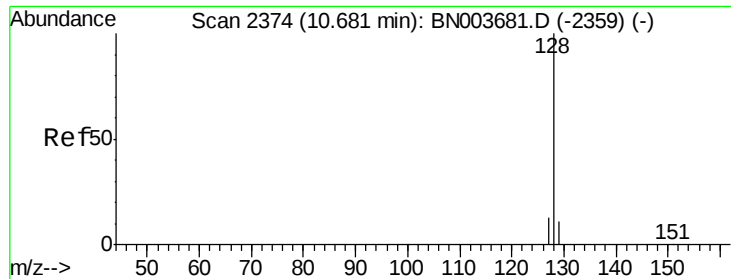

#3

Naphthalene

Concen: 0.055 ng/ul

RT: 10.68 min Scan# 2374

Delta R.T. -0.00 min

Lab File: BN003683.D

Acq: 03 Dec 2018 18:13


Tot Ion:128 Resp: 3154

Ion Ratio Lower Upper

128 100

129 14.5 9.0 13.6#




127 15.8 10.5 15.7#

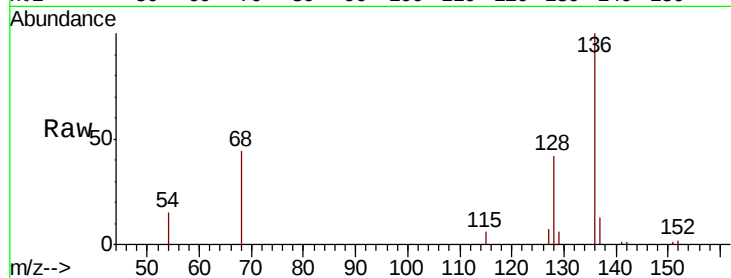

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

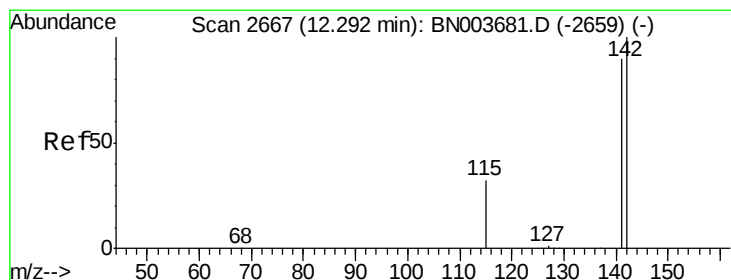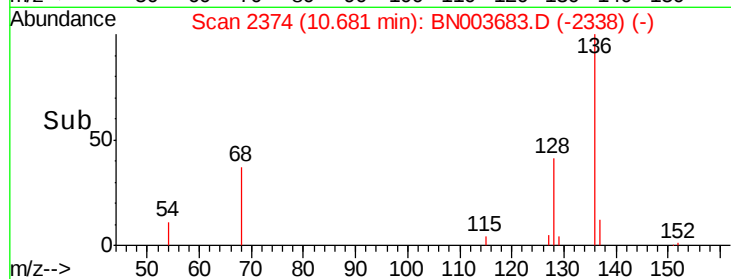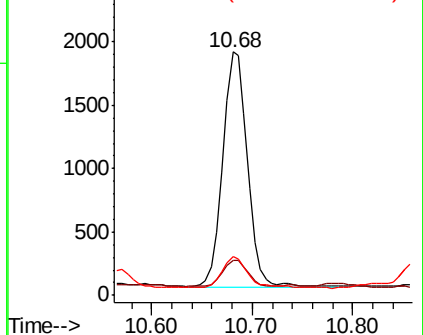

#5

2-Methylnaphthalene

Concen: 0.049 ng/ul

RT: 12.29 min Scan# 2667

Delta R.T. -0.00 min

Lab File: BN003683.D


Acq: 03 Dec 2018 18:13

Tgt Ion:142 Resp: 1976

Ion Ratio Lower Upper

142 100

141 87.8 71.5 107.3

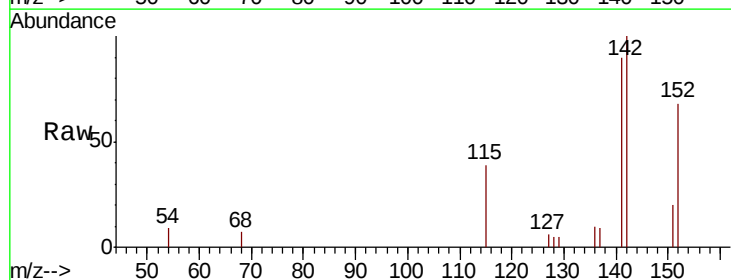

Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

