
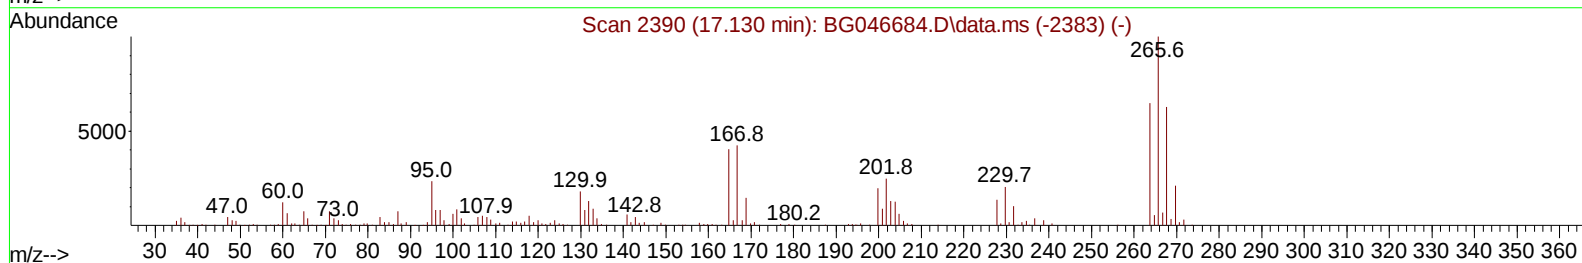
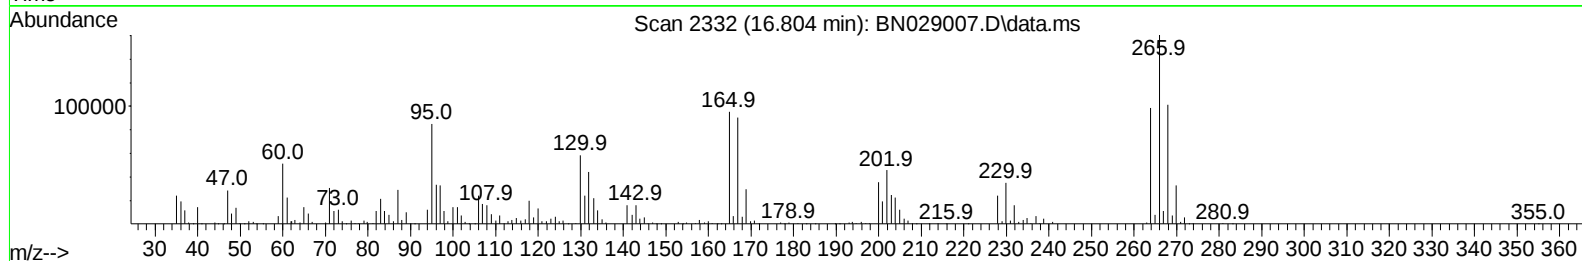


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120323\
Data File : BN029007.D
Acq On : 03 Dec 2023 06:47
Operator : MA/JU
Sample : DFTTP
Misc :
ALS Vial : 61 Sample Multiplier: 1

Quant Time: Dec 04 02:54:13 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 01 23:28:24 2023
Response via : Initial Calibration

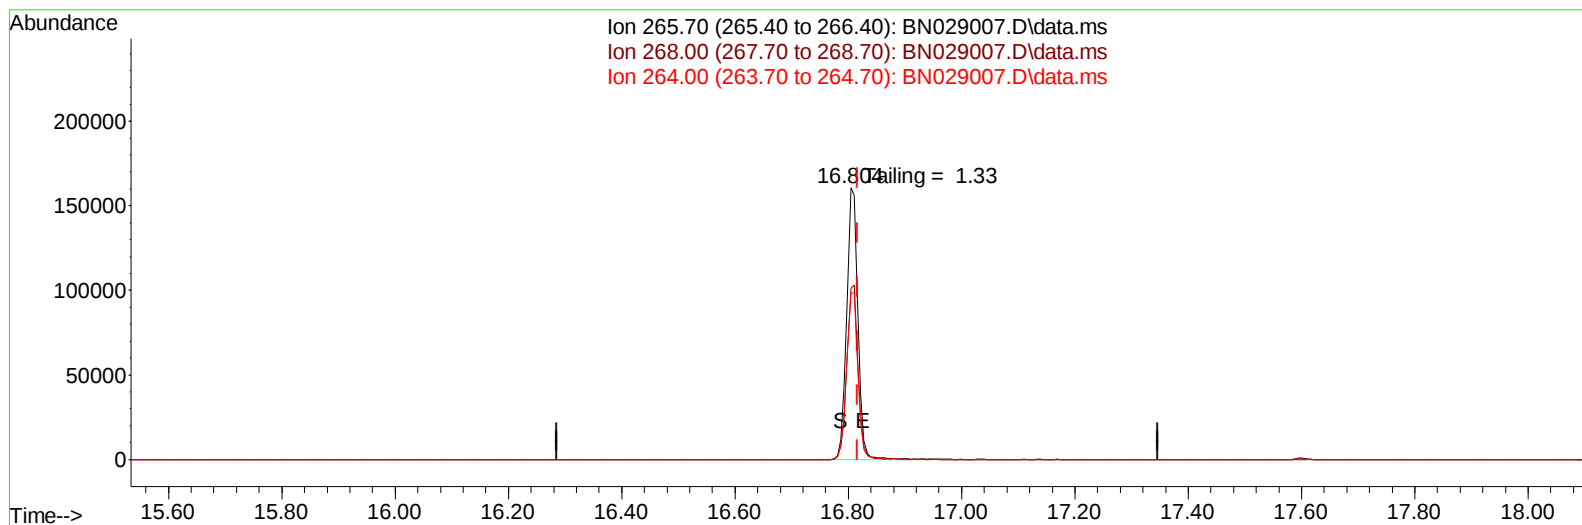

TIC: BN029007.D\data.ms

(70) Pentachlorophenol (C)




16.804min (-0.012) 12635.49 ng

response 219144

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.01
264.00	61.60	61.26
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120323\
Data File : BN029007.D
Acq On : 03 Dec 2023 06:47
Operator : MA/JU
Sample : DFTTP
Misc :
ALS Vial : 61 Sample Multiplier: 1

Quant Time: Dec 04 02:54:13 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 01 23:28:24 2023
Response via : Initial Calibration

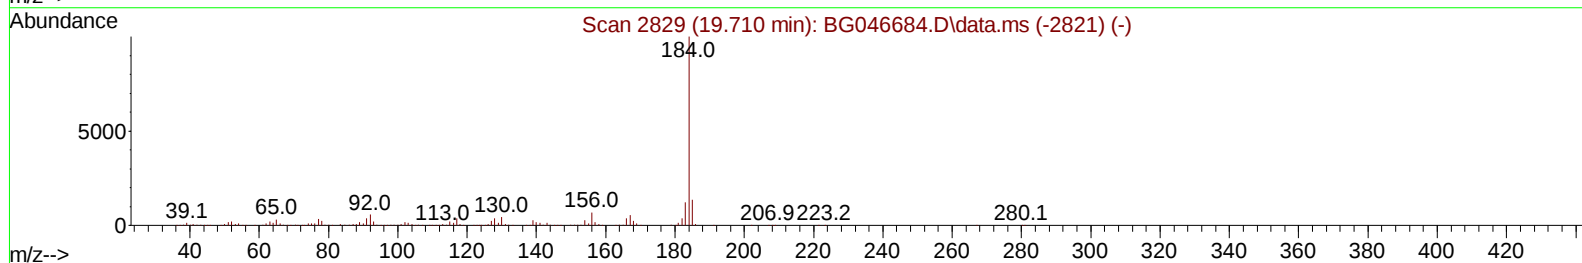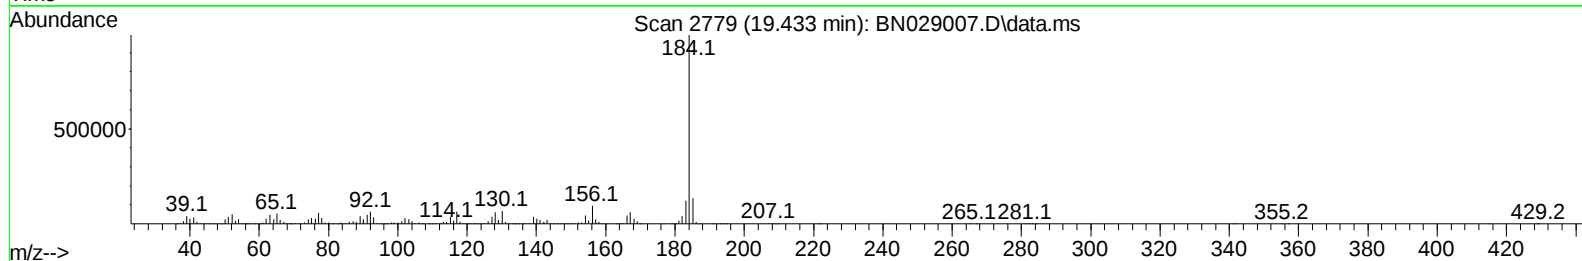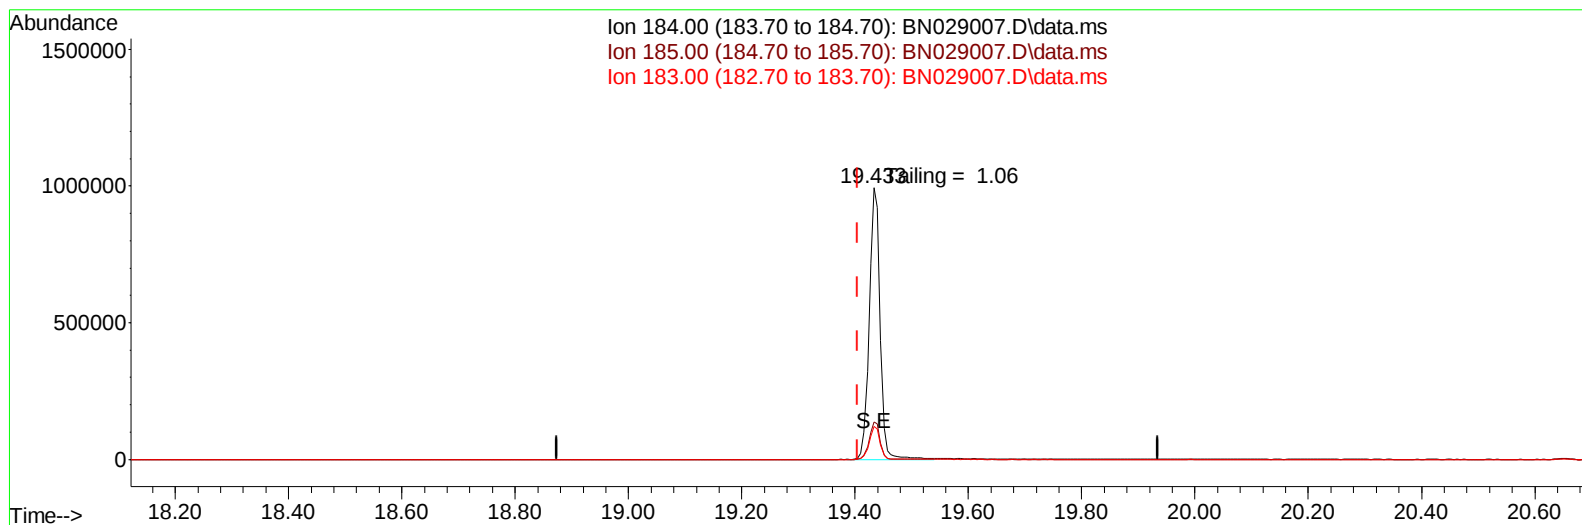

TIC: BN029007.D\data.ms

(77) Benzidine**19.433min (+ 0.029) 712210.31 ng****response 1339203**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.73
183.00	13.20	12.12
0.00	0.00	0.00