
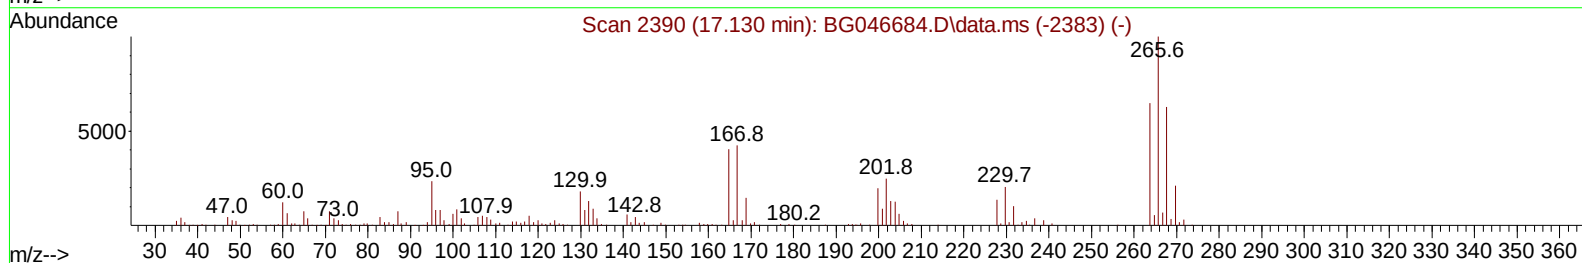
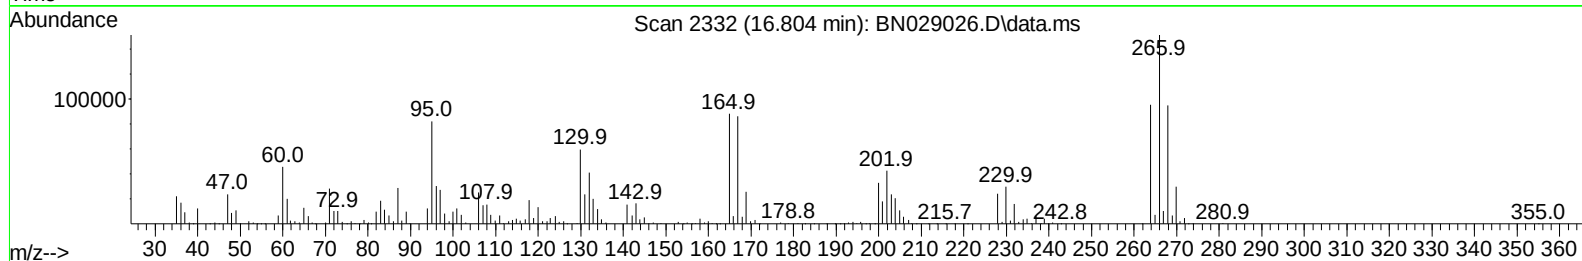


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120323\
Data File : BN029026.D
Acq On : 03 Dec 2023 19:17
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 81 Sample Multiplier: 1

Quant Time: Dec 04 03:26:09 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 01 23:28:24 2023
Response via : Initial Calibration

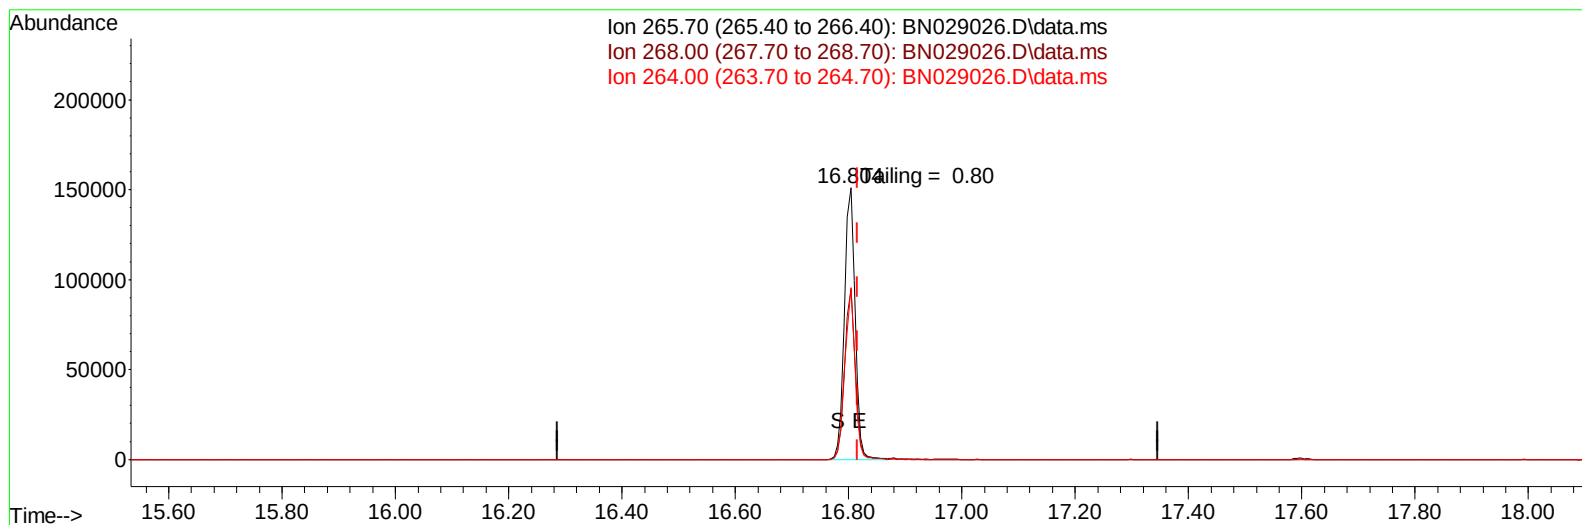

TIC: BN029026.D\data.ms

(70) Pentachlorophenol (C)




16.804min (-0.012) 14036.73 ng

response 197511

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.81
264.00	61.60	63.23
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120323\
Data File : BN029026.D
Acq On : 03 Dec 2023 19:17
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 81 Sample Multiplier: 1

Quant Time: Dec 04 03:26:09 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 01 23:28:24 2023
Response via : Initial Calibration

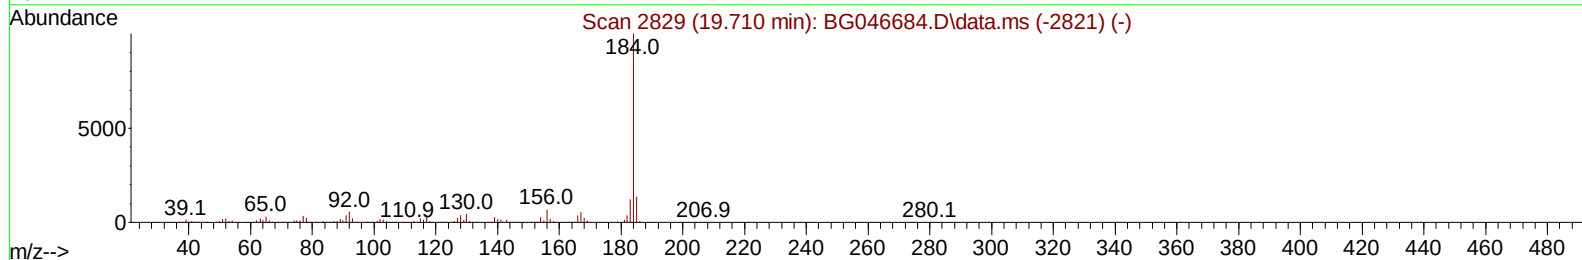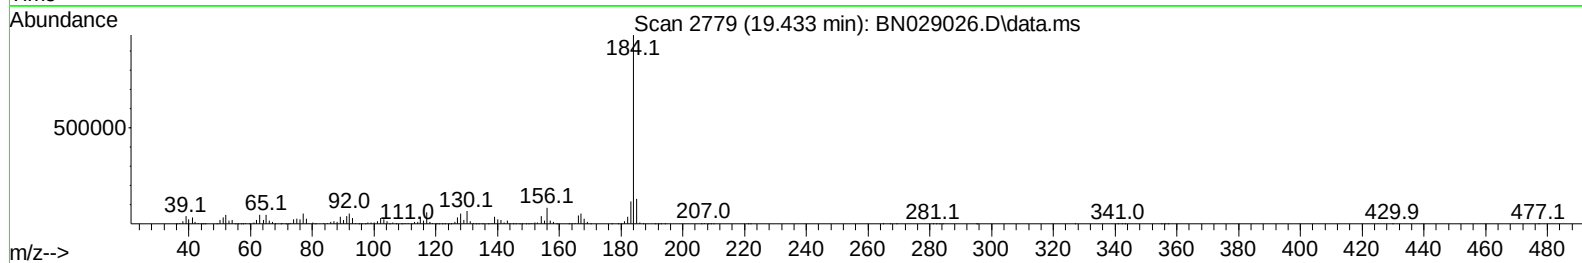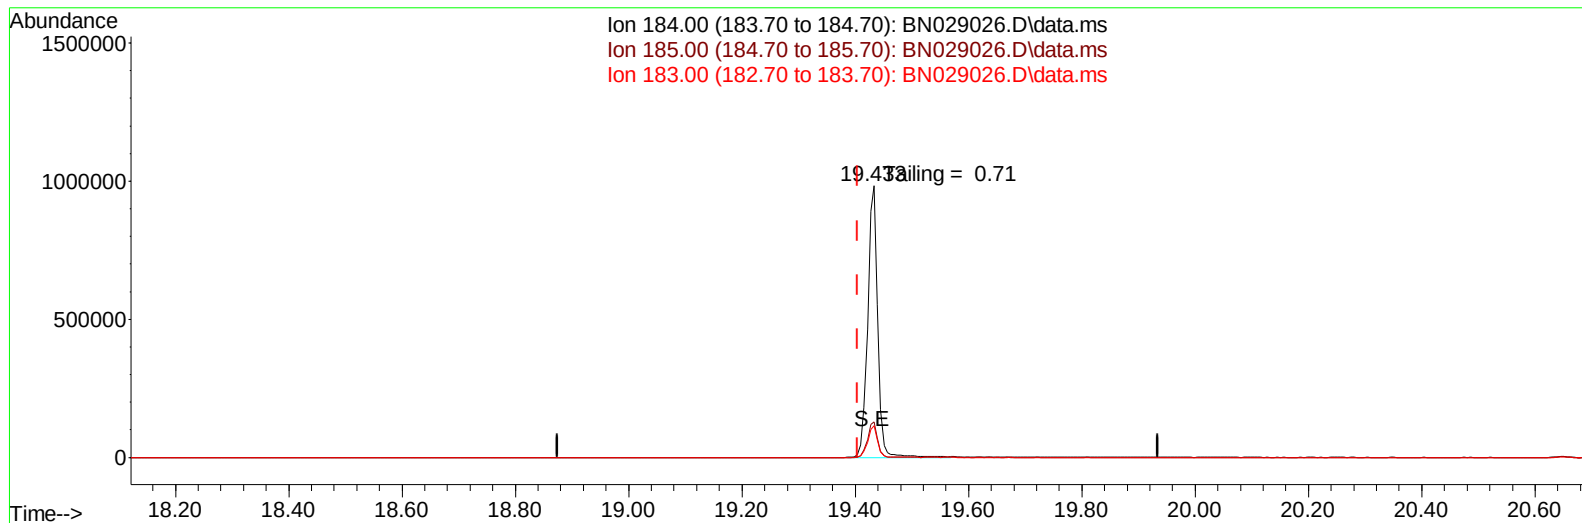

TIC: BN029026.D\data.ms

(77) Benzidine**19.433min (+ 0.029) 662282.36 ng****response 1224906**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.17
183.00	13.20	11.73
0.00	0.00	0.00