

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120323\
 Data File : BN029026.D
 Acq On : 03 Dec 2023 19:17
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 81 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Dec 04 03:28:31 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN113023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 04 00:28:48 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	0.000	152	0	0.000	ng	-7.78
7) Naphthalene-d8	0.000	136	0	0.000	ng	-10.56
13) Acenaphthene-d10	0.000	164	0	0.000	ng	-14.41
19) Phenanthrene-d10	0.000	188	0	0.000	ng	-17.16
29) Chrysene-d12	0.000	240	0	0.000	ng	-21.35
35) Perylene-d12	0.000	264	0	0.000	ng	-23.67
System Monitoring Compounds						
4) 2-Fluorophenol	0.000	112	0	0.000	ng	
5) Phenol-d6	0.000	99	0	0.000	ng	
8) Nitrobenzene-d5	0.000	82	0	0.000	ng	
11) 2-Methylnaphthalene-d10	0.000	152	0	0.000	ng	
14) 2,4,6-Tribromophenol	0.000	330	0	0.000	ng	
15) 2-Fluorobiphenyl	0.000	172	0	0.000	ng	
27) Fluoranthene-d10	0.000	212	0	0.000	ng	
31) Terphenyl-d14	0.000	244	0	0.000	ng	


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120323\
Data File : BN029026.D
Acq On : 03 Dec 2023 19:17
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 81 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 04 03:28:31 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN113023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 04 00:28:48 2023
Response via : Initial Calibration

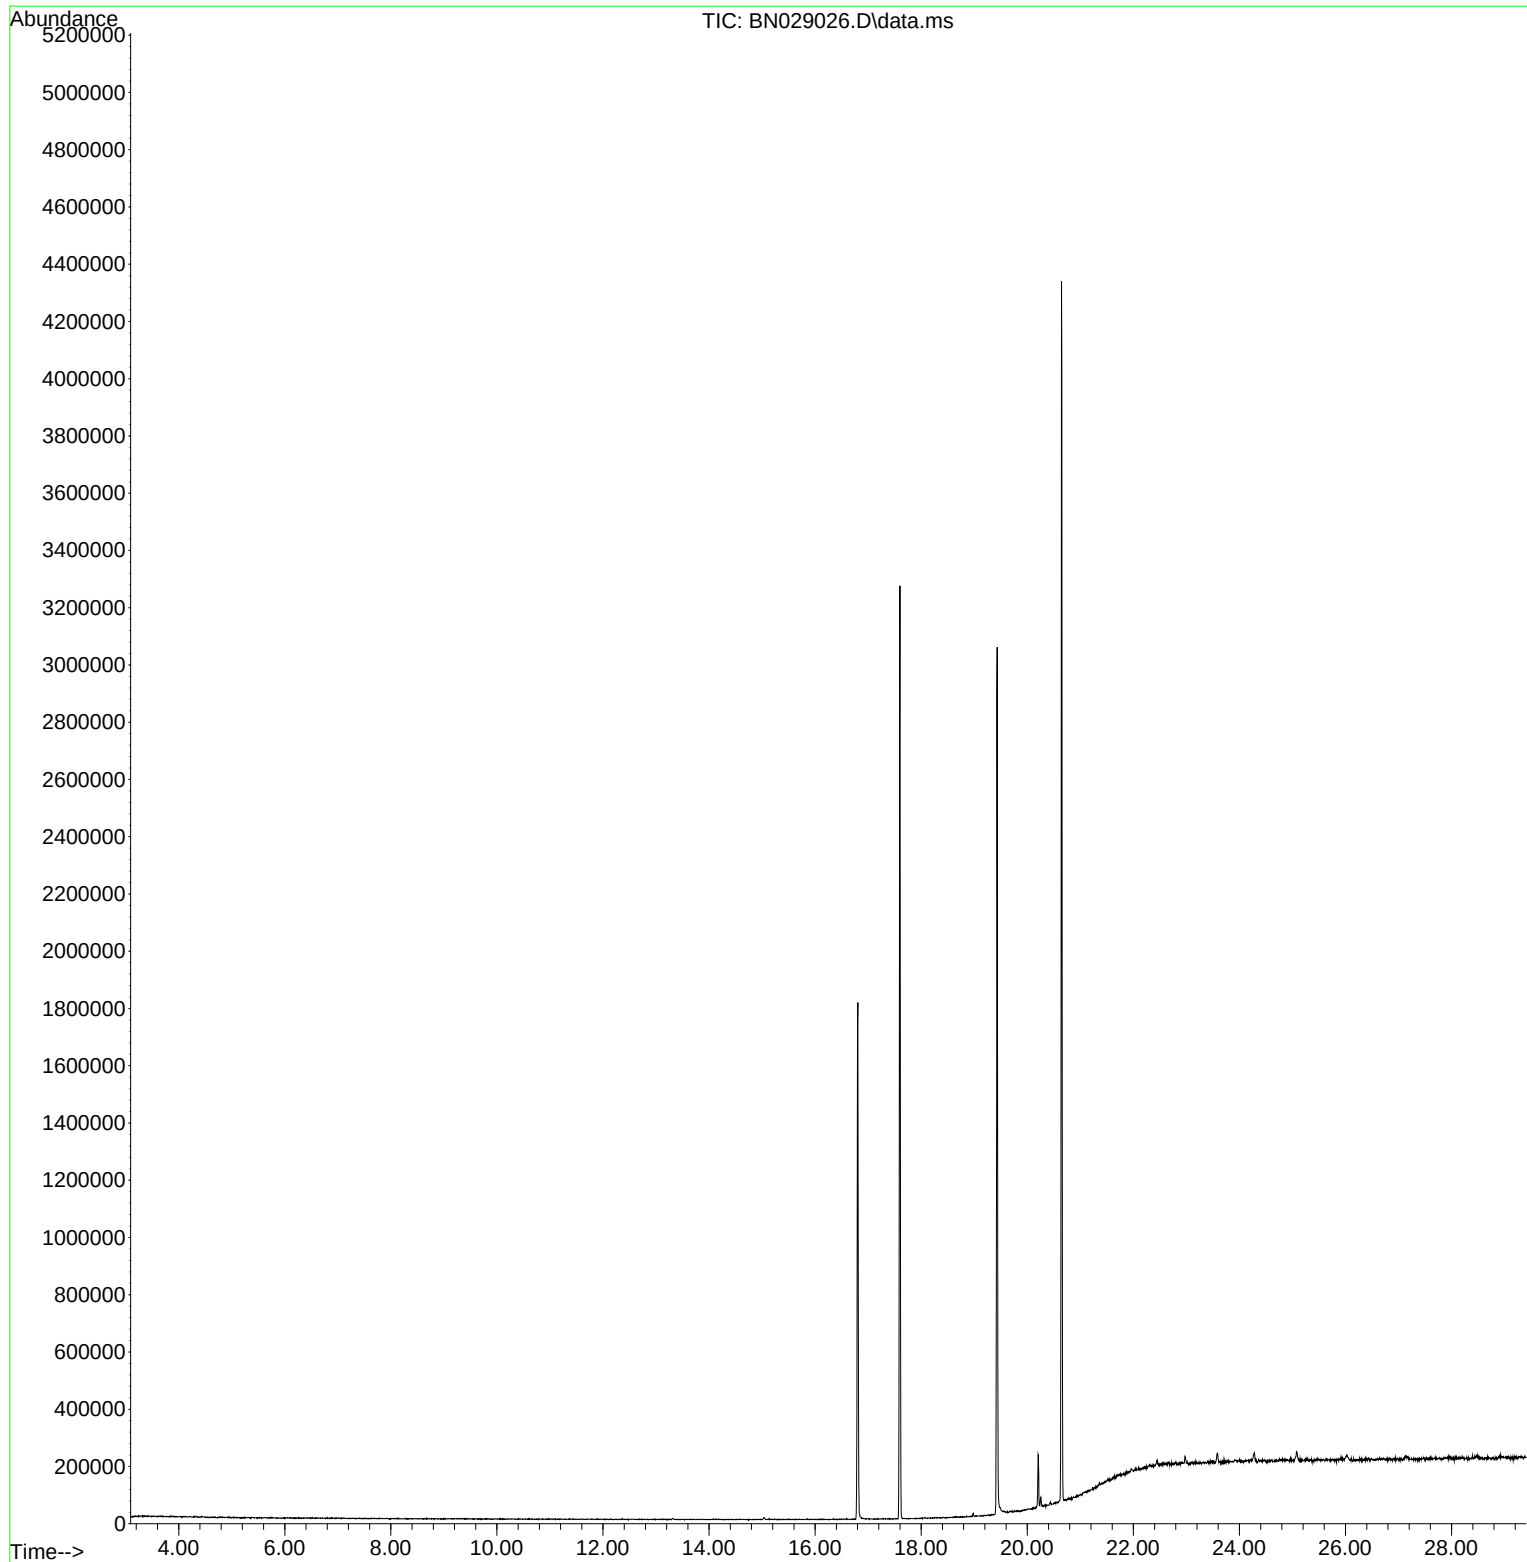


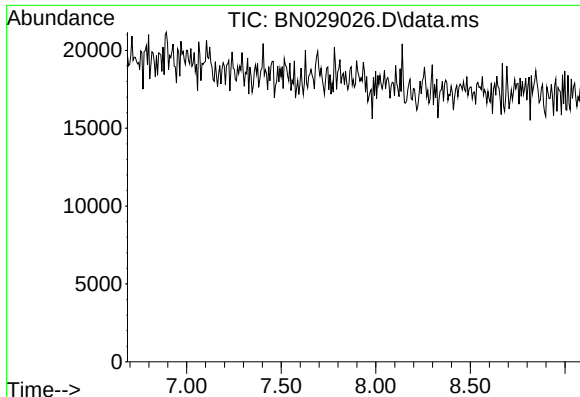


#1
 1,4-Dichlorobenzene-d4
 Concen: 0.000 ng
 Expected RT: 7.78 min
 Lab File: BN029026.D
 Acq: 03 Dec 2023 19:17

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Tgt Ion: 152


Sig	Exp Ratio
152	100
150	154.3
115	73.9

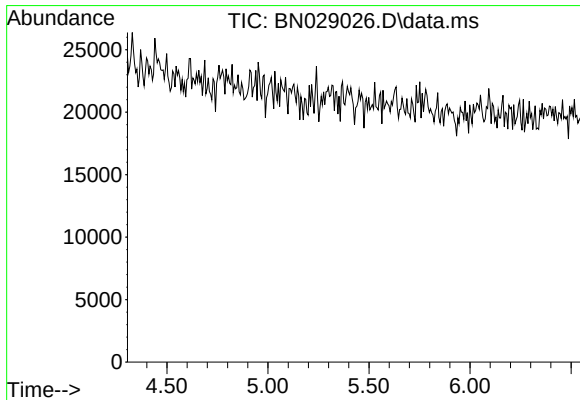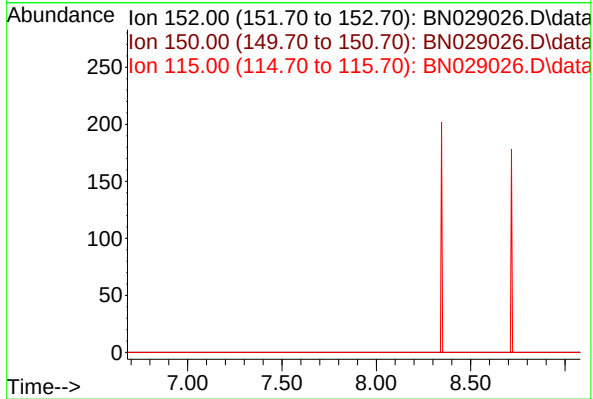


#4
 2-Fluorophenol
 Concen: 0.000 ng
 Expected RT: 5.40 min
 Lab File: BN029026.D
 Acq: 03 Dec 2023 19:17

Tgt Ion: 112

Sig	Exp Ratio
112	100
64	64.4
63	38.0

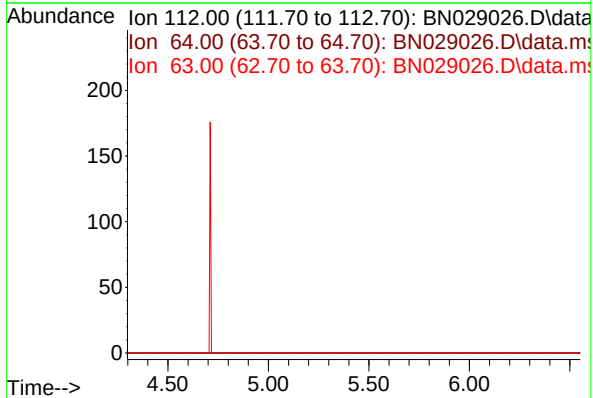


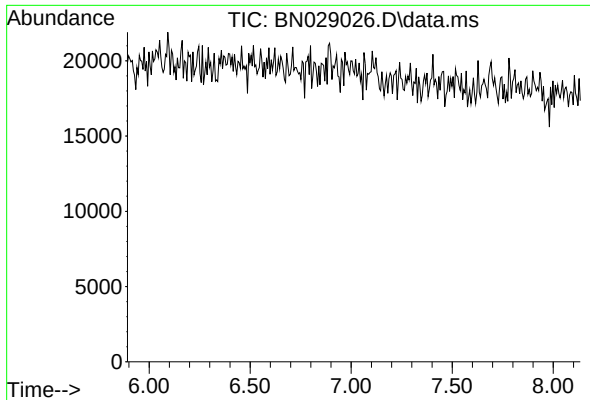


#5
 Phenol-d6
 Concen: 0.000 ng
 Expected RT: 6.99 min
 Lab File: BN029026.D
 Acq: 03 Dec 2023 19:17

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Tgt Ion: 99


Sig	Exp Ratio
99	100
42	26.5
71	44.2

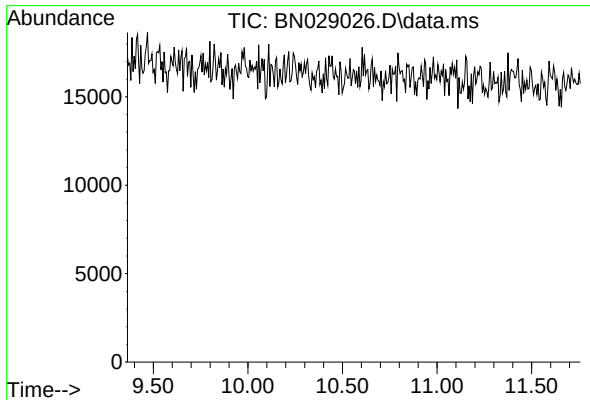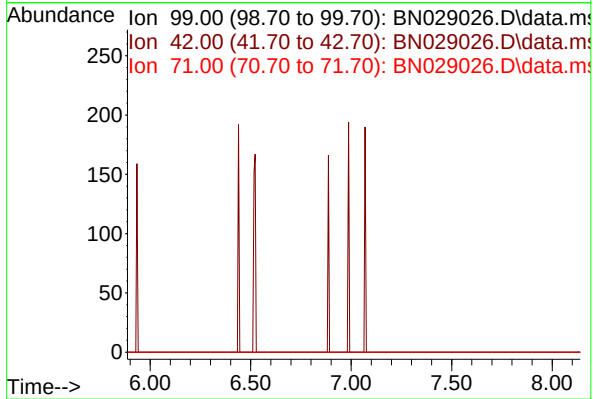


#7
 Naphthalene-d8
 Concen: 0.000 ng
 Expected RT: 10.56 min
 Lab File: BN029026.D
 Acq: 03 Dec 2023 19:17

Tgt Ion: 136

Sig	Exp Ratio
136	100
137	13.3
54	9.4
68	7.4

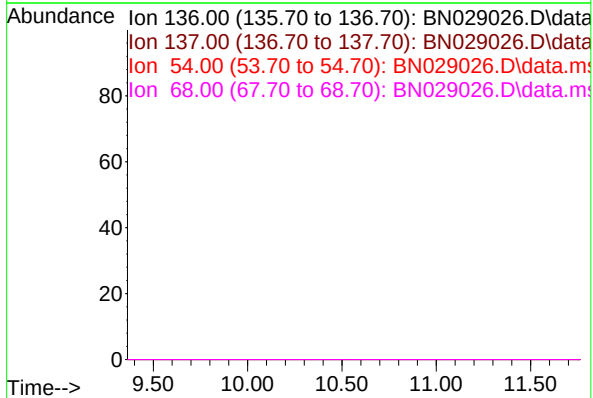


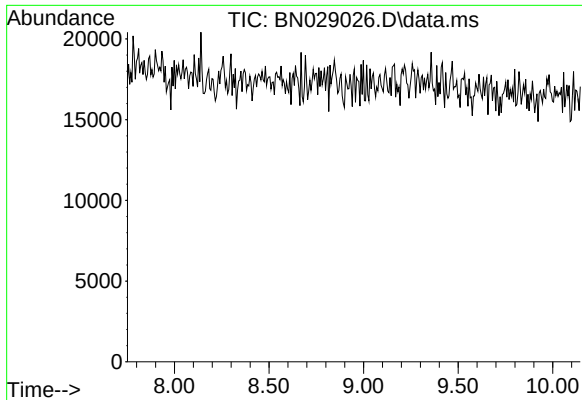


#8
Nitrobenzene-d5
Concen: 0.000 ng
Expected RT: 8.95 min

Lab File: BN029026.D
Acq: 03 Dec 2023 19:17

Instrument :
BNA_N
ClientSampleId :
DFTPP


Tgt Ion: 82
Sig Exp Ratio
82 100
128 36.5
54 58.8

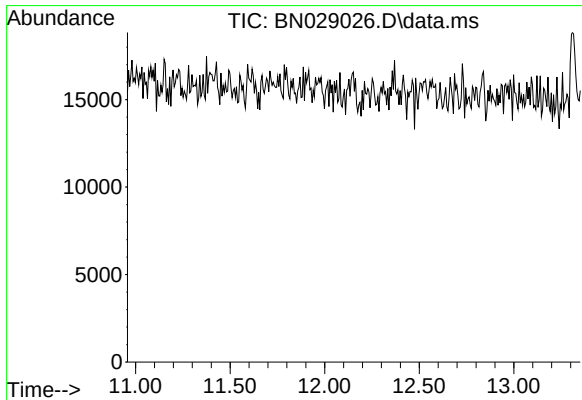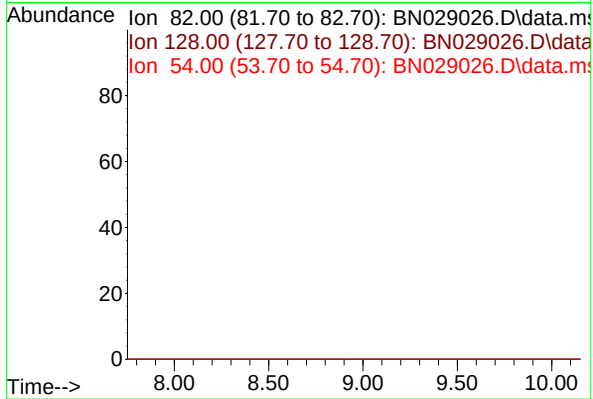


#11
2-Methylnaphthalene-d10
Concen: 0.000 ng
Expected RT: 12.15 min

Lab File: BN029026.D
Acq: 03 Dec 2023 19:17

Tgt Ion: 152
Sig Exp Ratio
152 100
151 20.9

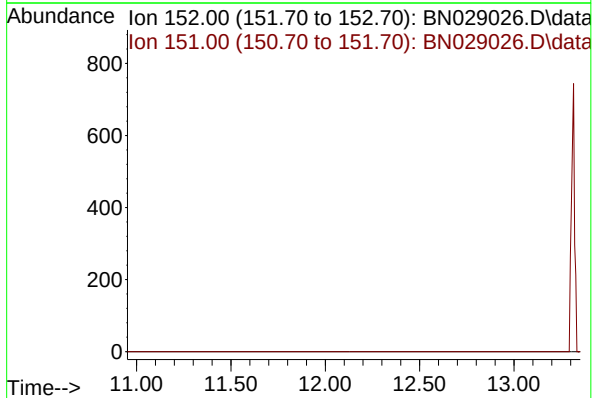


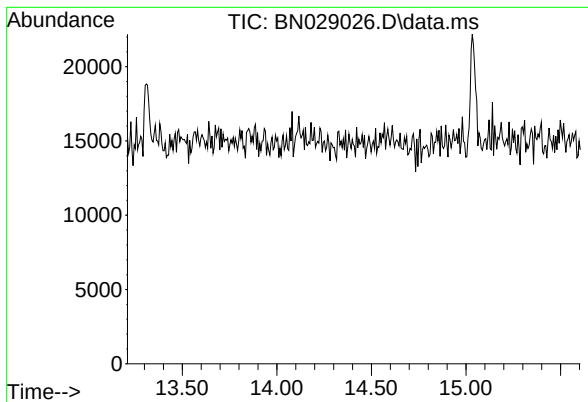


#13
 Acenaphthene-d10
 Concen: 0.000 ng
 Expected RT: 14.41 min
 Lab File: BN029026.D
 Acq: 03 Dec 2023 19:17

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Tgt Ion: 164


Sig	Exp Ratio
164	100
162	102.1
160	46.3

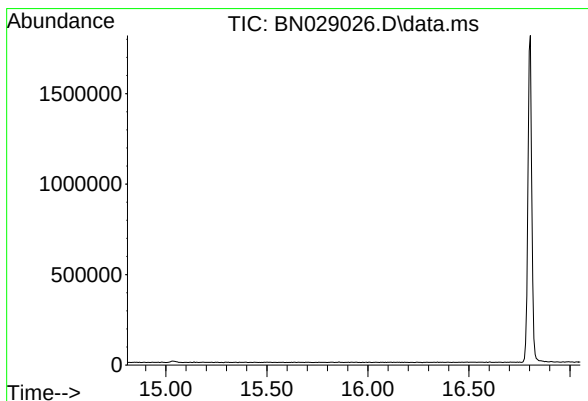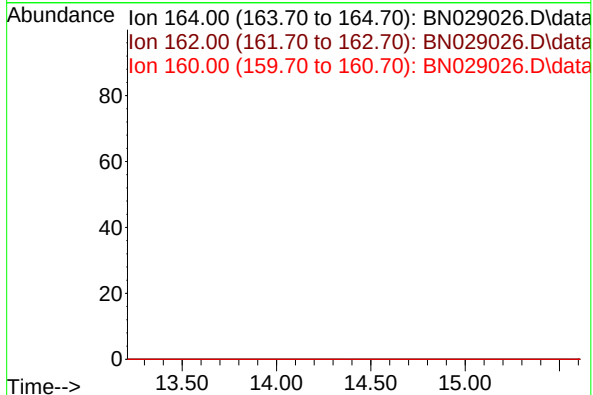


#14
 2,4,6-Tribromophenol
 Concen: 0.000 ng
 Expected RT: 15.91 min
 Lab File: BN029026.D
 Acq: 03 Dec 2023 19:17

Tgt Ion: 330

Sig	Exp Ratio
330	100
332	94.3
141	44.6

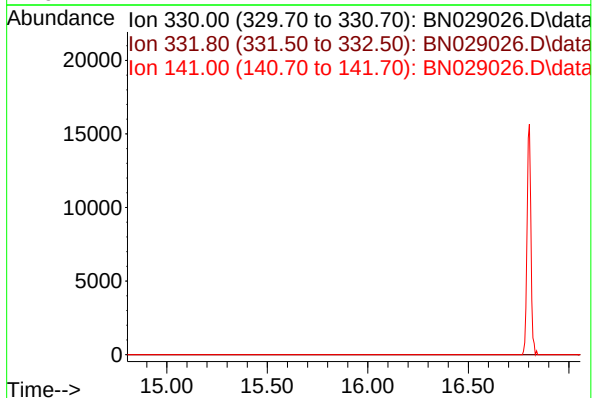


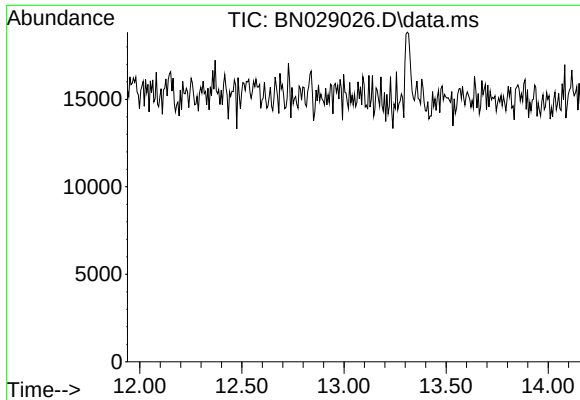


#15
 2-Fluorobiphenyl
 Concen: 0.000 ng
 Expected RT: 13.04 min
 Lab File: BN029026.D
 Acq: 03 Dec 2023 19:17

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Tgt Ion: 172


Sig	Exp Ratio
172	100
171	36.2
170	24.6

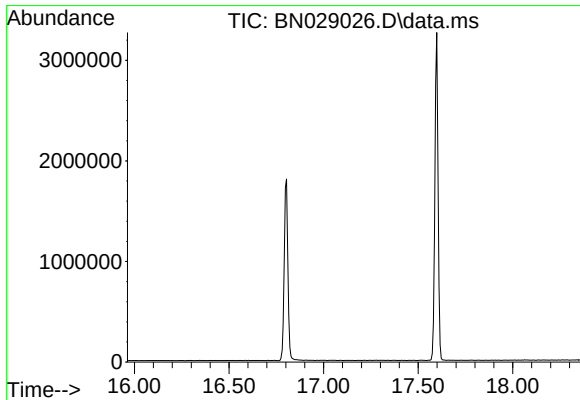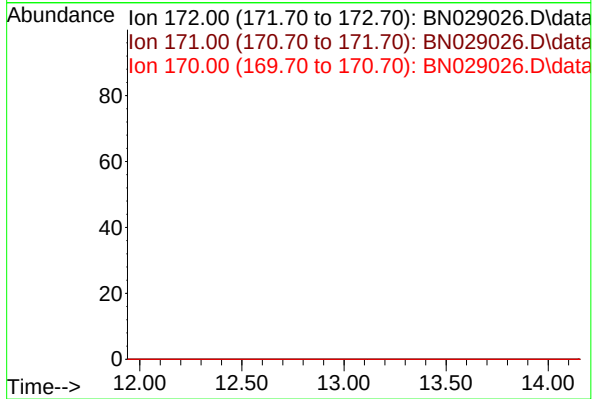


#19
 Phenanthrene-d10
 Concen: 0.000 ng
 Expected RT: 17.16 min
 Lab File: BN029026.D
 Acq: 03 Dec 2023 19:17

Tgt Ion: 188

Sig	Exp Ratio
188	100
94	0.0
80	11.3


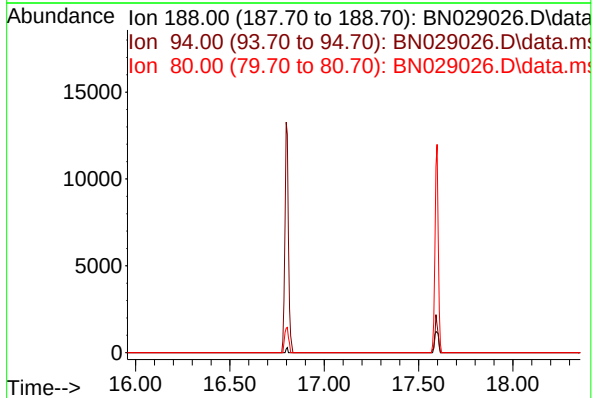


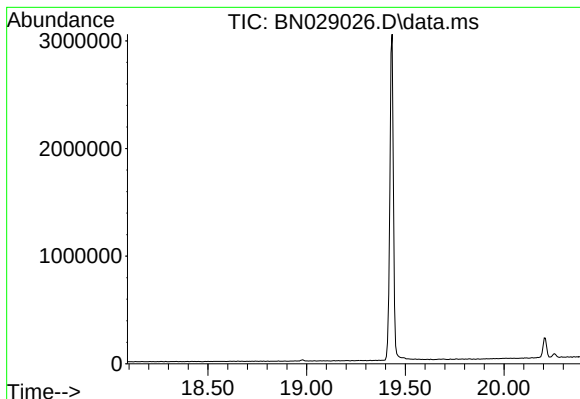

#27
 Fluoranthene-d10
 Concen: 0.000 ng
 Expected RT: 19.19 min
 Lab File: BN029026.D
 Acq: 03 Dec 2023 19:17

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP


Tgt Ion: 212
 Sig Exp Ratio
 212 100
 106 11.8
 104 7.7

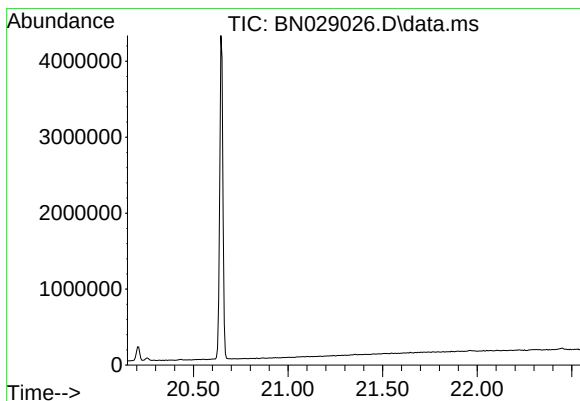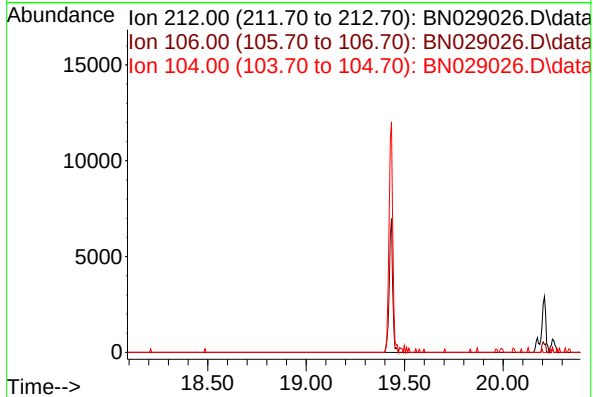


#29
 Chrysene-d12
 Concen: 0.000 ng
 Expected RT: 21.35 min

Lab File: BN029026.D
 Acq: 03 Dec 2023 19:17

Tgt Ion: 240
 Sig Exp Ratio
 240 100
 120 46.4
 236 40.5

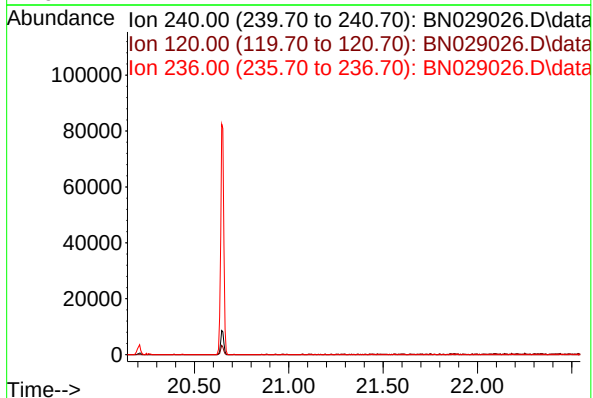


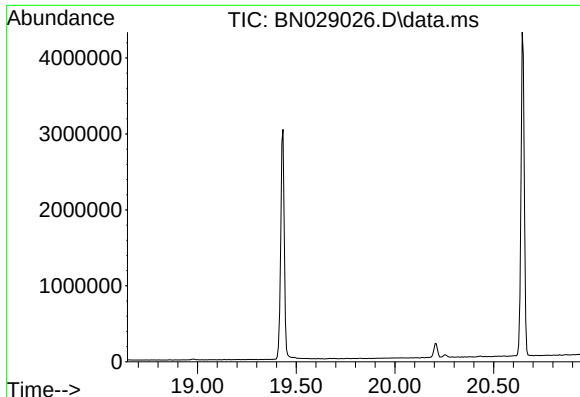


#31
 Terphenyl-d14
 Concen: 0.000 ng
 Expected RT: 19.79 min
 Lab File: BN029026.D
 Acq: 03 Dec 2023 19:17

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Tgt Ion: 244

Sig	Exp Ratio
244	100
212	14.4
122	16.5

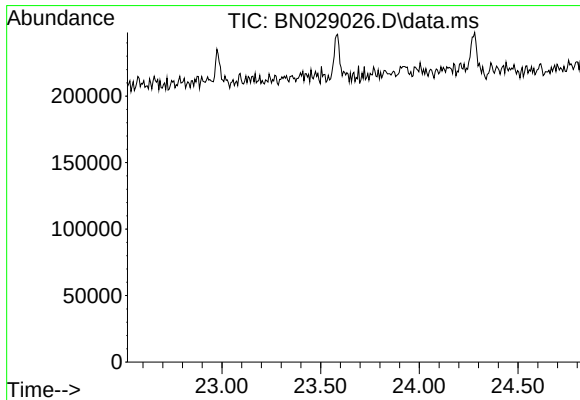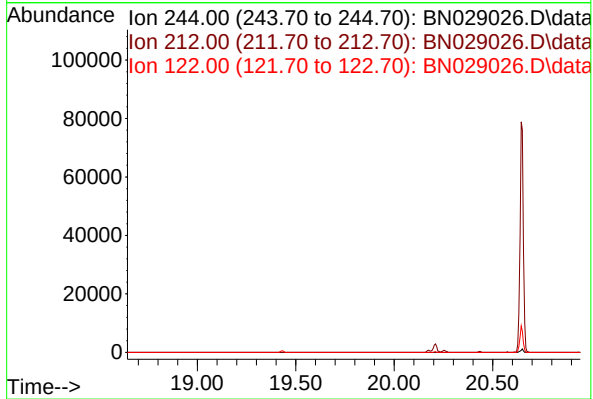

#35
 Perylene-d12
 Concen: 0.000 ng
 Expected RT: 23.67 min
 Lab File: BN029026.D
 Acq: 03 Dec 2023 19:17

Tgt Ion: 264

Sig	Exp Ratio
264	100
260	25.7
265	580.6

