

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120323\
 Data File : BN029037.D
 Acq On : 04 Dec 2023 03:02
 Operator : MA/JU
 Sample : 05428-03
 Misc :
 ALS Vial : 92 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 RE120D3-20231113

Quant Time: Dec 04 03:35:28 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN113023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 04 00:28:48 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.768	152	1551	0.400	ng	-0.01
7) Naphthalene-d8	10.551	136	4144	0.400	ng	#-0.01
13) Acenaphthene-d10	14.396	164	2535	0.400	ng	-0.01
19) Phenanthrene-d10	17.146	188	5537	0.400	ng	-0.01
29) Chrysene-d12	21.347	240	4107	0.400	ng	# 0.00
35) Perylene-d12	23.667	264	4032	0.400	ng	# 0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.384	112	484	0.103	ng	-0.01
5) Phenol-d6	6.980	99	283	0.054	ng	0.00
8) Nitrobenzene-d5	8.939	82	1220	0.296	ng	-0.01
11) 2-Methylnaphthalene-d10	12.144	152	1872	0.281	ng	0.00
14) 2,4,6-Tribromophenol	15.893	330	451	0.263	ng	-0.01
15) 2-Fluorobiphenyl	13.028	172	3426	0.313	ng	-0.01
27) Fluoranthene-d10	19.181	212	5146	0.353	ng	0.00
31) Terphenyl-d14	19.789	244	4734	0.403	ng	0.00


Target Compounds Qvalue

 (#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120323\
Data File : BN029037.D
Acq On : 04 Dec 2023 03:02
Operator : MA/JU
Sample : 05428-03
Misc :
ALS Vial : 92 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
RE120D3-20231113


Quant Time: Dec 04 03:35:28 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN113023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 04 00:28:48 2023
Response via : Initial Calibration

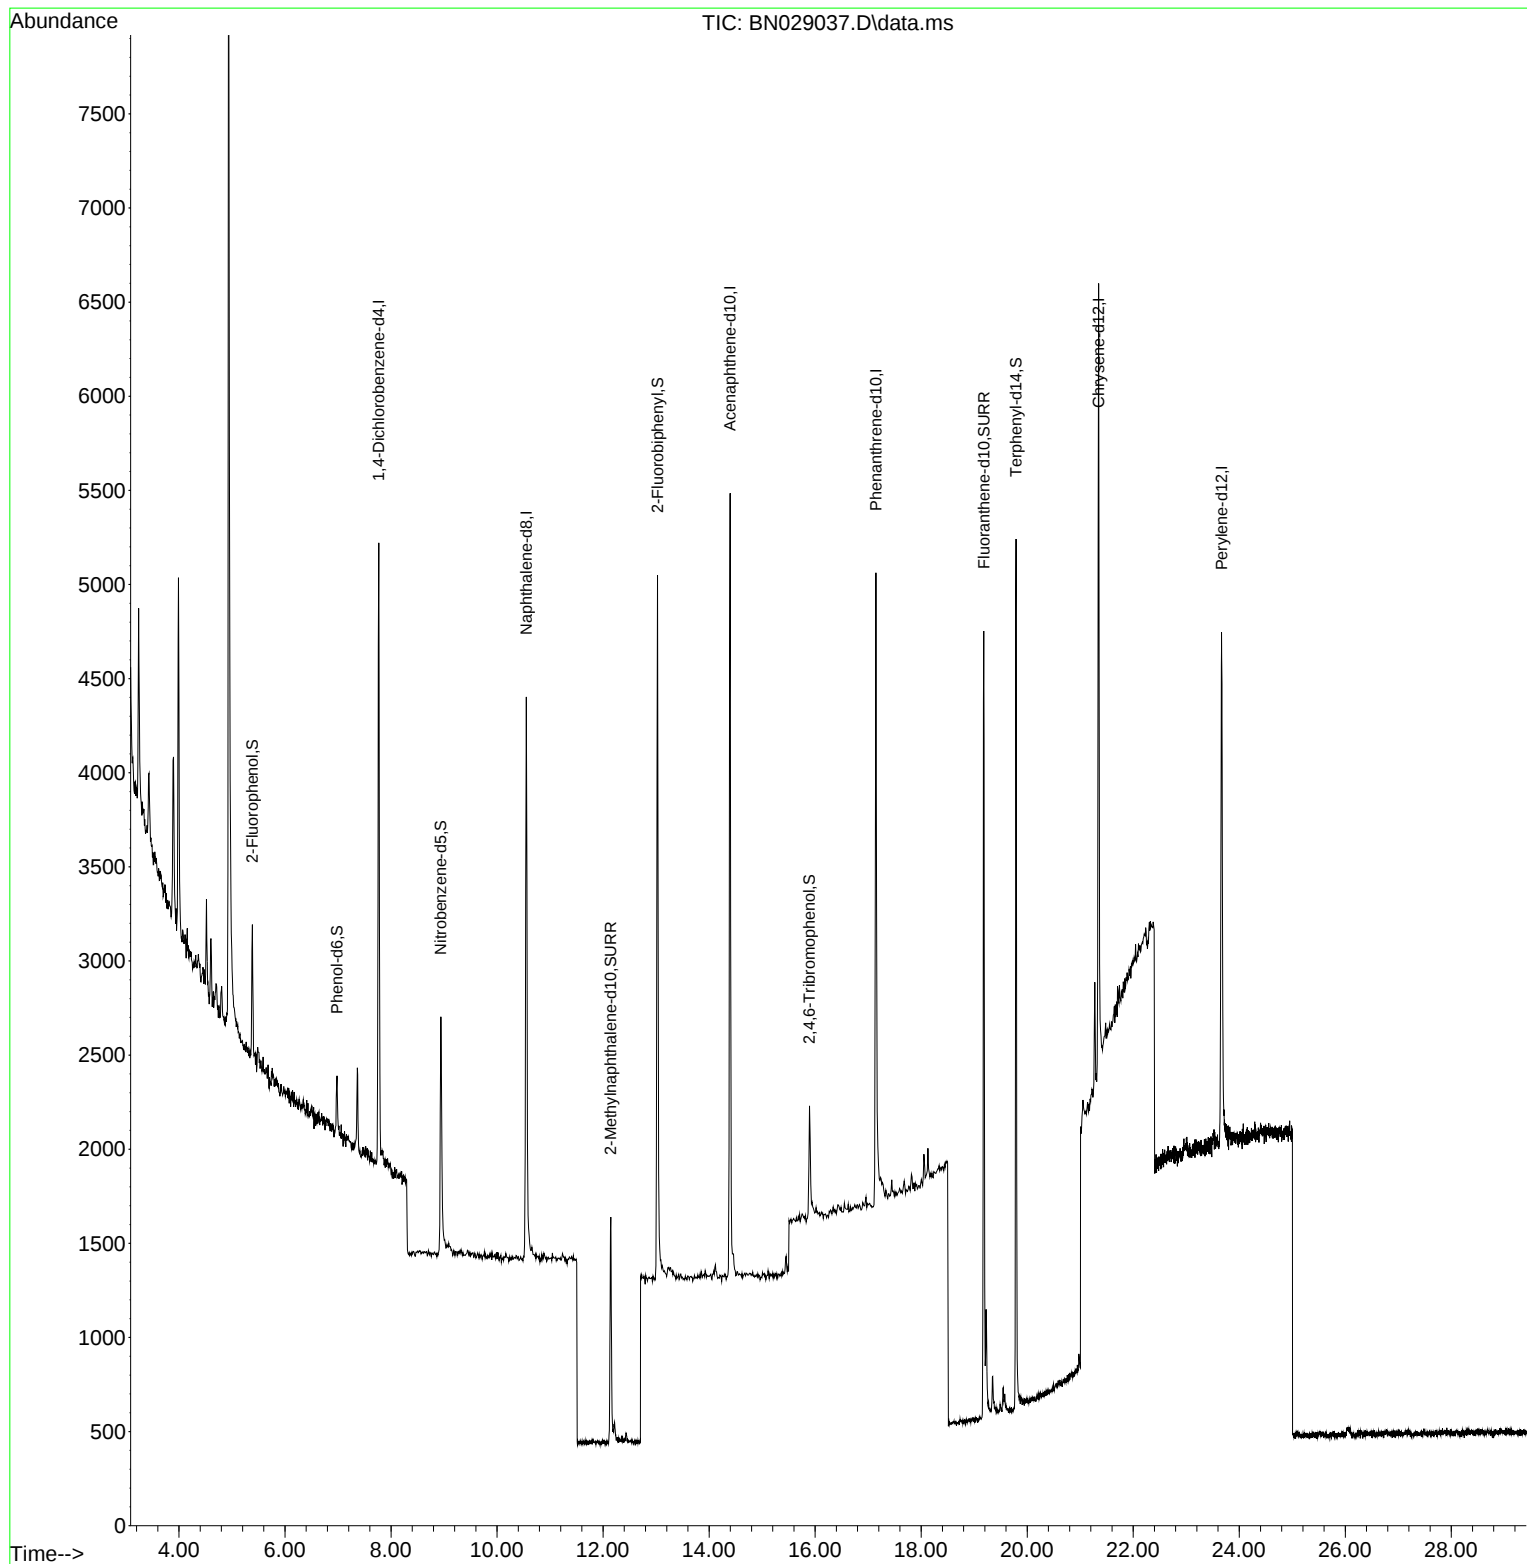






#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.768 min Scan# 64
 Delta R.T. -0.014 min
 Lab File: BN029037.D
 Acq: 04 Dec 2023 03:02

Instrument :
 BNA_N
 ClientSampleId :
 RE120D3-20231113



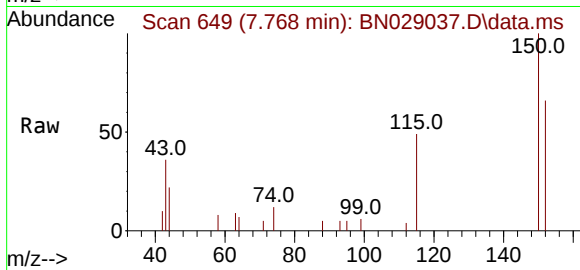



Tgt Ion:152 Resp: 1551
 Ion Ratio Lower Upper
 152 100
 150 151.1 123.4 185.2
 115 73.7 59.1 88.7

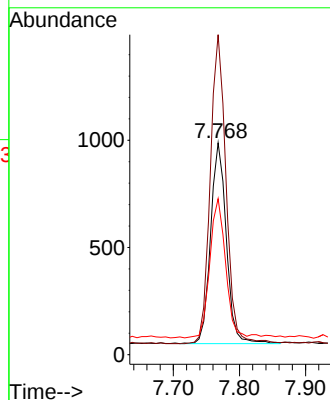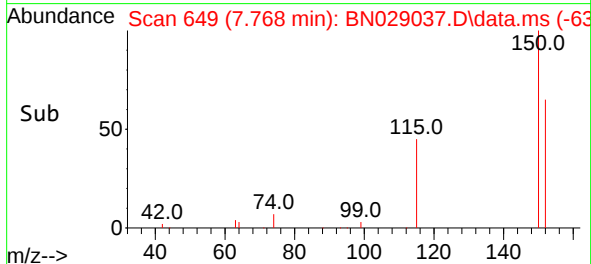

#4
 2-Fluorophenol
 Concen: 0.103 ng
 RT: 5.384 min Scan# 319
 Delta R.T. -0.015 min
 Lab File: BN029037.D
 Acq: 04 Dec 2023 03:02

Tgt Ion:112 Resp: 484
 Ion Ratio Lower Upper
 112 100
 64 61.2 51.5 77.3
 63 55.2 30.4 45.6#


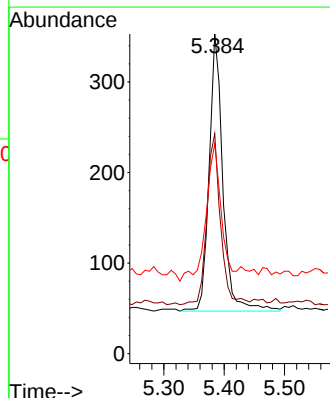

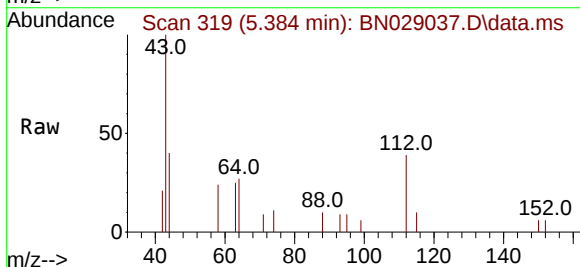




#5
Phenol-d6
Concen: 0.054 ng
RT: 6.980 min Scan# 54
Delta R.T. -0.007 min
Lab File: BN029037.D
Acq: 04 Dec 2023 03:02




Instrument :
BNA_N
ClientSampleId :
RE120D3-20231113


Tgt Ion: 99 Resp: 283
Ion Ratio Lower Upper
99 100
42 45.9 21.2 31.8#
71 55.1 35.4 53.0#

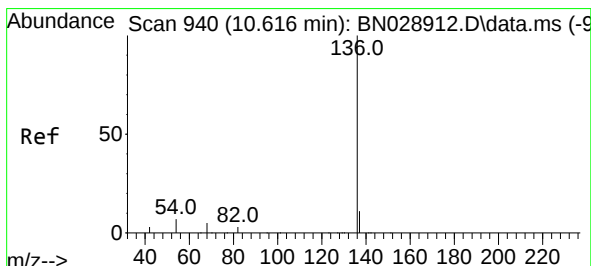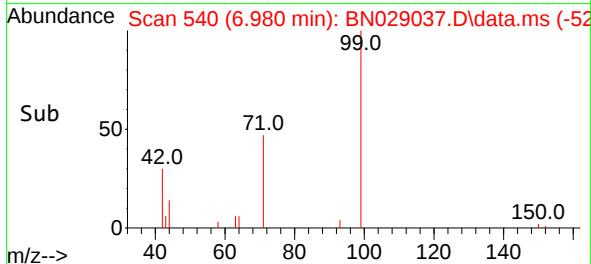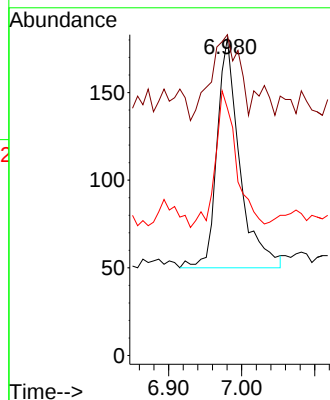

#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.551 min Scan# 934
Delta R.T. -0.011 min
Lab File: BN029037.D
Acq: 04 Dec 2023 03:02

Tgt Ion: 136 Resp: 4144
Ion Ratio Lower Upper
136 100
137 13.2 10.6 16.0
54 12.4 7.5 11.3#
68 5.9 5.9 8.9#


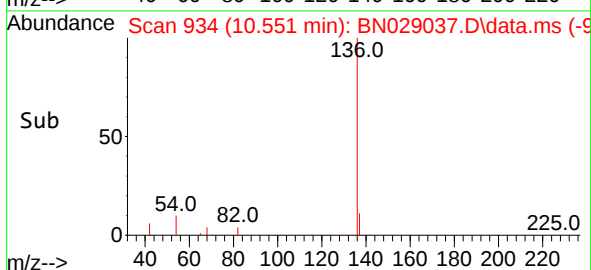
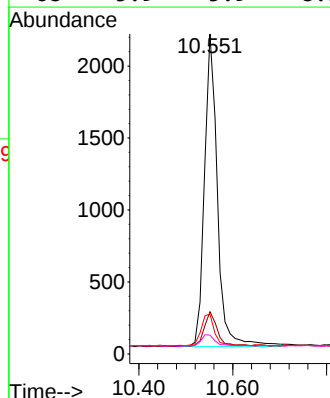
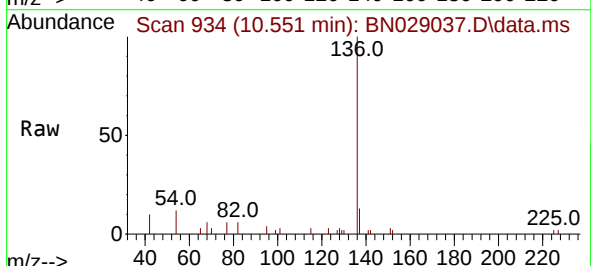


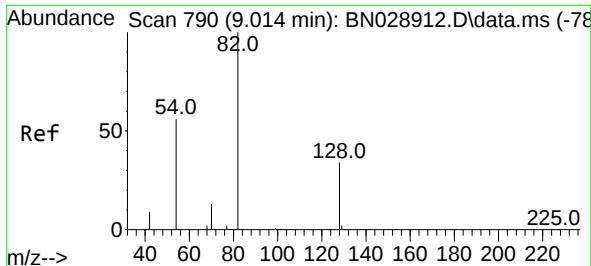

#8
Nitrobenzene-d5
Concen: 0.296 ng
RT: 8.939 min Scan# 71
Delta R.T. -0.011 min
Lab File: BN029037.D
Acq: 04 Dec 2023 03:02




Instrument :
BNA_N
ClientSampleId :
RE120D3-20231113


Tgt Ion: 82 Resp: 1220
Ion Ratio Lower Upper
82 100
128 43.3 29.2 43.8
54 72.9 47.0 70.6#

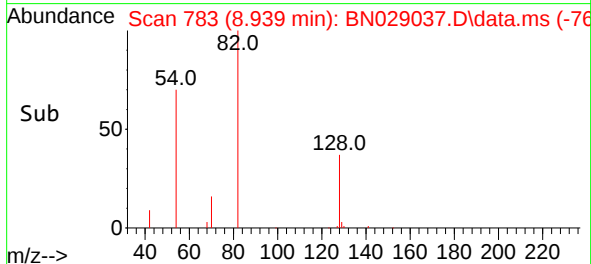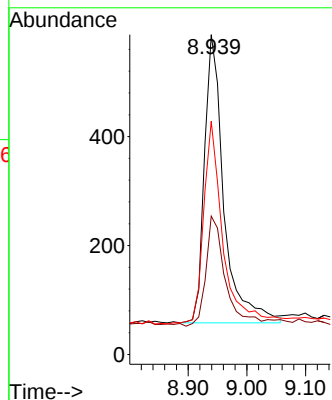

#11
2-Methylnaphthalene-d10
Concen: 0.281 ng
RT: 12.144 min Scan# 1191
Delta R.T. -0.008 min
Lab File: BN029037.D
Acq: 04 Dec 2023 03:02

Tgt Ion: 152 Resp: 1872
Ion Ratio Lower Upper
152 100
151 19.9 16.7 25.1



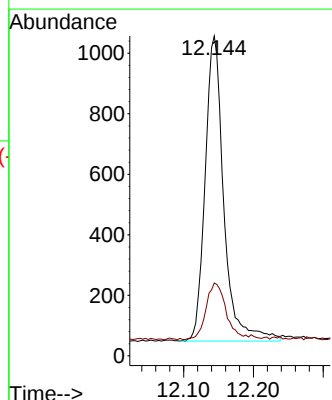
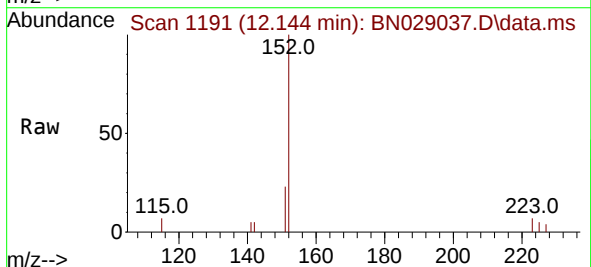




#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.396 min Scan# 14
Delta R.T. -0.011 min
Lab File: BN029037.D
Acq: 04 Dec 2023 03:02




Instrument :
BNA_N
ClientSampleId :
RE120D3-20231113


Tgt Ion:164 Resp: 2535
Ion Ratio Lower Upper
164 100
162 103.5 81.7 122.5
160 49.1 37.0 55.6

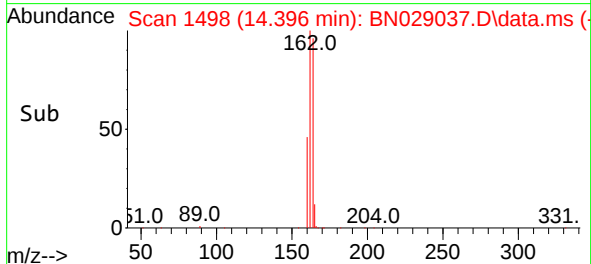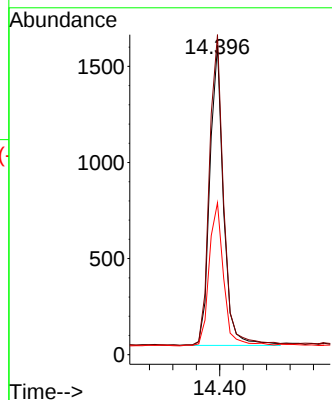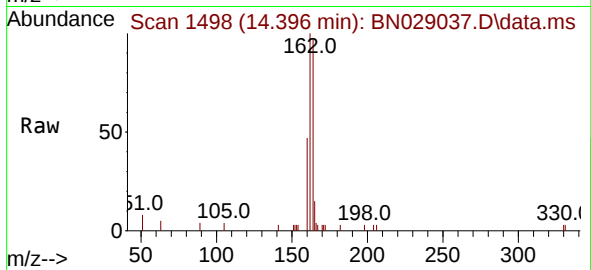

#14
2,4,6-Tribromophenol
Concen: 0.263 ng
RT: 15.893 min Scan# 1633
Delta R.T. -0.013 min
Lab File: BN029037.D
Acq: 04 Dec 2023 03:02

Tgt Ion:330 Resp: 451
Ion Ratio Lower Upper
330 100
332 92.9 75.4 113.2
141 49.9 35.7 53.5

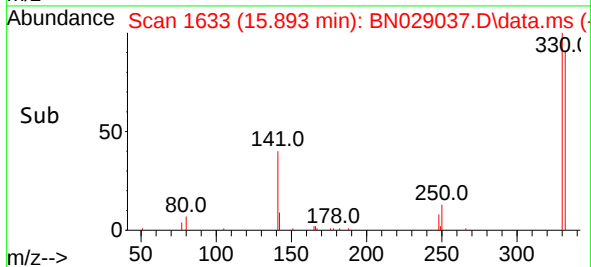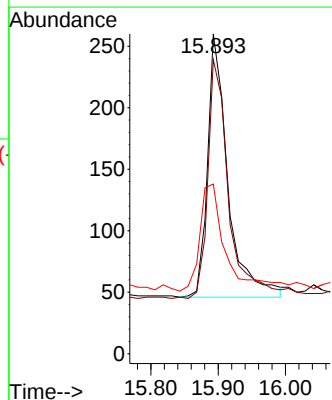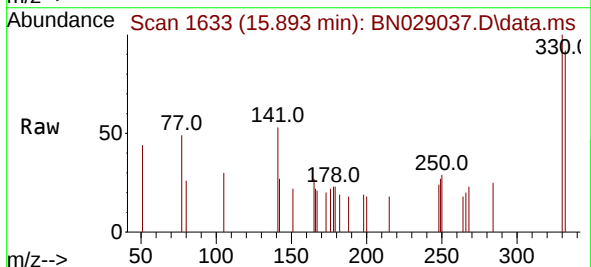



#15

2-Fluorobiphenyl

Concen: 0.313 ng

RT: 13.028 min Scan# 11

Delta R.T. -0.011 min

Lab File: BN029037.D

Acq: 04 Dec 2023 03:02

Instrument :

BNA_N

ClientSampleId :

RE120D3-20231113





Tgt Ion:172 Resp: 3426

Ion Ratio Lower Upper

172 100

171 36.6 29.0 43.4

170 23.9 19.7 29.5

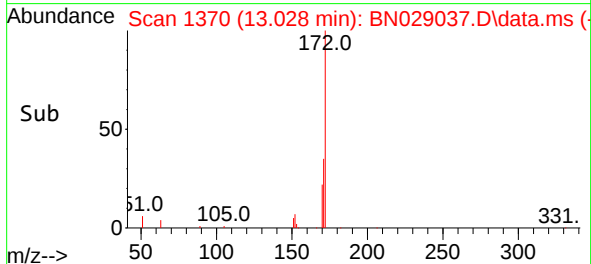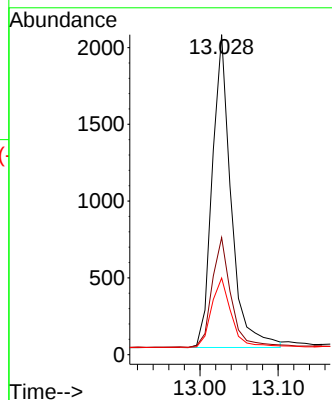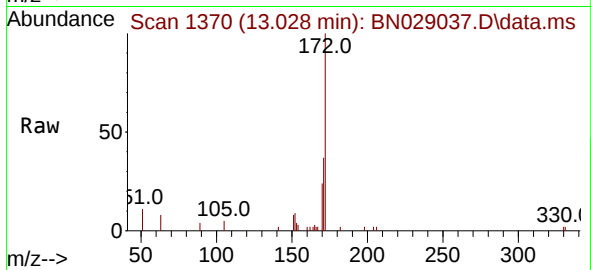

#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.146 min Scan# 1734

Delta R.T. -0.013 min

Lab File: BN029037.D

Acq: 04 Dec 2023 03:02




Tgt Ion:188 Resp: 5537


Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0

80 9.5 9.0 13.6


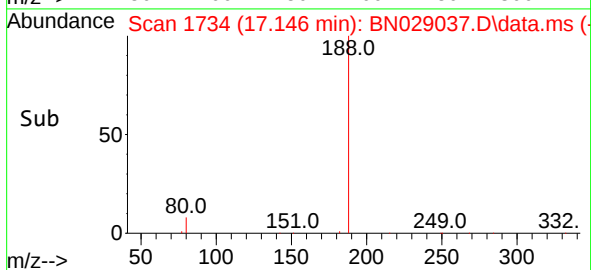
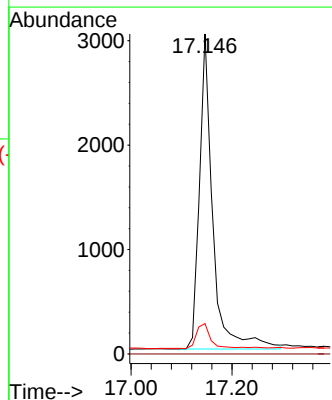
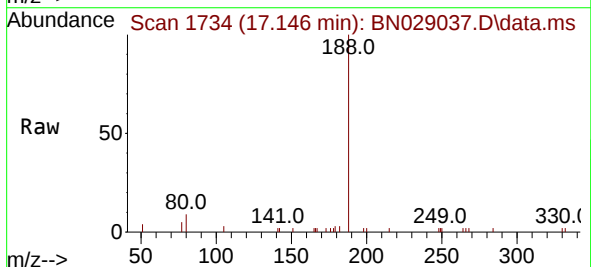


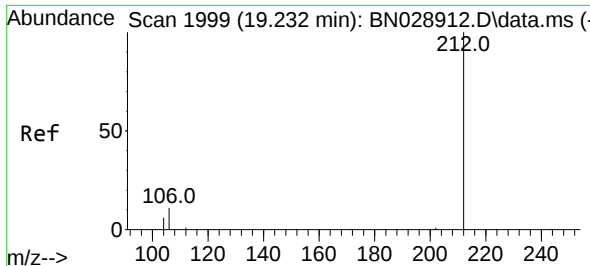

#27
Fluoranthene-d10
Concen: 0.353 ng
RT: 19.181 min Scan# 19
Delta R.T. -0.009 min
Lab File: BN029037.D
Acq: 04 Dec 2023 03:02




Instrument :
BNA_N
ClientSampleId :
RE120D3-20231113


Tgt Ion:212 Resp: 5146
Ion Ratio Lower Upper
212 100
106 9.6 9.4 14.2
104 6.1 6.2 9.2#

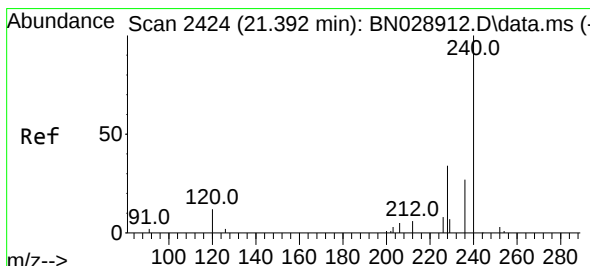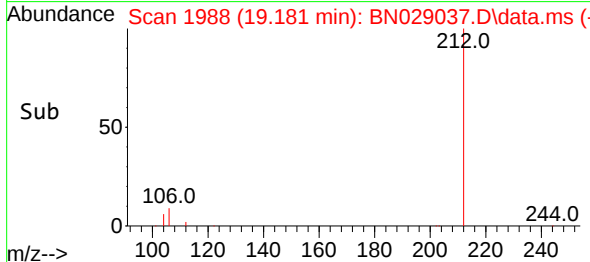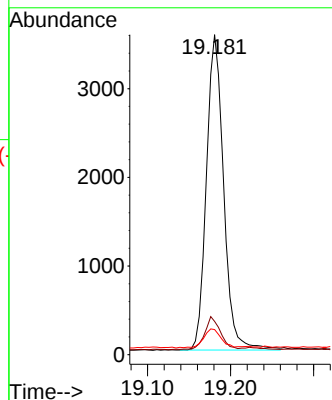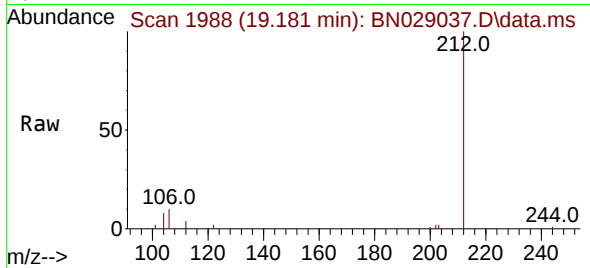

#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.347 min Scan# 2419
Delta R.T. -0.000 min
Lab File: BN029037.D
Acq: 04 Dec 2023 03:02

Tgt Ion:240 Resp: 4107
Ion Ratio Lower Upper
240 100
120 11.5 37.1 55.7#
236 29.7 32.4 48.6#


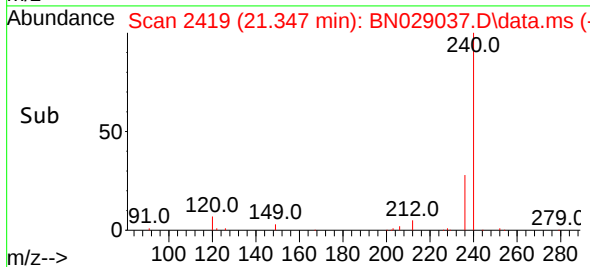
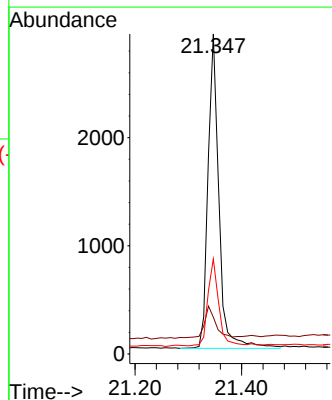
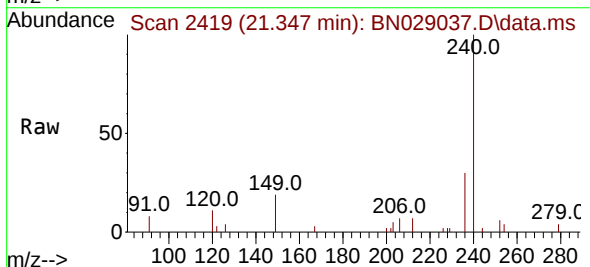


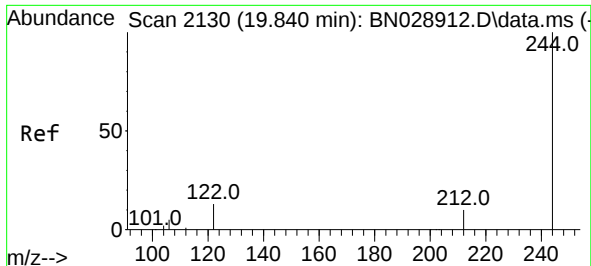

#31
 Terphenyl-d14
 Concen: 0.403 ng
 RT: 19.789 min Scan# 2130
 Delta R.T. -0.005 min
 Lab File: BN029037.D
 Acq: 04 Dec 2023 03:02

Instrument :
 BNA_N
 ClientSampleId :
 RE120D3-20231113

Tgt Ion:244 Resp: 4734
 Ion Ratio Lower Upper
 244 100
 212 11.9 11.5 17.3
 122 13.5 13.2 19.8

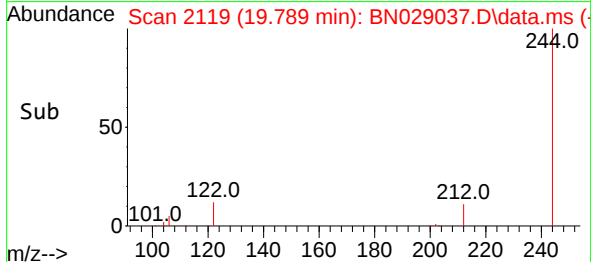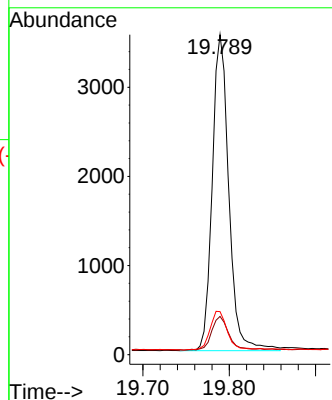

#35
 Perylene-d12
 Concen: 0.400 ng
 RT: 23.667 min Scan# 2969
 Delta R.T. -0.003 min
 Lab File: BN029037.D
 Acq: 04 Dec 2023 03:02

Tgt Ion:264 Resp: 4032
 Ion Ratio Lower Upper
 264 100
 260 26.7 20.6 30.8
 265 74.1 464.5 696.7#

