


Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN120323\  
Data File : BN029007.D  
Acq On : 03 Dec 2023 06:47  
Operator : MA/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 61 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN113023.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Mon Dec 04 00:28:48 2023

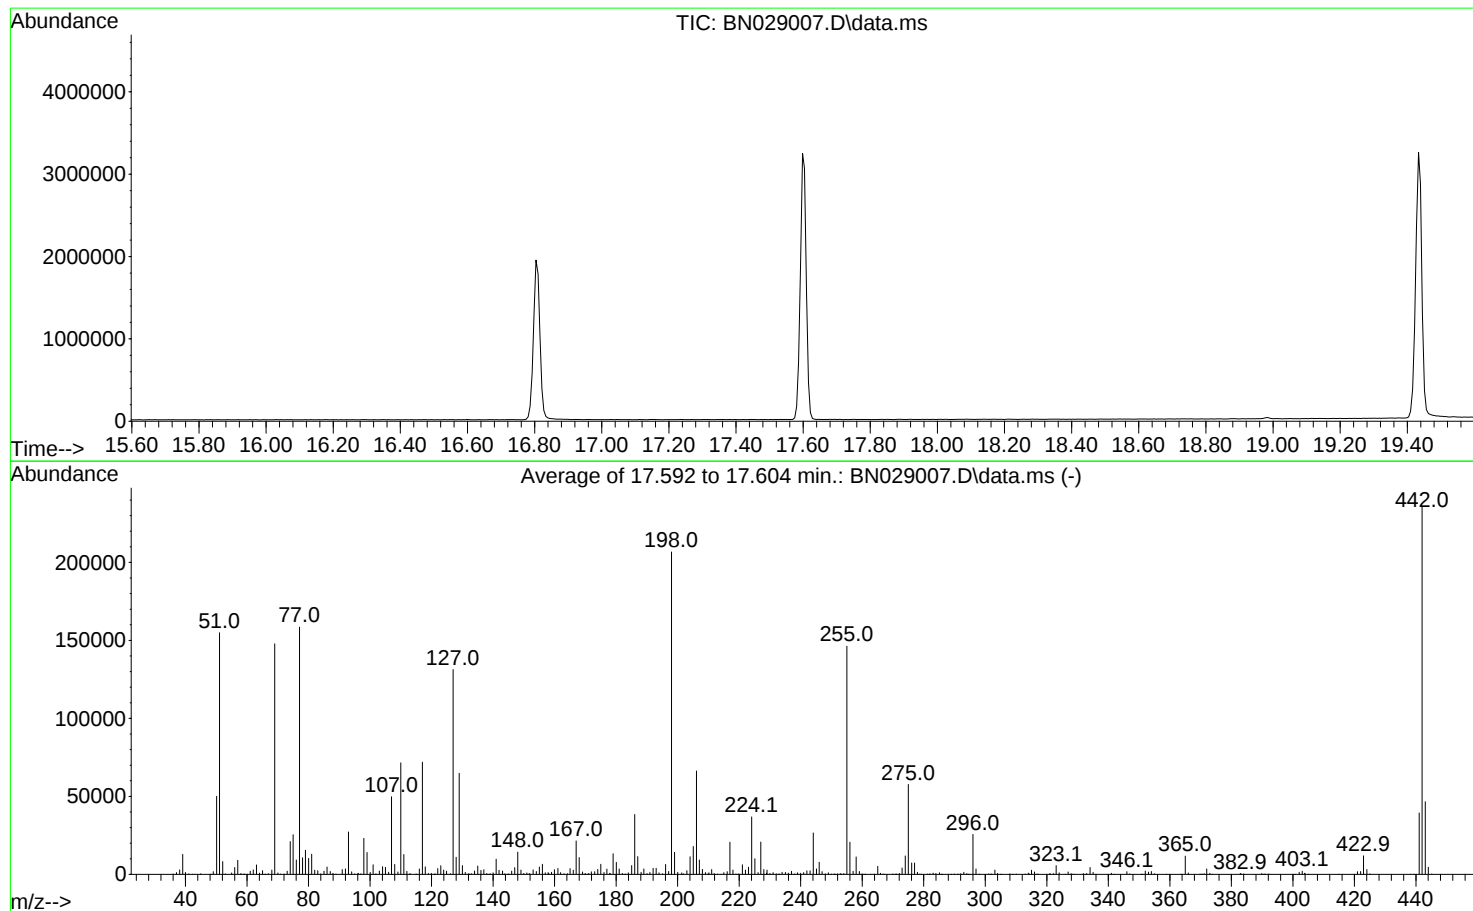




AutoFind: Scans 2466, 2467, 2468; Background Corrected with Scan 2459

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 74.9         | 154869     | PASS                |
| 68             | 69              | 0.00            | 2               | 1.9          | 2809       | PASS                |
| 69             | 198             | 0.00            | 100             | 71.5         | 147824     | PASS                |
| 70             | 69              | 0.00            | 2               | 0.6          | 943        | PASS                |
| 127            | 198             | 10              | 80              | 63.5         | 131325     | PASS                |
| 197            | 198             | 0.00            | 2               | 0.9          | 1900       | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 206720     | PASS                |
| 199            | 198             | 5               | 9               | 6.9          | 14170      | PASS                |
| 275            | 198             | 10              | 60              | 27.9         | 57645      | PASS                |
| 365            | 198             | 1               | 100             | 5.7          | 11739      | PASS                |
| 441            | 198             | 0.01            | 100             | 19.1         | 39392      | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 235851     | PASS                |
| 443            | 442             | 15              | 24              | 19.7         | 46579      | PASS                |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN120323\  
Data File : BN029007.D  
Acq On : 03 Dec 2023 06:47  
Operator : MA/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 61 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
DFTPP

Quant Time: Dec 04 02:54:13 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Dec 01 23:28:24 2023  
Response via : Initial Calibration

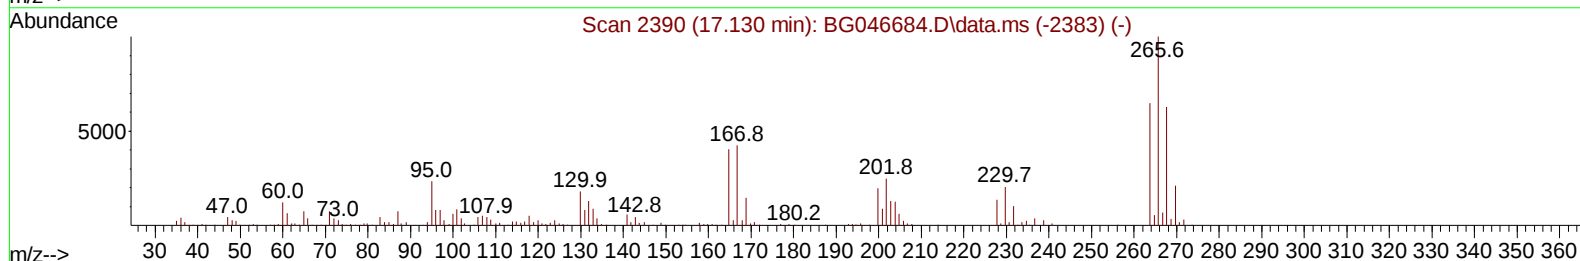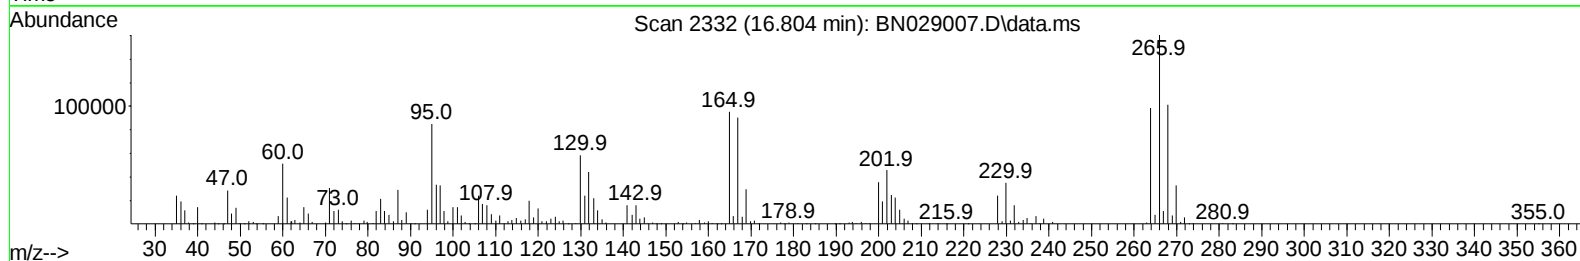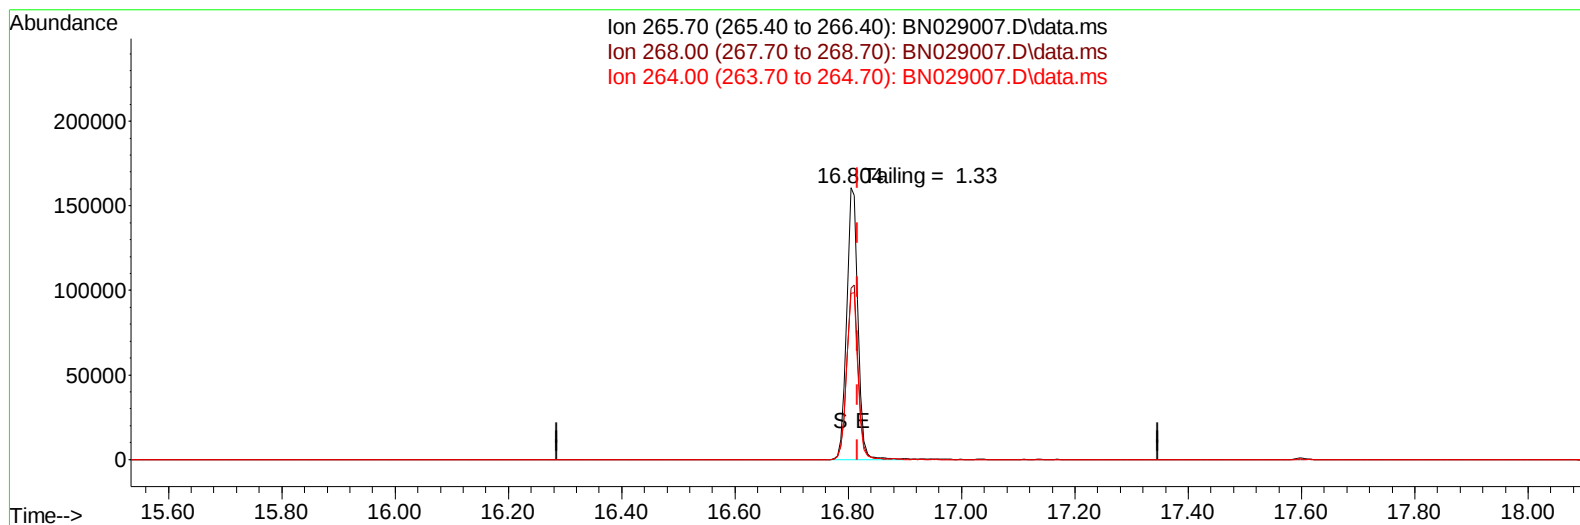

TIC: BN029007.D\data.ms

**(70) Pentachlorophenol (C)**

**16.804min (-0.012) 12635.49 ng**




**response 219144**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.20  | 63.01  |
| 264.00 | 61.60  | 61.26  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN120323\  
 Data File : BN029007.D  
 Acq On : 03 Dec 2023 06:47  
 Operator : MA/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 61 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 DFTPP

Quant Time: Dec 04 02:54:13 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Dec 01 23:28:24 2023  
 Response via : Initial Calibration

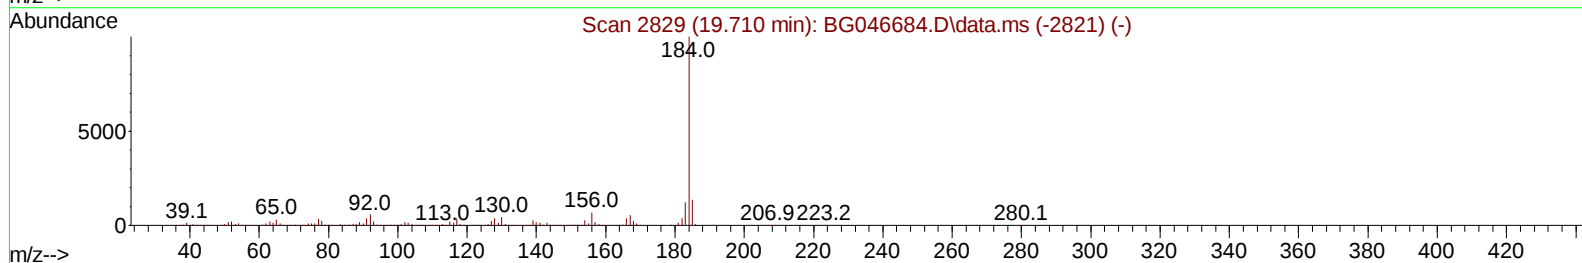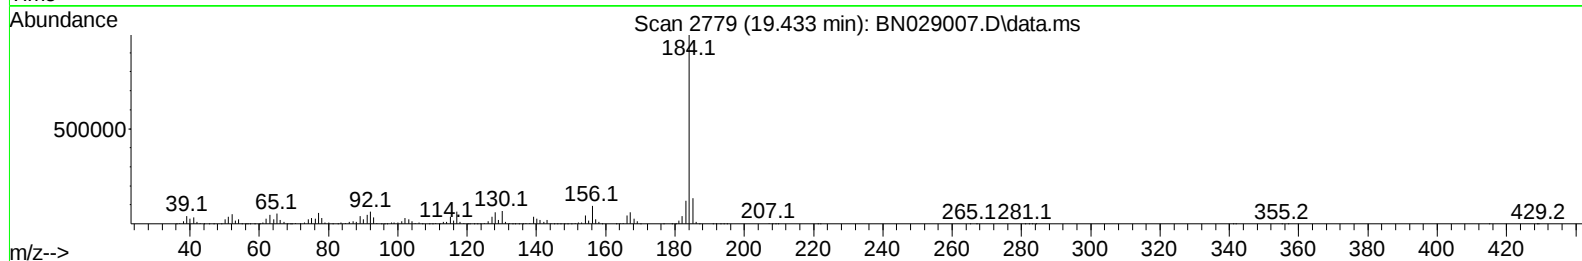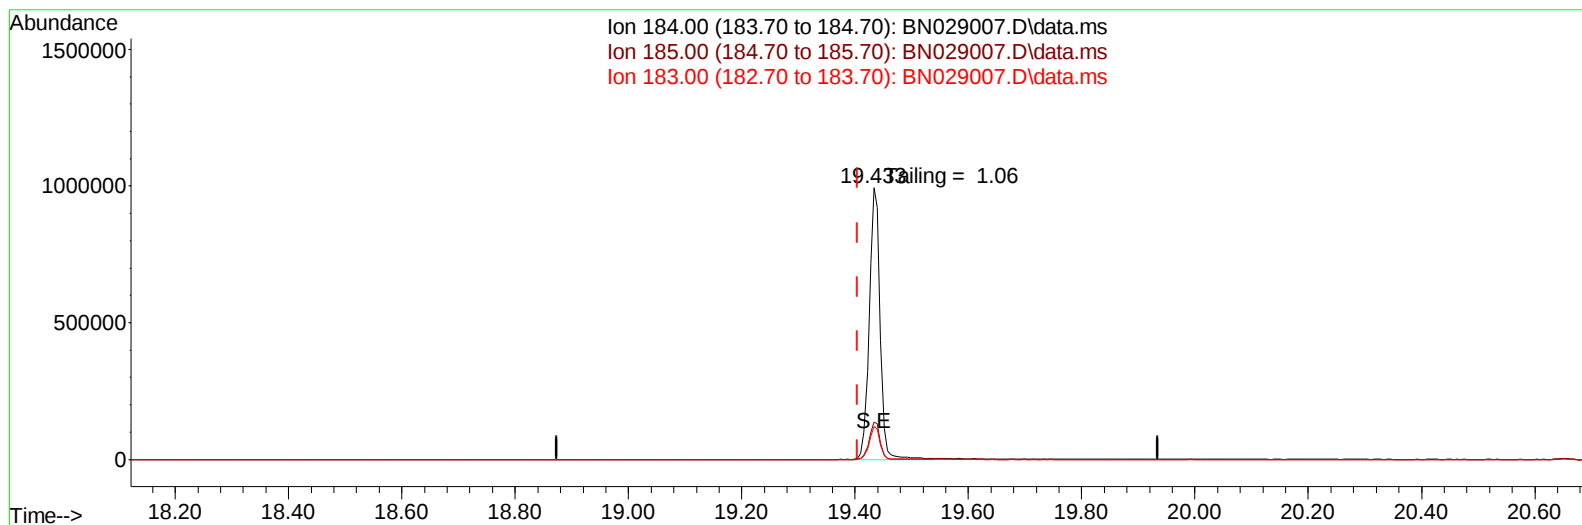

TIC: BN029007.D\data.ms

**(77) Benzidine****19.433min (+ 0.029) 712210.31 ng****response 1339203**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.50  | 13.73  |
| 183.00 | 13.20  | 12.12  |
| 0.00   | 0.00   | 0.00   |

# DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 12/3/2023     | BNA_N            | <u>BN029007.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 6913270          | 20.651             |
| DDD           | 46874            | 20.21              |
| DDE           | 387              | 19.698             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 47261         | 6960531          | 0.68               |
|               |                  |                    |

Instrument :  
BNA\_N  
ClientSampleId :  
DFTPP