
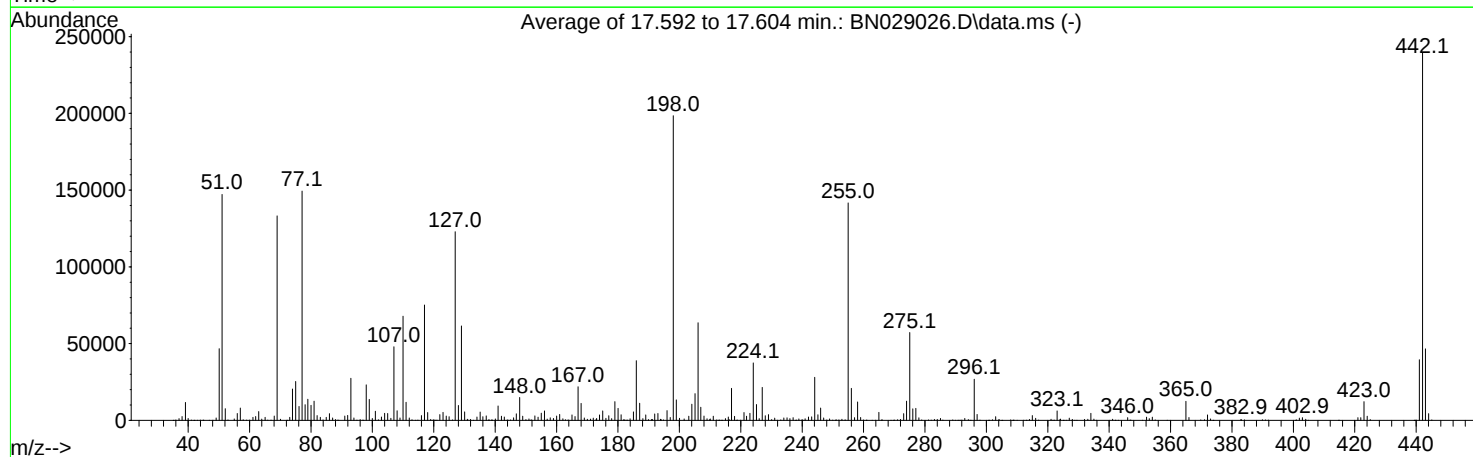


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120323\
Data File : BN029026.D
Acq On : 03 Dec 2023 19:17
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 81 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN113023.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Dec 04 00:28:48 2023

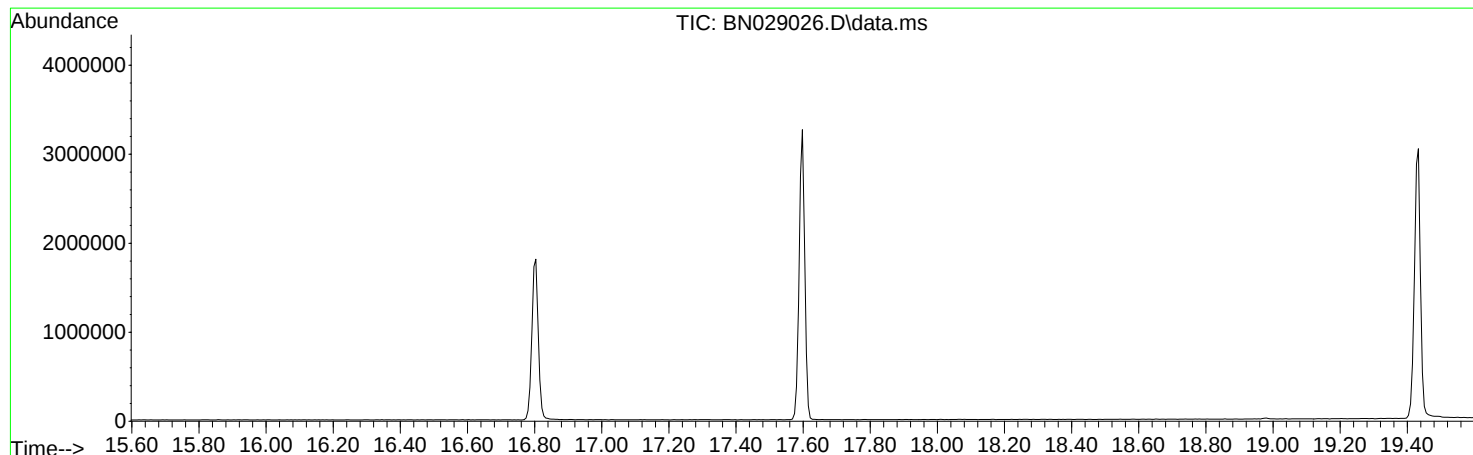




AutoFind: Scans 2466, 2467, 2468; Background Corrected with Scan 2459

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	74.2	147245	PASS
68	69	0.00	2	2.1	2853	FAIL*
69	198	0.00	100	67.1	133251	PASS
70	69	0.00	2	0.6	740	PASS
127	198	10	80	61.9	122891	PASS
197	198	0.00	2	1.0	1907	PASS
198	198	100	100	100.0	198443	PASS
199	198	5	9	6.7	13352	PASS
275	198	10	60	28.8	57235	PASS
365	198	1	100	6.3	12429	PASS
441	198	0.01	100	19.9	39504	PASS
442	442	50	100	100.0	239659	PASS
443	442	15	24	19.4	46613	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120323\
Data File : BN029026.D
Acq On : 03 Dec 2023 19:17
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 81 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 04 03:26:09 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 01 23:28:24 2023
Response via : Initial Calibration

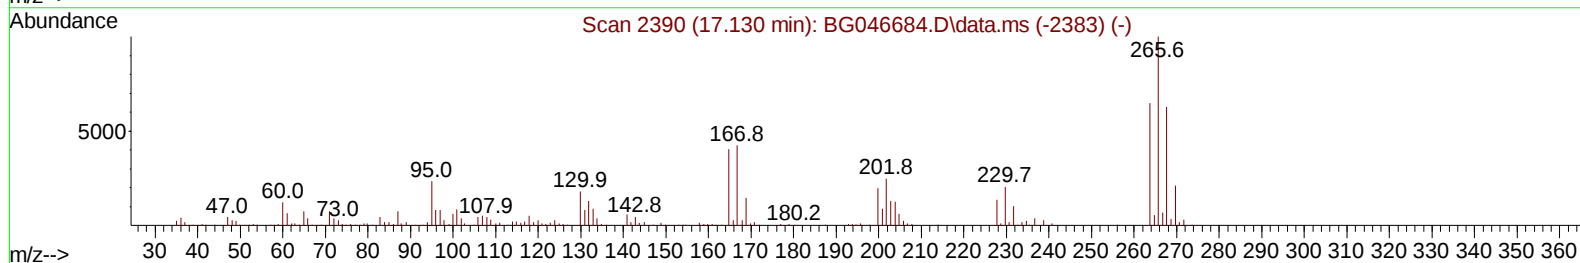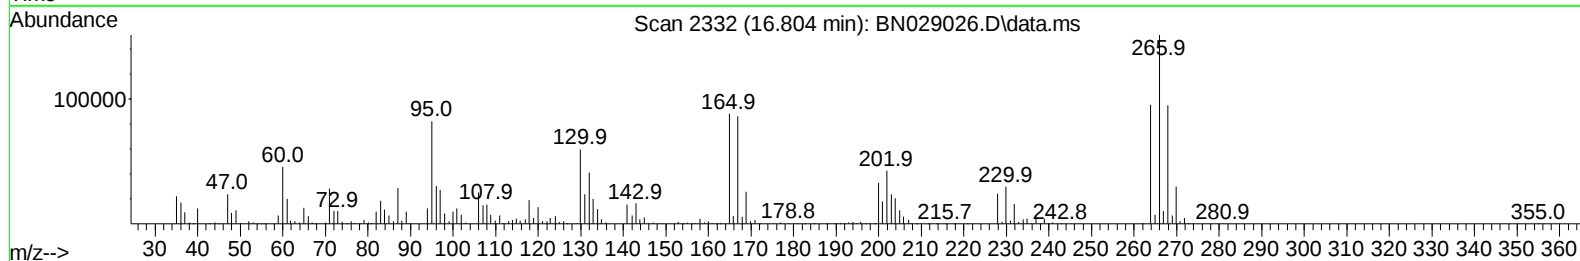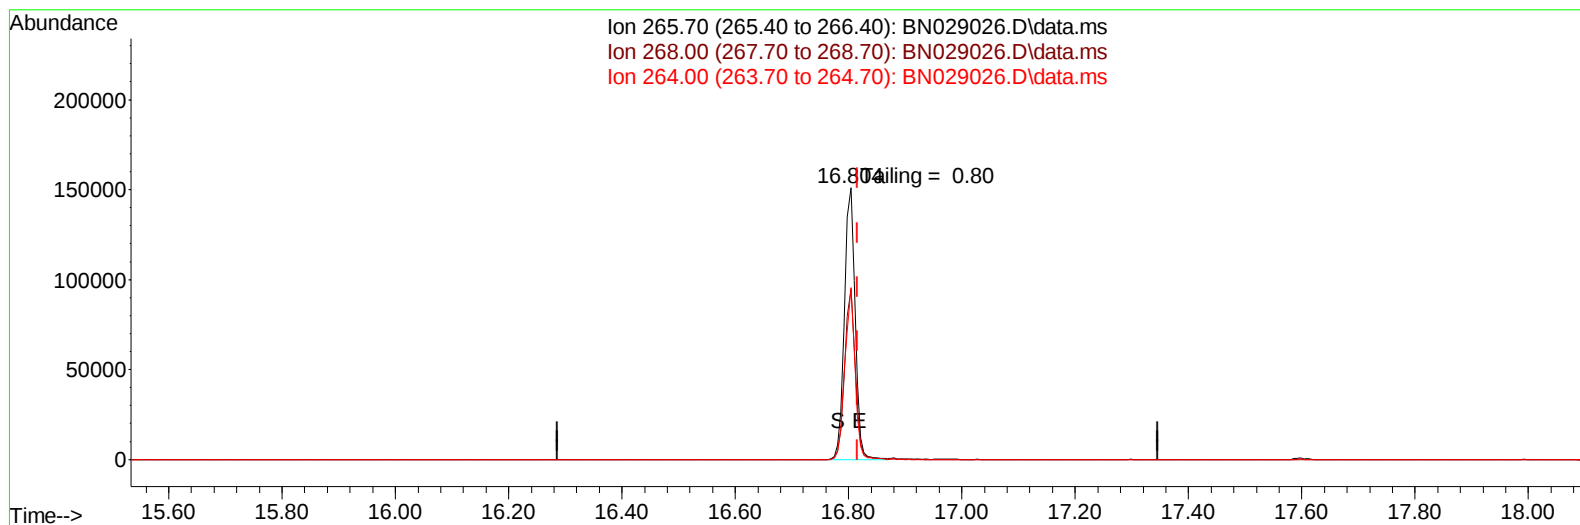

TIC: BN029026.D\data.ms

(70) Pentachlorophenol (C)

16.804min (-0.012) 14036.73 ng




response 197511

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.81
264.00	61.60	63.23
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120323\
Data File : BN029026.D
Acq On : 03 Dec 2023 19:17
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 81 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 04 03:26:09 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 01 23:28:24 2023
Response via : Initial Calibration

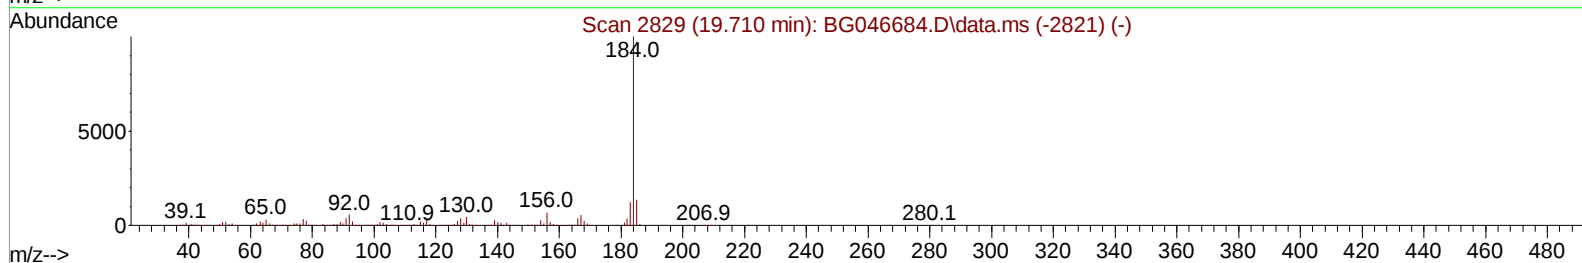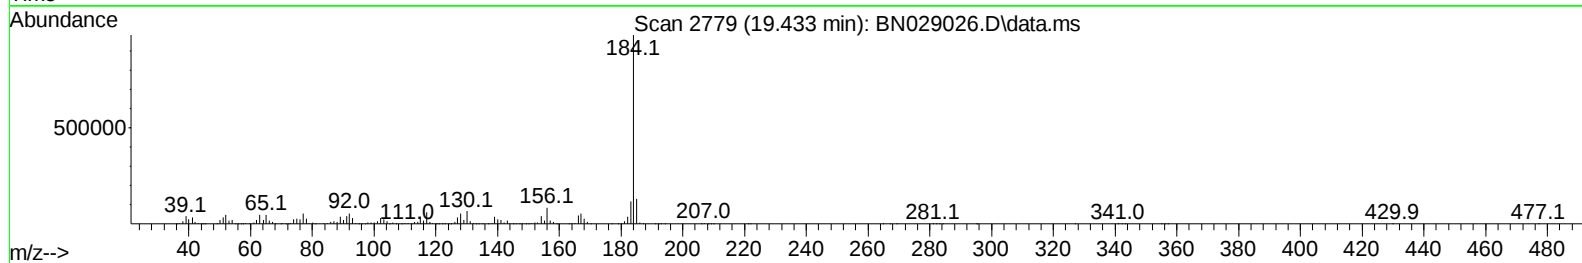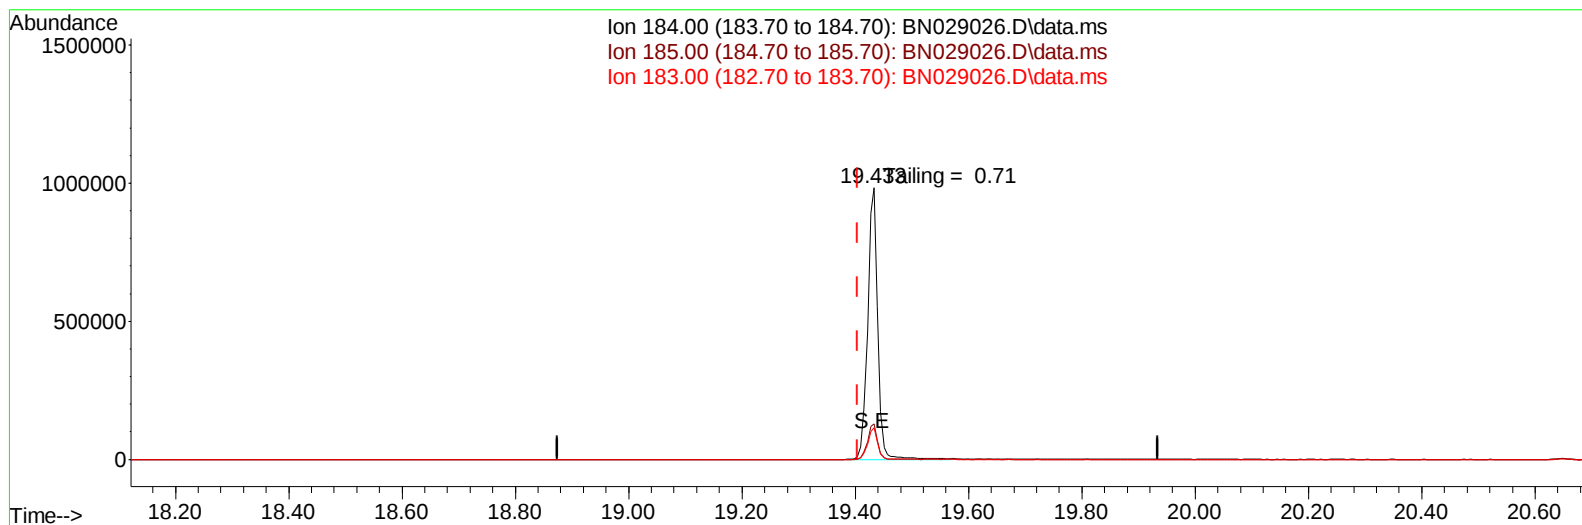

TIC: BN029026.D\data.ms

(77) Benzidine

19.433min (+ 0.029) 662282.36 ng

response 1224906

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.17
183.00	13.20	11.73
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/3/2023	BNA_N	<u>BN029026.D</u>
Compound Name	Response	Retention Time
DDT	632881	20.645
DDD	35501	20.21
DDE	266	19.692
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
35767	668648	5.35

Instrument :
BNA_N
ClientSampleId :
DFTPP