

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120418\
 Data File : BN003693.D
 Acq On : 04 Dec 2018 10:19
 Operator : JU/SJ
 Sample : PB115257BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Dec 04 11:11:40 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 04 01:17:12 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	7129	0.40	ng/ul	0.00
2) Naphthalene-d8	10.63	136	29528	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.47	164	17057	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.32	188	2886913	0.40	ng/ul	0.10
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.40
20) Perylene-d12	23.70	264	37342	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.22	152	16480	0.36	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
9) Fluorene	15.47	166	5567	0.071	ng/ul#	12
23) Benzo(a)pyrene	23.56	252	11584	0.087	ng/ul#	80


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120418\
Data File : BN003693.D
Acq On : 04 Dec 2018 10:19
Operator : JU/SJ
Sample : PB115257BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Dec 04 11:11:40 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 04 01:17:12 2018
Response via : Initial Calibration

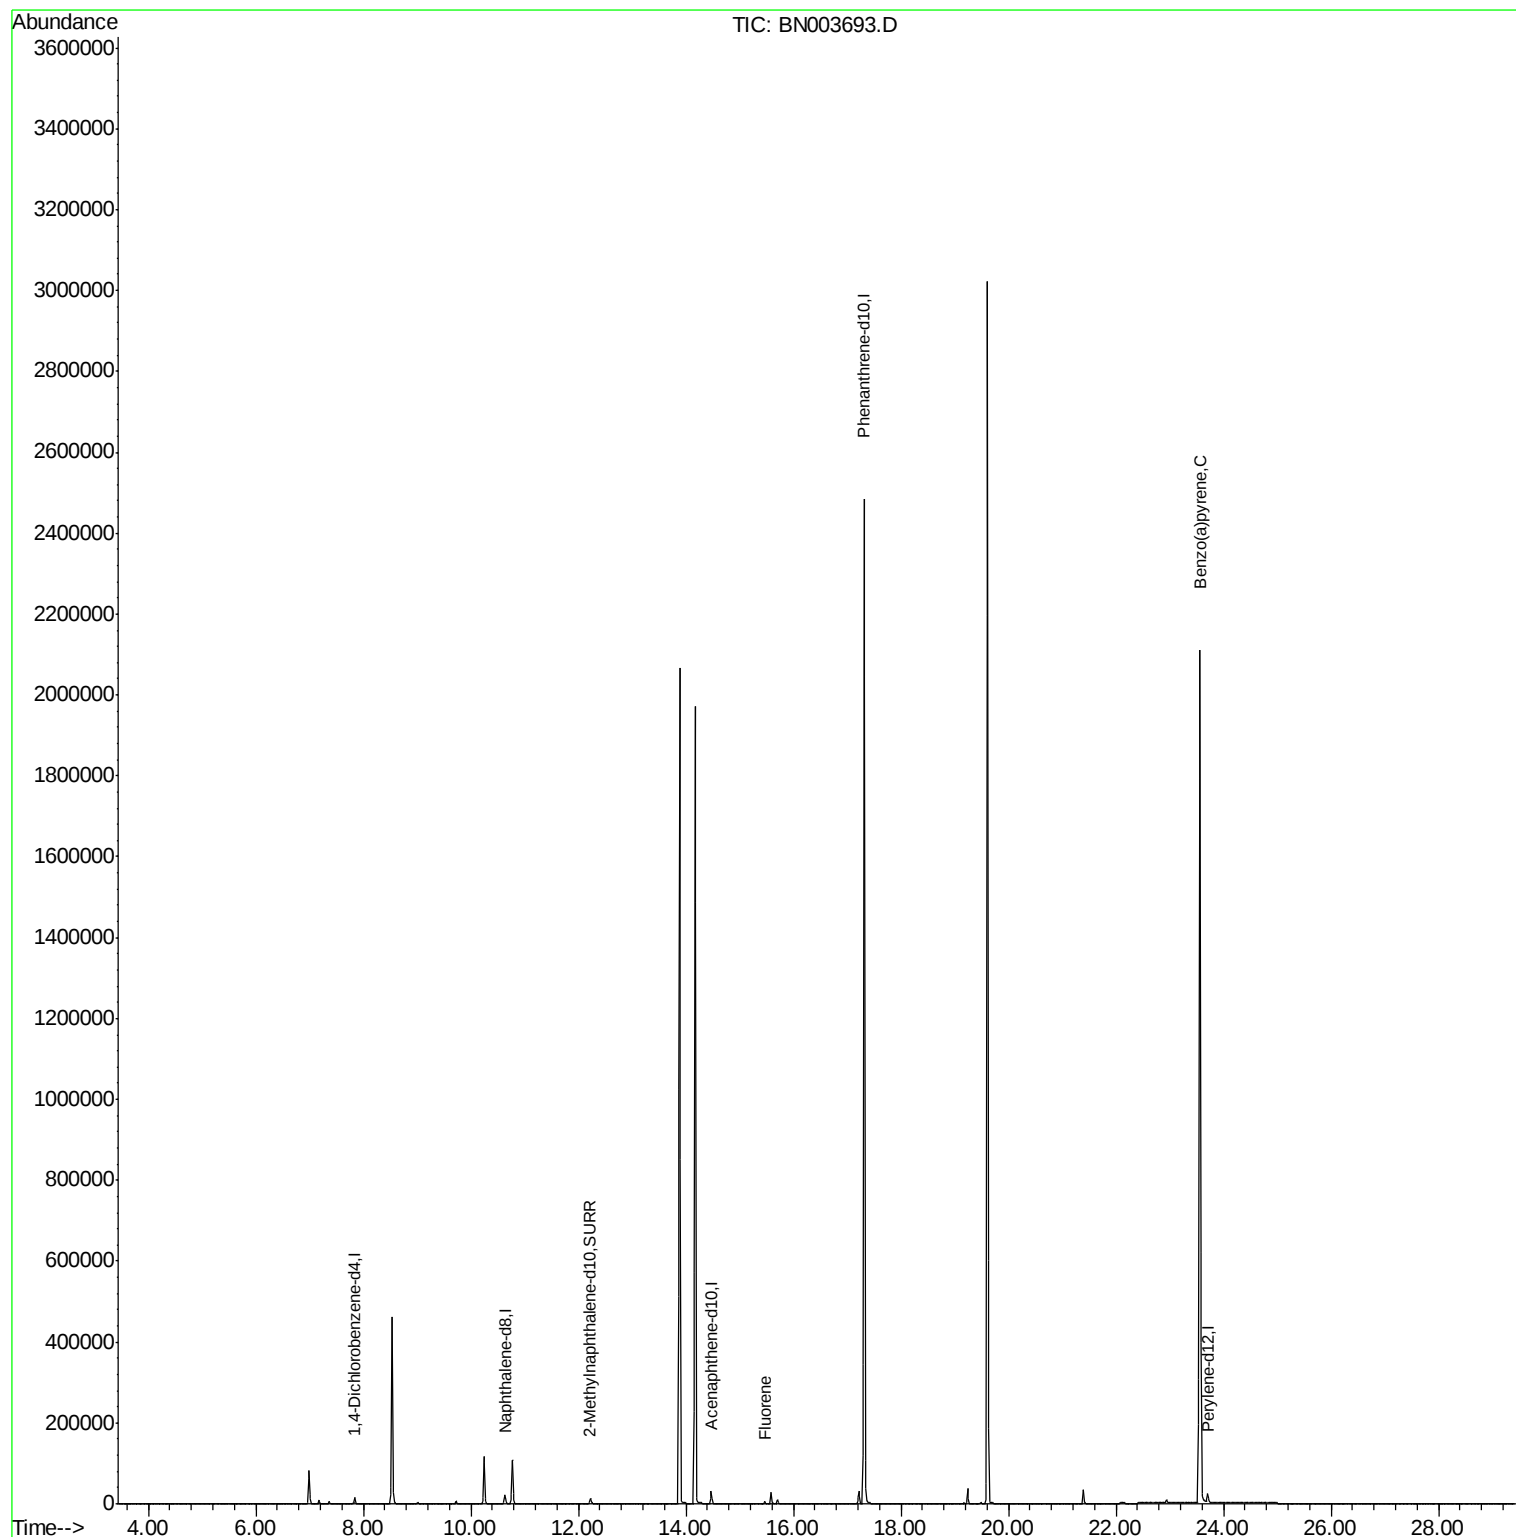

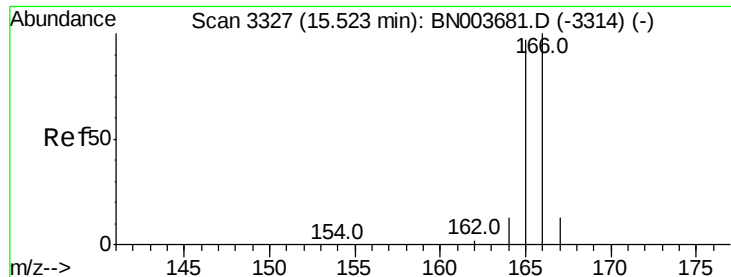

#9

Fluorene

Concen: 0.071 ng/ul

RT: 15.47 min Scan# 3315

Delta R.T. -0.06 min

Lab File: BN003693.D

Acq: 04 Dec 2018 10:19

Instrument :

BNA_N

ClientSampled :





Tot Ion:166 Resp: 5567

Ion Ratio Lower Upper

166 100

165 4.5 78.3 117.5#

167 31.5 11.3 16.9#

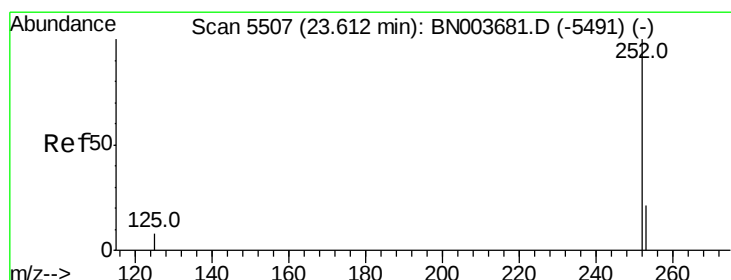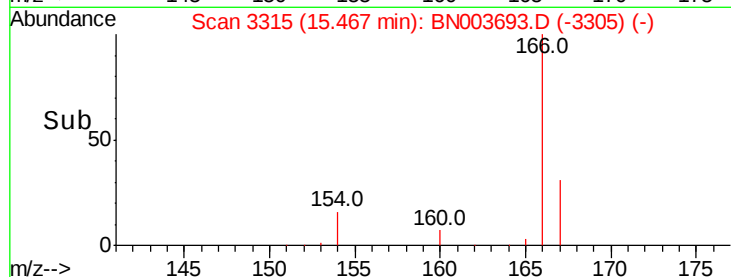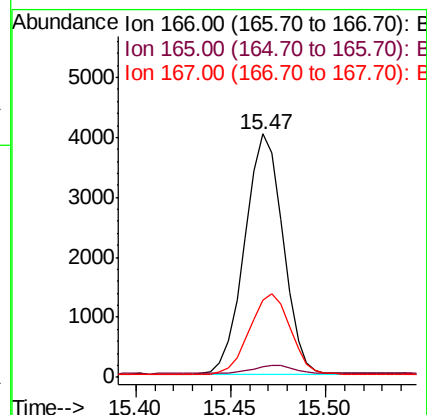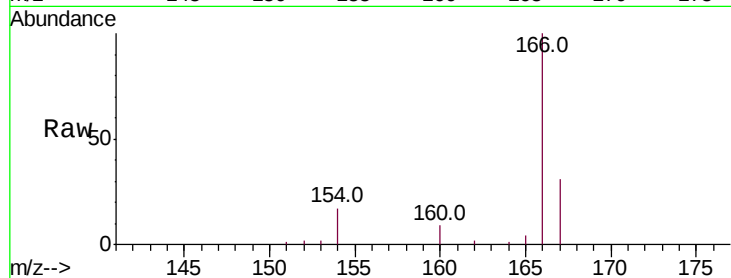

#23

Benzo(a)pyrene

Concen: 0.087 ng/ul

RT: 23.56 min Scan# 5489

Delta R.T. -0.04 min

Lab File: BN003693.D

Acq: 04 Dec 2018 10:19

Tgt Ion:252 Resp: 11584

Ion Ratio Lower Upper

252 100

253 31.1 19.0 28.4#

125 24.0 10.2 15.4#

