

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120518\
 Data File : BN003705.D
 Acq On : 05 Dec 2018 11:20
 Operator : JU/SJ
 Sample : J6155-06
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Dec 05 12:03:51 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 04 01:17:12 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	4588	0.40	ng/ul	0.00
2) Naphthalene-d8	10.63	136	18784	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.47	164	10886	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.31	188	1745449	0.40	ng/ul	0.10
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.40
20) Perylene-d12	23.70	264	22741	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.22	152	9902	0.34	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
21) Benzo(b)fluoranthene	23.01	252	1892	0.020	ng/ul#	Ovalue 46


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120518\
Data File : BN003705.D
Acq On : 05 Dec 2018 11:20
Operator : JU/SJ
Sample : J6155-06
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Dec 05 12:03:51 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 04 01:17:12 2018
Response via : Initial Calibration

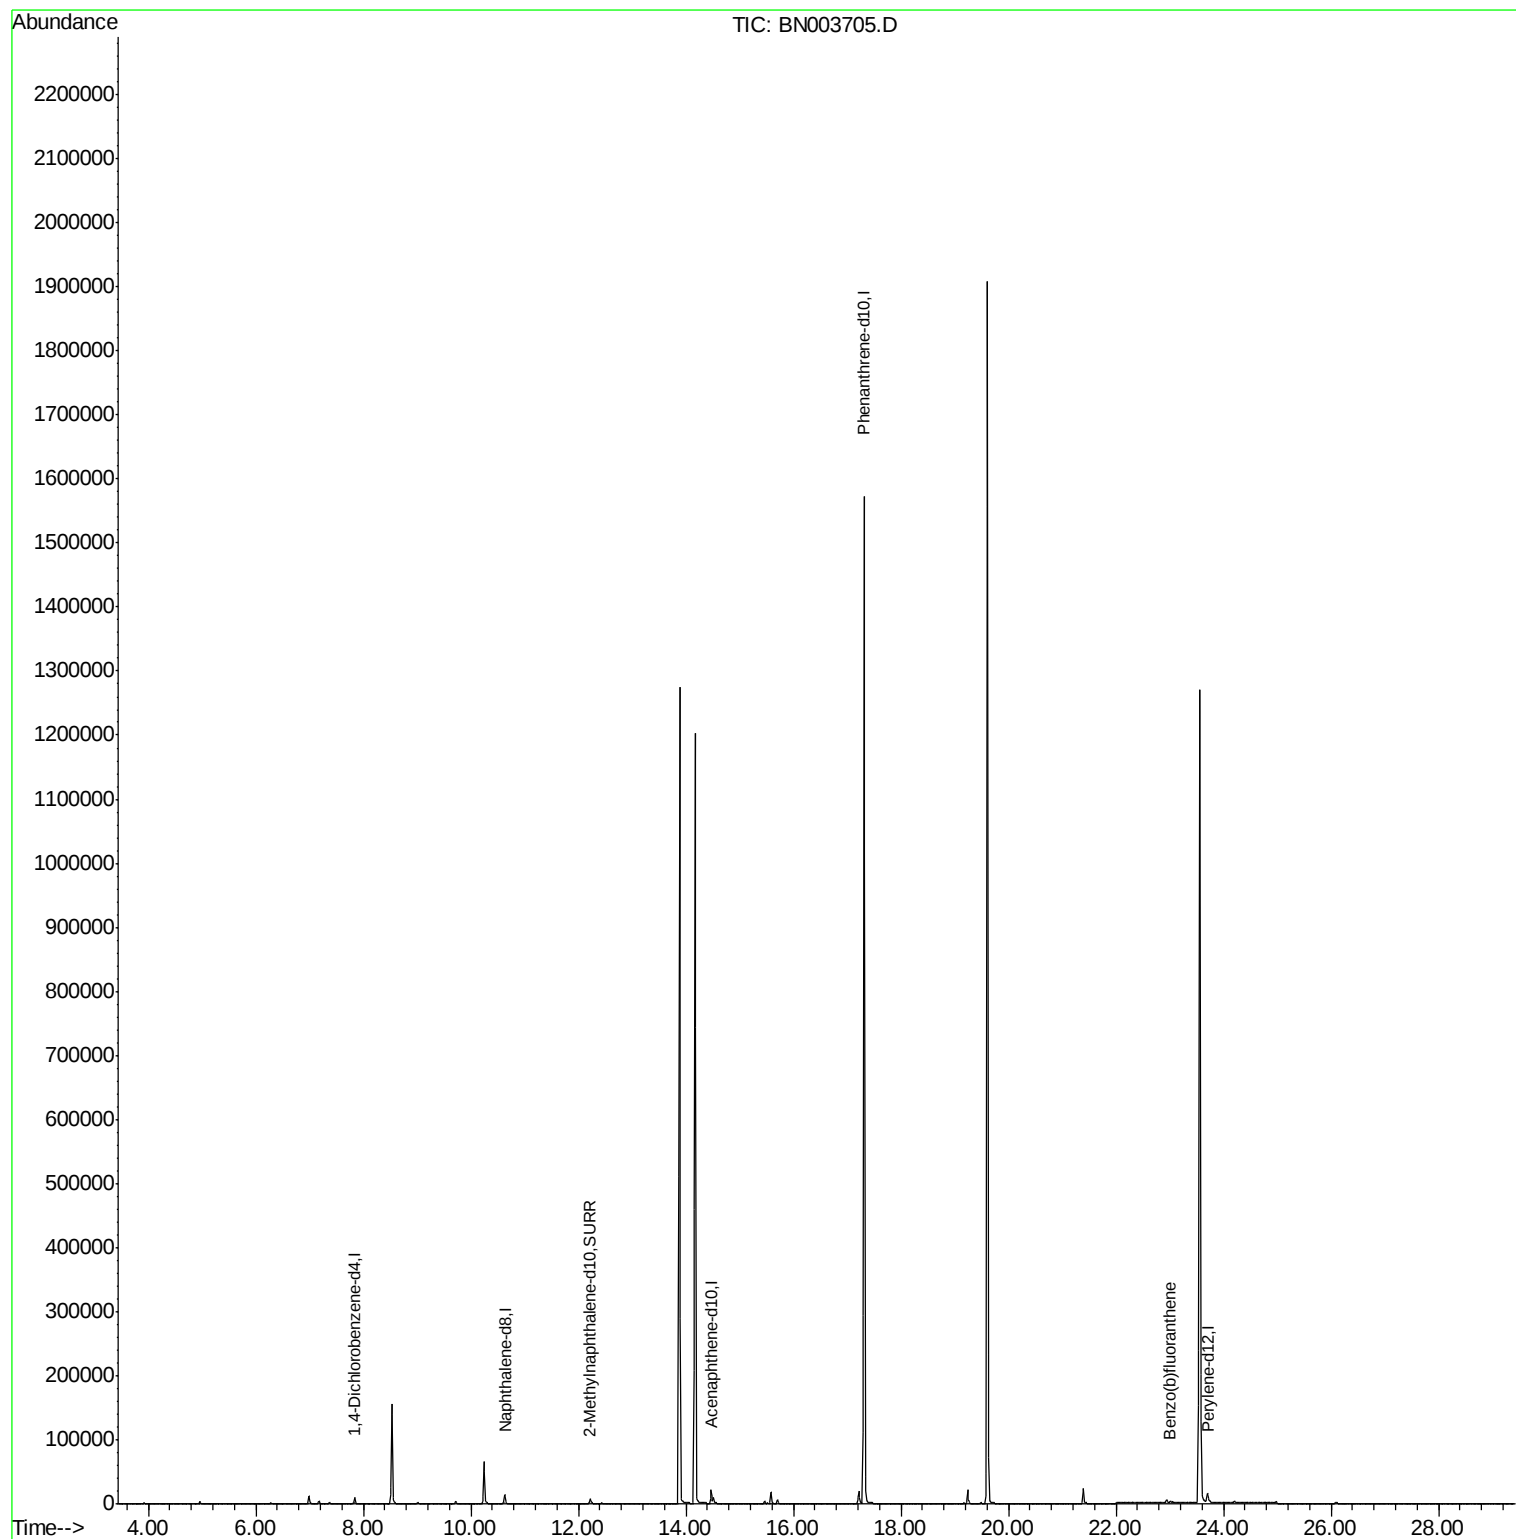

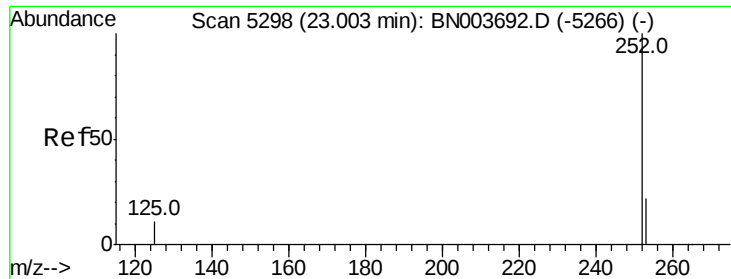

#21

Benzo(b)fluoranthene

Concen: 0.020 ng/ul

RT: 23.01 min Scan# 5299

Delta R.T. 0.00 min

Lab File: BN003705.D

Acq: 05 Dec 2018 11:20

Instrument :

BNA_N

ClientSampleId :


Tot Ion: 252 Resp: 1892

Ion Ratio Lower Upper

252 100

253 50.8 0.0 46.0#

125 29.7 0.0 22.4#

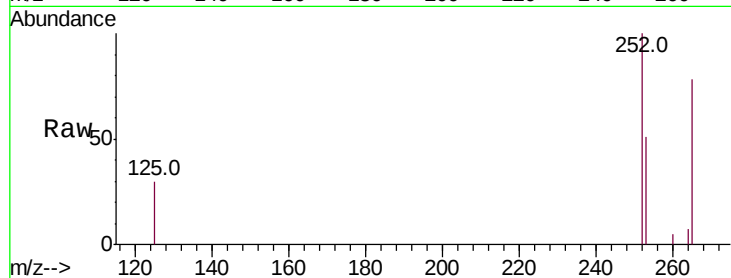

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

