

Data File : BN003719.D
Acq On : 05 Dec 2018 20:10
Operator : JU/SJ
Sample : J6170-05
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9M08

Quant Time: Dec 06 02:57:05 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 06 02:51:43 2018
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	5043	0.40	ng/ul	0.00
2) Naphthalene-d8	10.63	136	20885	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.47	164	11953	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.31	188	1865317	0.40	ng/ul	0.10
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.40
20) Perylene-d12	23.70	264	22209	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.22	152	10551	0.33	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
					Qvalue	
3) Naphthalene	10.68	128	1512	0.026	ng/ul#	86
5) 2-Methylnaphthalene	12.29	142	944	0.023	ng/ul	100
8) Acenaphthene	14.53	153	5987	0.127	ng/ul	100
9) Fluorene	15.52	166	2795	0.051	ng/ul	99
23) Benzo(a)pyrene	23.56	252	6779	0.085	ng/ul#	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BN003719.D
Acq On : 05 Dec 2018 20:10
Operator : JU/SJ
Sample : J6170-05
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9M08

Quant Time: Dec 06 02:57:05 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 06 02:51:43 2018
Response via : Initial Calibration

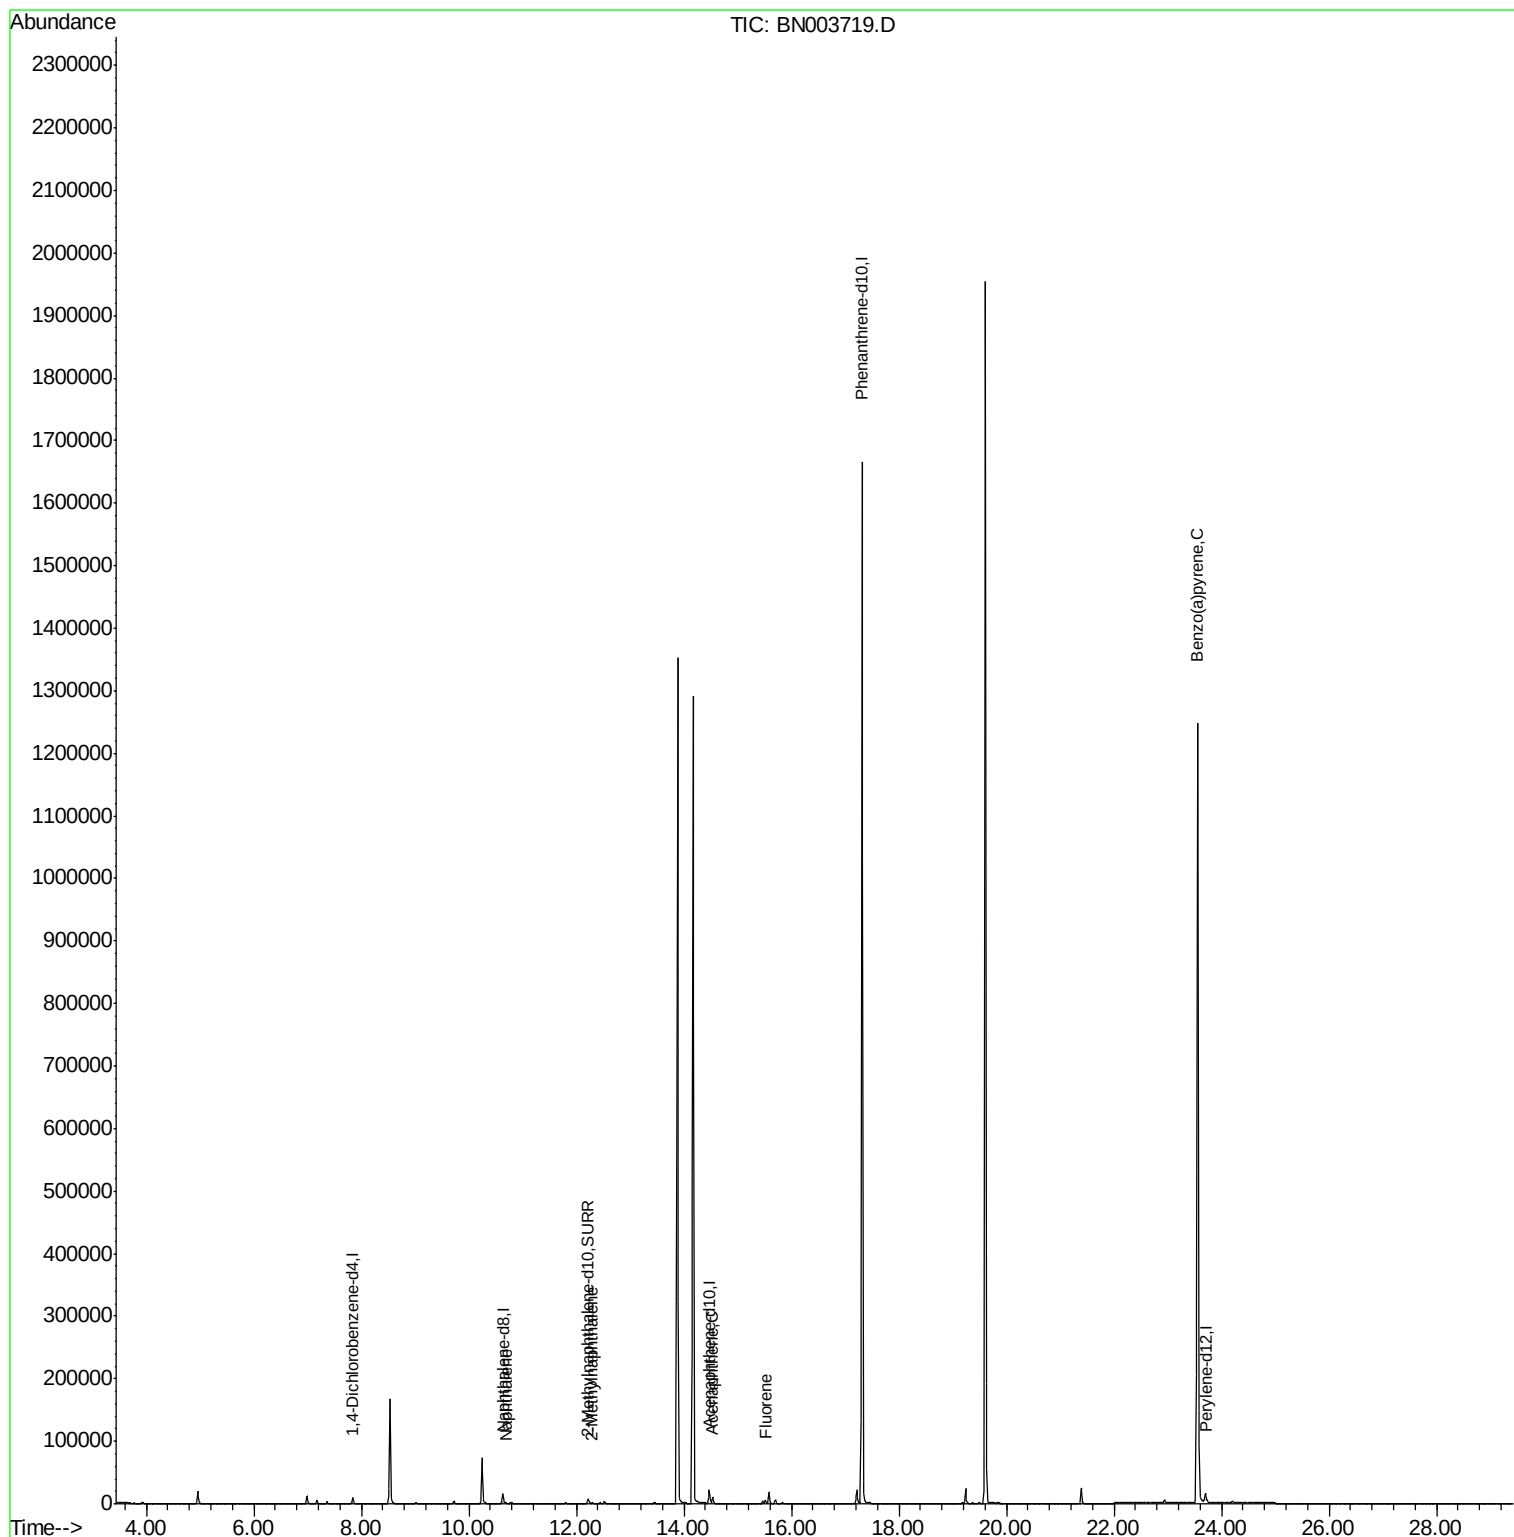

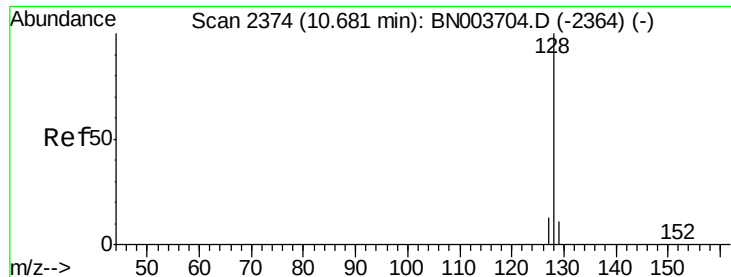

#3

Naphthalene

Concen: 0.026 ng/ul

RT: 10.68 min Scan# 2374

Delta R.T. 0.00 min

Lab File: BN003719.D

Acq: 05 Dec 2018 20:10

Instrument :

BNA_N

ClientSampleId :

F9M08


Tgt Ion:128 Resp: 1512

Ion Ratio Lower Upper

128 100

129 18.1 9.0 13.6#




127 17.4 10.5 15.7#

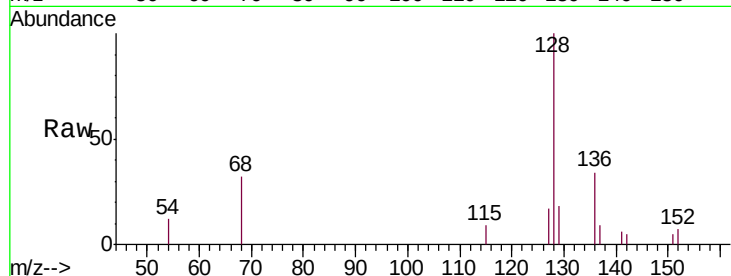

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

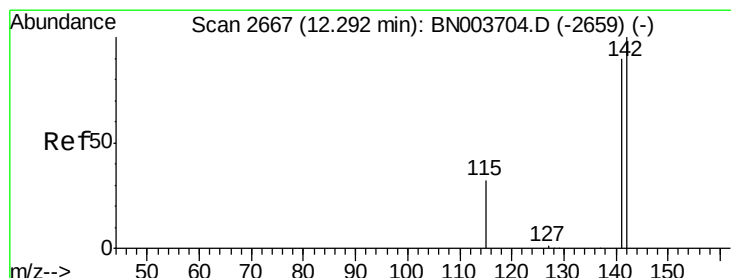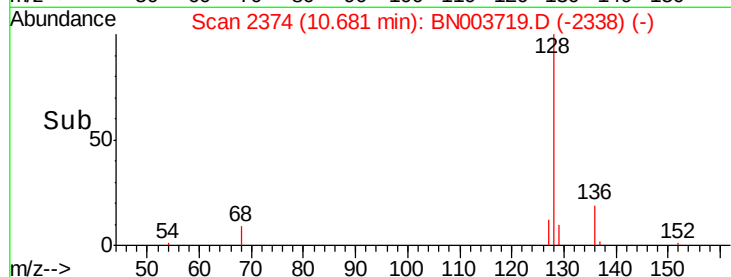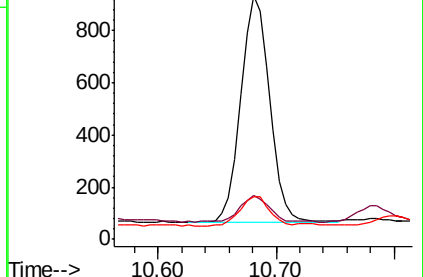

#5

2-Methylnaphthalene

Concen: 0.023 ng/ul

RT: 12.29 min Scan# 2667

Delta R.T. 0.00 min

Lab File: BN003719.D


Acq: 05 Dec 2018 20:10

Tgt Ion:142 Resp: 944

Ion Ratio Lower Upper



142 100


141 89.4 71.5 107.3

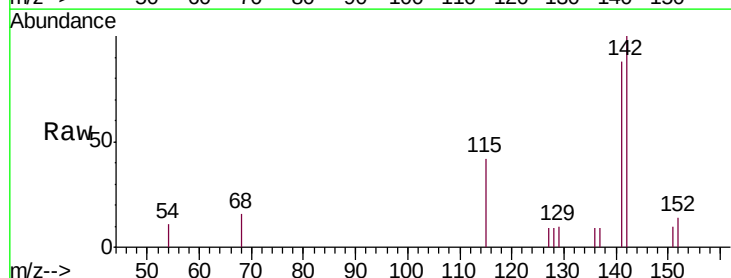

Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

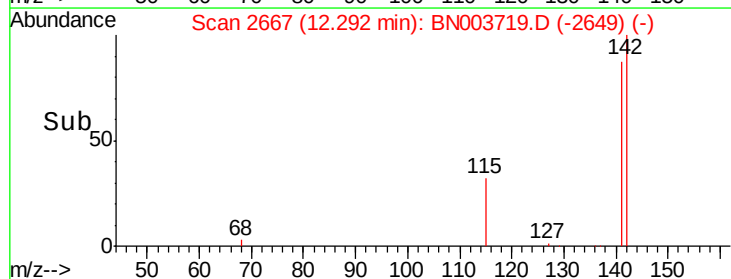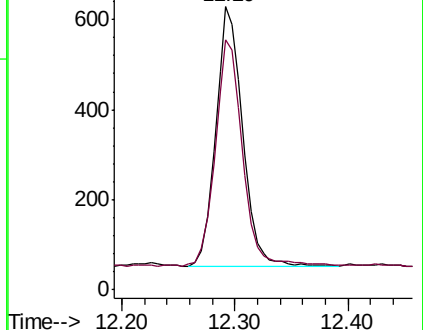

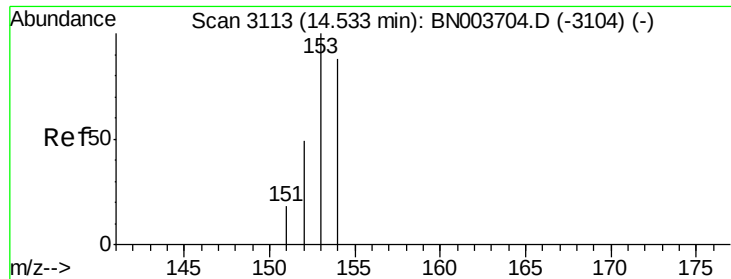

#8

Acenaphthene

Concen: 0.127 ng/ul

RT: 14.53 min Scan# 3113

Delta R.T. 0.00 min

Lab File: BN003719.D

Acq: 05 Dec 2018 20:10

Instrument :

BNA_N

ClientSampleId :

F9M08


Tgt Ion:153 Resp: 5987

Ion Ratio Lower Upper

153 100

152 49.1 39.3 58.9




154 88.3 70.3 105.5

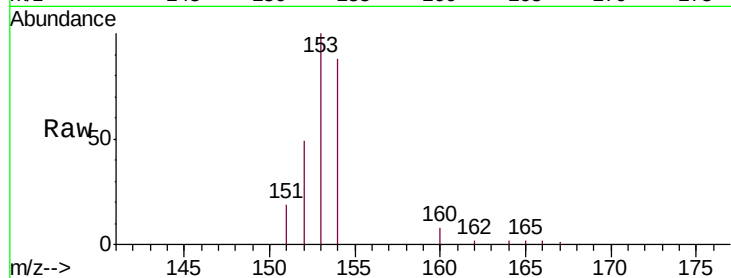

Abundance Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E

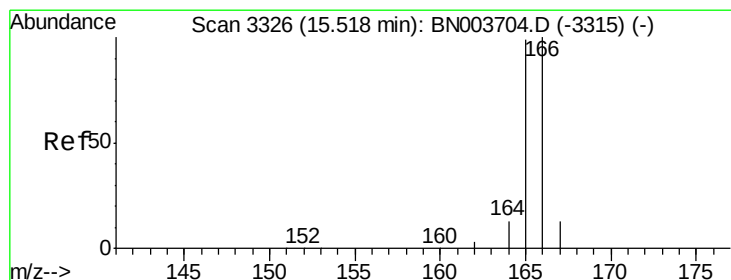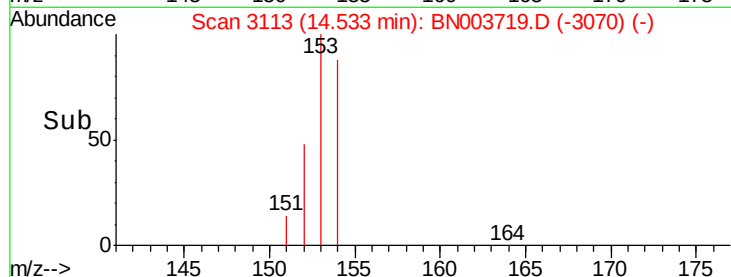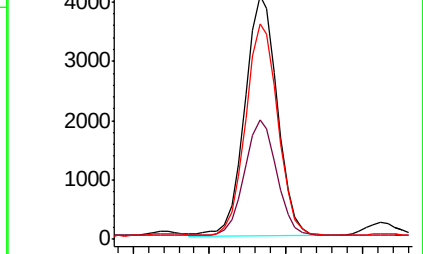

#9

Fluorene

Concen: 0.051 ng/ul

RT: 15.52 min Scan# 3326

Delta R.T. 0.00 min

Lab File: BN003719.D

Acq: 05 Dec 2018 20:10


Tgt Ion:166 Resp: 2795

Ion Ratio Lower Upper

166 100

165 98.7 78.3 117.5



167 16.4 11.3 16.9

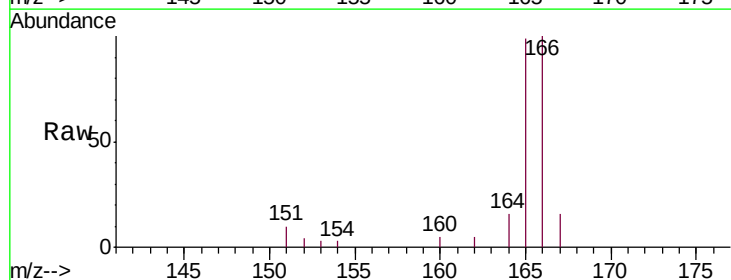


Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

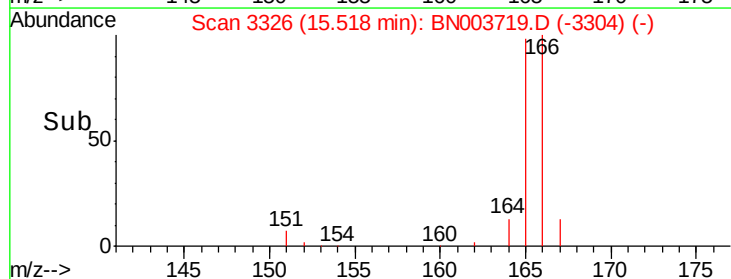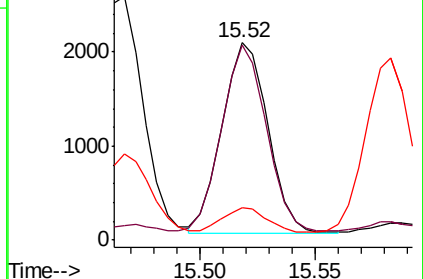

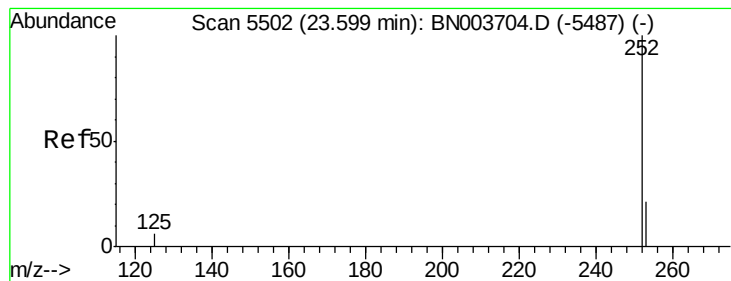

#23

Benzo(a)pyrene

Concen: 0.085 ng/ul

RT: 23.56 min Scan# 5487

Delta R.T. -0.05 min

Lab File: BN003719.D


Acq: 05 Dec 2018 20:10

Instrument :

BNA_N

ClientSampleId :

F9M08

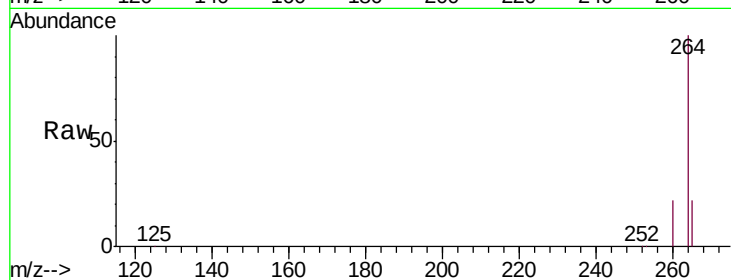

Tgt Ion: 252 Resp: 6779

Ion Ratio Lower Upper

252 100

253 36.7 19.0 28.4#

125 28.2 10.2 15.4#

