

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN120518\
Quantitation Report (Not Reviewed)

Data File : BN003720.D
Acq On : 05 Dec 2018 20:45
Operator : JU/SJ
Sample : J6170-06
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9M09

Quant Time: Dec 06 02:57:11 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 06 02:51:43 2018
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	5286	0.40	ng/ul	0.00
2) Naphthalene-d8	10.63	136	21663	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.47	164	11677	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.31	188	1258588	0.40	ng/ul	0.10
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.40
20) Perylene-d12	23.70	264	20245	0.40	ng/ul	-0.01
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.22	152	6948	0.21	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
23) Benzo(a)pyrene	23.55	252	4119	0.057	ng/ul#	Qvalue 47


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BN003720.D
Acq On : 05 Dec 2018 20:45
Operator : JU/SJ
Sample : J6170-06
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9M09

Quant Time: Dec 06 02:57:11 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 06 02:51:43 2018
Response via : Initial Calibration

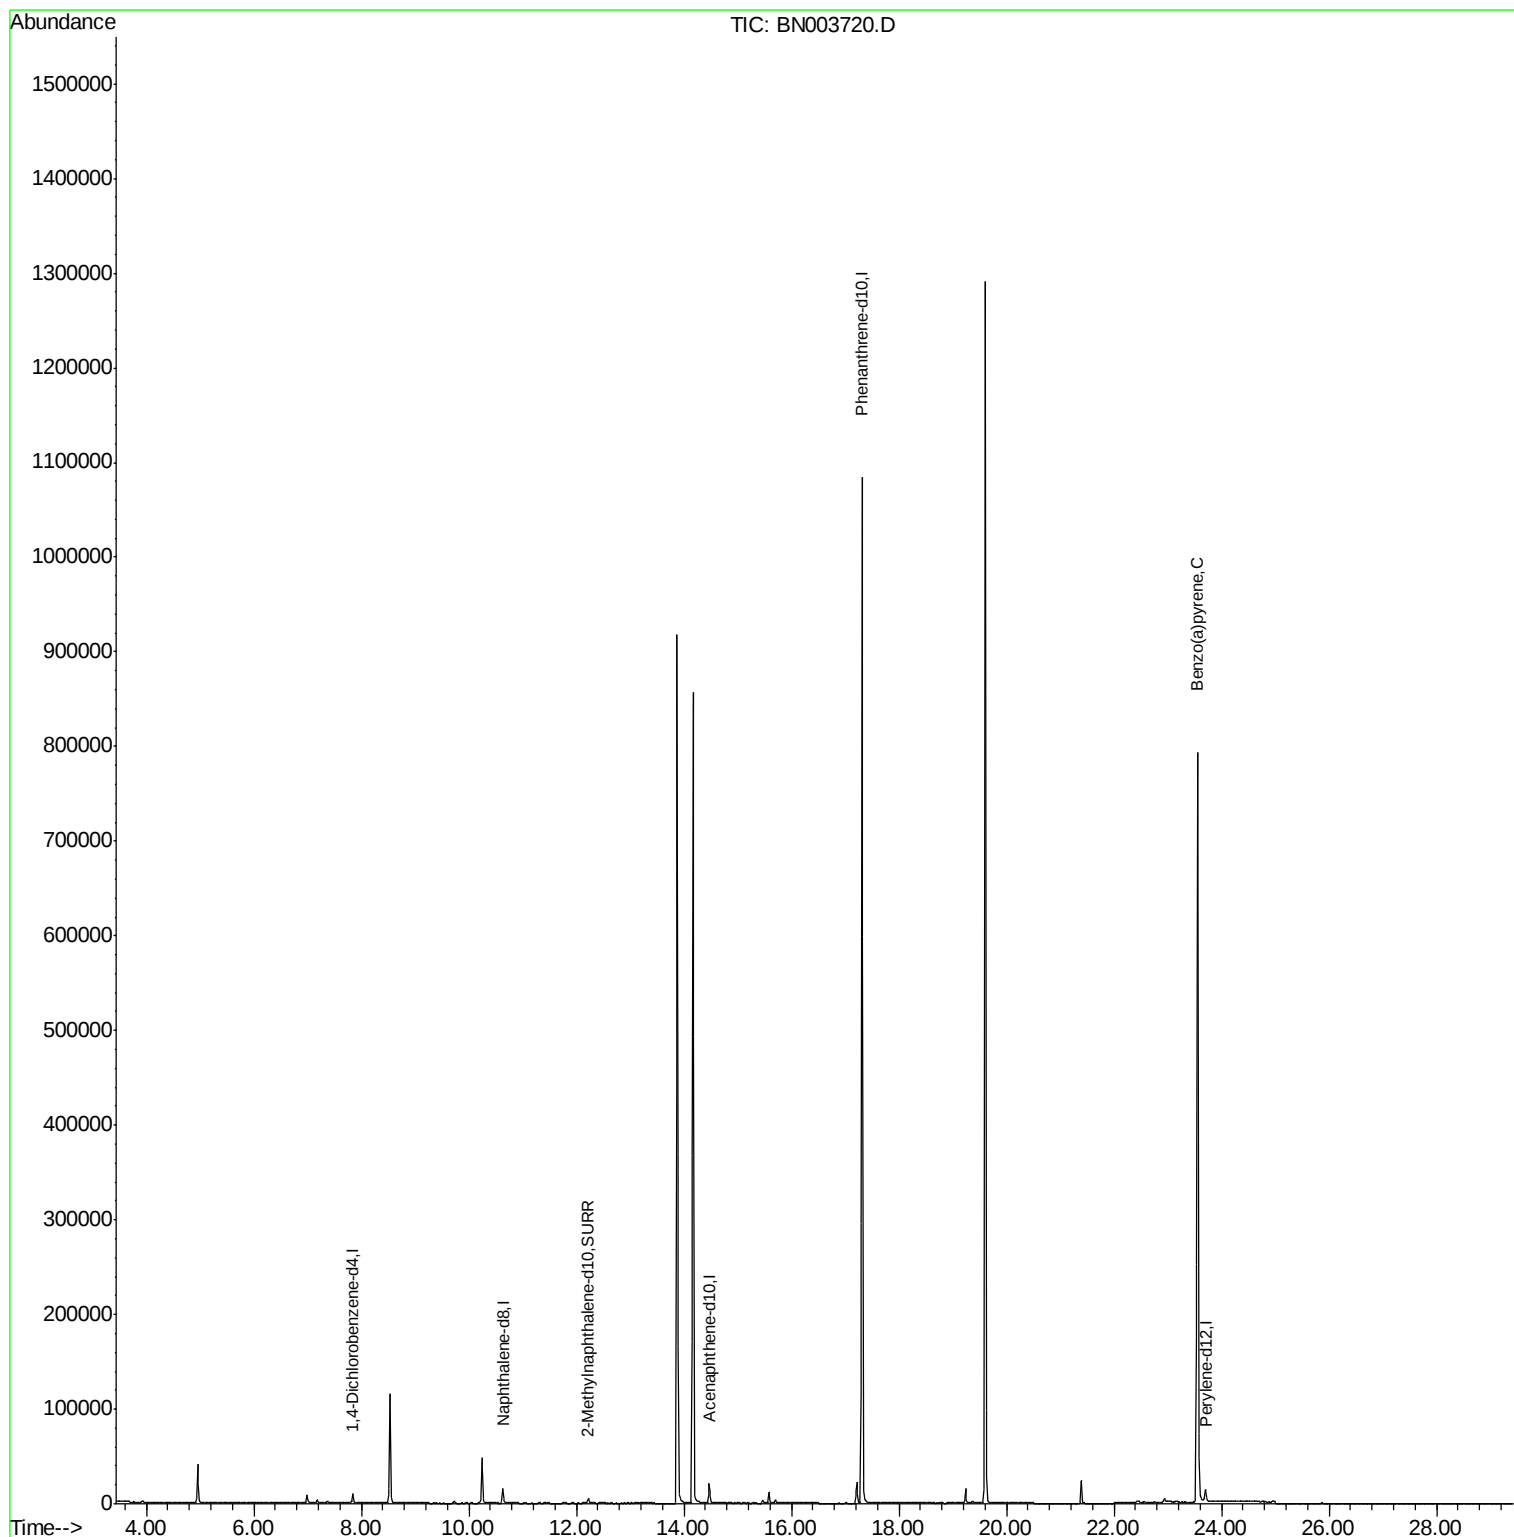

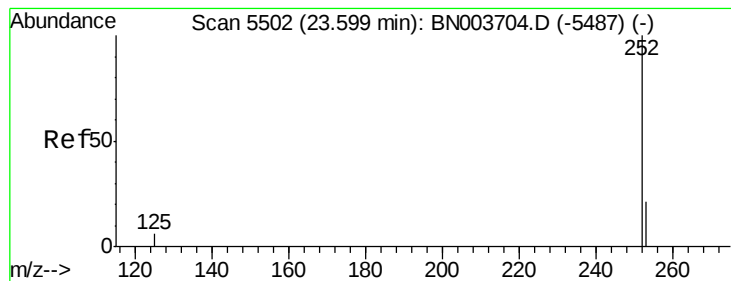

#23

Benzo(a)pyrene

Concen: 0.057 ng/ul

RT: 23.55 min Scan# 5486

Delta R.T. -0.05 min

Lab File: BN003720.D


Acq: 05 Dec 2018 20:45

Instrument :

BNA_N

ClientSampleId :

F9M09

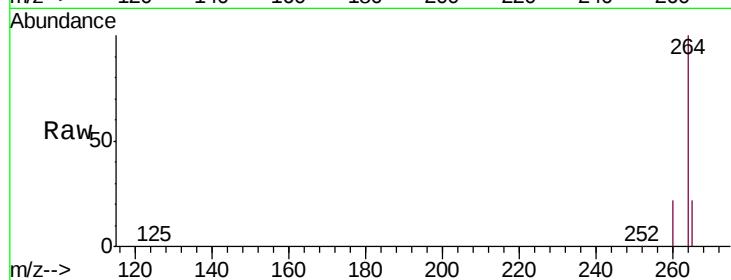


Tgt Ion: 252 Resp: 4119

Ion Ratio Lower Upper

252 100

253 45.5 19.0 28.4#

125 40.6 10.2 15.4#

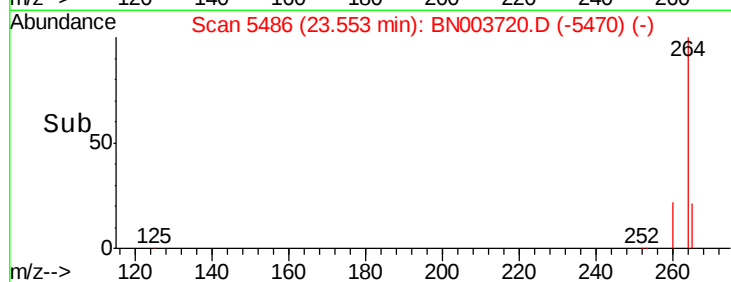

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

