

Data File : BN003722.D
Acq On : 05 Dec 2018 21:55
Operator : JU/SJ
Sample : J6170-08
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9J06

Quant Time: Dec 06 02:57:22 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 06 02:51:43 2018
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	5327	0.40	ng/ul	0.00
2) Naphthalene-d8	10.63	136	21821	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.47	164	12260	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.31	188	1943888	0.40	ng/ul	0.10
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.40
20) Perylene-d12	23.70	264	23187	0.40	ng/ul	-0.01
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.22	152	10938	0.33	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
3) Naphthalene	10.68	128	1928	0.031	ng/ul#	89
23) Benzo(a)pyrene	23.55	252	6659	0.080	ng/ul#	71


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BN003722.D
Acq On : 05 Dec 2018 21:55
Operator : JU/SJ
Sample : J6170-08
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9J06

Quant Time: Dec 06 02:57:22 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 06 02:51:43 2018
Response via : Initial Calibration

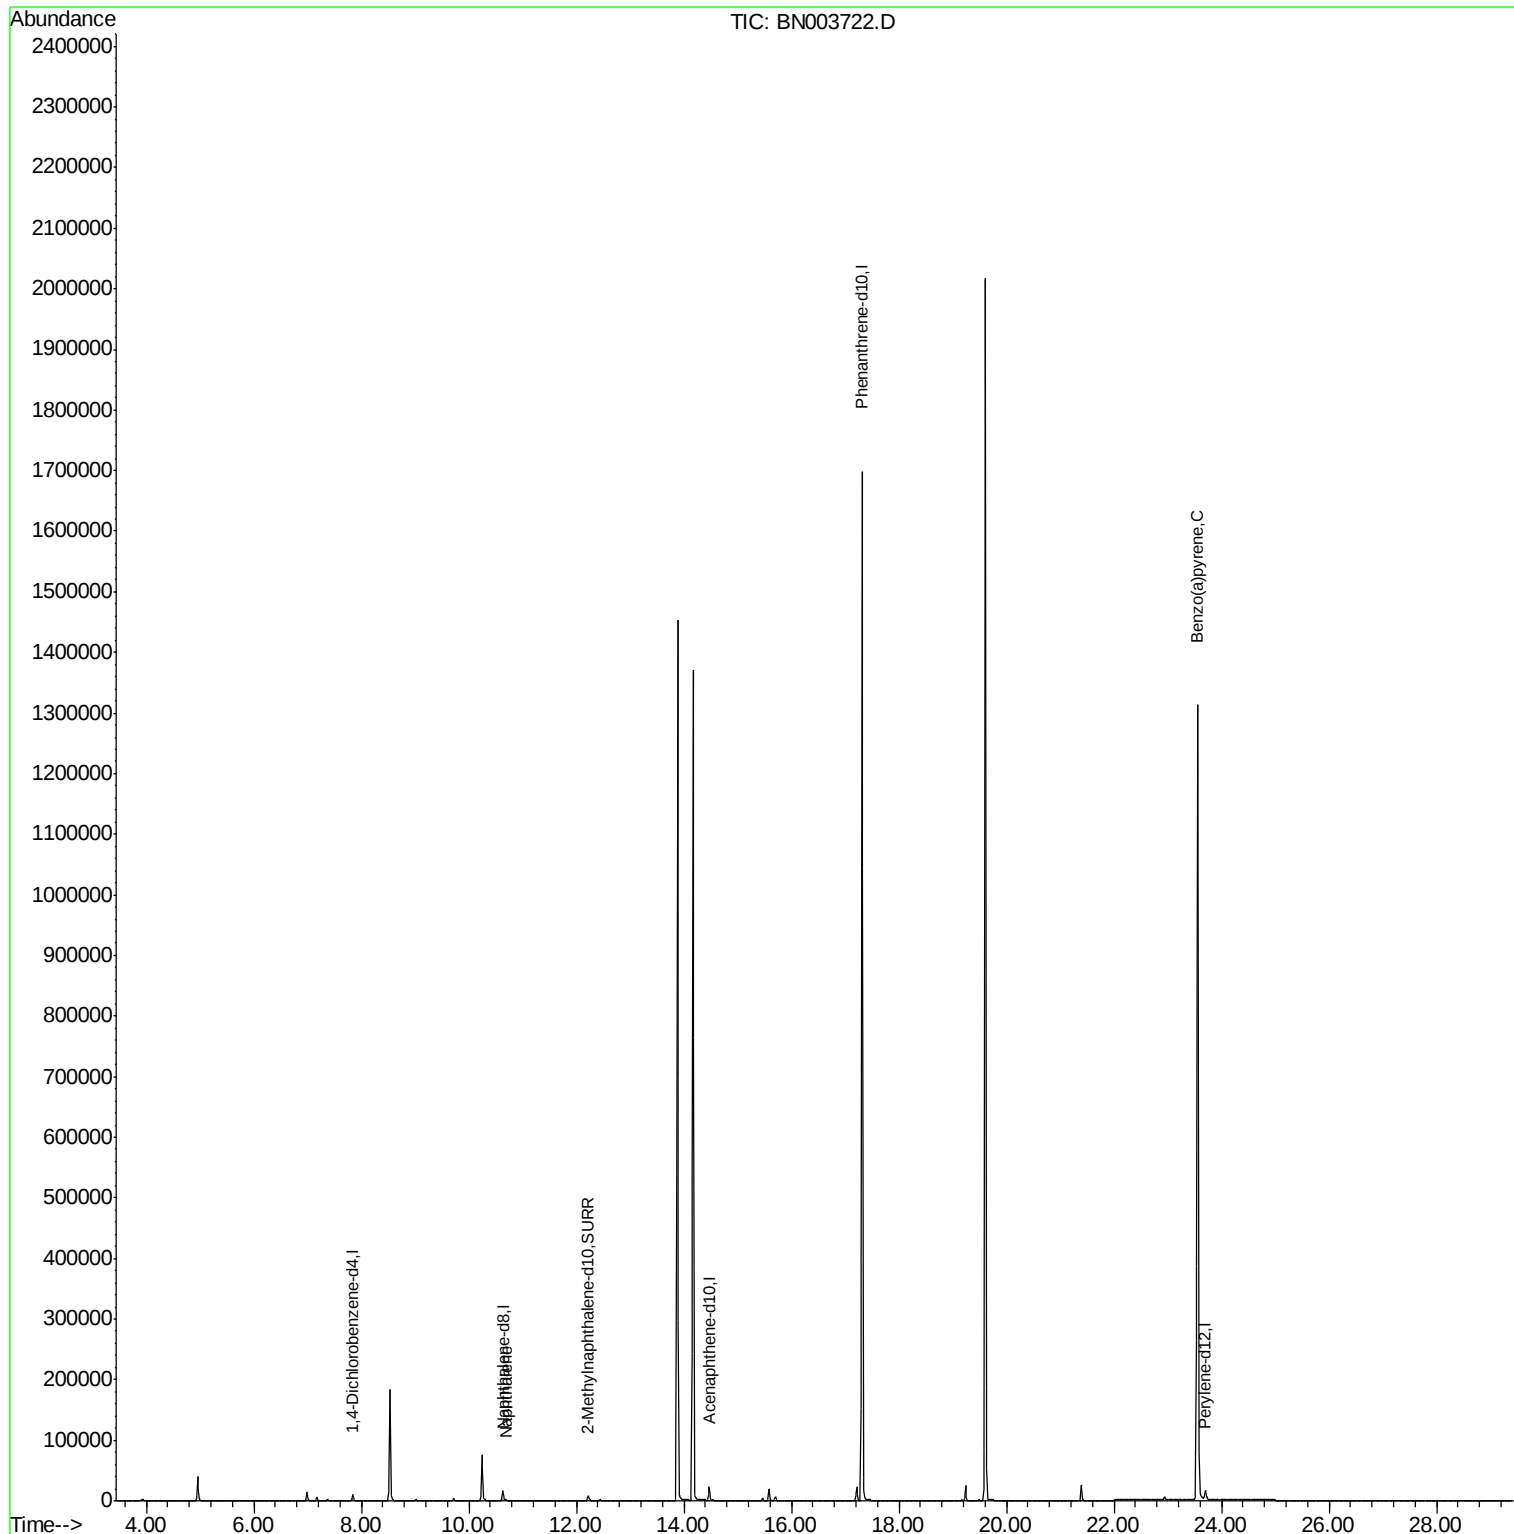

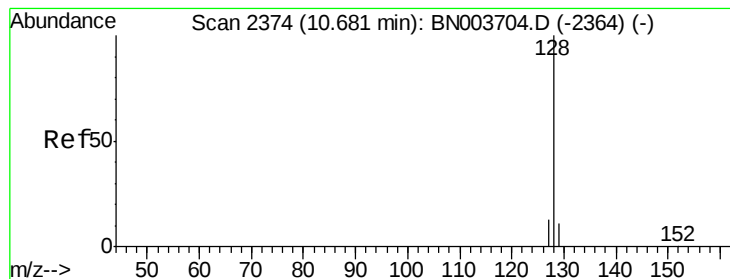

#3

Naphthalene

Concen: 0.031 ng/u1

RT: 10.68 min Scan# 2374

Delta R.T. 0.00 min

Lab File: BN003722.D

Acq: 05 Dec 2018 21:55

Instrument :

BNA_N

ClientSampleId :

F9J06


Tgt Ion:128 Resp: 1928

Ion Ratio Lower Upper

128 100

129 16.0 9.0 13.6#




127 16.8 10.5 15.7#

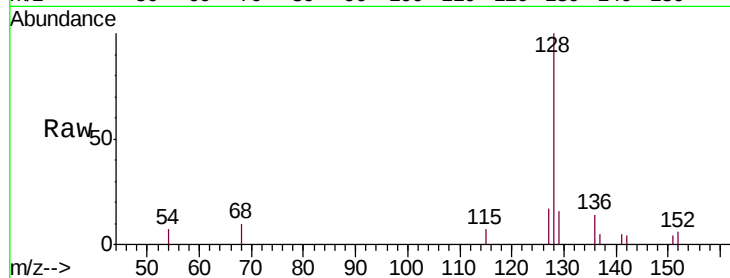

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

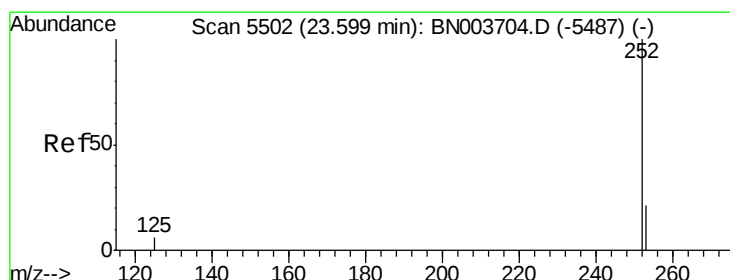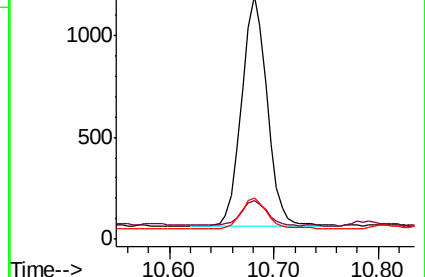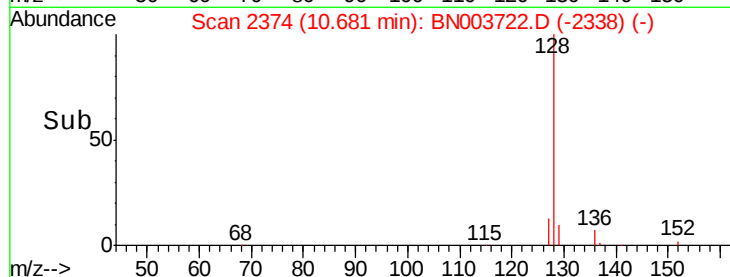

#23

Benzo(a)pyrene

Concen: 0.080 ng/u1

RT: 23.55 min Scan# 5486

Delta R.T. -0.05 min

Lab File: BN003722.D

Acq: 05 Dec 2018 21:55


Tgt Ion:252 Resp: 6659

Ion Ratio Lower Upper

252 100

253 36.1 19.0 28.4#

125 27.2 10.2 15.4#

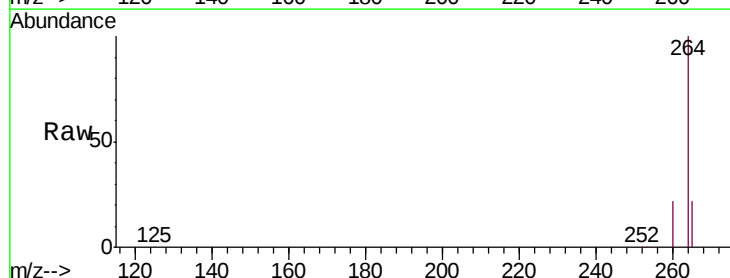

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

