


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN120519\
 Data File : BN008844.D
 Acq On : 05 Dec 2019 10:20
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN120419.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 04 15:42:09 2019

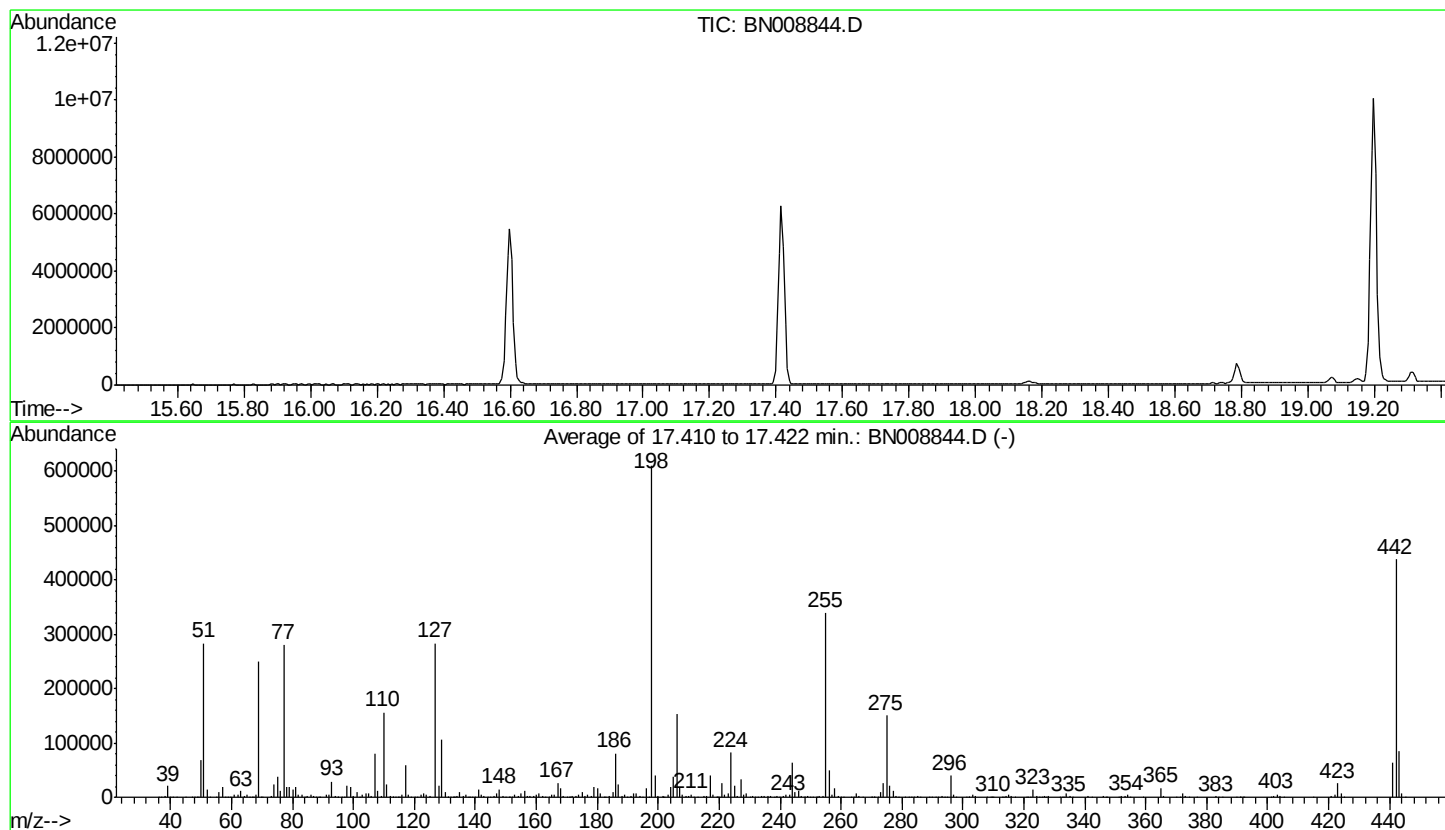

AutoFind: Scans 2452, 2453, 2454; Background Corrected with Scan 2445

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.5	283879	PASS
68	69	0.00	2	1.9	4851	PASS
69	198	0.00	100	41.1	250773	PASS
70	69	0.00	2	0.3	815	PASS
127	198	10	80	46.5	283989	PASS
197	198	0.00	2	0.2	1195	PASS
198	198	100	100	100.0	610432	PASS
199	198	5	9	6.7	40760	PASS
275	198	10	60	24.5	149853	PASS
365	198	1	100	2.9	17661	PASS
441	198	0.01	100	10.5	63840	PASS
442	198	50	100	71.7	437376	PASS
443	442	15	24	19.6	85629	PASS