


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120523\
Data File : BN029040.D
Acq On : 05 Dec 2023 18:16
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN120523.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Dec 06 00:49:47 2023

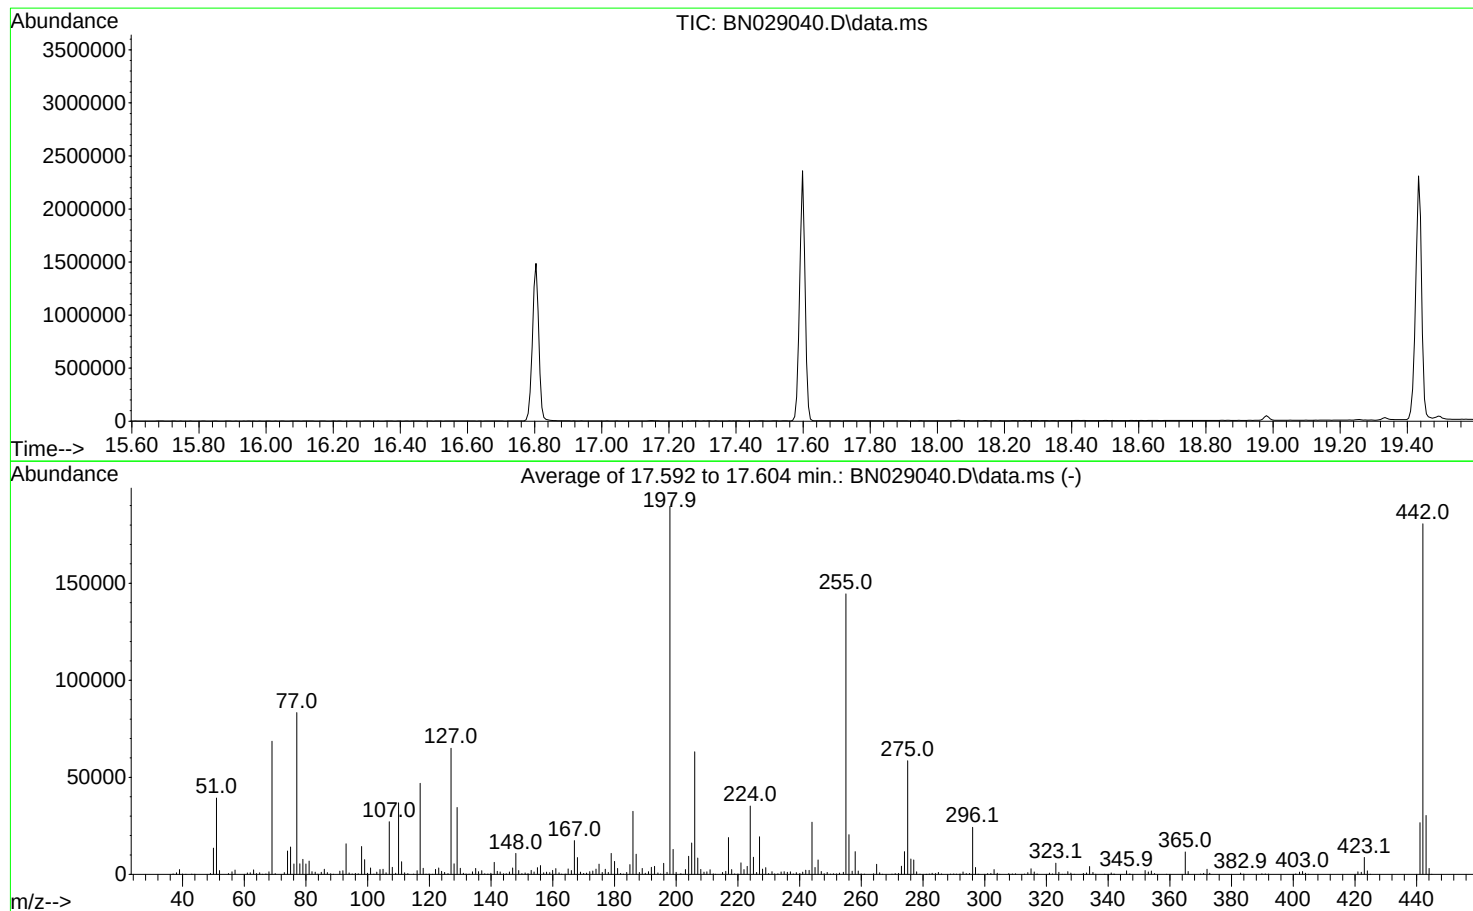




AutoFind: Scans 2466, 2467, 2468; Background Corrected with Scan 2459

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	20.8	39349	PASS
68	69	0.00	2	1.9	1335	PASS
69	198	0.00	100	36.2	68592	PASS
70	69	0.00	2	0.6	427	PASS
127	198	10	80	34.3	65013	PASS
197	198	0.00	2	0.6	1064	PASS
198	198	100	100	100.0	189547	PASS
199	198	5	9	6.8	12910	PASS
275	198	10	60	30.9	58525	PASS
365	198	1	100	6.1	11553	PASS
441	198	0.01	100	14.1	26669	PASS
442	442	50	100	100.0	180656	PASS
443	442	15	24	16.8	30373	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120523\
Data File : BN029040.D
Acq On : 05 Dec 2023 18:16
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 06 06:50:16 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 01 23:28:24 2023
Response via : Initial Calibration

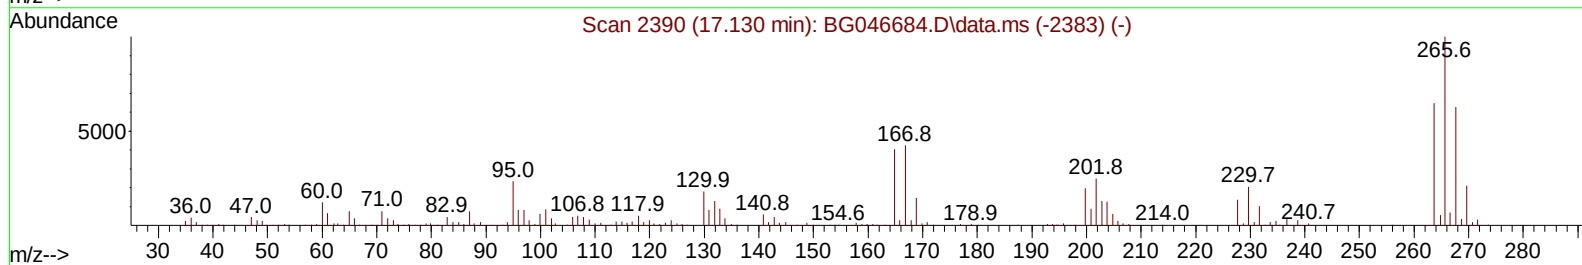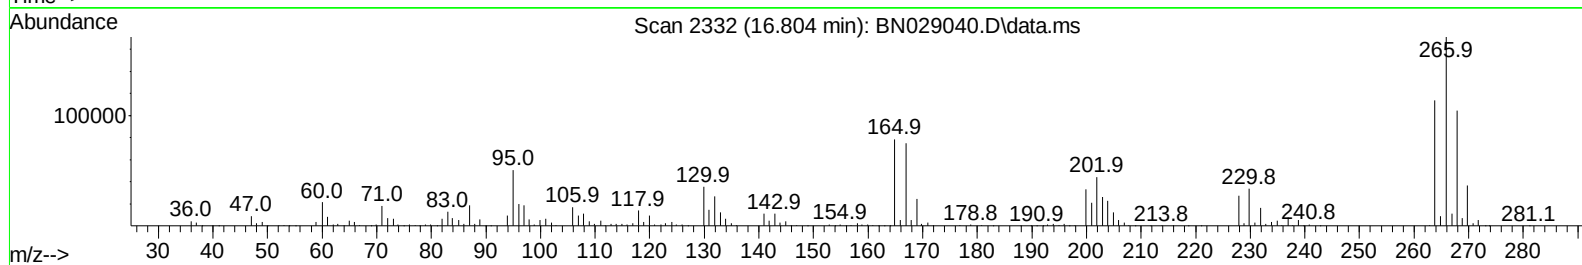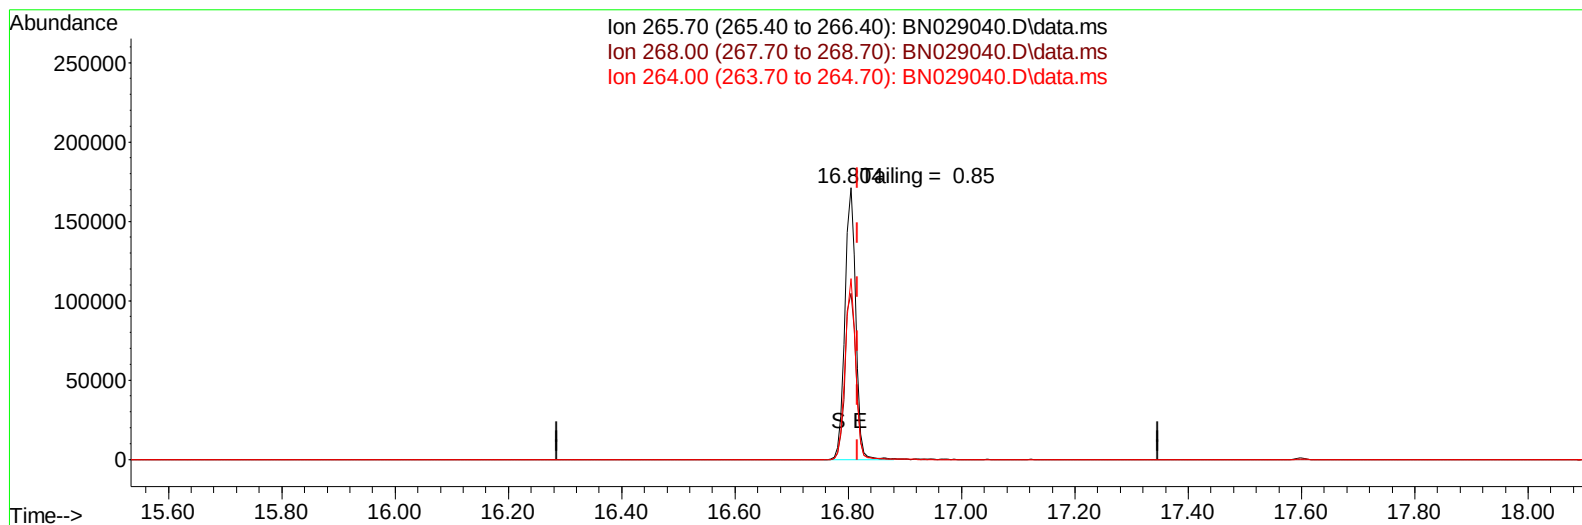

TIC: BN029040.D\data.ms

(70) Pentachlorophenol (C)

16.804min (-0.012) 22783.04 ng




response 223852

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.19
264.00	61.60	66.52
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120523\
Data File : BN029040.D
Acq On : 05 Dec 2023 18:16
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 06 06:50:16 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 01 23:28:24 2023
Response via : Initial Calibration

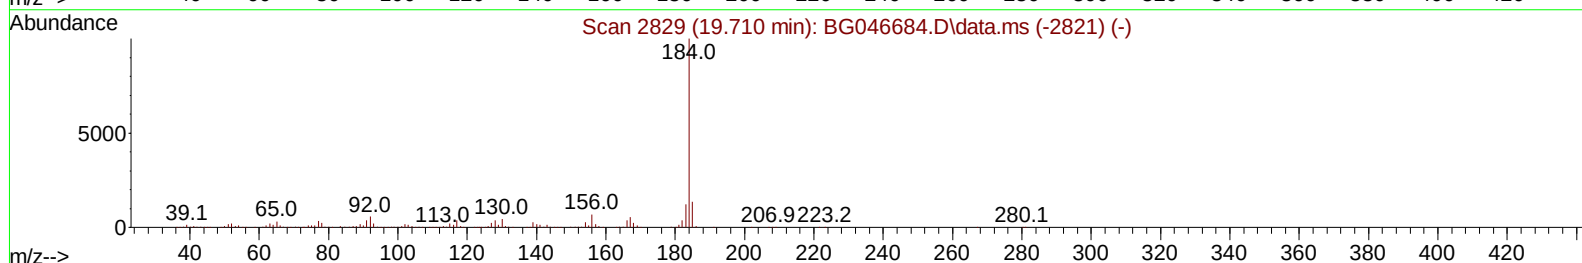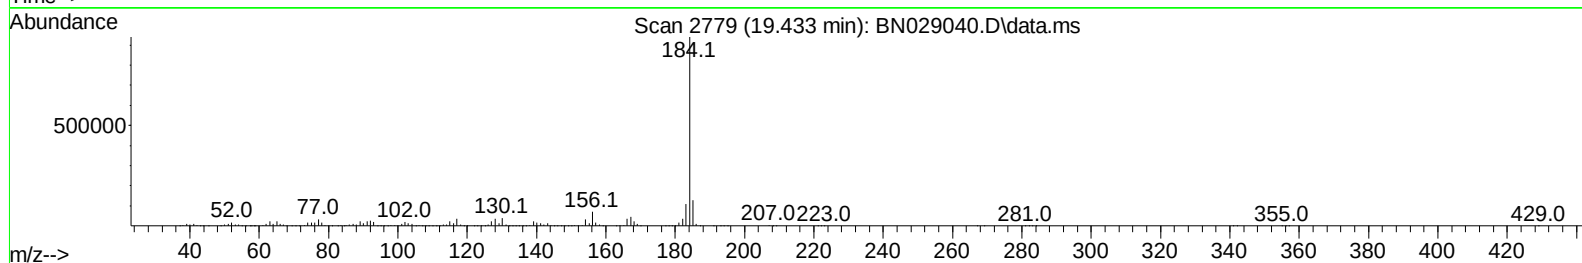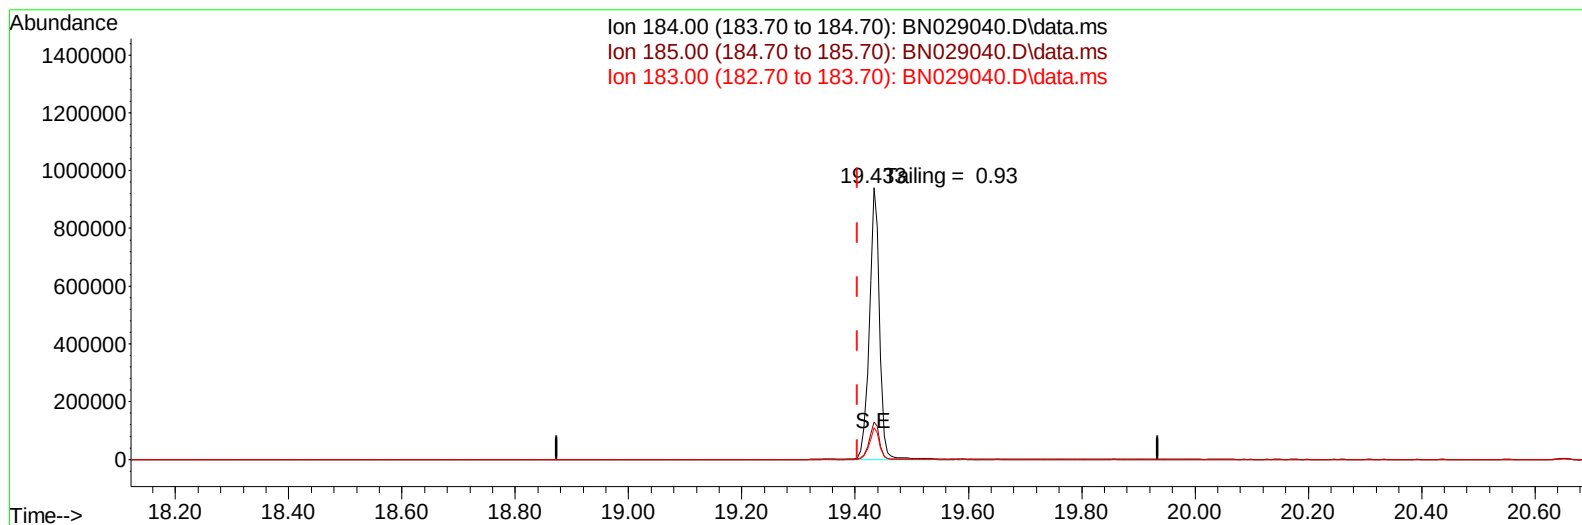

TIC: BN029040.D\data.ms

(77) Benzidine

19.433min (+ 0.029) 0.00 ng

response 1195395

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.71
183.00	13.20	11.66
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/5/2023	BNA_N	<u>BN029040.D</u>
Compound Name	Response	Retention Time
DDT	653382	20.651
DDD	27811	20.21
DDE	344	19.698
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
28155	681537	4.13

Instrument :
BNA_N
ClientSampleId :
DFTPP