

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120525\
 Data File : BN038280.D
 Acq On : 05 Dec 2025 18:08
 Operator : RC/JU
 Sample : Q3688-23DL 10X
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 M-28SDL

Quant Time: Dec 05 22:29:08 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN112625.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 01 16:36:13 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.762	152	7234	0.400	ng/u1	0.00
4) Naphthalene-d8	10.562	136	21968	0.400	ng/u1	-0.01
9) Acenaphthene-d10	14.428	164	10876	0.400	ng/u1	0.00
13) Phenanthrene-d10	17.179	188	15599	0.400	ng/u1	0.00
17) Chrysene-d12	21.368	240	10726	0.400	ng/u1	0.00
23) Perylene-d12	23.671	264	12870	0.400	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.214	96	1974	0.260	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.162	152	1097	0.035	ng/u1	-0.01
18) Fluoranthene-d10	19.211	212	1389	0.033	ng/u1	0.00
Target Compounds						
2) 1,4-Dioxane	3.247	88	16553	2.024	ng/u1	Qvalue 91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120525\
Data File : BN038280.D
Acq On : 05 Dec 2025 18:08
Operator : RC/JU
Sample : Q3688-23DL 10X
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
M-28SDL


Quant Time: Dec 05 22:29:08 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN112625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 01 16:36:13 2025
Response via : Initial Calibration

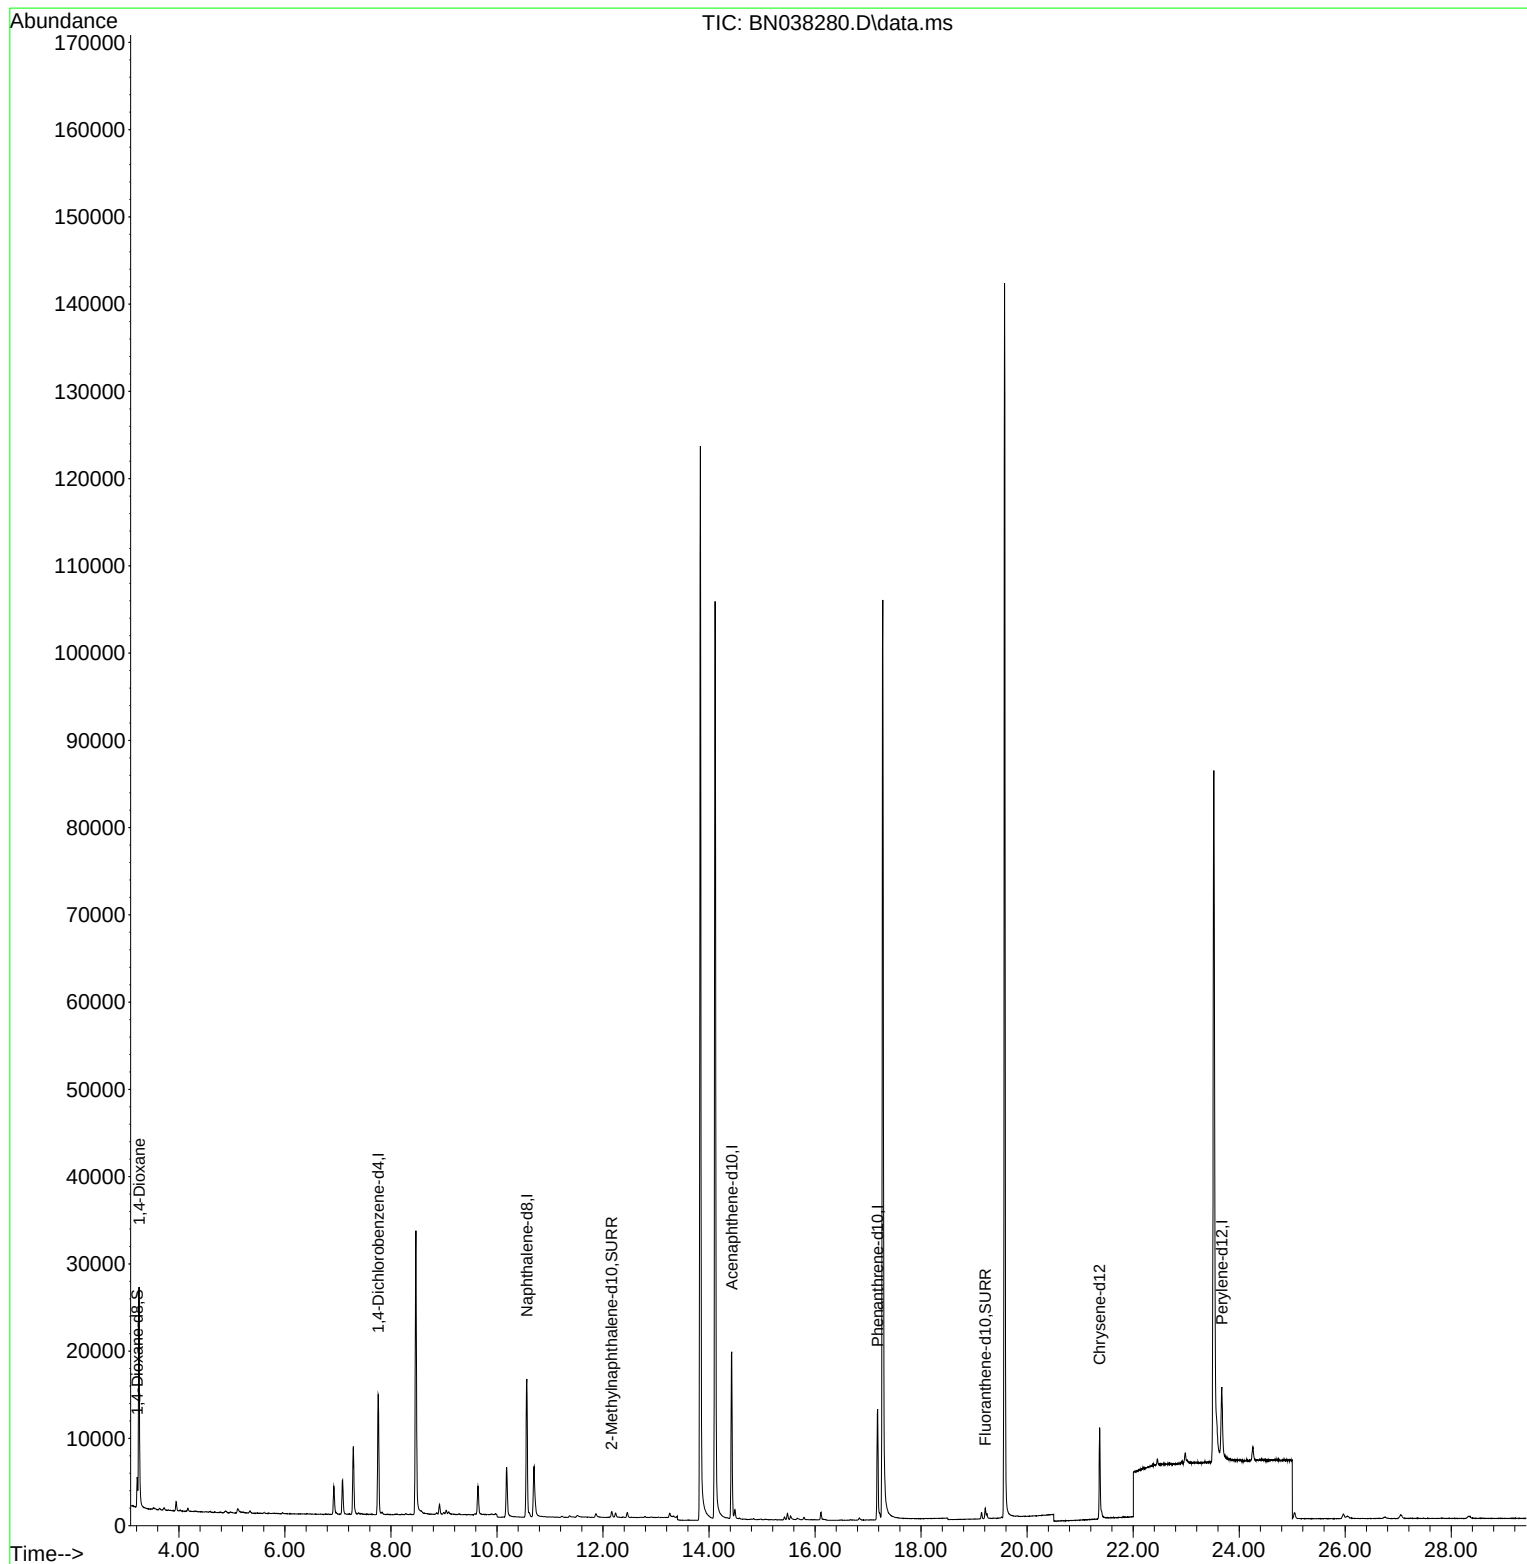

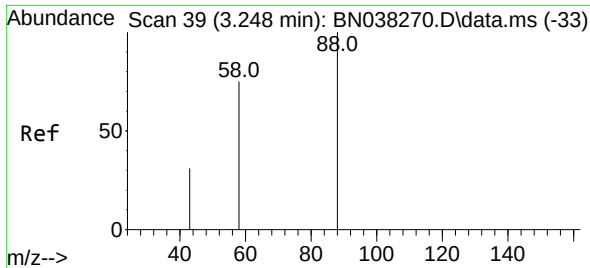

#2
 1,4-Dioxane
 Concen: 2.024 ng/ul
 RT: 3.247 min Scan# 39
 Delta R.T. -0.004 min
 Lab File: BN038280.D
 Acq: 05 Dec 2025 18:08

Instrument :
 BNA_N
 ClientSampleId :
 M-28SDL

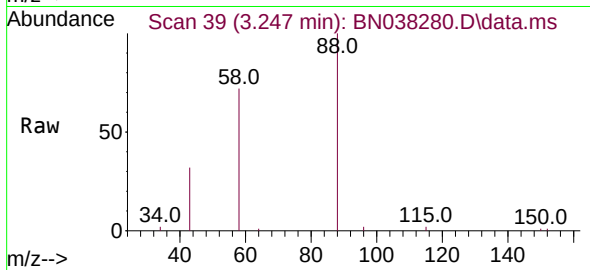

Tgt Ion:	88	Resp:	16553
Ion	Ratio	Lower	Upper
88	100		
43	31.9	27.5	41.3
58	72.2	50.5	75.7

