

Data File : BN003738.D
Acq On : 06 Dec 2018 19:24
Operator : JU/SJ
Sample : J6077-08
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9Y40

Quant Time: Dec 07 03:20:29 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 07 03:02:08 2018
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	5361	0.40	ng/ul	0.00
2) Naphthalene-d8	10.63	136	22328	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.47	164	12428	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.31	188	1814065	0.40	ng/ul	0.10
16) Chrysene-d12	21.53	240	114	0.40	ng/ul	0.13
20) Perylene-d12	0.00	264	0	0.00	ng/ul	-23.71
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.22	152	10340	0.30	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
17) Pyrene	19.61	202	3646	8.917	ng/ul#	1
18) Benzo(a)anthracene	21.54	228	21	0.058	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BN003738.D
Acq On : 06 Dec 2018 19:24
Operator : JU/SJ
Sample : J6077-08
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9Y40

Quant Time: Dec 07 03:20:29 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 07 03:02:08 2018
Response via : Initial Calibration




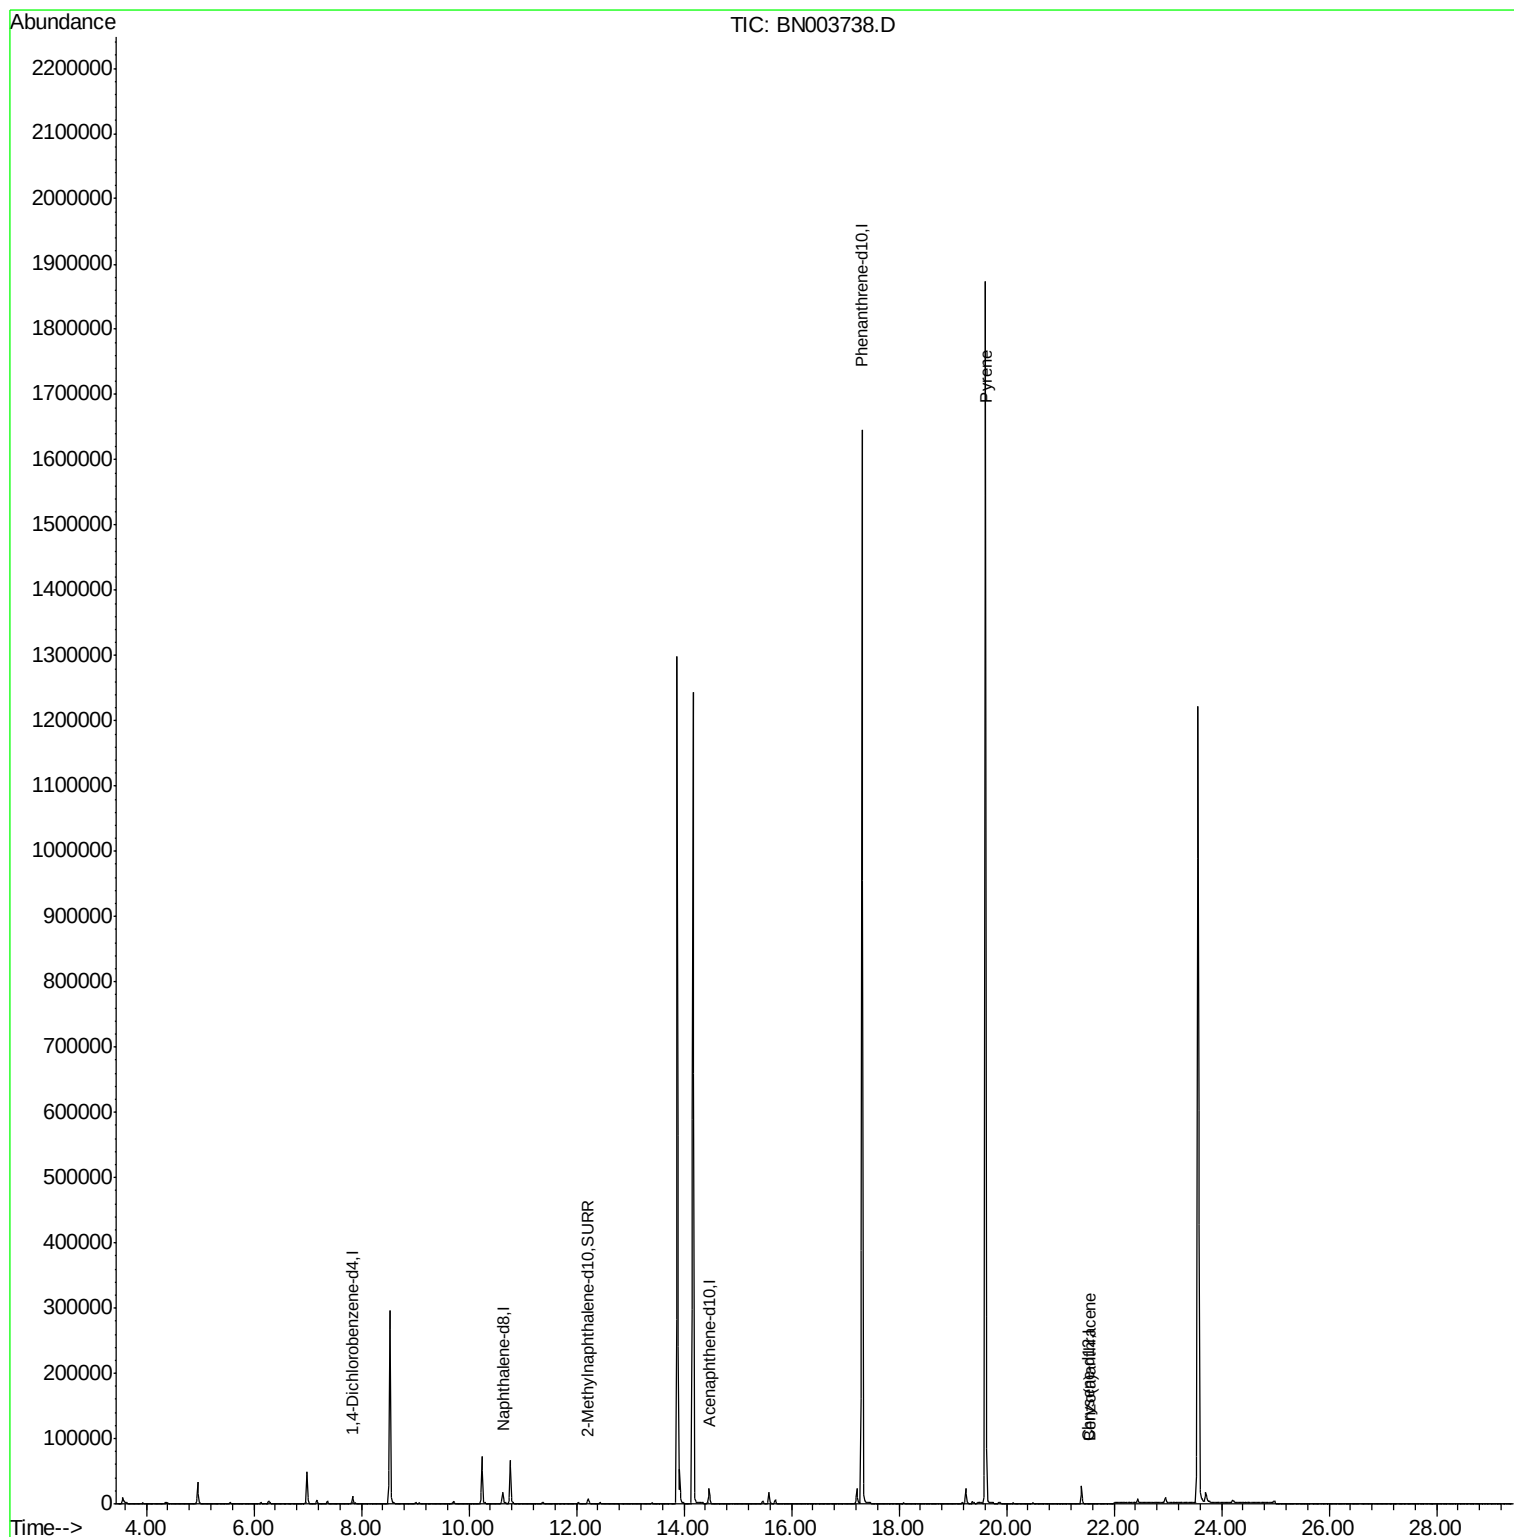


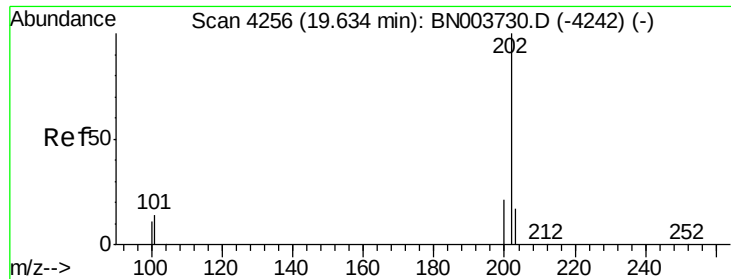

#17
 Pyrene
 Concen: 8.917 ng/ul
 RT: 19.61 min Scan# 4251
 Delta R.T. -0.02 min
 Lab File: BN003738.D
 Acq: 06 Dec 2018 19:24

Instrument :
 BNA_N
 ClientSampleId :
 F9Y40

Tgt Ion:202 Resp: 3646
 Ion Ratio Lower Upper
 202 100
 101 135.2 10.3 15.5#
 100 832.0 8.5 12.7#

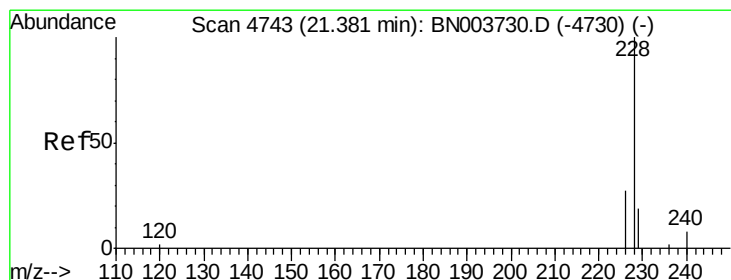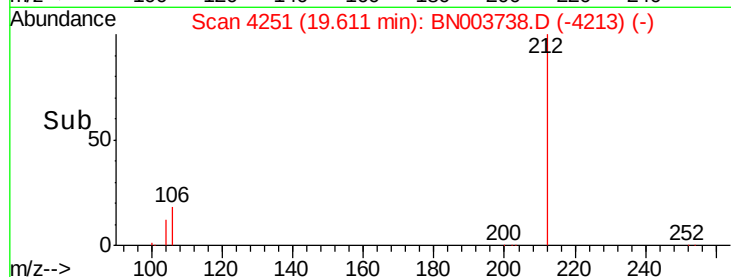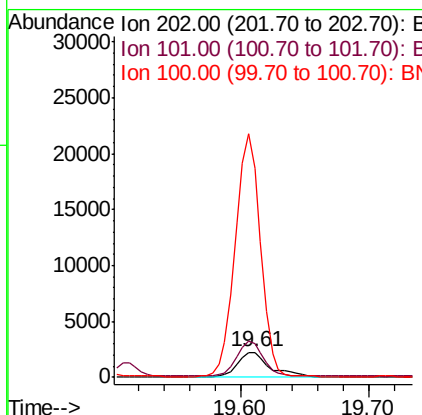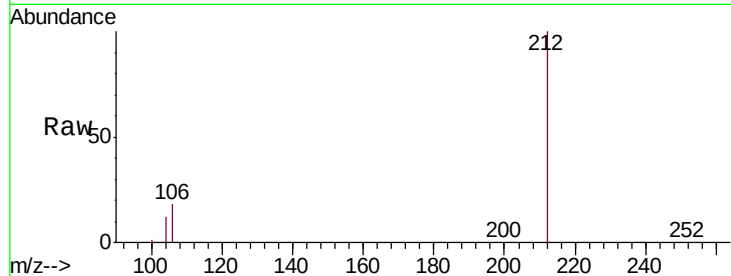

#18
 Benzo(a)anthracene
 Concen: 0.058 ng/ul
 RT: 21.54 min Scan# 4799
 Delta R.T. 0.16 min
 Lab File: BN003738.D
 Acq: 06 Dec 2018 19:24

Tgt Ion:228 Resp: 21
 Ion Ratio Lower Upper
 228 100
 229 108.6 15.6 23.4#
 226 104.3 21.1 31.7#

