

Data File : BN003746.D
Acq On : 07 Dec 2018 01:15
Operator : JU/SJ
Sample : J6227-06
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E75

Quant Time: Dec 07 04:12:35 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 07 04:08:50 2018
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	5576	0.40	ng/ul	0.00
2) Naphthalene-d8	10.63	136	23102	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.47	164	12525	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.31	188	914872	0.40	ng/ul	0.09
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.40
20) Perylene-d12	23.70	264	21171	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.22	152	5518	0.16	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
21) Benzo(b)fluoranthene	23.01	252	3381	0.039	ng/ul#	35
22) Benzo(k)fluoranthene	23.01	252	3381	0.040	ng/ul#	36


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BN003746.D
Acq On : 07 Dec 2018 01:15
Operator : JU/SJ
Sample : J6227-06
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E75

Quant Time: Dec 07 04:12:35 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 07 04:08:50 2018
Response via : Initial Calibration

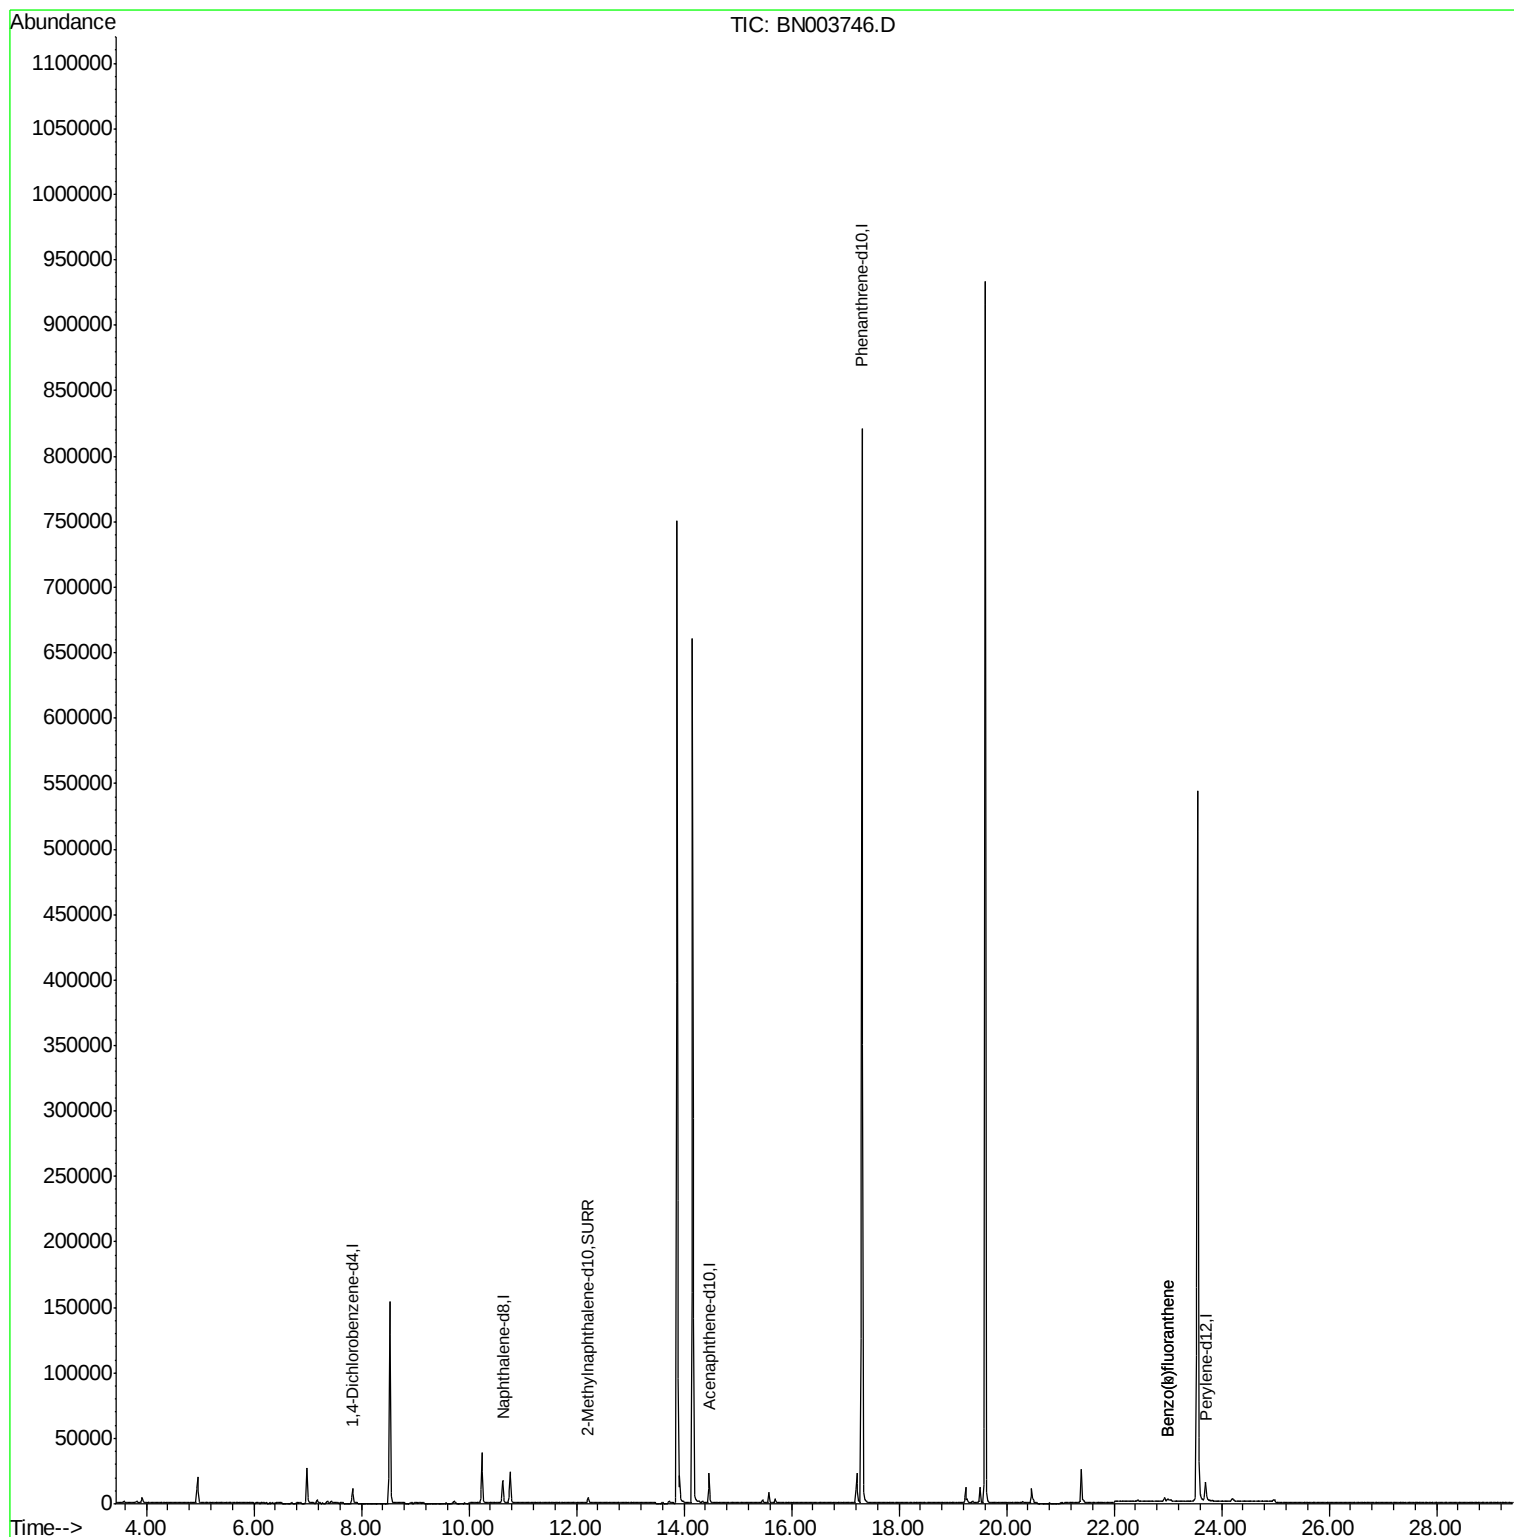

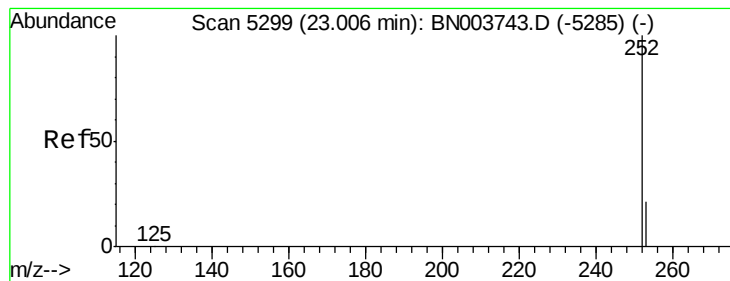

#21

Benzo(b)fluoranthene

Concen: 0.039 ng/ul

RT: 23.01 min Scan# 5299

Delta R.T. -0.00 min

Lab File: BN003746.D

Acq: 07 Dec 2018 01:15

Instrument :

BNA_N

ClientSampleId :

F9E75


Tgt Ion:252 Resp: 3381

Ion Ratio Lower Upper

252 100

253 54.4 0.0 46.0#




125 35.9 0.0 22.4#

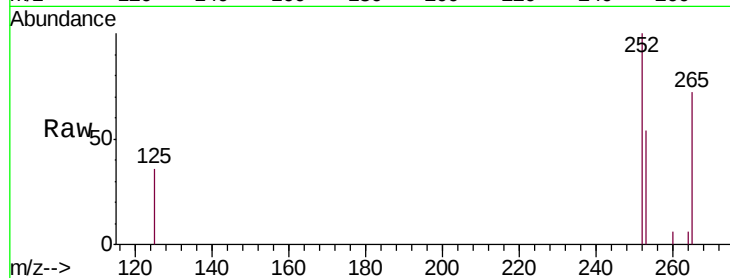

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

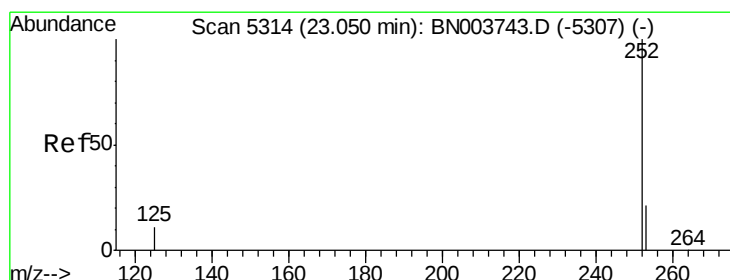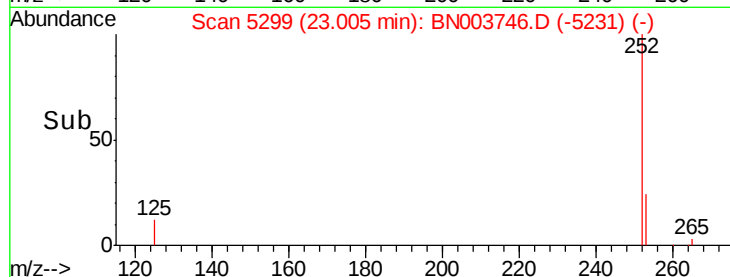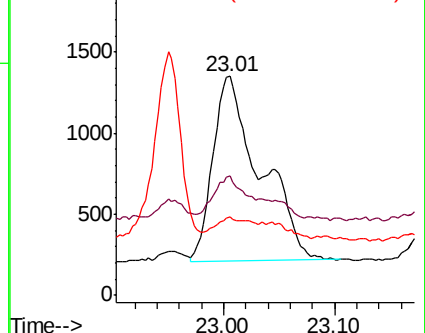

#22

Benzo(k)fluoranthene

Concen: 0.040 ng/ul

RT: 23.01 min Scan# 5299

Delta R.T. -0.04 min

Lab File: BN003746.D

Acq: 07 Dec 2018 01:15


Tgt Ion:252 Resp: 3381

Ion Ratio Lower Upper

252 100

253 54.4 18.5 27.7#

125 35.9 9.0 13.6#

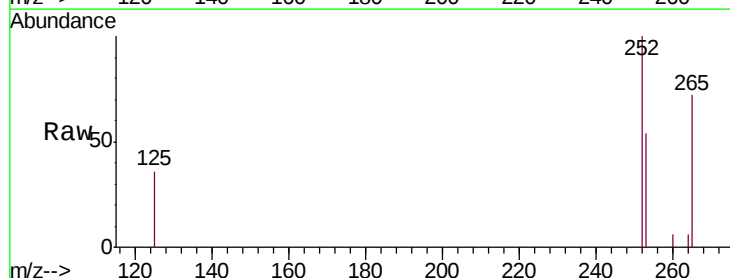

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

