

Data File : BN003748.D
Acq On : 07 Dec 2018 02:25
Operator : JU/SJ
Sample : J6227-09
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E54

Quant Time: Dec 07 04:12:46 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 07 04:08:50 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	5417	0.40	ng/ul	0.00
2) Naphthalene-d8	10.63	136	22528	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.47	164	12125	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.31	188	969392	0.40	ng/ul	0.09
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.40
20) Perylene-d12	23.70	264	21402	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.21	152	5879	0.17	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
21) Benzo(b)fluoranthene	23.00	252	2194	0.025	ng/ul#	24
22) Benzo(k)fluoranthene	23.00	252	2194	0.025	ng/ul#	24

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BN003748.D

Acq On : 07 Dec 2018 02:25

Operator : JU/SJ

Sample : J6227-09

Misc :

ALS Vial : 19 Sample Multiplier: 1

Instrument :

BNA_N

ClientSampleId :

F9E54


Quant Time: Dec 07 04:12:46 2018


Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN11918.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Fri Dec 07 04:08:50 2018

Response via : Initial Calibration

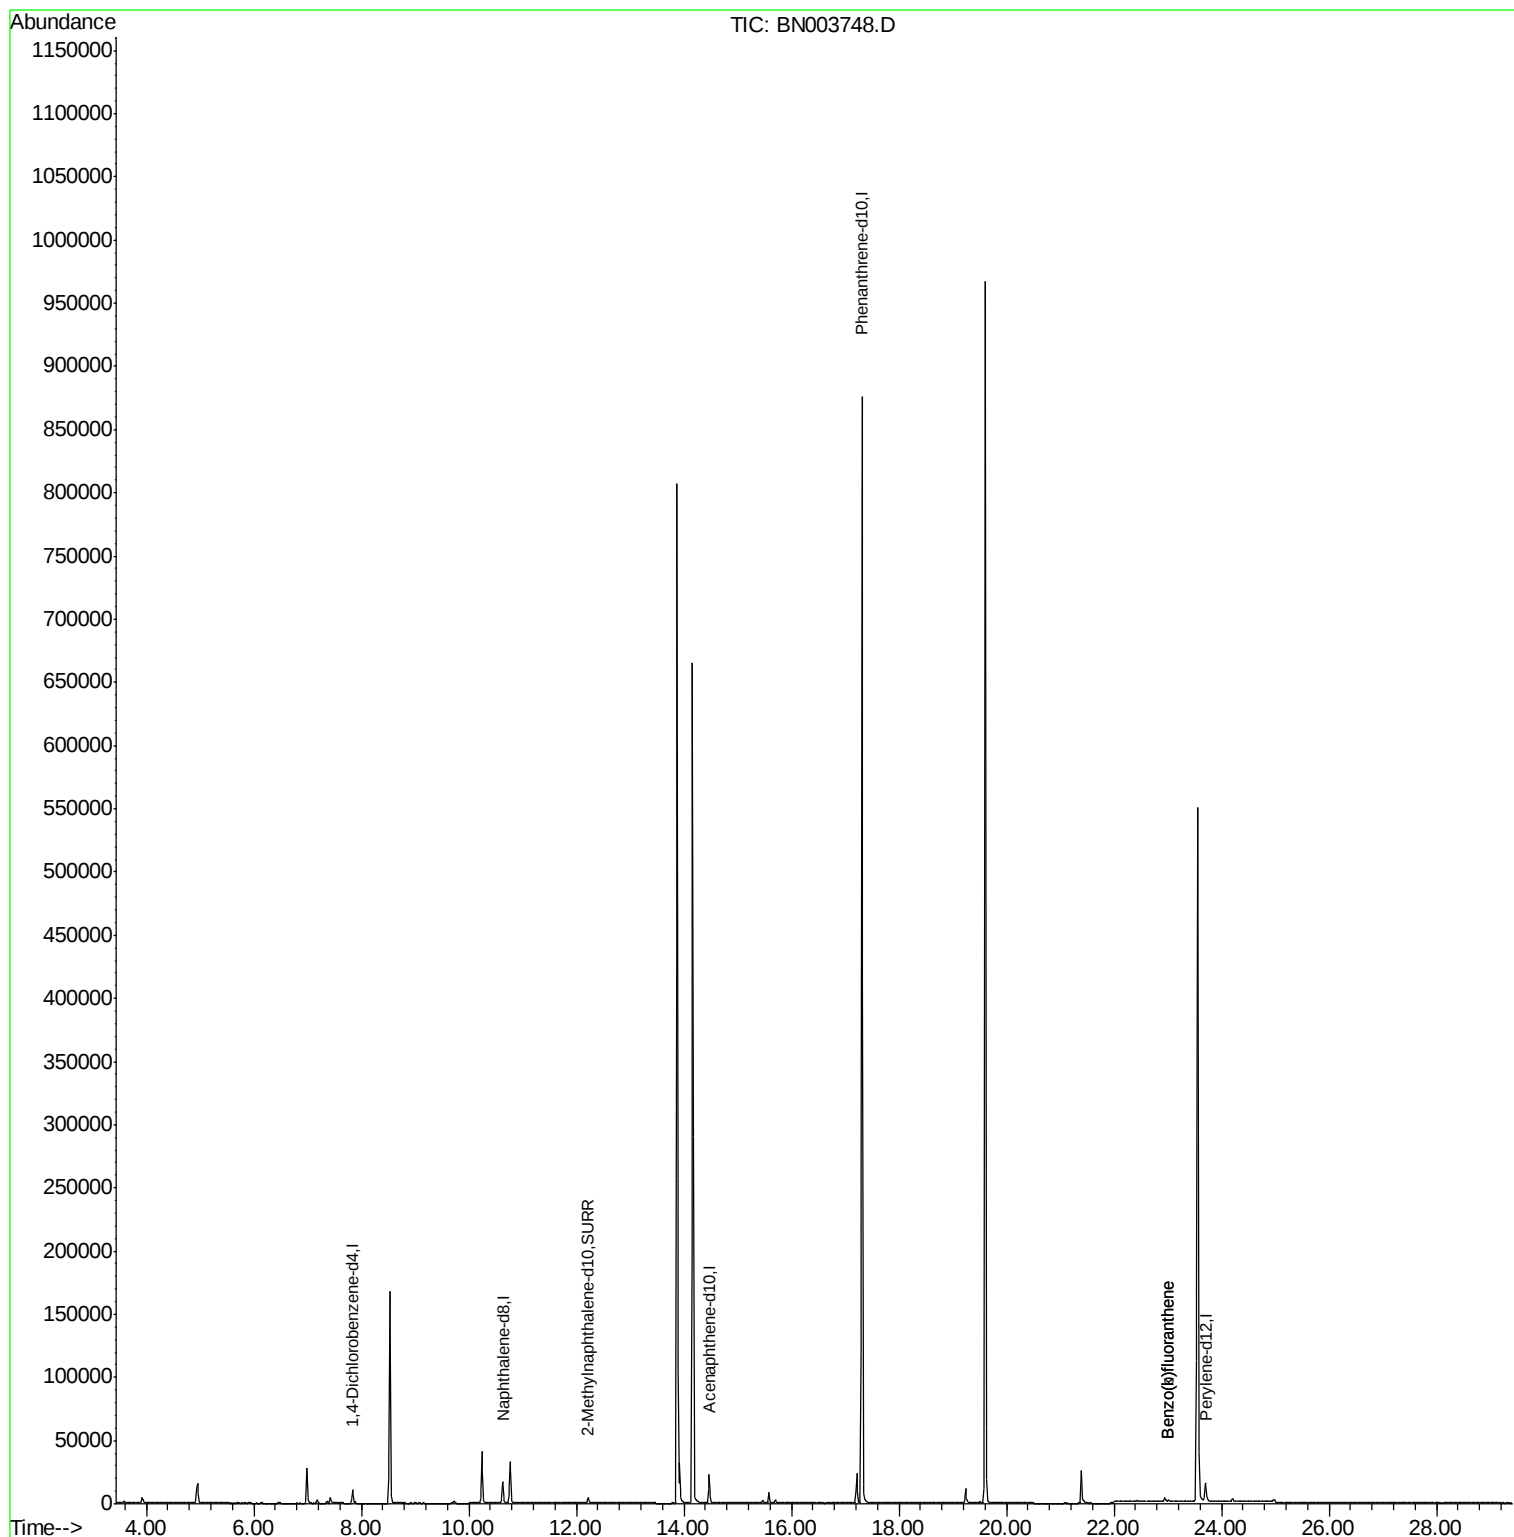

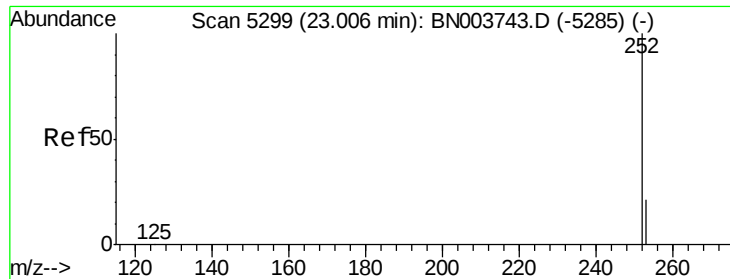

#21

Benzo(b)fluoranthene

Concen: 0.025 ng/ul

RT: 23.00 min Scan# 5298

Delta R.T. -0.00 min

Lab File: BN003748.D

Acq: 07 Dec 2018 02:25

Instrument :

BNA_N

ClientSampleId :

F9E54





Tgt Ion:252 Resp: 2194

Ion Ratio Lower Upper

252 100

253 60.8 0.0 46.0#

125 38.8 0.0 22.4#

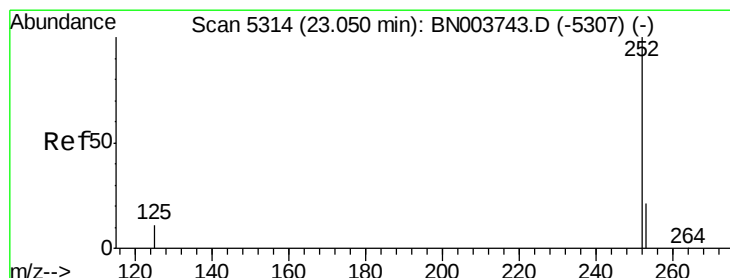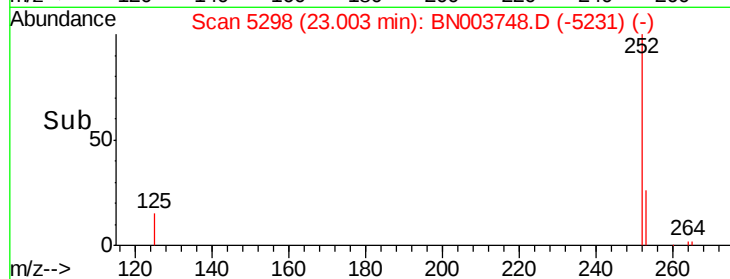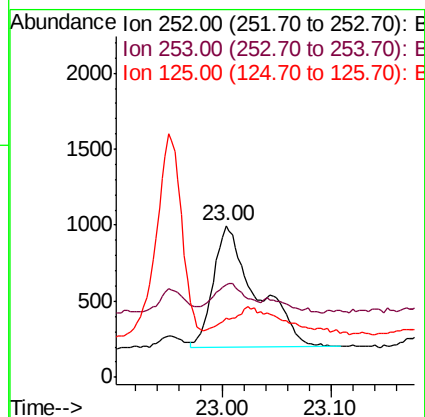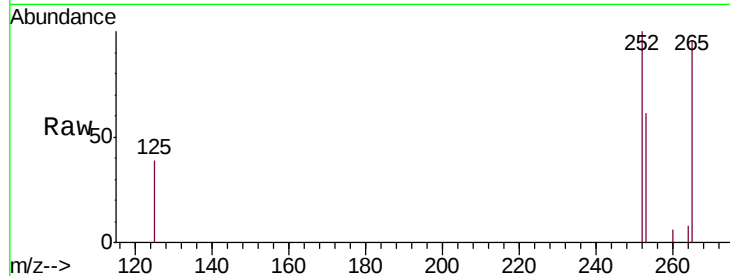

#22

Benzo(k)fluoranthene

Concen: 0.025 ng/ul

RT: 23.00 min Scan# 5298

Delta R.T. -0.05 min

Lab File: BN003748.D

Acq: 07 Dec 2018 02:25

Tgt Ion:252 Resp: 2194

Ion Ratio Lower Upper

252 100

253 60.8 18.5 27.7#

125 38.8 9.0 13.6#

