

Data File : BN003752.D
Acq On : 07 Dec 2018 04:44
Operator : JU/SJ
Sample : J6227-13
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E60

Quant Time: Dec 07 06:06:40 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 07 04:08:50 2018
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	5726	0.40	ng/ul	0.00
2) Naphthalene-d8	10.63	136	23662	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.47	164	12654	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.31	188	996884	0.40	ng/ul	0.09
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.40
20) Perylene-d12	23.70	264	20826	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.22	152	5921	0.16	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
21) Benzo(b)fluoranthene	23.01	252	2440	0.028	ng/ul#	10
22) Benzo(k)fluoranthene	23.01	252	2440	0.029	ng/ul#	11


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BN003752.D
Acq On : 07 Dec 2018 04:44
Operator : JU/SJ
Sample : J6227-13
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E60

Quant Time: Dec 07 06:06:40 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 07 04:08:50 2018
Response via : Initial Calibration

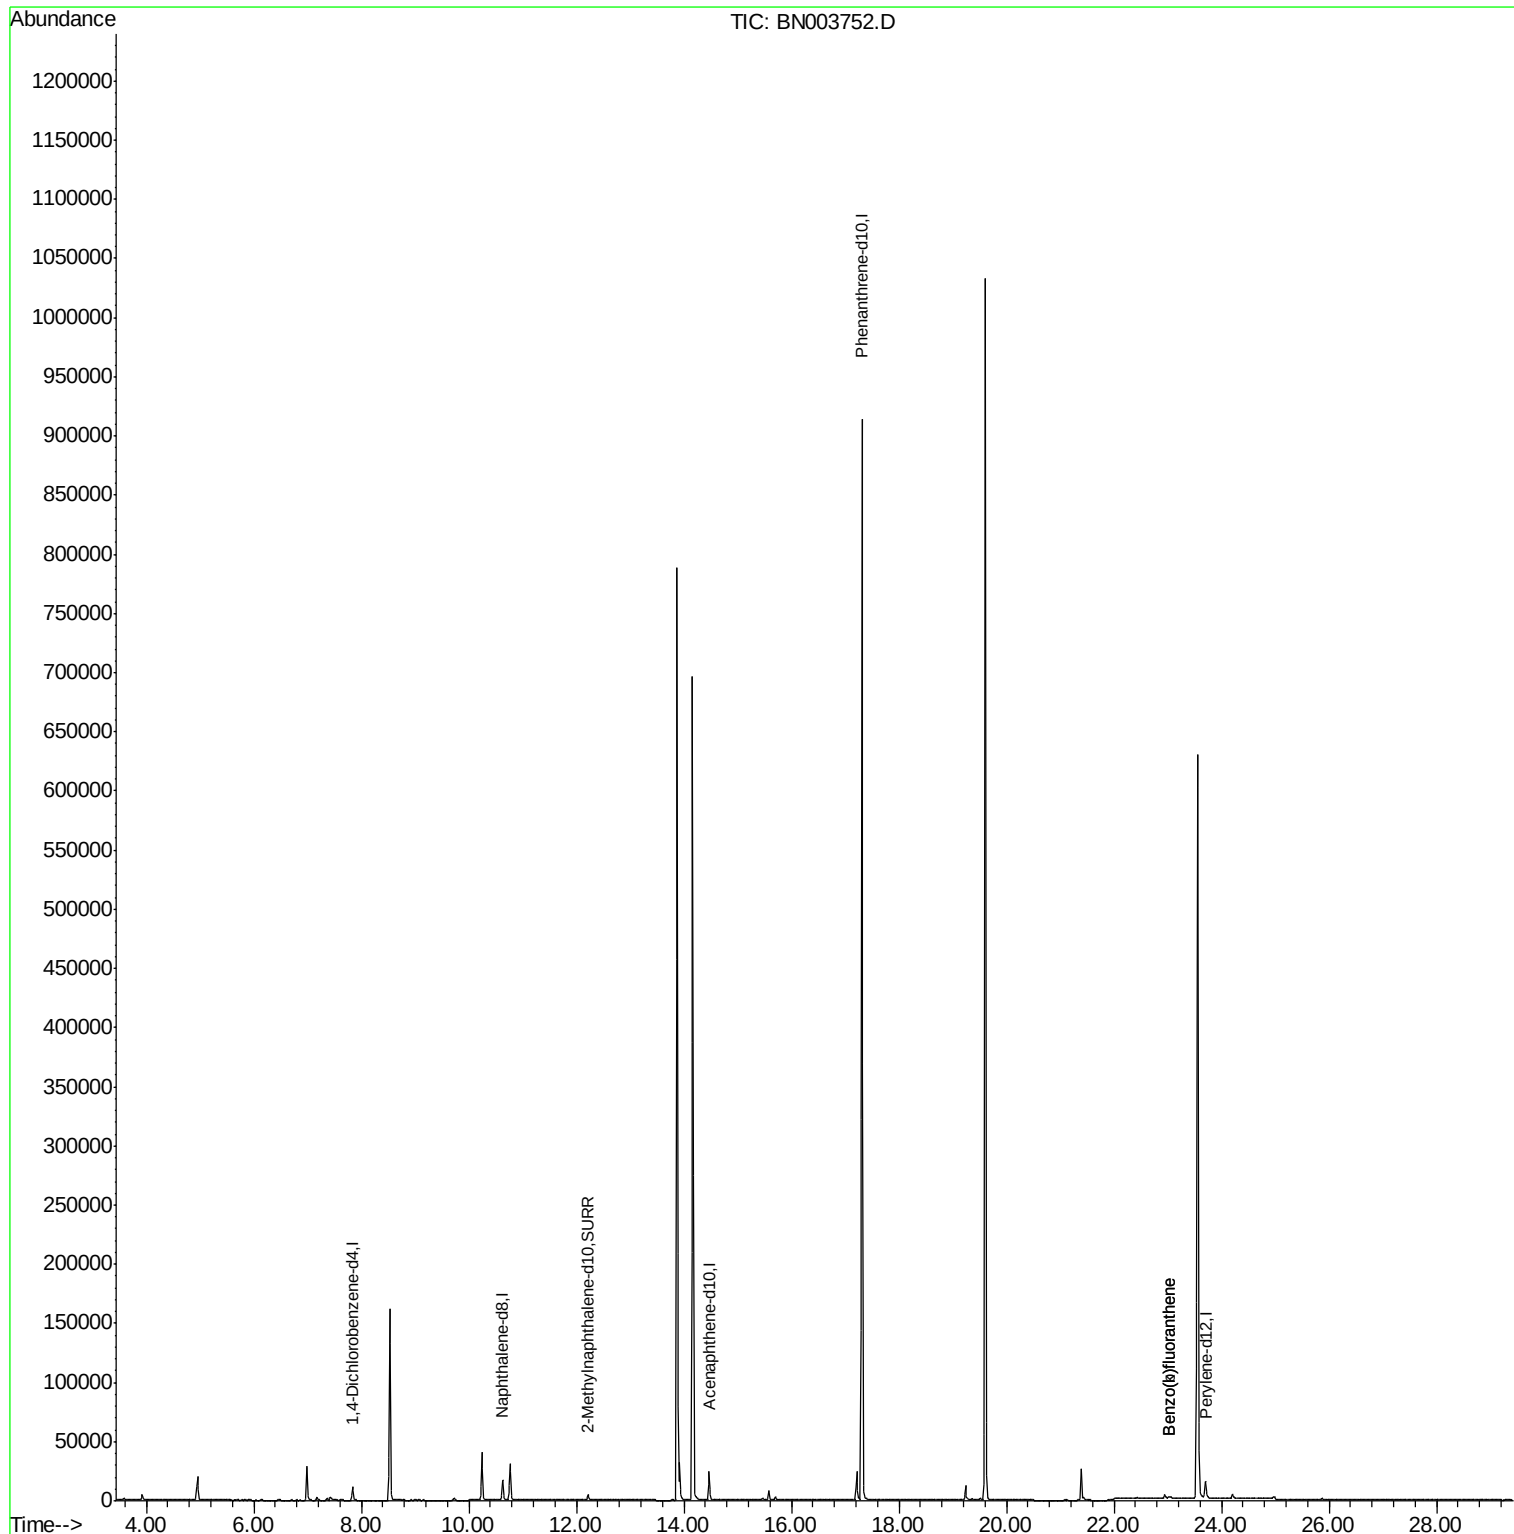

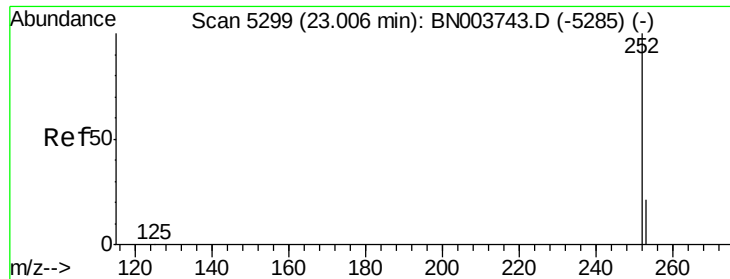

#21

Benzo(b)fluoranthene

Concen: 0.028 ng/ul

RT: 23.01 min Scan# 5299

Delta R.T. 0.00 min

Lab File: BN003752.D

Acq: 07 Dec 2018 04:44

Instrument :

BNA_N

ClientSampleId :

F9E60





Tgt Ion:252 Resp: 2440

Ion Ratio Lower Upper

252 100

253 61.7 0.0 46.0#

125 53.2 0.0 22.4#

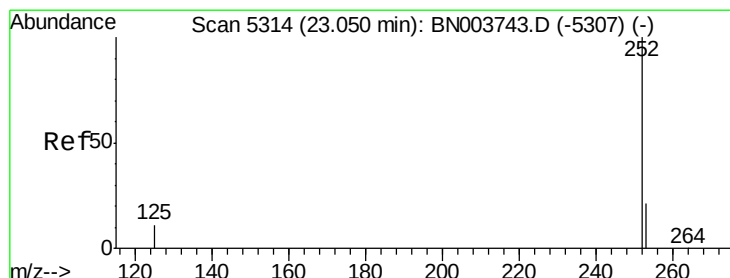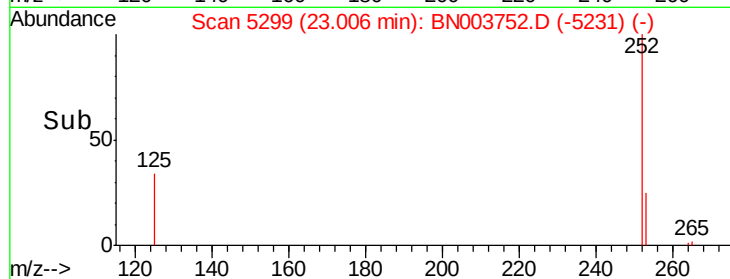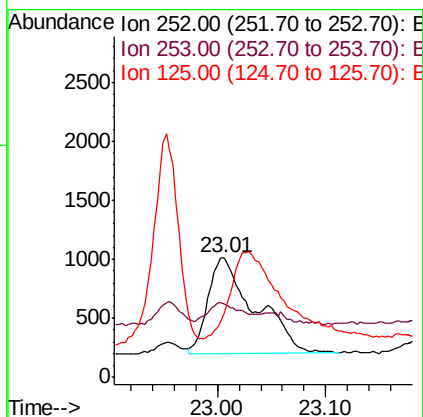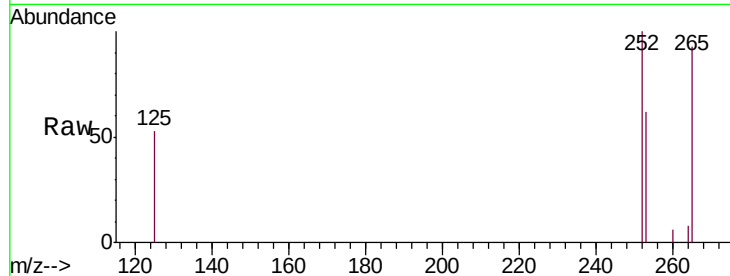

#22

Benzo(k)fluoranthene

Concen: 0.029 ng/ul

RT: 23.01 min Scan# 5299

Delta R.T. -0.04 min

Lab File: BN003752.D

Acq: 07 Dec 2018 04:44

Tgt Ion:252 Resp: 2440

Ion Ratio Lower Upper

252 100

253 61.7 18.5 27.7#

125 53.2 9.0 13.6#

