

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN120618\
Quantitation Report (Not Reviewed)

Data File : BN003755.D
Acq On : 07 Dec 2018 06:29
Operator : JU/SJ
Sample : J6227-18
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E63

Quant Time: Dec 07 08:06:10 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 07 04:08:50 2018
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	5385	0.40	ng/ul	0.00
2) Naphthalene-d8	10.63	136	22379	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.47	164	12364	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.31	188	1724369	0.40	ng/ul	0.09
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.40
20) Perylene-d12	23.70	264	22134	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.22	152	10364	0.30	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
23) Benzo(a)pyrene	23.56	252	6583	0.083	ng/ul#	Qvalue 69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BN003755.D
Acq On : 07 Dec 2018 06:29
Operator : JU/SJ
Sample : J6227-18
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E63

Quant Time: Dec 07 08:06:10 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 07 04:08:50 2018
Response via : Initial Calibration

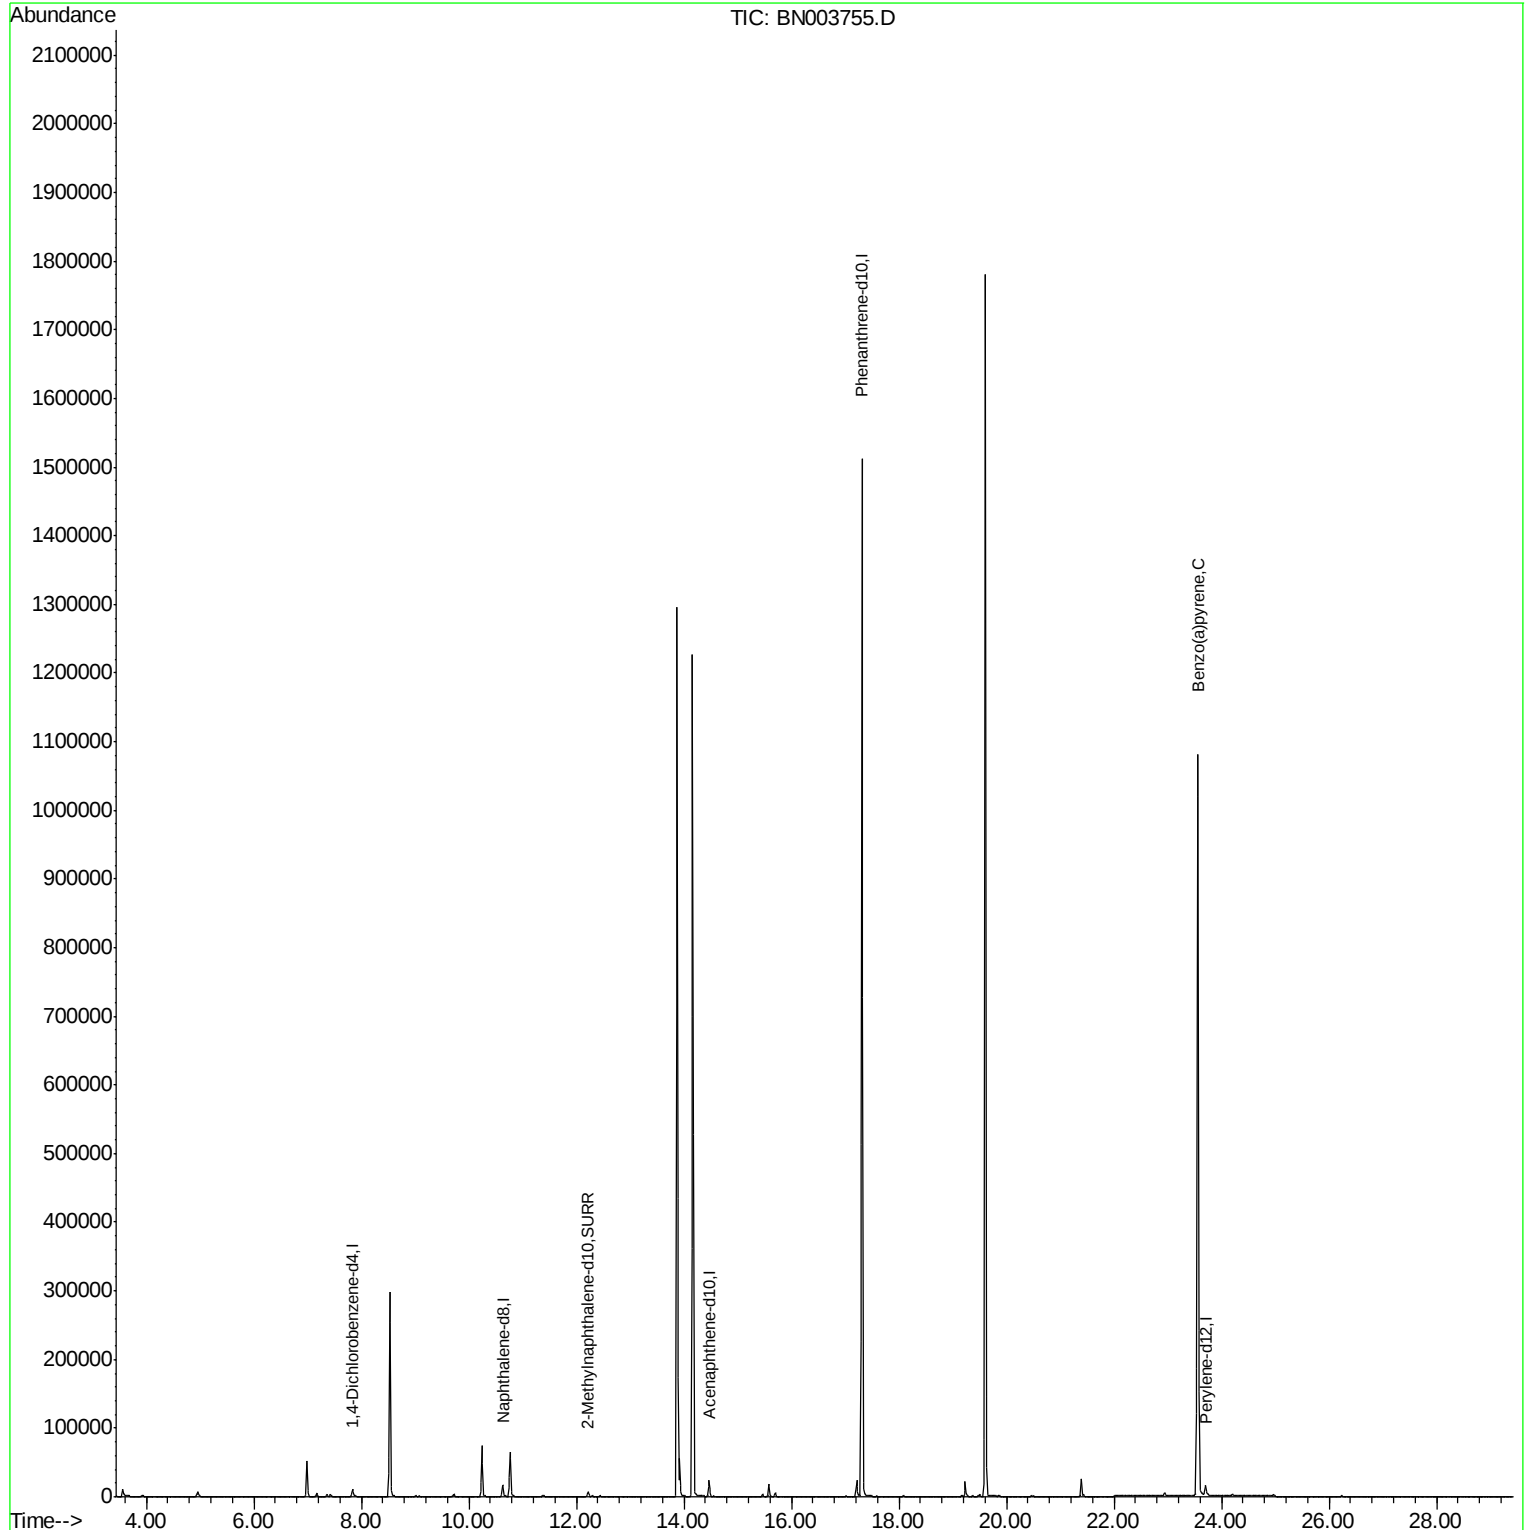

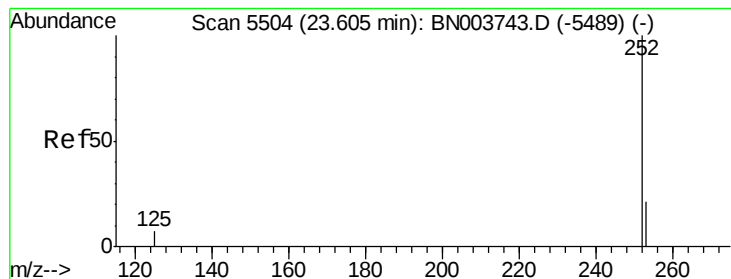

#23

Benzo(a)pyrene

Concen: 0.083 ng/ul

RT: 23.56 min Scan# 5489

Delta R.T. -0.04 min

Lab File: BN003755.D


Acq: 07 Dec 2018 06:29

Instrument :

BNA_N

ClientSampleId :

F9E63

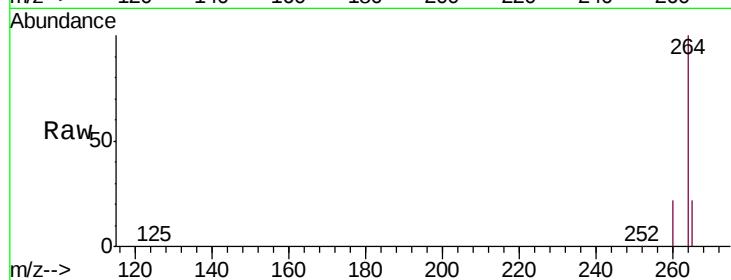

Tgt Ion: 252 Resp: 6583

Ion Ratio Lower Upper

252 100

253 38.2 19.0 28.4#

125 26.0 10.2 15.4#

