


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN120618\
Quantitation Report (QT Reviewed)
Data File : BN003740.D
Acq On : 06 Dec 2018 20:34
Operator : JU/SJ
Sample : J6077-10
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9Y44

Manual Integrations
APPROVED

mohammad
12/10/2018 12:20:27 PM

Quant Time: Dec 07 03:57:08 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 07 03:02:08 2018
Response via : Initial Calibration

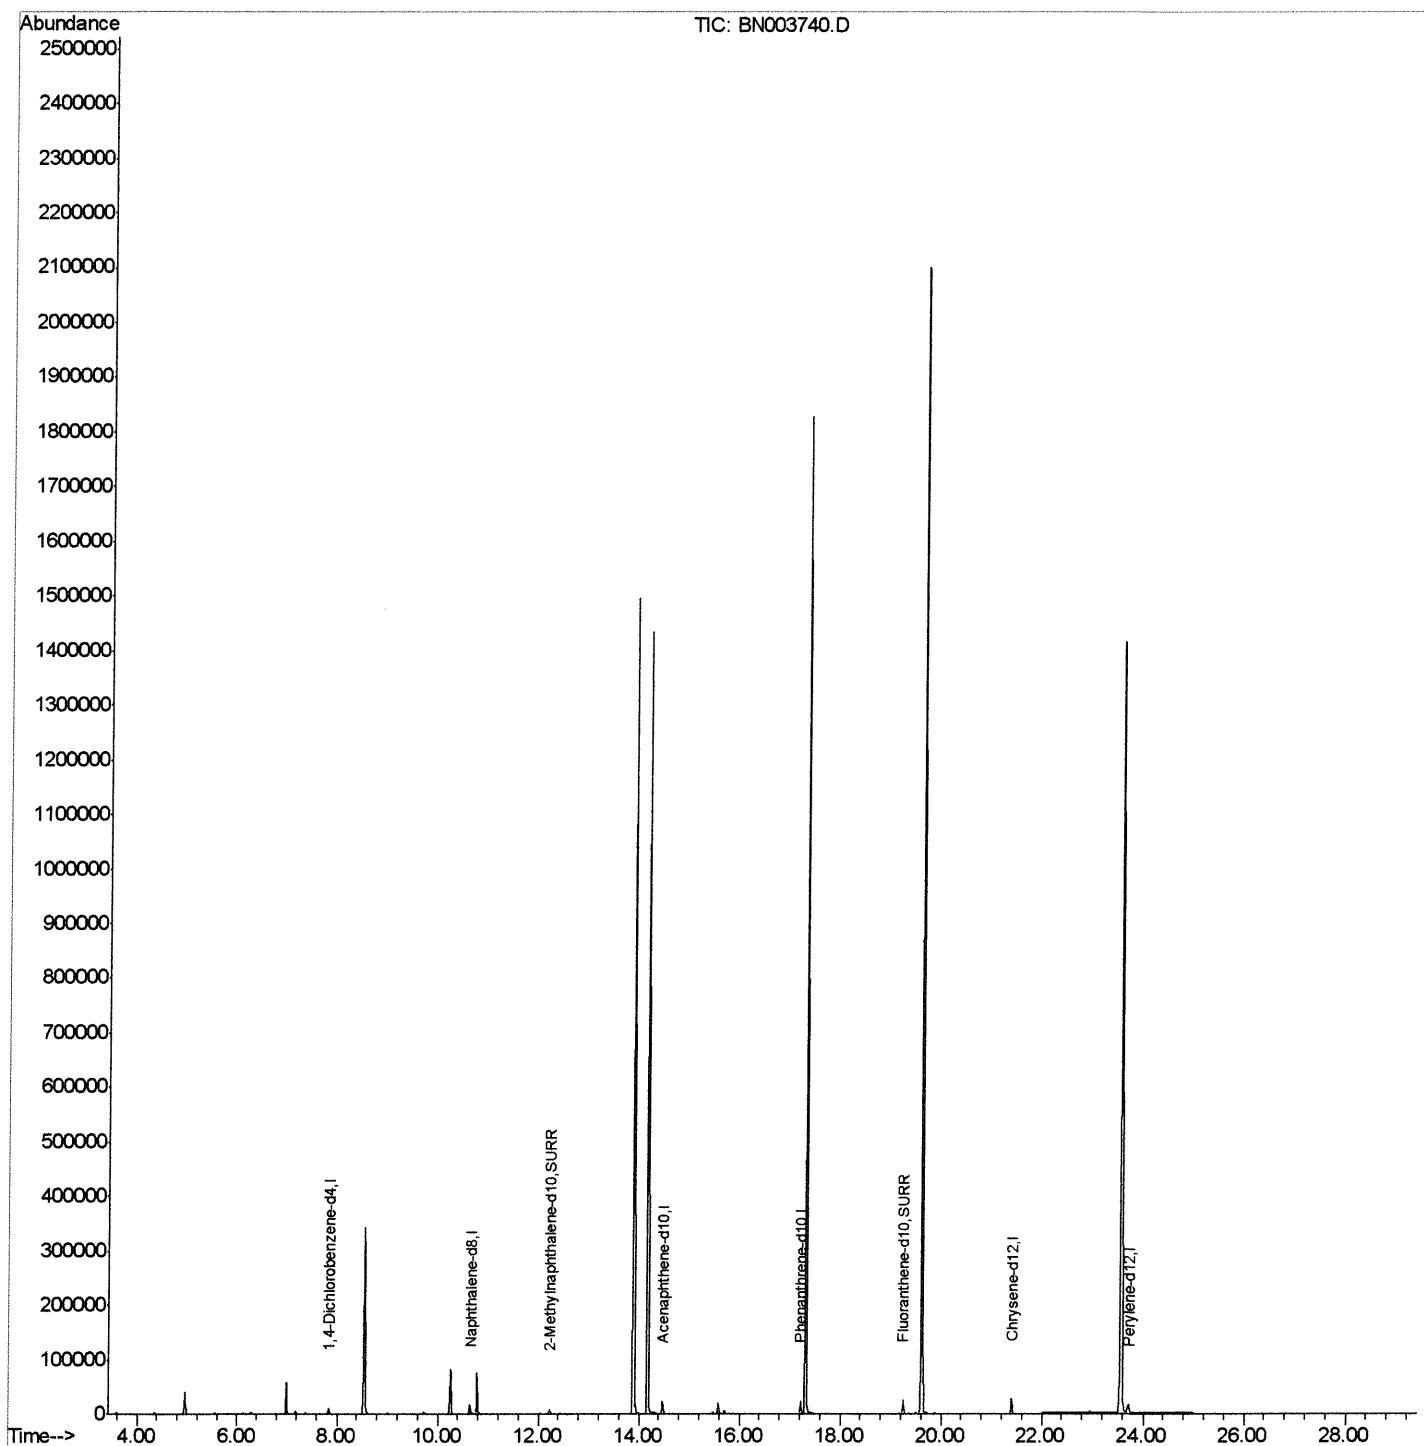

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN120618\
Quantitation Report (Qedit)




Data File : BN003740.D
Acq On : 06 Dec 2018 20:34
Operator : JU/SJ
Sample : J6077-10
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9Y44

Manual Integrations
APPROVED

mohammad
12/10/2018 12:20:27 PM

Quant Time: Dec 07 03:20:38 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 07 03:02:08 2018
Response via : Initial Calibration

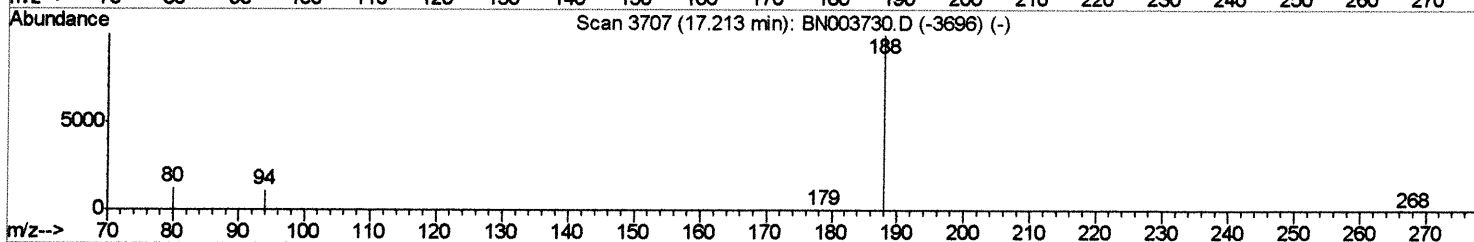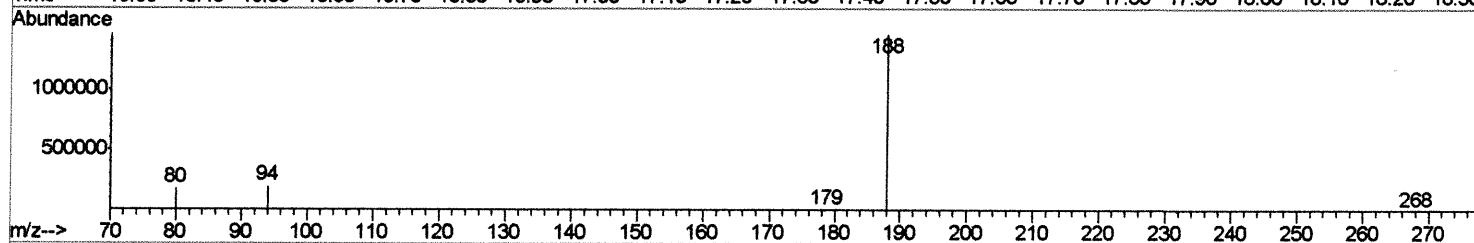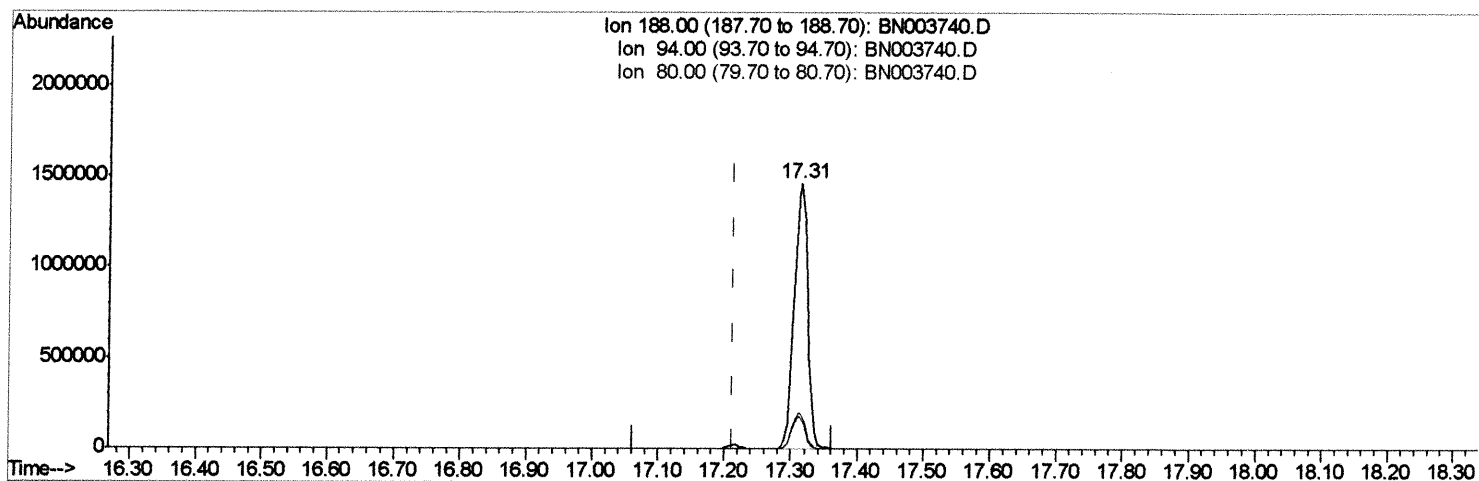

TIC: BN003740.D

(10) Phenanthrene-d10 (I)

17.314min (+0.101) 0.40ng/ul

response 2074067

Ion	Exp%	Act%
188.00	100	100
94.00	10.40	13.18#
80.00	11.60	11.72
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN120618\
Quantitation Report (Qedit)




Data File : BN003740.D
Acq On : 06 Dec 2018 20:34
Operator : JU/SJ
Sample : J6077-10
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9Y44

Manual Integrations
APPROVED

mohammad
12/10/2018 12:20:27 PM

Quant Time: Dec 07 03:20:38 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 07 03:02:08 2018
Response via : Initial Calibration

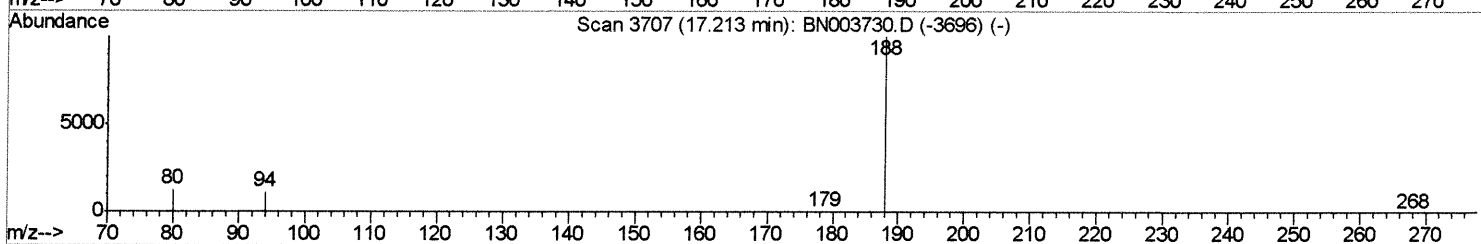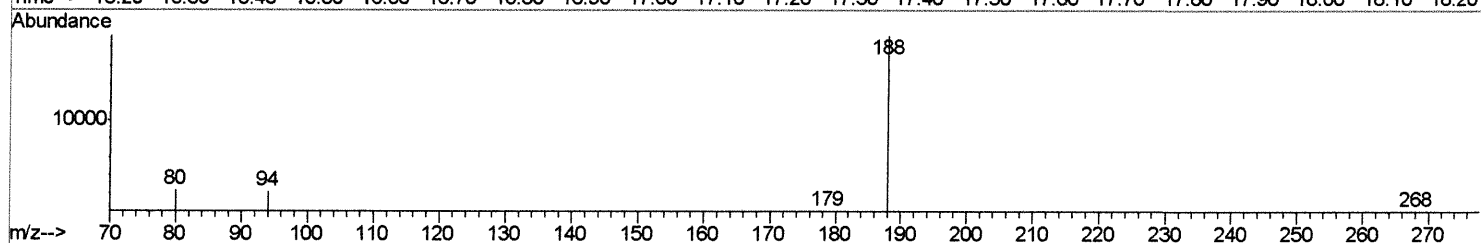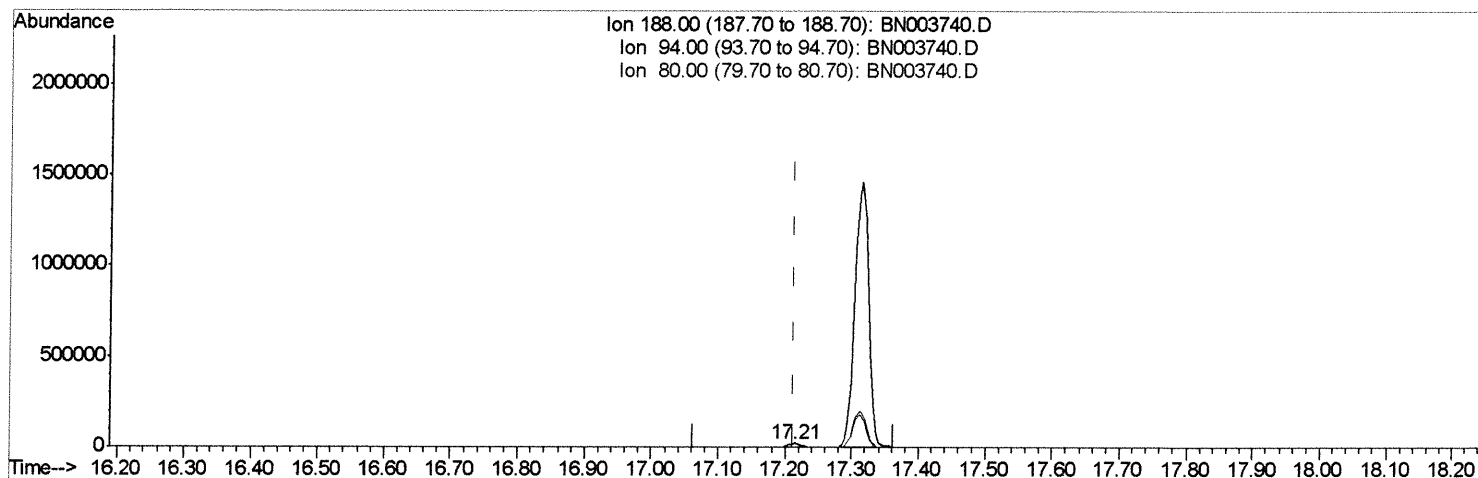

TIC: BN003740.D

(10) Phenanthrene-d10 (I)

17.213min (-0.000) 0.40ng/ul m) 52 12/11/18

response 27083

Ion	Exp%	Act%
188.00	100	100
94.00	10.40	11.42
80.00	11.60	12.44
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN120618\
Quantitation Report (Qedit)




Data File : BN003740.D
Acq On : 06 Dec 2018 20:34
Operator : JU/SJ
Sample : J6077-10
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9Y44

Manual Integrations
APPROVED

mohammad
12/10/2018 12:20:27 PM

Quant Time: Dec 07 03:55:56 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 07 03:02:08 2018
Response via : Initial Calibration

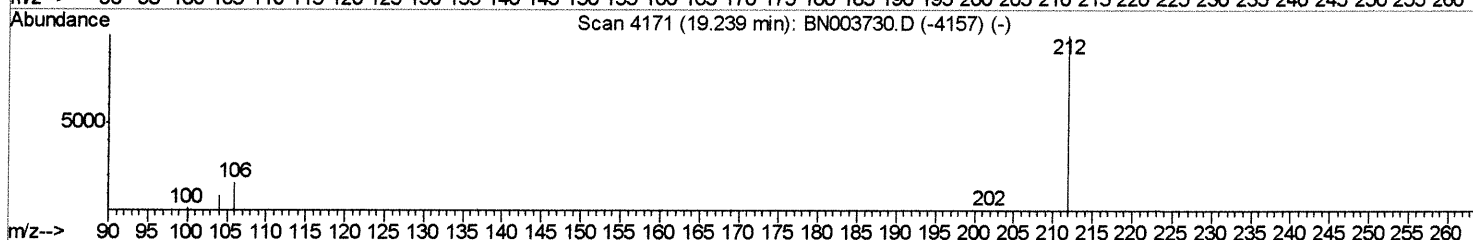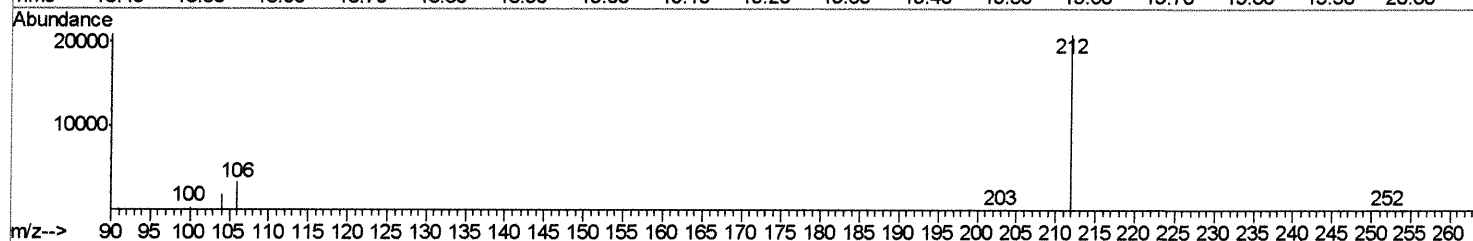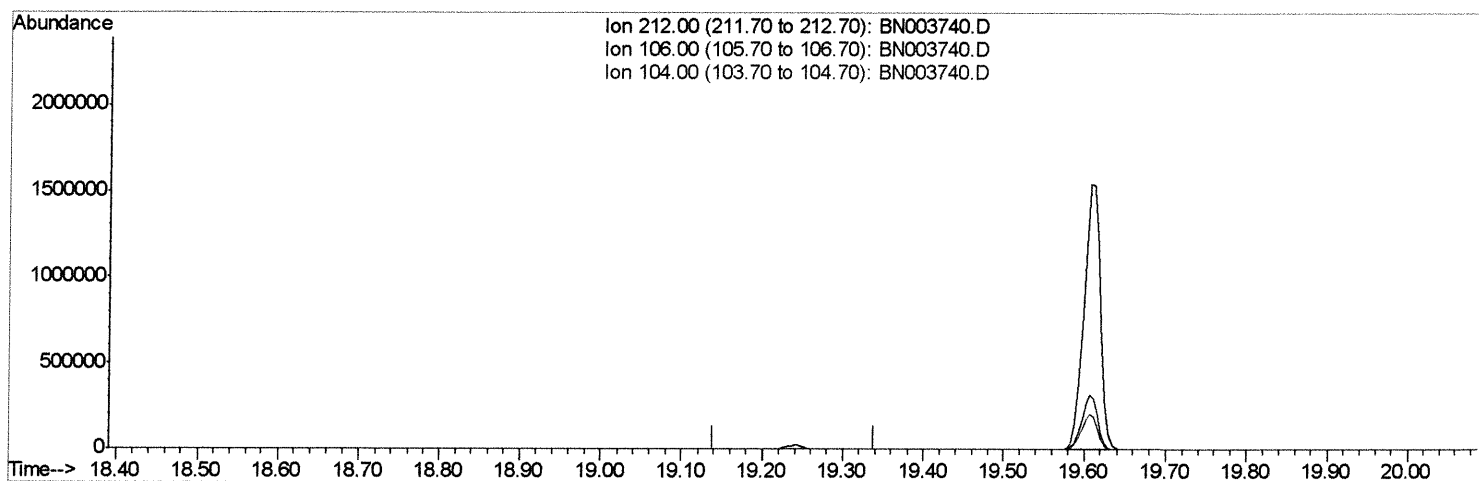

TIC: BN003740.D

(14) Fluoranthene-d10 (SURR)

19.239min (-19.239) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	14.20	0.00#
104.00	8.00	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN120618\
Quantitation Report (Qedit)




Data File : BN003740.D
Acq On : 06 Dec 2018 20:34
Operator : JU/SJ
Sample : J6077-10
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9Y44

Manual Integrations
APPROVED

mohammad
12/10/2018 12:20:27 PM

Quant Time: Dec 07 03:55:56 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 07 03:02:08 2018
Response via : Initial Calibration

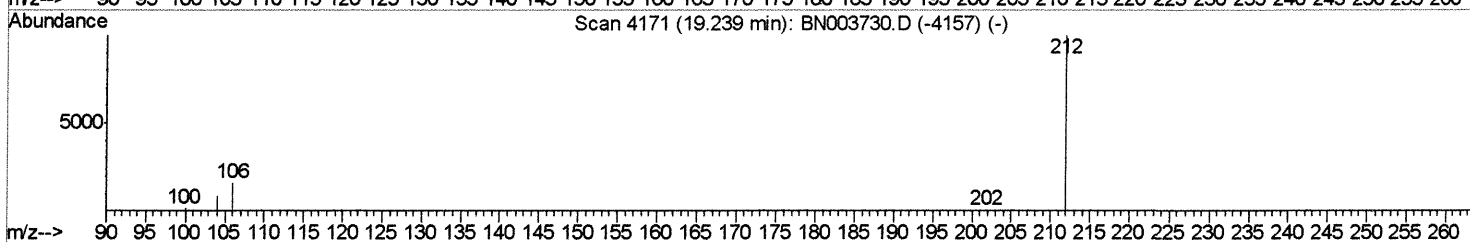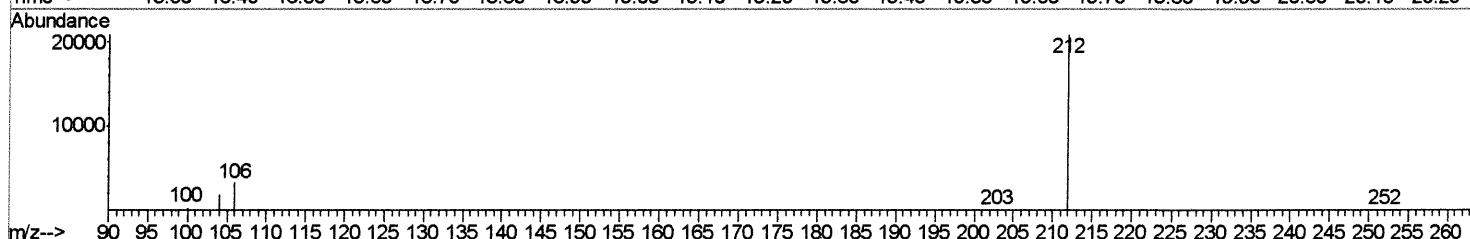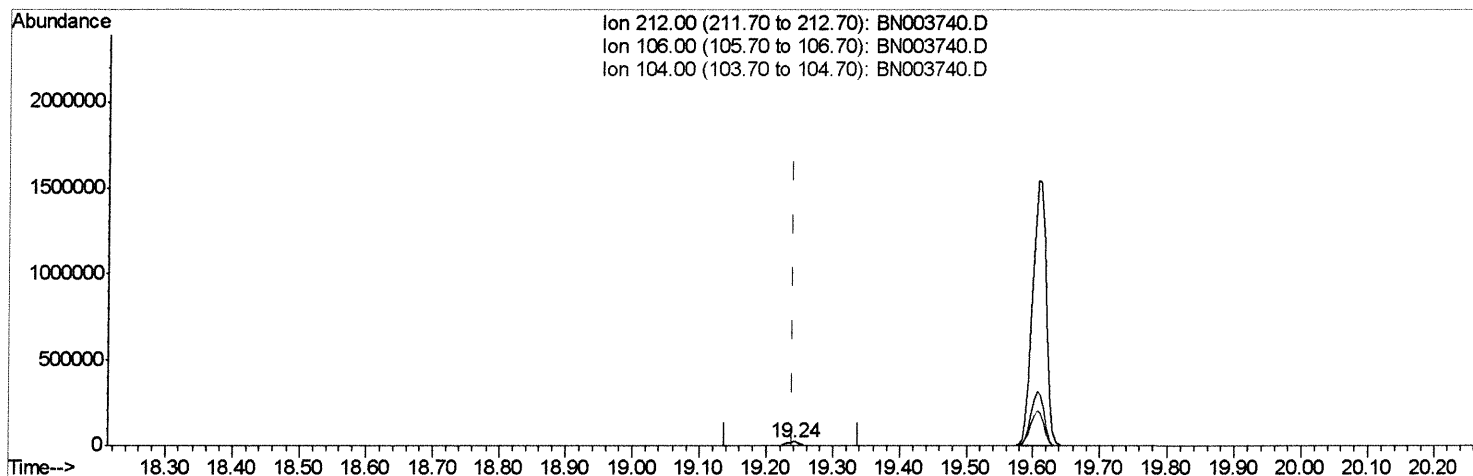

TIC: BN003740.D

(14) Fluoranthene-d10 (SURR)

19.239min (-0.000) 0.35ng/ul m) SJ 12/11/18

response 27891

Ion	Exp%	Act%
212.00	100	100
106.00	14.20	0.00#
104.00	8.00	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN120618\
Quantitation Report (Qedit)




Data File : BN003740.D
Acq On : 06 Dec 2018 20:34
Operator : JU/SJ
Sample : J6077-10
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9Y44

Manual Integrations
APPROVED

mohammad
12/10/2018 12:20:27 PM

Quant Time: Dec 07 03:55:56 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 07 03:02:08 2018
Response via : Initial Calibration

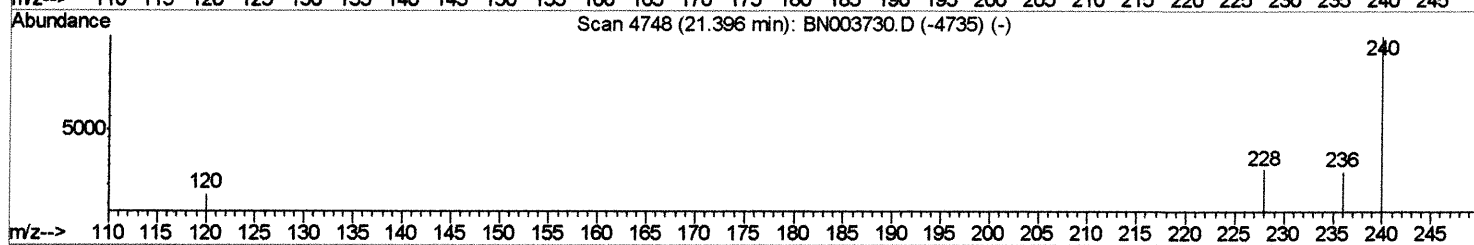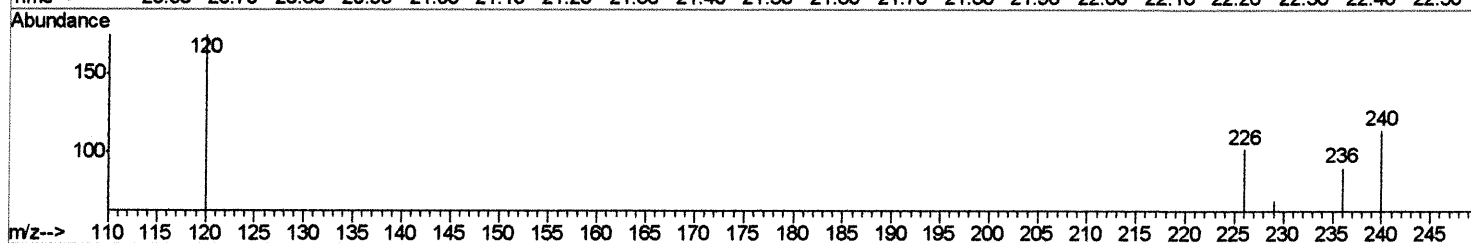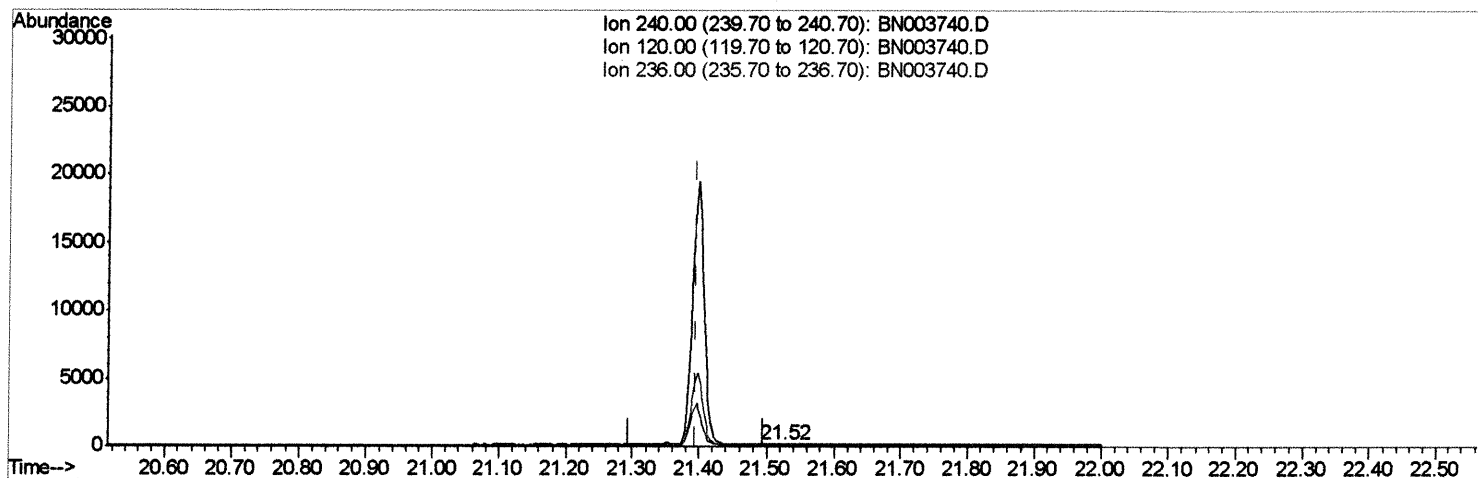

TIC: BN003740.D

(16) Chrysene-d12 (I)

21.524min (+0.128) 0.40ng/ul

response 46

Ion	Exp%	Act%
240.00	100	100
120.00	14.00	153.51#
236.00	27.60	78.95#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN120618\
Quantitation Report (Qedit)




Data File : BN003740.D
Acq On : 06 Dec 2018 20:34
Operator : JU/SJ
Sample : J6077-10
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9Y44

Manual Integrations
APPROVED

mohammad
12/10/2018 12:20:27 PM

Quant Time: Dec 07 03:55:56 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 07 03:02:08 2018
Response via : Initial Calibration

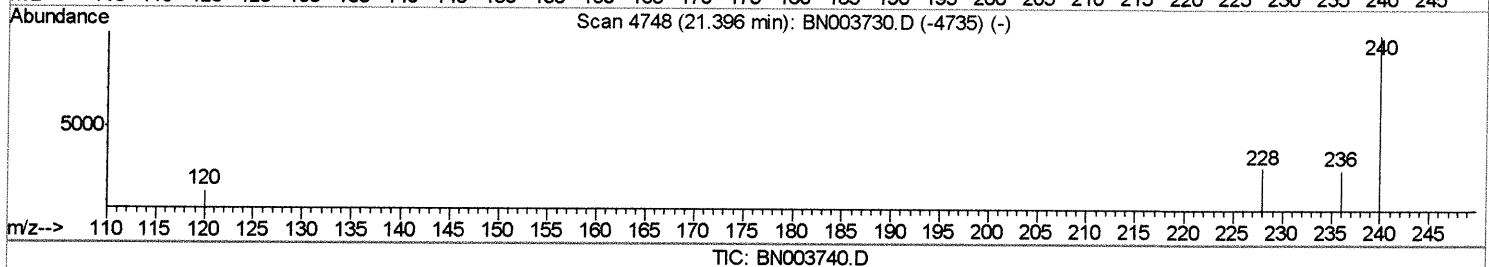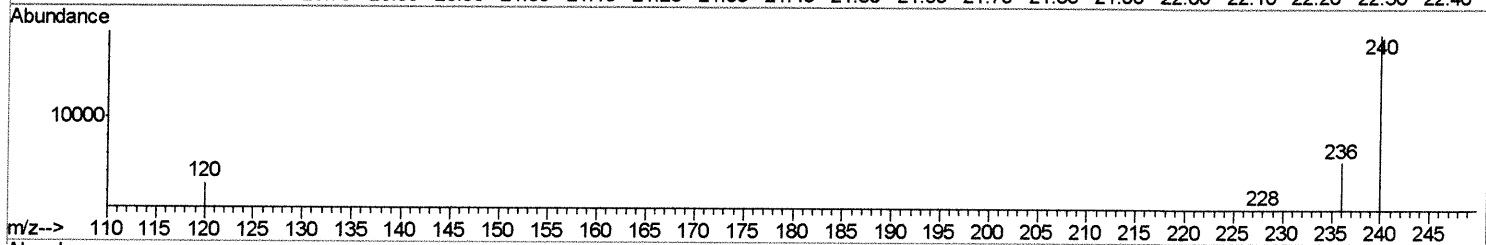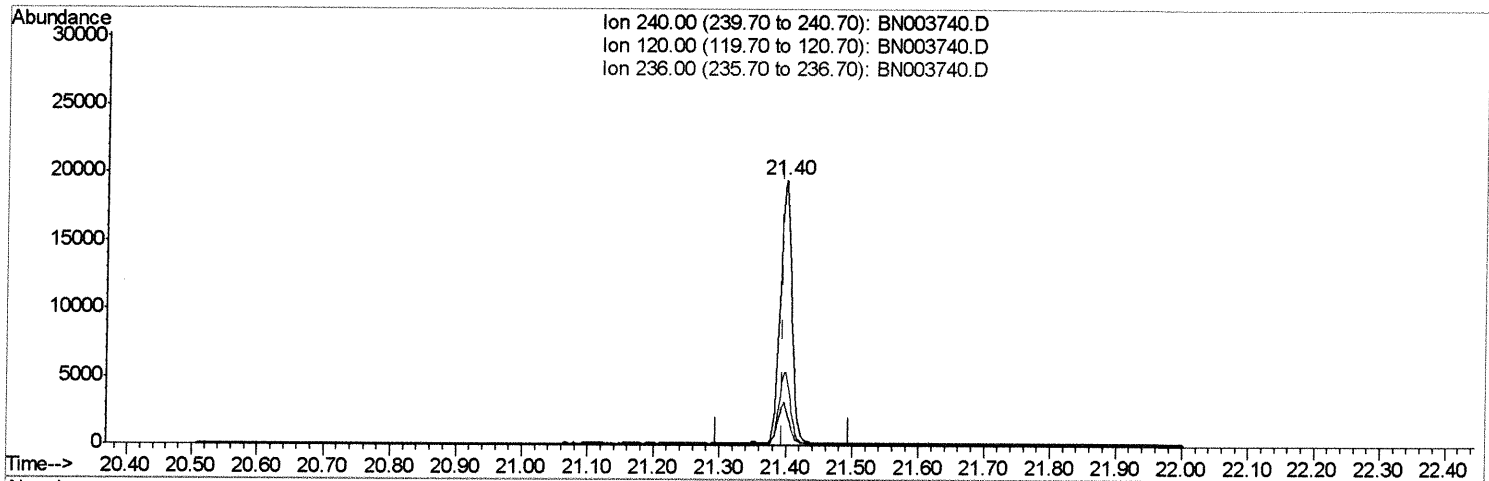

TIC: BN003740.D

(16) Chrysene-d12 (I)

21.398min (+0.003) 0.40ng/ul m > SJ 12/11/18

response 23795

Ion	Exp%	Act%
240.00	100	100
120.00	14.00	14.28
236.00	27.60	27.64
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN120618\
Quantitation Report (Qedit)




Data File : BN003740.D
Acq On : 06 Dec 2018 20:34
Operator : JU/SJ
Sample : J6077-10
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
F9Y44

Manual Integrations
APPROVED

mohammad
12/10/2018 12:20:27 PM

Quant Time: Dec 07 03:56:31 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 07 03:02:08 2018
Response via : Initial Calibration

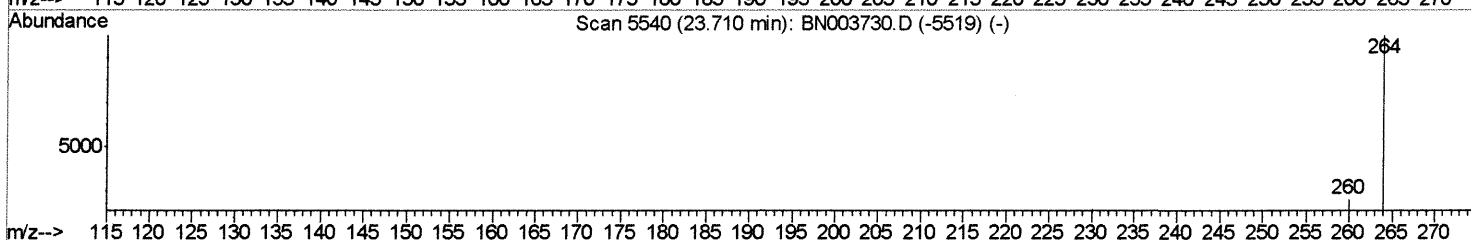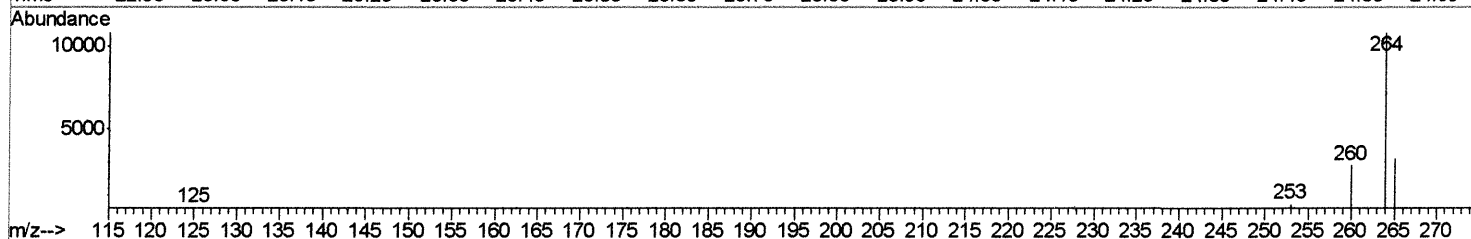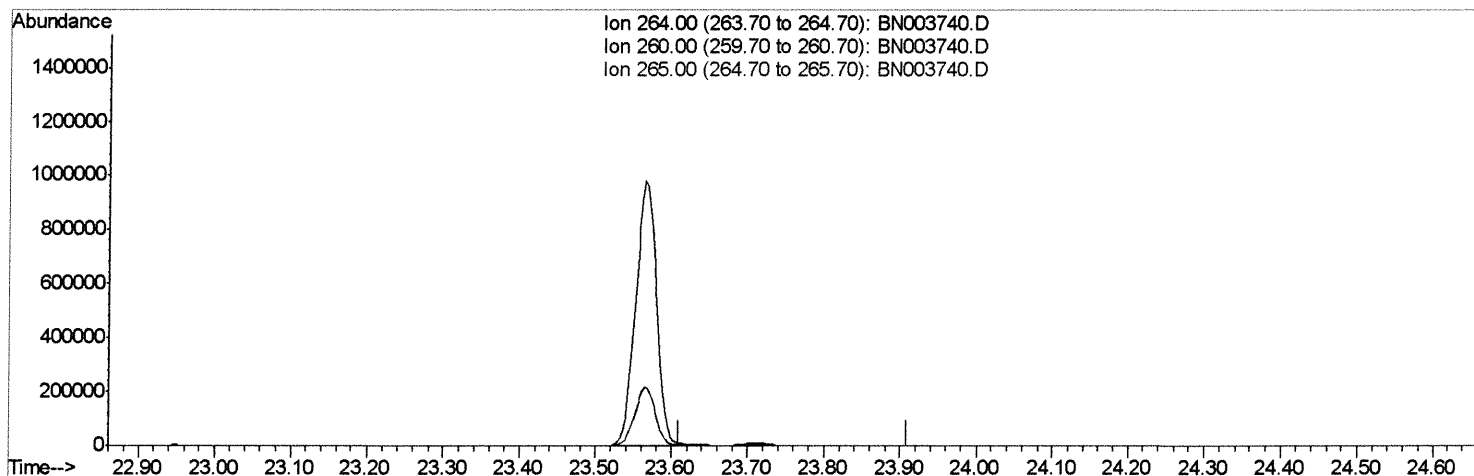

TIC: BN003740.D

(20) Perylene-d12 (I)

23.710min (-23.710) 0.00ng/ui

response 0

Ion	Exp%	Act%
264.00	100	0.00
260.00	26.20	0.00#
265.00	33.50	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN120618\
Quantitation Report (Qedit)




Data File : BN003740.D
Acq On : 06 Dec 2018 20:34
Operator : JU/SJ
Sample : J6077-10
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
F9Y44

Manual Integrations
APPROVED

mohammad
12/10/2018 12:20:27 PM

Quant Time: Dec 07 03:56:31 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 07 03:02:08 2018
Response via : Initial Calibration

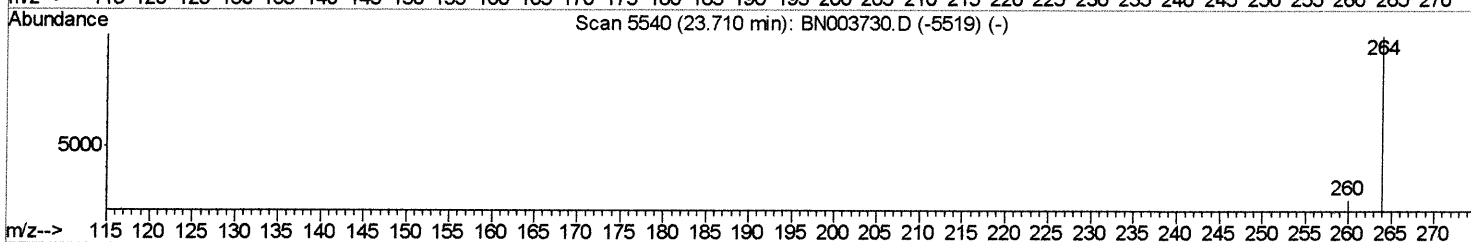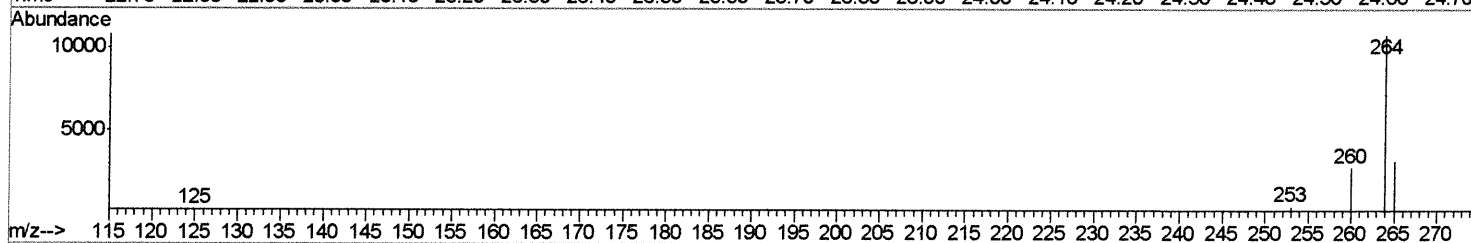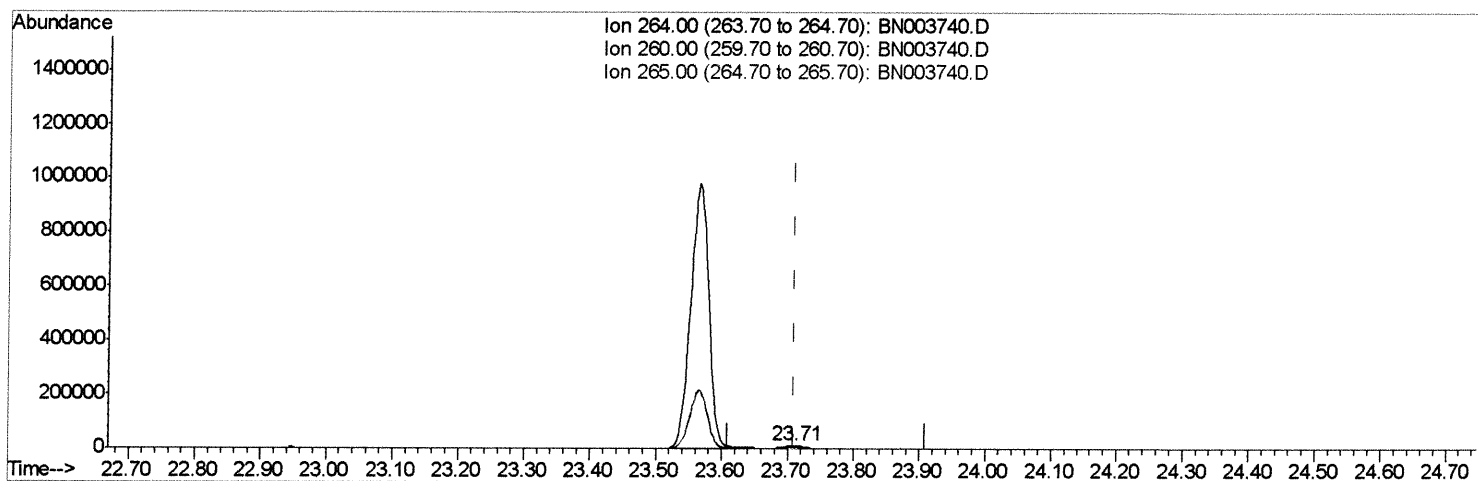

TIC: BN003740.D

(20) Perylene-d12 (I)

23.710min (-0.000) 0.40ng/ul m) SJ 12/11/18

response 17753

Ion	Exp%	Act%
264.00	100	100
260.00	26.20	26.11
265.00	33.50	29.67
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN120618\
Quantitation Report (QT Reviewed)

Data File : BN003740.D
Acq On : 06 Dec 2018 20:34
Operator : JU/SJ
Sample : J6077-10
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9Y44

Manual Integrations
APPROVED

mohammad
12/10/2018 12:20:27 PM

Quant Time: Dec 07 03:57:08 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 07 03:02:08 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	5314	0.40	ng/ul	0.00
2) Naphthalene-d8	10.63	136	22092	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.47	164	12519	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.21	188	27083m	0.40	ng/ul	0.00
16) Chrysene-d12	21.40	240	23795m	0.40	ng/ul	0.00
20) Perylene-d12	23.71	264	17753m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.22	152	12113	0.36	ng/ul	0.00
14) Fluoranthene-d10	19.24	212	27891m	0.35	ng/ul	0.00

SJ 12/11/18

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed