


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN120618\
Quantitation Report (QT Reviewed)
Data File : BN003749.D
Acq On : 07 Dec 2018 03:00
Operator : JU/SJ
Sample : J6227-10
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E55

Manual Integrations
APPROVED

mohammad
12/10/2018 12:20:52 PM

Quant Time: Dec 07 04:55:23 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 07 04:08:50 2018
Response via : Initial Calibration

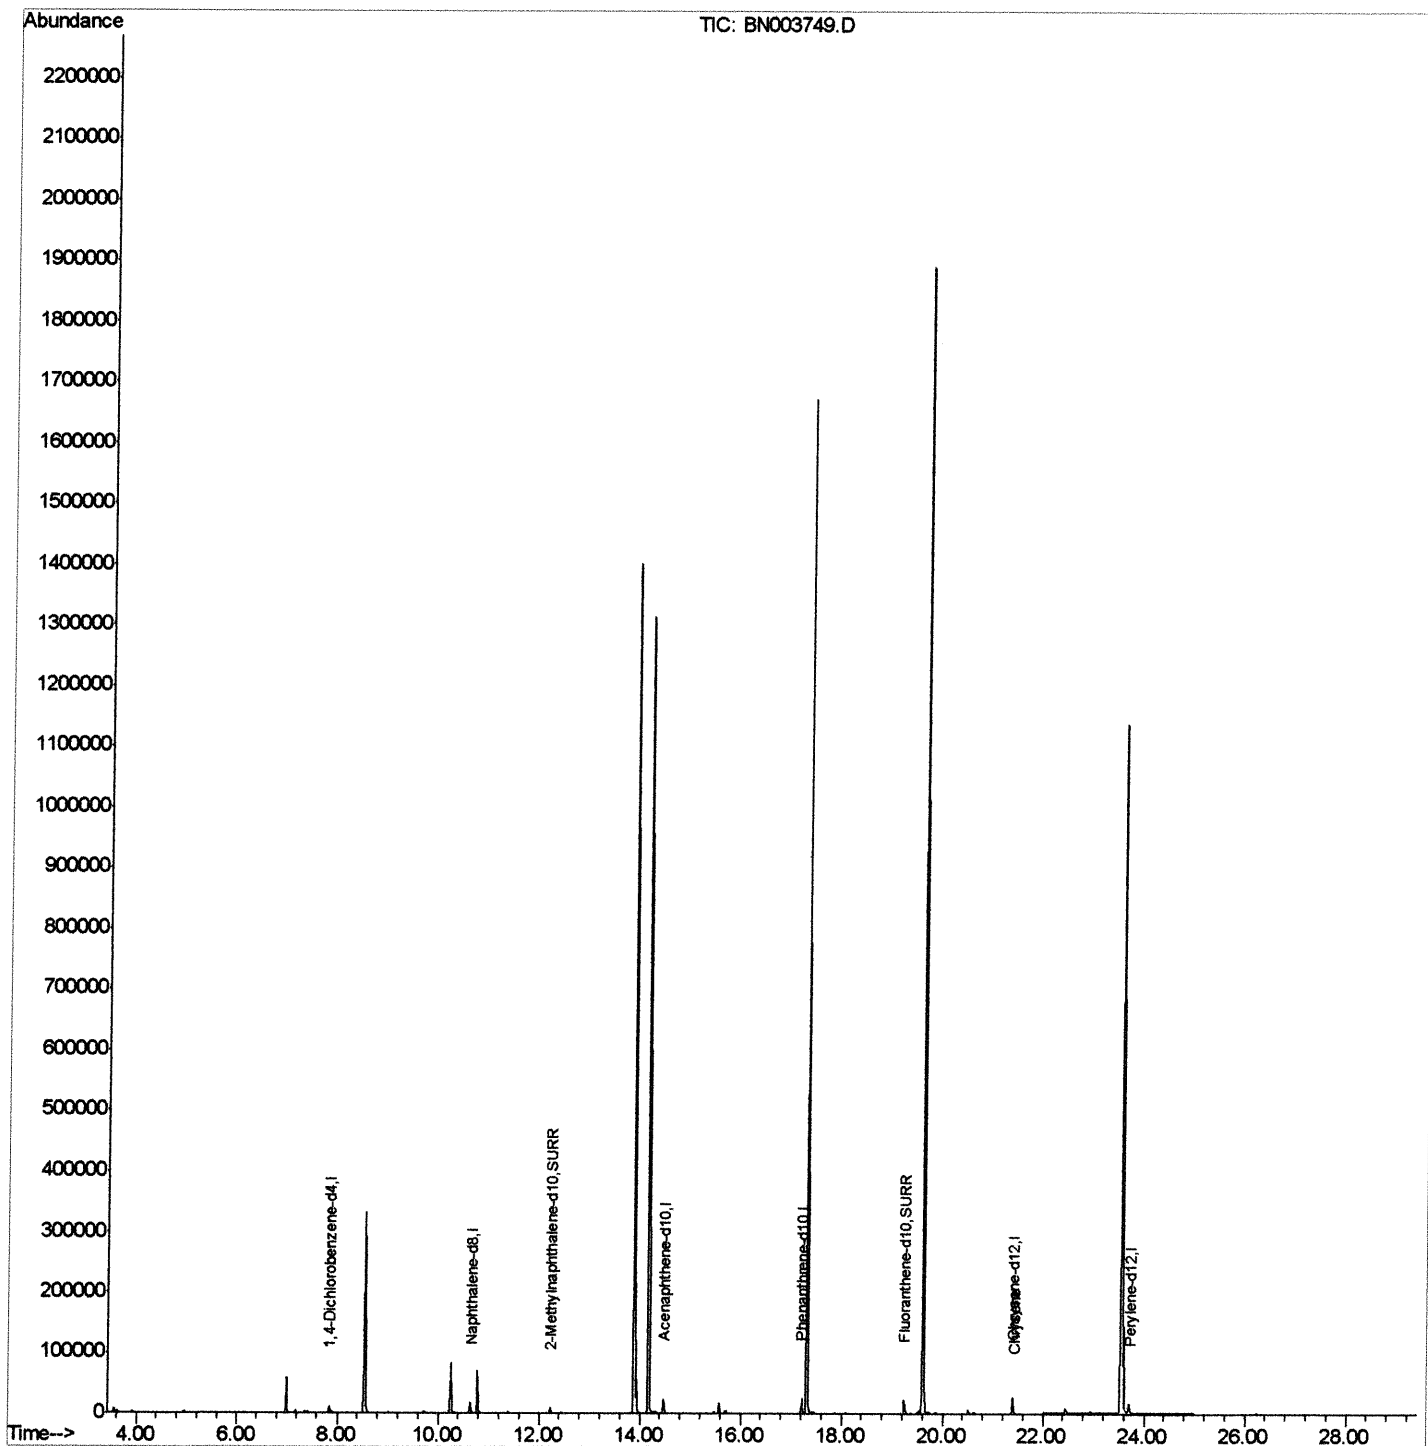

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN120618\
Quantitation Report (Qedit)




Data File : BN003749.D
Acq On : 07 Dec 2018 03:00
Operator : JU/SJ
Sample : J6227-10
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E55

Manual Integrations
APPROVED

mohammad
12/10/2018 12:20:52 PM

Quant Time: Dec 07 04:12:51 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 07 04:08:50 2018
Response via : Initial Calibration

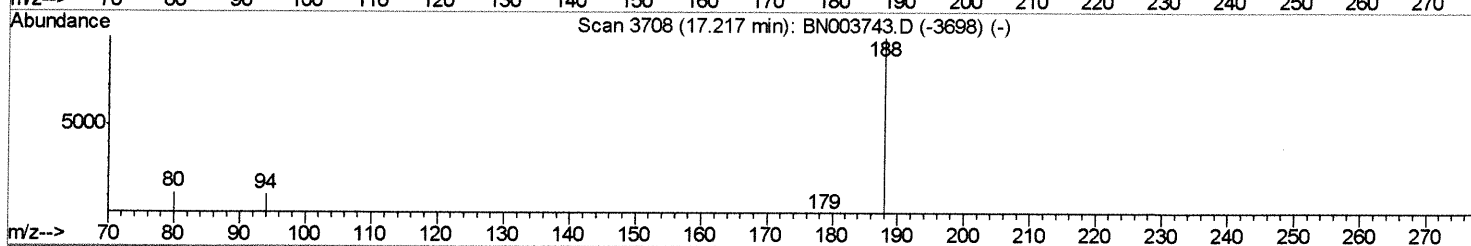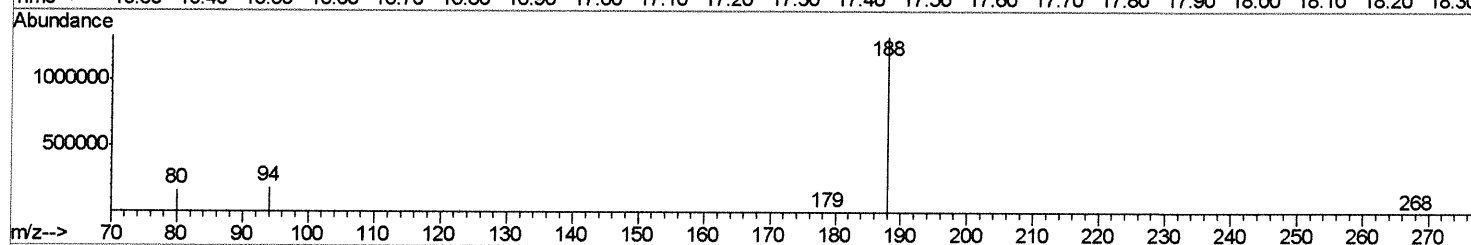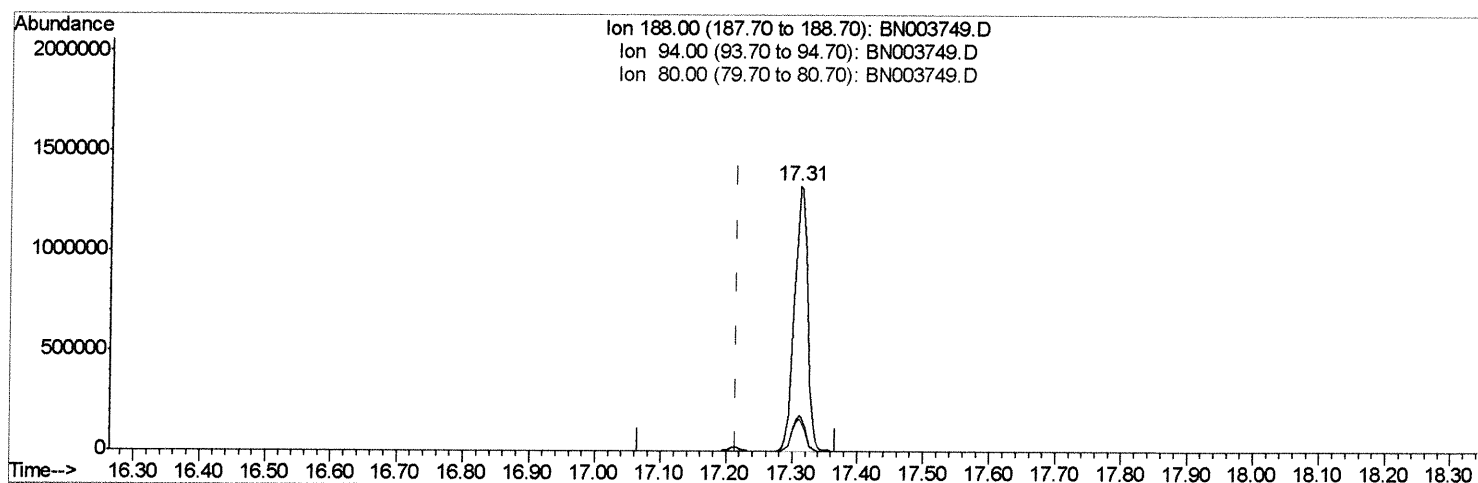

TIC: BN003749.D

(10) Phenanthrene-d10 (I)

17.310min (+0.093) 0.40ng/ul

response 1851432

Ion	Exp%	Act%
188.00	100	100
94.00	10.40	13.79#
80.00	11.60	12.44
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN120618\
Quantitation Report (Qedit)




Data File : BN003749.D
Acq On : 07 Dec 2018 03:00
Operator : JU/SJ
Sample : J6227-10
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E55

Manual Integrations
APPROVED

mohammad
12/10/2018 12:20:52 PM

Quant Time: Dec 07 04:12:51 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 07 04:08:50 2018
Response via : Initial Calibration

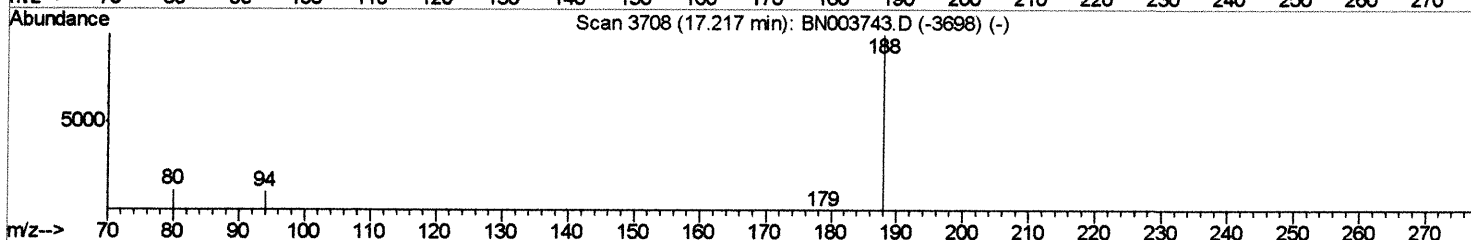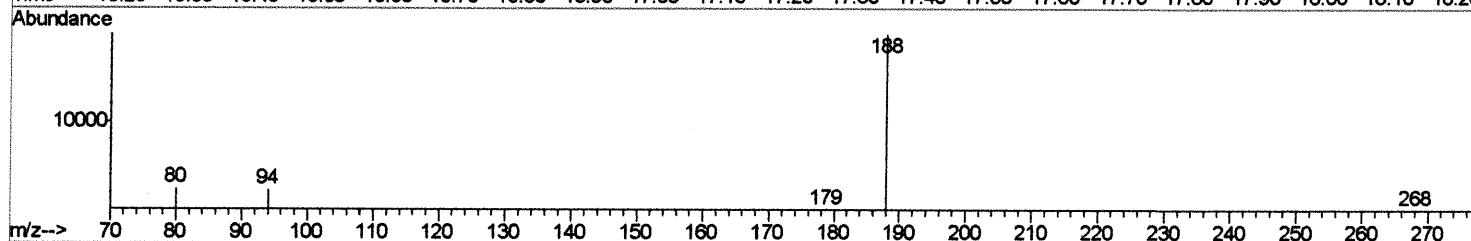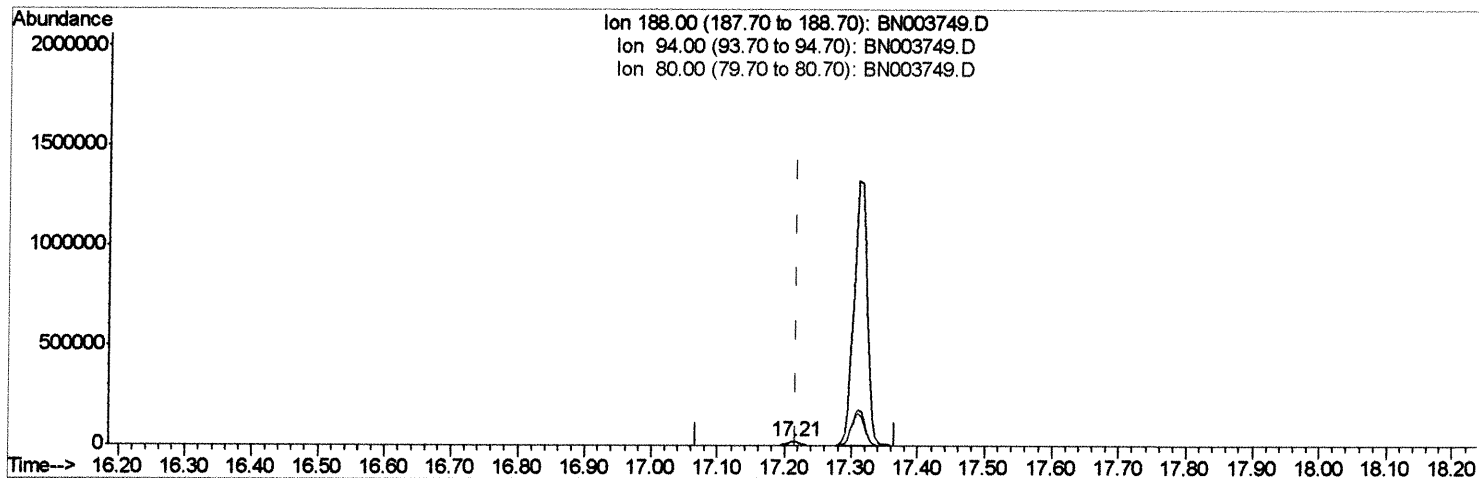

TIC: BN003749.D

(10) Phenanthrene-d10 (I)

17.213min (-0.004) 0.40ng/ul m

response 27422

Ion	Exp%	Act%
188.00	100	100
94.00	10.40	11.22
80.00	11.60	12.04
0.00	0.00	0.00

SS
12/11/18

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN120618\
Quantitation Report (Qedit)




Data File : BN003749.D
Acq On : 07 Dec 2018 03:00
Operator : JU/SJ
Sample : J6227-10
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E55

Manual Integrations
APPROVED

mohammad
12/10/2018 12:20:52 PM

Quant Time: Dec 07 04:53:23 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 07 04:08:50 2018
Response via : Initial Calibration

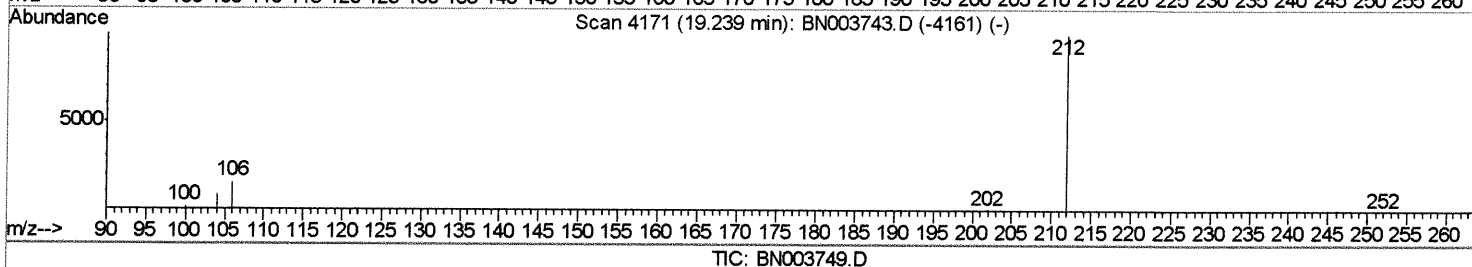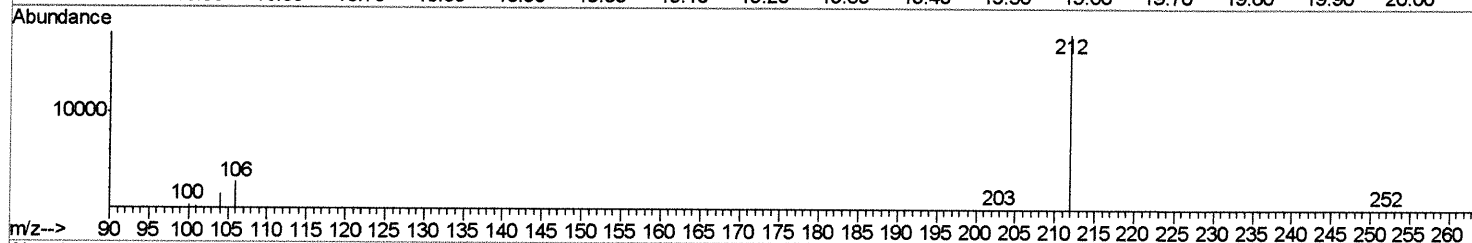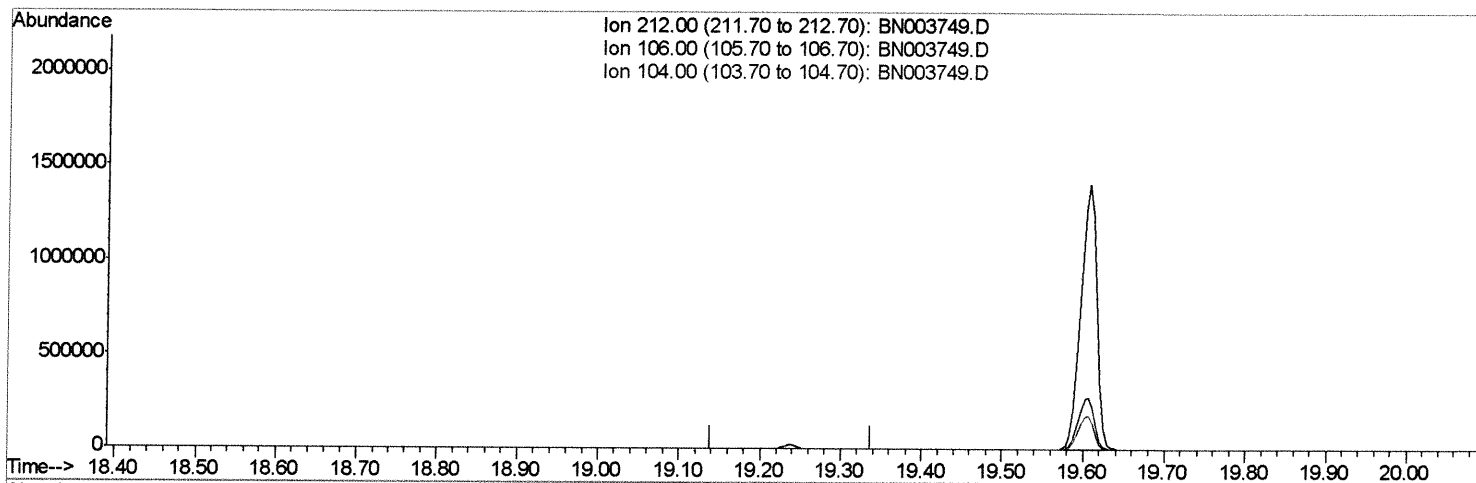

(14) Fluoranthene-d10 (SURR)

19.239min (-19.239) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	14.20	0.00#
104.00	8.00	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN120618\
Quantitation Report (Qedit)




Data File : BN003749.D
Acq On : 07 Dec 2018 03:00
Operator : JU/SJ
Sample : J6227-10
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E55

Manual Integrations
APPROVED

mohammad
12/10/2018 12:20:52 PM

Quant Time: Dec 07 04:53:23 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 07 04:08:50 2018
Response via : Initial Calibration

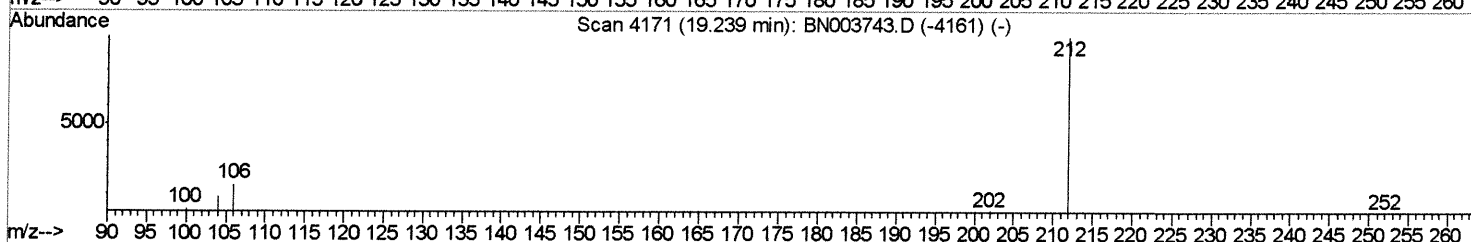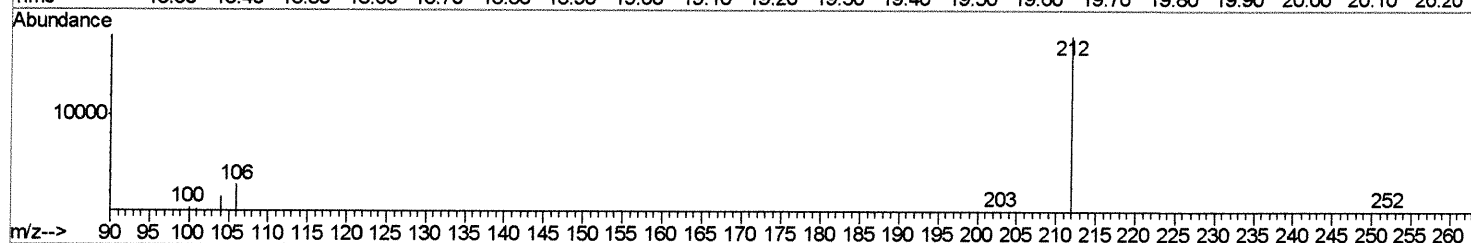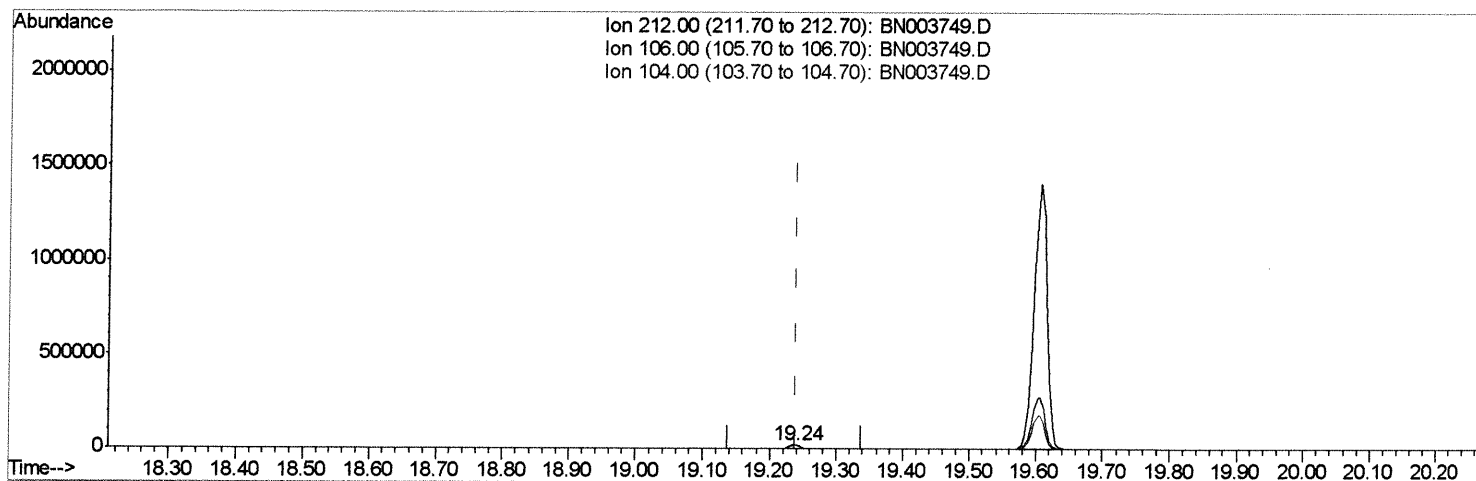

TIC: BN003749.D

(14) Fluoranthene-d10 (SURR)

19.239min (+0.000) 0.31ng/ul m

response 24621

Ion	Exp%	Act%
212.00	100	100
106.00	14.20	0.00#
104.00	8.00	0.00#
0.00	0.00	0.00

> SJ
12/11/18

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN120618\
Quantitation Report (Qedit)




Data File : BN003749.D
Acq On : 07 Dec 2018 03:00
Operator : JU/SJ
Sample : J6227-10
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E55

Manual Integrations
APPROVED

mohammad
12/10/2018 12:20:52 PM

Quant Time: Dec 07 04:53:23 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 07 04:08:50 2018
Response via : Initial Calibration

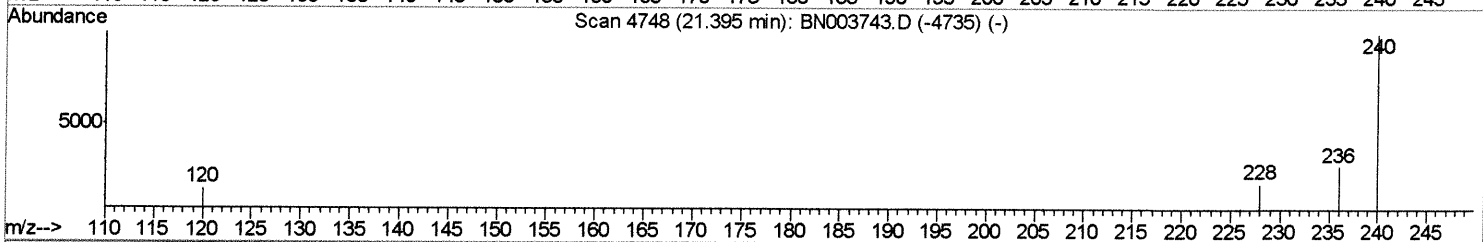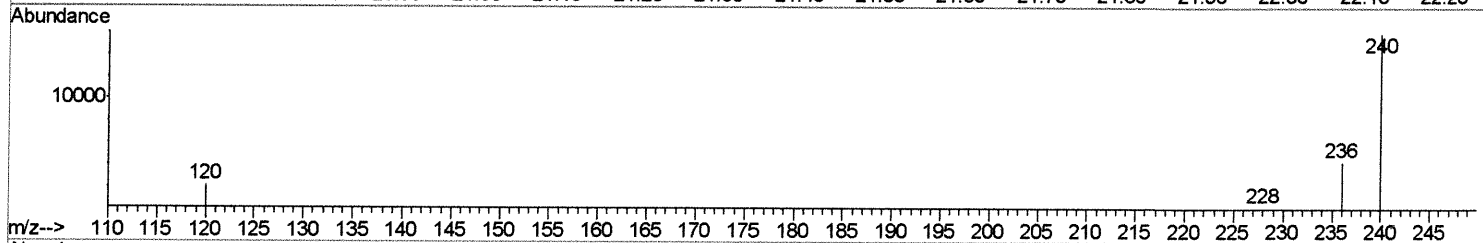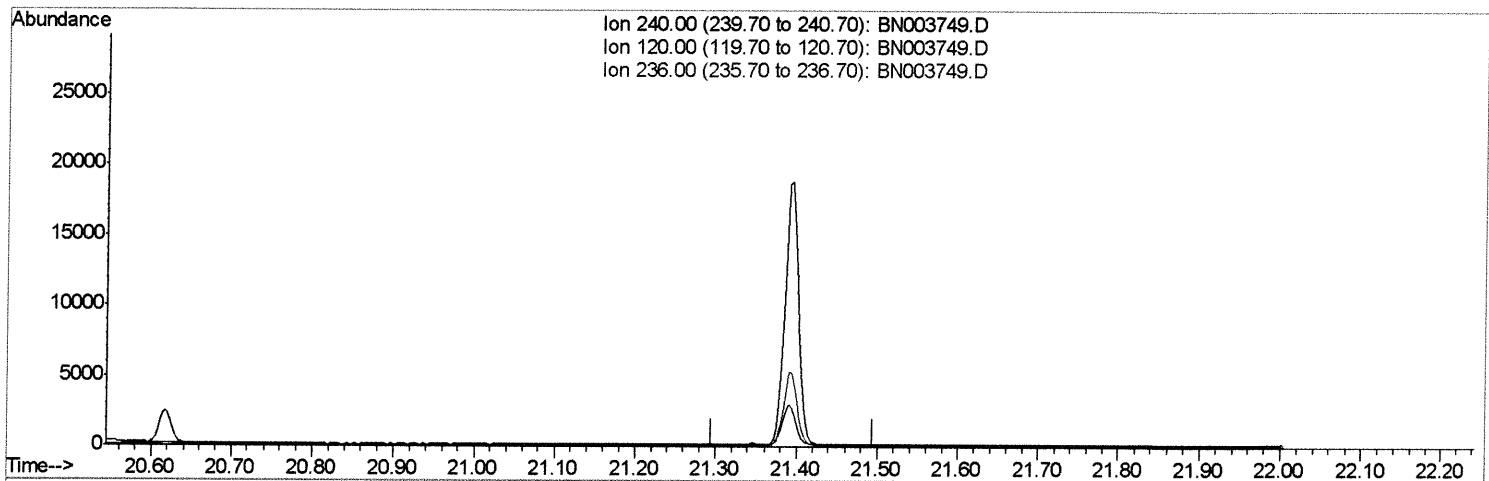

TIC: BN003749.D

(16) Chrysene-d12 (I)

21.395min (-21.395) 0.00ng/ul

response 0

Ion	Exp%	Act%
240.00	100	0.00
120.00	14.00	0.00#
236.00	27.60	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN120618\
Quantitation Report (Qedit)




Data File : BN003749.D
Acq On : 07 Dec 2018 03:00
Operator : JU/SJ
Sample : J6227-10
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E55

Manual Integrations
APPROVED

mohammad
12/10/2018 12:20:52 PM

Quant Time: Dec 07 04:53:23 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 07 04:08:50 2018
Response via : Initial Calibration

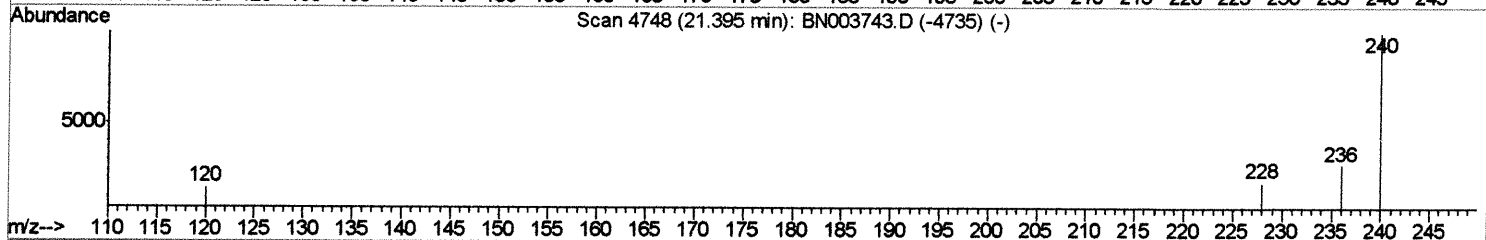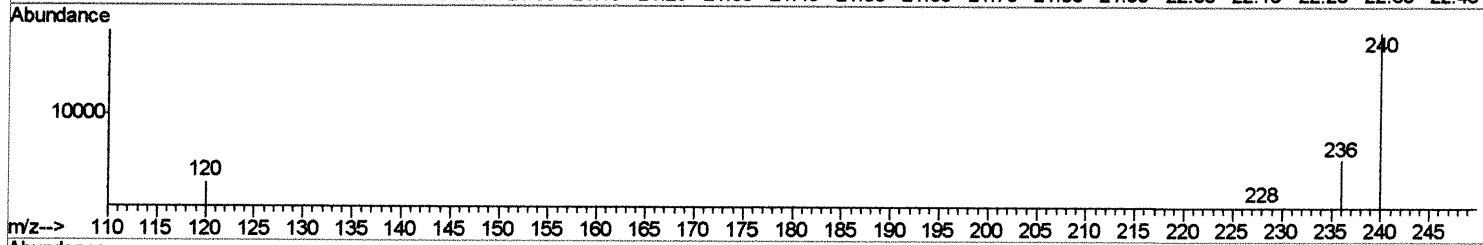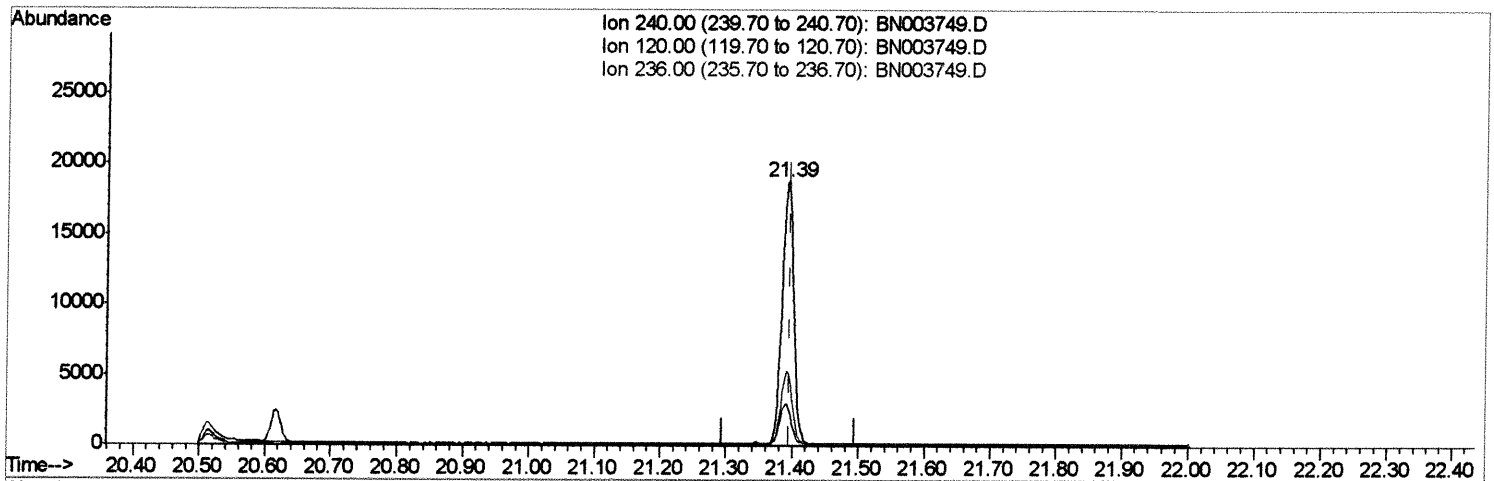

TIC: BN003749.D

(16) Chrysene-d12 (I)

21.394min (-0.002) 0.40ng/ul m

response 23253

Ion	Exp%	Act%
240.00	100	100
120.00	14.00	14.34
236.00	27.60	27.74
0.00	0.00	0.00

> SJ
12/11/18

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN120618\
Quantitation Report (Qedit)




Data File : BN003749.D
Acq On : 07 Dec 2018 03:00
Operator : JU/SJ
Sample : J6227-10
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E55

Manual Integrations
APPROVED

mohammad
12/10/2018 12:20:52 PM

Quant Time: Dec 07 04:54:01 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 07 04:08:50 2018
Response via : Initial Calibration

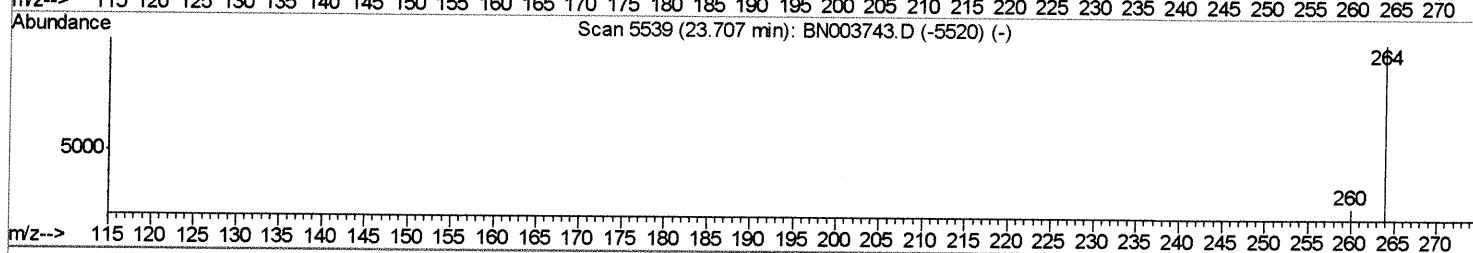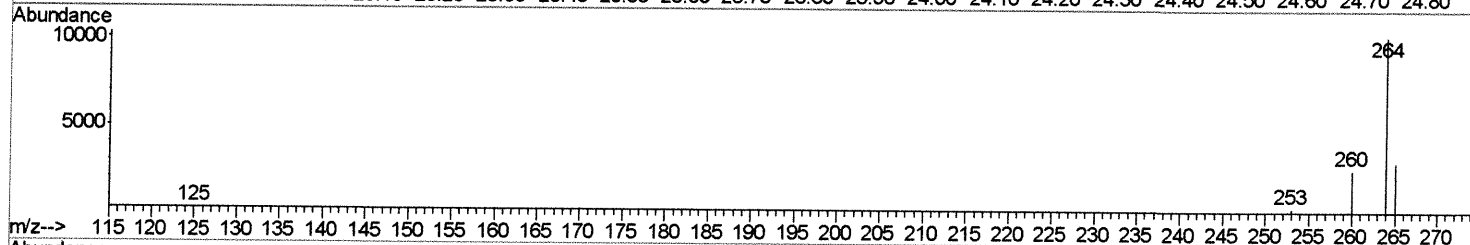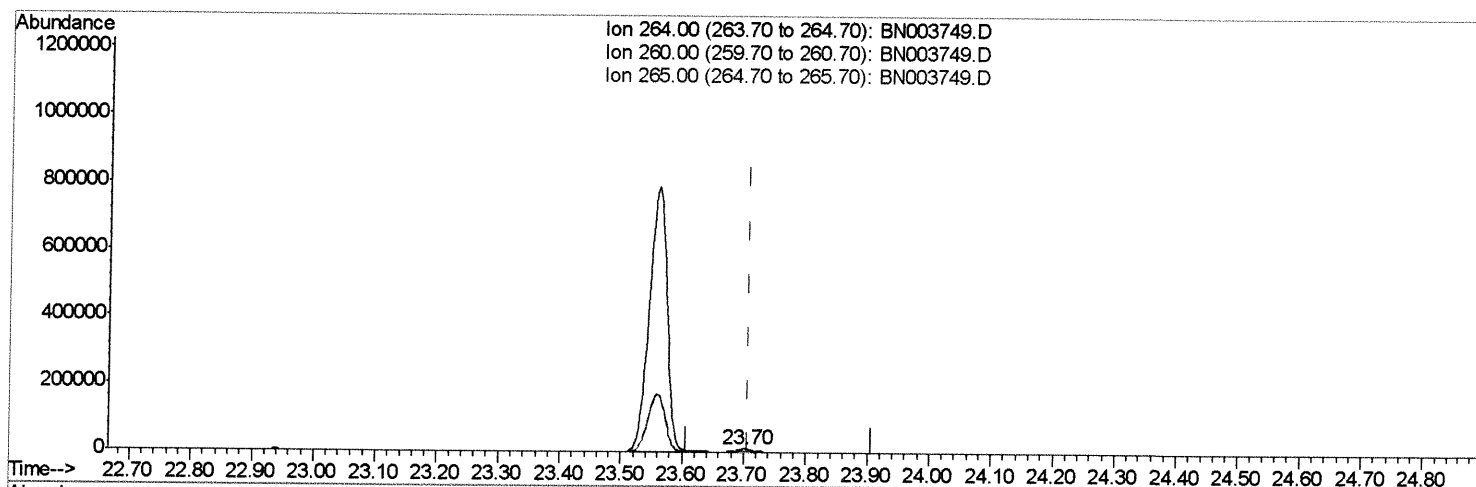

TIC: BN003749.D

(20) Perylene-d12 (I)

23.703min (-0.004) 0.40ng/ul

response 22878

Ion	Exp%	Act%
264.00	100	100
260.00	26.20	25.77
265.00	33.50	29.81
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN120618\
Quantitation Report (Qedit)




Data File : BN003749.D
Acq On : 07 Dec 2018 03:00
Operator : JU/SJ
Sample : J6227-10
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E55

Manual Integrations
APPROVED

mohammad
12/10/2018 12:20:52 PM

Quant Time: Dec 07 04:54:01 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 07 04:08:50 2018
Response via : Initial Calibration

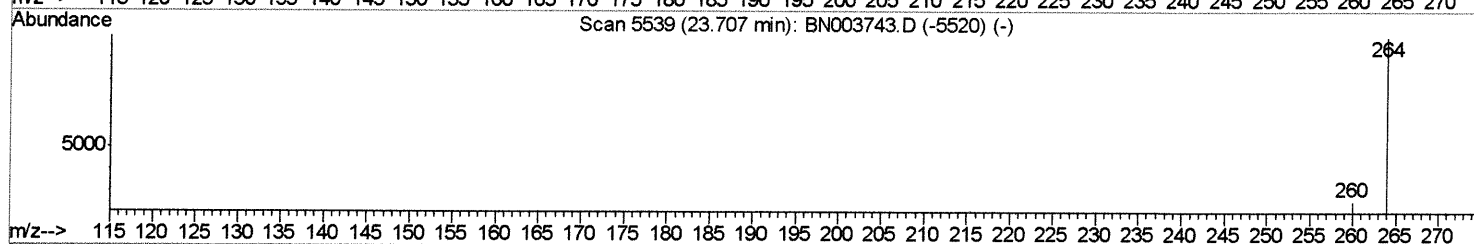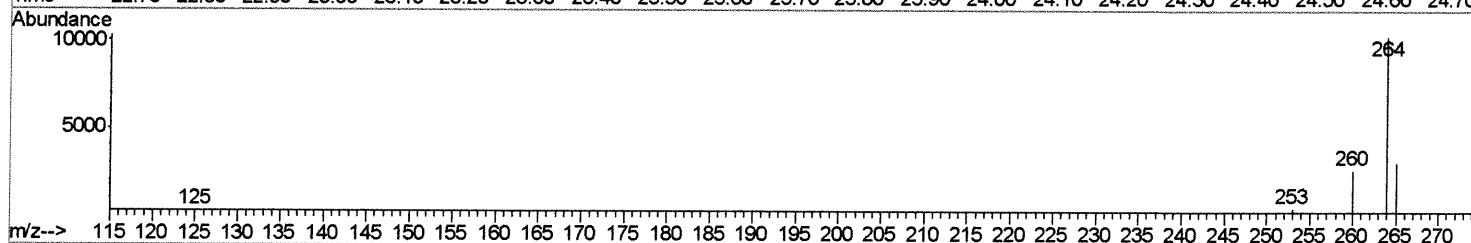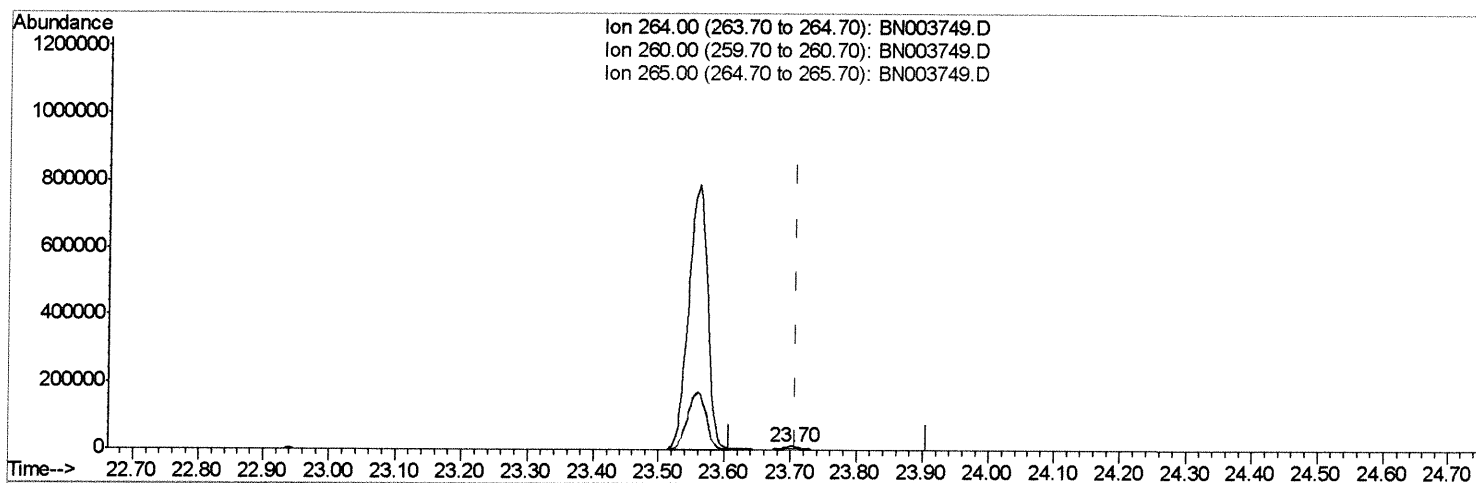

TIC: BN003749.D

(20) Perylene-d12 (I)

23.703min (-0.004) 0.40ng/ul m

response 17729

Ion	Exp%	Act%
264.00	100	100
260.00	26.20	25.77
265.00	33.50	29.81
0.00	0.00	0.00

> SJ
12/11/18

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN120618\
Quantitation Report (QT Reviewed)

Data File : BN003749.D
Acq On : 07 Dec 2018 03:00
Operator : JU/SJ
Sample : J6227-10
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E55

Manual Integrations
APPROVED

mohammad
12/10/2018 12:20:52 PM

Quant Time: Dec 07 04:55:23 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 07 04:08:50 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	5538	0.40	ng/ul	0.00
2) Naphthalene-d8	10.63	136	22965	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.47	164	12823	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.21	188	27422m	0.40	ng/ul	0.00
16) Chrysene-d12	21.39	240	23253m	0.40	ng/ul	0.00
20) Perylene-d12	23.70	264	17729m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.22	152	11320	0.32	ng/ul	0.00
14) Fluoranthene-d10	19.24	212	24621m	0.31	ng/ul	0.00
Target Compounds						
19) Chrysene	21.43	228	1794	0.021	ng/ul#	90

(#) = qualifier out of range (m) = manual integration (+) = signals summed

SS
12/11/18