

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120618\
 Data File : BN003744.D
 Acq On : 07 Dec 2018 00:05
 Operator : JU/SJ
 Sample : J6227-02
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F9E65

Manual Integrations
 APPROVED

mohammad
 12/10/2018 12:20:37 PM

Quant Time: Dec 07 04:18:23 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 07 04:08:50 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	5623	0.40	ng/ul	0.00
2) Naphthalene-d8	10.63	136	22974	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.47	164	12219	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.21	188	26434m	0.40	ng/ul	0.00
16) Chrysene-d12	21.39	240	21109m	0.40	ng/ul	0.00
20) Perylene-d12	23.70	264	15742m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.22	152	6456	0.18	ng/ul	0.00
14) Fluoranthene-d10	19.24	212	13547m	0.18	ng/ul	0.00
Target Compounds						
15) Fluoranthene	19.27	202	2137m	0.021	ng/ul	Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120618\
Data File : BN003744.D
Acq On : 07 Dec 2018 00:05
Operator : JU/SJ
Sample : J6227-02
Misc :
ALS Vial : 15 Sample Multiplier: 1




Instrument :
BNA_N
ClientSampleId :
F9E65

Quant Time: Dec 07 04:18:23 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 07 04:08:50 2018
Response via : Initial Calibration

Manual Integrations
APPROVED

mohammad
12/10/2018 12:20:37 PM

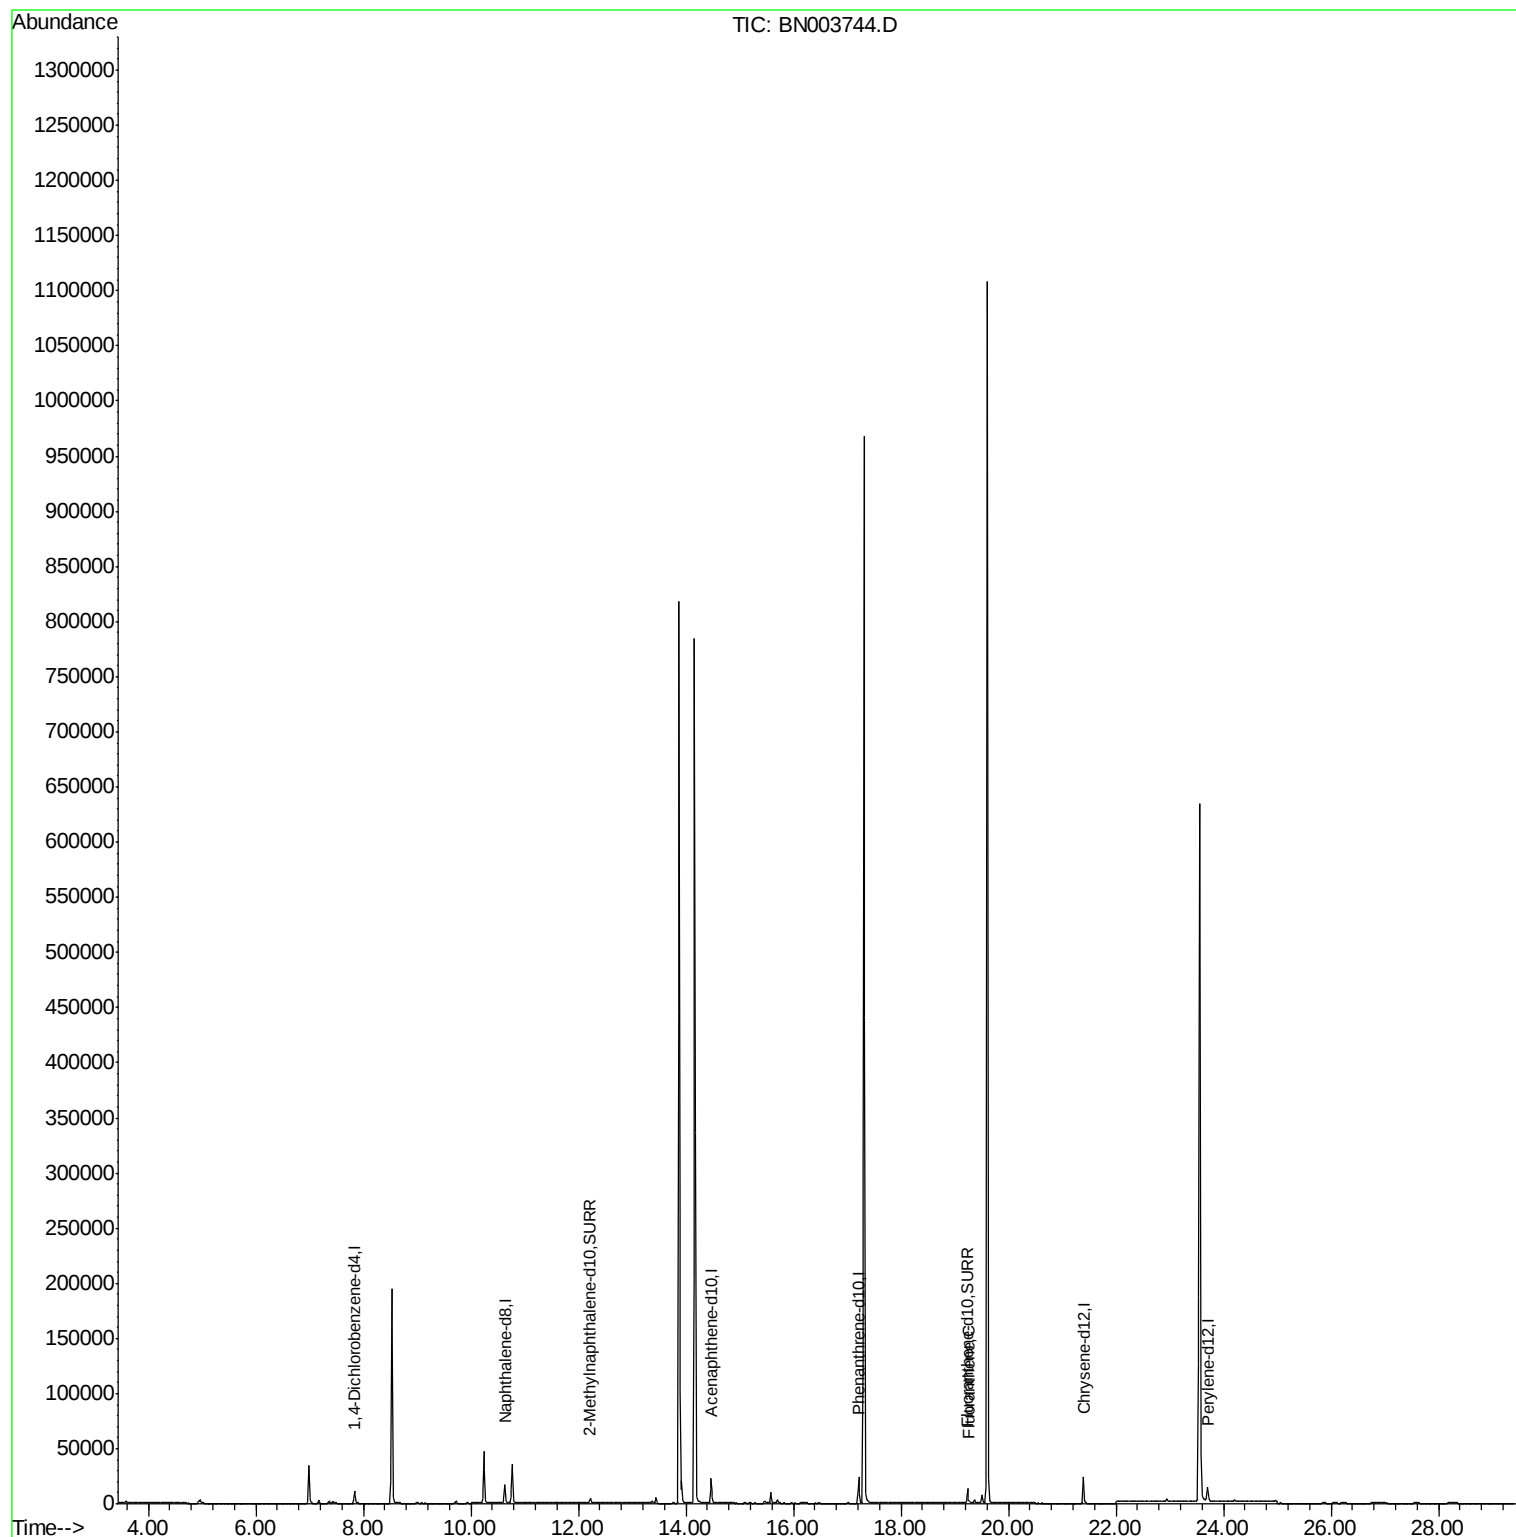

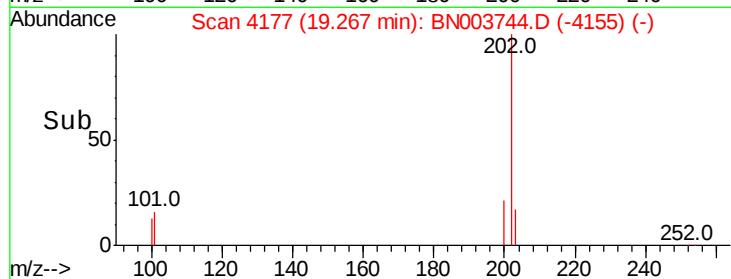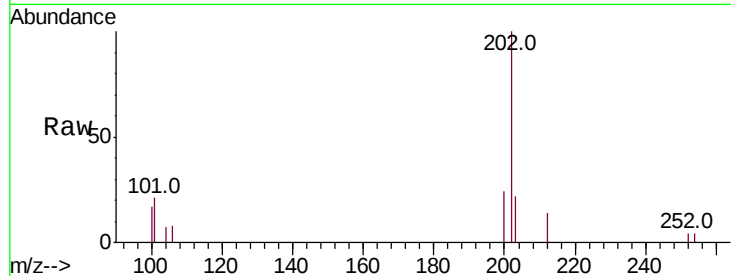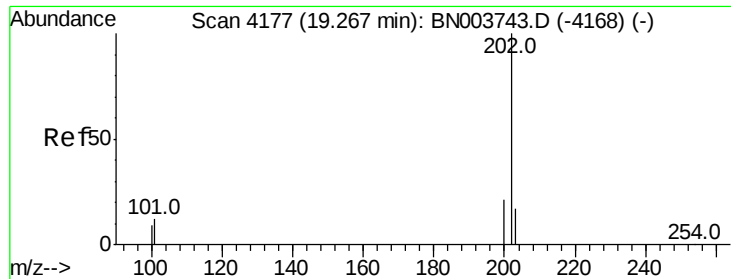

#15

Fluoranthene

Concen: 0.021 ng/ul m

RT: 19.27 min Scan# 4177

Delta R.T. 0.00 min

Lab File: BN003744.D

Acq: 07 Dec 2018 00:05

Instrument :

BNA_N

ClientSampleId :

F9E65

Tot Ion:	202	Resp:	2137
Ion Ratio	Lower	Upper	
202	100		
101	20.5	0.0	30.7
100	17.1	0.0	28.1

Manual Integrations
APPROVED

mohammad
12/10/2018 12:20:37 PM

