

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120619\
 Data File : BN008872.D
 Acq On : 06 Dec 2019 22:36
 Operator : JU
 Sample : K6007-14
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Dec 07 01:37:28 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 06 23:00:12 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	3002	0.40	ng/ul	0.00
2) Naphthalene-d8	10.32	136	13327	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.19	164	9033	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.94	188	20208	0.40	ng/ul	0.00
16) Chrysene-d12	21.14	240	17986	0.40	ng/ul	0.00
20) Perylene-d12	23.28	264	20172	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.92	152	4893	0.22	ng/ul	0.00
14) Fluoranthene-d10	18.97	212	12521	0.20	ng/ul	0.00
Target Compounds						
17) Pyrene	19.34	202	2027	0.028	ng/ul#	1
23) Benzo(a)pyrene	23.16	252	4108	0.053	ng/ul#	53


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120619\
Data File : BN008872.D
Acq On : 06 Dec 2019 22:36
Operator : JU
Sample : K6007-14
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Dec 07 01:37:28 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN11519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 06 23:00:12 2019
Response via : Initial Calibration

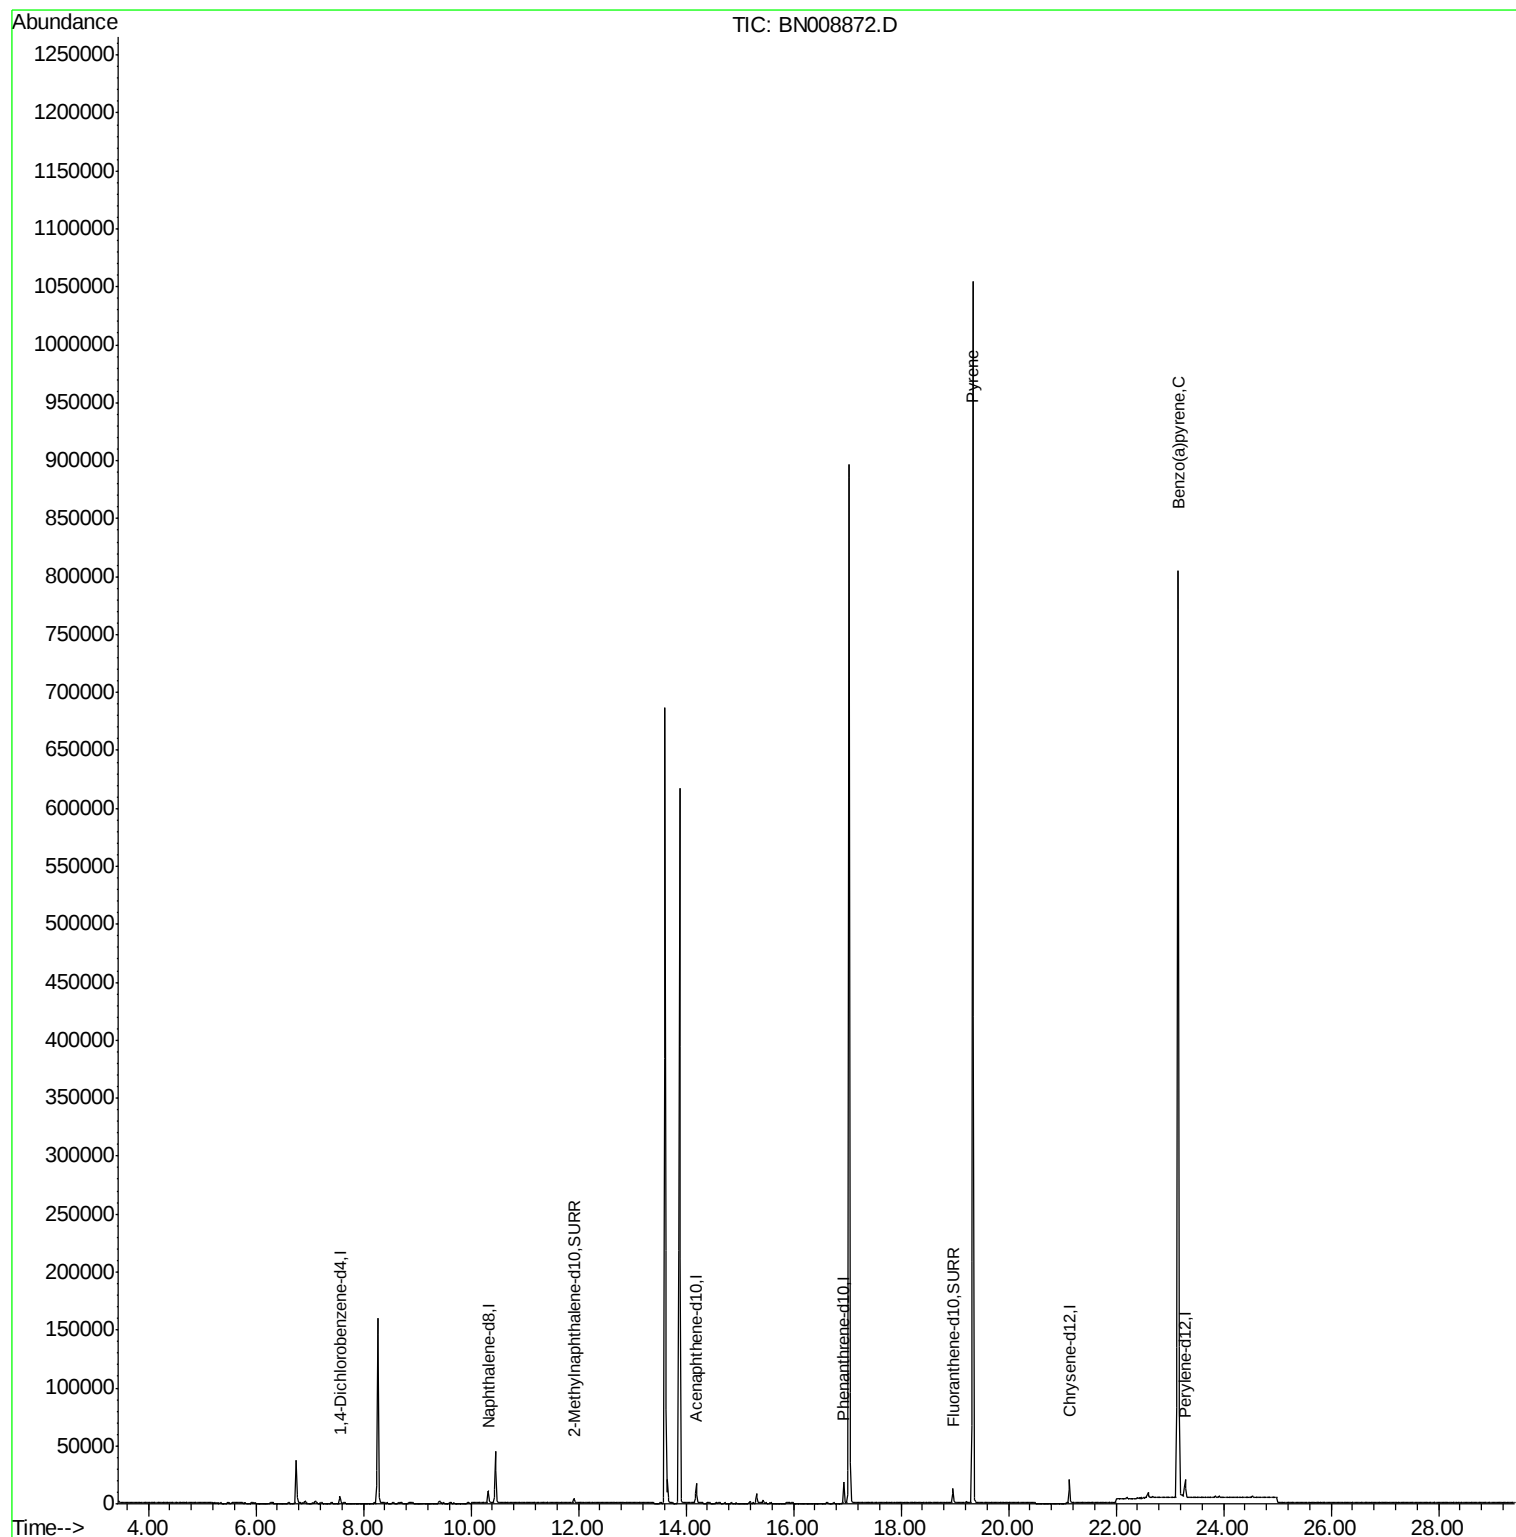


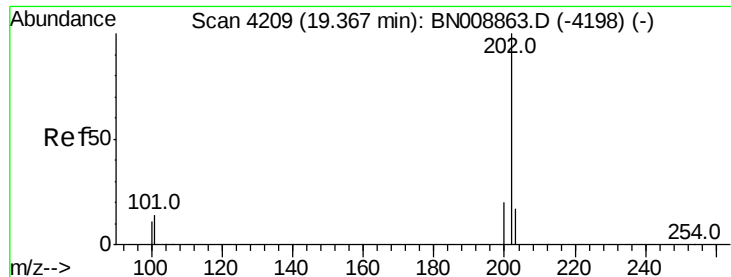




#17
Pvrene
Concen: 0.028 ng/ul
RT: 19.34 min Scan# 4203
Delta R.T. -0.03 min
Lab File: BN008872.D
Acq: 06 Dec 2019 22:36

Instrument :
BNA_N
ClientSampleId :

Tot Ion:202 Resp: 2027
Ion Ratio Lower Upper
202 100
101 160.1 12.2 18.4#
100 1023.8 9.5 14.3#

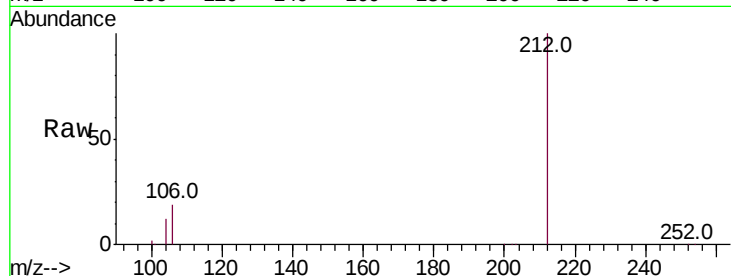


Abundance Ion 202.00 (201.70 to 202.70): E
Ion 101.00 (100.70 to 101.70): E
Ion 100.00 (99.70 to 100.70): B

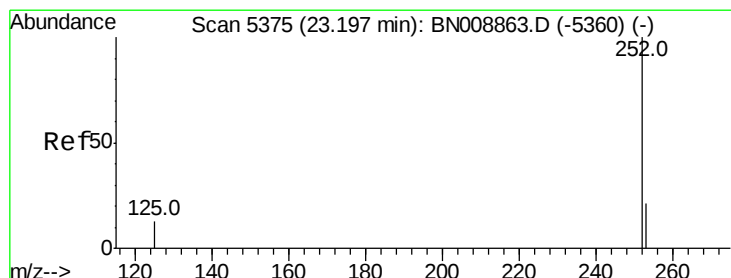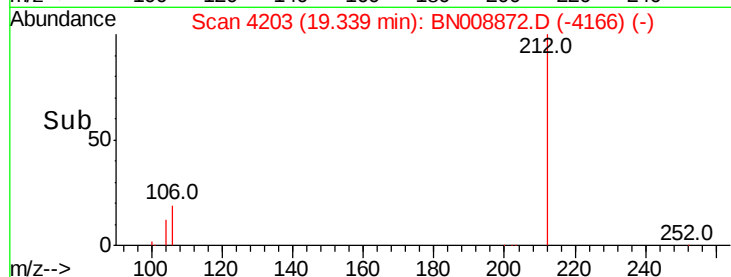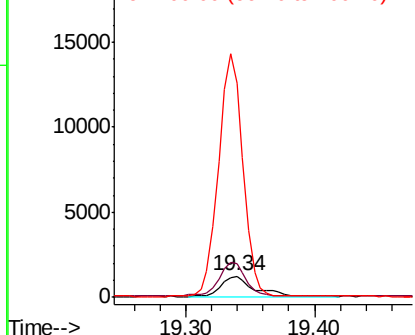

#23
Benzo(a)pyrene
Concen: 0.053 ng/ul
RT: 23.16 min Scan# 5361
Delta R.T. -0.04 min
Lab File: BN008872.D
Acq: 06 Dec 2019 22:36

Tgt Ion:252 Resp: 4108
Ion Ratio Lower Upper
252 100
253 43.0 19.9 29.9#
125 46.2 14.6 22.0#

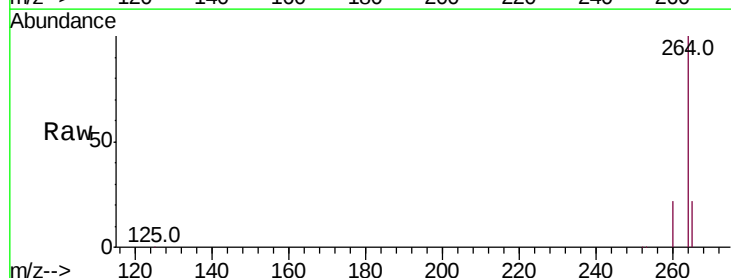

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

