


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120619\
Data File : BN008855.D
Acq On : 06 Dec 2019 12:28
Operator : JU
Sample : PB125156BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK56

Manual Integrations
APPROVED

mohammad
12/9/2019 3:06:48 PM

Quant Time: Dec 06 14:49:28 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 06 12:03:45 2019
Response via : Initial Calibration

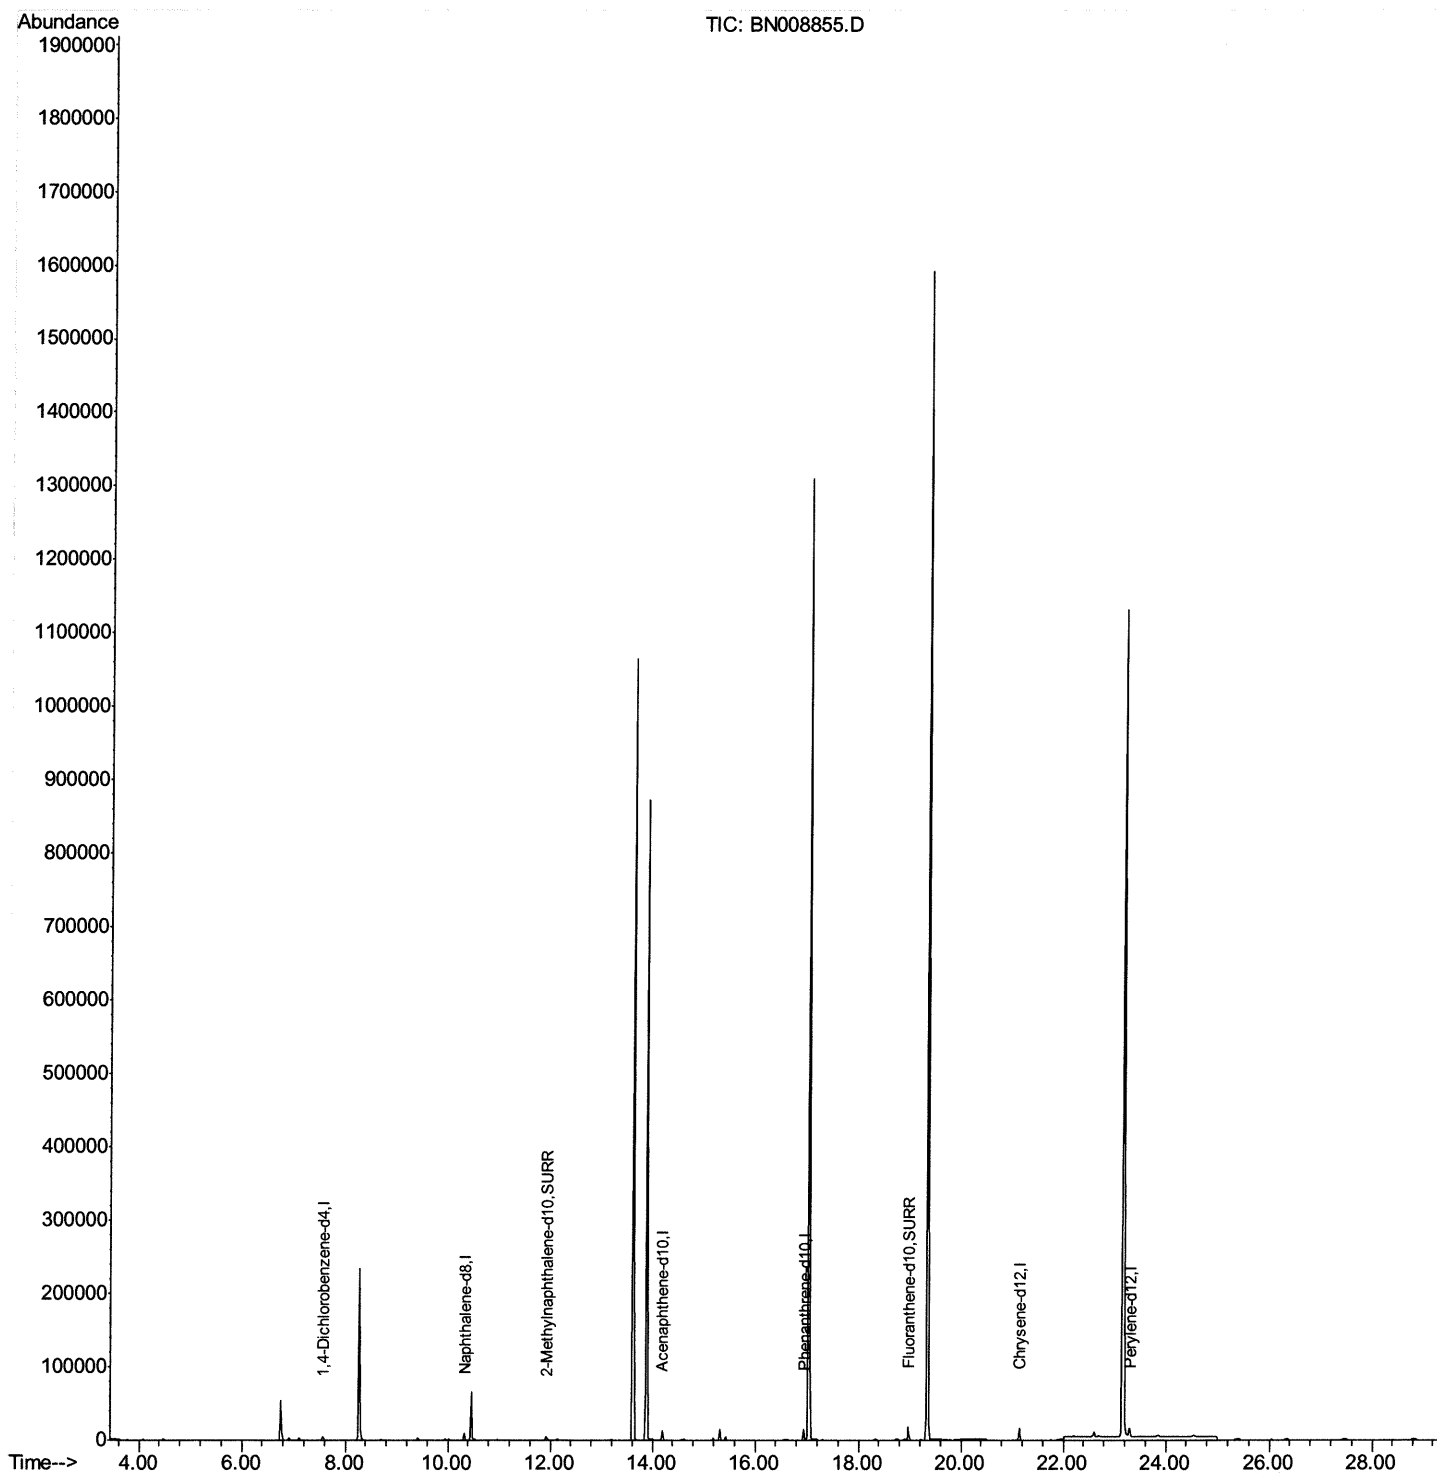

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120619\
 Data File : BN008855.D
 Acq On : 06 Dec 2019 12:28
 Operator : JU
 Sample : PB125156BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK56

Manual Integrations
 APPROVED

mohammad
 12/9/2019 3:06:48 PM

Quant Time: Dec 06 14:46:46 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 06 12:03:45 2019
 Response via : Initial Calibration

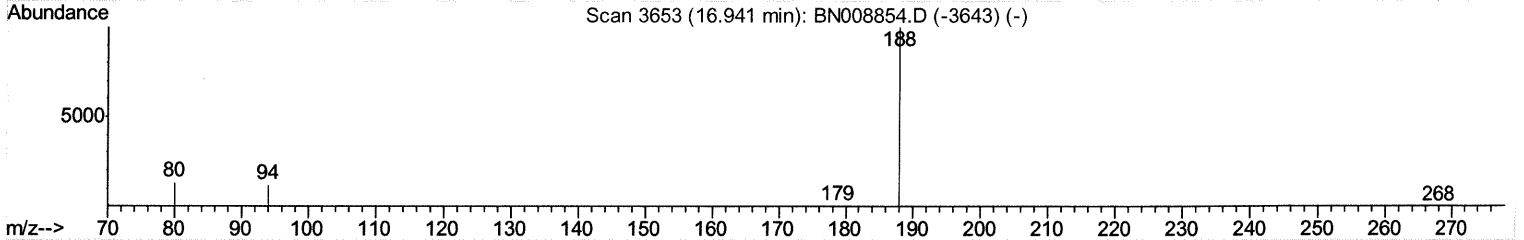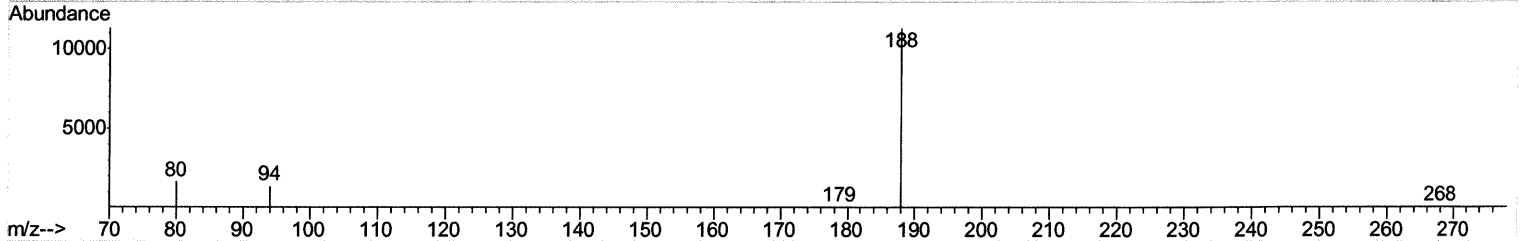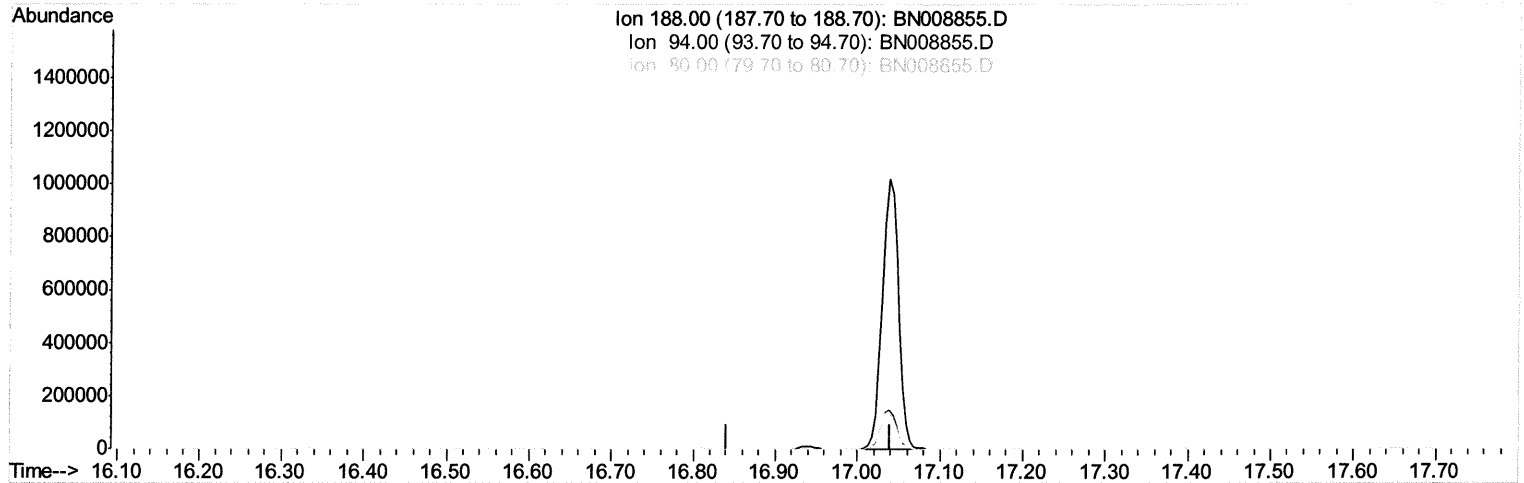

TIC: BN008855.D

(10) Phenanthrene-d10 (I)

16.941min (-16.941) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	12.20	0.00#
80.00	14.40	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120619\
 Data File : BN008855.D
 Acq On : 06 Dec 2019 12:28
 Operator : JU
 Sample : PB125156BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK56

Manual Integrations
 APPROVED

mohammad
 12/9/2019 3:06:48 PM

Quant Time: Dec 06 14:46:46 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 06 12:03:45 2019
 Response via : Initial Calibration

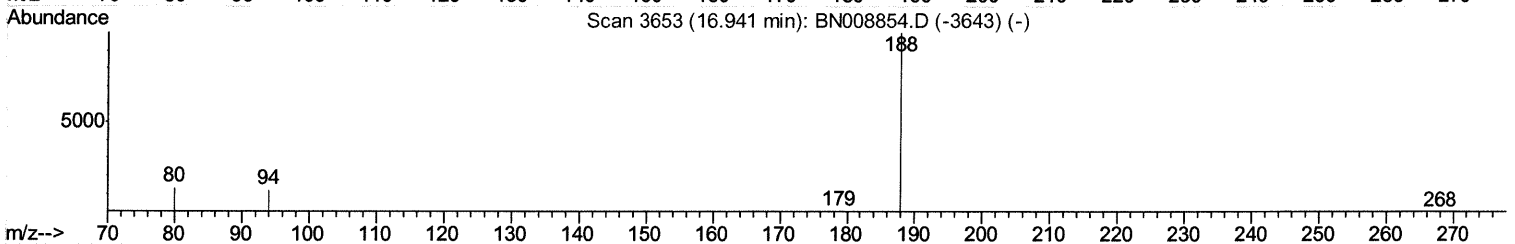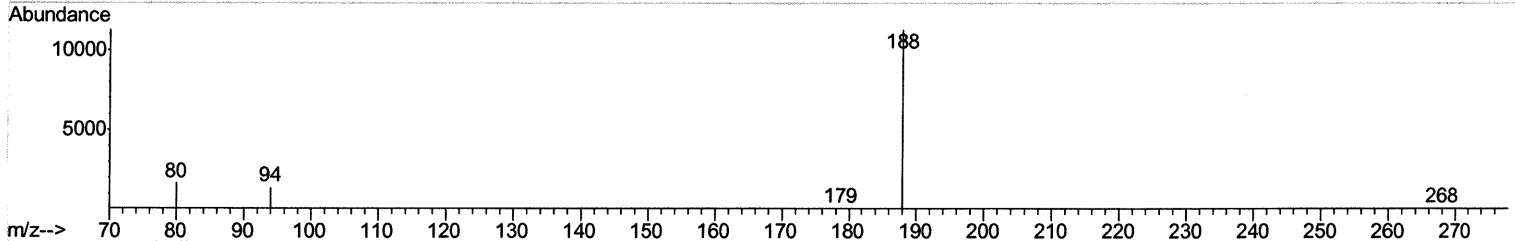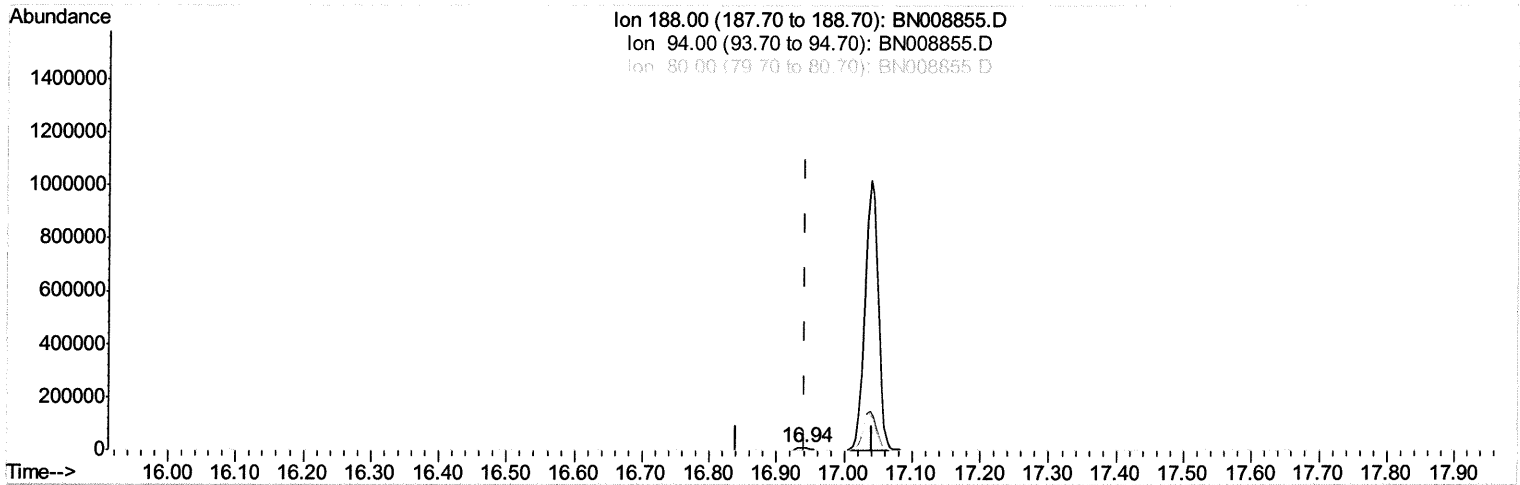

(10) Phenanthrene-d10 (I)

16.941min (-0.000) 0.40ng/ul m JU 12/10/19

response 15226

Ion	Exp%	Act%
188.00	100	100
94.00	12.20	12.35
80.00	14.40	14.44
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120619\
 Data File : BN008855.D
 Acq On : 06 Dec 2019 12:28
 Operator : JU
 Sample : PB125156BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK56

Manual Integrations
 APPROVED

mohammad
 12/9/2019 3:06:48 PM

Quant Time: Dec 06 14:49:28 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 06 12:03:45 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	2465	0.40	ng/ul	0.00
2) Naphthalene-d8	10.32	136	10775	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.19	164	6805	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.94	188	15226m	0.40	ng/ul	0.00
16) Chrysene-d12	21.14	240	13533	0.40	ng/ul	0.00
20) Perylene-d12	23.30	264	15114	0.40	ng/ul	0.00

JU 12/10/19

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	11.92	152	6930	0.39	ng/ul	0.00
14) Fluoranthene-d10	18.97	212	18773	0.40	ng/ul	0.00

Target Compounds

Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed