


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120619\
Data File : BN008878.D
Acq On : 07 Dec 2019 02:10
Operator : JU
Sample : K6007-20
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0BM6

Manual Integrations
APPROVED

mohammad
12/9/2019 3:08:21 PM

Quant Time: Dec 07 02:48:14 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 06 23:00:12 2019
Response via : Initial Calibration

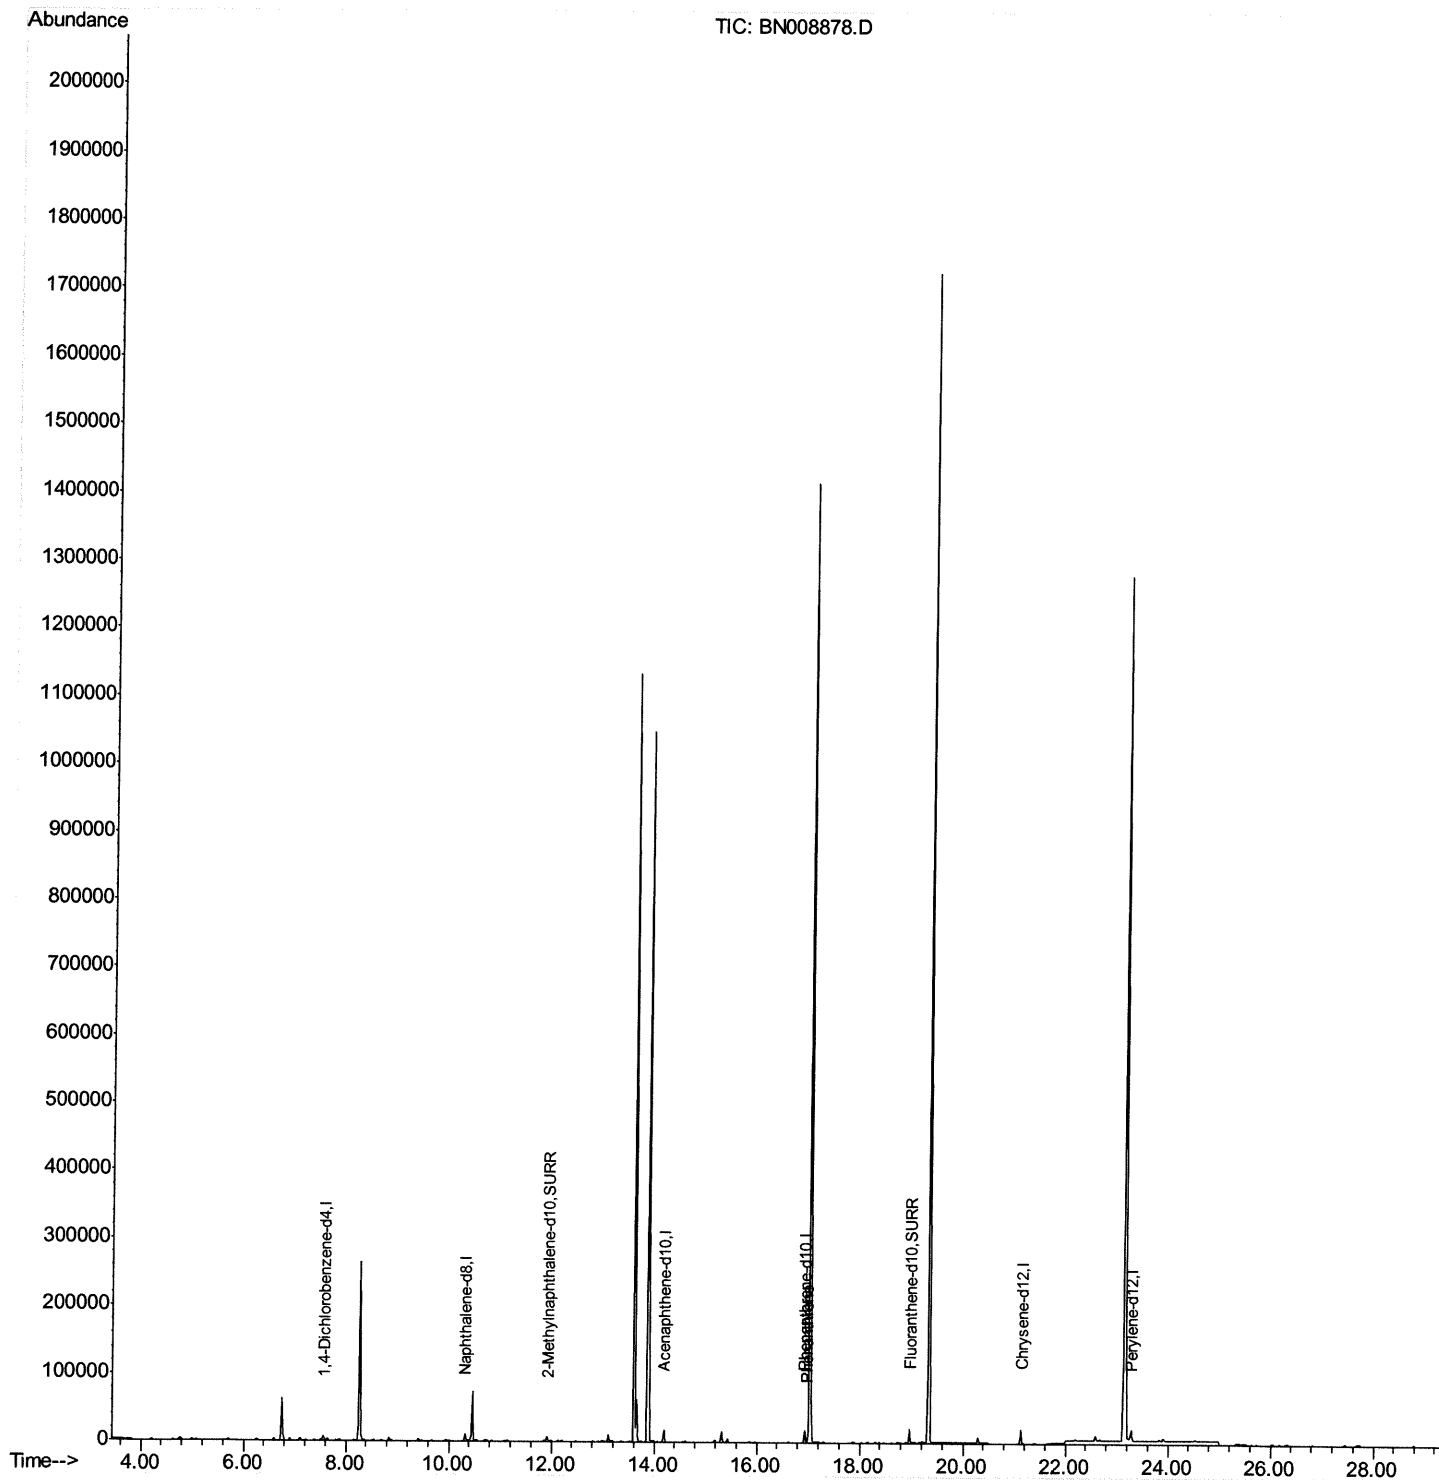

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120619\
 Data File : BN008878.D
 Acq On : 07 Dec 2019 02:10
 Operator : JU
 Sample : K6007-20
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_N
ClientSampleId :
 C0BM6

Manual Integrations
APPROVED

mohammad
 12/9/2019 3:08:21 PM

Quant Time: Dec 07 02:46:42 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 06 23:00:12 2019
 Response via : Initial Calibration

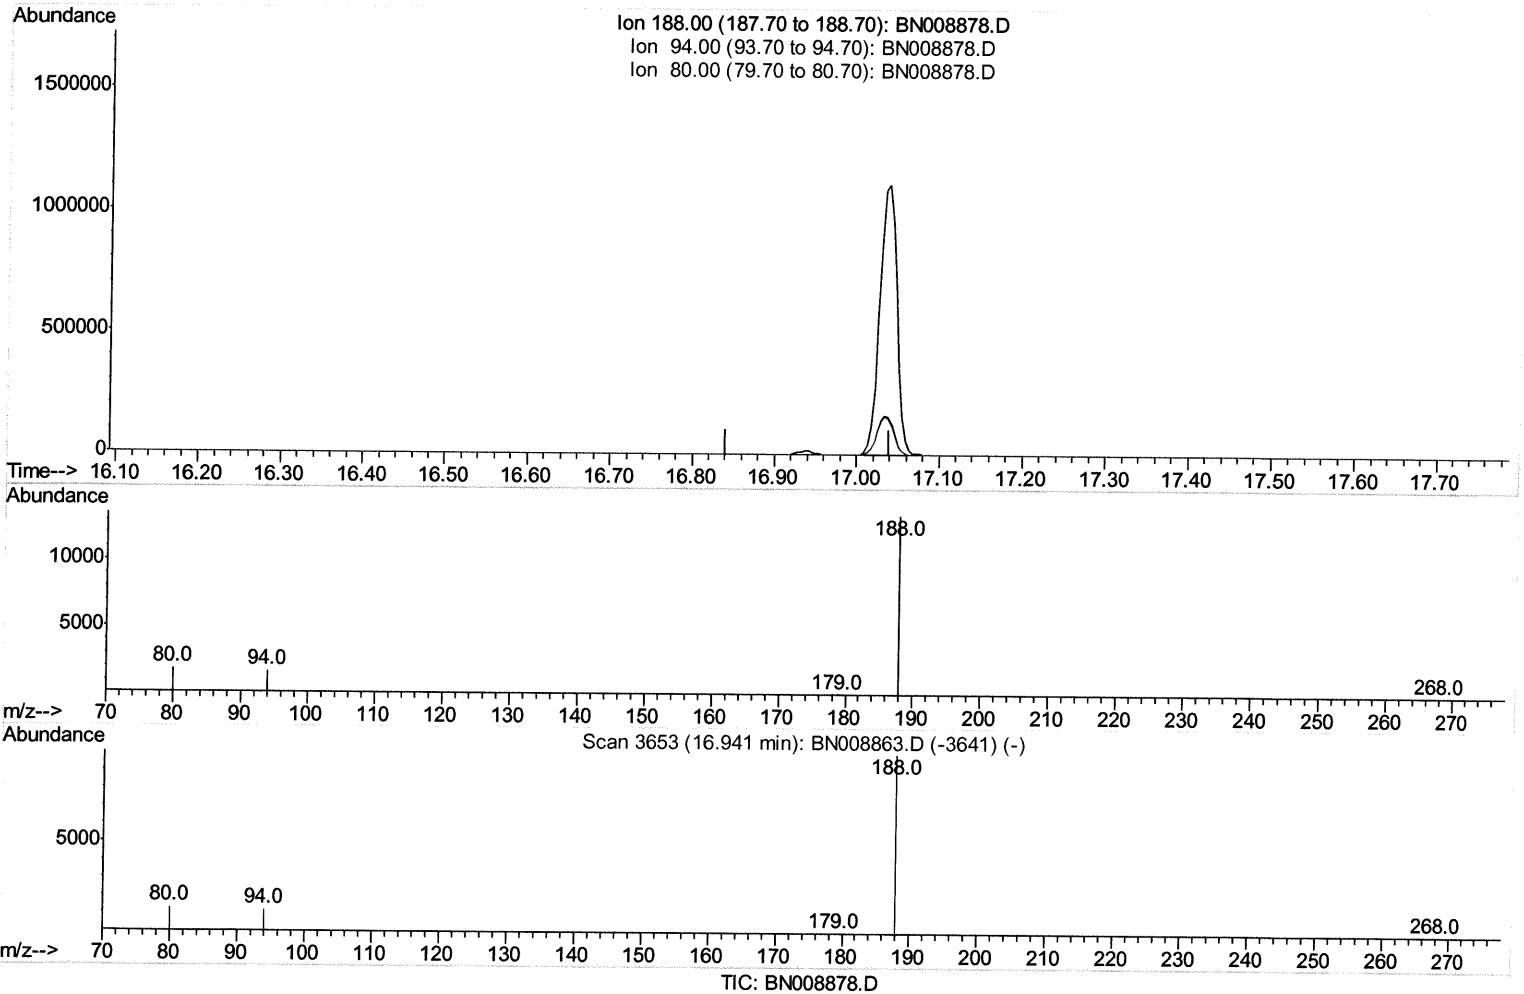

(10) Phenanthrene-d10 (I)

16.941min (-16.941) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	12.20	0.00#
80.00	14.40	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120619\
 Data File : BN008878.D
 Acq On : 07 Dec 2019 02:10
 Operator : JU
 Sample : K6007-20
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0BM6

Manual Integrations
 APPROVED

mohammad
 12/9/2019 3:08:21 PM

Quant Time: Dec 07 02:46:42 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 06 23:00:12 2019
 Response via : Initial Calibration

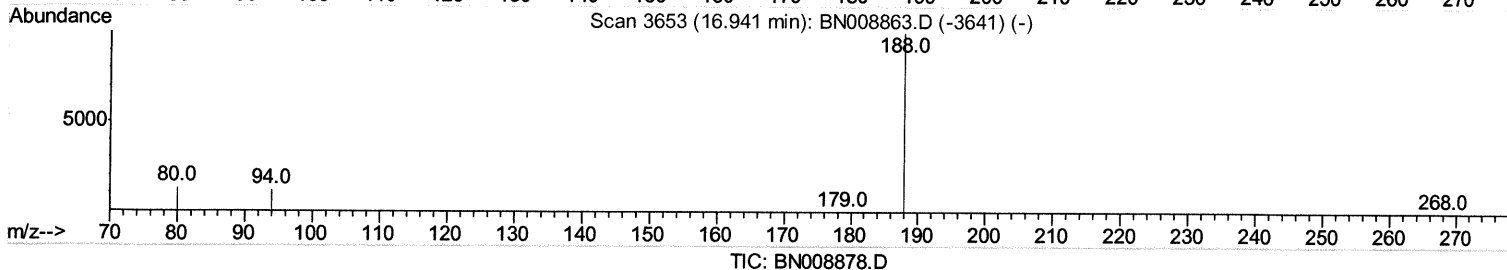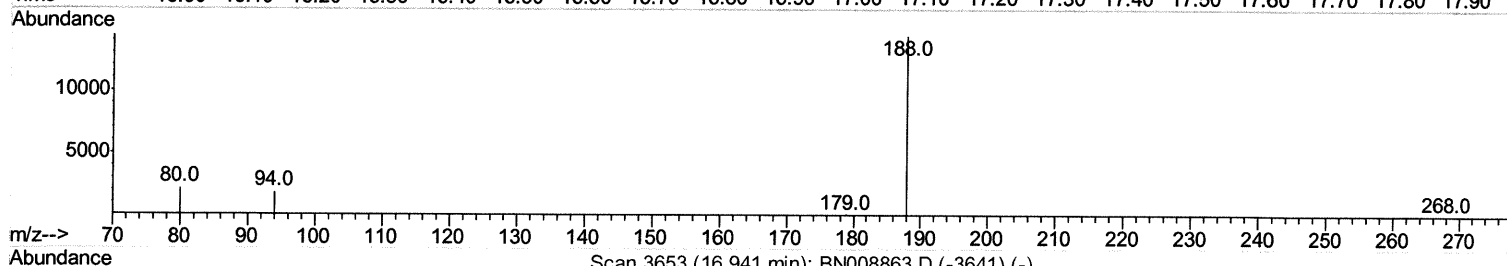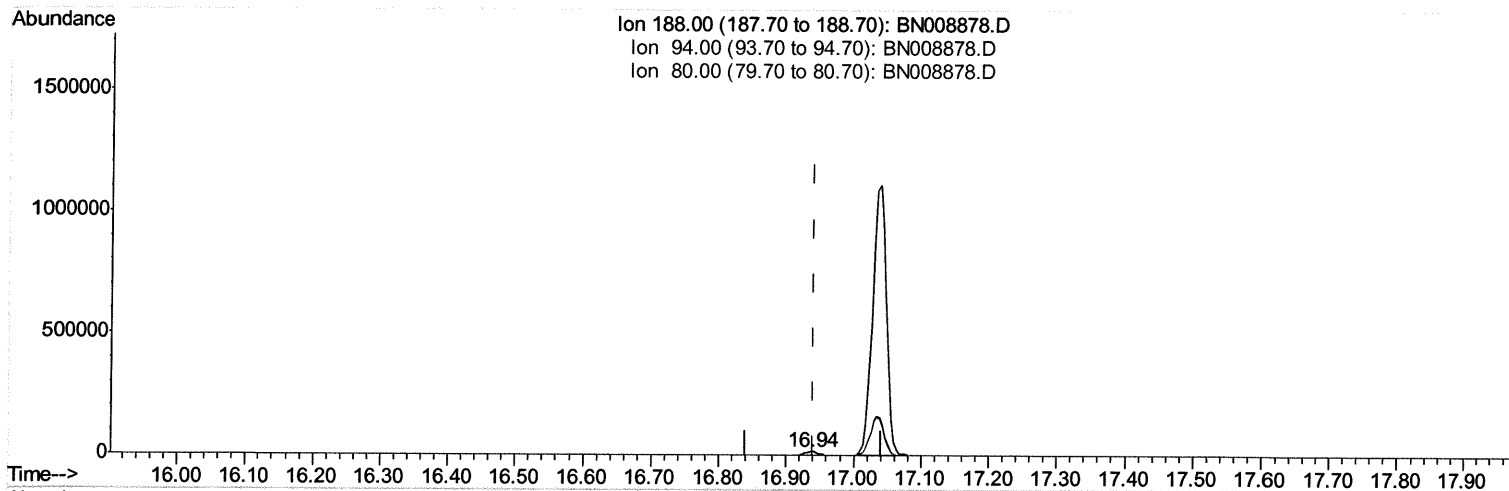

TIC: BN008878.D

(10) Phenanthrene-d10 (I)

16.937min (-0.004) 0.40ng/ul m JU 12/10/19

response 20177

Ion	Exp%	Act%
188.00	100	100
94.00	12.20	12.75
80.00	14.40	14.79
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120619\
 Data File : BN008878.D
 Acq On : 07 Dec 2019 02:10
 Operator : JU
 Sample : K6007-20
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0BM6

Manual Integrations
 APPROVED

mohammad
 12/9/2019 3:08:21 PM

Quant Time: Dec 07 02:48:14 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 06 23:00:12 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	2794	0.40	ng/ul	0.00
2) Naphthalene-d8	10.32	136	12957	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.19	164	8964	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.94	188	20177m >	0.40	ng/ul >	0.00
16) Chrysene-d12	21.14	240	18192	0.40	ng/ul	0.00
20) Perylene-d12	23.28	264	20204	0.40	ng/ul	0.00

Jul 12/10/19

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	11.92	152	8346	0.39	ng/ul	0.00
14) Fluoranthene-d10	18.97	212	22782	0.37	ng/ul	0.00

Target Compounds

				Ovalue
12) Phenanthrene	16.98	178	1557	0.023 ng/ul# 89

(#) = qualifier out of range (m) = manual integration (+) = signals summed