


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120623\
 Data File : BN029050.D
 Acq On : 06 Dec 2023 09:04
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN120523.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 06 00:49:47 2023

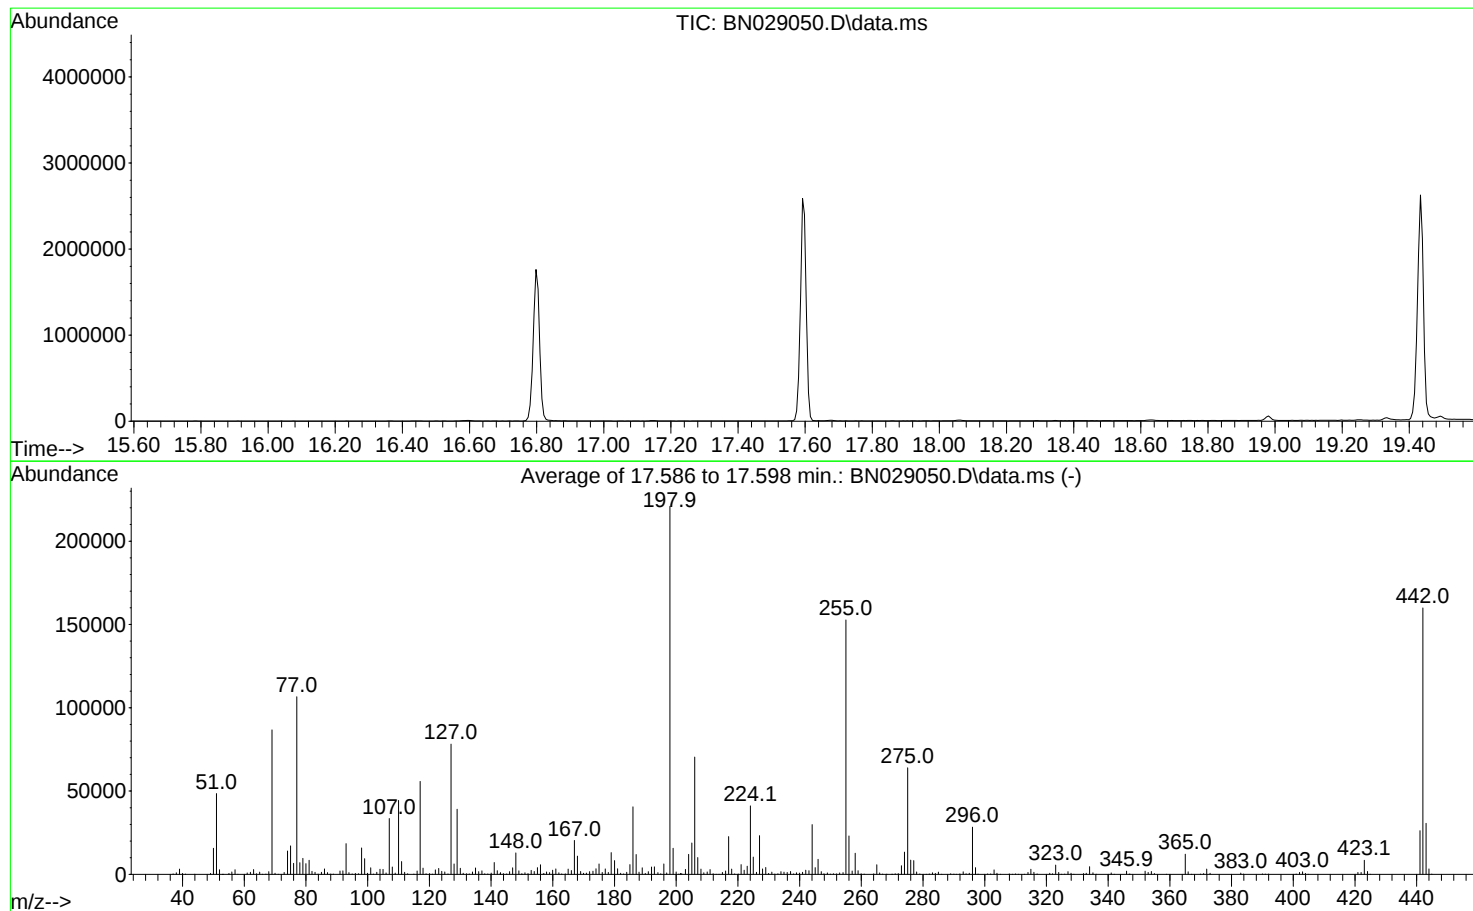




AutoFind: Scans 2465, 2466, 2467; Background Corrected with Scan 2458

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	22.0	48491	PASS
68	69	0.00	2	1.9	1661	PASS
69	198	0.00	100	39.3	86691	PASS
70	69	0.00	2	0.8	708	PASS
127	198	10	80	35.4	78160	PASS
197	198	0.00	2	0.4	876	PASS
198	198	100	100	100.0	220800	PASS
199	198	5	9	7.1	15623	PASS
275	198	10	60	29.0	63981	PASS
365	198	1	100	5.5	12117	PASS
441	198	0.01	100	11.9	26267	PASS
442	442	50	100	100.0	159936	PASS
443	442	15	24	19.2	30666	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120623\
 Data File : BN029050.D
 Acq On : 06 Dec 2023 09:04
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Dec 07 01:46:45 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 01 23:28:24 2023
 Response via : Initial Calibration

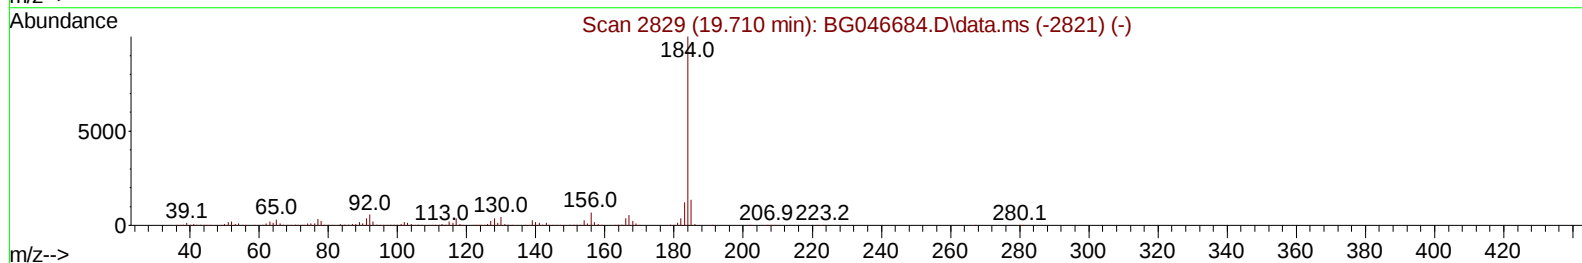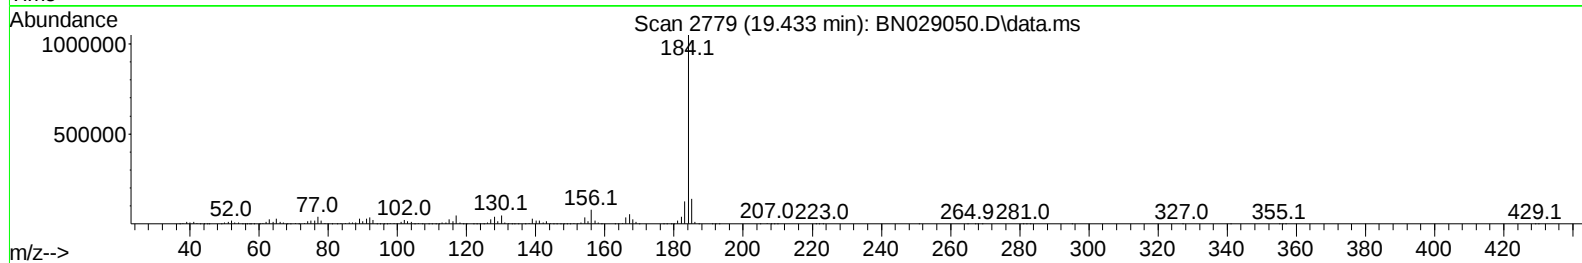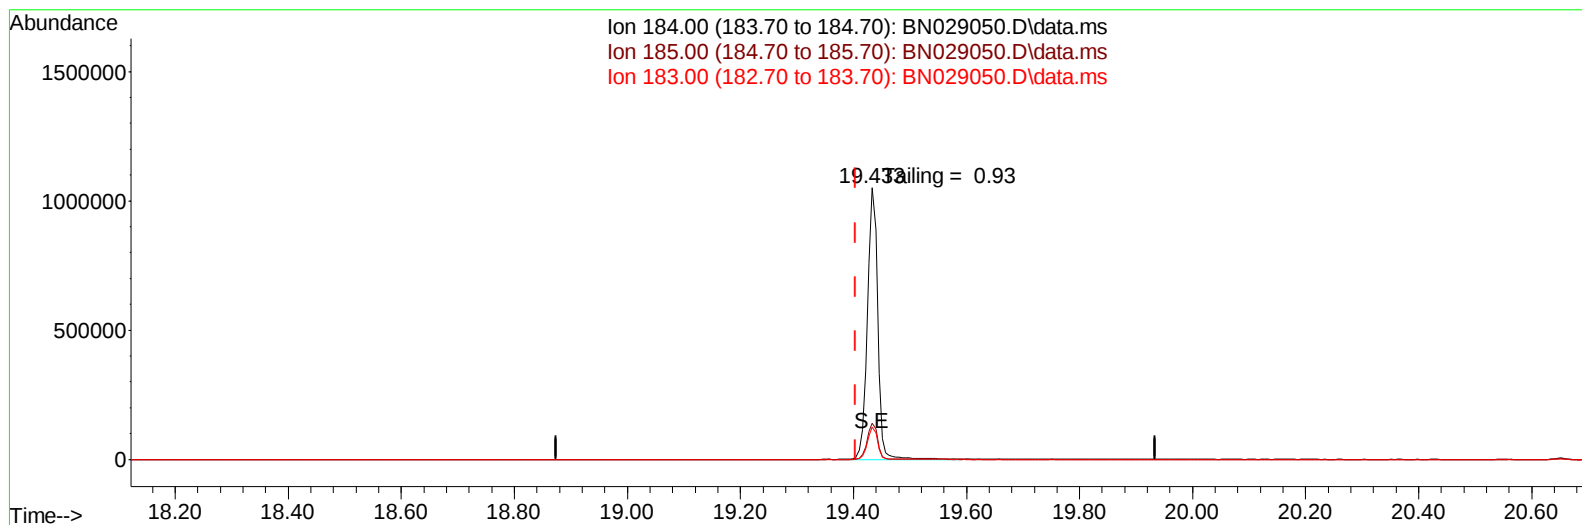

TIC: BN029050.D\data.ms

(77) Benzidine

19.433min (+ 0.029) 0.00 ng

response 1336369

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.38
183.00	13.20	11.91
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/6/2023	BNA_N	<u>BN029050.D</u>
Compound Name	Response	Retention Time
DDT	797316	20.651
DDD	32292	20.21
DDE	532	19.704
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
32824	830140	3.95

Instrument :
BNA_N
ClientSampleId :
DFTPP