
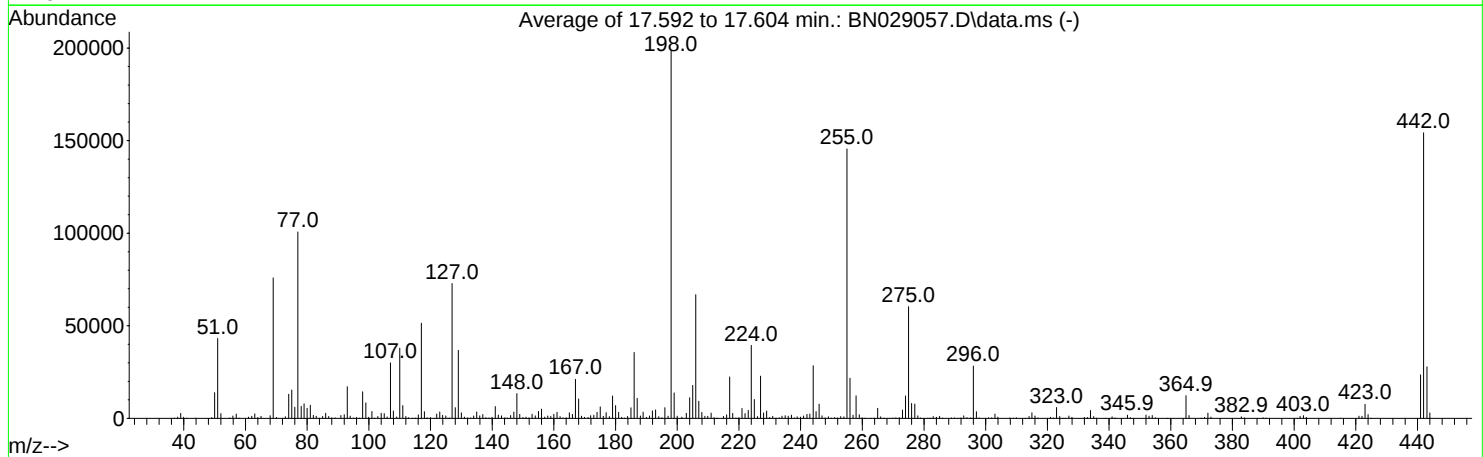


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120623\
Data File : BN029057.D
Acq On : 06 Dec 2023 16:01
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN120523.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Dec 06 00:49:47 2023

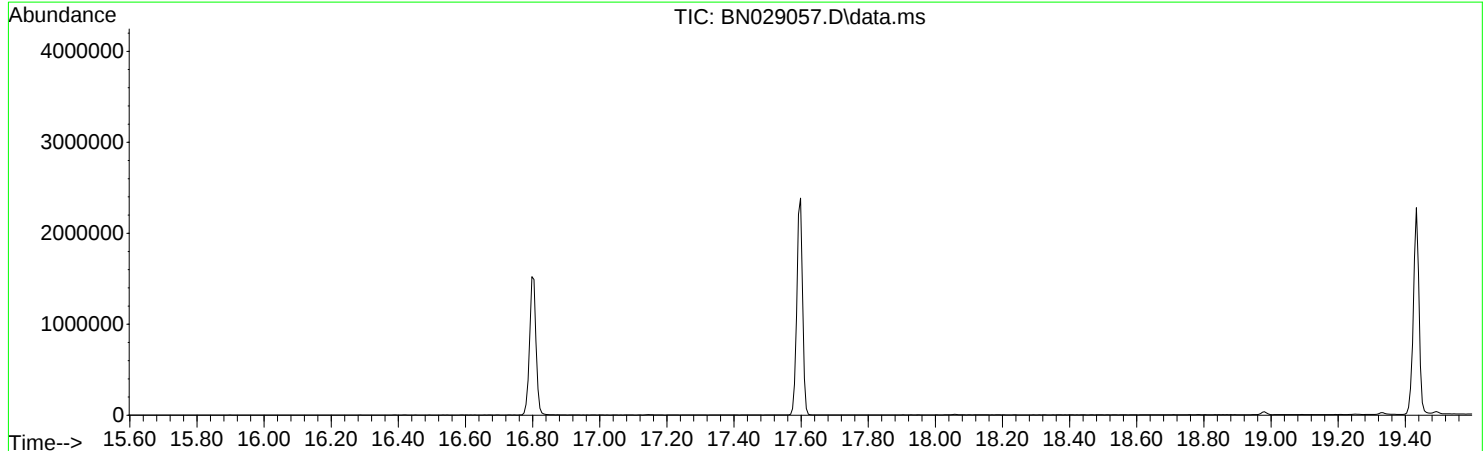




AutoFind: Scans 2466, 2467, 2468; Background Corrected with Scan 2459

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	21.7	43152	PASS
68	69	0.00	2	1.9	1464	PASS
69	198	0.00	100	38.2	75880	PASS
70	69	0.00	2	0.7	549	PASS
127	198	10	80	36.7	72864	PASS
197	198	0.00	2	0.6	1183	PASS
198	198	100	100	100.0	198667	PASS
199	198	5	9	6.9	13736	PASS
275	198	10	60	30.4	60331	PASS
365	198	1	100	6.2	12234	PASS
441	198	0.01	100	11.8	23533	PASS
442	442	50	100	100.0	154261	PASS
443	442	15	24	18.0	27795	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120623\
Data File : BN029057.D
Acq On : 06 Dec 2023 16:01
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 07 01:51:21 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 01 23:28:24 2023
Response via : Initial Calibration

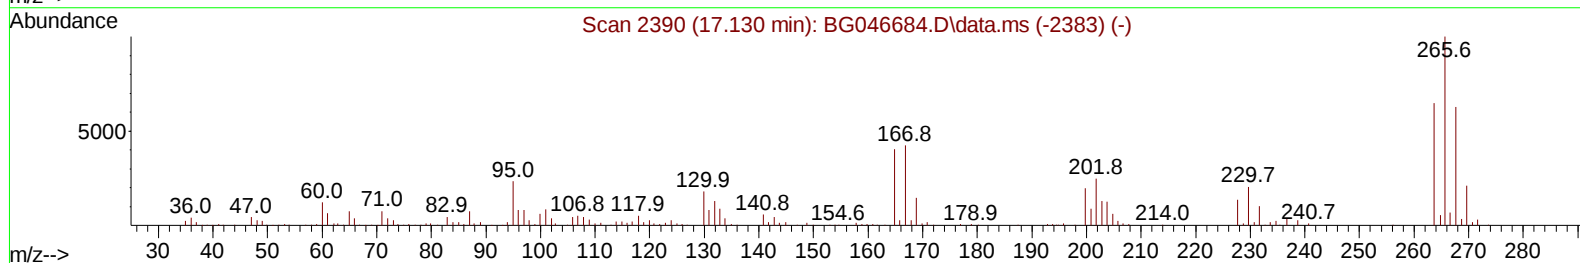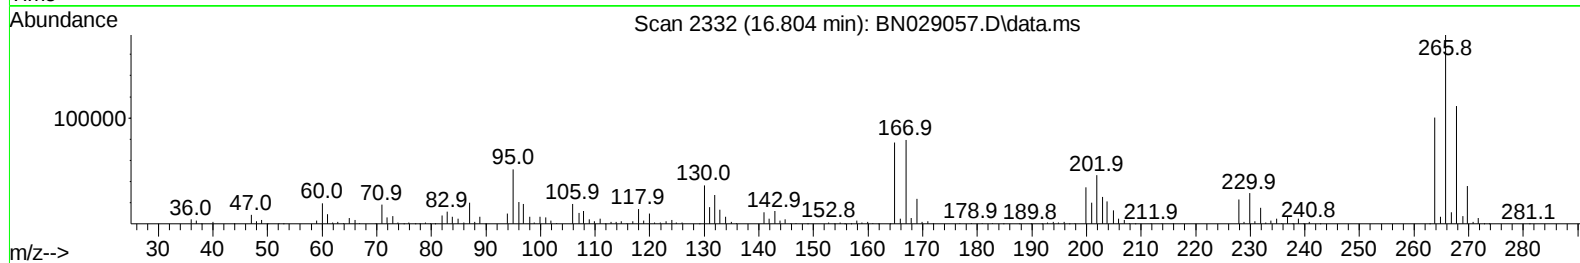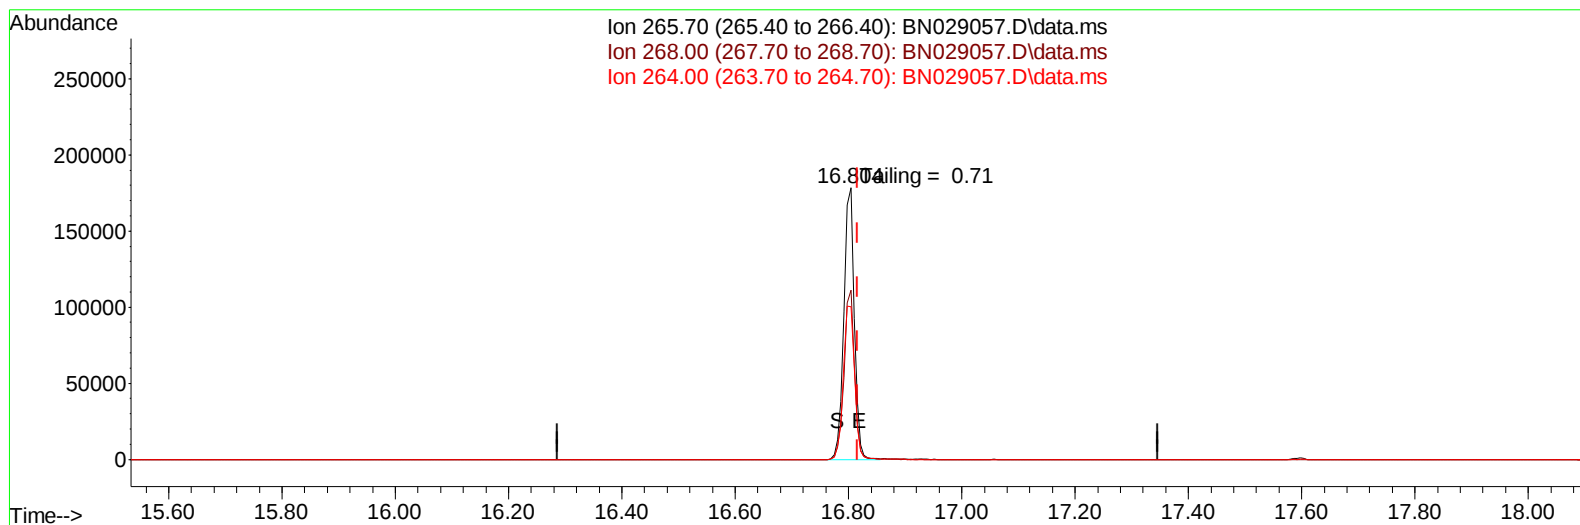

TIC: BN029057.D\data.ms

(70) Pentachlorophenol (C)

16.804min (-0.012) 16437.91 ng




response 227944

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.49
264.00	61.60	56.24
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120623\
Data File : BN029057.D
Acq On : 06 Dec 2023 16:01
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 07 01:51:21 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 01 23:28:24 2023
Response via : Initial Calibration

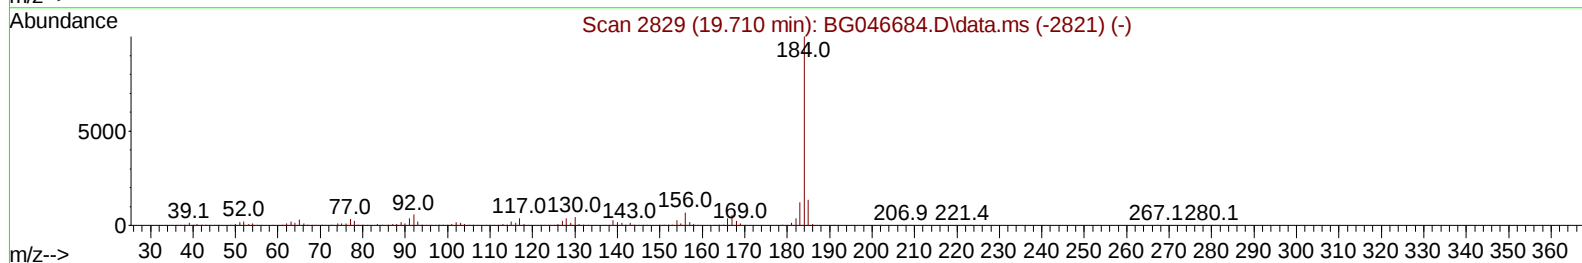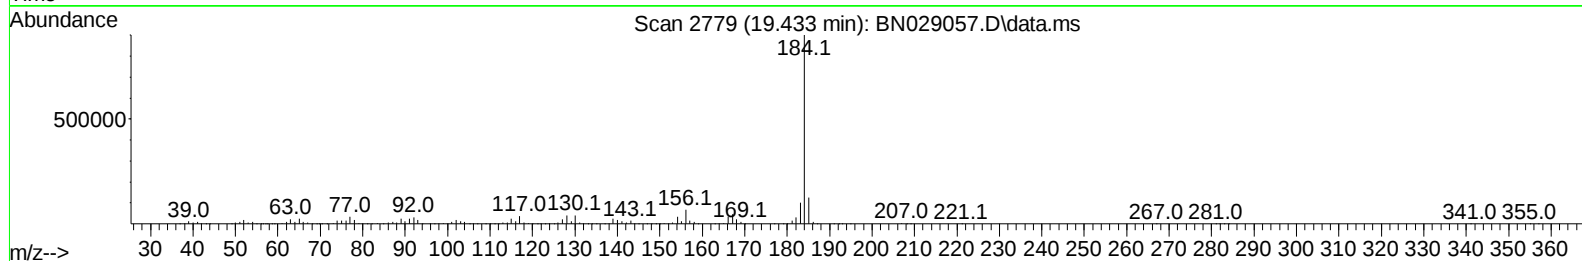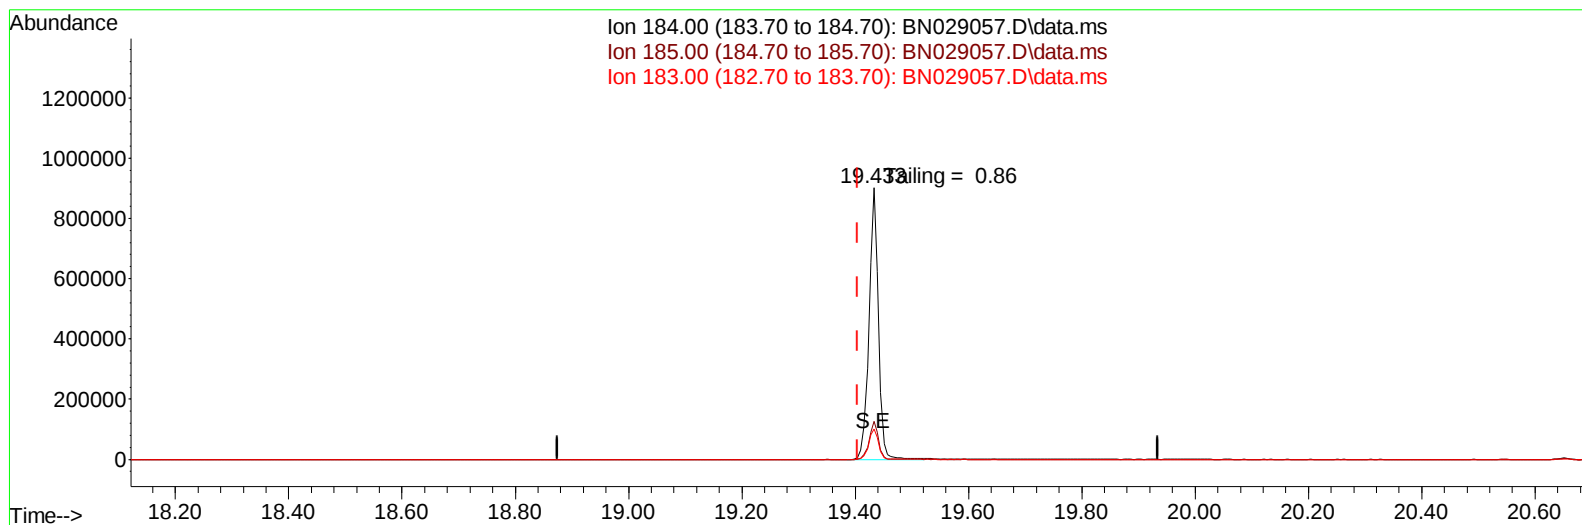

TIC: BN029057.D\data.ms

(77) Benzidine

19.433min (+ 0.029) 0.00 ng

response 1046200

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.98
183.00	13.20	11.13
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/6/2023	BNA_N	<u>BN029057.D</u>
Compound Name	Response	Retention Time
DDT	709084	20.651
DDD	23047	20.21
DDE	169	19.698
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
23216	732300	3.17

Instrument :
BNA_N
ClientSampleId :
DFTPP