


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120623\
Data File : BN029076.D
Acq On : 07 Dec 2023 04:37
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN120523.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Dec 06 00:49:47 2023

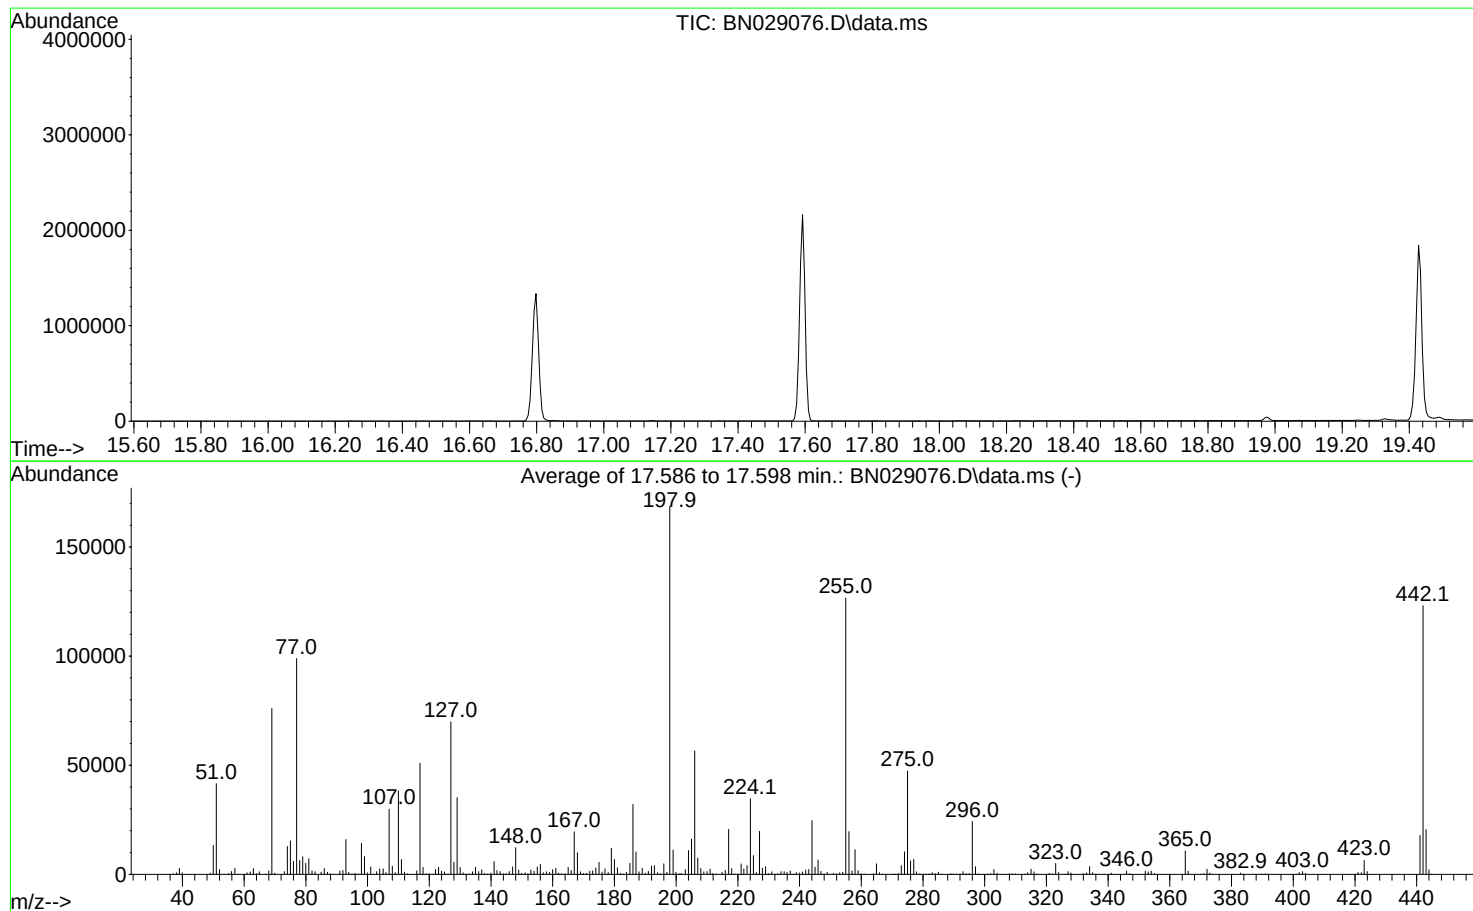




AutoFind: Scans 2465, 2466, 2467; Background Corrected with Scan 2458

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.7	41605	PASS
68	69	0.00	2	2.0	1558	PASS
69	198	0.00	100	45.1	76008	PASS
70	69	0.00	2	0.6	492	PASS
127	198	10	80	41.5	69885	PASS
197	198	0.00	2	0.6	953	PASS
198	198	100	100	100.0	168555	PASS
199	198	5	9	6.6	11163	PASS
275	198	10	60	28.1	47339	PASS
365	198	1	100	6.4	10774	PASS
441	198	0.01	100	10.6	17799	PASS
442	442	50	100	100.0	123101	PASS
443	442	15	24	16.7	20520	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120623\
Data File : BN029076.D
Acq On : 07 Dec 2023 04:37
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 07 05:09:52 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 01 23:28:24 2023
Response via : Initial Calibration

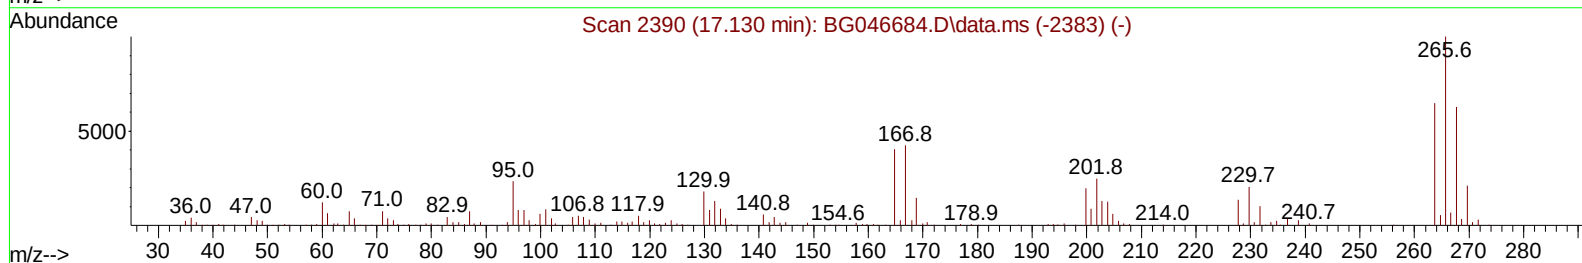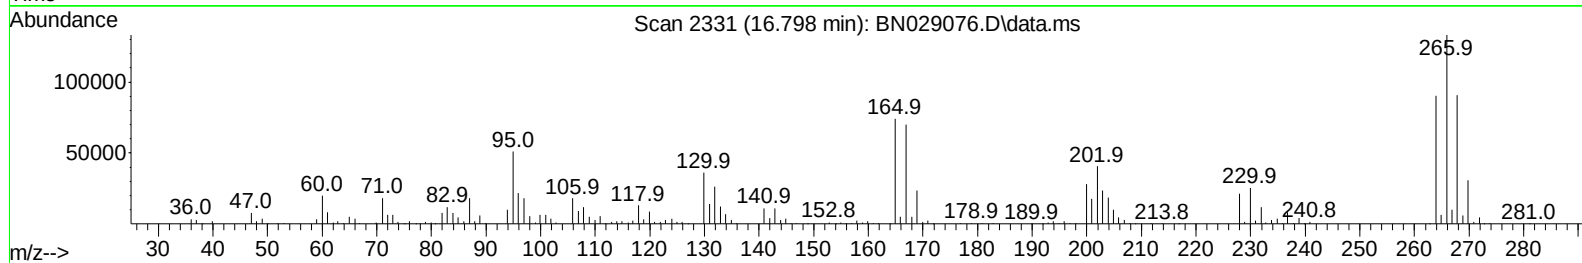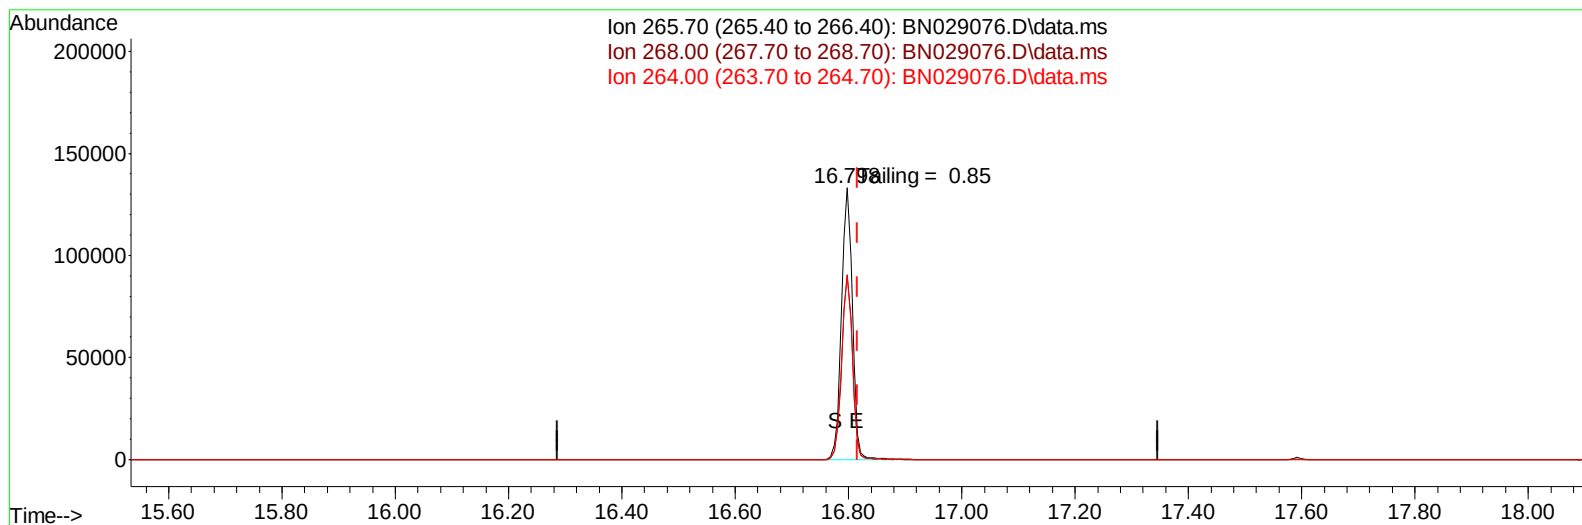

TIC: BN029076.D\data.ms

(70) Pentachlorophenol (C)

16.798min (-0.018) 14659.34 ng




response 177396

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	68.06
264.00	61.60	67.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120623\
 Data File : BN029076.D
 Acq On : 07 Dec 2023 04:37
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Dec 07 05:09:52 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 01 23:28:24 2023
 Response via : Initial Calibration

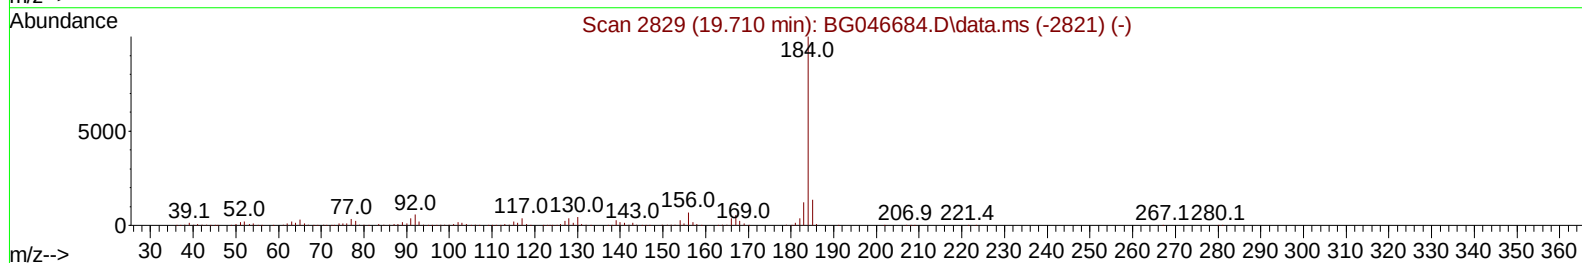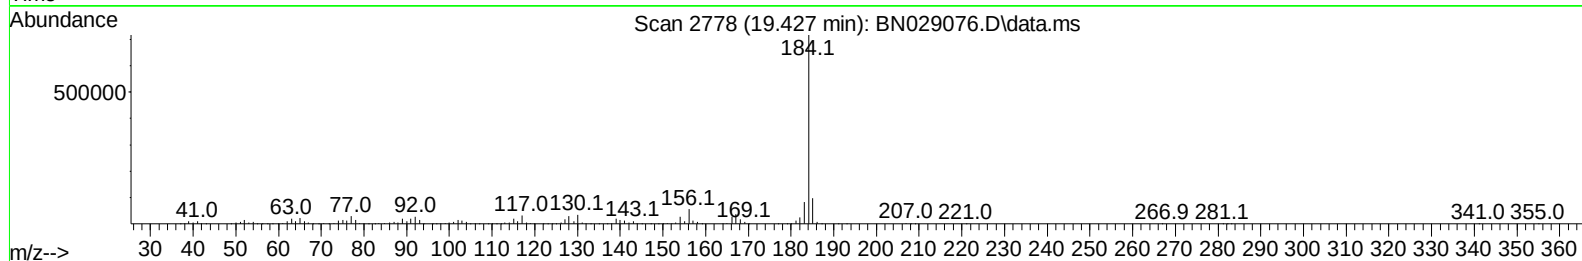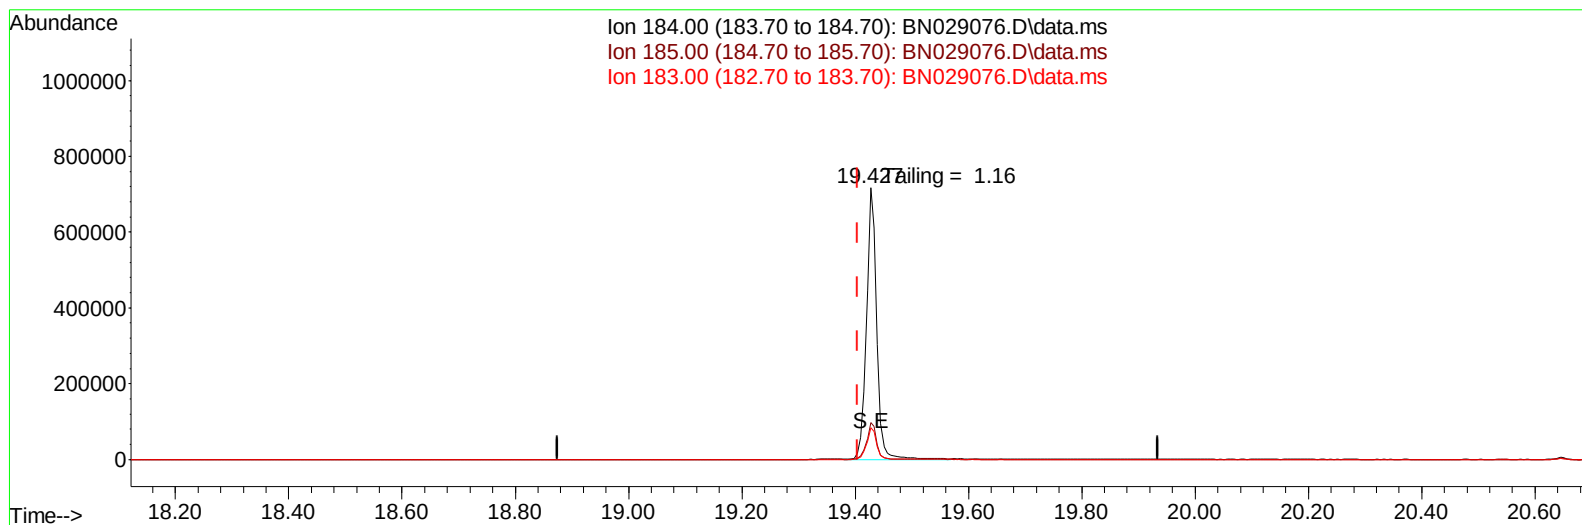

TIC: BN029076.D\data.ms

(77) Benzidine

19.427min (+ 0.023) 0.00 ng

response 906315

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.57
183.00	13.20	11.64
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/6/2023	BNA_N	<u>BN029076.D</u>
Compound Name	Response	Retention Time
DDT	655422	20.645
DDD	16550	20.204
DDE	320	19.692
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
16870	672292	2.51

Instrument :
BNA_N
ClientSampleId :
DFTPP