

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120720\
 Data File : BN012949.D
 Acq On : 07 Dec 2020 21:07
 Operator : CG/JU
 Sample : L4864-22
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0B68

Quant Time: Dec 08 00:17:07 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN120320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 08 00:15:39 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.39	152	1114	0.40	ng/ul	0.00
2) Naphthalene-d8	10.15	136	4652	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.05	164	2550	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.81	188	5405	0.40	ng/ul	0.00
16) Chrysene-d12	21.03	240	4864	0.40	ng/ul	0.00
20) Perylene-d12	23.13	264	4193	0.40	ng/ul	0.00

System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.76	152	952	0.14	ng/ul	0.00
14) Fluoranthene-d10	18.85	212	2245	0.15	ng/ul	0.00


Target Compounds				Ovalue		
3) Naphthalene	10.20	128	272	0.020	ng/ul#	59
7) Acenaphthylene	13.77	152	354	0.029	ng/ul#	70
8) Acenaphthene	14.12	153	208	0.021	ng/ul#	91
9) Fluorene	15.11	166	822	0.072	ng/ul	98
12) Phenanthrene	16.85	178	16360	0.903	ng/ul	98
13) Anthracene	16.94	178	12351	0.801	ng/ul	95
15) Fluoranthene	18.88	202	158276	7.350	ng/ul	97
17) Pyrene	19.25	202	158809	6.912	ng/ul	100
18) Benzo(a)anthracene	21.02	228	168946	8.395	ng/ul	98
19) Chrysene	21.07	228	186832	8.403	ng/ul	98
21) Benzo(b)fluoranthene	22.52	252	356915	18.400	ng/ul	89
22) Benzo(k)fluoranthene	22.67	252	30633	1.429	ng/ul	96
23) Benzo(a)pyrene	23.05	252	154769	8.599	ng/ul#	82
24) Indeno(1,2,3-cd)pyrene	25.19	276	100983	4.271	ng/ul#	98
25) Dibenzo(a,h)anthracene	25.20	278	26244	1.403	ng/ul	92
26) Benzo(a,h,i)perylene	25.82	276	80145	3.748	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120720\
Data File : BN012949.D
Acq On : 07 Dec 2020 21:07
Operator : CG/JU
Sample : L4864-22
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0B68

Quant Time: Dec 08 00:17:07 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN120320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 08 00:15:39 2020
Response via : Initial Calibration

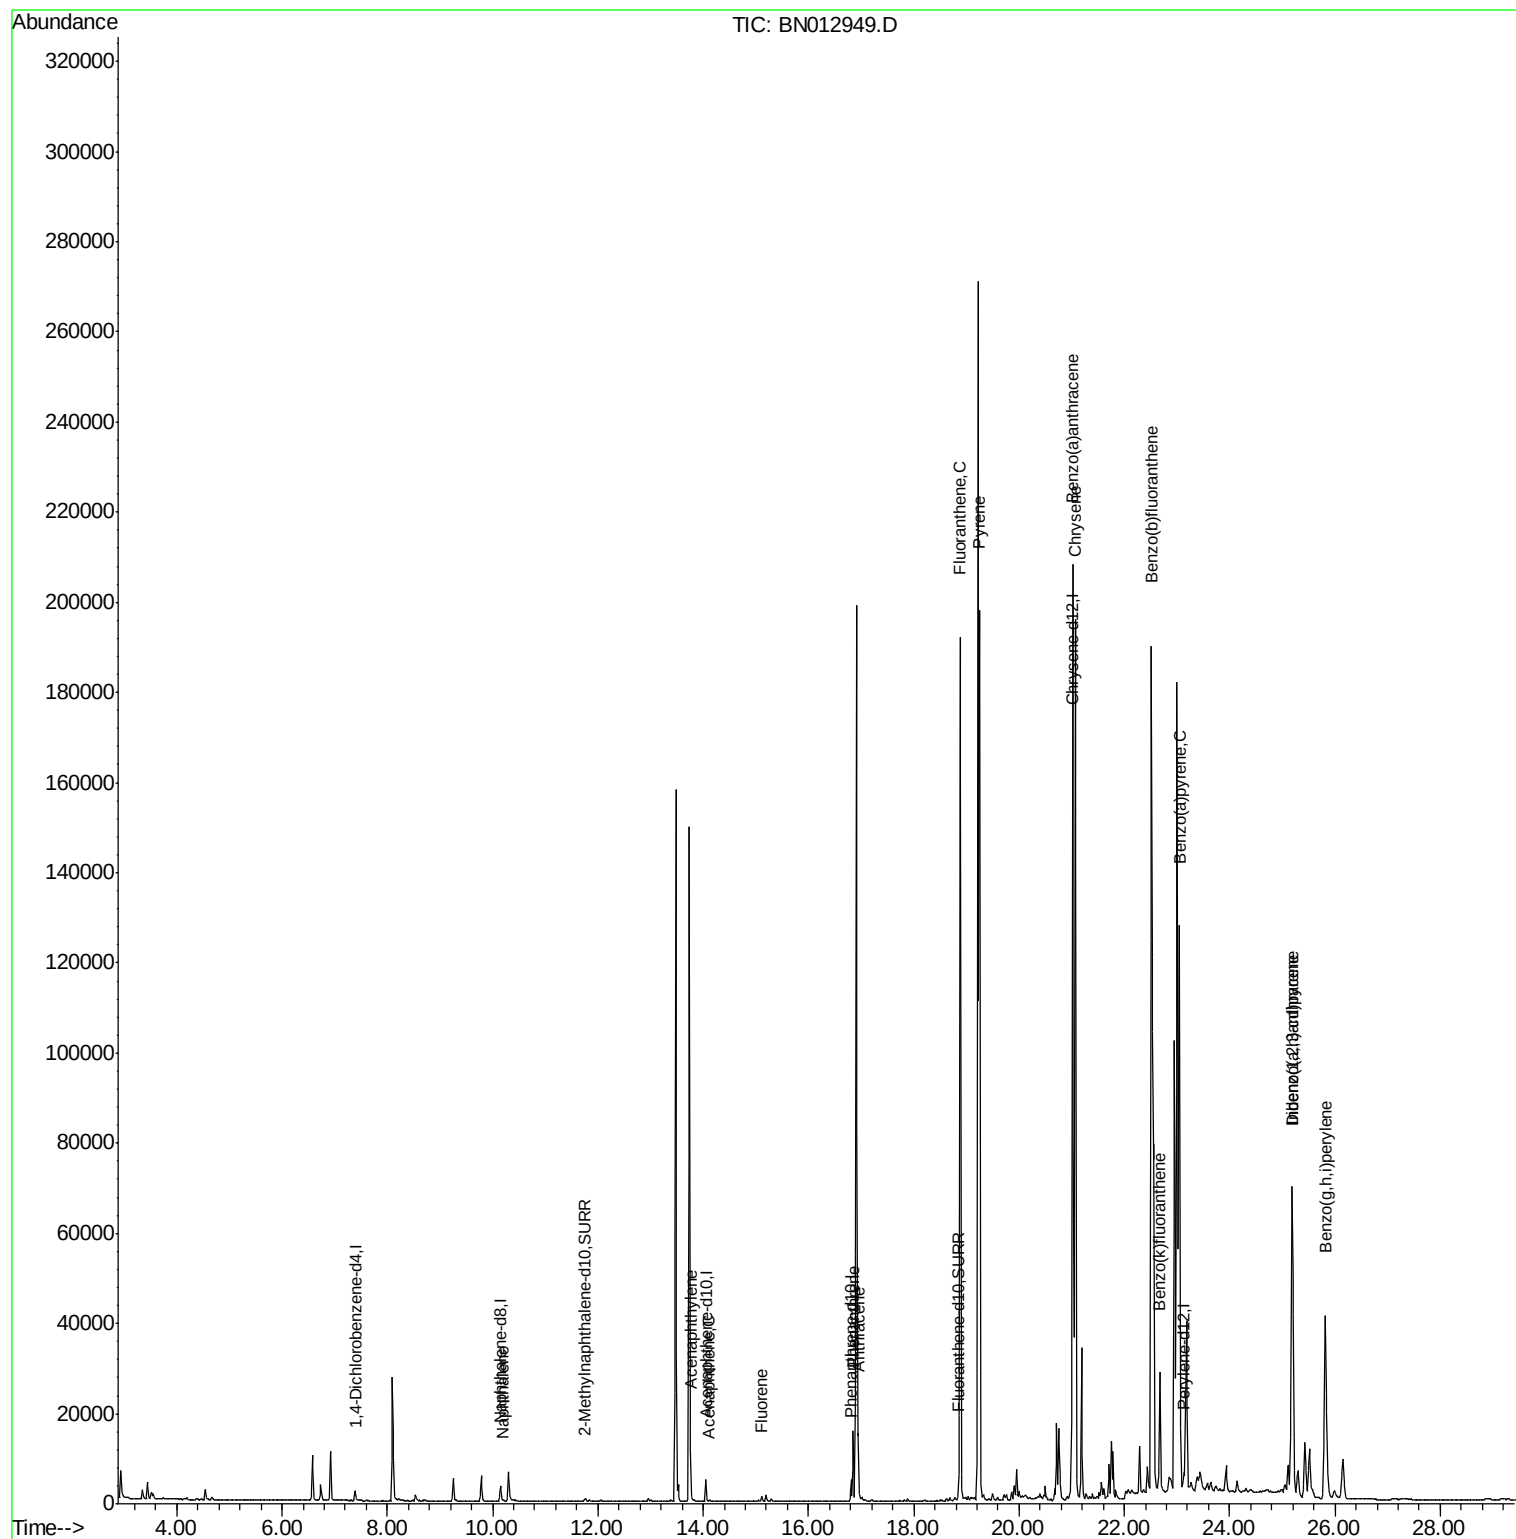

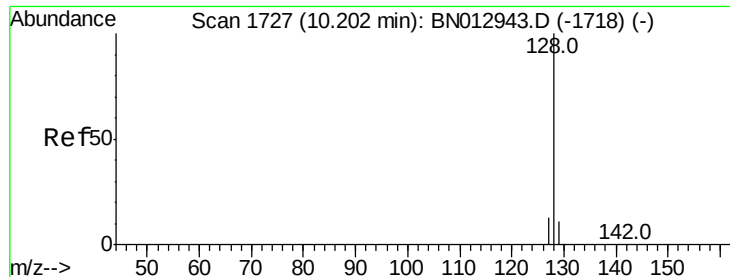

#3

Naphthalene

Concen: 0.020 ng/ul

RT: 10.20 min Scan# 1727

Delta R.T. 0.00 min

Lab File: BN012949.D

Acq: 07 Dec 2020 21:07

Instrument :

BNA_N

ClientSampleId :

C0B68


Tot Ion:128 Resp: 272

Ion Ratio Lower Upper

128 100

129 34.3 12.3 18.5#




127 34.3 14.2 21.4#

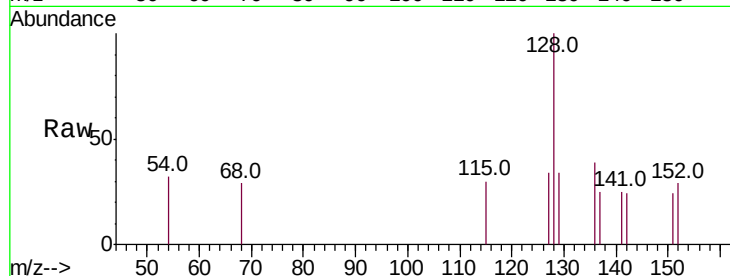

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

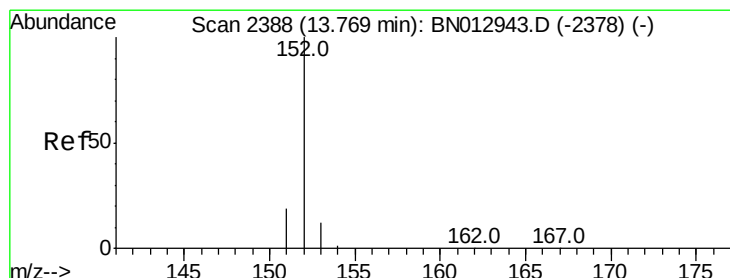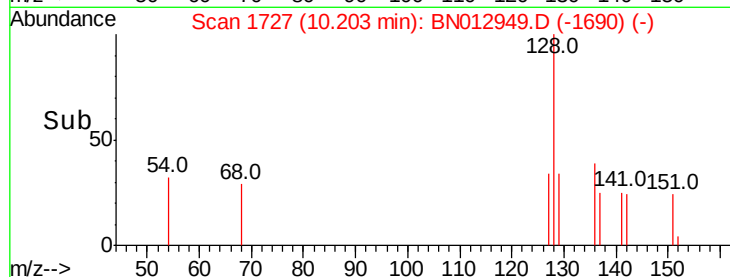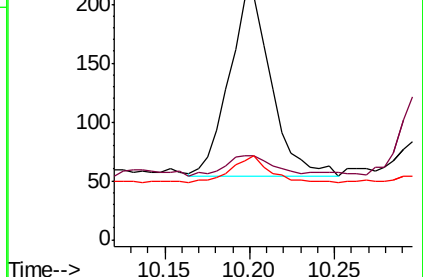

#7

Acenaphthylene

Concen: 0.029 ng/ul

RT: 13.77 min Scan# 2388

Delta R.T. 0.00 min

Lab File: BN012949.D

Acq: 07 Dec 2020 21:07


Tgt Ion:152 Resp: 354

Ion Ratio Lower Upper

152 100

151 36.0 18.2 27.4#



153 31.2 13.1 19.7#

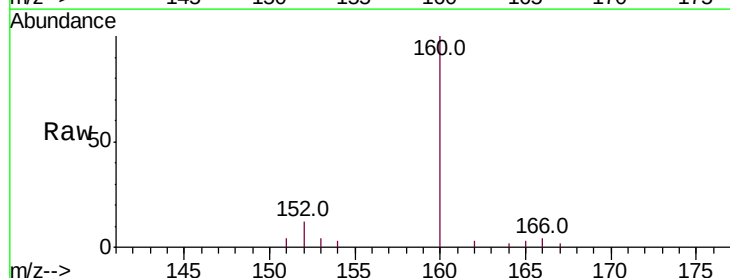


Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

Ion 153.00 (152.70 to 153.70): E

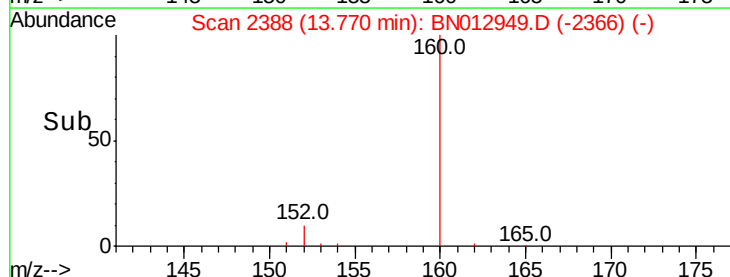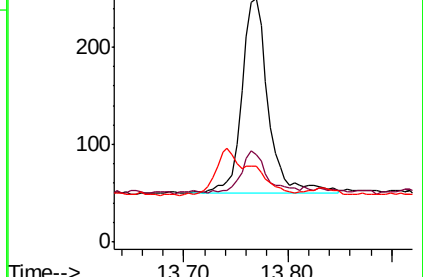

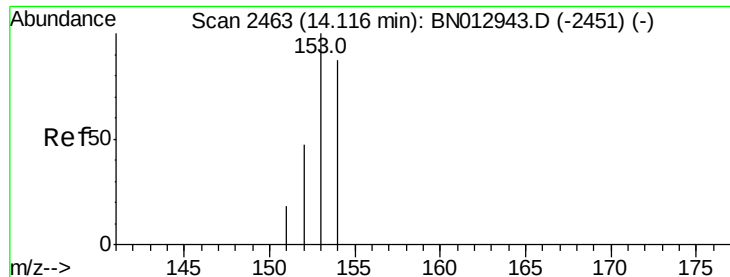

#8

Acenaphthene

Concen: 0.021 ng/ul

RT: 14.12 min Scan# 2463

Delta R.T. 0.00 min

Lab File: BN012949.D

Acq: 07 Dec 2020 21:07

Instrument :

BNA_N

ClientSampleId :

C0B68


Tot Ion:153 Resp: 208

Ion Ratio Lower Upper

153 100

152 63.4 40.7 61.1#




154 91.4 70.8 106.2

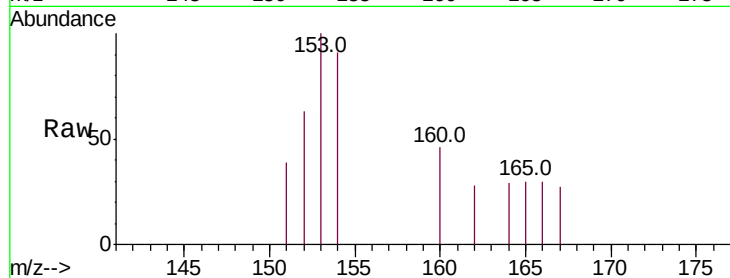

Abundance Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E

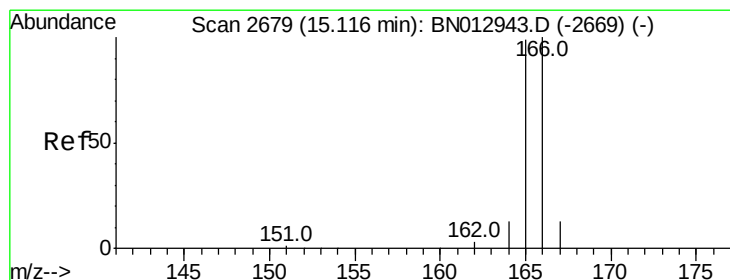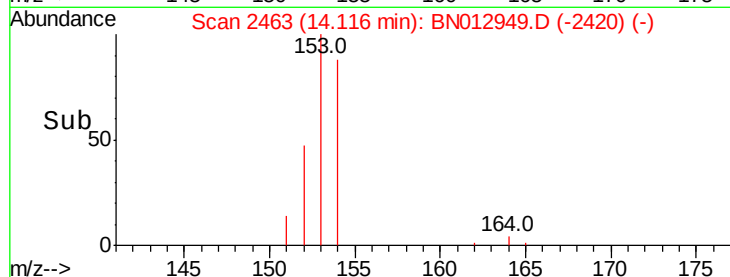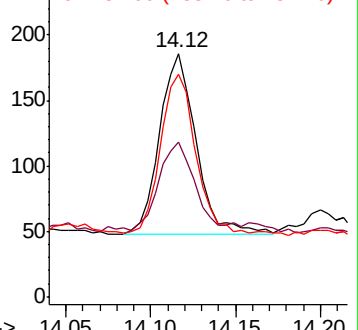

#9

Fluorene

Concen: 0.072 ng/ul

RT: 15.11 min Scan# 2678

Delta R.T. -0.00 min

Lab File: BN012949.D

Acq: 07 Dec 2020 21:07


Tgt Ion:166 Resp: 822

Ion Ratio Lower Upper

166 100

165 99.0 79.8 119.8



167 20.6 13.8 20.8

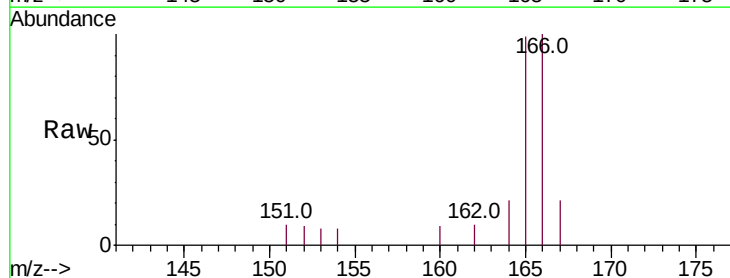


Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

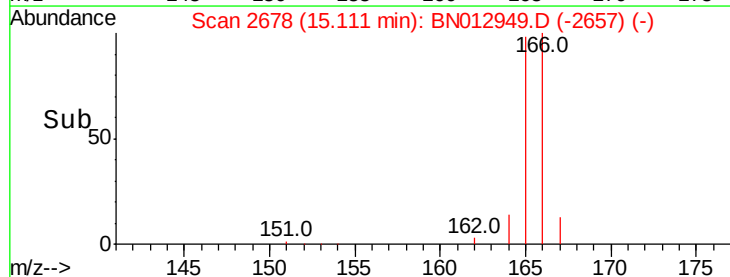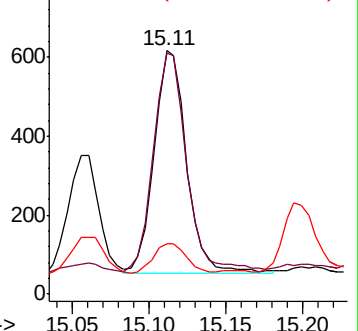

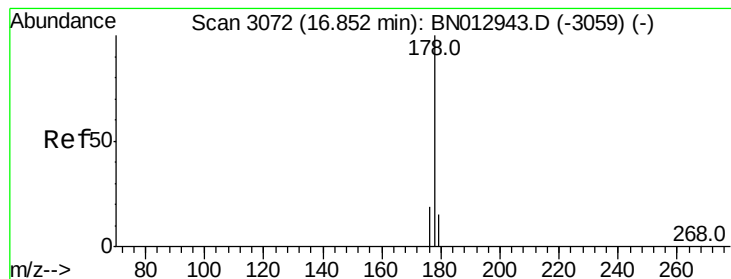

#12

Phenanthrene

Concen: 0.903 ng/ul

RT: 16.85 min Scan# 3072

Delta R.T. 0.00 min

Lab File: BN012949.D

Acq: 07 Dec 2020 21:07

Instrument :

BNA_N

ClientSampleId :

C0B68





Tot Ion:178 Resp: 16360

Ion Ratio Lower Upper

178 100

179 16.1 13.6 20.4

176 19.2 16.4 24.6

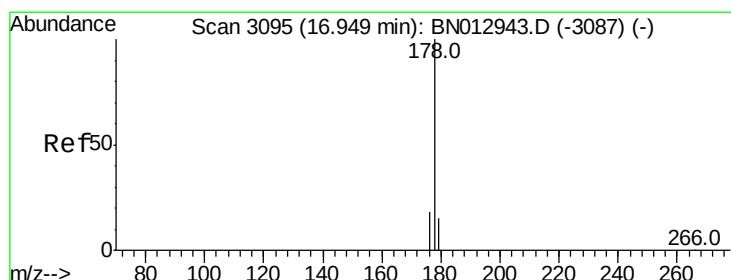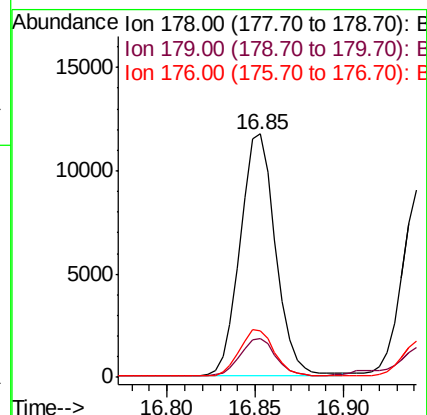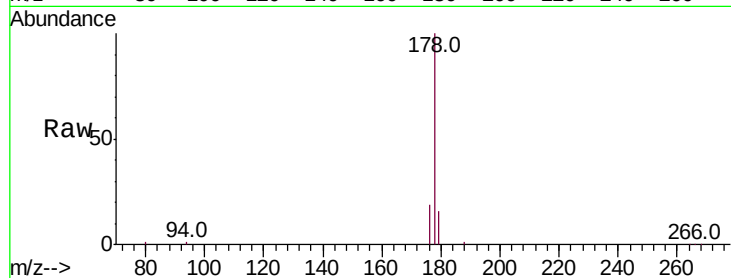

#13

Anthracene

Concen: 0.801 ng/ul

RT: 16.94 min Scan# 3093

Delta R.T. -0.00 min

Lab File: BN012949.D

Acq: 07 Dec 2020 21:07




Tgt Ion:178 Resp: 12351


Ion Ratio Lower Upper

178 100

179 16.0 14.6 21.8

176 19.1 17.1 25.7

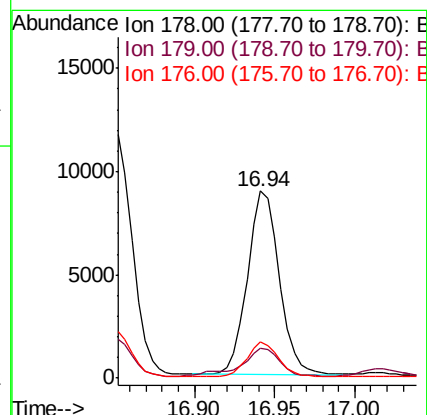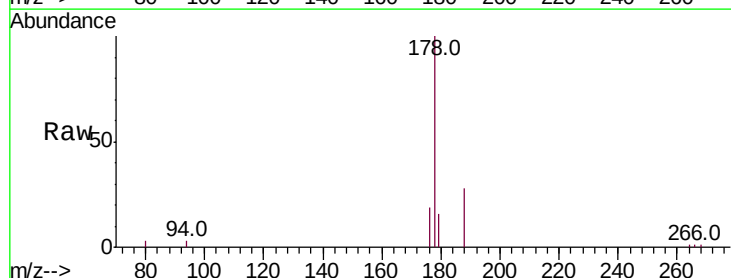



#15

Fluoranthene

Concen: 7.350 ng/ul

RT: 18.88 min Scan# 3545

Delta R.T. 0.00 min

Lab File: BN012949.D

Acq: 07 Dec 2020 21:07

Instrument :

BNA_N

ClientSampleId :

C0B68


Tot Ion:202 Resp: 158276

Ion Ratio Lower Upper

202 100

101 9.8 0.0 30.6




100 7.5 0.0 28.7

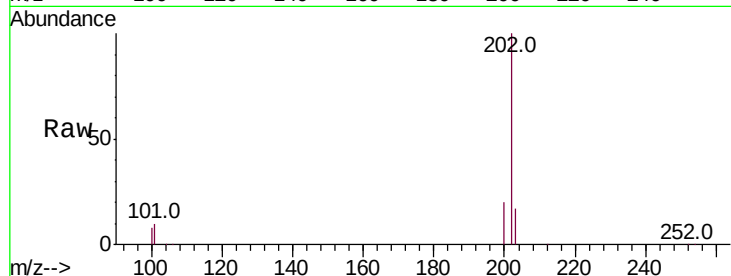

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

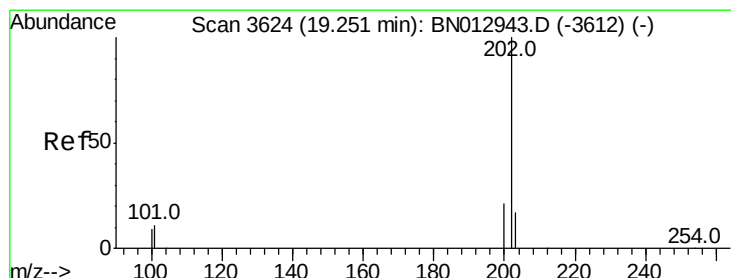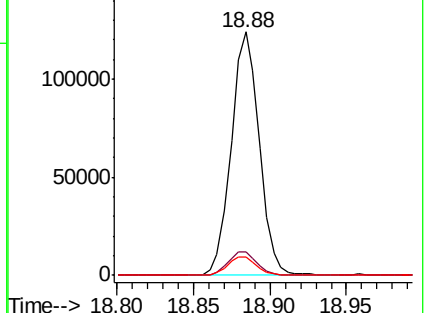

#17

Pyrene

Concen: 6.912 ng/ul

RT: 19.25 min Scan# 3624

Delta R.T. 0.00 min

Lab File: BN012949.D

Acq: 07 Dec 2020 21:07


Tgt Ion:202 Resp: 158809

Ion Ratio Lower Upper

202 100

101 11.4 9.1 13.7



100 9.4 7.5 11.3

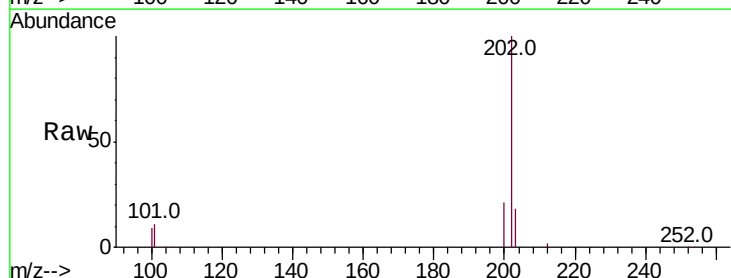


Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

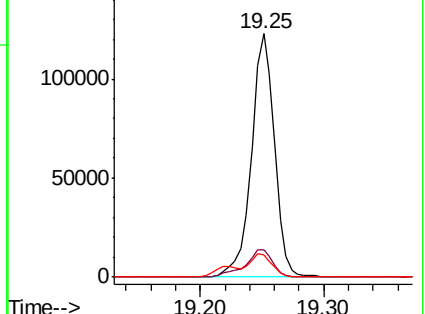

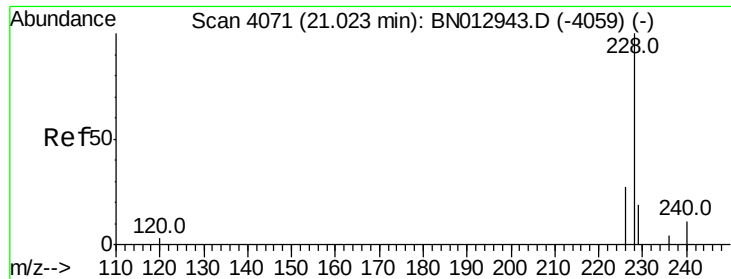

#18

Benzo(a)anthracene

Concen: 8.395 ng/ul

RT: 21.02 min Scan# 4069

Delta R.T. -0.00 min

Lab File: BN012949.D

Acq: 07 Dec 2020 21:07

Instrument :

BNA_N

ClientSampleId :

C0B68


Tot Ion:228 Resp: 168946

Ion Ratio Lower Upper

228 100

229 20.0 16.3 24.5




226 27.8 23.4 35.2

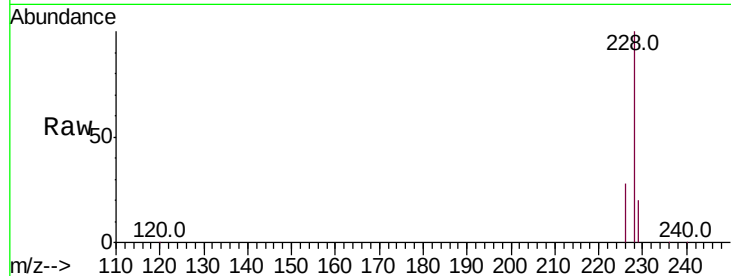

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 229.00 (228.70 to 229.70): E

Ion 226.00 (225.70 to 226.70): E

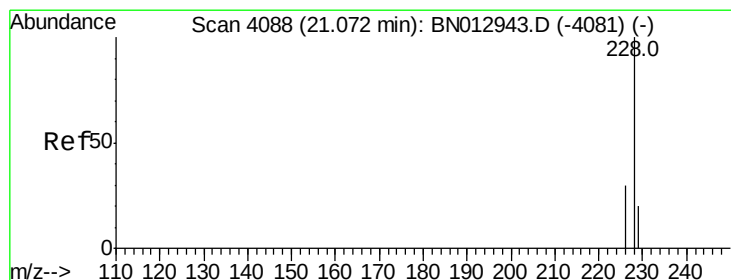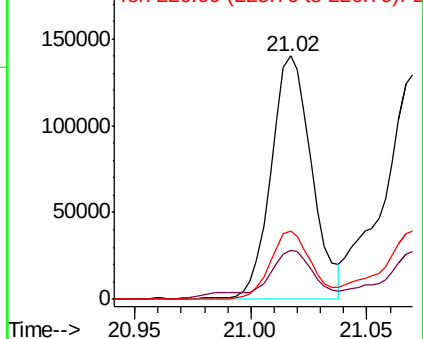

#19

Chrysene

Concen: 8.403 ng/ul

RT: 21.07 min Scan# 4087

Delta R.T. -0.00 min

Lab File: BN012949.D

Acq: 07 Dec 2020 21:07


Tgt Ion:228 Resp: 186832

Ion Ratio Lower Upper

228 100

226 30.2 25.0 37.6



229 21.1 16.4 24.6

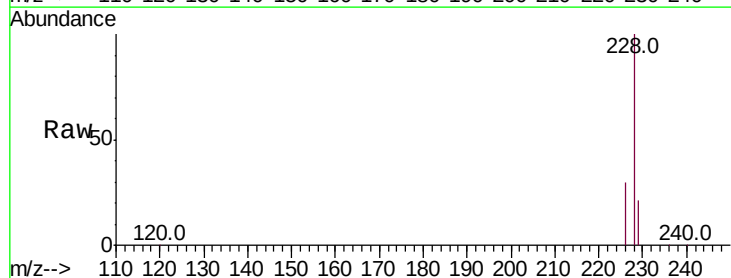


Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

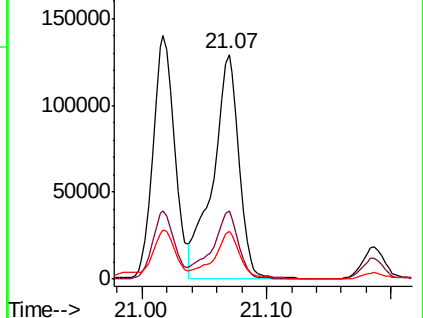

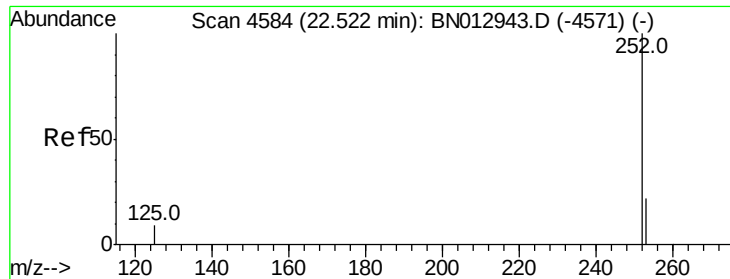

#21

Benzo(b)fluoranthene

Concen: 18.400 ng/ul

RT: 22.52 min Scan# 4582

Delta R.T. -0.00 min

Lab File: BN012949.D

Acq: 07 Dec 2020 21:07

Instrument :

BNA_N

ClientSampleId :

C0B68


Tot Ion:252 Resp: 356915

Ion Ratio Lower Upper

252 100

253 22.8 0.0 59.6




125 9.8 0.0 26.0

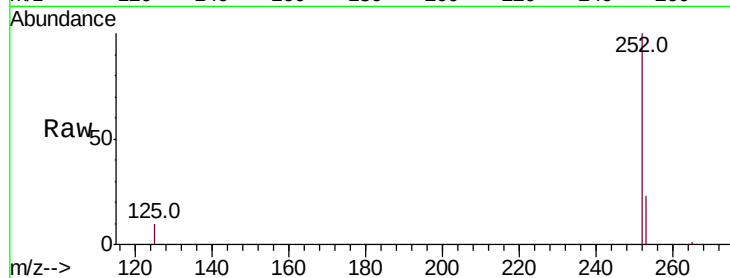

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

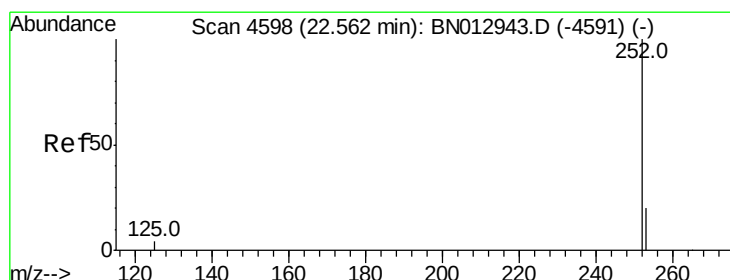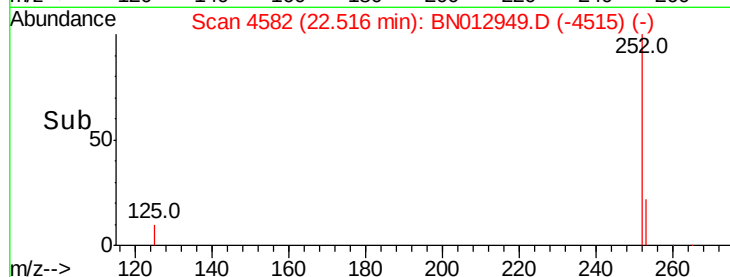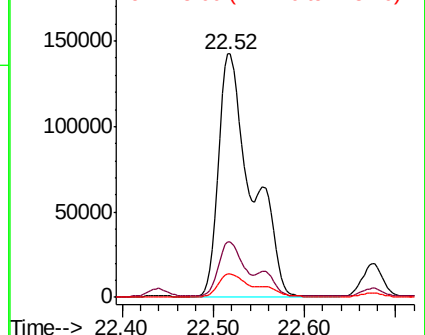

#22

Benzo(k)fluoranthene

Concen: 1.429 ng/ul

RT: 22.67 min Scan# 4636

Delta R.T. 0.11 min

Lab File: BN012949.D

Acq: 07 Dec 2020 21:07


Tgt Ion:252 Resp: 30633

Ion Ratio Lower Upper

252 100

253 26.7 23.4 35.2



125 12.6 11.1 16.7

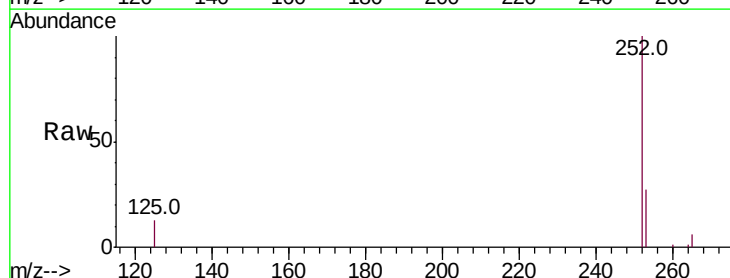


Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

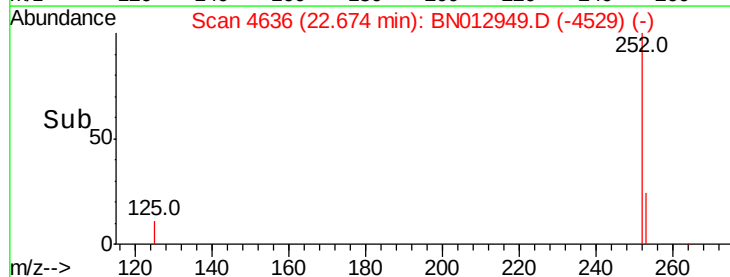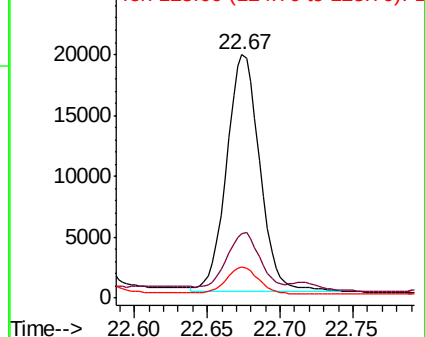

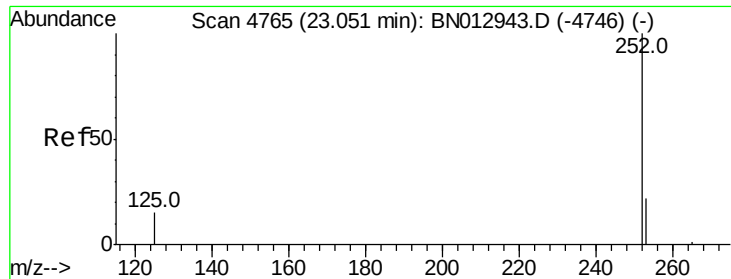

#23

Benzo(a)pyrene

Concen: 8.599 ng/ul

RT: 23.05 min Scan# 4763

Delta R.T. 0.00 min

Lab File: BN012949.D

Acq: 07 Dec 2020 21:07

Instrument :

BNA_N

ClientSampleId :

C0B68


Tot Ion:252 Resp: 154769

Ion Ratio Lower Upper

252 100

253 22.4 26.5 39.7#




125 10.6 14.2 21.2#

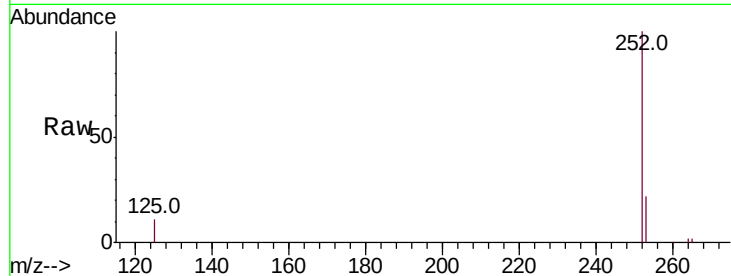

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

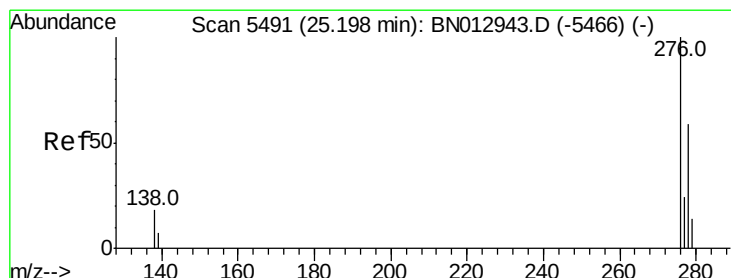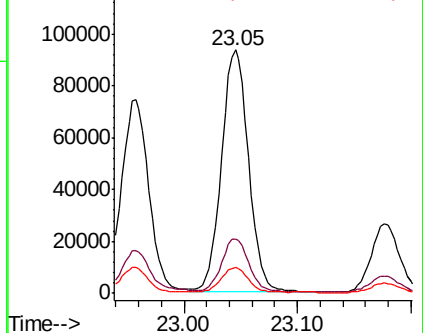

#24

Indeno(1,2,3-cd)pyrene

Concen: 4.271 ng/ul

RT: 25.19 min Scan# 5488

Delta R.T. -0.00 min

Lab File: BN012949.D

Acq: 07 Dec 2020 21:07


Tgt Ion:276 Resp: 100983

Ion Ratio Lower Upper

276 100

138 19.4 16.2 24.2



227 0.2 0.0 0.0#

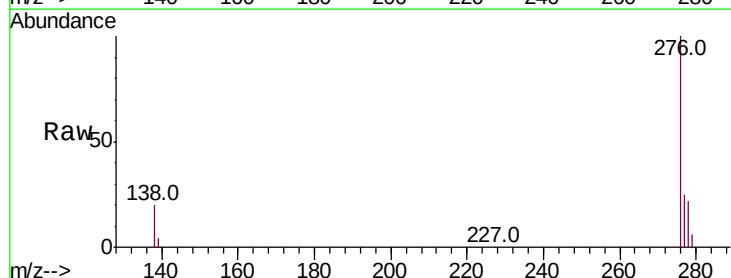


Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 227.00 (226.70 to 227.70): E

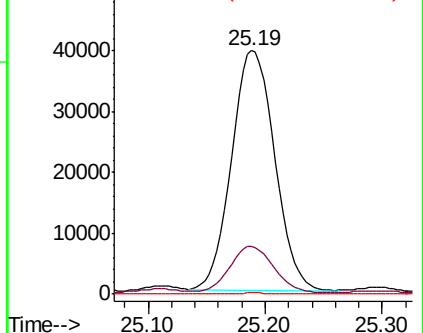







#25
Dibenzo(a,h)anthracene
Concen: 1.403 ng/ul
RT: 25.20 min Scan# 5491
Delta R.T. -0.01 min
Lab File: BN012949.D
Acq: 07 Dec 2020 21:07

Instrument :
BNA_N
ClientSampleId :
C0B68

Tot Ion:278 Resp: 26244

Ion	Ratio	Lower	Upper
278	100		
139	17.2	14.5	21.7
279	26.6	26.3	39.5

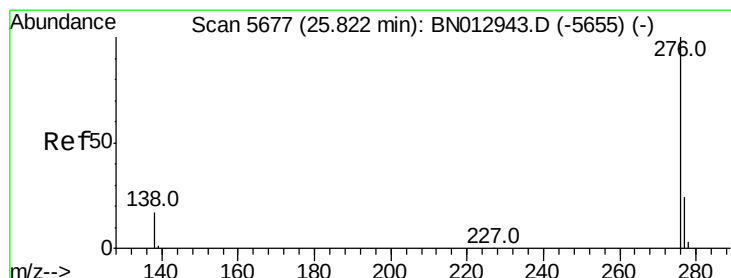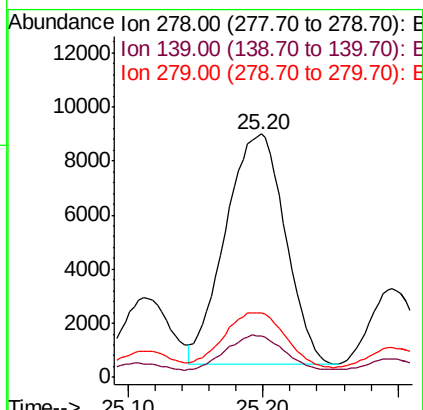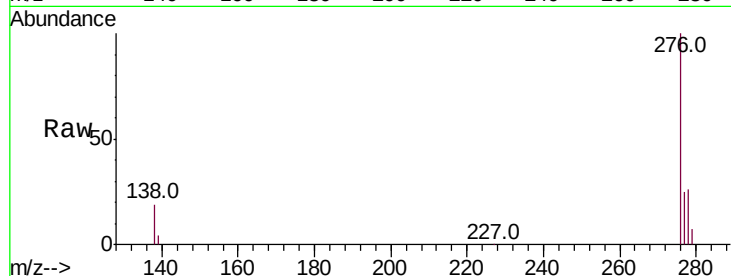

#26
Benzo(g,h,i)perylene
Concen: 3.748 ng/ul
RT: 25.82 min Scan# 5676
Delta R.T. -0.00 min
Lab File: BN012949.D
Acq: 07 Dec 2020 21:07

Tgt Ion:276 Resp: 80145

Ion	Ratio	Lower	Upper
276	100		
138	20.0	16.3	24.5
277	24.5	21.8	32.6

