

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120720\
 Data File : BN012979.D
 Acq On : 08 Dec 2020 17:16
 Operator : CG/JU
 Sample : L4864-20DL 2X
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0B63DL

Quant Time: Dec 09 00:13:59 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN120320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 09 00:11:42 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.38	152	931	0.40	ng/ul	0.00
2) Naphthalene-d8	10.15	136	3788	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.05	164	2104	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.81	188	4369	0.40	ng/ul	0.00
16) Chrysene-d12	21.03	240	3506	0.40	ng/ul	0.00
20) Perylene-d12	23.13	264	3238	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.76	152	775	0.14	ng/ul	0.00
14) Fluoranthene-d10	18.85	212	1758	0.15	ng/ul	0.00
Target Compounds				Ovalue		
8) Acenaphthene	14.11	153	226	0.028	ng/ul#	92
9) Fluorene	15.11	166	291	0.031	ng/ul#	93
12) Phenanthrene	16.85	178	9225	0.630	ng/ul	98
13) Anthracene	16.94	178	1471	0.118	ng/ul	98
15) Fluoranthene	18.88	202	27877	1.601	ng/ul	99
17) Pyrene	19.25	202	24172	1.460	ng/ul	99
18) Benzo(a)anthracene	21.02	228	10457	0.721	ng/ul	99
19) Chrysene	21.07	228	14161	0.884	ng/ul	100
21) Benzo(b)fluoranthene	22.52	252	24491	1.635	ng/ul	93
22) Benzo(k)fluoranthene	22.52	252	24491	1.479	ng/ul	94
23) Benzo(a)pyrene	23.04	252	10443	0.751	ng/ul#	91
24) Indeno(1,2,3-cd)pyrene	25.18	276	7499	0.411	ng/ul#	99
25) Dibenzo(a,h)anthracene	25.19	278	1778	0.123	ng/ul#	80
26) Benzo(g,h,i)perylene	25.81	276	6851	0.415	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120720\
Data File : BN012979.D
Acq On : 08 Dec 2020 17:16
Operator : CG/JU
Sample : L4864-20DL 2X
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0B63DL

Quant Time: Dec 09 00:13:59 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN120320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 09 00:11:42 2020
Response via : Initial Calibration

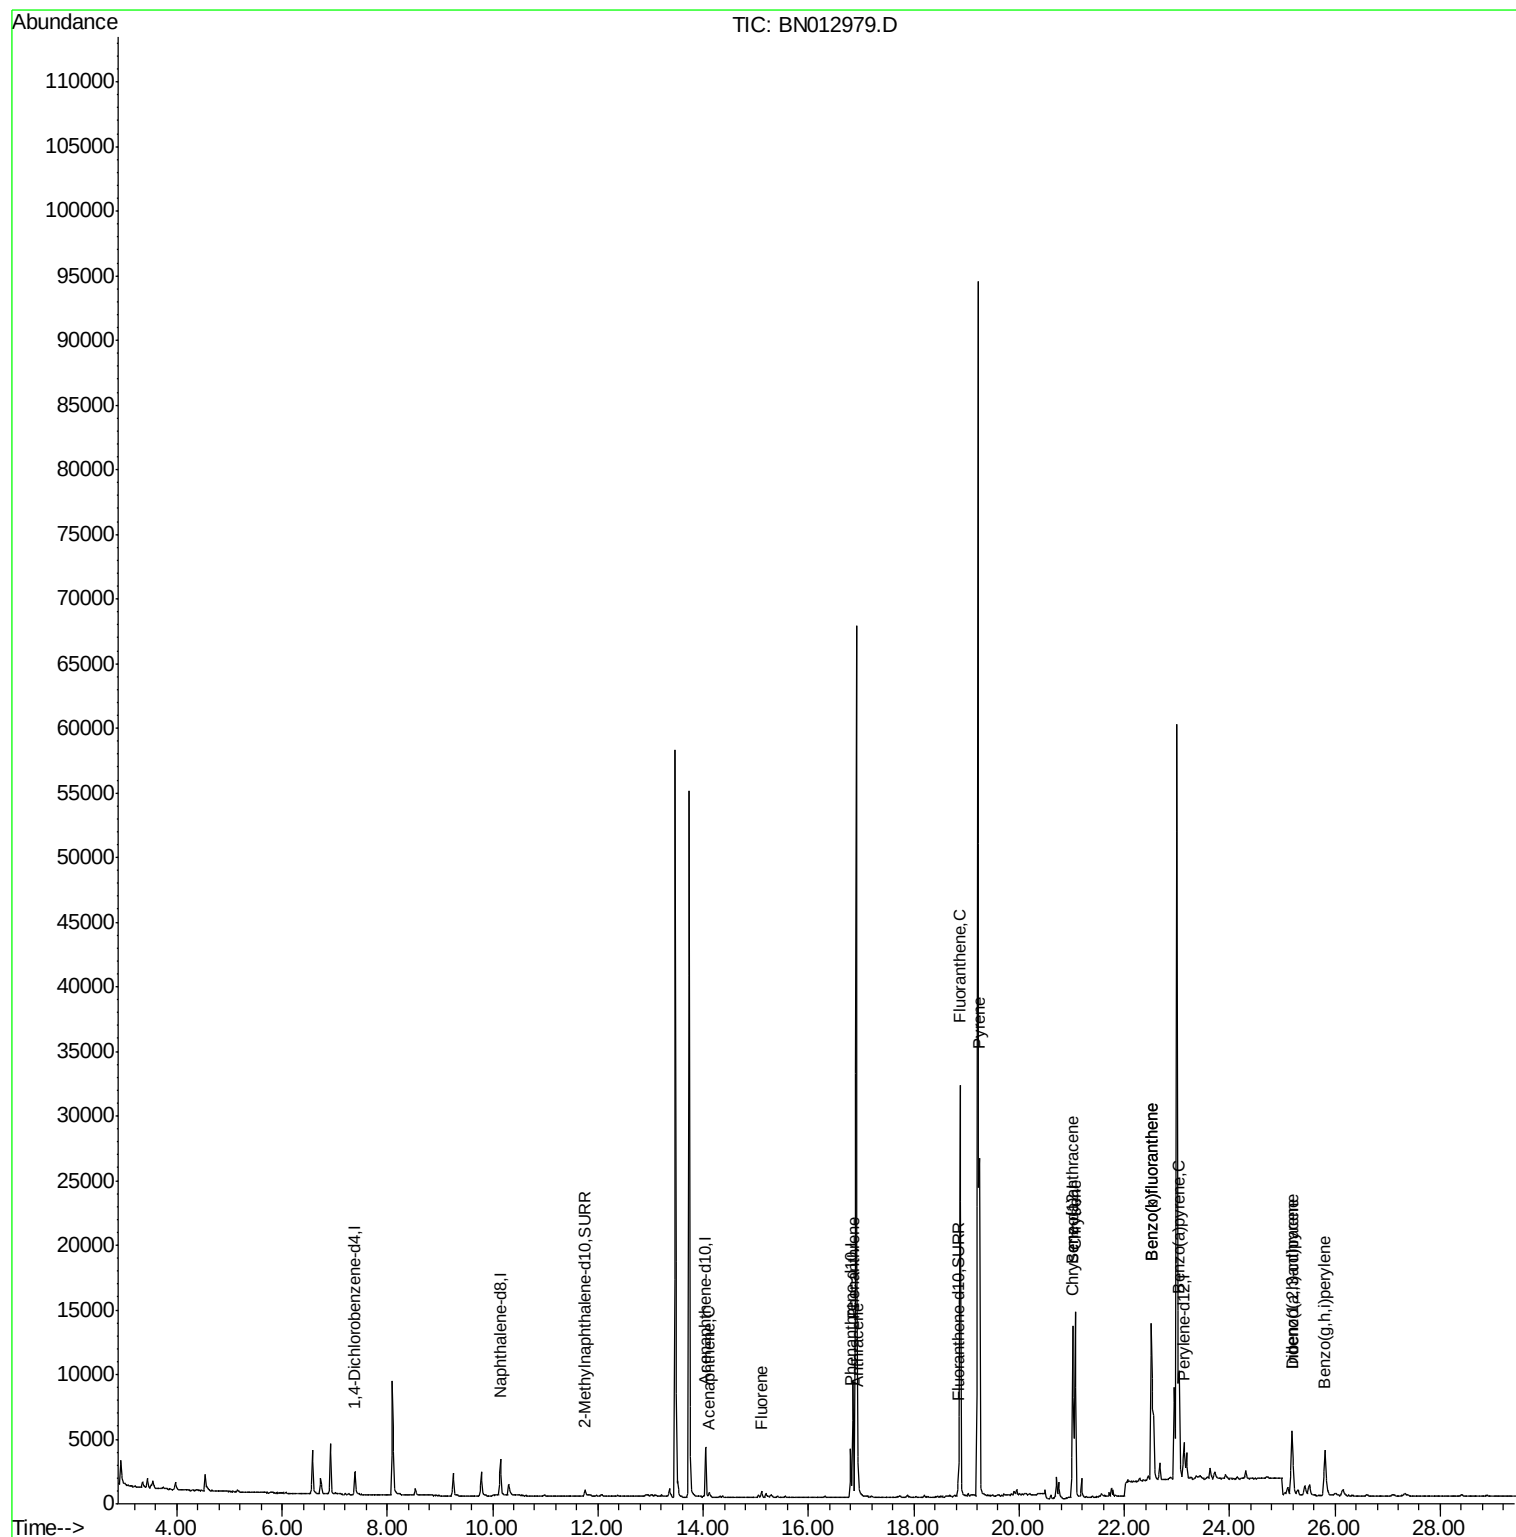

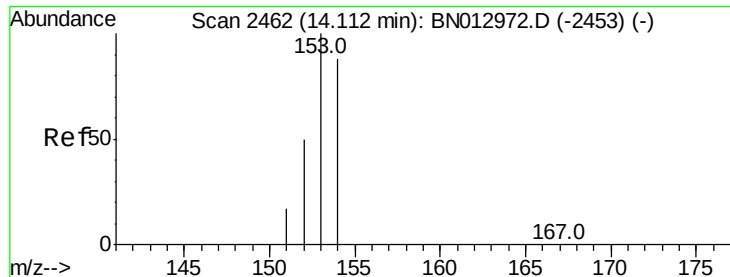

#8

Acenaphthene

Concen: 0.028 ng/ul

RT: 14.11 min Scan# 2462

Delta R.T. -0.00 min

Lab File: BN012979.D

Acq: 08 Dec 2020 17:16

Instrument :

BNA_N

ClientSampleId :

C0B63DL


Tot Ion:153 Resp: 226

Ion Ratio Lower Upper

153 100

152 65.0 40.7 61.1#




154 89.5 70.8 106.2

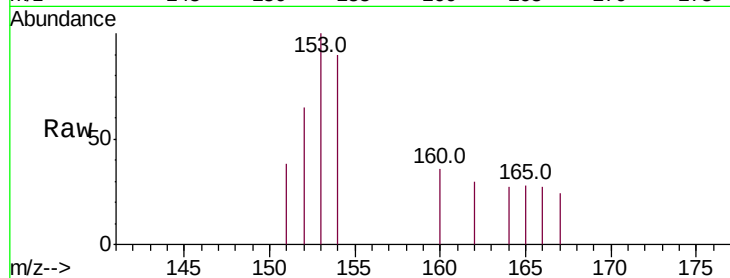

Abundance Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E

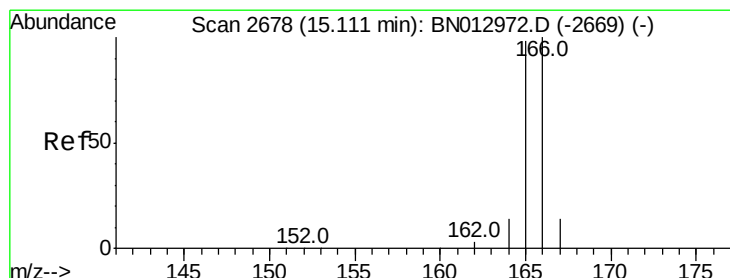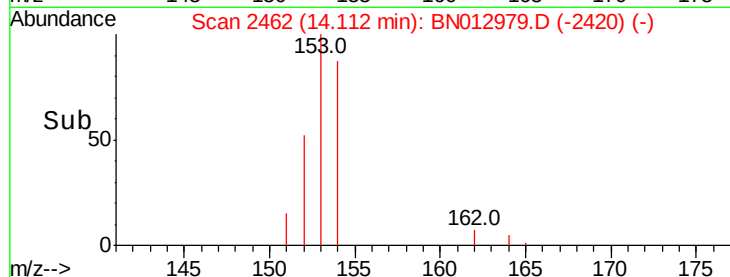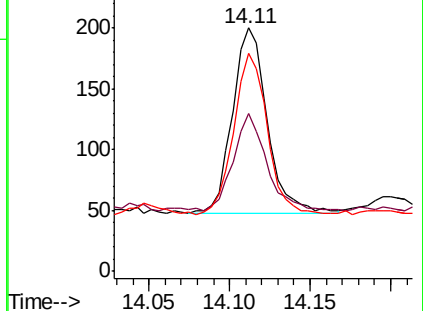

#9

Fluorene

Concen: 0.031 ng/ul

RT: 15.11 min Scan# 2678

Delta R.T. -0.00 min

Lab File: BN012979.D

Acq: 08 Dec 2020 17:16


Tgt Ion:166 Resp: 291

Ion Ratio Lower Upper

166 100

165 101.6 79.8 119.8



167 32.1 13.8 20.8#

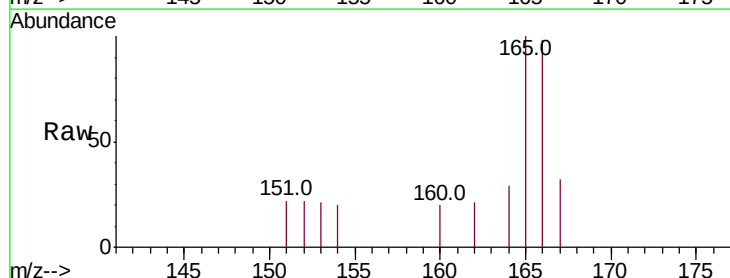


Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

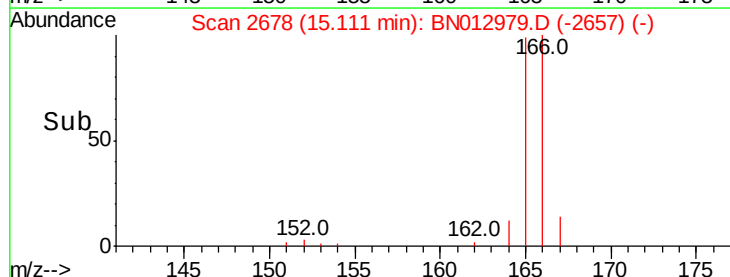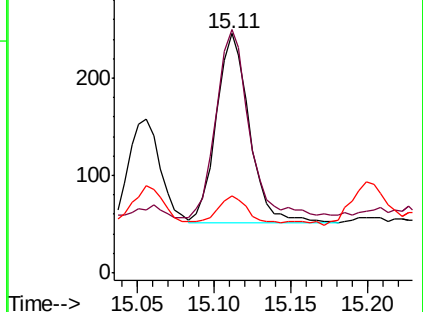

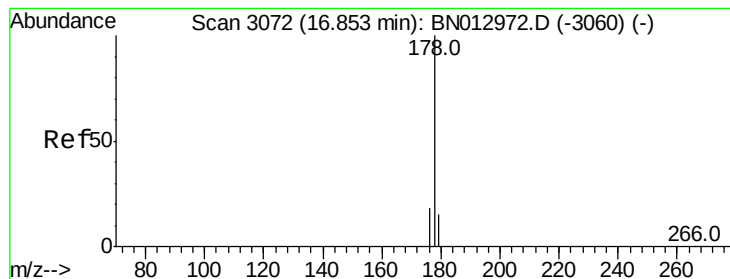

#12

Phenanthrene

Concen: 0.630 ng/ul

RT: 16.85 min Scan# 3071

Delta R.T. -0.00 min

Lab File: BN012979.D

Acq: 08 Dec 2020 17:16

Instrument :

BNA_N

ClientSampleId :

C0B63DL


Tot Ion:178 Resp: 9225

Ion Ratio Lower Upper

178 100

179 16.1 13.6 20.4




176 19.7 16.4 24.6

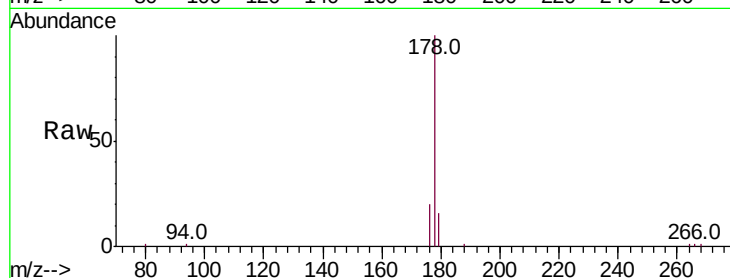

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

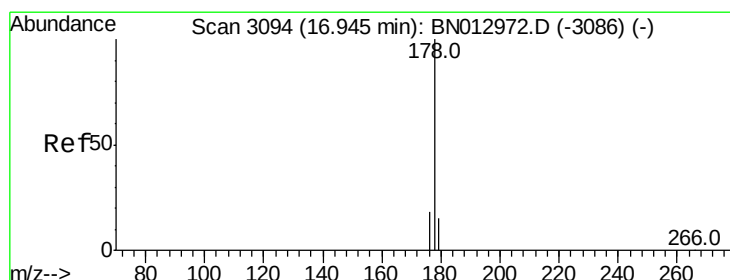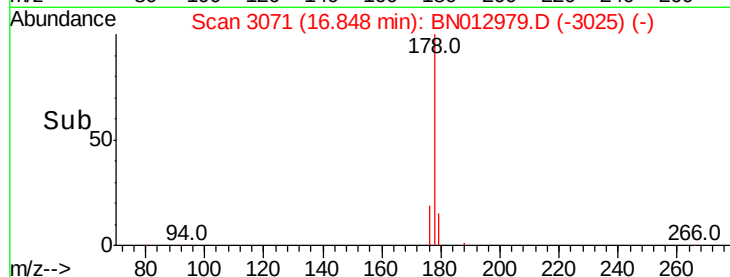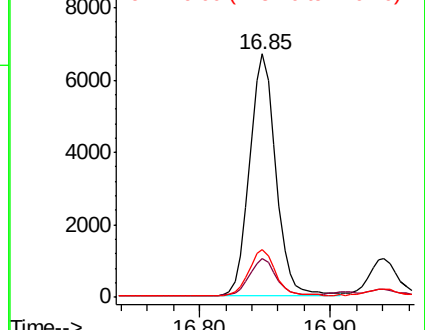

#13

Anthracene

Concen: 0.118 ng/ul

RT: 16.94 min Scan# 3093

Delta R.T. -0.00 min

Lab File: BN012979.D

Acq: 08 Dec 2020 17:16


Tgt Ion:178 Resp: 1471

Ion Ratio Lower Upper

178 100

179 20.1 14.6 21.8



176 21.7 17.1 25.7

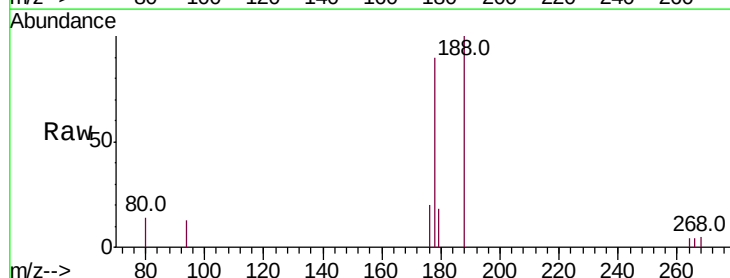


Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

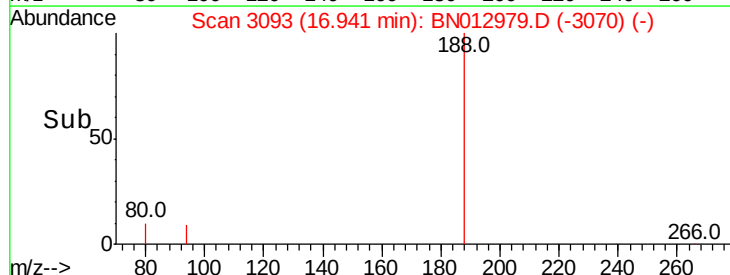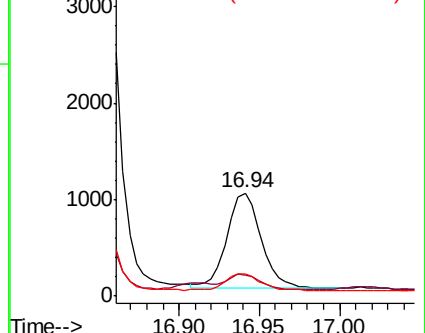

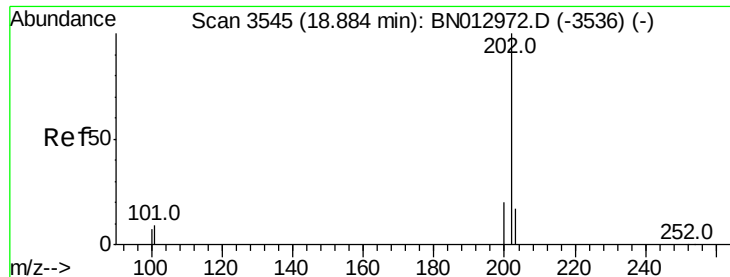

#15

Fluoranthene

Concen: 1.601 ng/ul

RT: 18.88 min Scan# 3544

Delta R.T. -0.00 min

Lab File: BN012979.D

Acq: 08 Dec 2020 17:16

Instrument :

BNA_N

ClientSampleId :

C0B63DL


Tot Ion:202 Resp: 27877

Ion Ratio Lower Upper

202 100

101 10.4 0.0 30.6




100 7.9 0.0 28.7

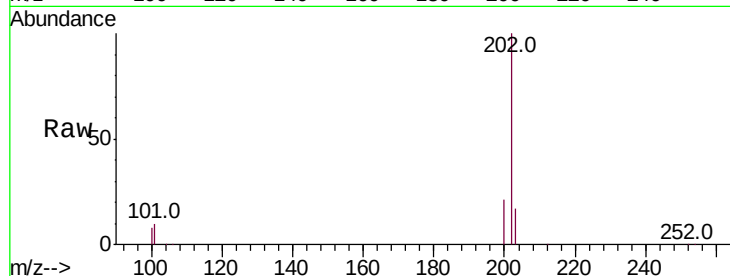

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

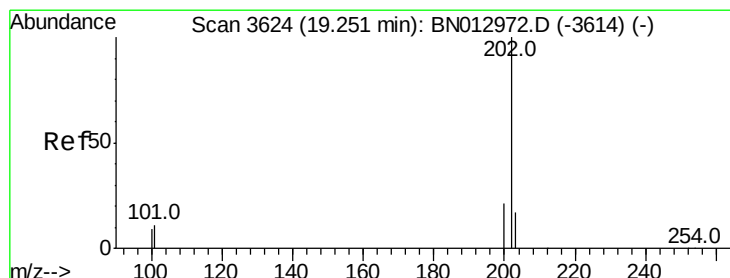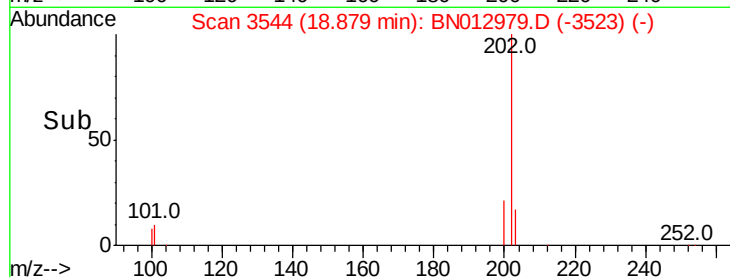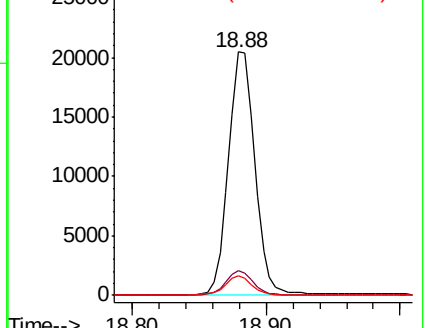

#17

Pyrene

Concen: 1.460 ng/ul

RT: 19.25 min Scan# 3623

Delta R.T. -0.00 min

Lab File: BN012979.D

Acq: 08 Dec 2020 17:16


Tgt Ion:202 Resp: 24172

Ion Ratio Lower Upper

202 100

101 11.8 9.1 13.7



100 9.8 7.5 11.3

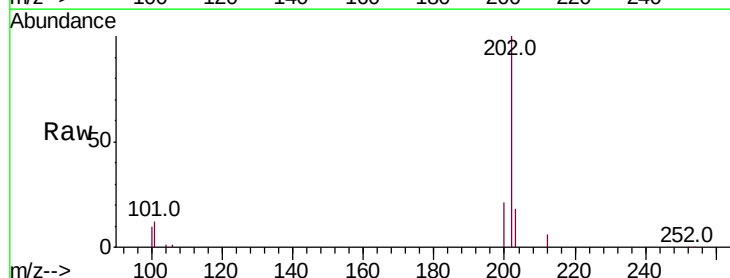


Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

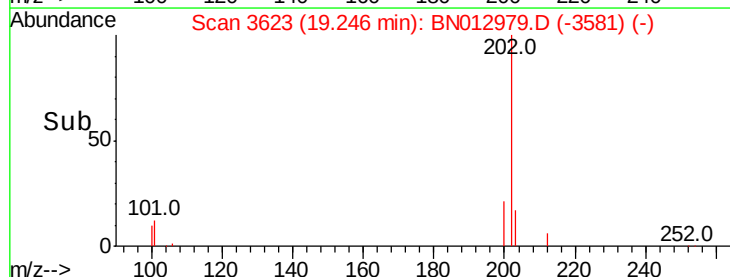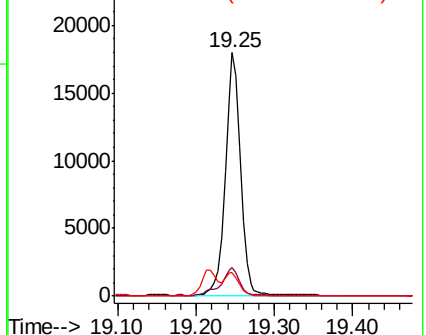

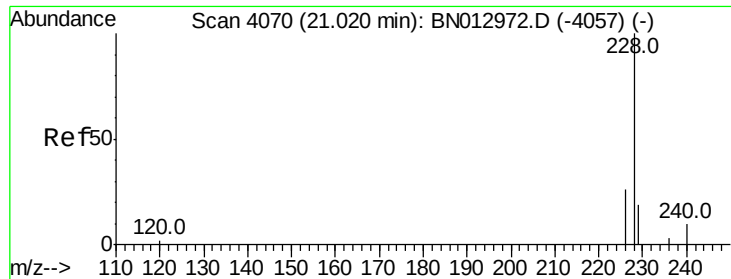

#18

Benzo(a)anthracene

Concen: 0.721 ng/ul

RT: 21.02 min Scan# 4069

Delta R.T. -0.00 min

Lab File: BN012979.D

Acq: 08 Dec 2020 17:16

Instrument :

BNA_N

ClientSampleId :

C0B63DL


Tot Ion:228 Resp: 10457

Ion Ratio Lower Upper




228 100

229 20.5 16.3 24.5

226 28.6 23.4 35.2

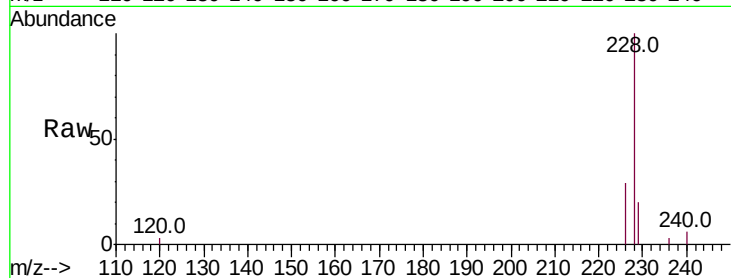

Abundance Ion 228.00 (227.70 to 228.70): E
Ion 229.00 (228.70 to 229.70): E
Ion 226.00 (225.70 to 226.70): E

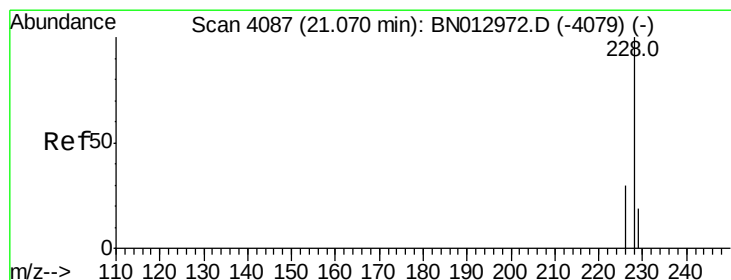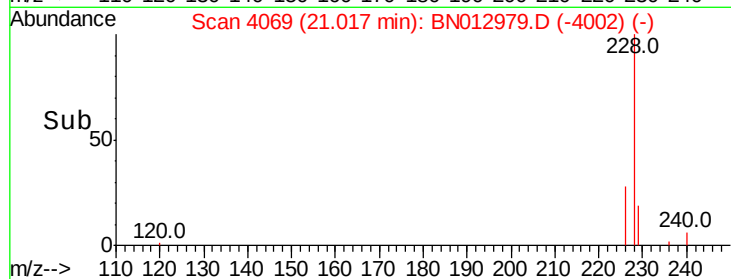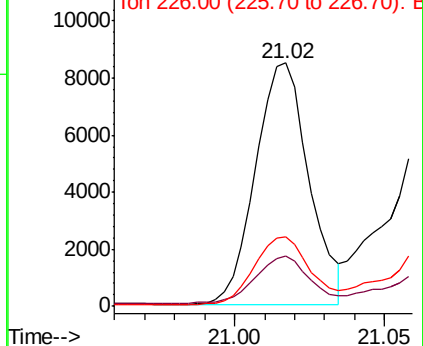

#19

Chrysene

Concen: 0.884 ng/ul

RT: 21.07 min Scan# 4086

Delta R.T. -0.01 min

Lab File: BN012979.D

Acq: 08 Dec 2020 17:16


Tgt Ion:228 Resp: 14161

Ion Ratio Lower Upper



228 100


226 30.9 25.0 37.6

229 20.5 16.4 24.6

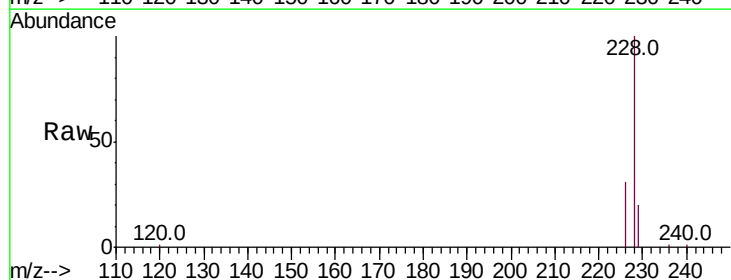

Abundance Ion 228.00 (227.70 to 228.70): E
Ion 226.00 (225.70 to 226.70): E
Ion 229.00 (228.70 to 229.70): E

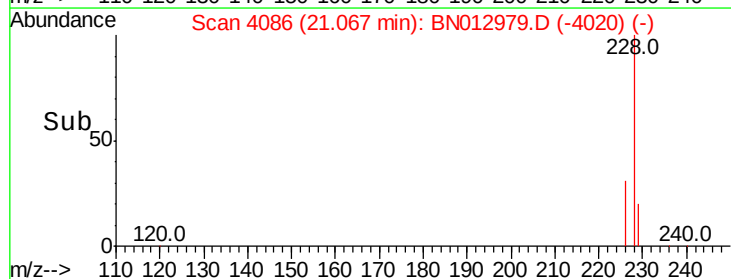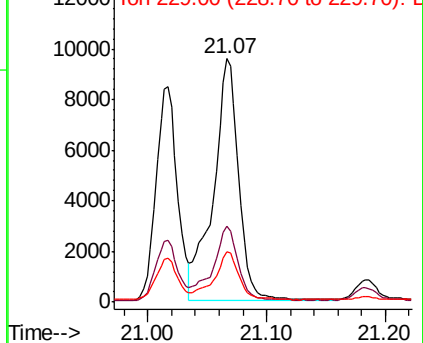

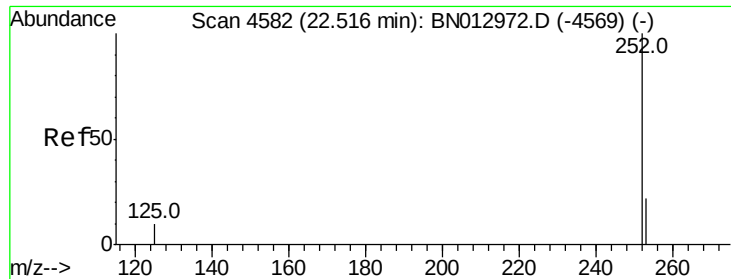

#21

Benzo(b)fluoranthene

Concen: 1.635 ng/ul

RT: 22.52 min Scan# 4582

Delta R.T. -0.00 min

Lab File: BN012979.D

Acq: 08 Dec 2020 17:16

Instrument :

BNA_N

ClientSampleId :

C0B63DL


Tot Ion:252 Resp: 24491

Ion Ratio Lower Upper

252 100

253 24.8 0.0 59.6




125 14.3 0.0 26.0

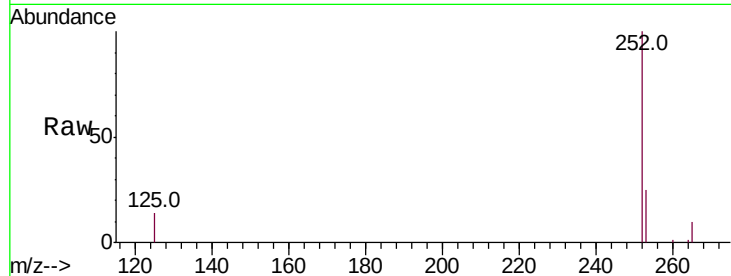

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

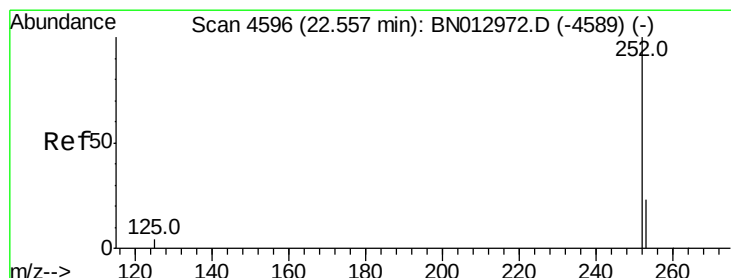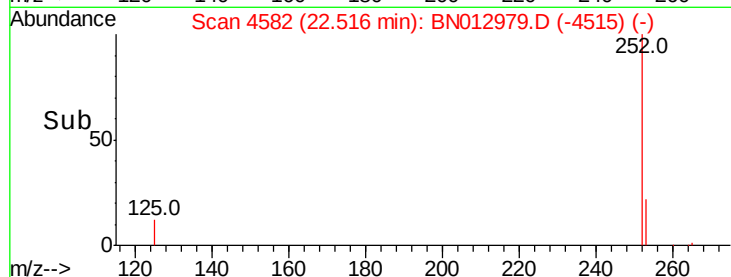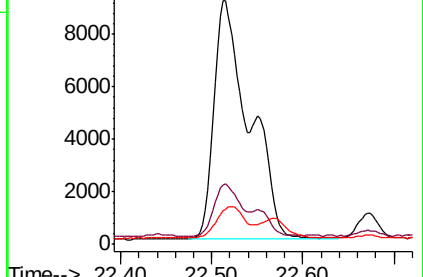

#22

Benzo(k)fluoranthene

Concen: 1.479 ng/ul

RT: 22.52 min Scan# 4582

Delta R.T. -0.04 min

Lab File: BN012979.D

Acq: 08 Dec 2020 17:16


Tgt Ion:252 Resp: 24491

Ion Ratio Lower Upper

252 100

253 24.8 23.4 35.2



125 14.3 11.1 16.7

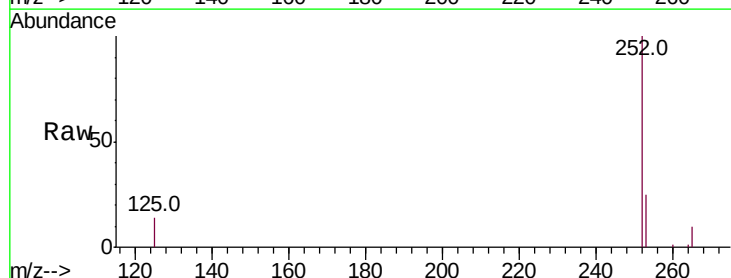


Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

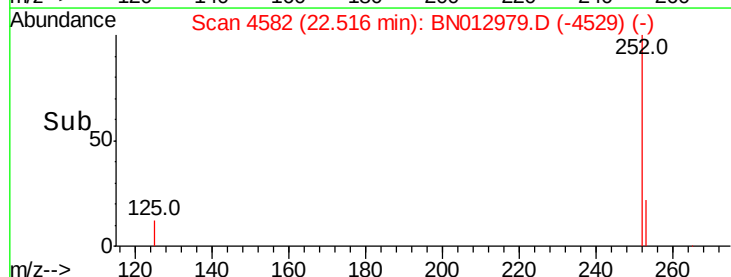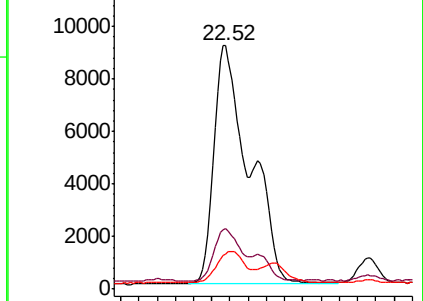

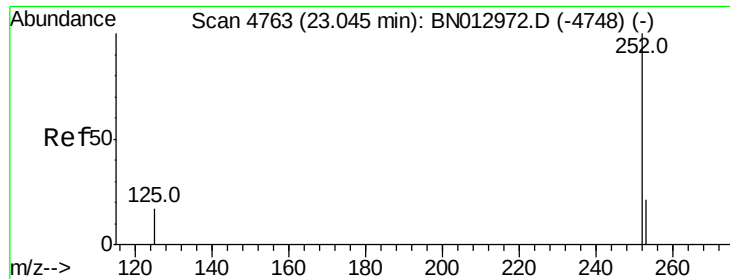

#23

Benzo(a)pyrene

Concen: 0.751 ng/ul

RT: 23.04 min Scan# 4761

Delta R.T. -0.01 min

Lab File: BN012979.D

Acq: 08 Dec 2020 17:16

Instrument :

BNA_N

ClientSampleId :

C0B63DL


Tot Ion:252 Resp: 10443

Ion Ratio Lower Upper




252 100

253 26.2 26.5 39.7#

125 19.5 14.2 21.2

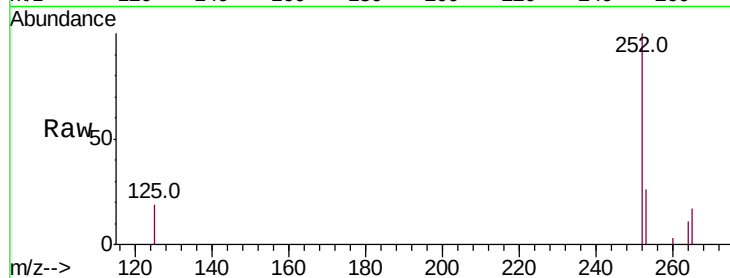

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

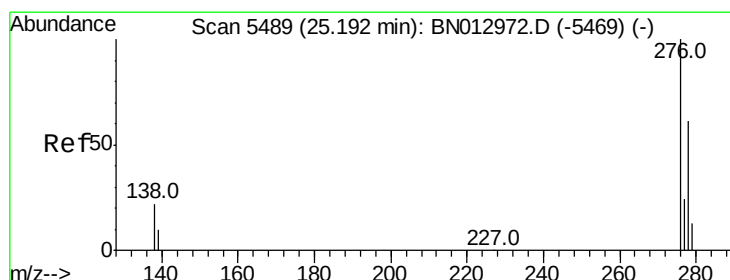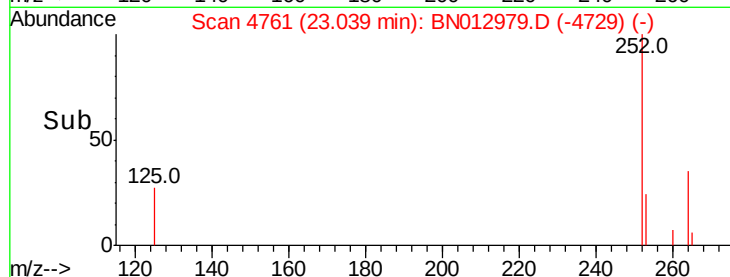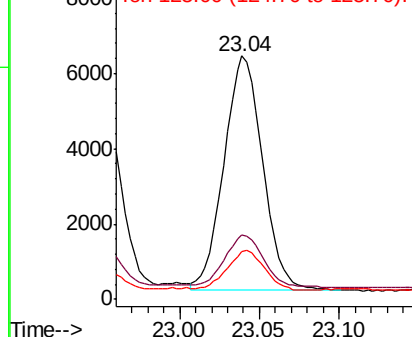

#24

Indeno(1,2,3-cd)pyrene

Concen: 0.411 ng/ul

RT: 25.18 min Scan# 5487

Delta R.T. -0.01 min

Lab File: BN012979.D

Acq: 08 Dec 2020 17:16


Tgt Ion:276 Resp: 7499

Ion Ratio Lower Upper



276 100


138 19.9 16.2 24.2

227 0.1 0.0 0.0#

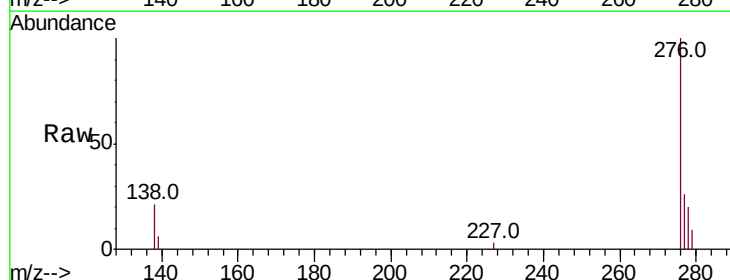

Abundance Ion 276.00 (275.70 to 276.70): E
Ion 138.00 (137.70 to 138.70): E
Ion 227.00 (226.70 to 227.70): E

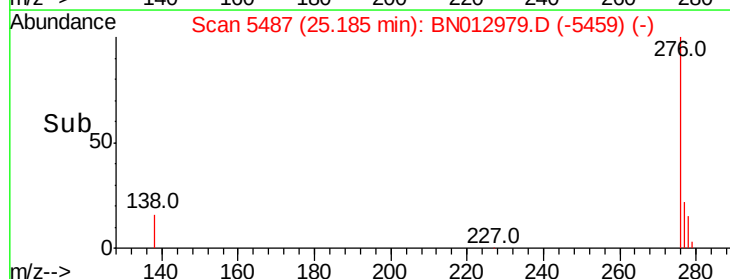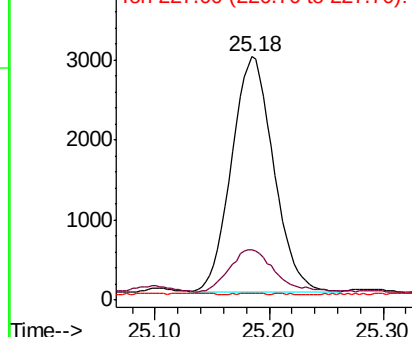

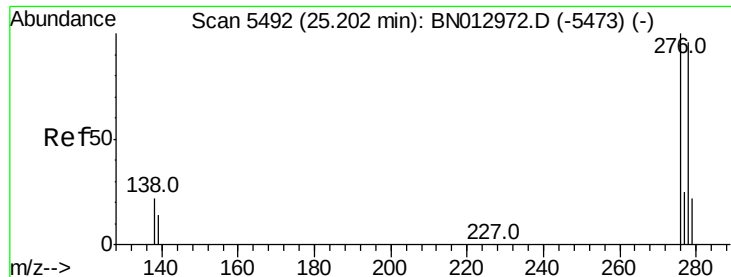

#25

Dibenzo(a,h)anthracene

Concen: 0.123 ng/ul

RT: 25.19 min Scan# 5489

Delta R.T. -0.02 min

Lab File: BN012979.D

Acq: 08 Dec 2020 17:16

Instrument :

BNA_N

ClientSampleId :

C0B63DL


Tot Ion:278 Resp: 1778

Ion Ratio Lower Upper

278 100

139 28.1 14.5 21.7#

279 43.2 26.3 39.5#

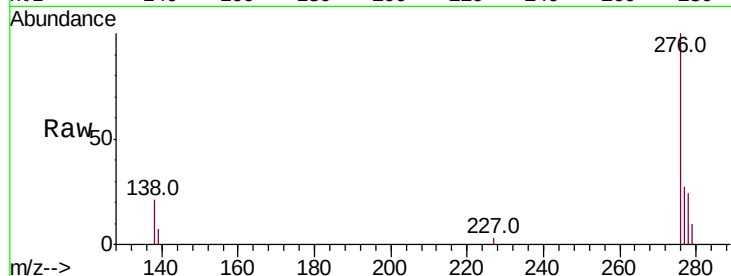


Abundance Ion 278.00 (277.70 to 278.70): E

Ion 139.00 (138.70 to 139.70): E


Ion 279.00 (278.70 to 279.70): E

25.19

Time-->

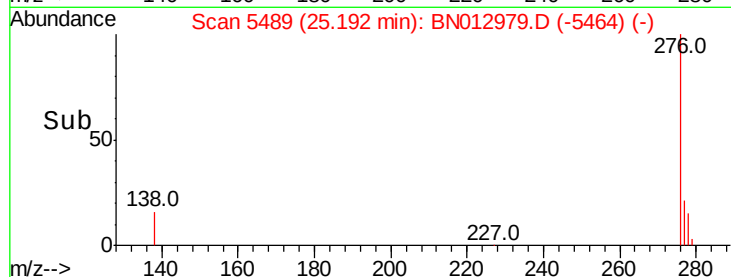

Time-->

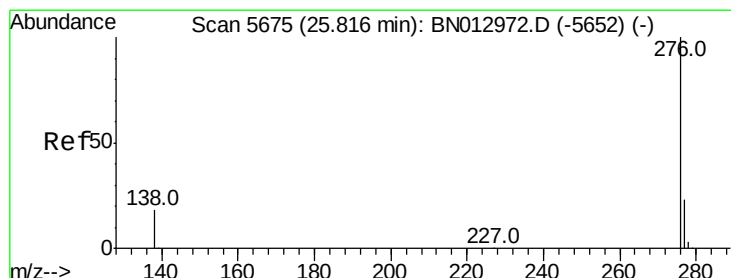

#26

Benzo(g,h,i)perylene

Concen: 0.415 ng/ul

RT: 25.81 min Scan# 5674

Delta R.T. -0.01 min

Lab File: BN012979.D

Acq: 08 Dec 2020 17:16


Tgt Ion:276 Resp: 6851

Ion Ratio Lower Upper

276 100

138 22.5 16.3 24.5

277 27.1 21.8 32.6

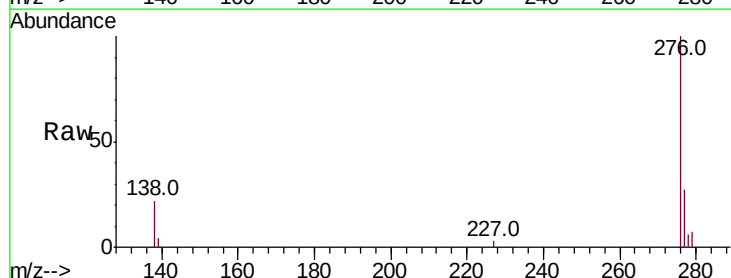


Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

25.81

Time-->

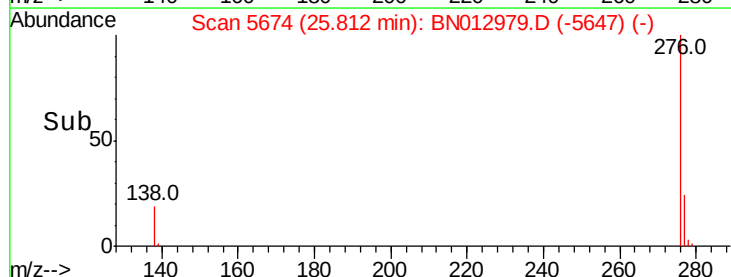

Time-->