

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120720\
 Data File : BN012986.D
 Acq On : 08 Dec 2020 21:29
 Operator : CG/JU
 Sample : L4859-04DL 10X
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0B94DL

Quant Time: Dec 09 00:14:55 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN120320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 09 00:11:42 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.39	152	1228	0.40	ng/ul	0.00
2) Naphthalene-d8	10.15	136	4859	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.05	164	2665	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.81	188	5349	0.40	ng/ul	0.00
16) Chrysene-d12	21.03	240	3759	0.40	ng/ul	0.00
20) Perylene-d12	23.13	264	3556	0.40	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	11.76	152	161	0.02	ng/ul	0.00
14) Fluoranthene-d10	18.85	212	345	0.02	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
7) Acenaphthylene	13.76	152	347	0.028	ng/ul#	67
8) Acenaphthene	14.11	153	211	0.020	ng/ul#	91
9) Fluorene	15.11	166	255	0.021	ng/ul#	91
12) Phenanthrene	16.85	178	6562	0.366	ng/ul	98
13) Anthracene	16.94	178	1295	0.085	ng/ul#	96
15) Fluoranthene	18.88	202	19458	0.913	ng/ul	97
17) Pyrene	19.25	202	17206	0.969	ng/ul	99
18) Benzo(a)anthracene	21.01	228	8547	0.550	ng/ul	98
19) Chrysene	21.07	228	9701	0.565	ng/ul	98
21) Benzo(b)fluoranthene	22.51	252	16644	1.012	ng/ul	95
22) Benzo(k)fluoranthene	22.51	252	16644	0.915	ng/ul	96
23) Benzo(a)pyrene	23.04	252	7858	0.515	ng/ul	93
24) Indeno(1,2,3-cd)pyrene	25.18	276	5519	0.275	ng/ul#	97
25) Dibenzo(a,h)anthracene	25.19	278	1339	0.084	ng/ul#	65
26) Benzo(g,h,i)perylene	25.81	276	4830	0.266	ng/ul	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120720\
Data File : BN012986.D
Acq On : 08 Dec 2020 21:29
Operator : CG/JU
Sample : L4859-04DL 10X
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0B94DL

Quant Time: Dec 09 00:14:55 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN120320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 09 00:11:42 2020
Response via : Initial Calibration

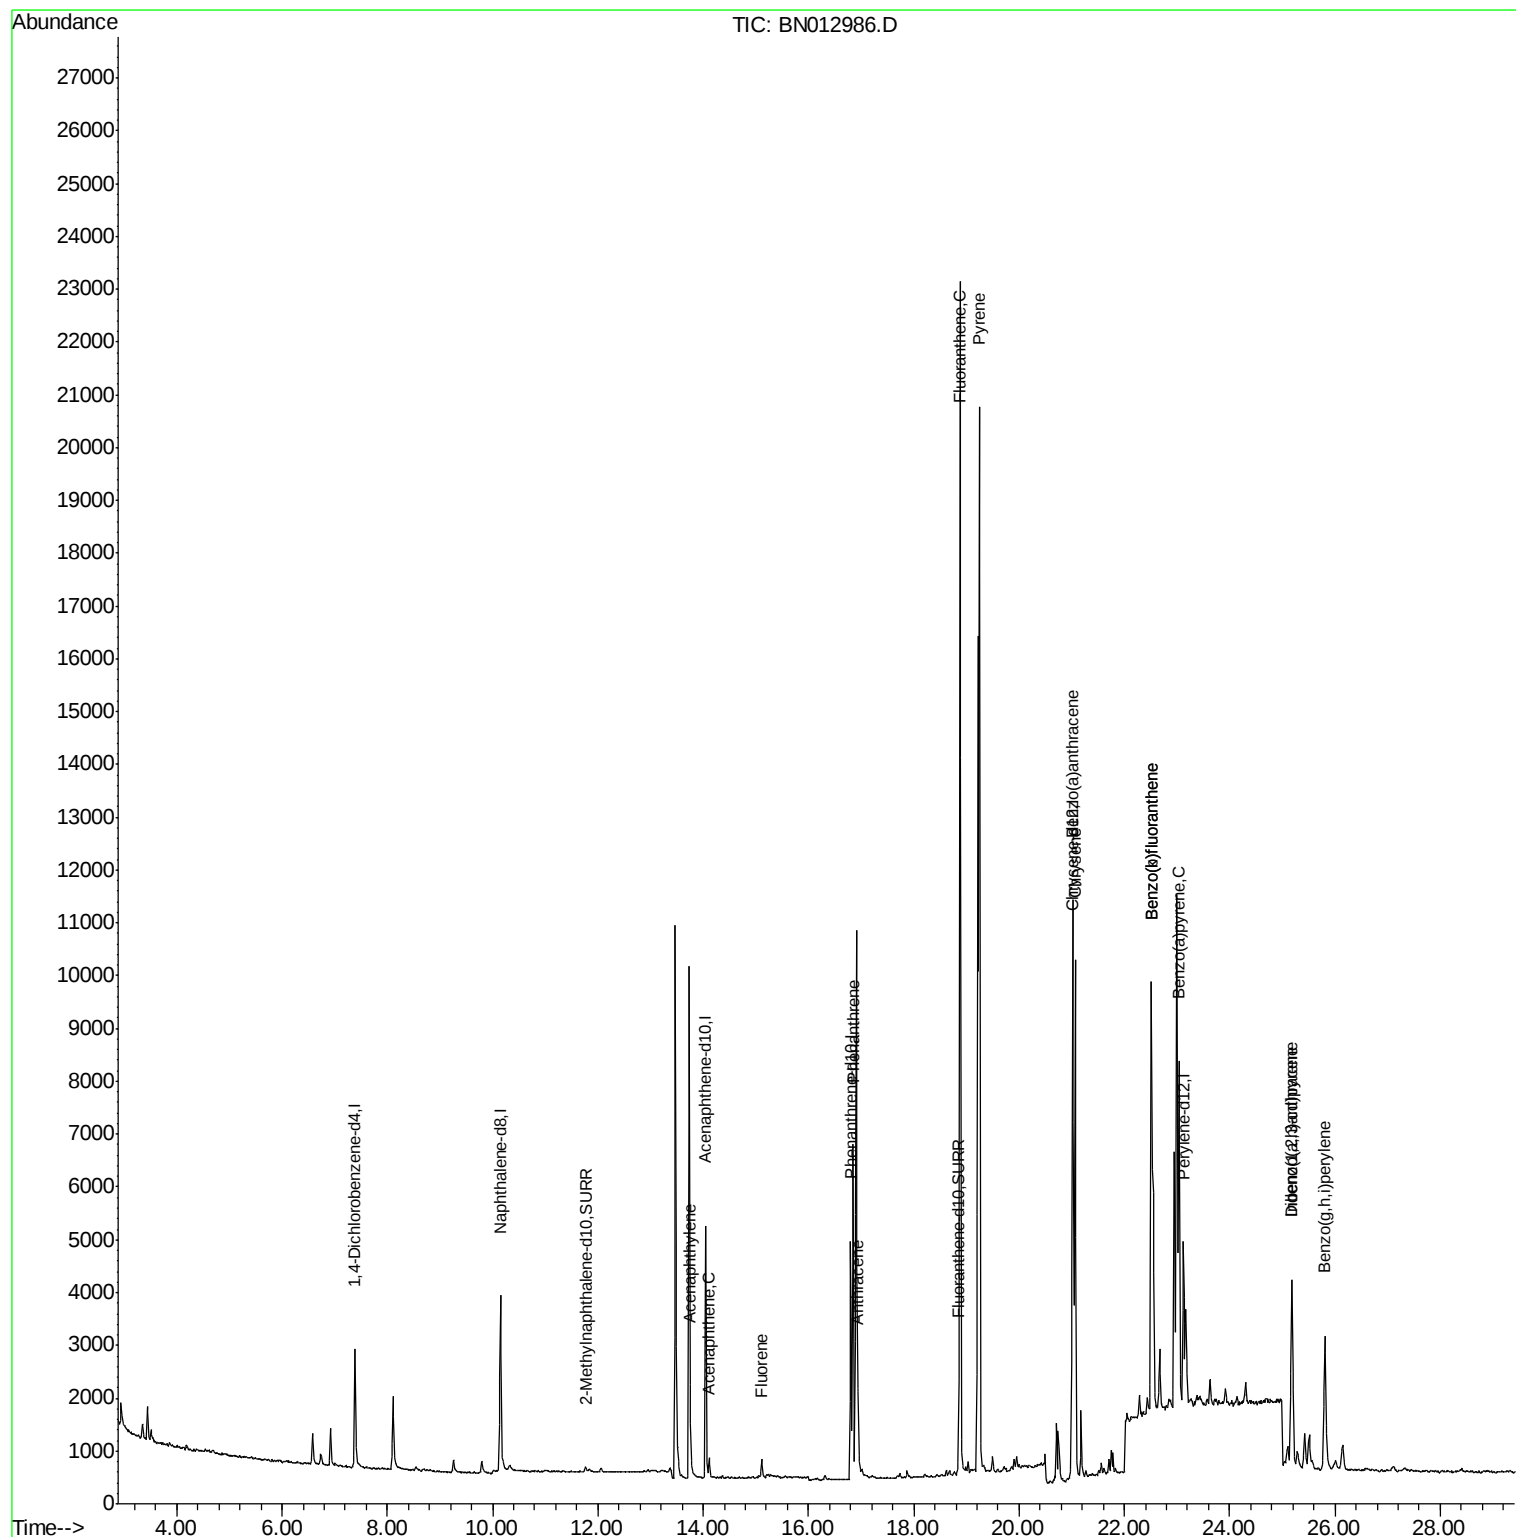

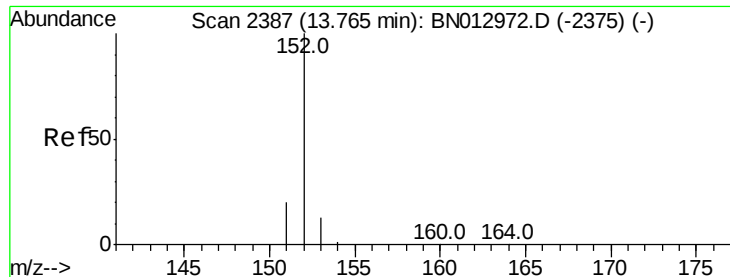

#7

Acenaphthylene

Concen: 0.028 ng/ul

RT: 13.76 min Scan# 2387

Delta R.T. -0.00 min

Lab File: BN012986.D

Acq: 08 Dec 2020 21:29

Instrument :

BNA_N

ClientSampleId :

C0B94DL


Tot Ion:152 Resp: 347

Ion Ratio Lower Upper

152 100

151 37.7 18.2 27.4#




153 31.4 13.1 19.7#

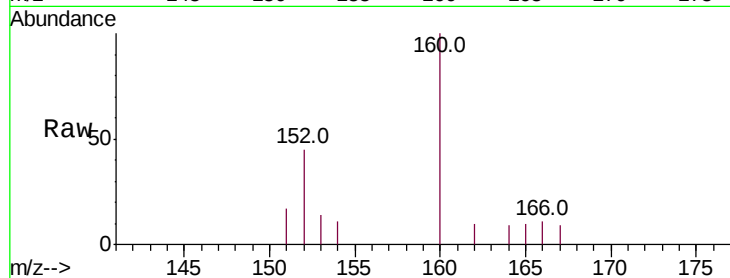

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

Ion 153.00 (152.70 to 153.70): E

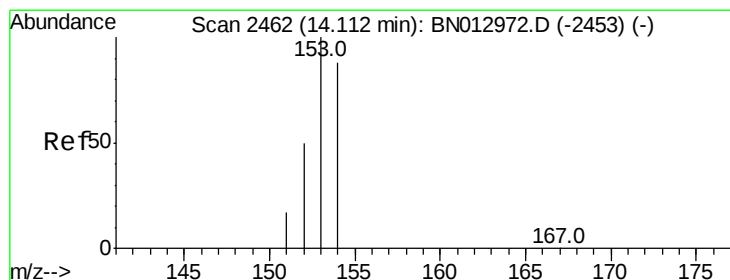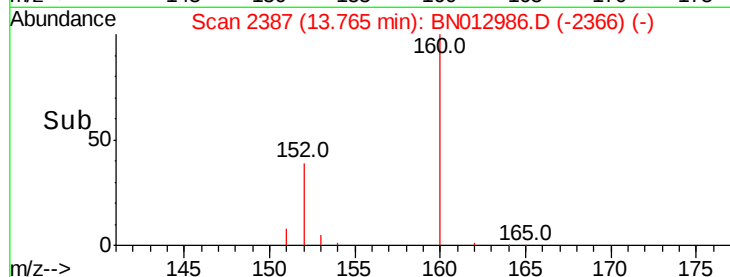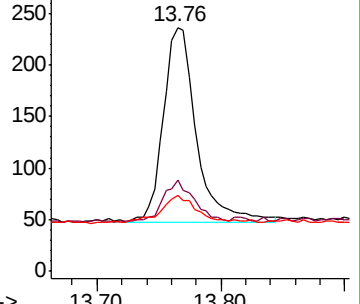

#8

Acenaphthene

Concen: 0.020 ng/ul

RT: 14.11 min Scan# 2462

Delta R.T. -0.00 min

Lab File: BN012986.D

Acq: 08 Dec 2020 21:29


Tgt Ion:153 Resp: 211

Ion Ratio Lower Upper

153 100

152 63.3 40.7 61.1#



154 92.0 70.8 106.2

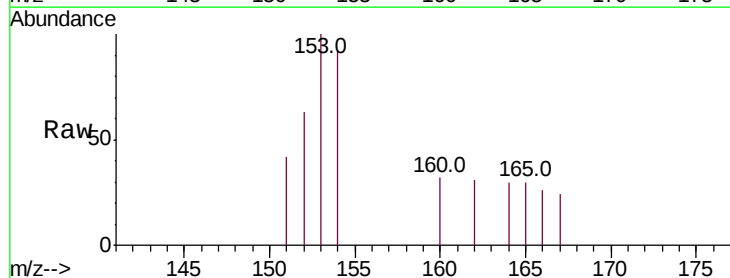


Abundance Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E

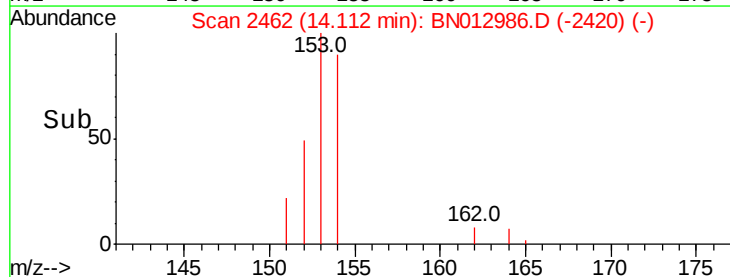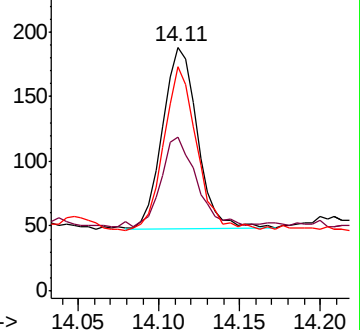



#9

Fluorene

Concen: 0.021 ng/ul

RT: 15.11 min Scan# 2678

Delta R.T. -0.00 min

Lab File: BN012986.D

Acq: 08 Dec 2020 21:29

Instrument :

BNA_N

ClientSampleId :

C0B94DL


Tot Ion:166 Resp: 255

Ion Ratio Lower Upper




166 100

165 97.0 79.8 119.8

167 35.5 13.8 20.8#



Abundance Ion 166.00 (165.70 to 166.70): E
Ion 165.00 (164.70 to 165.70): E
Ion 167.00 (166.70 to 167.70): E

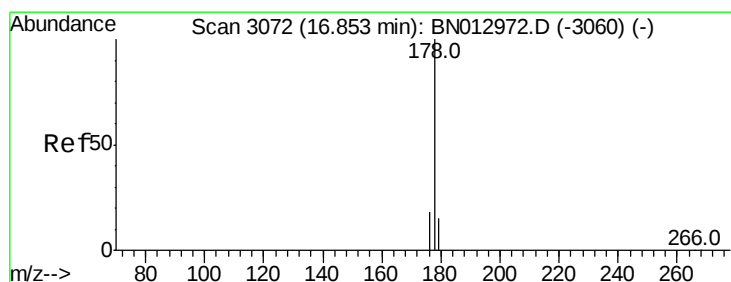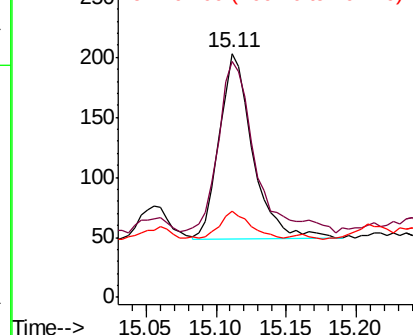

#12

Phenanthrene

Concen: 0.366 ng/ul

RT: 16.85 min Scan# 3071

Delta R.T. -0.00 min

Lab File: BN012986.D

Acq: 08 Dec 2020 21:29


Tgt Ion:178 Resp: 6562

Ion Ratio Lower Upper



178 100


179 16.1 13.6 20.4

176 20.0 16.4 24.6

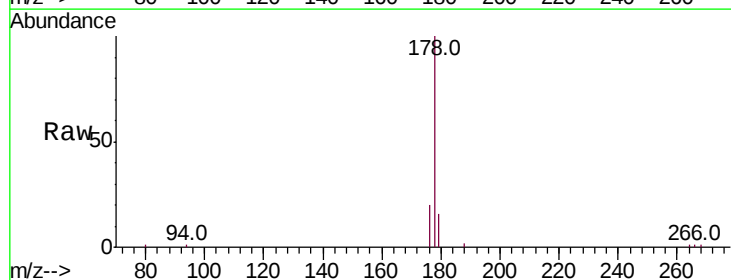

Abundance Ion 178.00 (177.70 to 178.70): E
Ion 179.00 (178.70 to 179.70): E
Ion 176.00 (175.70 to 176.70): E

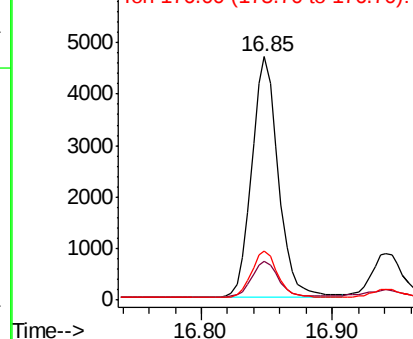

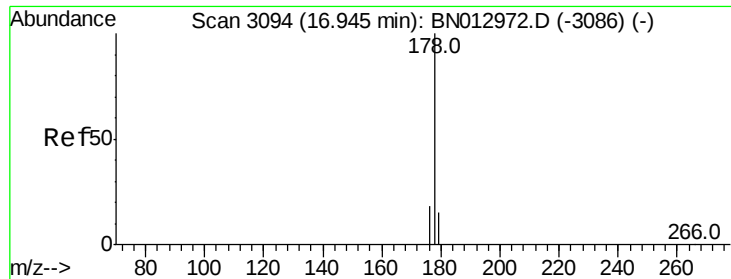

#13

Anthracene

Concen: 0.085 ng/ul

RT: 16.94 min Scan# 3093

Delta R.T. -0.00 min

Lab File: BN012986.D

Acq: 08 Dec 2020 21:29

Instrument :

BNA_N

ClientSampleId :

C0B94DL


Tot Ion:178 Resp: 1295

Ion Ratio Lower Upper

178 100

179 22.1 14.6 21.8#




176 21.7 17.1 25.7



Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

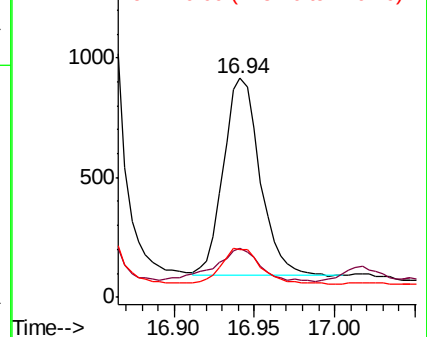

#15

Fluoranthene

Concen: 0.913 ng/ul

RT: 18.88 min Scan# 3544

Delta R.T. -0.00 min

Lab File: BN012986.D

Acq: 08 Dec 2020 21:29


Tgt Ion:202 Resp: 19458

Ion Ratio Lower Upper

202 100

101 9.7 0.0 30.6



100 7.6 0.0 28.7




Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

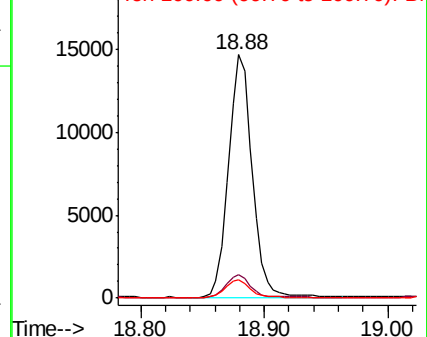



#17

Pvrene

Concen: 0.969 ng/ul

RT: 19.25 min Scan# 3623

Delta R.T. -0.00 min

Lab File: BN012986.D

Acq: 08 Dec 2020 21:29

Instrument :

BNA_N

ClientSampleId :

C0B94DL


Tot Ion:202 Resp: 17206

Ion Ratio Lower Upper

202 100

101 10.9 9.1 13.7




100 9.1 7.5 11.3

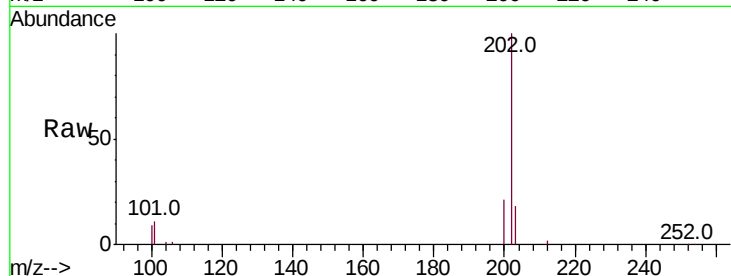

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

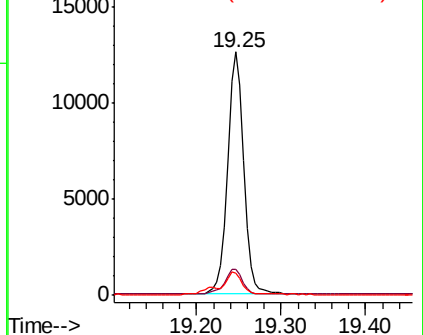

#18

Benzo(a)anthracene

Concen: 0.550 ng/ul

RT: 21.01 min Scan# 4068

Delta R.T. -0.01 min

Lab File: BN012986.D

Acq: 08 Dec 2020 21:29


Tgt Ion:228 Resp: 8547

Ion Ratio Lower Upper

228 100

229 21.3 16.3 24.5



226 28.6 23.4 35.2




Abundance Ion 228.00 (227.70 to 228.70): E

Ion 229.00 (228.70 to 229.70): E

Ion 226.00 (225.70 to 226.70): E

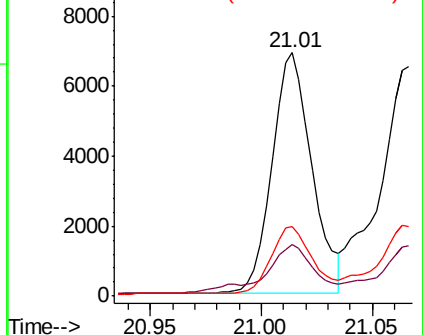

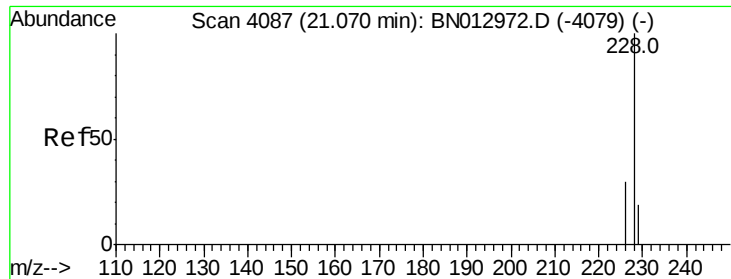

#19

Chrysene

Concen: 0.565 ng/ul

RT: 21.07 min Scan# 4086

Delta R.T. -0.01 min

Lab File: BN012986.D

Acq: 08 Dec 2020 21:29

Instrument :

BNA_N

ClientSampleId :

C0B94DL


Tot Ion:228 Resp: 9701

Ion Ratio Lower Upper

228 100

226 30.5 25.0 37.6




229 22.2 16.4 24.6



Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

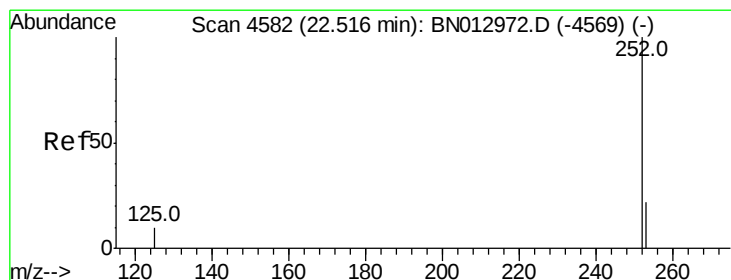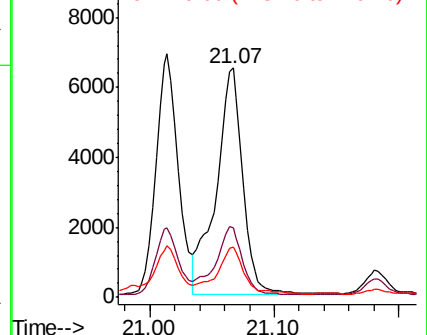

#21

Benzo(b)fluoranthene

Concen: 1.012 ng/ul

RT: 22.51 min Scan# 4580

Delta R.T. -0.01 min

Lab File: BN012986.D

Acq: 08 Dec 2020 21:29


Tgt Ion:252 Resp: 16644

Ion Ratio Lower Upper

252 100

253 26.5 0.0 59.6



125 13.5 0.0 26.0

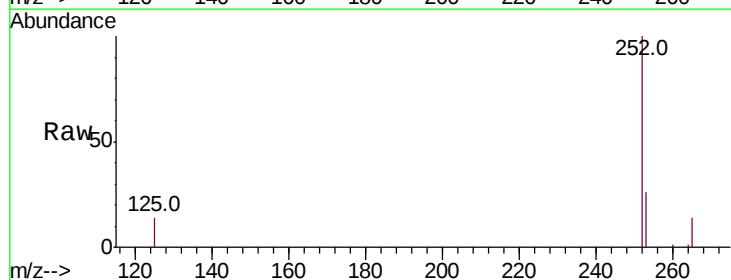


Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

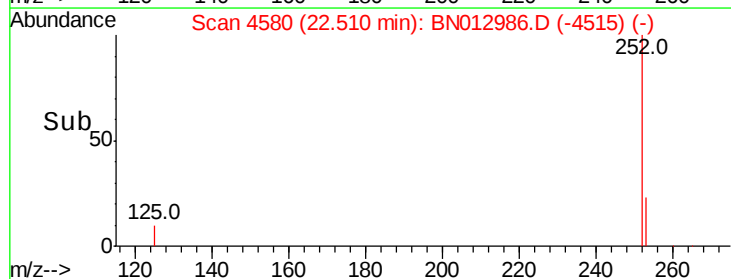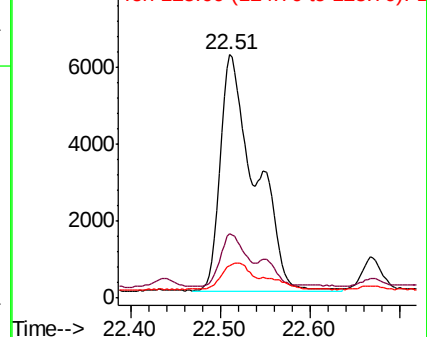

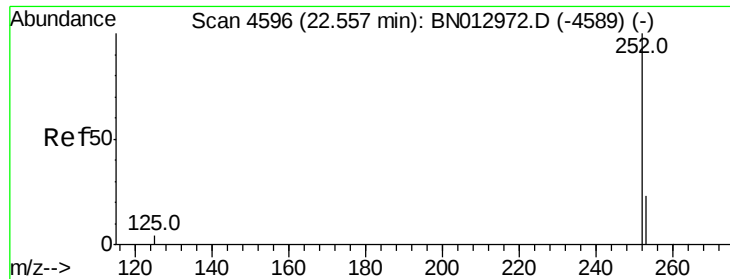

#22

Benzo(k)fluoranthene

Concen: 0.915 ng/ul

RT: 22.51 min Scan# 4580

Delta R.T. -0.05 min

Lab File: BN012986.D

Acq: 08 Dec 2020 21:29

Instrument :

BNA_N

ClientSampleId :

C0B94DL


Tot Ion:252 Resp: 16644

Ion Ratio Lower Upper




252 100

253 26.5 23.4 35.2

125 13.5 11.1 16.7

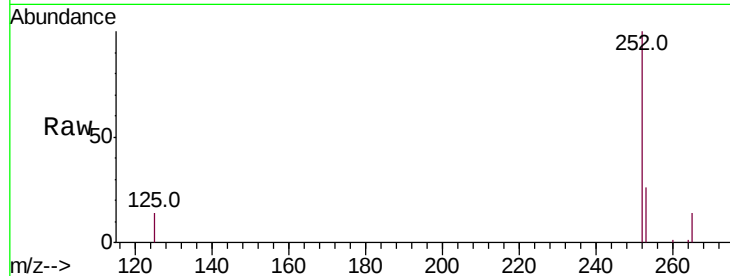

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

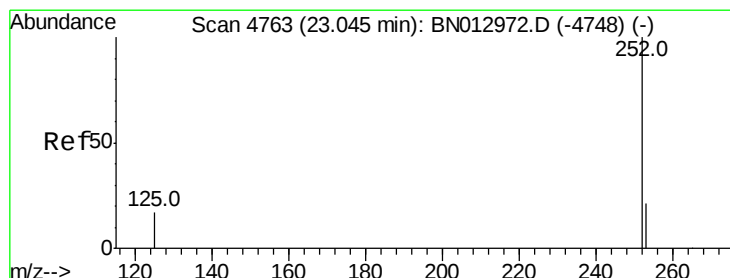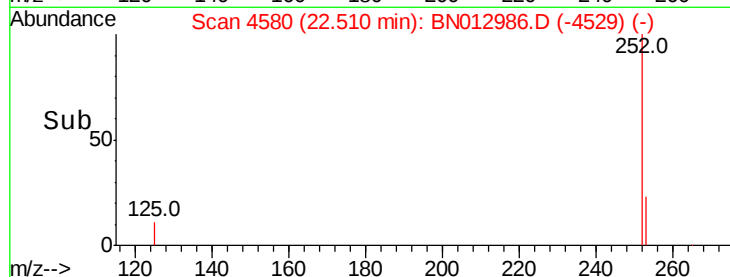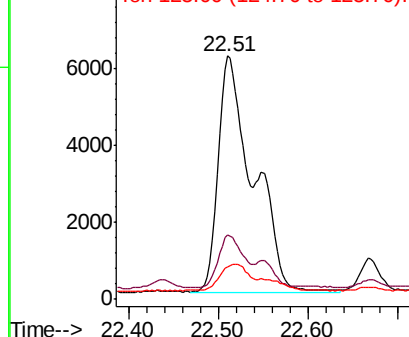

#23

Benzo(a)pyrene

Concen: 0.515 ng/ul

RT: 23.04 min Scan# 4760

Delta R.T. -0.01 min

Lab File: BN012986.D

Acq: 08 Dec 2020 21:29


Tgt Ion:252 Resp: 7858

Ion Ratio Lower Upper



252 100


253 28.2 26.5 39.7

125 19.9 14.2 21.2

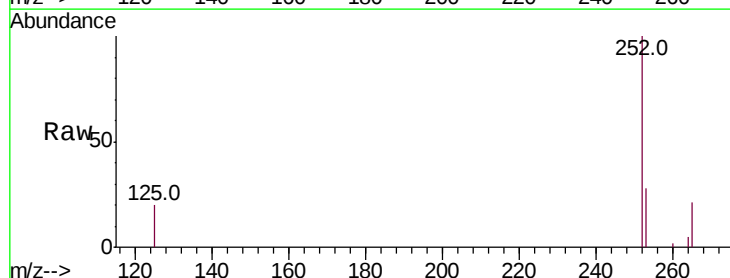

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

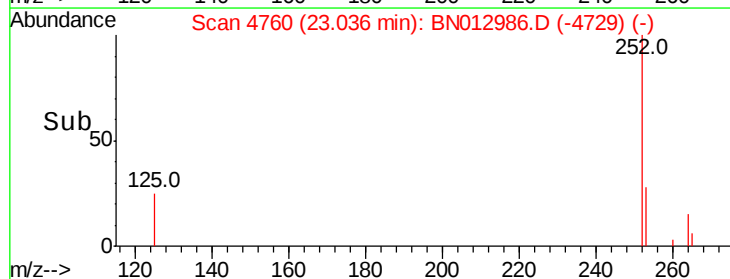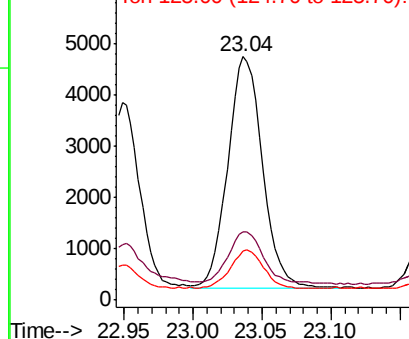



#24

Indeno(1,2,3-cd)pyrene

Concen: 0.275 ng/u1

RT: 25.18 min Scan# 5486

Delta R.T. -0.01 min

Lab File: BN012986.D

Acq: 08 Dec 2020 21:29

Instrument :

BNA_N

ClientSampleId :

C0B94DL


Tot Ion:276 Resp: 5519

Ion Ratio Lower Upper

276 100

138 18.8 16.2 24.2




227 0.1 0.0 0.0#



Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 227.00 (226.70 to 227.70): E

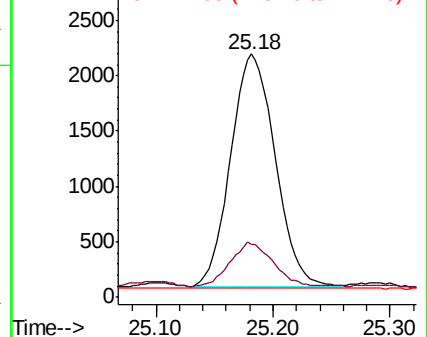

#25

Dibenzo(a,h)anthracene

Concen: 0.084 ng/u1

RT: 25.19 min Scan# 5488

Delta R.T. -0.02 min

Lab File: BN012986.D

Acq: 08 Dec 2020 21:29


Tgt Ion:278 Resp: 1339

Ion Ratio Lower Upper

278 100

139 31.8 14.5 21.7#



279 53.6 26.3 39.5#




Abundance Ion 278.00 (277.70 to 278.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 279.00 (278.70 to 279.70): E

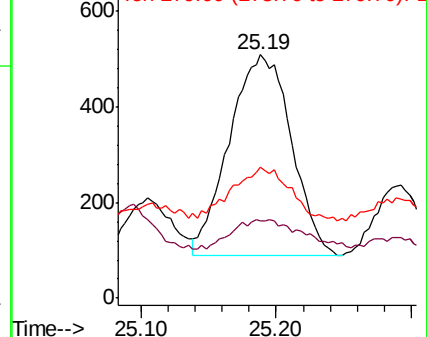



#26

Benzo(a,h,i)perylene

Concen: 0.266 ng/ul

RT: 25.81 min Scan# 5673

Delta R.T. -0.01 min

Lab File: BN012986.D

Acq: 08 Dec 2020 21:29

Instrument :

BNA_N

ClientSampleId :

C0B94DL


Tot Ion:276 Resp: 4830

Ion Ratio Lower Upper

276 100

138 23.2 16.3 24.5

277 28.4 21.8 32.6



Abundance

Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

