


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN120720\
Data File : BN012933.D
Acq On : 07 Dec 2020 11:28
Operator : CG/JU
Sample : PB133283BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK83

Manual Integrations
APPROVED

mohammad
12/9/2020 12:20:45 PM

Quant Time: Dec 07 12:27:16 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN120320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 07 12:24:06 2020
Response via : Initial Calibration

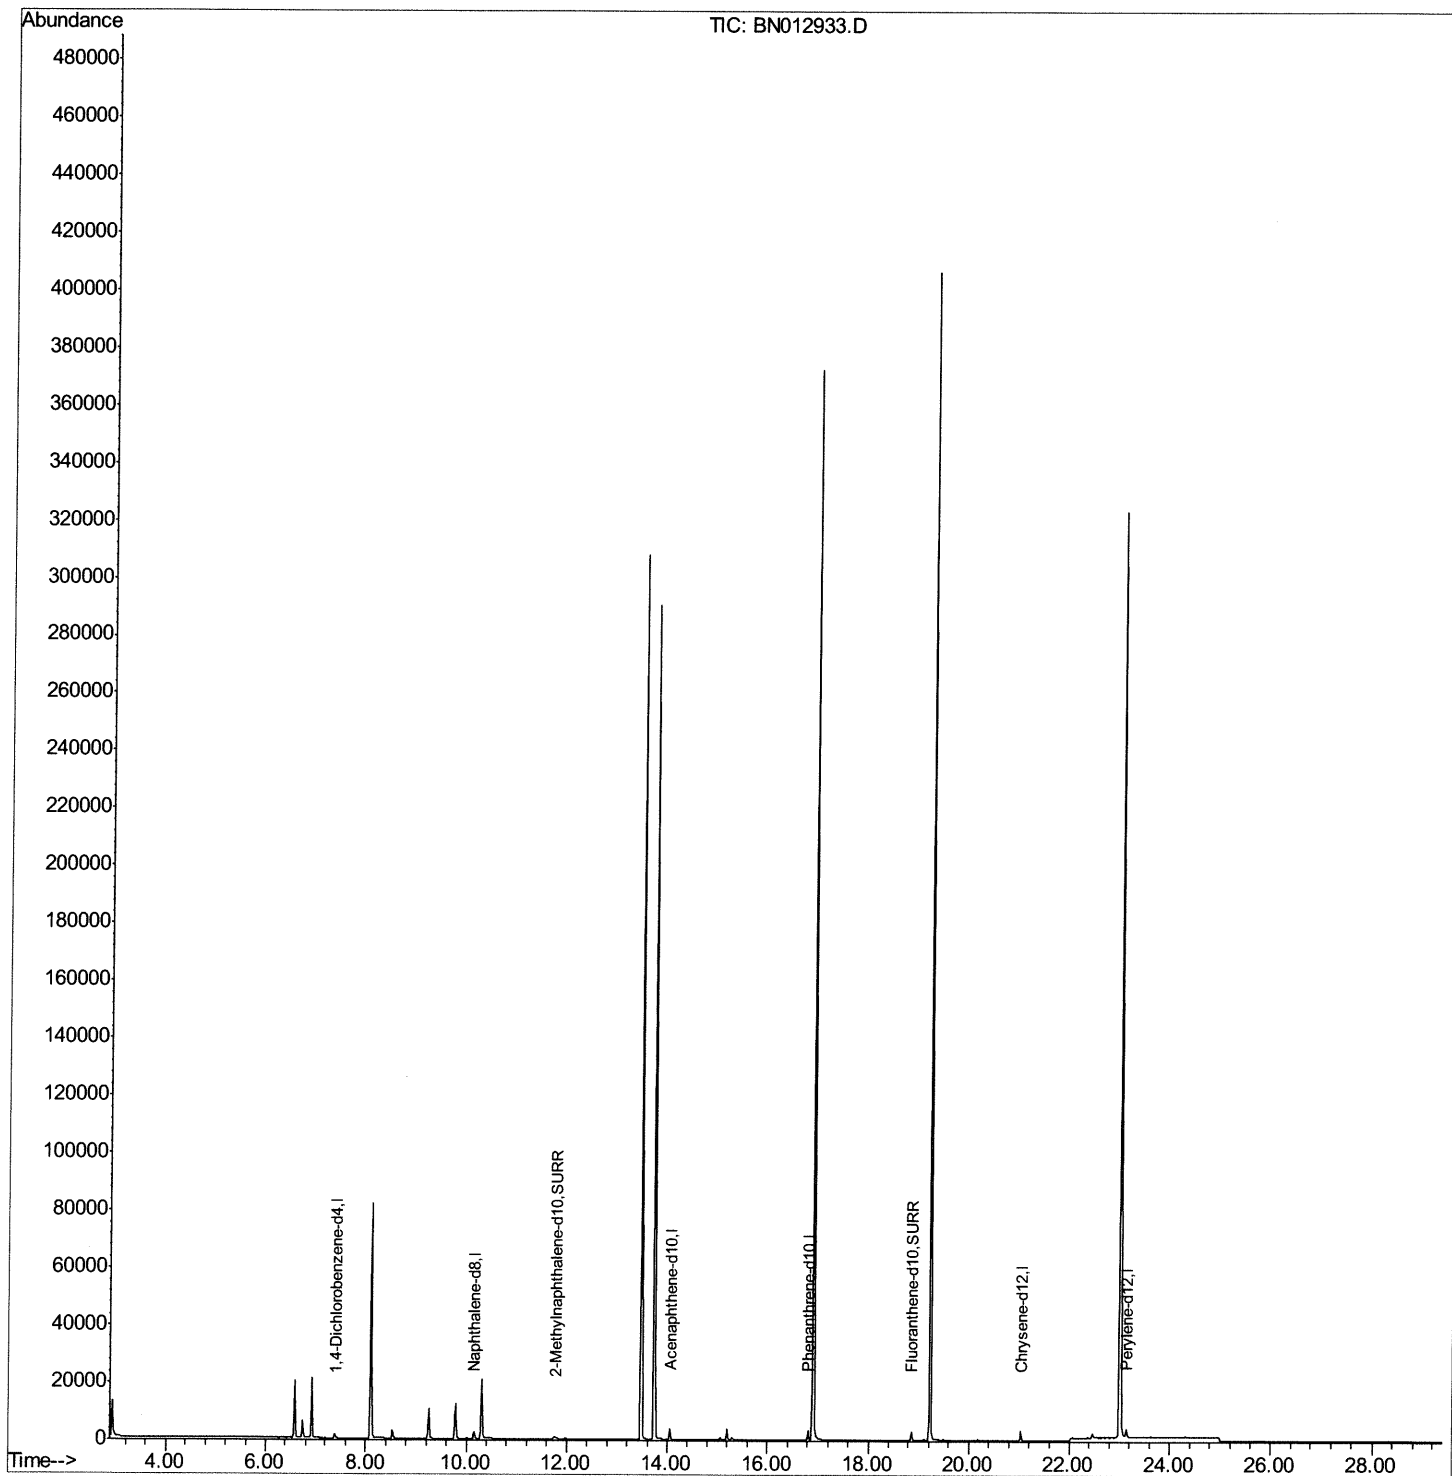




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN120720\
Data File : BN012933.D
Acq On : 07 Dec 2020 11:28
Operator : CG/JU
Sample : PB133283BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK83

Manual Integrations
APPROVED

mohammad
12/9/2020 12:20:45 PM

Quant Time: Dec 07 12:26:08 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN120320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 07 12:24:06 2020
Response via : Initial Calibration

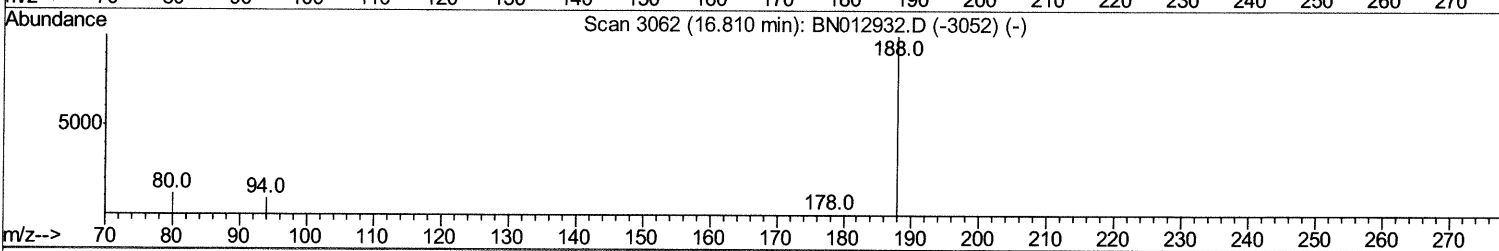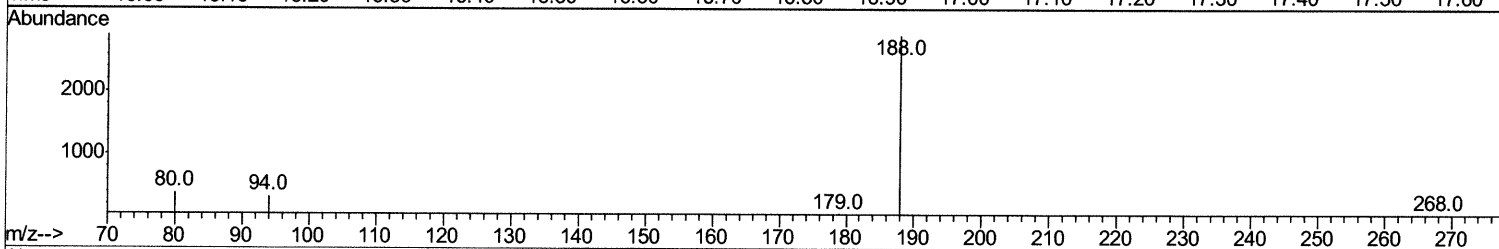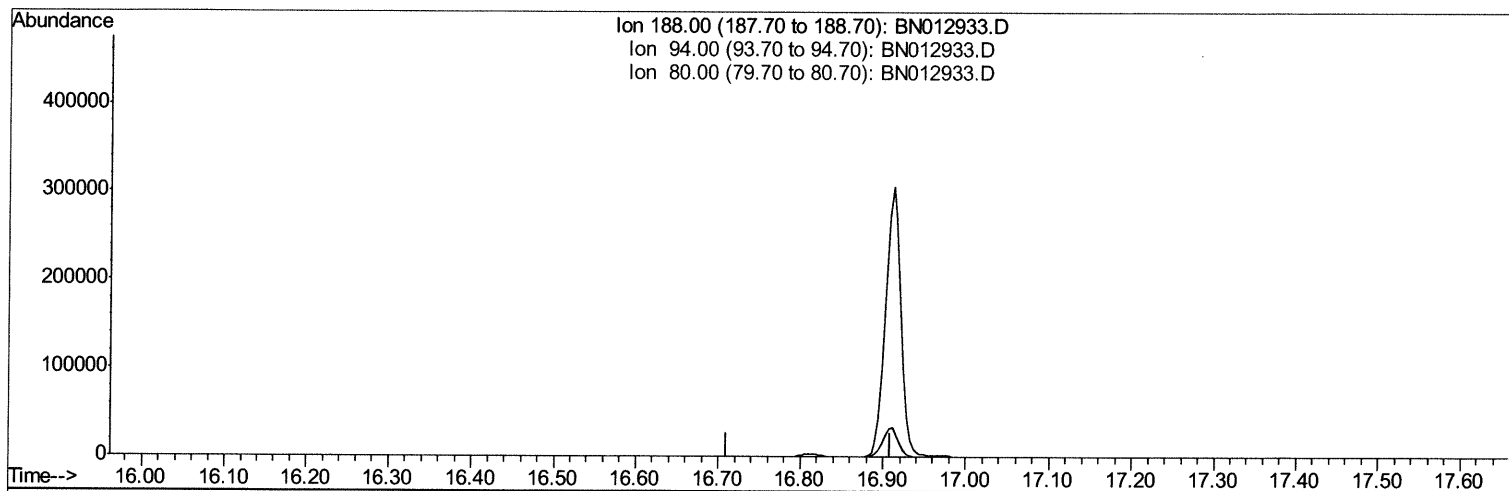

TIC: BN012933.D

(10) Phenanthrene-d10 (I)

16.810min (-16.810) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.40	0.00#
80.00	12.40	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN120720\
Data File : BN012933.D
Acq On : 07 Dec 2020 11:28
Operator : CG/JU
Sample : PB133283BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK83

Manual Integrations
APPROVED

mohammad
12/9/2020 12:20:45 PM

Quant Time: Dec 07 12:26:08 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN120320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 07 12:24:06 2020
Response via : Initial Calibration

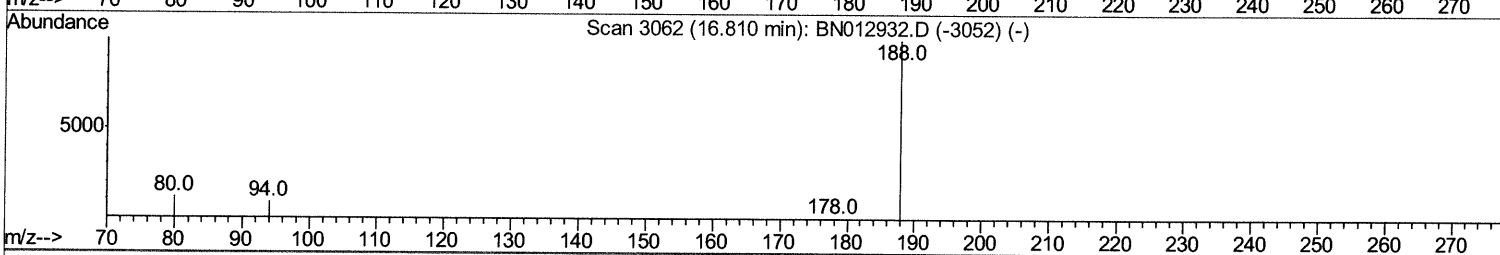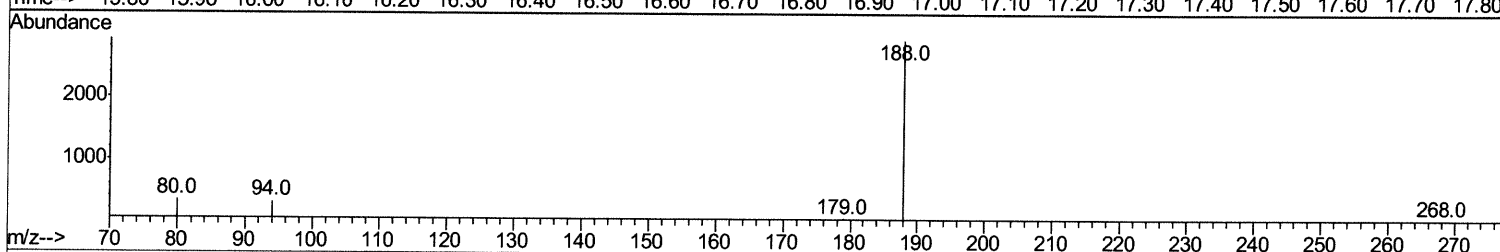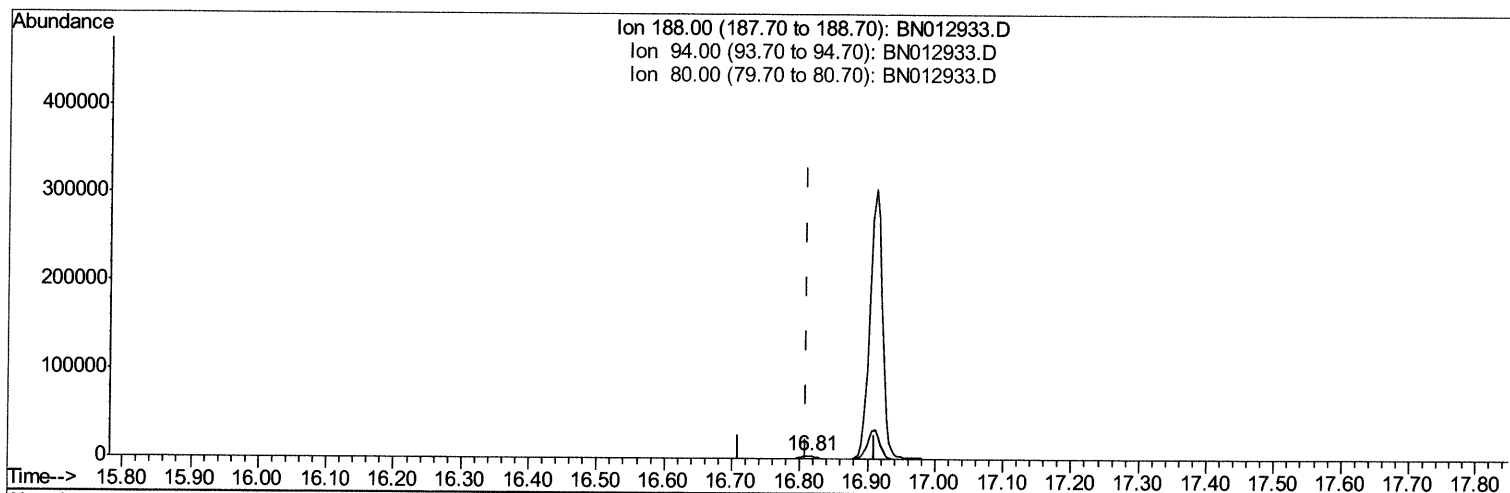

TIC: BN012933.D

(10) Phenanthrene-d10 (I)

16.814min (+0.004) 0.40ng/ul m 12/09/2020

response 4309

Ion	Exp%	Act%
188.00	100	100
94.00	11.40	10.49
80.00	12.40	11.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN120720\
 Data File : BN012933.D
 Acq On : 07 Dec 2020 11:28
 Operator : CG/JU
 Sample : PB133283BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK83

Manual Integrations
 APPROVED

mohammad
 12/9/2020 12:20:45 PM

Quant Time: Dec 07 12:27:16 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN120320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 07 12:24:06 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.39	152	854	0.40	ng/ul	0.00
2) Naphthalene-d8	10.15	136	3353	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.06	164	1986	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.81	188	4309m>	0.40	ng/ul >	0.00
16) Chrysene-d12	21.04	240	3302	0.40	ng/ul	0.00
20) Perylene-d12	23.14	264	3658	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.76	152	1634	0.33	ng/ul	0.00
14) Fluoranthene-d10	18.86	212	3467	0.30	ng/ul	0.00

Target Compounds

Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed