


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN120720\
Data File : BN012936.D
Acq On : 07 Dec 2020 13:16
Operator : CG/JU
Sample : L4859-10
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0BE3

Manual Integrations
APPROVED

mohammad
12/9/2020 12:20:53 PM

Quant Time: Dec 07 13:54:42 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN120320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 07 12:24:06 2020
Response via : Initial Calibration

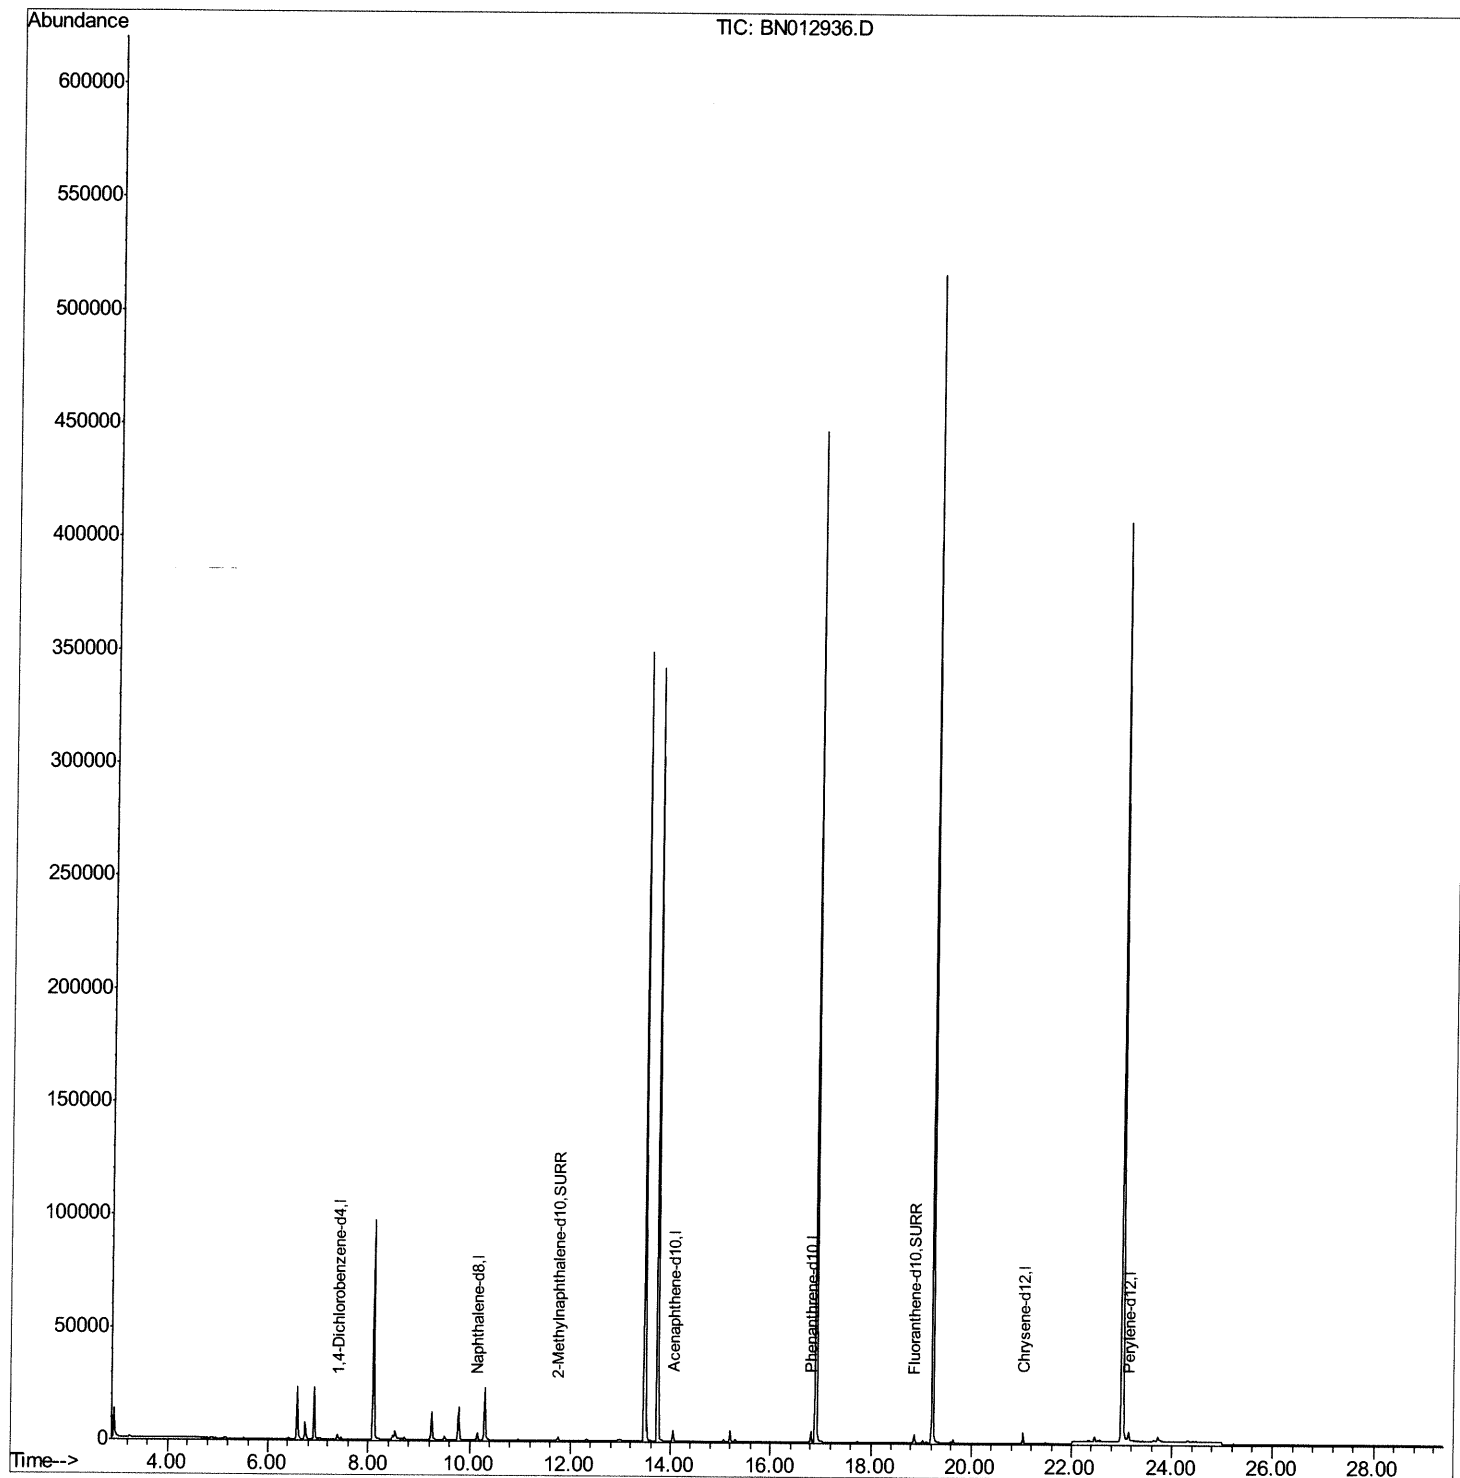

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN120720\
 Data File : BN012936.D
 Acq On : 07 Dec 2020 13:16
 Operator : CG/JU
 Sample : L4859-10
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
ClientSampleId :
 C0BE3

Manual Integrations
APPROVED

mohammad
 12/9/2020 12:20:53 PM

Quant Time: Dec 07 13:53:34 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN120320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 07 12:24:06 2020
 Response via : Initial Calibration

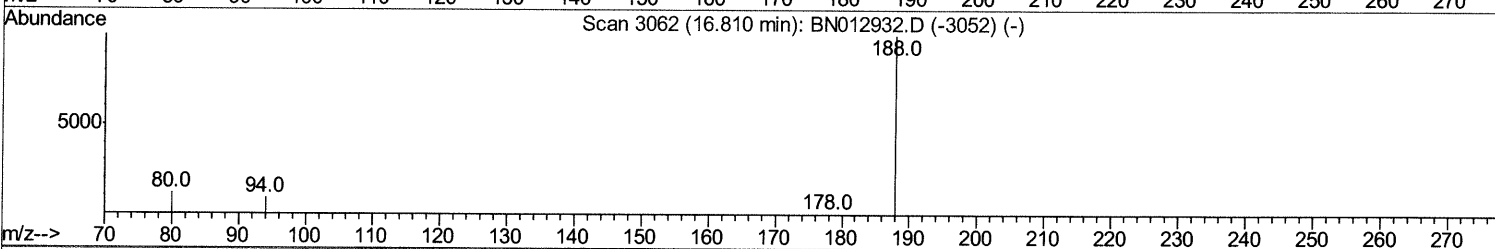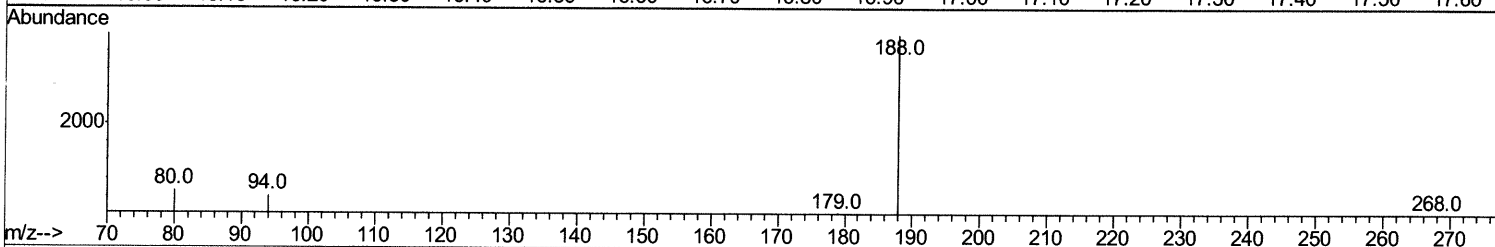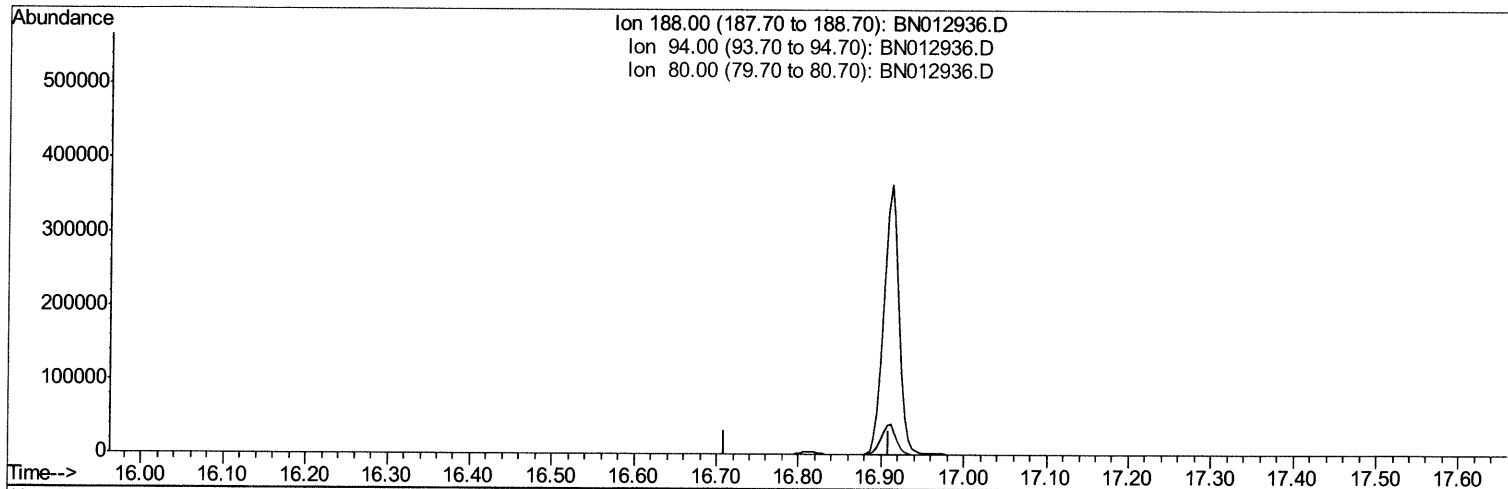

TIC: BN012936.D

(10) Phenanthrene-d10 (I)

16.810min (-16.810) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.40	0.00#
80.00	12.40	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN120720\
 Data File : BN012936.D
 Acq On : 07 Dec 2020 13:16
 Operator : CG/JU
 Sample : L4859-10
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0BE3

Manual Integrations
 APPROVED

mohammad
 12/9/2020 12:20:53 PM

Quant Time: Dec 07 13:53:34 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN120320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 07 12:24:06 2020
 Response via : Initial Calibration

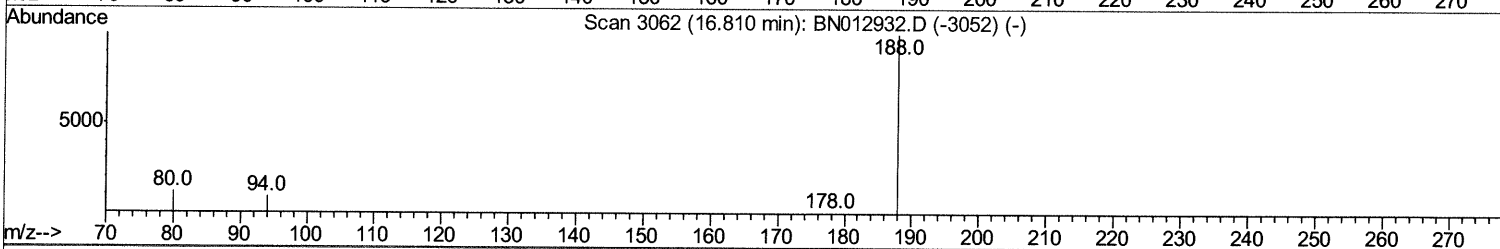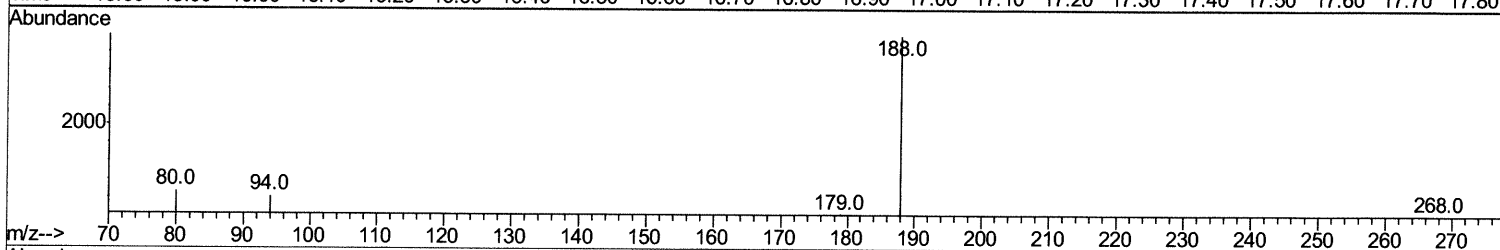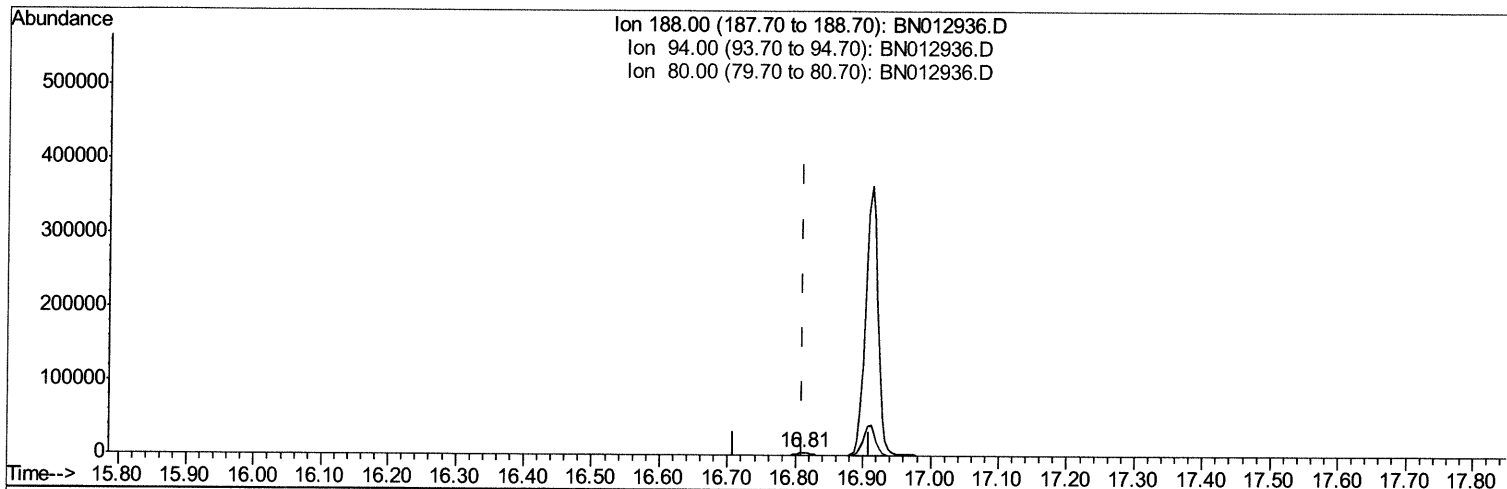

TIC: BN012936.D

(10) Phenanthrene-d10 (I)

16.810min (+0.000) 0.40ng/ul m 12/09/2020

response 5714

Ion	Exp%	Act%
188.00	100	100
94.00	11.40	10.68
80.00	12.40	13.57
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN120720\
 Data File : BN012936.D
 Acq On : 07 Dec 2020 13:16
 Operator : CG/JU
 Sample : L4859-10
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0BE3

Manual Integrations
 APPROVED

mohammad
 12/9/2020 12:20:53 PM

Quant Time: Dec 07 13:54:42 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN120320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 07 12:24:06 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.39	152	1048	0.40	ng/ul	0.00
2) Naphthalene-d8	10.15	136	4278	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.05	164	2563	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.81	188	5714m >	0.40	ng/ul >	0.00
16) Chrysene-d12	21.04	240	4861	0.40	ng/ul	0.00
20) Perylene-d12	23.14	264	5098	0.40	ng/ul	0.00

12/09/2020

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	11.76	152	1989	0.31	ng/ul	0.00
14) Fluoranthene-d10	18.86	212	4504	0.29	ng/ul	0.00

Target Compounds	Ovalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed