


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120720\
Data File : BN012957.D
Acq On : 08 Dec 2020 01:56
Operator : CG/JU
Sample : L4862-20
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0BH3

Manual Integrations
APPROVED

mohammad
12/9/2020 12:23:13 PM

Quant Time: Dec 08 02:35:31 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN120320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 08 00:15:39 2020
Response via : Initial Calibration

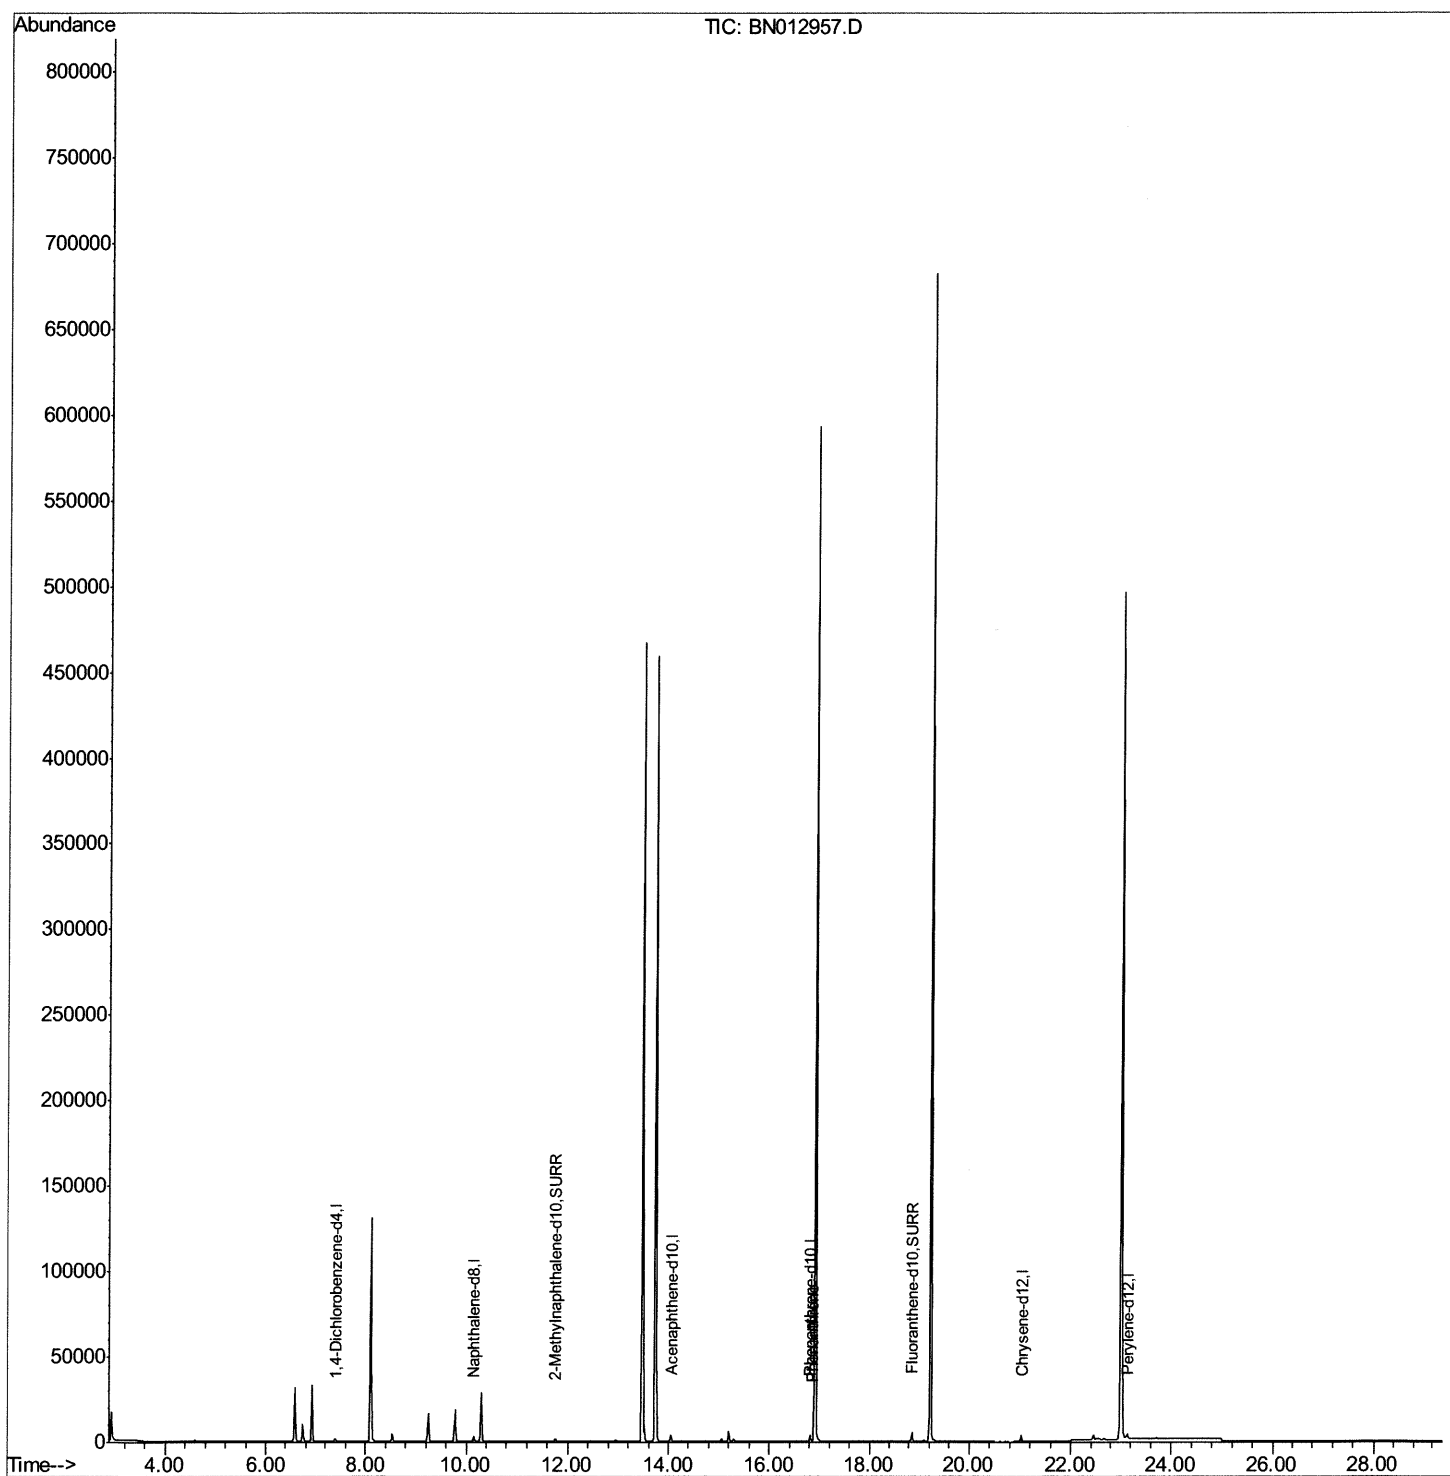

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120720\
 Data File : BN012957.D
 Acq On : 08 Dec 2020 01:56
 Operator : CG/JU
 Sample : L4862-20
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_N
ClientSampleId :
 C0BH3

Manual Integrations
APPROVED

mohammad
 12/9/2020 12:23:13 PM

Quant Time: Dec 08 02:32:33 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN120320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 08 00:15:39 2020
 Response via : Initial Calibration

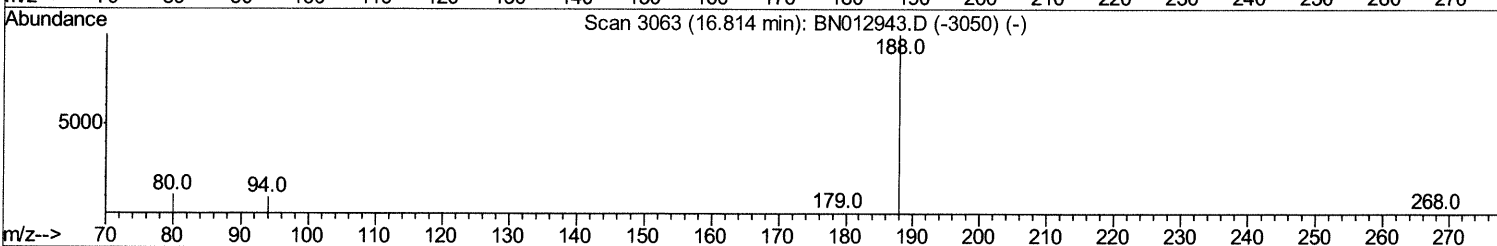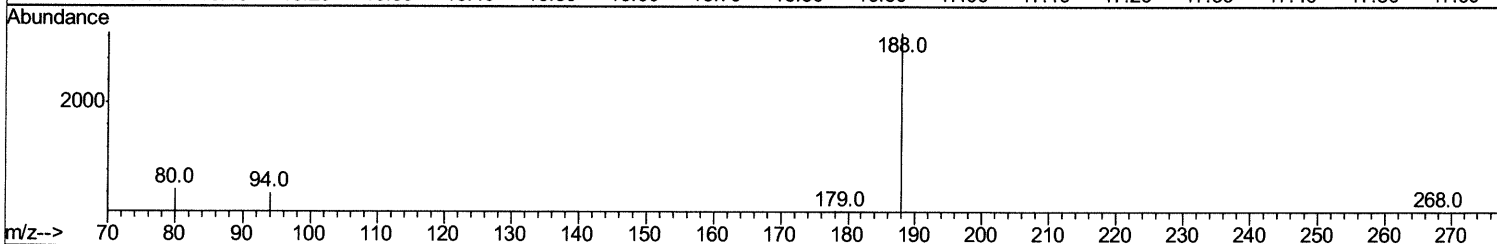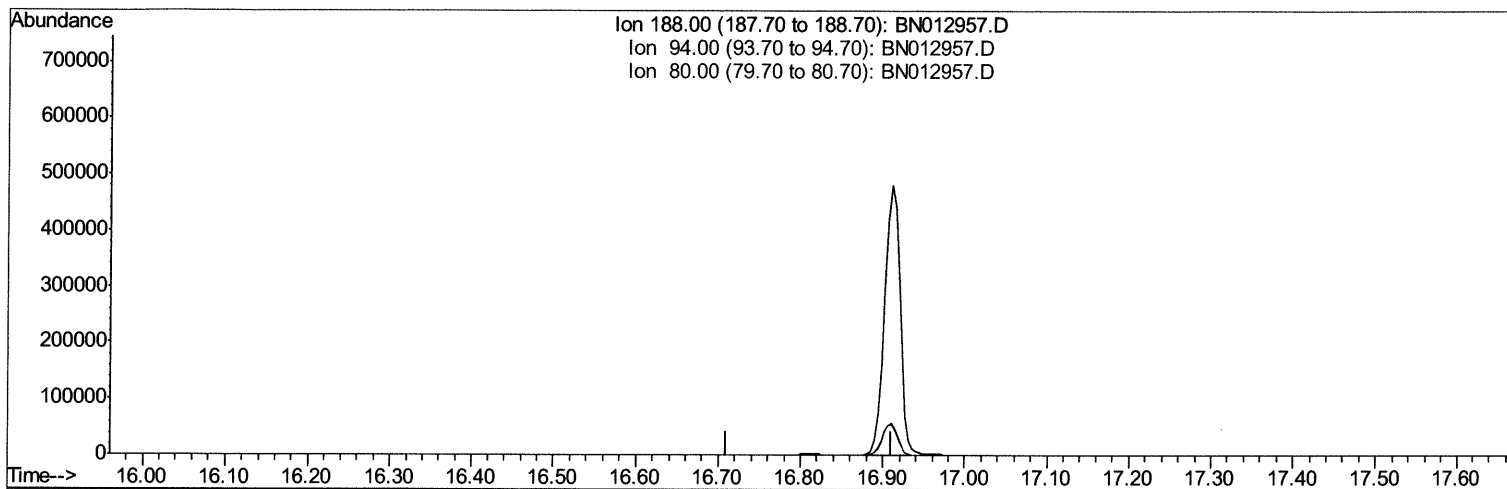

TIC: BN012957.D

(10) Phenanthrene-d10 (I)

16.810min (-16.810) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.40	0.00#
80.00	12.40	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120720\
 Data File : BN012957.D
 Acq On : 08 Dec 2020 01:56
 Operator : CG/JU
 Sample : L4862-20
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0BH3

Manual Integrations
 APPROVED

mohammad
 12/9/2020 12:23:13 PM

Quant Time: Dec 08 02:32:33 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN120320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 08 00:15:39 2020
 Response via : Initial Calibration

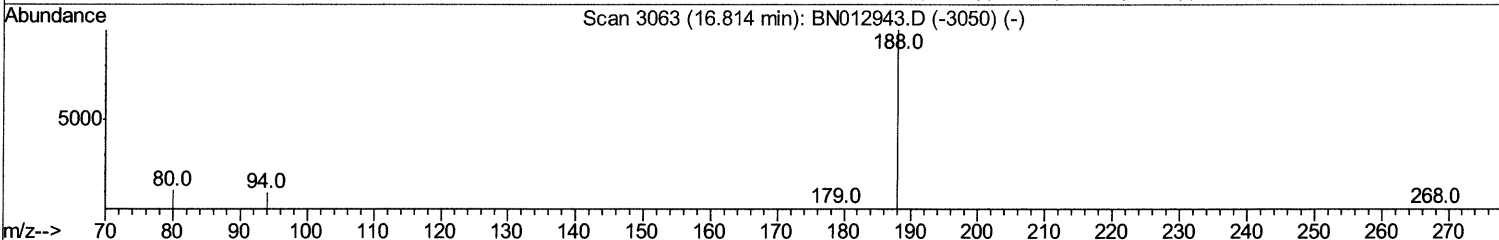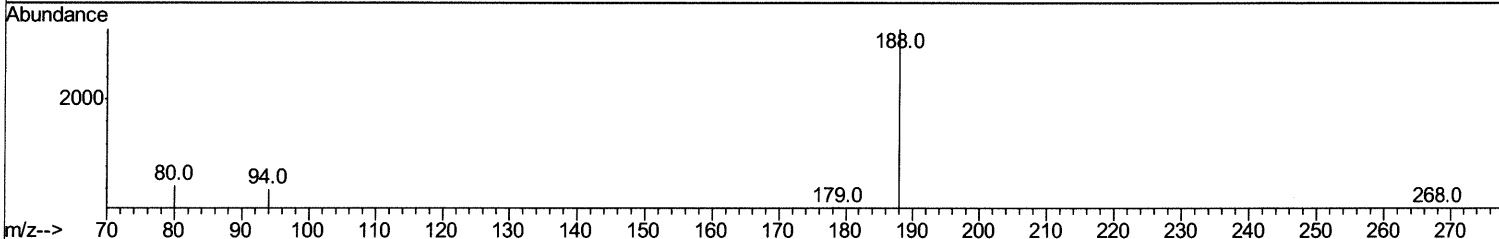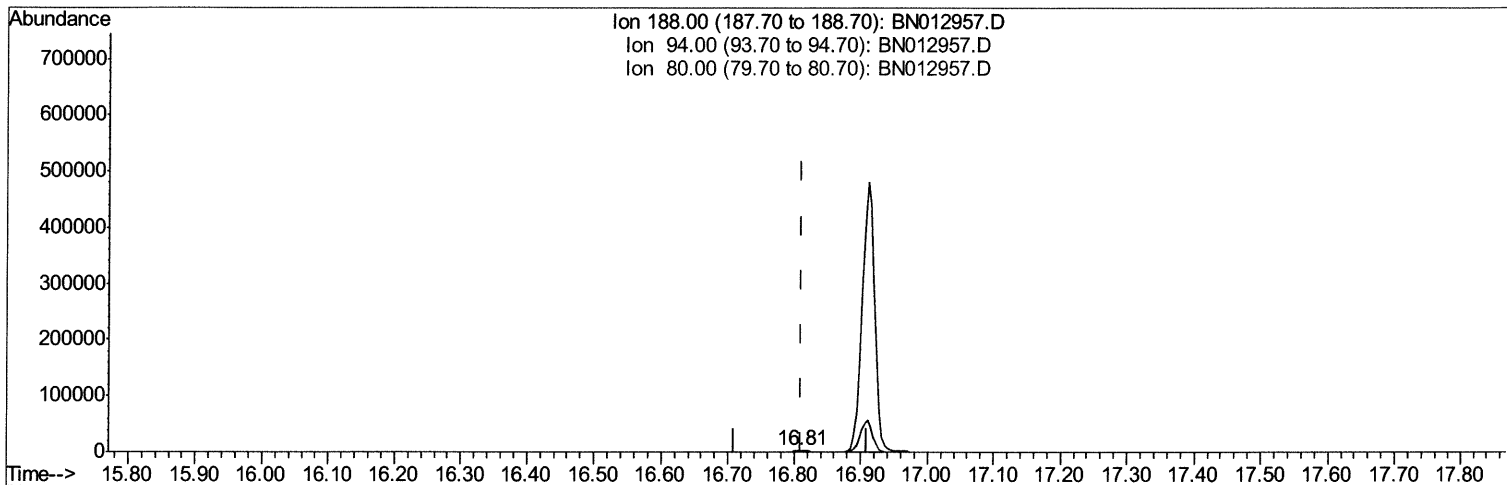

TIC: BN012957.D

(10) Phenanthrene-d10 (I)

16.809min (-0.001) 0.40ng/ul m 12/09/2020

response 4434

Ion	Exp%	Act%
188.00	100	100
94.00	11.40	11.61
80.00	12.40	13.61
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120720\
 Data File : BN012957.D
 Acq On : 08 Dec 2020 01:56
 Operator : CG/JU
 Sample : L4862-20
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0BH3

Manual Integrations
 APPROVED

mohammad
 12/9/2020 12:23:13 PM

Quant Time: Dec 08 02:35:31 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN120320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 08 00:15:39 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.38	152	852	0.40	ng/ul	0.00
2) Naphthalene-d8	10.15	136	3454	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.05	164	2135	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.81	188	4434m >	0.40	ng/ul >	0.00
16) Chrysene-d12	21.03	240	3682	0.40	ng/ul	0.00
20) Perylene-d12	23.13	264	3815	0.40	ng/ul	0.00

12/09/2020

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	11.76	152	2678	0.52	ng/ul	0.00
14) Fluoranthene-d10	18.85	212	5751	0.48	ng/ul	0.00

Target Compounds

	R.T.	QIon	Response	Conc	Units	Ovalue
12) Phenanthrene	16.85	178	327	0.022	ng/ul#	69

(#) = qualifier out of range (m) = manual integration (+) = signals summed