


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120720\
Data File : BN012989.D
Acq On : 08 Dec 2020 23:53
Operator : CG/JU
Sample : PB133396BL
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK96

Manual Integrations
APPROVED

mohammad
12/9/2020 12:25:32 PM

Quant Time: Dec 09 03:37:26 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN120320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 09 03:31:51 2020
Response via : Initial Calibration

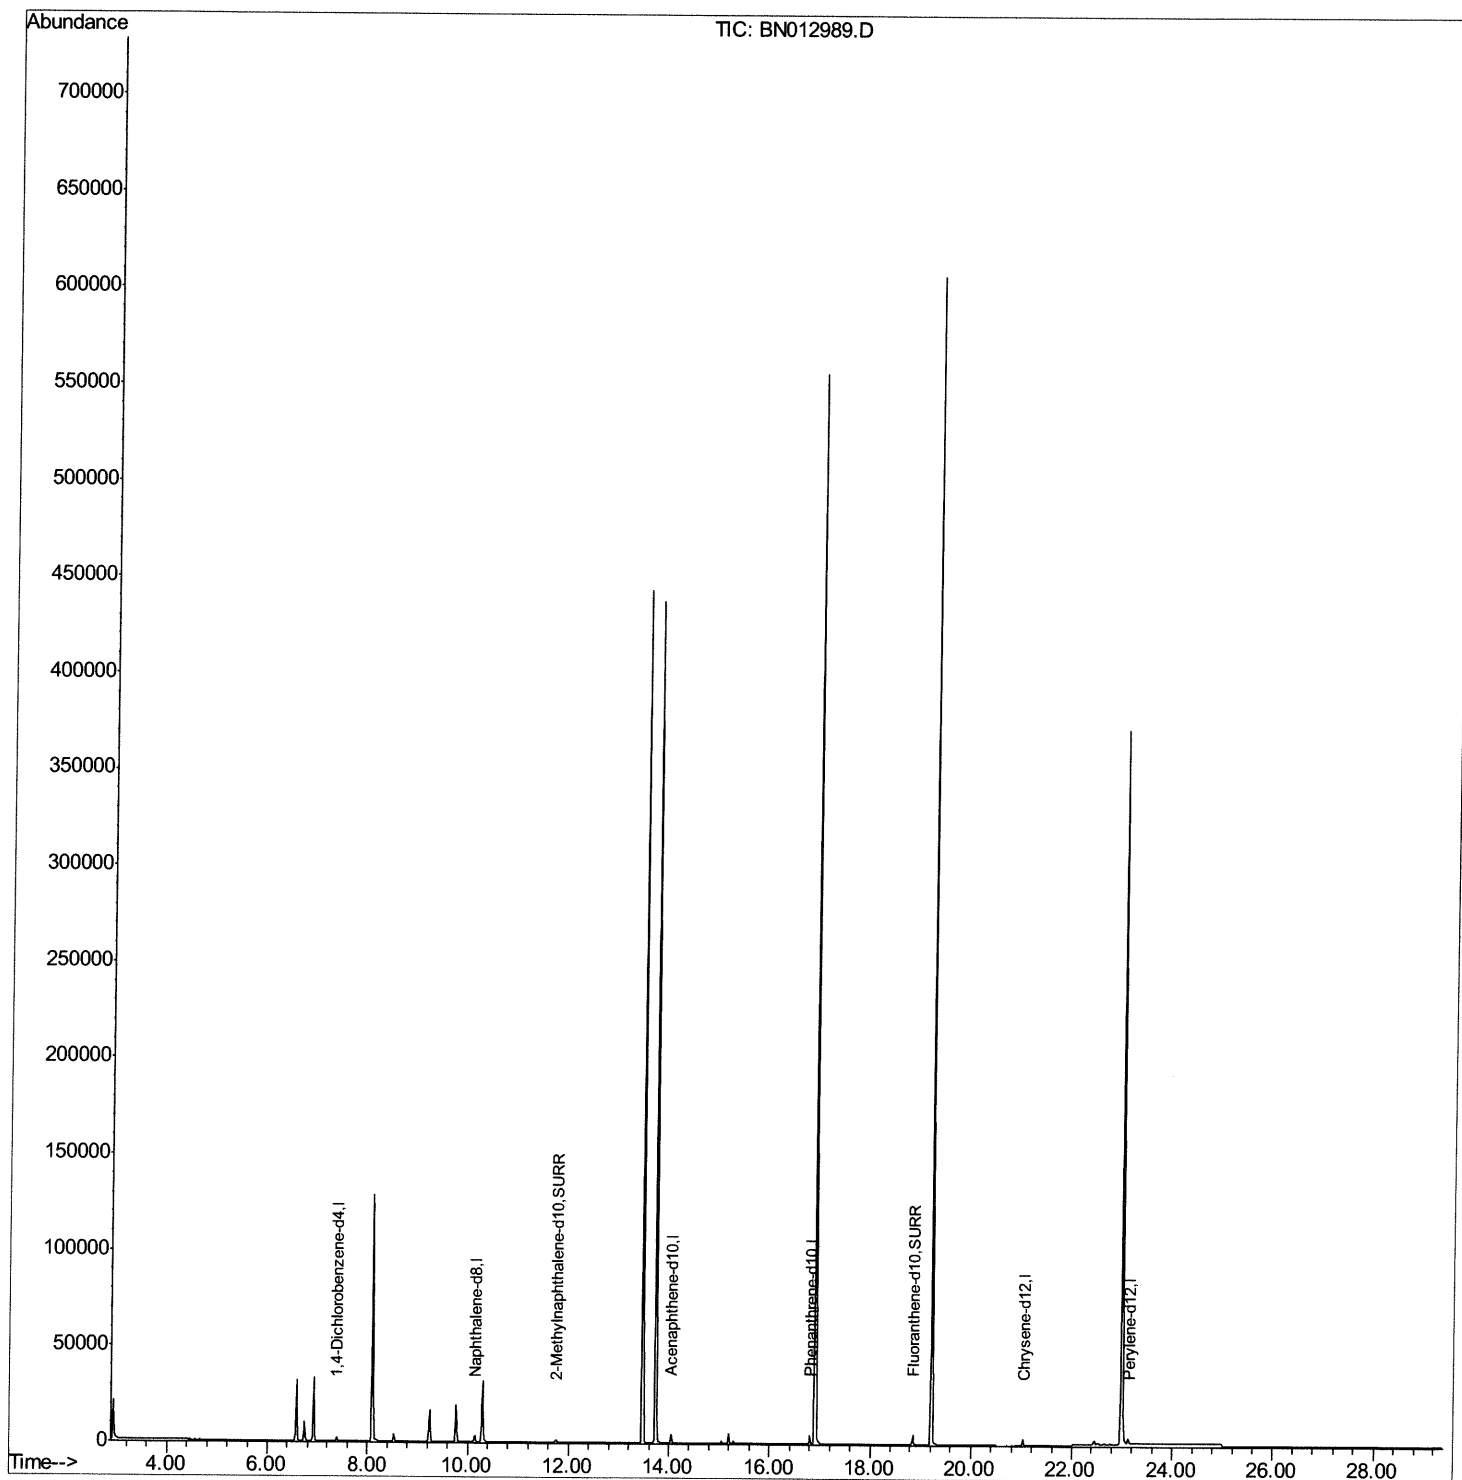

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120720\
 Data File : BN012989.D
 Acq On : 08 Dec 2020 23:53
 Operator : CG/JU
 Sample : PB133396BL
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK96

Manual Integrations
 APPROVED

mohammad
 12/9/2020 12:25:32 PM

Quant Time: Dec 09 03:35:44 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN120320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 09 03:31:51 2020
 Response via : Initial Calibration

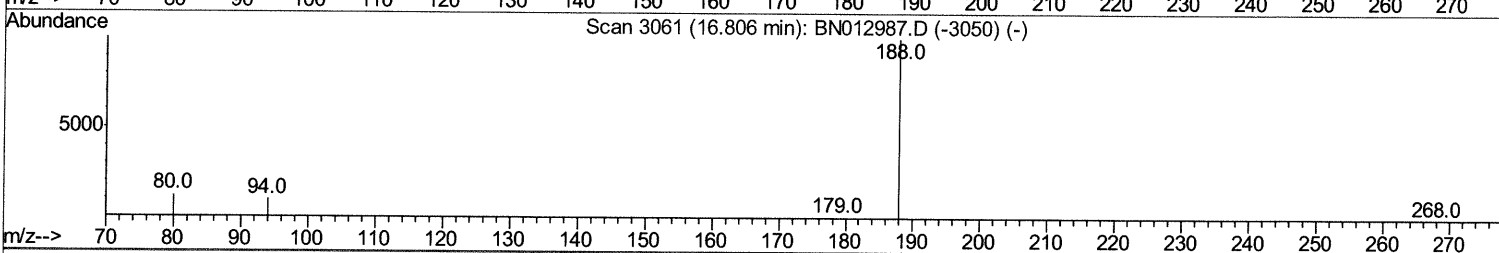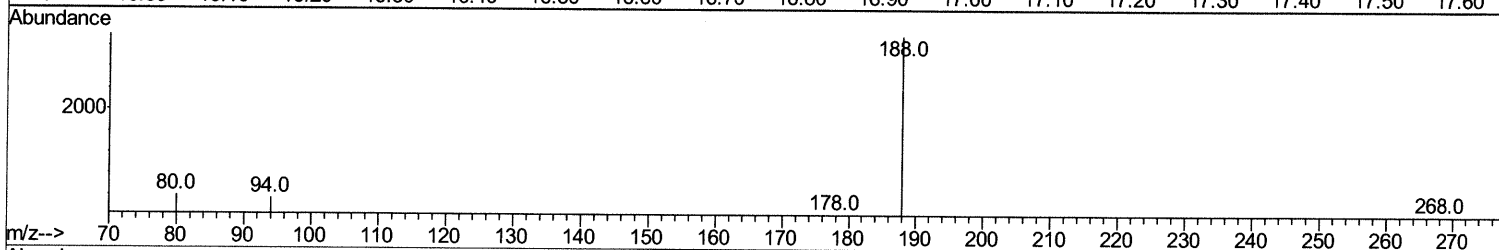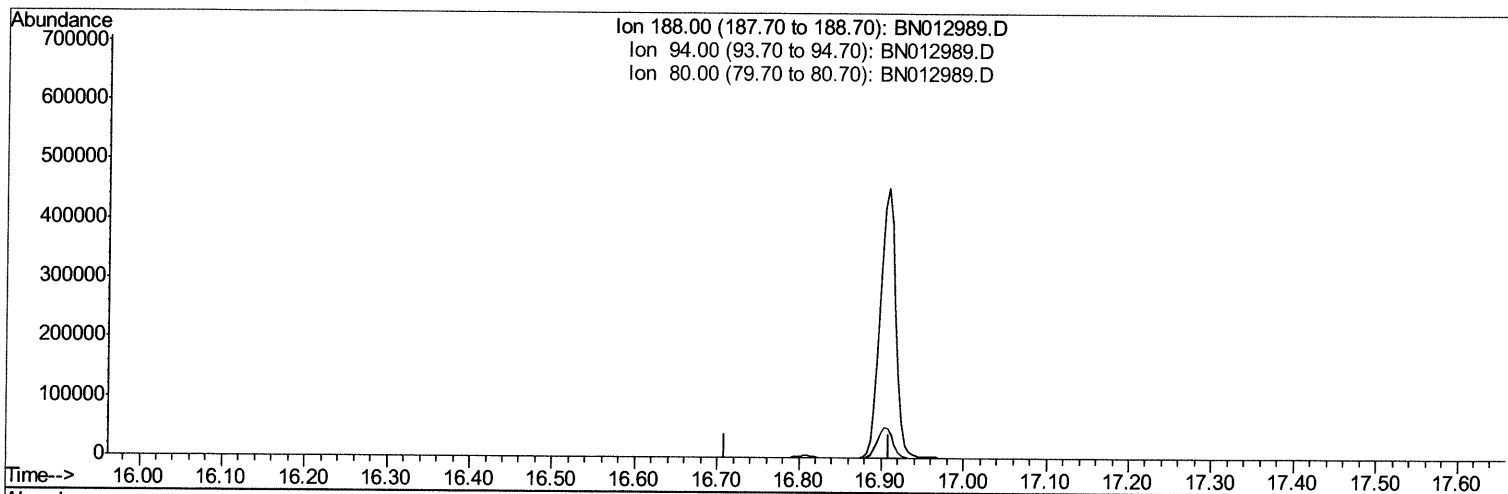

TIC: BN012989.D

(10) Phenanthrene-d10 (I)

16.810min (-16.810) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.40	0.00#
80.00	12.40	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120720\
 Data File : BN012989.D
 Acq On : 08 Dec 2020 23:53
 Operator : CG/JU
 Sample : PB133396BL
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK96

Manual Integrations
 APPROVED

mohammad
 12/9/2020 12:25:32 PM

Quant Time: Dec 09 03:35:44 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN120320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 09 03:31:51 2020
 Response via : Initial Calibration

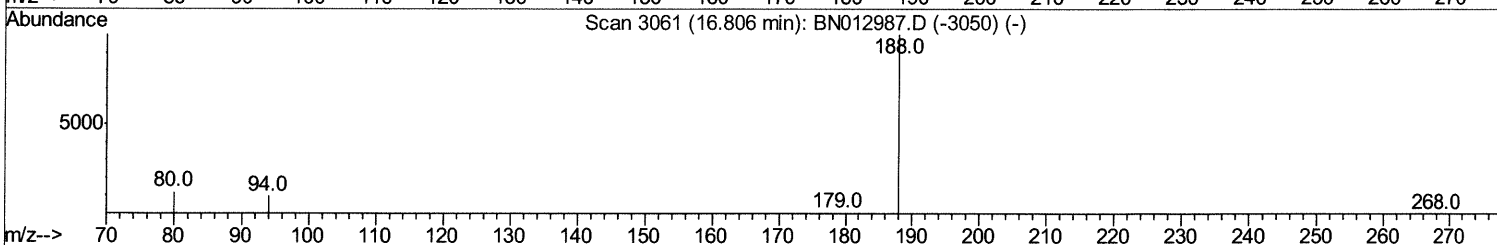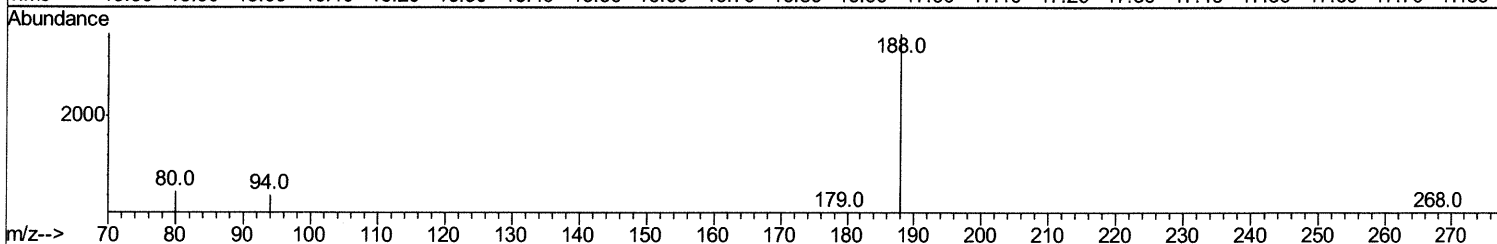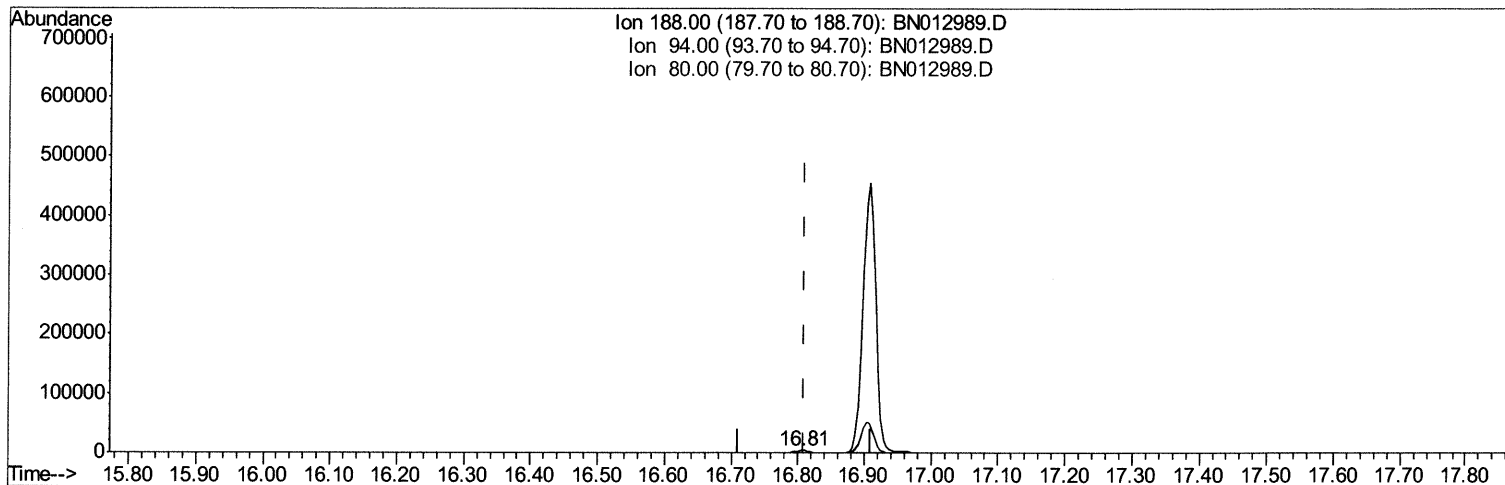

TIC: BN012989.D

(10) Phenanthrene-d10 (I)

16.806min (-0.004) 0.40ng/ul m 12/0/2024

response 5026

Ion	Exp%	Act%
188.00	100	100
94.00	11.40	10.83
80.00	12.40	12.71
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120720\
 Data File : BN012989.D
 Acq On : 08 Dec 2020 23:53
 Operator : CG/JU
 Sample : PB133396BL
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK96

Manual Integrations
 APPROVED

mohammad
 12/9/2020 12:25:32 PM

Quant Time: Dec 09 03:37:26 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN120320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 09 03:31:51 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.38	152	1076	0.40	ng/ul	0.00
2) Naphthalene-d8	10.15	136	4223	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.05	164	2515	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.81	188	5026m >	0.40	ng/ul >	0.00
16) Chrysene-d12	21.03	240	3243	0.40	ng/ul	0.00
20) Perylene-d12	23.13	264	3296	0.40	ng/ul	-0.01

12/10/2020

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	11.76	152	2785	0.44	ng/ul	0.00
14) Fluoranthene-d10	18.85	212	5654	0.41	ng/ul	0.00

Target Compounds

Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed